



# Standard Practice for Heat Treatment of Aluminum-Alloy Castings from All Processes<sup>1</sup>

This standard is issued under the fixed designation B917/B917M; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

*This standard has been approved for use by agencies of the U.S. Department of Defense.*

## 1. Scope\*

1.1 This practice covers, when specified by material specification or purchase order, the heat treatment of aluminum alloy castings from all casting processes.

1.1.1 The heat treatment of aluminum alloy castings used in specific aerospace applications is covered in AMS 2771<sup>2</sup> and specific AMS<sup>2</sup> material specifications.

1.1.2 The heat treatment of wrought aluminum alloys is covered in Practice B918/B918M.

1.2 The values stated in either SI units or inch-pound units are to be regarded separately as standard. The values stated in each system may not be exact equivalents; therefore, each system shall be used independently of the other. Combining values from the two systems may result in non-conformance with the standard.

1.2.1 *SI Units*—The SI units are shown in brackets or in separate tables.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

2.1 The following documents of the issue in effect on the date of material purchase form a part of this specification to the extent referenced herein:

2.2 *ASTM Standards*:<sup>3</sup>

<sup>1</sup> This practice is under the jurisdiction of ASTM Committee B07 on Light Metals and Alloys and is the direct responsibility of Subcommittee B07.01 on Aluminum Alloy Ingots and Castings.

Current edition approved May 1, 2012. Published June 2012. Originally approved in 2001. Last previous edition approved in 2011 as B917/B917M – 11. DOI: 10.1520/B0917\_B0917M-12.

<sup>2</sup> Available from Society of Automotive Engineers (SAE), 400 Commonwealth Dr., Warrendale, PA 15096-0001, <http://www.sae.org>.

<sup>3</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

B26/B26M Specification for Aluminum-Alloy Sand Castings

B108/B108M Specification for Aluminum-Alloy Permanent Mold Castings

B275 Practice for Codification of Certain Zinc, Tin and Lead Die Castings

B557 Test Methods for Tension Testing Wrought and Cast Aluminum- and Magnesium-Alloy Products

B557M Test Methods for Tension Testing Wrought and Cast Aluminum- and Magnesium-Alloy Products (Metric)

B618/B618M Specification for Aluminum-Alloy Investment Castings

B686/B686M Specification for Aluminum Alloy Castings, High-Strength

B881 Terminology Relating to Aluminum- and Magnesium-Alloy Products

B918/B918M Practice for Heat Treatment of Wrought Aluminum Alloys

B955/B955M Specification for Aluminum-Alloy Centrifugal Castings

B969 Specification for Aluminum-Alloy Castings Produced by the Squeeze Casting, Thixocast and Rheocast Semi-Solid Casting Processes

G110 Practice for Evaluating Intergranular Corrosion Resistance of Heat Treatable Aluminum Alloys by Immersion in Sodium Chloride + Hydrogen Peroxide Solution

2.3 *ANSI Standard*:

H35.1 Alloy and Temper Designation Systems for Aluminum<sup>4</sup>

2.4 *SAE Standard*:

AMS 2771 Heat Treatment of Aluminum Alloy Castings

## 3. Terminology

3.1 *Definitions*:

3.1.1 Refer to Terminology B881 for terminology relating to the heat treatment of castings.

<sup>4</sup> Available from Aluminum Association, Inc., 1525 Wilson Blvd., Suite 600, Arlington, VA 22209, <http://www.aluminum.org>.

\*A Summary of Changes section appears at the end of this standard

## 4. Equipment

4.1 *Heating Media*—Aluminum castings are typically heat treated in air chamber furnaces; however, lead baths, oil baths, fluidized beds, or even superheated steam may be used in specific applications. The use of uncontrolled heating is not permitted. Whichever heating means are employed, careful evaluation is required to ensure that the casting responds properly to heat treatment and is not overheated or damaged by the heat treatment environment. Salt baths are not recommended for the commercial heat treatment of aluminum castings in volume. (**Warning**—Nitrate baths must not be used in the heat treatment of 5xx.0 series castings because of the inherent explosion hazard.)

4.2 *Air Chamber Furnaces*—may be oil or gas-fired or may be electrically heated. The atmosphere in air chamber furnaces must be controlled to prevent porosity resulting from solution heat treatment. Furnace components that are significantly hotter than the metal should be suitably shielded for section thicknesses of less than 0.250 in. [6 mm] to prevent adverse radiation effects. The atmosphere in air chamber furnaces must be controlled to prevent porosity resulting from solution heat treatment (see **Note 1**). The suitability of the atmosphere in an air-chamber furnace can be demonstrated by testing, in accordance with 8.4.3.1, that products processed in that furnace are substantially free of heat treat induced porosity.

**NOTE 1**—Heat treat induced porosity may lower mechanical properties and commonly causes blistering of the surface of the material. The condition is most likely to occur in furnaces in which the products of combustion contact the work, particularly if the gases are high in water vapor or contain compounds of sulfur. Surface discoloration is a normal result of solution heat treatment of aluminum alloys and should not be interpreted as evidence of damage from overheating or as heat treat induced porosity.

4.3 *Automatic Recording and Control Equipment*—to control temperature of air furnaces shall be capable of maintaining temperature in the working zone to within  $\pm 10^{\circ}\text{F}$  [ $\pm 5^{\circ}\text{C}$ ] of the specified temperature.

4.4 *Quench Baths*—Quenching is normally performed by immersion of castings in a hot-water bath as described in **Tables 1-4**. The water baths must be located close enough to solution heat-treating facilities to minimize delay in quenching. Tanks must be of adequate size for the expected work load and must have the means of providing adequate circulation of the quenching media about the work load. Means for heating or cooling the quench water should be available when needed.

**NOTE 2**—Quenching may be performed by alternative means such as total immersion in a glycol and water solution, a liquefied gas, cold water, hot water, or boiling water, or by air blast or fog to minimize distortion provided samples from the material, so quenched, will conform to the (1) mechanical properties, (2) other requirements of the applicable casting specification and (3) not exhibit more intergranular corrosion susceptibility than if the metal was immersion quenched in cold water. The use of water sprays or high-velocity high-volume jets of water in which the material is thoroughly and effectively flushed is satisfactory for quenching. Alternative quench media are frequently contingent on the particular alloy and the end use of the casting.

## 5. Furnace Temperature Uniformity and Calibration Requirements

### 5.1 Calibration of Equipment:

5.1.1 Thermocouple wire and sensors shall be calibrated against wire or sensors whose calibration is traceable to NIST). Thermocouples made from calibrated wire rolls may be used in lieu of individually calibrated thermocouples in which case, the roll calibration shall be that of the average of samples taken from both ends of the roll. The roll shall not be used if the difference in the highest and lowest reading exceeds  $2^{\circ}\text{F}$  [ $1^{\circ}\text{C}$ ].

5.1.2 Working instruments shall be calibrated at least once every three months against a test instrument that is traceable to NIST. Accuracy shall be  $\pm 0.3\%$  of range.

### 5.2 Furnace Temperature Survey:

5.2.1 A temperature survey, to ensure compliance with the applicable recommendations presented herein, shall be performed for each furnace.

5.2.2 A new temperature survey shall be made after any modification, repair, adjustment (for example, to power controls, or baffles), or rebuild which may have altered the temperature uniformity characteristics of the furnace and reduced the effectiveness of the heat treatment.

### 5.3 Batch Furnace Surveys:

5.3.1 The initial temperature survey shall be made at the maximum and minimum temperature of solution heat treatments and precipitation heat treatments for which each furnace is to be used. There shall be at least one test location for each  $25\text{ ft}^3$  [ $0.70\text{ m}^3$ ] of air furnace volume up to a maximum of 40 test locations, with a minimum of nine test locations, one in each corner and one in the center.

5.3.2 After the initial survey, each furnace shall be surveyed monthly, except as provided in 5.3.7. The monthly survey shall be at one operating temperature for solution heat treatment and one for precipitation heat treatment.

5.3.3 There shall be at least one test location for each  $40\text{ ft}^3$  [ $1\text{ m}^3$ ] of load volume, with a minimum of nine test locations, one in each corner and one in the center.

5.3.4 The surveys shall reflect the normal operating characteristics of the furnace. If the furnace is normally charged after being stabilized at the correct operating temperature, the temperature-sensing elements shall be similarly charged. If the furnace is normally charged cold, the temperature-sensing elements shall be charged cold. After insertion of the temperature-sensing elements, readings should be taken frequently enough to determine when the temperature of the hottest region of the furnace approaches the bottom of the temperature range being surveyed. From that time until thermal equilibrium is reached, the temperature of all test locations should be determined at 2-min intervals in order to detect any over-shooting. After thermal equilibrium is reached, readings should be taken at 5-min intervals for sufficient time to determine the recurrent temperature pattern, but for not less than 30 min. Before thermal equilibrium is reached, none of the temperature readings should exceed the maximum temperature of the range being surveyed. After thermal equilibrium is reached, the maximum temperature variation of all elements (both load and furnace thermocouples) shall not exceed  $20^{\circ}\text{F}$  [ $10^{\circ}\text{C}$ ] and shall not vary outside the range being surveyed.

**TABLE 1 Recommended Heat Treatment for Sand and Investment Type Alloys (Inch-Pound Units)**

Alloy <sup>A</sup>	Final Temper <sup>A</sup>	Solution Heat Treatment <sup>B, C</sup>		Precipitation Heat Treatment <sup>D</sup>	
		Metal Temperature, ±10°F	Time at Temperature, h	Metal Temperature, ±10°F	Time at Temperature, h
201.0	T6	960 then 980	2 <sup>E</sup> 14 to 20	room temperature then 310	12 to 24 20
	T7	960 then 980	2 <sup>E</sup> 14 to 20	room temperature then 370	12 to 24 5
A201.0	T7	955 then 985	2 <sup>E</sup> 14 to 20	room temperature then 370	12 to 24 5
203.0	T6	955 then 1010	2 <sup>E</sup> 5	room temperature then 425	12 to 24 16
204.0	T4	970	10	room temperature	5 days <sup>F</sup>
A206.0	T4	950 then 985	2 <sup>E</sup> 14 to 20	room temperature	5 days
	T43	950 then 985	2 <sup>E</sup> 14 to 20	room temperature then 320	12 to 24 0.5 to 1
	T6 <sup>G</sup>	950 then 985	2 <sup>E</sup> 14 to 20	room temperature then 310	12 to 24 20
	T7	950 then 985	2 <sup>E</sup> 14 to 20	room temperature then 370	12 to 24 4 to 5
	...	...	...	600 <sup>H</sup>	3
222.0	O <sup>D, H</sup> T61	945	6 to 12	310	11
242.0	O <sup>D, H</sup> T571	...	...	650 <sup>H</sup>	3
	T61	...	...	400	8
	T61	960	2 to 6 <sup>I</sup>	450	1 to 3
A242.0	T75	965	6 to 10	550	2 to 5
295.0	T4	960	6 to 12	...	...
	T6	960	6 to 12	310	3 to 6
	T62	960	6 to 12	310	12 to 24
	T7	960	6 to 12	500	4 to 6
296.0	T4	950	4 to 8	...	...
	T6	950	4 to 8	310	2 to 8
	T7	950	4 to 8	500	4 to 6
319.0	T4	940	6 to 10	...	...
	T5	...	...	400	8
	T6	940	6 to 12	310	2 to 5
328.0	T6	960	12	310	2 to 5
355.0	T51	...	...	440	7 to 9
	T6	980	6 to 12	310	3 to 5
	T7	980	6 to 12	440	3 to 5
	T71	980	6 to 12	475	4 to 6
C355.0 <sup>J</sup>	T6	985	6 to 12	room temperature then 310	8 3 to 5
	...	...	...	440	7 to 9
356.0	T51	...	...	440	7 to 9
	T6	1000	6 to 12 <sup>K</sup>	310	3 to 5
	T7	1000	6 to 12 <sup>K</sup>	400	3 to 5
	T71	1000	6 to 12 <sup>K</sup>	475	2 to 4
A356.0	T6	1000	6 to 12 <sup>K</sup>	310	2 to 5
	T61	1000	6 to 12 <sup>K</sup>	330	6 to 12
	T7	1000	6 to 12 <sup>K</sup>	440	8
	T71	1000	6 to 12 <sup>K</sup>	475	3 to 6
357.0	T6	1000 <sup>H</sup>	8 <sup>K</sup>	330	6 to 12
	T61	1000	10 to 12 <sup>K</sup>	310	10 to 12
A357.0 <sup>J</sup>	T61	1000 <sup>H</sup>	8 to 10 <sup>K</sup>	room temperature then 310	8 8
A390.0	T6	925	8 to 12	350	8
520.0	T4	810	12 to 18 <sup>L</sup>	...	...
705.0	T1	...	...	room temperature	21 days
	T5	...	...	210	8
707.0	T1	...	...	room temperature	21 days
	T5	...	...	210	8
	T7	990	8 to 16	350	4 to 10
710.0	T5	...	...	room temperature or 315	21 days 6 to 8
712.0	T5	...	...	room temperature or 315	21 days 6 to 8
713.0	T1	...	...	room temperature	21 days
	T5	...	...	250	16
771.0	T5	...	...	355	3 to 5
	T51	...	...	405	6
	T52	...	...	330 <sup>J</sup>	6 to 16 <sup>M</sup>
	T6	1090	6 <sup>D</sup>	265	3
	T53	...	...	360 <sup>J, D</sup>	4
	T71	1090	6 <sup>D</sup>	285	15
850.0	T5	...	...	430	7 to 9
851.0	T5	...	...	430	7 to 9

**TABLE 1** *Continued*

Alloy <sup>A</sup>	Final Temper <sup>A</sup>	Solution Heat Treatment <sup>B, C</sup>		Precipitation Heat Treatment <sup>D</sup>	
		Metal Temperature, ±10°F	Time at Temperature, h	Metal Temperature, ±10°F	Time at Temperature, h
852.0	T5	...	...	430	7 to 9

<sup>A</sup> Designations conform to ANSI H35.1 and to Practice B275.

<sup>B</sup> Quench in water at 150 to 212°F except as noted.

<sup>C</sup> Time at solution temperature may be increased for section thickness over 1 in.

<sup>D</sup> No quenching required. Cool in still air outside the furnace.

<sup>E</sup> Cooling not required prior to second step.

<sup>F</sup> In order to expedite testing, alloy 204.0 test specimens may be precipitation heat treated after quenching by holding at 255°F for 2 h.

<sup>G</sup> This alloy is stress corrosion crack prone when in the T6 temper and should not be used in the T6 temper for applications that see, even mildly corrosive environments.

<sup>H</sup> Solution treatment temperature of 1010°F may be used (to obtain higher solubility) provided no portion of the heat treat oven exceeds 1020°F.

<sup>I</sup> Quenching is accomplished by air blast.

<sup>J</sup> Stress relieve for dimensional stability in the following manner: (1) Hold at 775 ± 25°F for 5 h; (2) Furnace cool to 650°F for 2 or more h; (3) Furnace cool to 450°F for not more than ¾ h; (4) Furnace cool to 250°F for approximately 2 h; and (5) Cool to room temperature in still air outside the furnace.

<sup>K</sup> The solution times may be reduced when the silicon eutectic has been well modified such as when modified with Sr or Na.

<sup>L</sup> Quench in water at 150 to 212°F for a controlled time of 10 to 20 s, then cool in still air outside the furnace.

<sup>M</sup> Time required depends on variations in cooling rate between 650° and 450°F during stress-relief procedure (Footnote J).

5.3.5 For furnaces of 10 ft<sup>3</sup> [0.25 m<sup>3</sup>] or less the temperature survey may be made with a minimum of three thermocouples located at front, center, and rear or at top, center, and bottom of the furnace.

5.3.6 For furnaces used only for precipitation treatment, after the initial temperature-uniformity survey, as outlined in 5.3.7, surveys need not be made more often than at each 6-month interval provided that (1) test specimens from each lot are tested and meet applicable material specifications requirements, (2) the furnace is equipped with a multipoint recorder, or (3) one or more separate load thermocouples are employed to measure and record actual metal temperatures.

5.3.7 Monthly surveys for batch furnaces are not necessary when the furnace or bath is equipped with a permanent multipoint recording system with at least two sensing thermocouples in each zone or when one or more separate load thermocouples are employed to measure actual metal temperature, providing that uniformity surveys show a history of satisfactory performance for a period of at least 6 months. The sensing thermocouples shall be installed so as to record the temperature of the heated media (air, lead, and so forth) or actual metal temperatures. However, periodic surveys shall also be made at 6-month intervals in accordance with the procedures outlined for the monthly survey.

#### 5.4 Continuous Furnace Surveys:

5.4.1 For continuous heat-treating furnaces, the type of survey and the procedures for performing the survey should be established for each particular furnace involved. The types of continuous heat-treating furnaces may vary considerably, depending upon the product and sizes involved. For some types and sizes of furnaces, the only practical way to survey the furnace is to perform an extensive mechanical property survey of the limiting product sizes to verify conformance with the specified mechanical properties for such items. When the type and size of the furnace makes this practical, monthly surveys should be made, using a minimum of two load thermocouples attached to the material. The surveys should reflect the normal operating characteristics of the furnace. The results of these surveys shall indicate that the metal temperature never exceeds the allowable maximum metal temperature specified for solu-

tion heat treatment (Tables 1-4 as appropriate) after all load thermocouples have reached the minimum metal temperature specified.

5.4.2 Furnace control temperature-measuring instruments shall not be used to read the temperature of the test temperature sensing elements.

5.5 *Monitoring of Quench*—A monitoring plan shall be developed and utilized for all modes of quenching for all products covered by this practice. The plan should incorporate conductivity or hardness checking, or both, to determine the uniformity of the quench. Areas having substantially higher conductivity or lower hardness than other areas of similar thickness in the lot shall be investigated to ensure that the requirements of the material specification are met.

5.6 *Temperature-Measuring System Check*—The accuracy of the temperature-measuring system shall be checked under operating conditions weekly. Check should be made by inserting a calibrated test temperature-sensing element adjacent to the furnace temperature-sensing element and reading the test temperature-sensing element with a calibrated test potentiometer. When the furnace is equipped with dual potentiometer measuring systems which are checked daily against each other, the above checks may be conducted every 3 months rather than every week. The test temperature-sensing element, potentiometer, and cold junction compensation combination shall have been calibrated against NIST primary or secondary certified temperature-sensing elements, within the previous 3 months, to an accuracy of ±2°F [±1°C].

5.6.1 If the difference between the two readings in 5.6 exceeds ±10°F [±6°C], the cause of the difference shall be determined and corrected before commencing additional thermal processing. The responsible quality organization shall be notified and appropriate corrective action shall be taken and documented including an evaluation of the possible effects of the deviation on castings processed since the last successful test.

## 6. Preparation for Heat Treatment

### 6.1 Furnace Loading:

**TABLE 2 Recommended Heat Treatment for Sand and Investment Type Aluminum Alloys [SI Units]**

Alloy <sup>A</sup>	Final Temper <sup>A</sup>	Solution Heat Treatment <sup>B, C</sup>		Precipitation Heat Treatment <sup>D</sup>	
		Metal Temperature, ±5°C	Time at Temperature, h	Metal Temperature, ±5°C	Time at Temperature, h
201.0	T6	515 then 525	2 <sup>E</sup> 14 to 20	room temperature then 155	12 to 24 20
	T7	515 then 525	2 <sup>E</sup> 14 to 20	room temperature then 190	12 to 24 5
A201.0	T7	515 then 530	2 <sup>E</sup> 14 to 20	room temperature then 190	12 to 24 5
203.0	T6	515 then 545	2 <sup>E</sup> 5	room temperature then 220	12 to 24 16
204.0	T4	520	10	room temperature	5 days <sup>F</sup>
A206.0	T4	510 then 530	2 <sup>E</sup> 14 to 20	room temperature	5 days
	T43	510 then 530	2 <sup>E</sup> 14 to 20	room temperature then 160	12 to 24 0.5 to 1
	T6 <sup>G</sup>	510 then 530	2 <sup>E</sup> 14 to 20	room temperature then 155	12 to 24 20
	T7	510 then 530	2 <sup>E</sup> 14 to 20	room temperature then 190	12 to 24 4 to 5
	222.0	O <sup>D, H</sup> T61	... 510	... 6 to 12	315 <sup>H</sup> 155
242.0	O <sup>D, H</sup> T571	... ...	... ...	345 <sup>H</sup> 205	3 8
	T61	515	2 to 6 <sup>I</sup>	230	1 to 3
A242.0	T75	520	6 to 10	290	2 to 5
295.0	T4	515	6 to 12	...	...
	T6	515	6 to 12	155	3 to 6
	T62	515	6 to 12	155	12 to 24
	T7	515	6 to 12	260	4 to 6
296.0	T4	510	4 to 8	...	...
	T6	510	4 to 8	155	2 to 8
	T7	510	4 to 8	260	4 to 6
319.0	T4	505	6 to 10	...	...
	T5	...	...	205	8
	T6	505	6 to 12	155	2 to 5
	T6	515	12	155	2 to 5
328.0	T6	515	12	155	2 to 5
355.0	T51	...	...	225	7 to 9
	T6	525	6 to 12	155	3 to 5
	T7	525	6 to 12	225	3 to 5
	T71	525	6 to 12	245	4 to 6
C355.0 <sup>J</sup>	T6	530	6 to 12	room temperature then 155	8 3 to 5
	T51	...	...	225	7 to 9
356.0	T6	540	6 to 12 <sup>K</sup>	155	3 to 5
	T7	540	6 to 12 <sup>K</sup>	205	3 to 5
	T71	540	6 to 12 <sup>K</sup>	245	2 to 4
	T6	540	6 to 12 <sup>K</sup>	155	2 to 5
A356.0	T61	540	6 to 12 <sup>K</sup>	165	6 to 12
	T7	540	6 to 12 <sup>K</sup>	225	8
	T71	540	6 to 12 <sup>K</sup>	245	3 to 6
	T6	540 <sup>H</sup>	8 <sup>K</sup>	165	6 to 12
357.0	T61	540	10 to 12 <sup>K</sup>	155	10 to 12
A357.0 <sup>J</sup>	T61	540 <sup>H</sup>	8 to 10 <sup>K</sup>	room temperature then 155	8 8
	T6	495	8 to 12	175	8
A390.0	T6	495	8 to 12	175	8
520.0	T4	430	12 to 18 <sup>L</sup>	...	...
705.0	T1	...	...	room temperature	21 days
	T5	...	...	100	8
707.0	T1	...	...	room temperature	21 days
	T5	...	...	99	8
	T7	530	8 to 16	175	4 to 10
710.0	T5	...	...	room temperature or 155	21 days 6 to 8
712.0	T5	...	...	room temperature or 155	21 days 6 to 8
713.0	T1	...	...	room temperature	21 days
771.0	T5	...	...	120	16
	T5	...	...	180	3 to 5
	T51	...	...	205	6
	T52	...	...	165 <sup>J</sup>	6 to 16 <sup>M</sup>
	T6	590	6 <sup>D</sup>	130	3
850.0	T53	...	...	180 <sup>J, D</sup>	4
	T71	590	6 <sup>D</sup>	140	15
	T5	...	...	220	7 to 9
851.0	T5	...	...	220	7 to 9

**TABLE 2 Continued**

Alloy <sup>A</sup>	Final Temper <sup>A</sup>	Solution Heat Treatment <sup>B, C</sup>		Precipitation Heat Treatment <sup>D</sup>	
		Metal Temperature, ±5°C	Time at Temperature, h	Metal Temperature, ±5°C	Time at Temperature, h
852.0	T5	...	...	220	7 to 9

<sup>A</sup> Designations conform to ANSI H35.1 and to Practice B275.

<sup>B</sup> Quench in water at 65 to 100°C except as noted.

<sup>C</sup> Time at solution temperature may be increased for section thickness over 25 mm.

<sup>D</sup> No quenching required. Cool in still air outside the furnace.

<sup>E</sup> Cooling not required prior to second step.

<sup>F</sup> In order to expedite testing, alloy 204.0 test specimens may be precipitation heat treated after quenching by holding at 125°C for 2 h.

<sup>G</sup> This alloy is stress corrosion crack prone when in the T6 temper and should not be used in the T6 temper for applications that see, even mildly corrosive environments.

<sup>H</sup> Solution treatment temperature of 545°C may be used (to obtain higher solubility) provided no portion of the heat treat oven exceeds 550°C.

<sup>I</sup> Quenching is accomplished by air blast.

<sup>J</sup> Stress relieve for dimensional stability in the following manner: (1) Hold at 415 ± 15°C for 5 h; (2) Furnace cool to 345°C for 2 or more h; (3) Furnace cool to 230°C for not more than ¾ h; (4) Furnace cool to 120°C for approximately 2 h; and (5) Cool to room temperature in still air outside the furnace.

<sup>K</sup> The solution times may be reduced when the silicon eutectic has been well modified such as when modified with Sr or Na.

<sup>L</sup> Quench in water at 65 to 100°C for a controlled time of 10 to 20 s, then cool in still air outside the furnace.

<sup>M</sup> Time required depends on variations in cooling rate between 345° and 230°C during stress-relief procedure (Footnote J).

6.1.1 Aluminum alloy castings shall be supported and spaced in the furnace racks so as to permit uniform heating to the final heat-treat temperature.

6.1.2 Racking and spacing procedures shall be documented.

6.1.3 Racking and spacing procedures shall allow free circulation of the quench media throughout the workload so that all product surfaces receive an adequate quench to meet the requirements of the material specification.

6.1.4 Batch furnace loading of small parts in baskets to be water quenched shall be controlled by limiting the depth of parts in each layer and the minimum spacing between layers to preclude steam generated in any portion of the load from degrading the quench in another part of the load. Random packing of castings 1 in. [25 mm] or less in thickness should be limited to a maximum layer thickness of 3 in. [75 mm] with a minimum spacing of 3 in. [75 mm] between layers.

NOTE 3—Quenching by dumping small parts into water ensures access of the quenching media to all surfaces of each part.

## 7. Heat Treatment Procedures

7.1 *Solution Heat Treating*—Recommended solution heat-treatment times and temperatures for various heat-treatable aluminum castings appear in Tables 1 and 2 for sand and investment castings, Tables 3 and 4 for permanent mold-castings, Tables 5 and 6 for centrifugal castings, and Tables 7 and 8 for thixocast and rheocast castings.

7.2 *Soak Time*—The solution heat-treatment temperature specified in the tables is the temperature of the metal being treated. In the absence of a suitable metal temperature measuring device, the soaking times appearing in Tables 1-4 as applicable, may be used. Note that the time ranges quoted are, in most cases quite wide. Typically, structurally modified castings that are solidified rapidly require heat treat soak times close to the low end of each range. Examples include thin permanent mold castings and sand castings in which a fine microstructure is produced due to a rapid rate of cooling. Unmodified castings and those with thick sections will require soak times closer to the high end of the appropriate range. In Al-Si-Mg casting alloys which do not contain copper, it takes only an hour or two to place the silicon and magnesium into solid solution and to remove coring or microsegregation

present in the as-cast structure. The solution times called for in Tables 1-4 have been used primarily to change the size and shape of the silicon phase (see 8.4.3.3). In castings where the silicon phase is well modified acceptable elongations (depending on the customer requirements) may be obtained at soak times less than the recommended values specified in Tables 1-4. In any situation, the times chosen must result in castings which meet the required physical and mechanical properties.

7.3 *Quench*—During quenching it is important that cooling proceeds rapidly through the 750 to 500°F [400 to 260°C] range in order to avoid the type of premature precipitation detrimental to tensile properties and corrosion resistance. For casting alloys the quench delay should not exceed 45 s. Reduced quench delay time may be necessary to attain the tensile requirements shown in the product specifications for C355.0 and A356.0 sand-castings or investment-castings and 354.0, A356.0, A357.0, and A444.0 permanent mold castings.

### 7.4 Precipitation Heat Treatment (Artificial Aging):

7.4.1 Recommended times and temperature ranges for precipitation heat-treating various heat-treatable aluminum alloys appear in Tables 1 and 2 for sand castings, Tables 3 and 4 for permanent mold castings, Tables 5 and 6 for centrifugal castings, and Tables 7 and 8 for thixocast and rheocast castings.

7.4.2 Selection of the correct aging time involves knowledge of the aging curve for the alloy in question. As a casting precipitation hardens, there is a natural trade-off of ductility for strength. In choosing an aging time, this must be kept in mind as it relates to the application under consideration. Times towards the minimum in the precipitation hardening ranges in the tables will generate more ductility at a sacrifice in strength. Conversely, the long end of the range may well generate higher strength and hardness but a lower ductility.

7.4.3 At completion of precipitation time at temperature, the work shall be allowed to cool normally to room temperature.

## 8. Quality Assurance

8.1 *Responsibility for Inspection and Tests*—Unless otherwise specified in the contract, the heat treater is responsible for the performance of all inspection and test requirements specified herein.



TABLE 3 Recommended Heat Treatment for Permanent Mold Type Alloys (Inch-Pound Units)

Alloy <sup>A</sup>	Final Temper <sup>A</sup>	Solution Heat Treatment <sup>B, C</sup>		Precipitation Heat Treatment <sup>D</sup>	
		Metal Temperature, ±10°F	Time at Temperature, h	Metal Temperature, ±10°F	Time at Temperature, h
201.0	T6	960	2	room temperature	12 to 24
	T7	then 980	14 to 20	then 310	20
A201.0	T7	960	2	room temperature	12 to 24
	T7	then 980	14 to 20	then 370	5
	T6	955	2	room temperature	12 to 24
203.0	T6	then 985	14 to 20	then 370	5
	T4	955	2	room temperature	12 to 24
204.0	T4	then 1010	5	then 425	16
	T4	970	10	room temperature	5 days <sup>F</sup>
A206.0	T4	950	2	room temperature	5 days
	T43	then 985	14 to 20	room temperature	12 to 24
208.0	T6 <sup>F</sup>	950	2	then 320	0.5 to 1
	T7	then 985	14 to 20	room temperature	12 to 24
222.0	T6	950	2	then 310	20
	T65	then 985	14 to 20	room temperature	12 to 24
242.0	T571	950	2	then 370	5
	T61	then 985	14 to 20	310	2 to 5
296.0	T6	940	4 to 12	340	16 to 22
	T4	...	...	340	7 to 9
319.0	T6	940	4 to 12	340	22 to 26
	T5	...	...	or 400	7 to 9
332.0	T551	...	...	400	3 to 5
	T65	960	8	400	1 to 8
333.0	T5	...	...	...	...
	T6	940	6 to 12	310	2 to 5
354.0	T7	940	6 to 12	400	7 to 9
	T61	980	10 to 12	400	7 to 9
355.0	T62	980	10 to 12	500	2 to 5
	T51	...	...	room temperature	4 to 6
355.0	T6	980	4 to 12	then 310	8
	T62	980	4 to 12	room temperature	10 to 12
C355.0 <sup>G</sup>	T7	980	4 to 12	then 340	8
	T71	980	4 to 12	440	6 to 10
356.0	T61	980	6 to 12	440	7 to 9
	T51	...	...	310	2 to 5
356.0	T6	1000	4 to 12 <sup>H</sup>	340	14 to 18
	T6	1000	4 to 12 <sup>H</sup>	440	7 to 9
A356.0 <sup>G</sup>	T6	1000	4 to 12 <sup>H</sup>	440	2 to 5
	T7	1000	4 to 12 <sup>H</sup>	room temperature	8
357.0	T6	1000 <sup>I</sup>	8 <sup>H</sup>	then 310	6 to 12
	T61	1000 <sup>I</sup>	10 <sup>H</sup>	440	8
A357.0 <sup>G</sup>	T6	1000 <sup>I</sup>	8 <sup>H</sup>	475	3 to 6
	T61	1000 <sup>I</sup>	10 <sup>H</sup>	330	6 to 12
				room temperature	8
				then 310	8



TABLE 3 Continued

Alloy <sup>A</sup>	Final Temper <sup>A</sup>	Solution Heat Treatment <sup>B, C</sup>		Precipitation Heat Treatment <sup>D</sup>	
		Metal Temperature, ±10°F	Time at Temperature, h	Metal Temperature, ±10°F	Time at Temperature, h
359.0 <sup>G</sup>	T61	1000	10 to 14 <sup>H</sup>	room temperature then 310	8
	T62	1000	10 to 14 <sup>H</sup>	room temperature then 340	10 to 12
A390.0	T6	925	6 to 12	350	8
A444.0	T4	1000	8 to 12 <sup>H</sup>	...	...
705.0	T1	...	...	room temperature	21 days
	T5	...	...	210	10
707.0	T1	...	...	room temperature	21 days
	T5	...	...	210	8
711.0	T7	990	8 to 16	350	4 to 10
713.0	T1	...	...	room temperature	21 days
	T5	...	...	room temperature	21 days
850.0	T5	...	...	250	16
851.0	T5	...	...	430	7 to 9
	T6	950	6	430	7 to 9
852.0	T5	...	...	430	4
					7 to 9

<sup>A</sup> Designations conform to ANSI H35.1 and to Practice B275.

<sup>B</sup> Quench in water at 150 to 212°F except as noted.

<sup>C</sup> Time at solution temperature may be increased for section thickness over 1 in.

<sup>D</sup> No quenching required. Cool in still air outside the furnace.

<sup>E</sup> In order to expedite testing, alloy 204.0 test specimens may be precipitation heat treated after quenching by holding at 255°F for 2 h.

<sup>F</sup> This alloy is stress corrosion crack prone when in the T6 temper and should not be used in the T6 temper for applications in which even mildly corrosive environments may be encountered.

<sup>G</sup> Stress relieve for dimensional stability in the following manner: (1) Hold at 775 ± 25°F for 5 h; (2) Furnace cool to 650°F for 2 or more h; (3) Furnace cool to 450°F for not more than ¾ h; (4) Furnace cool to 250°F for approximately 2 h; (5) Cool to room temperature in still air outside the furnace.

<sup>H</sup> The solution times may be reduced when the silicon eutectic has been well modified such as when modified with Sr or Na.

<sup>I</sup> Solution treatment temperature of 1010°F may be used (to obtain higher solubility) provided no portion of the heat treat oven exceeds 1020°F.





TABLE 4 Recommended Heat Treatment for Permanent Mold Type Alloys [SI Units]

Alloy <sup>A</sup>	Final Temper <sup>A</sup>	Solution Heat Treatment <sup>B, C</sup>		Precipitation Heat Treatment <sup>D</sup>	
		Metal Temperature, ± 5°C	Time at Temperature, h	Metal Temperature, ± 5°C	Time at Temperature, h
2010	T6	515	2	room temperature	12 to 24
		then 525	14 to 20	then 155	20
	T7	515	2	room temperature	12 to 24
		then 525	14 to 20	then 190	5
A201.0	T7	515	2	room temperature	12 to 24
		then 530	14 to 20	then 190	5
203.0	T6	515	2	room temperature	12 to 24
		then 545	5	then 220	16
204.0	T4	520	10	room temperature	5 days <sup>E</sup>
A206.0	T4	510	2	room temperature	5 days
		then 530	14 to 20	room temperature	12 to 24
	T43	510	2	room temperature	then 160
		then 530	14 to 20	room temperature	0.5 to 1
	T6 <sup>F</sup>	510	2	room temperature	12 to 24
		then 530	14 to 20	then 155	20
	T7	510	2	room temperature	12 to 24
		then 530	14 to 20	then 190	5
	T6	505	4 to 12	155	2 to 5
208.0	T6	515	4 to 12	170	16 to 22
222.0	T551	510	8	or 205	7 to 9
	T65	510	4 to 12	170	22 to 26
242.0	T571	...	...	205	7 to 9
		...	...	155	3 to 5
	T61	515	4 to 12	...	1 to 8
	T6	510	8	155	...
296.0	T6	510	4 to 10	205	2 to 5
319.0	T4	505	4 to 12	205	7 to 9
	T6	505	4 to 12	205	7 to 9
332.0	T5	...	...	205	7 to 9
336.0	T551	515	8	205	7 to 9
	T65	515	8	155	2 to 5
333.0	T5	...	6 to 12	260	2 to 5
	T6	505	6 to 12	room temperature	4 to 6
	T7	505	10 to 12	then 155	8
354.0	T61	525	10 to 12	room temperature	10 to 12
	T62	525	10 to 12	then 170	8
355.0	T51	...	...	255	6 to 10
	T6	525	4 to 12	155	7 to 9
	T62	525	4 to 12	170	2 to 5
	T7	525	4 to 12	225	14 to 18
C355.0 <sup>G</sup>	T71	525	4 to 12	245	7 to 9
	T61	525	6 to 12	room temperature	3 to 6
356.0	T51	...	...	then 155	8
	T6	540	4 to 12 <sup>H</sup>	225	10 to 12
	T71	540	4 to 12 <sup>H</sup>	155	7 to 9
	T6	540	4 to 12 <sup>H</sup>	225	2 to 5
A356.0 <sup>G</sup>	T61	540	4 to 12 <sup>H</sup>	155	7 to 9
	T7	540	4 to 12 <sup>H</sup>	room temperature	2 to 5
	T71	540	4 to 12 <sup>H</sup>	then 155	8
		540	4 to 12 <sup>H</sup>	225	6 to 12
357.0	T6	540 <sup>I</sup>	8 <sup>H</sup>	245	3 to 6
	T61	540 <sup>I</sup>	10 <sup>H</sup>	165	6 to 12
A357.0 <sup>G</sup>				room temperature	8
				then 155	8



TABLE 4 Continued

Alloy <sup>A</sup>	Final Temper <sup>A</sup>	Solution Heat Treatment <sup>B, C</sup>		Precipitation Heat Treatment <sup>D</sup>	
		Metal Temperature, ± 5°C	Time at Temperature, h	Metal Temperature, ± 5°C	Time at Temperature, h
359.0 <sup>G</sup>	T61	540	10 to 14 <sup>H</sup>	room temperature then 155	8
	T62	540	10 to 14 <sup>H</sup>	room temperature then 170	10 to 12
A390.0	T6	495	6 to 12	175	8
	T4	540	8 to 12 <sup>H</sup>	...	...
705.0	T1	...	...	room temperature	21 days
	T5	...	...	100	10
707.0	T1	...	...	room temperature	21 days
	T5	...	...	99	8
711.0	T1	530	8 to 16	175	4 to 10
	T7	...	...	room temperature	21 days
713.0	T1	...	...	room temperature	21 days
	T5	...	...	120	16
850.0	T5	...	...	220	7 to 9
	T5	...	...	220	7 to 9
851.0	T6	510	6	220	4
	T5	...	...	220	7 to 9

<sup>A</sup> Designations conform to ANSI H35.1 and to Practice B275.

<sup>B</sup> Quench in water at 65 to 100°C except as noted.

<sup>C</sup> Time at solution temperature may be increased for section thickness over 25 mm.

<sup>D</sup> No quenching required. Cool in still air outside the furnace.

<sup>E</sup> In order to expedite testing, alloy 204.0 test specimens may be precipitation heat treated after quenching by holding at 125°C for 2 h.

<sup>F</sup> This alloy is stress corrosion crack prone when in the T6 temper and should not be used in the T6 temper for applications in which even mildly corrosive environments may be encountered.

<sup>G</sup> Stress relieve for dimensional stability in the following manner: (1) Hold at 415 ± 15°C for 5 h; (2) Furnace cool to 345°C for 2 or more h; (3) Furnace cool to 230°C for not more than ¾ h; (4) Furnace cool to 120°C for approximately 2 h; (5) Cool to room temperature in still air outside the furnace.

<sup>H</sup> The solution times may be reduced when the silicon eutectic has been well modified such as when modified with Sr or Na.

<sup>I</sup> Solution treatment temperature of 545°C may be used (to obtain higher solubility) provided no portion of the heat treat oven exceeds 550°C.

**TABLE 5 Recommended Heat Treatment for Centrifugal Casting Alloys (Inch-Pound Units)**

Alloy <sup>A</sup>	Final Temper <sup>A</sup>	Solution Heat Treatment <sup>B,C</sup>		Precipitation Heat Treatment <sup>D</sup>	
		Metal Temperature, ± 10°F	Time at Temperature, h	Metal Temperature, ± 10°F	Time at Temperature, h
356.0	T6	1000	4 to 12 <sup>E</sup>	310	2 to 5
505.0	T61	985	6 to 12	370	6 to 8
709.0	T61	870	9 to 12	250	24
850.0	T5	...	...	430	7 to 9

<sup>A</sup> Designations conform to ANSI H35.1 and to Practice B275.

<sup>B</sup> Quench in water at 150 to 212°F, except as noted.

<sup>C</sup> Time at solution temperature may be increased for section thickness over 1 in.

<sup>D</sup> No quenching required. Cool in still air outside the furnace.

<sup>E</sup> The solution times may be reduced when the silicon eutectic has been well modified such as when modified with Sr or Na.

**TABLE 6 Recommended Heat Treatment for Centrifugal Casting Alloys [SI Units]**

Alloy <sup>A</sup>	Final Temper <sup>A</sup>	Solution Heat Treatment <sup>B,C</sup>		Precipitation Heat Treatment <sup>D</sup>	
		Metal Temperature, ± 5°C	Time at Temperature, h	Metal Temperature, ± 5°C	Time at Temperature, h
356.0	T6	540	4 to 12 <sup>E</sup>	155	2 to 5
505.0	T61	530	6 to 12	190	6 to 8
709.0	T61	465	9 to 12	120	24
850.0	T5	...	...	220	7 to 9

<sup>A</sup> Designations conform to ANSI H35.1 and to Practice B275.

<sup>B</sup> Quench in water at 65 to 100°C, except as noted.

<sup>C</sup> Time at solution temperature may be increased for section thickness over 25 mm.

<sup>D</sup> No quenching required. Cool in still air outside the furnace.

<sup>E</sup> The solution times may be reduced when the silicon eutectic has been well modified such as when modified with Sr or Na.

**TABLE 7 Recommended Heat Treatment for Semi-Solid Thixocast and Rheocast Castings (Inch-Pound Units)<sup>A</sup>**

Alloy <sup>B</sup>	Final Temper <sup>B</sup>	Solution Heat Treatment <sup>C,D</sup>		Precipitation Heat Treatment <sup>E</sup>	
		Metal Temperature, ±10°F	Time at Temperature, h	Metal Temperature, ±10°F	Time at Temperature, h
319.0	T6	930	4	338	4
355.0	T5	...	...	338	10
356.0	T51	...	...	440	7-9
	T61	1000	4-12 <sup>F</sup>	155	6-12
	T71	1000	4-12 <sup>F</sup>	440	7-9
A356.0	T5	...	...	320	6-12
	T6	1000	4-10 <sup>F</sup>	320	3-6
357.0	T5	...	...	338	6
	T6	1000	10 <sup>F</sup>	338	6
366.0	T5	...	...	356	4-6
	T6	1000	4-10 <sup>F</sup>	356	4-6
380.0	T6	940	8	310	3
	T6	930	6	338	6

<sup>A</sup> Practices reprinted with permission from NADCA publication #403.

<sup>B</sup> Designations conform to ANSI H35.1/H35.1(M) and to Practice B275.

<sup>C</sup> Quench in water at 150 to 212°F except as noted.

<sup>D</sup> Time at solution temperature may be increased for section thickness over 1 in.

<sup>E</sup> No quenching required. Cool in still air outside the furnace.

<sup>F</sup> The solution times may be reduced when the silicon eutectic has been well modified such as when modified with Sr or Na.

8.1.1 The heat treater may use his own or any other suitable facilities for the performance of inspection and test requirements specified herein.

8.2 *Records*—Records shall be maintained for each furnace to show compliance with this standard. These records shall include the following: furnace number or description; size; temperature range of usage; whether used for solution heat treatment, precipitation heat treatment, or both; temperature(s) at which uniformity was surveyed; dates of each survey, number and locations of thermocouples used; and dates of major repairs or alterations (see 5.2.2).

8.2.1 The heat treater shall maintain records of all tests required by this practice and make them available for examination at the heat treaters facility.

### 8.3 Tests and Verification of Equipment:

#### 8.3.1 Surveillance Test Requirements:

8.3.1.1 Heat-treating equipment operated in accordance with documented procedures, shall have a demonstrated capability of producing material and components meeting the tensile and physical properties specified for each alloy heat-treated. Surveillance tests are required to verify the continued acceptability of the heat treatment.

**TABLE 8 Recommended Heat Treatment for Semi-Solid Thixocast and Rheocast Castings (SI Units) [Metric]<sup>A</sup>**

Alloy <sup>B</sup>	Final Temper <sup>B</sup>	Solution Heat Treatment <sup>C,D</sup>				Precipitation Heat Treatment <sup>E</sup>	
		Metal		Time at		Metal	
		Temperature, ± 5°C	Temperature, h	Temperature, ± 5°C	Temperature, h	Temperature, ± 5°C	Temperature, h
319.0	T6	500	4	170	4		
355.0	T5	...	...	170	10		
356.0	T51	...	...	225	7-9		
	T61	540	4–12 <sup>F</sup>	155	6-12		
	T71	540	4–12 <sup>F</sup>	225	7-9		
A356.0	T5	...	...	160	6-12		
	T6	540	4–10 <sup>F</sup>	160	3-6		
357.0	T5	...	...	170	6		
	T6	540	10 <sup>F</sup>	170	6		
366.0	T5	...	...	180	4-6		
	T6	540	4–10 <sup>F</sup>	180	4-6		
380.0	T6	505	8	155	3		
A390.0	T6	500	6	170	6		

<sup>A</sup> Practices reprinted with permission from NADCA publication #403.

<sup>B</sup> Designations conform to ANSI H35.1/H35.1(M) and to Practice B275.

<sup>C</sup> Quench in water at 65 to 100°C except as noted.

<sup>D</sup> Time at solution temperature may be increased for section thickness over 1 inch.

<sup>E</sup> No quenching required. Cool in still air outside the furnace.

<sup>F</sup> The solution times may be reduced when the silicon eutectic has been well modified such as when modified with Sr or Na.

8.3.1.2 *Frequency of Tests*—Tests shall be made once each month or more frequently as may be required. Testing one load per furnace per month shall constitute conformance with the requirements of this paragraph.

8.3.1.3 *Use of Production Test Results*—In all cases, the results of tests made to determine conformance of heat-treated material to the requirements of the respective material specifications are acceptable as evidence of the properties being obtained with the equipment and procedure employed.

8.3.1.4 When frequent testing is desired, per batch or daily, the use of separately cast tensile bars or cast-on coupons as a surveillance test for heat treatment is highly recommended. Separately cast bars shall be cast as per the recommendations of Specifications B26/B26M, B108/B108M, B618/B618M, B955/B955M, or B969 as appropriate to sand, permanent mold, investment, centrifugal, squeeze, thixocast, or rheocast castings respectively. The bars shall be processed through the heat treatment equipment together with the related castings. In the case of high strength castings in which cast-on coupons are used, these shall be processed as outlined in Specification B686/B686M.

#### 8.4 Surveillance Test Methods:

8.4.1 *Tensile Properties*—Tensile properties specified for the alloy involved shall be established by tension testing in accordance with Test Methods B557 [B557M].

8.4.2 When allowed by the casting specification, separately cast tensile bars may be used for both furnace surveillance and production tensile testing. Note that these bars shall meet a pass/fail material specification established for the given alloy and temper, as separately cast bars. The separately cast bars may differ from those machined from the castings, particularly with respect to ductility, a property very sensitive to section thickness and solidification rate. In any case, the required tests for casting properties shall conform to the respective casting specifications and any mechanical property requirements called out on the drawings. In the case of cast-on coupons the test results shall meet the highest strength requirements of the casting in accordance with Specification B686/B686M.

8.4.3 *Periodic Physical Property Testing*—The following physical property tests may be specified as part of the reaction or Failure Mode and Effects Analysis (FMEA) for dealing with failure to meet mechanical properties. They may also be specified as part of regular testing under circumstances in which the combination of alloy, temper, and service environment makes this advisable.


8.4.3.1 *Eutectic Melting and Porosity Resulting from Solution Heat Treatment*—Specimens from heat-treated product or samples shall be sectioned and the sections polished to appropriate fineness. The unetched surface shall be examined at 500 diameters magnification with a metallurgical microscope to detect evidence of porosity resulting from solution heat treatment. The sections may then be mildly etched (approximately 2 s) in an etchant and examined at 500 diameters magnification to detect evidence of eutectic melting.

8.4.3.2 *Intergranular Corrosion Test*—Intergranular Corrosion tests shall be conducted in accordance with the procedure outlined in Practice G110.

8.4.3.3 *Metallographic Examination of Eutectic Si*—In the case of structurally modified 3xx.0 and 4xx.0 alloys, which exhibit large amounts of Al-Si eutectic, the coarseness of the eutectic gives evidence of solution heat treatment. Sections taken from product or test specimens shall be compared to suitable known specimens in both the F temper and the T4, T6, or T7 tempers. The fine fibrous eutectic Si seen in structurally modified 3xx.0 castings in the F temper will have undergone ripening and spheroidization if properly solution heat treated. This test shall only be applied to structurally modified Al-Si based foundry alloys. A comparison pair of micrographs is reproduced in Fig. 1 as an example of the difference to be expected in Al-Si eutectic microstructure before and after solution heat treatment.

#### 8.5 Interpretation of Results:

8.5.1 Test specimens prepared in accordance with 8.3, and treated in accordance with the applicable parts of Section 7 shall meet the requirements specified below. Failure to meet the specified mechanical or physical requirements is reason to

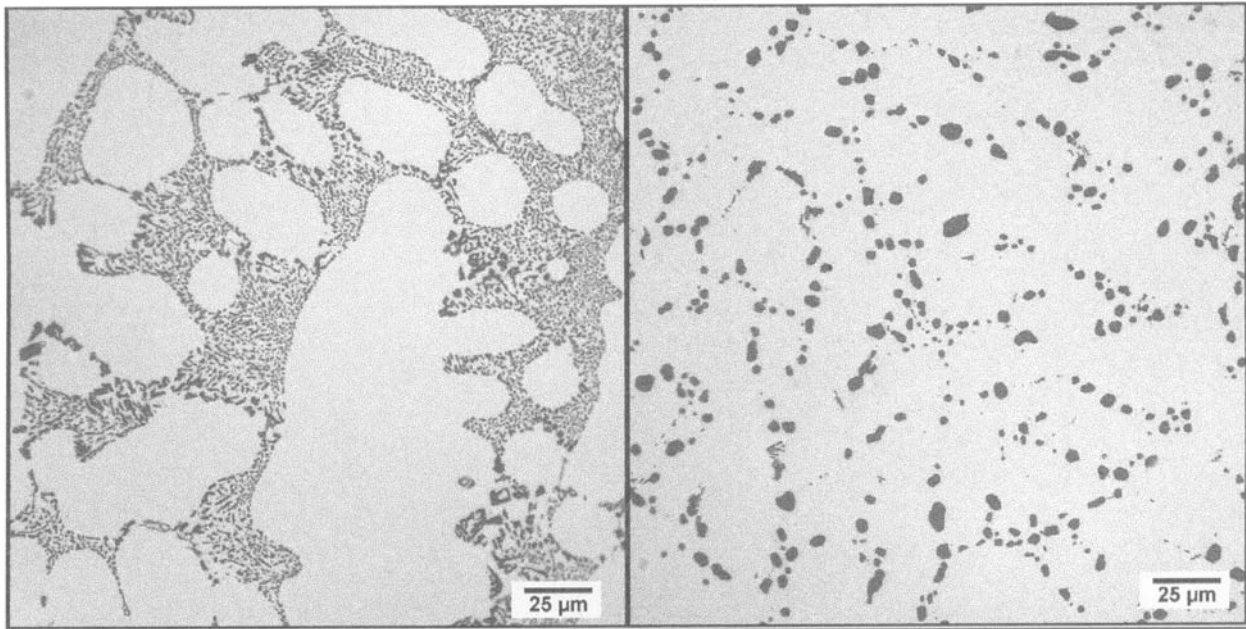

Comparison of the microstructure of a Sr modified A356 sample in the F temper (left) and after a full T6 heat treatment (right). The Si fibres spheroidize and ripen. For best results this comparison should only be made between samples solidified at the same rate as evidenced by the secondary dendrite arm spacing. Ideally, samples being compared should come from the same location in the same casting.

**FIG. 1 Microstructure Comparison**

disqualify the heat-treating equipment and associated process until the reason for the failure is determined and appropriate corrective action completed.

**8.5.2 Tensile Properties**—Heat-treated test samples or separately cast test bars shall exhibit tensile strength, yield strength, and elongation properties not less than those specified in applicable procurement specifications or detail drawings.

**8.5.3 Eutectic Melting**—Specimens shall be free from eutectic melting as evidenced by rosettes or eutectic structure at grain boundary triple points.

**8.5.4 Intergranular Corrosion**—There shall be no evidence of excessive intergranular corrosion. Consideration shall be given to size and thickness of the material in deciding whether the intergranular corrosion is excessive. Degree of susceptibility to intergranular corrosion shall be not greater than normally experienced when following this practice.

**8.5.5 Metallographic Examination of Eutectic Si**—The morphology of the Al-Si eutectic must be consistent with the heat treatment. Solution heat treating shall be deemed to have failed if the eutectic morphology is consistent with the F-temper.

**8.5.6 Rejection and Reheat Treatment**—Materials heat treated in the furnace since the time of the previous satisfactory

tests and found unsatisfactory shall be rejected or reheat treated (beginning with the solution heat treatment) in an acceptable furnace, depending on the character of the failed tests. Materials in which eutectic melting resulting from solution heat treatment is found shall be rejected and no reheat treatment permitted. Materials that fail for reasons other than those enumerated above may be heat treated again.

## 9. Precision and Bias

9.1 No information is presented about either precision or bias of metallurgical testing for evaluation of eutectic melting and heat treat induced porosity (8.4.3.1), or intergranular corrosion (8.4.3.2), since the test results are non-quantitative.

## 10. Keywords

10.1 aluminum alloys; centrifugal casting; investment casting; permanent mold casting; precipitation heat treatment; rheocast casting; sand casting; solution heat treatment; squeeze casting; thixocast casting

**SUMMARY OF CHANGES**

Committee B07 has identified the location of selected changes to this standard since the last issue (B917/B917M – 11) that may impact the use of this standard. (Approved May 1, 2012.)

- (1) Added footnote ‘K’ **Tables 1 and 2**, ‘H’ **Tables 3 and 4**, ‘E’ **Tables 5 and 6**, ‘F’ **Tables 7 and 8**.
- (2) Revised section **7.2**.

Committee B07 has identified the location of selected changes to this standard since the last issue (B917/B917M – 09) that may impact the use of this standard. (Approved May 1, 2011.)

- (1) Reference to **B955/B955M** and **B969** added to **2.2**.
- (2) Revised **7.1**, **7.4**, **8.3.1.4**, and **10**.
- (3) Added **Table 7** and **Table 8**.

Committee B07 has identified the location of selected changes to this standard since the last issue (B917/B917M – 08) that may impact the use of this standard. (Approved Nov. 1, 2009.)

- (1) Added Alloy A390.0-T6 to **Tables 1-4**.

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>*