



Standard Test Methods for Flow Rate of Metal Powders Using the Carney Funnel¹

This standard is issued under the fixed designation B964; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope*

1.1 These test methods cover the determination of a flow rate, by use of the Carney funnel, of metal powders and powder mixtures that do not readily flow through the Hall funnel of Test Method B213.

1.2 This is a non-destructive quantitative test performed in the laboratory.

1.3 With the exception of the values for density and the mass used to determine density, for which the use of gram per cubic centimetre (g/cm^3) and gram (g) units is the longstanding industry practice, the values in inch-pound units are to be regarded as standard. The values given in parentheses are mathematical conversions to SI units that are provided for information only, and are not considered standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*²

B213 Test Methods for Flow Rate of Metal Powders Using the Hall Flowmeter Funnel

B215 Practices for Sampling Metal Powders

B243 Terminology of Powder Metallurgy

B855 Test Method for Volumetric Flow Rate of Metal Powders Using the Arnold Meter and Hall Flowmeter Funnel

3. Terminology

3.1 Definitions of powder metallurgy (PM) terms can be found in Terminology B243.

¹ These test methods are under the jurisdiction of ASTM Committee B09 on Metal Powders and Metal Powder Products and are the direct responsibility of Subcommittee B09.02 on Base Metal Powders.

Current edition approved June 1, 2016. Published June 2016. Originally approved in 2009. Last previous edition approved in 2009 as B964-09. DOI: 10.1520/B0964-16.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

3.2 Definitions of Terms Specific to This Standard:

3.2.1 *Carney flow rate (FR_C), n*—the time required for a metal powder sample of specified mass to flow through the orifice in a Carney funnel according to a specified procedure.

3.3 3 Additional descriptive information is available in the Related Materials section of Vol 02.05 of the Annual Book of ASTM Standards.

4. Summary of Test Methods

4.1 A weighed mass of metal powder is timed as it flows through the orifice of a Carney funnel.

5. Significance and Use

5.1 The rate and uniformity of die cavity filling are related to flow properties, which thus influence production rates and uniformity of compacted parts.

5.2 The ability of a powder to flow is a function of interparticle friction. As interparticle friction increases, flow is slowed. Some powders, often fine powders and lubricated powder mixtures, may not flow through the Hall funnel of Test Method B213. Nevertheless, if a larger orifice is provided, such as in the Carney funnel, a meaningful flow rate may be determined, providing specific information for certain applications.

5.3 Test Method B213, using the Hall funnel, is the preferred method for determining the flowability of metal powders. The Carney funnel of these test methods should only be used when a powder will not flow through the Hall funnel. These test methods may also be used for comparison of several powders when some flow through the Hall funnel and some do not.

5.4 Humidity and moisture content influence flow rate. Wet or moist powders may not flow through either the Hall or the Carney funnel.

5.5 These test methods are based on flow of a specific mass of powder. If flow of a specific volume of powder is preferred, Test Method B855 may be used for powders that flow readily through the Hall funnel.

5.6 These test methods may be part of the purchase agreement between powder suppliers and powder metallurgy (PM) part producers, or it can be an internal quality control test by either the supplier or the end user.

*A Summary of Changes section appears at the end of this standard

6. Apparatus

6.1 *Carney Powder Flowmeter Funnel*³—A flowmeter funnel (Fig. 1) having an orifice of 0.200 ± 0.005 in. (5.08 ± 0.13 mm) in diameter.

6.2 *Stand*³—A stand (Fig. 1) to support the powder flowmeter funnel.

6.3 *Base*—A level, vibration-free base to support the powder flowmeter stand.

6.4 *Timing Device*—A stopwatch or other suitable timing device capable of measuring to the nearest 0.1 s.

6.5 *Balance*—Having a capacity of at least 250 g and a sensitivity of 0.01 g.

6.6 *Weighing Dish*—An ordinary laboratory weighing dish (pan), capable of containing the full mass of tested powder, and preferably made of metal to avoid powder sticking to the dish via electrostatic charges.

7. Sampling

7.1 A test sample of powder sufficient to run the desired number of flow tests shall be obtained in accordance with Practices B215.

7.2 Individual test portions, each of approximately the required mass, shall be obtained from the test sample in accordance with Practices B215.

8. Preparation of Apparatus

8.1 Clean the funnel with a clean, dry paper towel.

8.2 Clean the funnel orifice with a clean dry pipe cleaner.

³ The sole source of supply of the flowmeter funnel and stand known to the committee at this time is ACuPowder International, LLC, 901 Lehigh Avenue, Union, NJ 07083. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,¹ which you may attend.

9. Calibration of Apparatus

9.1 Plans are under way for developing a reference material that can be used to calibrate the Carney powder flowmeter funnel, similar to the material used for calibration of the Hall powder flowmeter funnel in Test Method B213.

9.2 In the absence of such a reference material, it is recommended that the dimensions of the Carney powder flowmeter funnel be checked periodically, at least every six months. If the dimensions are no longer within the specified tolerances, replace the flowmeter funnel.

10. Procedure

10.1 *Method 1*—Stationary Powder Start to Flow Measurement:

10.1.1 Weigh the required mass of powder, as sampled, into a clean weighing dish. Use 150.0 g of powder for ferrous and copper-based materials, and 200.0 g for tungsten-based powders. Appropriate quantities for other powders shall be determined by experiment.

10.1.2 Block the discharge orifice at the bottom of the funnel with a dry or gloved finger.

10.1.3 Carefully pour the test portion of powder into the center of the Carney funnel without any tapping, vibration or movement of the funnel.

10.1.4 Place the emptied weighing dish on the flowmeter stand directly under the funnel orifice.

10.1.5 Remove your finger from the discharge orifice.

10.1.6 If the powder fails to start flowing, one light tap on the funnel rim is permitted. Further tapping of the funnel, however, or poking or stirring of the powder in the funnel with a wire or any other implement is not permitted.

10.1.7 Start the timing device the instant the powder begins to exit the orifice.

10.1.8 Stop the timing device the instant the last of the powder exits the orifice.

10.1.9 Record the elapsed time to the nearest 0.1 s.

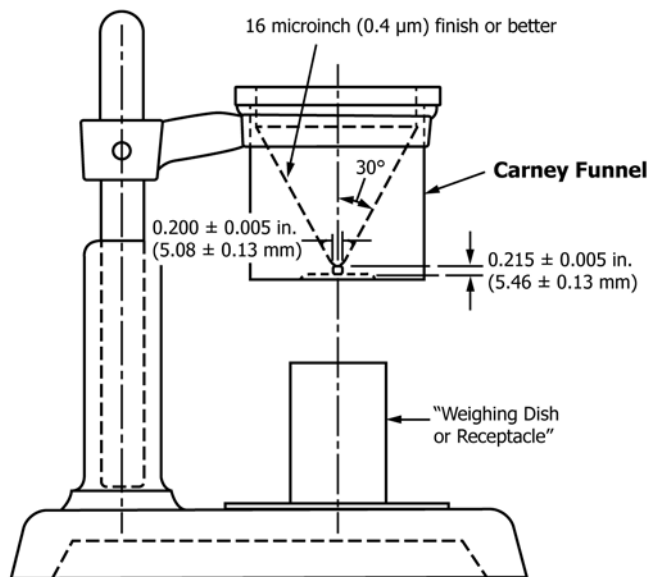


FIG. 1 Carney Funnel and Stand

10.1.10 More than one flow test may be run if desired. Use a fresh quantity of powder (test portion) for each flow test. Average the flow times.

10.2 *Method 2—Moving Powder Start to Flow Measurement:*

10.2.1 Place an empty receptacle directly under the discharge orifice.

10.2.2 Weigh the required mass of powder, as sampled, into a clean weighing dish. Use 150.0 g of powder for ferrous and copper-based materials, and 200.0 g for tungsten-based powders. Appropriate quantities for other powders shall be determined by experimentation.

10.2.3 Quickly pour the test portion of powder into the center of the funnel and start the timing device the instant the powder begins to exit the orifice.

10.2.4 Stop the timing device the instant the last of the powder exits the orifice.

10.2.5 Record the elapsed time to the nearest 0.1 s.

10.2.6 More than one flow test may be run if desired. Use a fresh quantity of powder for each flow test. Average the flow times.

11. Report

11.1 Report the Carney flow rate (FR_C) as “ $FR_C = t \text{ s}/M \text{ g}$,” where t is the flow time (in seconds) and M is the mass (in grams) of powder tested. For example, “ $FR_C = 8.3 \text{ s}/200 \text{ g}$,” or “ $FR_C = 27 \text{ s}/150 \text{ g}$.”

11.1.1 Report the Carney flow rate (FR_C) to the nearest 0.1 second for flow times less than or equal to 15 s.

11.1.2 Report the Carney flow rate (FR_C) to the nearest 1 second for flow times greater than 15 seconds.

11.2 Report the method of measurement used: Method 1 (stationary start) or Method 2 (moving start).

12. Precision and Bias

12.1 *Precision*—The precision of Test Methods B964 has not been fully determined. A Gage R&R study performed in a single laboratory, using only tungsten powders, shows a coefficient of variation (repeatability) of approximately 1%. A full round-robin interlaboratory study to determine the repeatability and reproducibility of the procedures in Test Methods B964 is underway. Results will be available in or before April 2021.

12.2 *Bias*—No information can be presented on the bias of the procedure in Test Methods B964 for measuring the Carney flow rate because no material having an accepted reference value is available.

13. Keywords

13.1 Carney Hall; Hall; flow rate; metal powder flow; powder flow

SUMMARY OF CHANGES

Committee B09 has identified the location of selected changes to this standard since the last issue (B964-09) that may impact the use of this standard. (Approved June 1, 2016.)

- (1) Reverted to inch-pound units, with g and g/cm^3 exceptions. (3) Added Summary of Changes section.
 (2) Updated precision statements (12.1).

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; http://www.copyright.com/