



# Standard Test Method for Specular Gloss of Plastic Films and Solid Plastics<sup>1</sup>

This standard is issued under the fixed designation D2457; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reappraisal.

## 1. Scope\*

1.1 This test method describes procedures for the measurement of gloss of plastic films and solid plastics, both opaque and transparent. It contains four separate gloss angles (**Note 1**):

- 1.1.1 60-deg, recommended for intermediate-gloss films,
- 1.1.2 20-deg, recommended for high-gloss films,
- 1.1.3 45-deg, recommended for intermediate and low-gloss films,
- 1.1.4 85-deg, recommended for intermediate and low gloss films, and
- 1.1.5 75-deg, recommended for plastic siding and soffit.

**NOTE 1**—The 85-deg, 75-deg, 60-deg, and 20-deg apparatus and method of measurement duplicate those in Test Method **D523** and **D3679**; those for the 45° procedure are similarly taken from Test Method **C346**.

1.2 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

**NOTE 2**—There is no known ISO equivalent to this standard.

## 2. Referenced Documents

2.1 *ASTM Standards*:<sup>2</sup>

- C346** Test Method for 45-deg Specular Gloss of Ceramic Materials
- D523** Test Method for Specular Gloss
- D3679** Specification for Rigid Poly(Vinyl Chloride) (PVC) Siding
- E284** Terminology of Appearance
- E691** Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method
- E1347** Test Method for Color and Color-Difference Measurement by Tristimulus Colorimetry
- E1349** Test Method for Reflectance Factor and Color by

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee **D20** on Plastics and is the direct responsibility of Subcommittee **D20.40** on Optical Properties.

Current edition approved April 1, 2013. Published April 2013. Originally approved in 1965. Last previous edition approved in 2008 as D2457 – 08<sup>ε1</sup>. DOI: 10.1520/D2457-13.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

## Spectrophotometry Using Bidirectional (45°:0° or 0°:45°) Geometry

## 3. Terminology

3.1 *Definitions*—For definitions of terms used in this test method, see Terminology **E284**.

## 4. Significance and Use

4.1 Specular gloss is used primarily as a measure of the shiny appearance of films and surfaces. Precise comparisons of gloss values are meaningful only when they refer to the same measurement procedure and same general type of material. In particular, gloss values for transparent films should not be compared with those for opaque films, and vice versa. Gloss is a complex attribute of a surface which cannot be completely measured by any single number.

4.2 Specular gloss usually varies with surface smoothness and flatness. It is sometimes used for comparative measurements of these surface properties.

## 5. Apparatus

5.1 *Instrumental Components*—Each apparatus (**Note 3**) shall consist of an incandescent light source furnishing an incident beam, means for locating the surface of the specimen, and a receptor located to receive the required pyramid of rays reflected by the specimen. The receptor shall be a photosensitive device responding to visible radiation.

**NOTE 3**—The 75-, 60-, and 20-deg procedures require apparatus identical to that specified in Test Method **D523**. The 45° procedure requires apparatus like that specified in Test Method **C346**.

5.2 *Geometric Conditions*—The axis of the incident beam shall be at one of the specified angles from the perpendicular to the specimen surface. The axis of the receptor shall be at the mirror reflection of the axis of the incident beam. With a flat piece of polished black glass or other front-surface mirror in specimen position, an image of the source shall be formed at the center of the receptor field stop (receptor window). The length of the illuminated area of the specimen shall be equal to not more than one third of the distance from the center of this area to the receptor field stop. The angular dimensions and tolerances of the geometry of the source and receptor shall be as indicated in **Table 1**. The angular dimensions of the receptor field stop are measured from the center of the test surface. The

\*A Summary of Changes section appears at the end of this standard

TABLE 1 Angular Dimensions and Tolerances of Geometry of Source and Receptor Field Stops

Geometry, deg	Incidence Angle, deg	Source Field Stop		Receptor Field Stop	
		In Plane of Measurement, deg	Perpendicular to Plane of Measurement, deg	In Plane of Measurement, deg	Perpendicular to Plane of Measurement, deg
75	75 ± 0.1		3.0 max		
60	60 ± 0.1	0.75 ± 0.25	3.0 max	4.4 ± 0.1	11.7 ± 0.2
20	20 ± 0.1	0.75 ± 0.25	3.0 max	1.80 ± 0.05	3.6 ± 0.1
45	45 ± 0.1	1.4 ± 0.4	3.0 ± 1.0	8.0 ± 0.1	10.0 ± 0.2

angular dimensions of the source field stop are mostly easily measured by the specimen-to-window angular size of the mirror image of the source formed in the receptor field stop. (See Fig. 1 for a generalized illustration of the dimensions.) The tolerances are chosen so that errors of no more than one gloss unit at any point on the scale will result from errors in the source and receptor aperture.

5.3 *Vignetting*—There shall be no vignetting of rays that lie within the field angles specified in 5.2.

5.4 *Spectral Conditions*—Results should not differ significantly from those obtained with a source-filter-photocell combination that is spectrally corrected to yield CIE luminous efficiency with CIE Source C. Since specular reflection is, in general, spectrally nonselective, spectral corrections need be applied only to highly chromatic, low-gloss specimens upon agreement of users of this test method.

5.5 *Measurement Mechanism*—The receptor-measurement mechanism shall give a numerical indication that is proportional to the light flux passing the receptor field stop within ±1 percent of full-scale reading.

6. Reference Standards

6.1 *Primary Working Standards* may be highly polished, plane, black glass surfaces. The specular reflectance, in percent, ( $R_s$ ) of such surfaces shall be computed by the following equation:

$$R_s \text{ (percent)} = 50 \left[ \left[ \frac{\cos i - \sqrt{n^2 - \sin^2 i}}{\cos i + \sqrt{n^2 - \sin^2 i}} \right]^2 + \left[ \frac{n^2 \cos i - \sqrt{n^2 - \sin^2 i}}{n^2 \cos i + \sqrt{n^2 - \sin^2 i}} \right]^2 \right] \tag{1}$$

where:

- $i$  = the specular (incidence) angle, and
- $n$  = the index of refraction of the surface.

Multiply the computed  $R_s$  at each angle by the scale factors shown in Table 2.

NOTE 4—On the 45 and 60° scales, a perfect mirror measures 1000.

6.2 *Secondary Working Standards* of ceramic tile, glass, porcelain enamel, or other materials having hard, flat, and uniform surfaces may be calibrated from the primary standard on a glossmeter determined to be in strict conformance with the requirements prescribed in 5.2.

7. Preparation and Selection of Test Specimens

7.1 This test method does not cover preparation techniques. Whenever a test for gloss requires the preparation of a test specimen, report the technique of specimen preparation.

7.2 Test results have been found to be seriously affected by surface warpage, waviness, or curvature. Ensure that specimen surfaces have good planarity. Perform tests with the directions of machine marks, or similar texture effects, both parallel and perpendicular to the plane of the axes of the incident and reflected beams, unless otherwise specified. (Note that this does not avoid the second-surface reflection.)

7.3 Surface test areas shall be kept free of soil and abrasion. Gloss is due chiefly to reflection at the surface; therefore, anything that changes the surface physically or chemically is likely to affect gloss.

8. Mounting Films for Measurement

8.1 Any nonrigid film must be mounted in a device that will hold it flat, but will not stretch the film while it is measured. Three different filmholding devices have each proved satisfactory for at least some types of films:

8.1.1 *Vacuum Plate* (see Fig. 2) is required for stiff films. Connect the vacuum plate by rubber tube to a vacuum pump or vacuum line. With thin, soft films it is sometimes necessary to use a valve and pressure gage and to limit the vacuum so as to keep from collapsing the soft film into the pores of the ground plate.

8.1.2 *Flat Plate* with two-side pressure-sensitive tape (see Fig. 3). Make sure each specimen is pulled smooth, but not stretched before holding it by the two strips of adhesive tape. Replace the tape whenever it loses its adhesiveness.

8.1.3 *Telescoping Ring or Hoop* (see Fig. 4)—To mount the specimen in the telescoping ring, lay the flexible film over the base (male) section and drop the top over the base. Push down carefully, taking care to pull the test film taut without stretching it. Measure the taut area.

8.2 *Backing for Films That Transmit Light*—A matt black backing or (even better) a black cavity must be placed behind any film that transmits light. Erroneous measurements will occur without a suitable trap or backing.

9. Procedure

9.1 Operate the glossmeter in accordance with the manufacturer’s instructions.

9.2 Calibrate the instrument at the start and completion of every period of glossmeter operation and during the operation

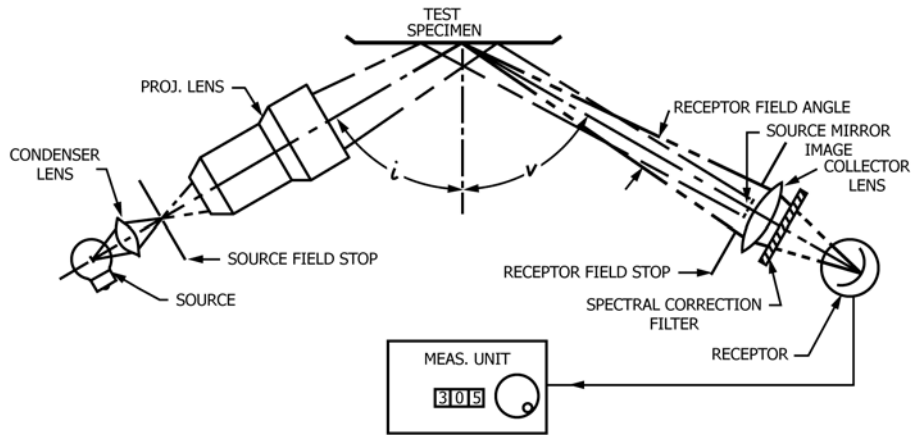


FIG. 1 Diagram of Glossmeter Showing Essential Components and Dimensions

TABLE 2 Scale Factors for Gloss Standards, Perfect Mirror and Perfect Matt White<sup>A</sup>

Geometry	Scale Factors (multiply $R_s$ of black glass standard by)	Value for Black Glass when $n = 1.540$	Value for Perfect Mirror	Value for Perfect Matt White
60°	10.0	95.8	1000	2.1
20°	20.3	92.3	2030	1.4
45°	10.0	55.9	1000	5.4

<sup>A</sup> The latter are useful for estimating corrections to gloss readings for reflection from sample backing (see Note 6).

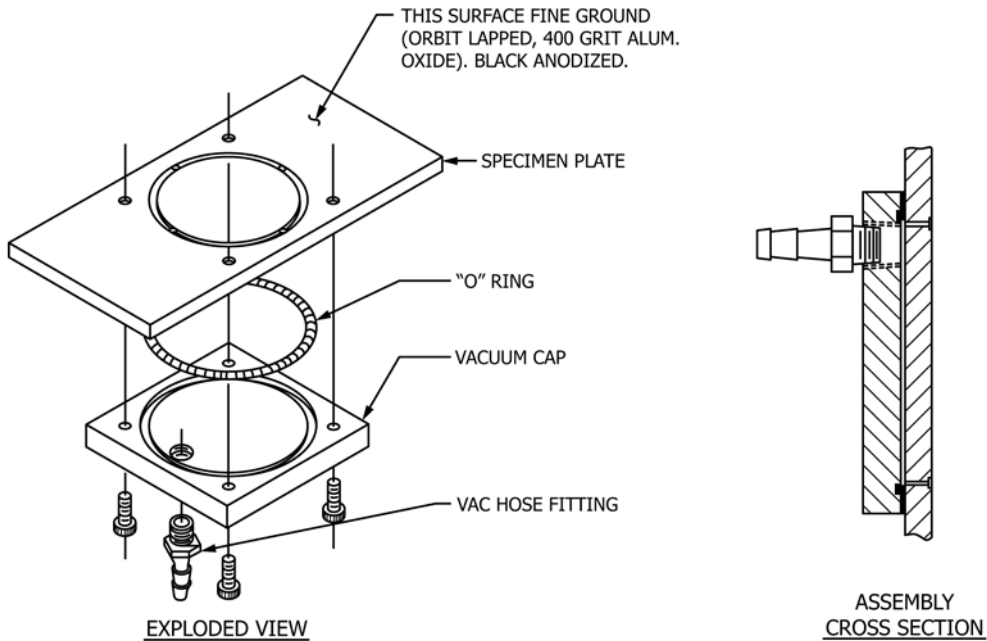


FIG. 2 Vacuum Plate Used to Hold Films Flat

at sufficiently frequent intervals to assure that the instrument response is practically constant. If at any time an instrument fails to repeat readings of the standard to within 2 percent of the prior setting, the intervening results should be rejected. To calibrate, adjust the instrument to read correctly the gloss of a highly polished standard, and then read the gloss of a standard having poorer image-forming characteristics. If the instrument reading for the second standard does not agree within 1 percent

of its assigned value, do not use the instrument without readjustment, preferably by the manufacturer.

NOTE 5—Correct readings on black-glass and intermediate standards do not guarantee instrument conformity to specification requirements. In addition to measurements with gloss standards, dimensional checks for conformity to the geometric requirements of 4.2 should be made.

9.3 Reduction of Amplification to Read over 100 Gloss Films on 0 to 100 Gloss Scale—A single smooth surface with

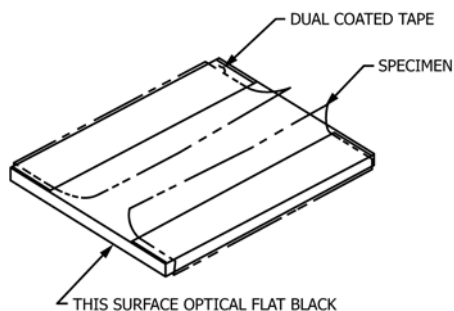


FIG. 3 Flat Plate with Two-Sided Pressure-Sensitive Tape Used to Hold Flexible Films for Gloss Measurement

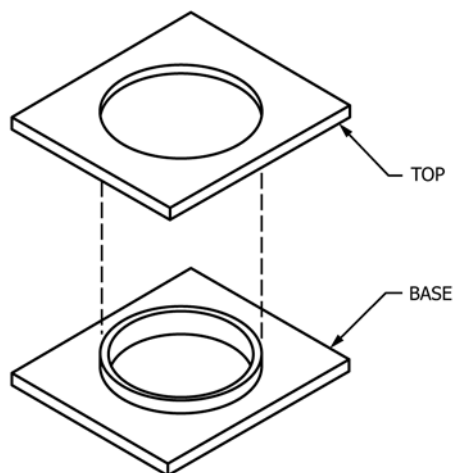


FIG. 4 Telescoping Ring Used to Hold Flexible Films for Gloss and Haze Measurements

refractive index of 1.567 measures 100 on both the 60 and 20-deg scales. Clear plastic films have two specularly reflecting surfaces. Even though they are less than perfectly smooth and less than 1.567 in refractive index, adding the reflections from the two surfaces frequently leads to gloss values of more than 100. If these gloss values are off-scale on the glossmeter used, recalibrate the instrument with the reading of the primary gloss standard set to a smaller value  $f$  (such as  $f = 50$ ) and correct the gloss readings by multiplying them by  $(100/f)$ .

9.4 Position each specimen (mounted in a holder in the case of films) in turn beneath (or on) the glossmeter. For specimens with extrusion lines or other direction texture effects, orient the marks both parallel and perpendicular to the plane of the axes of the incident and reflected beams. Measure at least three portions of the specimen surface in each direction to obtain an indication of uniformity. If no directionality is detected in the specimen, then the test may be performed only in the parallel or perpendicular orientation.

NOTE 6—In the case of films, it is often desirable to compare these readings with readings taken across the machine direction. Difference in the readings will relate to the prominence of the machine marks.

## 10. Report

10.1 Report the following information:

TABLE 3 Precision Data

		45° Gloss (13 Labs) <sup>A</sup>						
		Average	$S_r$ <sup>B</sup>	$S_R$ <sup>C</sup>	$V_r$ <sup>D</sup>	$V_R$ <sup>E</sup>	$I_r$ <sup>F</sup>	$I_R$ <sup>G</sup>
M	PP	9.87	0.230	1.48	2.3	15.0	0.64	4.14
O								
L	PP	38.7	0.82	3.00	2.1	7.7	2.38	8.40
D								
I	PP	53.6	0.79	1.16	1.5	2.2	2.21	3.25
N								
G	PC	62.4	1.03	1.03	1.6	1.6	2.88	2.88
F	LLDPE	83.6	1.35	3.11	1.6	3.7	3.78	8.71
I								
L	OPP	89.7	2.39	3.03	2.7	3.4	6.69	8.48
M	PET	115.2	0.86	3.49	0.7	3.0	2.41	9.77

<sup>A</sup>Results were obtained using unknown directional orientation.

<sup>B</sup> $S_r$  = within-laboratory standard deviation of a test result

<sup>C</sup> $S_R$  = between-laboratories standard deviation of a test result.

<sup>D</sup> $V_r$  =  $(S_r/\text{average}) * 100$

<sup>E</sup> $V_R$  =  $(S_R/\text{average}) * 100$

<sup>F</sup> $I_r$  =  $2.8 S_r$

<sup>G</sup> $I_R$  =  $2.8 S_R$

10.1.1 Type of specimen, its gloss (mean of three readings for each direction or mean of both directions), nominal thickness, whether transparent, and the specimen holder employed if specimen is a film.

10.1.2 All individual gloss readings for a specimen shall be reported if any of the gloss readings differ by more than 10 % from the average for that specimen.

10.1.3 Where preparation of the test specimen has been necessary, description or identification of the method of preparation,

10.1.4 Identification of the glossmeter by the manufacturer's name and model designation, and

10.1.5 Identification of the working standard or standards of gloss used.

NOTE 7—Diffuse Correction—It can be said that the light reflected by a specimen may be divided into one part reflected specularly in the direction of mirror reflection (associated with gloss) and another part reflected diffusely in all directions (associated with lightness on the white-gray-black scale). According to this picture, a gloss reading always needs to be diminished to compensate for that amount of the measured light attributable to diffuse reflectance. Although it is seldom possible in practice to analyze reflected light according to this picture and say exactly what part is diffuse and what part is specular, it is nevertheless frequent practice where gloss values of light and dark surfaces are being compared to “correct” (diminish) specular gloss settings for diffuse reflectance. If diffuse corrections are desired as additional information, measure 45-deg, 0-deg luminous directional reflectances of specimens in accordance with Test Methods E1347 or E1349. Multiply reflectance values in percentage by the following factors<sup>3</sup> for diffuse corrections in gloss units:

60-deg	0.021
20-deg	0.013
45-deg	0.055

## 11. Precision and Bias<sup>4</sup>

11.1 Table 3, Table 4 and Table 5 are based on a round robin conducted in 1987 and 1988 per Practice E691 involving seven test samples. The test results in Table 3 were from 13 labs; Table 4 from seven labs and Table 5 from five labs. For each

<sup>3</sup> Taken from Test Methods D523 and C346.

<sup>4</sup> Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D20-1175.

TABLE 4 Precision Data

	Average	60° Gloss (7 Labs) <sup>A</sup>					
		S <sub>r</sub> <sup>B</sup>	S <sub>R</sub> <sup>C</sup>	V <sub>r</sub> <sup>D</sup>	V <sub>R</sub> <sup>E</sup>	I <sub>r</sub> <sup>F</sup>	I <sub>R</sub> <sup>G</sup>
M PP	14.1	0.53	1.94	3.7	1.9	1.48	5.43
O							
L PP	80.6	1.35	2.34	1.7	2.3	3.78	6.55
D							
I PP	92.7	0.70	1.10	0.8	1.1	1.96	3.08
N							
G PC	99.8	0.71	6.16	0.7	6.2	1.99	17.2
F LLDPE	126.3	1.54	7.74	1.2	6.0	4.31	21.7
I							
L OPP	143.4	2.56	3.37	1.8	1.5	7.17	9.44
M PET	152.3	3.38	8.73	2.2	5.3	9.46	24.4

<sup>A</sup>Results were obtained using unknown directional orientation.

<sup>B</sup>S<sub>r</sub> = within-laboratory standard deviation of a test result.

<sup>C</sup>S<sub>R</sub> = between-laboratories standard deviation of a test result.

<sup>D</sup>V<sub>r</sub> = (S<sub>r</sub>/average) \*100

<sup>E</sup>V<sub>R</sub> = (S<sub>R</sub>/average) \*100

<sup>F</sup>I<sub>r</sub> = 2.8 S<sub>r</sub>

<sup>G</sup>I<sub>R</sub> = 2.8 S<sub>R</sub>

TABLE 5 Precision Data

	Average	20° Gloss (5 Labs) <sup>A</sup>					
		S <sub>r</sub> <sup>B</sup>	S <sub>R</sub> <sup>C</sup>	V <sub>r</sub> <sup>D</sup>	V <sub>R</sub> <sup>E</sup>	I <sub>r</sub> <sup>F</sup>	I <sub>R</sub> <sup>G</sup>
M PP	0.66	0.14	0.95	21.6	144.4	1.85	2.66
O							
L PP	19.1	1.04	3.19	5.4	16.7	2.91	8.93
D							
I PP	78.8	3.92	8.81	5.0	11.2	11.0	24.7
N							
G PC	96.9	2.37	4.83	2.4	5.0	6.64	13.5
F LLDPE	71.3	1.00	17.71	1.4	24.9	2.80	49.6
I							
L OPP	97.1	9.05	31.44	9.3	32.4	25.3	88.0
M PET	169.4	9.26	21.02	5.5	12.4	25.9	58.9

<sup>A</sup>Results were obtained using unknown directional orientation.

<sup>B</sup>S<sub>r</sub> = within-laboratory standard deviation of a test result.

<sup>C</sup>S<sub>R</sub> = between-laboratories standard deviation of a test result.

<sup>D</sup>V<sub>r</sub> = (S<sub>r</sub>/average) \*100

<sup>E</sup>V<sub>R</sub> = (S<sub>R</sub>/average) \*100

<sup>F</sup>I<sub>r</sub> = 2.8 S<sub>r</sub>

<sup>G</sup>I<sub>R</sub> = 2.8 S<sub>R</sub>

material, all samples were from a single roll of film or a single injection molding run. Each lab obtained two test results on separate days for each material.

11.2 **Table 6** is based on a round robin conducted in 2006 in accordance with Practice E691 involving four test samples. The test results in **Table 6** were from six labs. Each sample was an extruded piece of vinyl siding from a commercial extrusion line. Each lab measured the gloss three times per sample.

NOTE 8—Vinyl siding is designed to have a gloss of approximately 20 % independent of the color surface design.

11.3 **Warning**—The following explanations of I<sub>r</sub> and I<sub>R</sub> (11.4.1 – 11.4.3) are only intended to present a meaningful way

TABLE 6 Precision Data

	Average	75° Gloss (6 Labs) <sup>A</sup>					
		S <sub>r</sub> <sup>B</sup>	S <sub>R</sub> <sup>C</sup>	V <sub>r</sub> <sup>D</sup>	V <sub>R</sub> <sup>E</sup>	I <sub>r</sub> <sup>F</sup>	I <sub>R</sub> <sup>G</sup>
E Vinyl	20.40	0.52	1.42	2.5	7.0	1.46	4.00
X Siding A							
T Vinyl	22.94	0.49	0.66	2.1	2.9	1.37	1.85
R Siding B							
U Vinyl	21.53	0.55	0.90	2.6	4.2	1.54	2.52
S Siding C							
I Vinyl	21.44	0.37	0.61	3.8	2.8	1.04	1.71
O Siding D							
N							

<sup>A</sup>Results were obtained using unknown directional orientation.

<sup>B</sup>S<sub>r</sub> = within-laboratory standard deviation of a test result.

<sup>C</sup>S<sub>R</sub> = between-laboratories standard deviation of a test result.

<sup>D</sup>V<sub>r</sub> = (S<sub>r</sub>/average) \*100

<sup>E</sup>V<sub>R</sub> = (S<sub>R</sub>/average) \*100

<sup>F</sup>I<sub>r</sub> = 2.8 S<sub>r</sub>

<sup>G</sup>I<sub>R</sub> = 2.8 S<sub>R</sub>

of considering the approximate precision of the data in **Table 3**, **Table 4** and **Table 5** and should not be rigorously applied to acceptance or rejection of material, as those data are specific to the round robin and may not be representative of other lots, conditions, materials, or laboratories. Users of this test method should apply the principles outlined in Practice E691 to generate data specific to their laboratory and materials, or between specific laboratories. The principles of 11.4.1 – 11.4.3 would then be valid for such data.

11.4 *Concept of I<sub>r</sub> and I<sub>R</sub>*—If S<sub>r</sub> and S<sub>R</sub> have been calculated from a large enough body of data, (Use **Table 5** with caution as only five labs participated) and for test results that were averages from testing five specimens then the following definitions of S<sub>r</sub> and S<sub>R</sub> are valid.

11.4.1 *Repeatability I<sub>r</sub>*—In comparing two test results for the same material, obtained by the same operator using the same equipment on the same day, the two test results should be judged not equivalent if they differ by more than I<sub>r</sub> value for that material.

11.4.2 *Reproducibility I<sub>R</sub>*—In comparing two test results for the same material, obtained by different operators using different equipment on different days, the two test results should be judged not equivalent if they differ by more than the I<sub>R</sub> value for that material.

11.4.3 Any judgment made in accordance with 11.4.1 and 11.4.2 would have an approximate 95 % (0.95) probability of being correct.

11.5 *Bias* is a systematic error that contributes to the difference between a test result and a true (or reference) value. There are no recognized standards on which to base an estimate of bias for this test method.

12. Keywords

12.1 gloss; plastic films; solid plastics



**SUMMARY OF CHANGES**

Committee D20 has identified the location of selected changes to this standard since the last issue (D2457 - 08<sup>e1</sup>) that may impact the use of this standard. (April 1, 2013)

- (1) Added a new subsection **1.1.4**.
- (2) Revised **Note 1** and **Note 2**.

- (3) Added **D3679** to the Referenced Documents section since it was added to **Note 1**.

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or [service@astm.org](mailto:service@astm.org) (e-mail); or through the ASTM website ([www.astm.org](http://www.astm.org)). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>*