



Standard Test Method for Rubber Property—Resilience by Vertical Rebound¹

This standard is issued under the fixed designation D2632; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

This standard has been approved for use by agencies of the U.S. Department of Defense.

1. Scope

1.1 This test method covers the determination of impact resilience of solid rubber from measurement of the vertical rebound of a dropped mass.

1.2 This test method is not applicable to the testing of cellular rubbers or coated fabrics.

1.3 A standard test method for impact resilience and penetration of rubber by a rebound pendulum is described in Test Method [D1054](#).

1.4 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*²

- [D618 Practice for Conditioning Plastics for Testing](#)
- [D832 Practice for Rubber Conditioning For Low Temperature Testing](#)
- [D1054 Test Method for Rubber Property—Resilience Using a Goodyear-Healey Rebound Pendulum \(Withdrawn 2010\)](#)³
- [D1349 Practice for Rubber—Standard Conditions for Testing](#)
- [D1566 Terminology Relating to Rubber](#)
- [D3182 Practice for Rubber—Materials, Equipment, and Procedures for Mixing Standard Compounds and Preparing](#)

¹ This test method is under the jurisdiction of ASTM Committee [D11](#) on Rubber and is the direct responsibility of Subcommittee [D11.10](#) on Physical Testing.

Current edition approved Aug. 1, 2015. Published January 2016. Originally approved in 1967. Last previous edition approved in 2014 as D2632 – 14. DOI: 10.1520/D2632-15.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ The last approved version of this historical standard is referenced on www.astm.org.

Standard Vulcanized Sheets

[D3183 Practice for Rubber—Preparation of Pieces for Test Purposes from Products](#)

[D4483 Practice for Evaluating Precision for Test Method Standards in the Rubber and Carbon Black Manufacturing Industries](#)

2.2 *Other Documents:*⁴

[ISO-10012-1 Quality Assurance Requirements for Measuring Equipment—Part 1: Metrological Confirmation System for Measuring Equipment](#)⁵

[ANSI/NCSL-Z540-1 American National Standard for Calibration—Calibration Laboratories and Measuring and Test Equipment—General Requirements](#)⁶

3. Summary of Test Method

3.1 Resilience is determined as the ratio of rebound height to drop height of a metal plunger of prescribed mass and shape which is allowed to fall on the rubber specimen.

4. Significance and Use

4.1 Resilience is a function of both dynamic modulus and internal friction of a rubber. It is very sensitive to temperature changes and to depth of penetration of the plunger. Consequently, resilience values from one type of rebound instrument may not, in general, be predicted from results on another type of rebound instrument.

4.2 This test method is used for development and comparison of materials. It may not directly relate to end-use performance.

5. Apparatus

5.1 A diagram of the essential features and dimensions of the apparatus appears in [Fig. 1](#). It includes means for suspending a plunger at a given height above the specimen, its release, and measuring the subsequent rebound height.

⁴ This test method previously referenced MIL-STD-4662a *Military Standard: Calibration System Requirements*, which was subsequently canceled by the Department of Defense in February 1995. These are the DoD recommended replacement documents.

⁵ Available from the International Organization for Standardization, 1 rue de Varembe, Case postale 56, CH-1211, Geneva 20, Switzerland.

⁶ Available from the American National Standards Institute, 25 W. 43rd St., 4th Floor, New York, NY 10036.

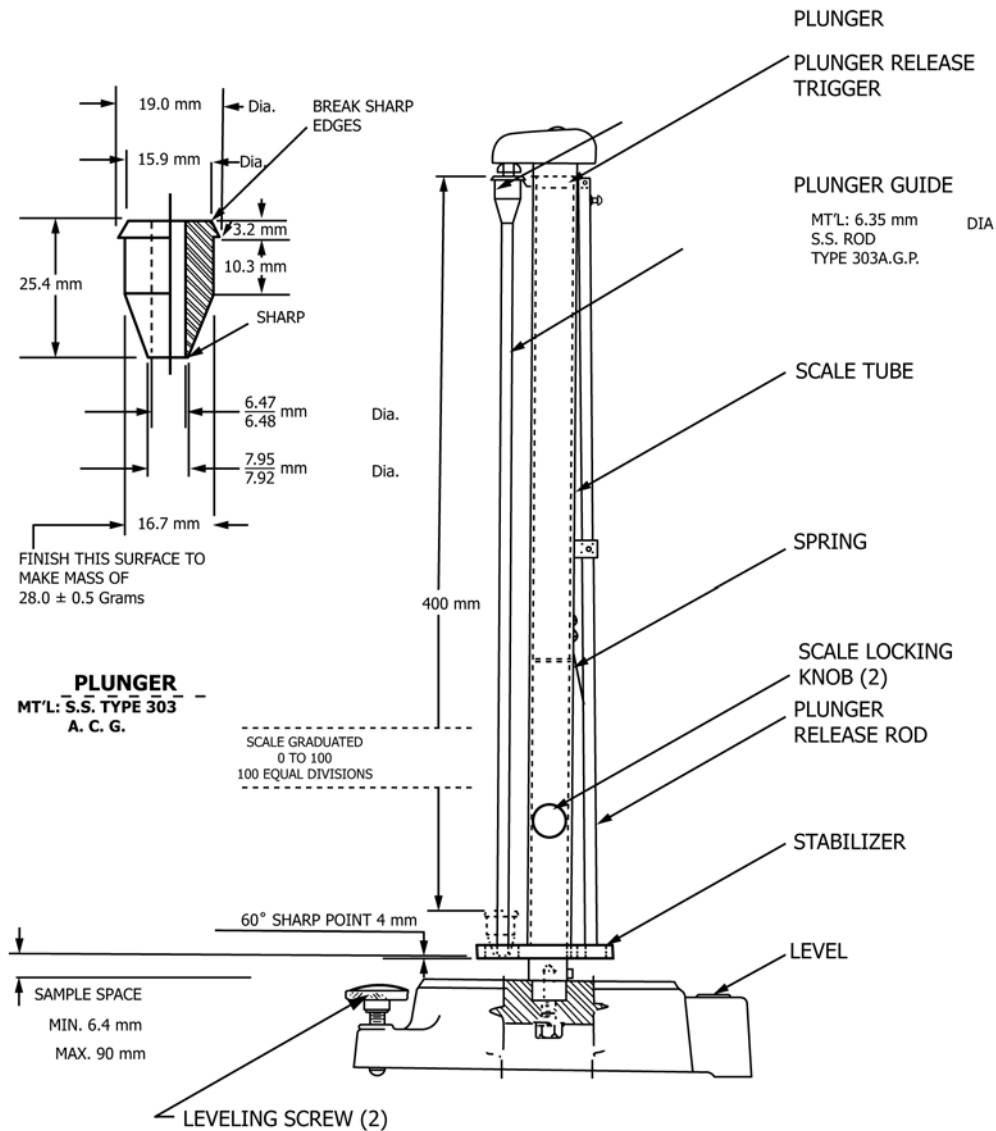


FIG. 1 Vertical Rebound Apparatus

5.1.1 Each resilience instrument shall have a unique identification number assigned and permanently and visibly imprinted or affixed upon it.

5.2 The plunger dimensions are also given in Fig. 1. Its mass shall be 28 ± 0.5 g.

5.3 The height of the drop point and of the resilience scale above the base of the instrument shall be adjustable so that the drop height is always 400 ± 1 mm (16 ± 0.04 in.) above the specimen surface. The resilience scale shall be marked in 100 equally spaced divisions.

5.3.1 The top of the plunger should be in line with 100 on the scale when the plunger is locked in the elevated position. Some models of the apparatus do not meet this requirement, but may be modified to do so.

5.4 The descent of the plunger and its ensuing ascent (rebound) is guided by a vertical rod (plunger guide). In order to minimize friction between the plunger and the vertical rod, a means shall be provided for leveling the base of the

instrument and adjusting the perpendicularity of the vertical rod to the instrument base.

5.4.1 The bottom of the vertical rod shall have a 4 mm diameter sharp point formed by a 60° angle, to secure the location of the bottommost end of the vertical rod. This point should indent the test specimen, providing a secure location for the free end of the guide rod.

5.4.2 The plunger shall be allowed to rest at the lowest point of travel and act as a guide to position the rod in the center of the stabilizer, as is visually practical under 10× magnification, as it is lowered onto the test specimen.

5.5 An opaque shield may be mounted between the operator and the plunger scale to be used for pass-fail test determinations. In use, the shield is adjusted so that its upper edge (or central-most graduation within a range) is even with the desired test determination. If the top of the rebounding plunger is visible above the shield (or within graduations demarcating a predetermined range of acceptability), the specimen passes.

6. Test Specimen

6.1 Mixing, sheeting, and curing shall be performed in accordance with Practices D3182 and D3183, unless otherwise specified.

6.2 The standard test specimen shall have a thickness of 12.5 ± 0.5 mm (0.50 ± 0.02 in.). The specimen shall be cut from a slab or specifically molded so that the point of plunger impact is a minimum distance of 14 mm (0.55 in.) from the edge of the specimen.

6.2.1 Any variation from the standard test specimen shall be reported (see 11.3).

6.3 Alternative specimens may be prepared by plying samples cut from a standard test slab. These samples shall be plied, without cementing, to the thickness required. Such plies shall be smooth, flat, and of uniform thickness. The results obtained with these specimens will not necessarily be identical with those obtained using a solid specimen of the same material and state of cure.

6.3.1 A thin specimen reaches a higher state of cure at a given time and temperature of cure than does a thicker specimen. Therefore, if plied specimens are used, their cure time should be appropriately lower than that of unplied specimens used for comparison.

6.4 Specimens may be prepared from finished products by cutting and buffing to the required dimensions, making sure that the opposing faces are parallel and that grain direction, where applicable, is uniform.

6.4.1 When buffing is required, it is recommended that only one side be buffed and the unbuffed side tested or, if both sides must be buffed, comparisons should not be made between buffed and unbuffed specimens.

7. Calibration

7.1 All materials, instruments, or equipment used for the determination of force, mass, or dimension in the calibration of this instrument or mechanical spring calibration device shall be traceable to the National Institute for Standards and Technology (NIST) or other internationally recognized organization parallel in nature and scope.

7.2 Calibration Device:

7.2.1 A mechanical spring calibration device (see Fig. 2) shall be used to calibrate this instrument.⁷

7.2.2 The force required to compress the spring 3.302 ± 0.0254 mm (0.130 ± 0.010 in.), while mounted in the receptacle, shall be 44.45 ± 0.4445 N (4532.6 ± 45.33 gf).

7.2.2.1 The spring shall be deflected 3.302 mm while mounted in the receptacle, and the force required shall be measured and reported.

7.2.2.2 A force of 44.45 N shall be applied to the spring while mounted in the receptacle, and the deflection shall be measured and reported.

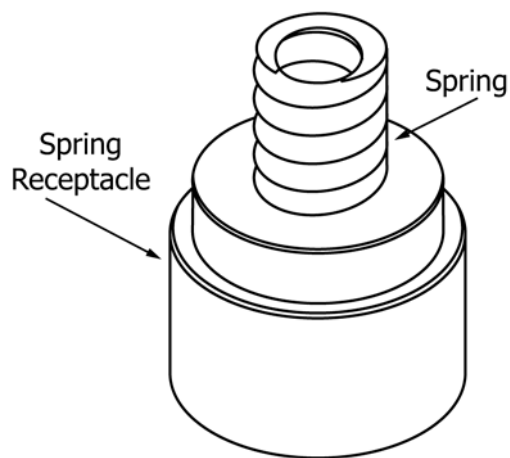


FIG. 2 Spring Calibration Device

7.2.2.3 The results of 7.2.2.1 and 7.2.2.2 shall be within the tolerances stated in 7.2.2 and, accordingly, shall determine the calibration of the spring.

7.2.2.4 The results achieved on a Resiliometer instrument, described in Section 5, that is in current calibration and properly used, will typically be in the range of 89 ± 2 Resiliometer points.

7.2.3 The mechanical spring calibration device shall have a unique identification number assigned and permanently and visibly imprinted or affixed upon it.

7.2.4 The resilience values assigned to an instrument using the mechanical spring calibration device shall be established at the time of calibration. These values are recorded as part of the calibration report.

7.3 Calibration Procedure:

7.3.1 The instrument shall be situated on a flat, level, vibration-free platform. The instrument shall be adjusted so that it is plumb and level, verified either by the integral level or by an external device designed for this purpose and in accordance with the manufacturer's instructions.

7.3.2 Perpendicularity of the vertical rod (plunger guide) to the support surface shall be verified by a device designed for this purpose and in accordance with the manufacturer's instructions.

7.3.3 The dimensions and mass of the plunger (see 5.2 and Fig. 1), the scale graduations, height of the drop point, and of the resilience scale above the base of the instrument (see 5.3 and Fig. 1) shall be verified by devices designed for this purpose.

7.3.4 The calibration procedure shall be performed in the standard laboratory atmosphere as defined in Practice D618. The instrument, mechanical spring calibration device, and any instrument or equipment used in the calibration procedure shall equilibrate at the standard laboratory temperature for a minimum of 12 h prior to performing the calibration.

7.3.5 Situate the mechanical spring calibration device securely in the instrument as described in Section 5 and in accordance with the manufacturer's instructions.

7.3.6 Make three sets of five readings, averaging each set. Each set becomes a test determination. Average the three test

⁷ The sole source of supply of the calibration device known to the committee at this time is CCSi, Inc., University Park, 221 Beaver Street, Akron, OH 44304. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,¹ which you may attend.

determinations to the nearest whole number. This whole number becomes the resilience calibration value for the instrument.

7.3.7 The instrument shall be considered in calibration if the resilience calibration value is within ± 2 points of the resilience calibration value established for the mechanical spring calibration device.

7.3.8 The resilience calibration value is assigned to the mechanical spring calibration device by the manufacturer or by the calibration service supplier using an identical resilience instrument, following the procedure outlined herein.

7.3.9 Calibration frequencies and calibration records should be kept in accordance with procedures outlined in the documents described in 2.2 or as required by the user's proprietary quality system.

7.4 Reference Spring:

7.4.1 If the instrument is provided with a mechanical spring device as a reference spring, this device shall have a resilience calibration value assigned, following the procedure outlined herein.

7.4.2 This device may be used to determine the state of calibration of the instrument during routine testing at a frequency determined by the user.

7.4.3 It shall not be used as a calibration device, however it should be routinely calibrated (refer to 7.2.2) to ensure the validity of its assigned values.

7.5 Report—The calibration report shall contain the following information:

7.5.1 Date of calibration.

7.5.2 Date of last calibration.

7.5.3 Manufacturer, type, model, and serial number of the instrument.

7.5.4 Manufacturer, type, model, and serial number of the mechanical spring calibration devices.

7.5.5 Values obtained (pre- and post-calibration results), following the procedure outlined in 7.3.

7.5.6 Ambient temperature.

7.5.7 Relative humidity.

7.5.8 Technician identification.

7.5.9 Applicable standards to which the instrument is calibrated.

7.5.10 Calibrating instrument information to include type, serial number, manufacturer, date of last calibration, and a statement of traceability of standards used to NIST or other acceptable organization. See 7.1.

8. Test Temperature

8.1 Test procedures shall be performed in the standard laboratory atmosphere as defined in Practice D1349 unless otherwise agreed upon between customer and supplier or between laboratories.

8.2 The instrument and test specimens shall be conditioned in the standard laboratory atmosphere as described in Practice D618 unless otherwise agreed upon between customer and supplier or between laboratories.

8.3 When test procedures are conducted at temperatures or conditions other than those specified in 8.1 and 8.2, they shall

be chosen from those enumerated in Practices D618, D832, or D1349 and the procedures described therein shall be followed unless otherwise agreed upon between customer and supplier or between laboratories.

9. Procedure

9.1 Level the instrument (see 7.3.1) and raise the plunger to the top of its guide rod.

9.2 Position the resilience scale (see 5.3) so that its full mass rests upon the specimen (see 5.3.1). Lock it in this position.

9.3 Release the plunger, ensuring that it slides freely on the vertical rod (plunger guide) (see 5.3.1).

9.3.1 Lateral force or impact on the guide rod may result in the hindrance of the descent of the plunger. Do not lubricate any part of the instrument. Always keep a standard test specimen under the stabilizer when not in use to avoid damage to the plunger.

9.4 Test three specimens from the same sample, making six test determinations on each specimen. Refer to Terminology D1566 for definitions of specimen and sample and to Practice D4483 for definitions of determinations and results.

9.4.1 Do not reposition the specimen once the initial test determination has been made.

9.4.2 Do not record the first three test determinations, as these condition and stabilize the specimen.

9.4.3 Record the last three test determinations.

10. Calculations

10.1 The instrument scale is divided into 100 equal parts, therefore a test determination is equal to the resilience value in percent.

10.2 Average the 4th, 5th, and 6th test determinations (see 9.4.3) from a specimen to calculate the test result from the specimen.

10.3 Average or alternatively, determine the median, the test results from the three specimens to the nearest whole number. This whole number is the resilience value of the sample. The median may also be used.

11. Report

11.1 Report the test results from the specimens (see 10.2).

11.2 Report the average or alternatively, the median, of the three test results (see 10.3).

11.3 Describe and report any variation from standard test specimen or standard conditions.

12. Precision and Bias

12.1 This precision and bias section has been prepared in accordance with Practice D4483. Refer to this practice for terminology and other statistical calculation details.

12.2 A Type 1 (interlaboratory) precision was evaluated in 1987. Both repeatability and reproducibility are short term, a period of a few days separates replicate test results. A test result is the average value, as specified by this test method, obtained on three determination(s) or measurement(s) of the property or parameter in question.

12.3 Three different materials were used in the interlaboratory program; these were tested in six laboratories on two different days.

12.4 The results of the precision calculations for repeatability and reproducibility are given in **Table 1**, in ascending order of material average or level, for each of the materials evaluated.

12.5 The precision of this test method may be expressed in the format of the following statements that use an appropriate value of r , R , (r) , or (R) , that is, that value to be used in decisions about test results (obtained with the test method). The *appropriate value* is that value of r or R associated with a mean level in the precision table closest to the mean level under consideration at any given time, for any given material in routine testing operations.

TABLE 1 Type 1 Precision

NOTE 1—

S_r = repeatability standard deviation.

r = repeatability.

(r) = repeatability (on relative basis, %).

S_R = reproducibility standard deviation.

R = reproducibility.

(R) = reproducibility (on relative basis, %).

Material	Average Test Level ^A	Within Laboratories			Between Laboratories		
		S_r	r	(r)	S_R	R	(R)
RA	37.9	0.48	1.36	3.58	2.65	7.50	19.8
RE	45.7	0.53	1.50	3.28	1.41	3.99	8.73
RF	48.5	0.59	1.66	3.42	1.37	3.89	8.02

^A Resilience value, scale reading.

12.6 *Repeatability*—The repeatability, r , of this test method has been established as the *appropriate value* tabulated in the precision table. Two single test results, obtained under normal test method procedure, that differ by more than this tabulated r (for any given level) must be considered as derived from different or non-identical sample populations.

12.7 *Reproducibility*—The reproducibility, R , of this test method has been established as the *appropriate value* tabulated in the precision table. Two single test results obtained in two different laboratories, under normal test method procedures, that differ by more than the tabulated R (for any given level) must be considered to have come from different or non-identical sample populations.

12.8 Repeatability and reproducibility expressed as a percentage of the mean level, (r) and (R) , have equivalent application statements as above for r and R . For the (r) and (R) statements, the difference in the two single test results is expressed as a percentage of the arithmetic mean of the two test results.

12.9 *Bias*—In test method terminology, bias is the difference between an average test value and the reference (or true) test property value. Reference values do not exist for this test method since the value (of the test property) is exclusively defined by the test method. Bias, therefore, cannot be determined.

13. Keywords

13.1 impact; rebound; resilience; rubber

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; http://www.copyright.com/