



# Standard Test Method for Determining Logarithmic Viscosity Number of Poly(Vinyl Chloride) (PVC) in Formulated Compounds<sup>1</sup>

This standard is issued under the fixed designation D3591; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This test method covers the determination of the logarithmic viscosity number of poly(vinyl chloride) (PVC) homopolymers after compounding or processing.

1.2 It is the basic assumption of this technique that the formulation of the compounded resin is known and that any additives present can be separated from the resin by extraction with diethyl ether. This is necessary to permit adjustment of the amount of sample used in the test to give a resin concentration in cyclohexanone of  $0.2 \pm 0.002$  g/100 mL.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* Specific precautionary statements are given in 7.3 and 8.4.1.

NOTE 1—This test method and ISO 1628-2 are not equivalent.

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>2</sup>

D445 Test Method for Kinematic Viscosity of Transparent and Opaque Liquids (and Calculation of Dynamic Viscosity)

D446 Specifications and Operating Instructions for Glass Capillary Kinematic Viscometers

D1243 Test Method for Dilute Solution Viscosity of Vinyl Chloride Polymers

D2124 Test Method for Analysis of Components in Poly(Vinyl Chloride) Compounds Using an Infrared Spectrophotometric Technique

E1 Specification for ASTM Liquid-in-Glass Thermometers

E691 Practice for Conducting an Interlaboratory Study to

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee D20 on Plastics and is the direct responsibility of Subcommittee D20.70 on Analytical Methods.

Current edition approved Feb. 1, 2011. Published March 2011. Originally approved in 1977. Last previous edition approved in 2003 as D3591 – 97(2003). DOI: 10.1520/D3591-97R11.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

### Determine the Precision of a Test Method

IEEE/ASTM SI-10 Standard for the Use of International System of Units (SI)

### 2.2 ISO Standard:

1628-2 Plastics—Determination of Viscosity Number and Limiting Viscosity Number—Part 2: Poly (Vinyl Chloride) Resins<sup>3</sup>

## 3. Terminology

3.1 Units and symbols used in this test method are those recommended in IEEE/ASTM SI-10.

### 3.2 Definitions of Terms Specific to This Standard:

3.2.1 The term *logarithmic viscosity number* is defined by the equation is 9.1.

## 4. Summary of Test Method

4.1 The sample is pressed into a thin film and extracted to remove the plasticizer.

4.2 The plasticizer-free film is dissolved in cyclohexanone and centrifuged to remove insoluble matter.

4.3 The viscosity of the cyclohexanone solution is measured in accordance with Test Method D1243.

## 5. Significance and Use

5.1 The logarithmic viscosity number provides information on the effect of compounding or processing of PVC.

5.2 Exposure of PVC compositions to shear or to high temperatures can result in a change in the logarithmic viscosity number of the resin.

## 6. Apparatus

6.1 *Centrifuge*, capable of 2500 rpm with 100-mL sample container.

6.2 *Heated Hydraulic Press*, capable of 620-kN ram force and a temperature of 165°C.

6.3 *Soxhlet Extraction Apparatus* with a 150-mL flask and a 27 by 100-mm thimble.

<sup>3</sup> Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, http://www.ansi.org.

6.4 Volumetric Flasks, 100-mL.

6.5 Viscometers.<sup>4</sup>

6.6 Infrared Spectrophotometer, see 5.4 of Method D2124.

7. Reagents

7.1 Cyclohexanone, high-purity (see Annex A1).

7.2 Diethyl Ether, anhydrous, reagent grade.

7.3 (Warning—Safety precautions should be taken to avoid personal contact, to eliminate toxic vapors, and to guard against explosive hazards in accordance with the hazardous nature of the particular reagent being used.)

8. Procedure

8.1 Prepare the PVC sample for extraction by pressing a film. The film should be 0.02 to 0.5 mm (1 to 2 mil) thick. Prepare two films in order to make duplicate runs.

8.1.1 Heat the hydraulic press to 165°C (330°F).

8.1.2 Place 2 g of sample between two sheets of aluminum foil and insert into the press.

8.1.3 Allow the sample to come to temperature for 2.5 min. During the next 0.5 min, increase the force on the sample to 620 kN. Maintain the force for 3 min, then cool while maintaining the force.

8.2 Weigh, to ±0.2 mg, approximately 1 g of pressed film into a 27 by 100-mm extraction thimble.

8.3 Place the thimble in a Soxhlet extraction apparatus fitted with a tared 150-mL flask, and extract with 120 mL of diethyl ether for 20 h.

8.4 Remove the tared 150-mL flask containing the diethyl ether and extracted plasticizer from the extraction apparatus, and gently heat to boil off the ether.

8.4.1 (Warning—When evaporating a quantity of ether to near dryness, precautions should be taken to guard against an explosive hazard, due to peroxides which may be in the ether or which may have been formed during use.)

8.5 Place the flask in an evacuated desiccator for a minimum of 1 h to remove the last traces of ether.

8.6 Weigh, to ±0.2 mg, the flask containing the extracted plasticizer.

8.7 Calculate the percentage plasticizer as follows:

$$\text{Plasticizer, \%} = (A \times 100)/B \tag{1}$$

where:

- A = weight of extracted plasticizer (7.6), and
- B = sample weight (7.2).

8.8 Dry the film to remove all solvent.

8.8.1 The extracted film must be free of plasticizer. Errors in excess of 10 % will result from small residual amounts of plasticizer. Examine the extracted film by infrared spectroscopy to ascertain that the plasticizer level is less than 0.05 % in order to obtain satisfactory results. An example for a carbonyl containing plasticizer is shown in Fig. 1 and Fig. 2.

<sup>4</sup> Cannon Fenske No. 75 or Ubbelohde No. 1 have been found satisfactory for this purpose.

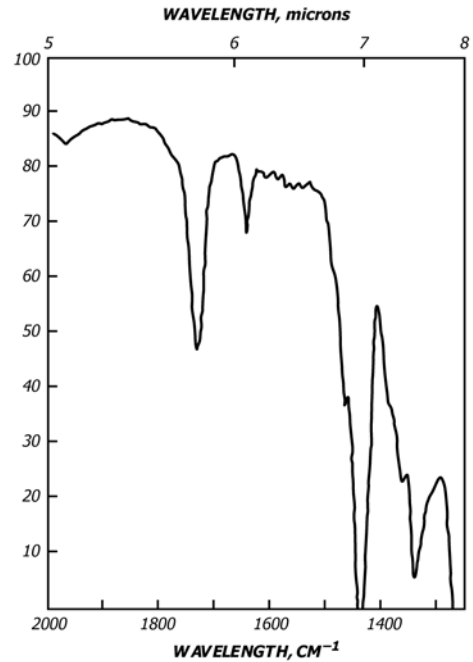


FIG. 1 Calibration Curve, 1 % Plasticizer in PVC Resin at 5.8 μm

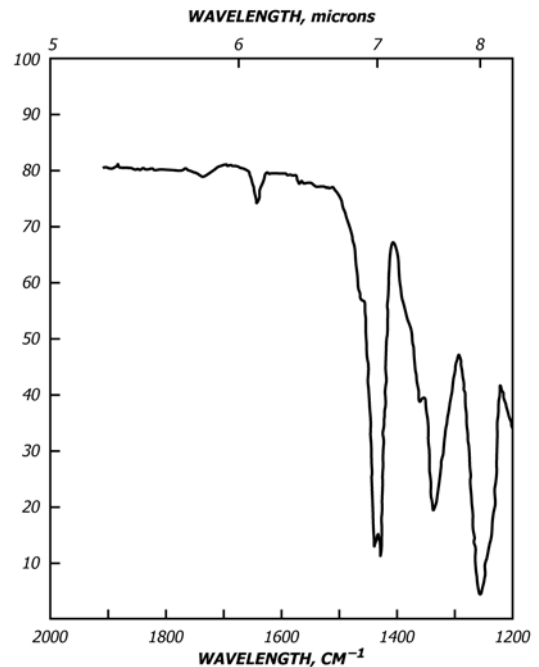


FIG. 2 Acceptable Residual Plasticizer, Less than 0.05 % at 5.8 μm

8.9 Determine the sample size of the extracted film that will yield 0.02 ± 0.002 g of PVC resin as follows:

$$F = \frac{100 - P}{R} \times 0.2 \tag{2}$$

where:

- F = weight of extracted film, g,
- P = plasticizer, %, and
- R = PVC, %.

8.10 Weigh a sample of extracted film as determined in 8.9 and transfer to a 100-mL glass-stopped volumetric flask. Take care to transfer all of the weighed sample.

8.11 Add 50 to 70 mL of cyclohexanone to the flask. Make sure that all the sample is in the solvent and not attached to the neck of the flask.

8.11.1 Use freshly distilled cyclohexanone. Serious errors of greater than 10 % can occur by not observing this factor. Details of the distillation are discussed in Annex A1.

8.12 Heat the flask to  $85 \pm 10^\circ\text{C}$  until the resin is dissolved. Occasional shaking will reduce the time required for solution. Heating should not exceed 12 h and should preferably be less to minimize degradation.

8.13 Cool the solution and adjust to a solution volume of 100 mL.

8.14 Centrifuge for 30 min at about 2500 rpm until the solution is reasonably clear. A slight haze has been found to make no significant difference in the measurements. (As a standard for this haze level, disperse 3 mg of Dythal<sup>5</sup> powder in 100 g of cyclohexanone; this 30-ppm suspension is known to give no effect on the measurements.)

8.15 Decant the supernatant liquid through a fritted-glass filter directly into the viscometer.

8.16 Place the viscometer in a water bath at a temperature of  $30 \pm 0.5^\circ\text{C}$  controlled to within  $\pm 0.01^\circ\text{C}$ . Allow at least 10 min for the viscometer to come to equilibrium.

8.17 Measure the efflux time of the solution and the pure solvent (aged at  $85 \pm 10^\circ\text{C}$ ) in the viscometer. The efflux time of the solution or the solvent should be within 0.1 % for repeated runs on the same filling.

8.18 Duplicate determination should be run.

## 9. Calculation

9.1 Calculate the logarithmic viscosity number as follows:

$$\text{Logarithmic viscosity number} = \ln(t/t_o)/C \quad (3)$$

where:

ln = natural logarithm,

$t$  = efflux time of solution, s,

$t_o$  = efflux time of solvent, s, and

$C$  = concentration, weight of PVC sample used per 100 mL of solution, g/100 mL.

9.2 The units of logarithmic viscosity number are millilitres per gram.

## 10. Report

10.1 Report the following information:

10.1.1 Complete identification of the sample tested,

10.1.2 Date,

10.1.3 Efflux time of solution,

10.1.4 Efflux time of solvent, and

10.1.5 Logarithmic viscosity number.

**TABLE 1 Logarithmic Viscosity Number (Inherent Viscosity) of Formulated PVC Compounds at 30°C**

Material	Mean	$S_r$	$S_R$
PVC-1	1.0006	0.00953	0.0430
PVC-4	1.2425	0.01138	0.0430
PVC-5	1.2322	0.00584	0.0609
PVC-6	1.2619	0.00971	0.0411
PVC-7	0.9605	0.01062	0.0695
Overall average		0.0097	0.053

Based on five laboratories, two determinations. PVC-1 used four laboratories.

## 11. Precision and Bias

11.1 Table 1 is based on a round robin<sup>5,6</sup> conducted in 1976 in accordance with Practice E691, involving five materials tested by five laboratories. For each material, all the samples were prepared at one source, but the individual specimens were prepared at the laboratories which tested them. Each test result was the average of two individual determinations. Each laboratory obtained two test results for each material.

NOTE 2—The explanations of  $r$  and  $R$  (11.2 – 11.2.3) only are intended to present a meaningful way of considering the approximate precision of this test method. The data in Table 1 should not be applied to acceptance or rejection of materials, as these data apply only to the materials tested in the round robin and are unlikely to be rigorously representative of other lots formulations, conditions, materials, or laboratories. Users of this test method should apply the principles outlined in Practice E691 to generate data specific to their materials and laboratory (or between specific laboratories). The principles of 11.2 – 11.2.3 then would be valid for such data.

11.2 Concept of  $r$  and  $R$  in Table 1—If  $S_r$  and  $S_R$  have been calculated from a large enough body of data, and for test results that were averages from testing two specimens for each test result, then:

11.2.1 Repeatability—Two test results obtained within one laboratory shall be judged not equivalent if they differ by more than the  $r$  value for that material. The  $r$  value is the interval representing the critical difference between two test results for the same material, obtained by the same operator using the same equipment on the same day in the same laboratory.

11.2.2 Reproducibility—Two test results obtained by different laboratories shall be judged not equivalent if they differ by more than the  $R$  value for that material. The  $R$  value is the interval representing the critical difference between two test results for the same material, obtained by different operators using different equipment in different laboratories. Only five laboratories participated in this round robin, making this value somewhat questionable.

11.2.3 Any judgment in accordance with 11.2.1 or 11.2.2 would have an approximate 95 % (0.95) probability of being correct, provided that the correct number of laboratories had participated.

11.3 There are no recognized standards by which to estimate bias of this test method.

<sup>5</sup> The sole source of supply of the Dythal powder known to the committee at this time is National Lead Co., 111 Broadway, New York, NY 10006. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee<sup>1</sup>, which you may attend.

<sup>6</sup> Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D20-1057.

## 12. Keywords

12.1 formulations; logarithmic viscosity number; poly(vinyl chloride); PVC

## ANNEX

### (Mandatory Information)

#### A1. DISTILLATION OF CYCLOHEXANONE

A1.1 The distillation of the cyclohexanone is important, particularly if the refractive index of the solvent is above 1.4500 at 20°C. To obtain the required purity, a 5 to 10-plate column is recommended. Columns in excess of 1 plate are required.

A1.2 As a measure of the purity of the cyclohexanone, the solvent should have a refractive index in the range from 1.4498 to 1.4499 at 20°C.

A1.3 It is preferable to use up the freshly distilled cyclohexanone within 1 week. The solvent should still be good for a longer time period if (1) the liquid has not taken on a yellow tint, (2) the refractive index has not increased above 1.4500, or (3) the viscosity is 1.95 mm<sup>2</sup> /s (1.95 cSt) or less.

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>*