



Standard Practice for Calibrating Moisture Analyzers¹

This standard is issued under the fixed designation D4178; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This practice covers a calibration technique based on the preparation of standards of known water content. This technique is applicable to the production of standards between 20 and 2000 cm³/m³ water.

1.2 The values stated in SI units are to be regarded as standard. The values given in parentheses are for information only.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Summary of Practice²

2.1 The practice is based on the principle that ice has a vapor pressure of 0.611 kPa at 0°C. Therefore, when a carrier gas at a constant gauge pressure of 207 kPa (30 psig) is passed through a molecular sieve saturated with water and held at 0°C, the total pressure is equal to 207 kPa plus 98 kPa (one atmosphere) and the water concentration of the gas leaving the molecular sieve is $[0.611/(207 + 98)] \times 10^6$ ppm or 2000 ppm volume water, regardless of flow.

2.1.1 A carrier gas at a constant gauge pressure of 207 kPa is passed through a molecular sieve drier and then routed over a molecular sieve support saturated with water and equilibrated at 0°C.

2.1.2 By blending different volumes of the wet carrier gas with dried carrier gas, gas standards of known water concentration can be prepared.

2.2 The moisture analyzer to be calibrated is then connected to the source of the gas standard of known water concentration.

¹ This practice is under the jurisdiction of ASTM Committee D02 on Petroleum Products, Liquid Fuels, and Lubricants and is the direct responsibility of Subcommittee D02.D0 on Hydrocarbons for Chemical and Special Uses.

Current edition approved April 15, 2012. Published May 2012. Originally approved in 1982. Last previous edition approved in 2005 as D4178–82(2005). DOI: 10.1520/D4178-82R12.

² For a more complete discussion of this procedure, see Mator, R. T., "Trace Moisture Analyzers and Their Calibration," *Proceedings of the 20th Annual ISA Analysis Instrumentation Symposium, May 12-15, 1974, Pittsburgh, PA*, "Session: Sampling and Calibration Systems," 1974, p. 125.

3. Significance and Use

3.1 This practice is intended to provide a method to calibrate moisture analyzers used on-stream or in the laboratory.

4. Apparatus

4.1 *Ice Bath Primary Standard Moisture Apparatus*—Fig. 1 illustrates a typical system.

4.2 *Wet Test Meter*, 1-L divisions.

4.3 *Bubble Meter*, graduated in cubic centimetres.

4.4 *Pressure Gauge*—A Bourdon-type spring gauge of test gauge quality, 100 to 250 mm in diameter, with a scale range from 0 to 400 kPa (0 to 60 psi), maximum intermediate graduations of 1.5 kPa (0.25 psi).

4.5 *Wet Mole Sieve 5A*, 60/80 mesh (other mesh sizes may be used, except powder).

5. Preparation of Apparatus

5.1 Saturate mole sieve with water.

5.1.1 Cover in beaker enough mole sieve to fill the wet mole sieve container. Add water to cover mole sieve. Let stand overnight.

5.1.2 Drain the excess water by pouring the mole sieve slurry into a filtering funnel and letting all the free water drain out.

NOTE 1—The useful lifetime of the wet mole sieve is not known. It is recommended that the procedure described in 5.1.1 and 5.1.2 be followed prior to each calibration.

6. Procedure

6.1 Fill the ice bath bucket for the primary standard apparatus one third full of water; then add ice to bring the level to full.

6.2 Close the wet flow and the diluent flow needle valves.

6.3 Turn on the carrier gas supply (nitrogen or air) and adjust the regulator to 207 kPa (30 psig).

6.4 Open the diluent flow needle valve to obtain a carrier gas flow of 1 L/min, as measured with a wet test meter.

6.5 Allow the apparatus to equilibrate for 1 h. This allows the wet mole sieve to equilibrate at 0°C.

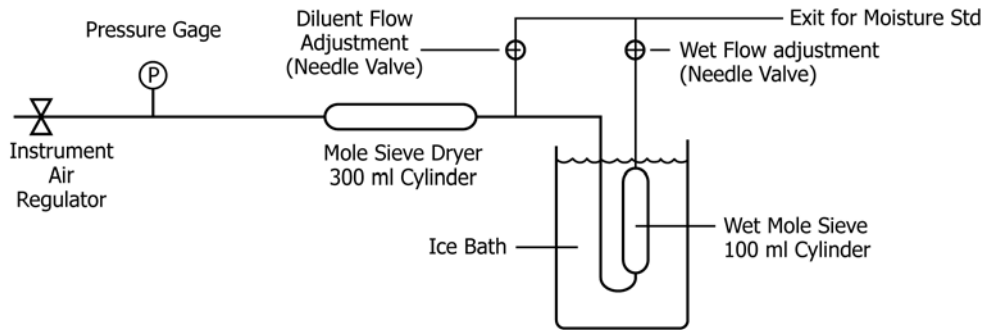


FIG. 1 Schematic of Ice Bath “Primary Standard” Moisture Apparatus

6.6 After 1 h, attach the moisture analyzer to be calibrated and check that the blank moisture content of the carrier gas is 6 ppm or less.

6.7 Turn off the diluent flow, cm^3/m^3 .

6.8 Attach a bubble meter to the exit of the apparatus and check that there is no flow through the system.

6.9 Adjust the wet flow needle valve to obtain a flow of $40 \text{ cm}^3/\text{min}$, as measured with a bubble meter.

6.10 In a similar manner, adjust the diluent flow needle valve to obtain a *total* flow of $200 \text{ cm}^3/\text{min}$, as measured with a bubble meter.

6.11 Connect the moisture analyzer to be calibrated to the exit of the “primary standard” moisture apparatus and allow its probe to equilibrate (10 to 15 min).

6.12 The analyzer should read the calculated value of 400 ppm for a carrier gas pressure of 207 kPa gauge. If it does not, adjust the necessary analyzer controls to obtain the correct reading.

6.13 Turn off both the wet flow and the diluent flow needles valves.

6.14 Attach a bubble meter to the exit of the apparatus and check that there is no flow through the system.

6.15 Adjust the wet flow needle valve to obtain a flow of $10 \text{ cm}^3/\text{min}$ using a bubble meter, and then adjust the diluent flow needle valve to obtain a *total* flow of 1 L/min. Use a wet test meter to check the total flow.

6.16 After the analyzer equilibrates (10 to 15 min), check to see that it reads the correct calculated value of $20 \text{ cm}^3/\text{m}^3$ plus the blank moisture content found in 6.6 for 207 kPa gauge carrier gas supply.

6.17 When the analyzer reads correctly at the 400-ppm level but is not within ± 2 ppm of the 20 ppm plus the blank moisture content value, then the sensor may be bad and needs replacing.

7. Calculation

7.1 Calculate water concentration in saturated gas (wet flow) as follows:

$$P_{\text{H}_2\text{O}} @ 0^\circ\text{C} = 0.611 \text{ kPa} \quad (1)$$

$$P_{\text{total}} = A \text{ kPa} + 98 \text{ kPa gauge}$$

A kPa = carrier gas pressure (should be 207 ± 2 kPa)

$$\frac{C_{\text{H}_2\text{O}}}{P_{\text{total}}} = \frac{(P_{\text{H}_2\text{O}})(10^6)}{207 + 98} = \frac{(0.611)(10^6)}{207 + 98} = 2000 \text{ cm}^3/\text{m}^3$$

where:

- $P_{\text{H}_2\text{O}} @ 0^\circ\text{C}$ = vapor pressure of water at 0°C ,
- P_{total} = total pressure applied to the water on the molecular sieve, and
- $C_{\text{H}_2\text{O}}$ = cm^3/m^3 volume moisture in wet flow.

7.2 Calculate water concentration in blended gas (total flow) as follows:


$$CT_{\text{H}_2\text{O}} = \frac{(\text{wet flow})(C_{\text{H}_2\text{O}})}{\text{total flow}} + \text{ppm H}_2\text{O blank} \quad (2)$$

where:

- $C_{\text{H}_2\text{O}}$ = cm^3/m^3 moisture in wet flow,
- $CT_{\text{H}_2\text{O}}$ = cm^3/m^3 moisture in total flow, and
- total flow = wet flow plus diluent flow.

8. Keywords

8.1 calibration; carrier gas; moisture analyzer; water content

 **D4178 – 82 (2012)**

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>