



# Standard Test Methods for Mechanical Properties of Lumber and Wood-Base Structural Material<sup>1</sup>

This standard is issued under the fixed designation D4761; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## INTRODUCTION

Numerous evaluations of the mechanical properties of wood-based structural material have been satisfactorily conducted since the late 1920s, using Test Methods [D198](#). Those methods are best suited to a laboratory environment and are adaptable to a variety of products such as stress-graded lumber, sawn timber, laminated timbers, wood-plywood composite members, reinforced and prestressed timbers.

The procedures presented in these test methods have been derived from those set forth in Test Methods [D198](#). They are intended primarily for application to stress-graded lumber, but can be used for other wood-base structural material as well. The procedures are more flexible than those in Test Methods [D198](#), making testing in a nonlaboratory environment more feasible. Thus the test methods can be used on production sites for field testing and quality control, as well as in laboratories for research applications. Key differences from Test Methods [D198](#) are the testing speed, the deflection-measuring procedures for test specimens under load, and the detail of data reporting. Furthermore, the test methods do not require that specimens be loaded to failure.

Since these test methods allow latitude in testing procedures, the procedures used shall be fully documented in the test report. It may also be desirable to correlate the results from tests carried out according to these test methods with test results obtained through the use of a traditional procedure, such as that set forth in Test Methods [D198](#).

## 1. Scope

1.1 These test methods cover the determination of the mechanical properties of stress-graded lumber and other wood-base structural material.

1.2 These test methods appear in the following order:

	Section
Bending edge-wise	6
Bending flat-wise:	
Center point loading	7
Third point loading	8
Axial strength in tension	9
Axial strength in compression	10

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

- [D9 Terminology Relating to Wood and Wood-Based Products](#)
- [D198 Test Methods of Static Tests of Lumber in Structural Sizes](#)
- [D2915 Practice for Sampling and Data-Analysis for Structural Wood and Wood-Based Products](#)
- [D4442 Test Methods for Direct Moisture Content Measurement of Wood and Wood-Base Materials](#)
- [D7438 Practice for Field Calibration and Application of Hand-Held Moisture Meters](#)
- [E4 Practices for Force Verification of Testing Machines](#)
- [E6 Terminology Relating to Methods of Mechanical Testing](#)
- [E177 Practice for Use of the Terms Precision and Bias in ASTM Test Methods](#)

<sup>1</sup> These test methods are under the jurisdiction of ASTM Committee [D07](#) on Wood and are the direct responsibility of Subcommittee [D07.01](#) on Fundamental Test Methods and Properties.

Current edition approved April 1, 2013. Published May 2013. Originally approved in 1988. Last previous edition approved in 2011 as [D4761 – 11](#). DOI: 10.1520/D4761-13.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

## 2.2 Other Document:<sup>3</sup>

### NIST Voluntary Product Standard PS20 American Softwood Lumber Standard

NOTE 1—The current version of PS20 is given as an example of a product standard applicable to stress-graded lumber. Other product standards may apply to stress-graded lumber. For wood-base structural materials other than stress-graded lumber, relevant product standards may apply.

## 3. Terminology

3.1 *Definitions*—See Terminologies **D9** and **E6** and Practices **E4** and **E177** for definitions of terms used in these test methods.

### 3.2 Definitions of Terms Specific to This Standard:

3.2.1 *breadth*—that dimension of the test specimen in the direction perpendicular to the span and perpendicular to the direction of an applied bending load.

3.2.2 *depth*—that dimension of the test specimen in the direction perpendicular to the span and parallel to the direction of an applied bending load.

3.2.3 *span*—the distance between the center lines of the pivot points upon which the test specimen is supported to accommodate a transverse bending load or, for tension loading, the distance between the grips.

## 4. Significance and Use

4.1 These test methods provide procedures that are applicable under true field conditions, such as in a plant with specimens not at moisture equilibrium.

4.2 The data established by these test methods can be used as follows:

4.2.1 Develop strength and stiffness properties for the population represented by the material being tested (that is, individual grades, grade combinations, species, species groups, or any other defined, identifiable sample).

4.2.2 Confirm the validity of strength and stiffness properties for the population represented by the material being tested.

4.2.3 Investigate the effect of parameters that may influence the strength and stiffness properties of the material, such as moisture content, temperature, knot size and location, or slope of grain.

4.3 The procedures chosen in accordance with these test methods shall be fully documented in the report to facilitate correlation with test results obtained through the use of traditional procedures, such as those set forth in Test Methods **D198**.

## 5. Precision and Bias

5.1 The precision and bias of these test methods have not yet been established.

## 6. BENDING EDGE-WISE

### 6.1 Scope

6.1.1 This test method provides procedures for the determination of the strength and modulus of elasticity of stress-graded lumber and other wood-base structural material in bending edge-wise.

### 6.2 Summary of Test Methods

6.2.1 The test specimen is simply supported and loaded by two concentrated forces spaced equidistant from the supports. The specimen is loaded at a prescribed rate and, as applicable, observation of load or deflection, or both, is made until failure occurs or a preselected load is reached.

### 6.3 Apparatus

6.3.1 *Testing Machine*—A device that combines (1) a reaction frame to support the test specimen, (2) a loading mechanism for applying load at a specified rate, and (3) a force-measuring apparatus that can be calibrated to the accuracy requirements of **6.3.3.2** following the procedures outlined in Practices **E4**.

6.3.1.1 *Load and Support Apparatus*, including bearing plates at least as wide as the specimen is broad and not exceeding the member depth in length. The bearing plates shall have eased edges and sufficient bearing lengths to avoid a localized crushing failure at the load and support points. The apparatus shall also include appropriate mechanisms, such as rollers or pivots, to minimize the development of axial forces in the test specimen. Each bearing point shall include an in-plane pivot point. Bearing plates and rollers shall be initially centered about their pivot points.

6.3.1.2 *Loading Configuration*—The simply supported test specimen shall be subjected to two equal transverse concentrated loads spaced equidistant from the supports.

NOTE 2—The apparent modulus of elasticity varies for different loading configurations (see Practice **D2915**). While the loading configuration that commonly serves as the basis for assigning design values assumes a uniformly distributed load, a configuration with two concentrated loads symmetrically placed within the test span usually is more suitable for structural tests. This configuration also produces a constant bending moment, free of shear, in the portion of the specimen between the load points.

6.3.1.3 *Lateral Supports*, when necessary, to restrict the specimen lateral deflection. Specimens having a depth-to-breadth ratio of three or greater are subject to lateral instability during loading and may require lateral supports. These supports shall allow movement of the specimen in the direction of load application and have minimal frictional restraint.

6.3.2 *Deflection-Measuring Apparatus*, for modulus of elasticity calculations, to monitor the deflection of the test specimen. Deflection may be measured directly as the displacement of the loading head of the testing machine. In this case, deflection is expressed as the average deflection of the load points with respect to the end reaction plates. If, because of the design of the apparatus, the deflection measurement includes extraneous components, the deflection data may be adjusted for such extraneous components (**Note 3**). In all instances, the report shall include a complete description of test conditions, extraneous components, and data adjustment procedures.

NOTE 3—If the extraneous components are an appreciable portion of the total measurement, the test apparatus should be reexamined for its suitability.

<sup>3</sup> Available from National Institute of Standards and Technology (NIST), 100 Bureau Dr., Stop 3460, Gaithersburg, MD 20899-3460.

### 6.3.3 Accuracy:

6.3.3.1 The two load points shall be located within  $\frac{1}{8}$  in. (3 mm) of the distance determined in accordance with 6.3.1.2 and 6.4.2.2.

6.3.3.2 The force-measuring apparatus shall be such as to permit load measurements with an error not to exceed  $\pm 1.0\%$  of the load for loads greater than or equal to 1000 lbf (4450 N). For loads smaller than 1000 lbf, the error shall not exceed  $\pm 10$  lbf (45 N).

6.3.3.3 The deflection-measuring apparatus shall be such as to permit deflection measurements with an error not to exceed  $\pm 2.0\%$  of the deflection for deflections greater than or equal to 0.150 in. (4 mm). For deflections smaller than 0.150 in., the error shall not exceed  $\pm 0.003$  in. (0.08 mm).

## 6.4 Test Specimen

6.4.1 *Cross Section*—Unless the effect of cross-section modifications is a test evaluation objective, test the specimen without modifying the dimensions of the commercial cross section.

### 6.4.2 Length:

6.4.2.1 The minimum specimen length shall be the span, determined in accordance with 6.4.2.2, plus an extension beyond the center lines of the end reactions to accommodate the bearing plates, such that the specimen will not slip off the end reactions during the test. In cases where the unsupported specimen length outside the test span at an end reaction (overhang) exceeds 10 times the specimen depth, report the amount of overhang at each end reaction.

6.4.2.2 The span will depend on the purpose of the test program. It is customary to express the span as a multiple of the test specimen depth (Note 4). While spans that currently serve as a basis suitable for testing range from 17 times the depth of the specimen to 21 times the depth, other spans may be used under this test method. Practice D2915 gives an indication of the variation of the apparent modulus of elasticity with span-to-depth ratios.

NOTE 4—The depth here refers to the relevant size specified in the size classification of the applicable product standard (for stress-graded lumber, for example, the depth here may refer to the dressed dry size specified in the size classification of the current version of PS20 for the nominal size, for example, 3.5 in. (89 mm) for a nominal 4 in.).

6.4.3 *Conditioning*—Specimens may be tested as produced or conditioned (for example, temperature, moisture content, or treatment), depending on the purpose of the test program. If the temperature of the specimens at the time of testing is less than 45°F (7°C) or more than 90°F (32°C), report that temperature.

## 6.5 Procedure

### 6.5.1 Specimen Measurements:

6.5.1.1 Before testing, measure and record the cross-sectional dimensions of every specimen to the nearest 0.01 in. (0.2 mm). The dimensions shall be reported to three significant figures. Make measurements at midlength of the specimen unless another location is more appropriate to the purpose of the test.

6.5.1.2 Following the test, measure the moisture content of the specimens at a location away from the ends of the specimen and as close to the failure zone as practical in accordance with the procedures outlined in Test Methods D4442 or using a

calibrated moisture meter according to Practice D7438. The number of moisture content samples shall be determined using Practice D7438 guidelines, with consideration of the expected moisture content variability, and any related requirements in the referenced product standards.

### 6.5.2 Test Setup:

6.5.2.1 *Lengthwise Positioning*—If the specimen is to be located within the test span without bias regarding defects, achieve this by centering the specimen in the span or by any other scheme suitable to the purpose of the test program.

6.5.2.2 *Selection of the Tension Edge*—Randomly select the edge to be subjected to tension testing.

6.5.3 *Speed of Testing*—The test rate shall be such that the sample target failure load would be achieved in approximately 1 min (Note 5). The failure load should not be reached in less than 10 s nor more than 10 min (Note 6).

NOTE 5—Some caution is warranted here. A test rate to achieve the average failure load for the sample in approximately 1 min will differ from that to achieve a lower percentile load for the same sample in approximately 1 min.

NOTE 6—For stress-graded lumber, a rate of motion of the testing machine loading head of approximately 3 in. (75 mm)/min will usually permit the test to be completed in the prescribed time for span to depth ratios of 17:1 and in cases where the target failure load is the average failure load for the sample.

6.5.4 *Load-Deflection Data*—Obtain load-deflection data, as required, using the apparatus specified in 6.3.2.

NOTE 7—For stress-graded lumber, data obtained for loads corresponding to maximum stresses in the specimen ranging from 400 to 1000 psi (2.75 to 7 MPa) will usually be adequate for modulus of elasticity calculations.

6.5.5 *Maximum Load*—If the purpose of the test is to determine strength properties, record the maximum load attained in the test.

NOTE 8—In proof loading, the intended load target may not be reached or may be exceeded slightly. The actual attained load as well as the target load should therefore be recorded.

6.5.6 *Record of Failure*—Depending on the purpose of the test, a description of the characteristic causing failure, and its location within the test span, may be required.

NOTE 9—An example of a coding scheme for recording characteristic type and failure location is given in Appendix X1. This example was derived for application to stress-graded lumber.

## 6.6 Report

6.6.1 The report content depends on the purpose of the test program. The report shall include, at the minimum, the following information:

6.6.1.1 Description of the testing machine, including detailed drawings, the span, and the deflection-measuring apparatus, if applicable.

6.6.1.2 Description of calibration procedures, frequency, and records.

6.6.1.3 Method used for the measurement of the moisture content of specimens.

6.6.1.4 Speed of testing and means of control of the speed of testing.

6.6.1.5 Specimens lengthwise positioning and selection of the tension edge.

6.6.1.6 As applicable, the type of load-deflection data for the calculation of the modulus of elasticity of specimens, including a description of test conditions, extraneous components, and data adjustment procedures in accordance with 6.3.2.

6.6.1.7 Description of the population sampled, in accordance with Practice D2915.

6.6.1.8 Description of the sample, including (1) sample size, (2) conditioning, if applicable, (3) temperature of specimens at the time of testing, and (4) number of specimens that failed during the test.

6.6.1.9 Data on test specimens, including, as applicable, (1) grade, (2) actual cross-sectional dimensions, (3) moisture content, (4) overhang in accordance with 6.4.2.1, (5) load-deflection data, (6) maximum load, (7) time to maximum load, and (8) failure description and location.

6.6.1.10 Details of any deviations from the prescribed or recommended procedures as outlined in this test method.

## 7. BENDING FLAT-WISE—CENTER-POINT LOADING

### 7.1 Scope

7.1.1 This test method provides procedures for the determination of long-span modulus of elasticity of lumber and other wood-base structural material in flat-wise bending under center-point load.

### 7.2 Definition of Modulus of Elasticity

7.2.1 Long-span modulus of elasticity ( $E$ ) is defined as the modulus of elasticity calculated from deflection measured in a flat-wise test of lumber with center point loading and a span-depth ratio ( $L/h$ ) of approximately 100 (90 to 110).

### 7.3 Summary of Test Methods

7.3.1 A known concentrated load is applied at mid-span of a simply supported piece of lumber oriented flatwise. A displacement measurement device is used to determine the deflection of the lumber piece under the load. The modulus of elasticity ( $E$ ) is determined by relating the deflection to the size of lumber and the test span.

### 7.4 Apparatus

7.4.1 *Support System*—Any may be used that provides unrestrained support at both ends. The support at one end should be constructed so that stability is provided for a piece of twisted lumber, such as a pedestal with a single point bearing support, a support that is designed to tilt to match the twist of the lumber, or special shims that restrain the lumber from rocking on the supports. Each bearing point shall include an in-plane pivot point. Bearing plates, when employed, shall be initially centered about their pivot points.

7.4.2 *Displacement Measurement Device*, with the capacity to measure deflections up to at least 1 in. (25 mm) to the nearest 0.001 in. (0.025 mm).

7.4.3 A weight of approximately 5 lbf (22.24 N) to be used for preloading. Compact calibrated accurately (to 0.05 lbf) (0.22 N) weights for loading.

NOTE 10—Three 5-lbf (22.24 N) weights and one 10-lbf (44.5 N) weight have been found to provide an adequate combination of weights for 2 by 4 through 2 by 12 surfaced dimension lumber sizes.

### 7.5 Procedure

7.5.1 *Specimen Measurements*—The procedures of 6.5.1 shall be followed.

7.5.2 Space the supports to provide a span-to-depth ratio for the test specimen of approximately 100 (90 to 110). This spacing shall be determined to plus or minus 1/8 in. (3 mm) for use in the calculation of the modulus of elasticity.

7.5.3 Place the displacement measurement device midway between the supports and adjust it so the downward deflection of the lumber can be measured when loaded. Construct or arrange the apparatus such that the relative position of the displacement measurement device to the supports is not changed more than 0.001 in. (0.025 mm) when the load weight is placed on the test specimen.

7.5.4 Place the test specimen flatwise on the supports and in firm contact with both end supports.

7.5.5 Apply the preload weight to the test specimen at or near the center of the span.

7.5.6 Then apply the load weight(s) to the test specimen at the center of the span. This load shall be such that it will induce 0.2 in. (5 mm) or more deflection in a specimen with  $2.0 \times 10^6$  psi (13 790 MPa) long-span modulus of elasticity.

7.5.7 Monitor the displacement measurement device to determine the deflection of the test specimen due to the load weight(s).

7.5.8 Long-span modulus of elasticity is determined using the following equation:

$$E = PL^3 / (48\Delta I)$$

where:

- $E$  = modulus of elasticity, psi (MPa),
- $P$  = increment of applied load, lbf (N),
- $L$  = span, in. (mm),
- $\Delta$  = increment of deflection corresponding to the increment of applied load, in. (mm), and
- $I$  = moment of inertia, in.<sup>4</sup>

### 7.6 Report

7.6.1 The content of the report depends on the purpose of the test program. The report shall include, at the minimum, all applicable information as presented in Section 6.6.

## 8. BENDING FLAT-WISE—THIRD-POINT LOADING

### 8.1 Scope

8.1.1 This test method provides procedures for the determination of bending strength and modulus of elasticity of stress-graded lumber and other wood base structural material in flat-wise bending on short spans under third-point load.

### 8.2 Summary of Test Methods

8.2.1 The test specimen is simply supported and loaded on the wide face by two equal, concentrated forces spaced equidistant between the supports. The specimen is loaded at a prescribed rate and, as applicable, observation of load or deflection, or both, is made until failure occurs or a preselected load or deflection is reached.

8.2.2 For modulus of elasticity calculation, a step-wise load may be used, for example, pre-loading and then adding a known weight for deflection measurement.

### 8.3 Apparatus



8.3.1 *Testing Machine*—A device that combines (1) a reaction frame to support the test specimen; (2) a loading mechanism for applying load at a specified rate or prescribed load interval; and (3) a force-measuring apparatus that can be calibrated to the requirements of 8.3.3.2, following the procedures outlined in Practices E4. If the test is for modulus of elasticity only, no force-measuring device is required. Fig. 1 illustrates the traditional device meeting the requirements of these test methods for modulus of elasticity measurement.

8.3.1.1 *Load and Support Apparatus*, including bearing plates at least as wide as the specimen is broad and not exceeding the member depth in length. The bearing plates shall have eased edges and sufficient bearing lengths to avoid a localized crushing failure at the load and support points. The apparatus shall also include appropriated mechanisms such as rollers or pivots to minimize the development of axial forces in the test specimen. If only the modulus of elasticity is to be determined in accordance with 8.2.2, then roller support surfaces similar to those depicted in Fig. 1 are permitted in place of bearing plates. Each bearing point shall include an in-plane pivot point. Bearing plates, when employed, shall be initially centered about their pivot points.

8.3.1.2 *Loading Configuration*—The simply supported test specimen shall be subjected to two equal, concentrated loads spaced equidistant between the supports. (See Note 2).

8.3.1.3 If an incremental load system is used for modulus of elasticity, the pre-load shall be sufficient to force the specimen into contact with the supports, firmly seat moveable parts, and produce sufficient deflection to permit establishing the base for the incremental measurement. The known incremental load shall be of sufficient magnitude to produce deflection greater than 0.050 in.

NOTE 11—In North American practice, these incremental loads are selected to give deflections ranging from 0.070 in. (1.8 mm) to 0.210 in. (5.3 mm), with a minus tolerance of approximately 10 %, at respective *E*

levels of 1.0 and  $3.0 \times 10^6$  psi (6.9 GPa and 21 GPa) for dimension sizes ranging from 2 by 3 to 2 by 10 (38 by 63 to 38 by 235 mm).

8.3.1.4 Deflections in the support system shall be measured to determine that either they are negligible or that calibration of the system can compensate for the deflections. (See also 8.3.2).

NOTE 12—As the span/depth ratio decreases, the magnitude of the applied load must be increased to produce deflections in the range required by 8.3.1.3. Stability of the applied load is a safety consideration in design of the apparatus. For high loads, the applied loads may need to be hung rather than supported as shown in Fig. 1. These higher loads may also increase deflections in the support apparatus.

8.3.2 *Deflection-Measuring Apparatus*, for modulus of elasticity calculations, to monitor the deflection of the test specimen. Deflection may be measured directly as the displacement of the loading head of the testing machine. In this case, deflection is expressed as the average deflection of the load points with respect to the end reactions. If, because of the design of the apparatus, the deflection measurement includes extraneous components, the deflection data may be adjusted for such extraneous components (Note 3). In all instances, the report shall include a complete description of test conditions, extraneous components, and data adjustment procedures.

8.3.2.1 If an incremental load is applied for determination of modulus of elasticity, the deflection-measuring device shall be suitable for measuring the deflection caused by the incremental load.

8.3.3 *Accuracy*:

8.3.3.1 The two load points shall be located within 1/8 in. (3 mm) of the distance determined in accordance with 8.3.1.2 and 8.4.2.2.

8.3.3.2 The force-measuring apparatus shall be such as to permit load measurements with an error not to exceed  $\pm 1.0$  % of the load for loads greater than or equal to 1000 lbf (4450 N). For loads smaller than 1000 lbf, the error shall not exceed  $\pm 10$  lbf (45 N).

(1) For modulus of elasticity based on incremental loads, these loads shall be calibrated to within  $\pm 1$  % of the stipulated value.

8.3.3.3 The deflection-measuring apparatus shall be such as to permit deflection measurements with an error not to exceed  $\pm 2.0$  % of the deflection for deflections greater than or equal to 0.150 in. (4 mm). For deflections smaller than 0.150 in., the error shall not exceed  $\pm 0.003$  in. (0.08 mm).


8.4 *Test Specimen*

8.4.1 *Cross Section*—Unless the effect of cross-section modifications is a test evaluation objective, test the specimen without modifying the dimensions of the commercial cross section.

8.4.2 *Length*:

8.4.2.1 The minimum specimen test length shall be the span, determined in accordance with 6.4.2, plus an extension beyond the center lines of the end reactions to accommodate the bearing plates, such that the specimen will not slip off the end reactions during the test.

8.4.2.2 Because this is a short-span test, the length of the specimen will often exceed the test length of 8.4.2.1. A sampling procedure shall specify where, along the specimen length, the test length shall be positioned.

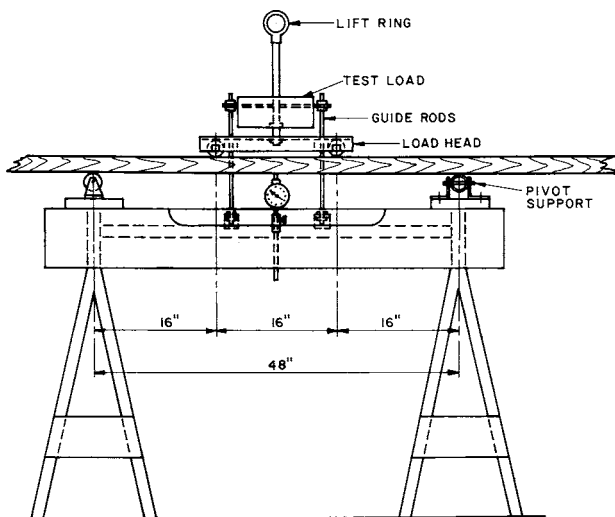

16 in. = 410 mm  
48 in. = 1220 mm

NOTE 1—This device is used for assessment of *E* in third-point, flat-wise bending on a span-to-depth ratio of 32 for 1 1/2-in. (38-mm) thick lumber.

FIG. 1 Schematic of Static Bending Testing Device

(1) The standard span for this test is 32 times the depth for nominal 2 in. (38 mm) lumber. Other spans/depth ratios are permissible but load levels and within-piece sampling methods shall be carefully documented, noting changes from the traditional span/depth ratio.

8.4.3 *Conditioning*—Specimens may be tested as produced or as conditioned (for example, temperature, moisture content, or treatment), depending on the purpose of the test program. If the temperature of the specimens at the time of testing is less than 45°F (7°C) or more than 90°F (32°C), report that temperature.

### 8.5 Procedure

8.5.1 *Specimen Measurement*—The procedures of 6.5.1 shall be followed.

#### 8.5.2 Test Setup:

8.5.2.1 *Lengthwise Positioning*—The objective may be to locate the test span within the total length without bias regarding defects, or it may be to locate the test span at locations predetermined by specified criteria. This positioning shall be achieved by a within-piece sampling plan that specifies the method of locating the test area (see 8.4.2.2). The procedure shall be documented (see Section 8.6).

(1) If this method is being used to determine specimen strength, after the test location is determined, the specimen length shall be adjusted if necessary to provide equal extension over both test supports (prevent unequal overhang).

(2) If this method is being used for modulus of elasticity only, unequal extension beyond the supports is permitted. A weight may be placed directly over a support to stabilize the specimen where a long extension (overhang) is present.

#### 8.5.3 Rate of Load Application:

8.5.3.1 *Strength and Modulus of Elasticity by Continuous Loading*—The practices of 6.5.3 shall be followed.

8.5.3.2 *Modulus of Elasticity by Incremental Test*—If the incremental loading method is used, a pre-load shall be applied, followed by the incremental load. Loads shall be applied and deflections recorded rapidly to prevent the influence of creep.

NOTE 13—It is common North American practice to complete the pre-load, deflection zero, prescribed load application, and the incremental deflection measurement within approximately 6 s.

8.5.4 *Load-Deflection Data*—Obtain load-deflection data, as required, using the apparatus specified in 8.3.2.

8.5.5 *Maximum Load*—If the purpose of the test is to determine strength properties, record the maximum load attained in the test.

NOTE 14—In proof loading, the intended load target may not be reached or may be exceeded slightly. For some applications, it is recommended that both the actual attained load and the target load be recorded.

8.5.6 *Record of Failure*—Depending on the purpose of the test, a description of the characteristic causing failure, and its location within the test span, may be required. (See Note 9.)

### 8.6 Report

8.6.1 The content of the report depends on the purpose of the test program. The report shall include, at the minimum, all applicable information as outlined in Section 6.6.

## 9. AXIAL STRENGTH IN TENSION

### 9.1 Scope

9.1.1 This test method provides procedures for the determination of the axial tensile strength of stress-graded lumber and other wood-base structural material.

### 9.2 Summary of Test Methods

9.2.1 The specimen is subjected to an axial tensile load applied near its ends. The specimen is loaded at a prescribed rate and observation of load is made until failure occurs or a preselected load is reached.

### 9.3 Apparatus

9.3.1 *Testing Machine*, combining (1) a loading mechanism for applying an axial tensile load at a specified rate and (2) a force-measuring apparatus that can be calibrated to the accuracy requirements of 9.3.3 following procedures outlined in Practices E4.

9.3.2 *Grips or Clamping Devices*, to transmit the tensile load from the testing machine to the test specimen such that (1) the specimen damage due to clamping is minimized and (2) slippage is minimized during load application.

9.3.2.1 *Distance Between Grips*—The clear distance between grips depends on the purpose of the test program and the material being tested.

NOTE 15—It is recommended that, for stress-graded lumber, the clear distance between grips be, at the minimum, 25 times the width of the test specimen in order to minimize problems of end fixity and to properly account for the effect of grain deviations on strength. Because of practical limitations on the use of equipment for field testing, this may not always be feasible for the wider width of stress-graded lumber, for which a clear distance between grips less than 12 times the width of the test specimen is not recommended. The width here refers to the dressed dry size specified in the size classification the current version of PS20. To minimize problems in the interpretation of data results, it is further recommended that all specimens be tested at a constant clear span between grips.

9.3.3 *Accuracy*—The force-measuring apparatus shall be such as to permit load measurements with an error not to exceed  $\pm 2.0\%$  of the load.

### 9.4 Test Specimen

9.4.1 *Cross Section*—See 6.4.1.

9.4.2 *Length*—The minimum specimen length shall be the clear distance between grips, determined in accordance with 9.3.2.1, plus any required length to achieve contact along the full length of the grips.

9.4.3 *Conditioning*—See 6.4.3.

### 9.5 Procedure

9.5.1 *Specimen Measurements*—The procedures of 6.5.1 shall be followed.

9.5.2 *Test Setup*—Center the specimen in the grips, taking care to have the long axis of the specimen coincide with the direction of load application. Apply load to the specimen at a rate determined in accordance with 9.5.3.

9.5.3 *Speed of Testing*—The test rate shall be such that the sample target failure load would be achieved in approximately 1 min (Note 5). Failure load should not be reached in less than 10 s nor more than 10 min.

NOTE 16—For stress-graded lumber, a stress rate of approximately 4000 psi (30 MPa)/min will usually permit the test to be completed in the

prescribed time, in cases where the target failure load is the average failure load for the sample.

9.5.4 *Maximum Load*—See 6.5.5.

9.5.5 *Record of Failure*—See 6.5.6.

## 9.6 Report

9.6.1 The content of the report depends on the purpose of the test program. The report shall include, at the minimum, all applicable information as presented in Section 6.6.

## 10. AXIAL STRENGTH IN COMPRESSION

### 10.1 Scope

10.1.1 This test method provides procedures for the determination of the axial compressive strength of stress-graded lumber and other wood-base structural material.

### 10.2 Summary of Test Methods

10.2.1 The specimen is subjected to an axial compressive load applied at its ends. The specimen is loaded at a prescribed rate until failure occurs or a preselected load is reached. This test method permits either tests of commercial lengths or tests of short specimens cut from commercial lengths.

### 10.3 Apparatus

10.3.1 *Testing Machine*, that combines (1) a loading mechanism for applying an axial compressive load at a specified rate and (2) a force-measuring apparatus that can be calibrated to the accuracy requirements of 10.3.4 following procedures outlined in Practices E4.

10.3.2 *Bearing Blocks*, to transmit the compressive load from the testing machine to the test specimen such that (1) the load is uniformly applied over the full contact surfaces and (2) eccentric loading of the specimen is prevented. Accordingly, one spherical bearing block at least shall be used.

10.3.2.1 Alternatively, it is possible, in this test method, to use grips or clamping devices in place of bearing blocks, but means of avoiding eccentric loading should be provided.

10.3.3 *Lateral Supports*, to prevent buckling of the specimen during the test. These supports may be either continuous or intermittent. They shall allow the specimen movement in the direction of load application and provide minimal frictional restraint. If intermittent supports are provided, they shall be spaced so that the distance between supports on a given face of the specimen is less than 17 times the radius of gyration of the cross section about the centroidal axis parallel to the face considered.

10.3.3.1 If tests are to be run on commercial lengths of lumber, support shall be intermittent if results comparable to published design values and to short specimen tests (8.3.3.2) are to be obtained.

10.3.3.2 If tests are to be run on short specimens cut from commercial lengths, continuous support within the loading mechanism may be used. See Annex A1 and Appendix X2.

10.3.4 *Accuracy*—See 9.3.3.

### 10.4 Test Specimen

10.4.1 *Selection*—Specimens shall be tested as selected in accordance with the sampling plan, unless short sections are to be selected for testing.

10.4.1.1 If small specimens are to be tested, at least two test specimens shall be cut from each sample piece, representing the weakest sections in axial strength in compression as judged by experienced grading personnel.

10.4.2 *Cross Section*—See 6.4.1.

10.4.3 *Length*—The length of the test specimen shall be at least 2.5 times its greater cross-sectional dimension.

NOTE 17—The greater cross-sectional dimension refers to the relevant size specified in the size classification of the applicable product standard. For stress-graded lumber, for example, the test specimen length shall be at least 2.5 times its width where width refers to the dressed dry size specified in the size classification of the current version of PS20, for example, 3.5 in. (89 mm) for a nominal 4 in.

10.4.4 *Conditioning*—See 6.4.3.

### 10.5 Procedure

10.5.1 *Specimen Preparation*—Cut the specimen to the proper length so that the contact surfaces are plane, parallel to each other, and normal to the long axis of the specimen.

10.5.2 *Specimen Measurements*—Follow procedures similar to those stipulated for axial strength in tension in 9.5.1.

10.5.3 *Test Setup*—Center the specimen on the bearing blocks or in the grips, taking care to have the long axis of the specimen coincide with the direction of load application. Apply load to the specimen at a rate determined in accordance with 10.5.4.

10.5.4 *Speed of Testing*—The test rate shall be such that the sample target failure load would be achieved in approximately 1 min (Note 5). Failure load should not be reached in less than 10 s nor more than 10 min.

NOTE 18—For stress-graded lumber, a deformation rate of approximately 0.01 in./in.·min (0.01 mm/mm·min) will usually permit the test to be completed in the prescribed time, in cases where the target failure load is the average failure load for the sample.

10.5.5 *Maximum Load*—See 6.5.5.

10.5.6 *Record of Failure*—See 6.5.6.

### 10.6 Report

10.6.1 The content of the report depends on the purpose of the test program. The report shall include, at the minimum, all applicable information as presented in Section 6.6.

## 11. Keywords

11.1 lumber; mechanical properties; wood-base

(Mandatory Information)

A1. SAMPLING FOR SHORT SPECIMEN AXIAL STRENGTH IN COMPRESSION TESTS

A1.1 The use of the short specimen axial strength in compression test to produce data comparable to tests of commercial lengths depends on proper selection of the weakest short length specimen from the commercial length. The procedures of these test methods shall be followed.

A1.1.1 *Compression Sample Preparation:*<sup>4</sup>

A1.1.1.1 Locate the most strength-reducing characteristic in the piece (see Note A1.1).

A1.1.1.2 Mark and cut the board to the required length with the strength-reducing characteristic centered in the length. The minimum test specimen lengths according to lumber size are as

follows: 2 by 4 by 14 in. (350 mm); 2 by 6 by 18 in. (450 mm); 2 by 8 by 26 in. (650 mm); and 2 by 10 by 26 in. (650 mm).

A1.1.1.3 Locate the next most strength-reducing characteristic.

A1.1.1.4 Mark and cut the board as stated in A1.1.1.2.

NOTE A1.1—For pieces in which the two largest strength-reducing characteristics are less than the required length apart, but still well separated, cut the piece halfway between the two. Then cut each test piece to the required length. Where the two characteristics are not well separated, include both in one piece (even if it has to be longer than required). Then choose a second test section as above.

A1.2 When analyzing the results of a sample of lumber to obtain near-minimum test results comparable to tests of commercial lengths, assign to each piece the lowest test value of the two (or more) tests run on that piece.

<sup>4</sup> Barrett, J. D., "Comparison of Two ASTM D198 Compression Parallel-to-Grain Test Methods," ASTM Committee D07 Meeting, Tacoma, WI, 1987.

APPENDIXES

(Nonmandatory Information)

X1. RECORDING SCHEME


X1.1 The following is an example of a recording scheme to describe (1) characteristics in stress-graded lumber and (2) specimen failure (type and cause) for stress-graded lumber.

X1.1.1 *Characteristics Description* —The recording scheme  $X - Y$  where  $X$  = a two-digit number identifying a characteristic and  $Y$  = a two-digit number unless otherwise specified, describing the extent of the characteristic listed in Table X1.1.

X1.1.2 *Specimen Failure Description* —The type of failure is recorded using the following code:

Type of Failure	Code
Tension side failure	000
Compression side failure	001
Combined tension and compression failure	002
Lateral buckling failure	003
Shear failure	004
Grip slip (tension only)	005
Failure at edge of grip (tension only)	006

X1.1.2.1 The cause of failure usually is associated with a characteristic. Accordingly, the recording scheme in Table X1.1 is used to describe the cause of failure. If failure occurs in clear wood, however, there is no need to record  $X$  and  $Y$ . If failure occurs at a knot, a code "XXYYAABB" is recorded, unless otherwise indicated in Fig. X1.1, where  $X$ ,  $Y$ ,  $A$ , and  $B$

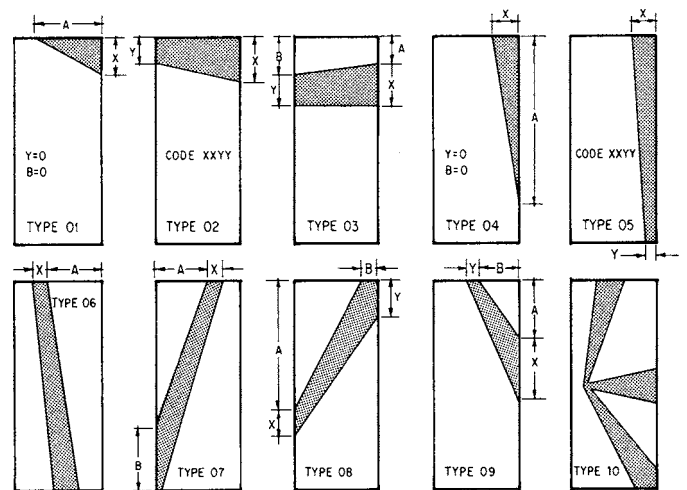

Code—Percent of cross section occupied by knot (2 digit numbers) applies to Type 10 only.

FIG. X1.1 Knot Measurements for Indicating the Description of Knot(s) Causing Specimen Failure

are knot measurements shown in Fig. X1.1, for ten types of knots.



**TABLE X1.1 Recording Scheme to Describe Characteristics in Stress-Graded Lumber**

Characteristic	X	Y	Characteristic	X	Y
Narrow face or spike knot intergrown	11		Splits	44	01 for very short
Narrow face or spike knot encased	12	displacement, %			02 for short
Narrow face or spike knot unsound	13				03 for medium 04 for long
Wide face knot, center line intergrown	14	knot size (nearest 1/16 in.)	Skip	45	01 for light
Wide face knot, center line encased	15	for example, 08 for 1/2-in.			02 for medium
Wide face knot, center line unsound	16	knot.			03 for heavy
Wide face knot, at edge intergrown	17		Warp	46	00 for 1/2 of medium
Wide face knot, at edge encased	18	knot size (nearest 1/16 in.)			01 for light
Wide face knot, at edge unsound	19				02 for medium 03 for heavy
Knots, not well spaced, or combinations	20	cross section, %			
Hole	21	size as knot (nearest 1/16 in.)	Mechanical damage	47	percent
			Crossbreak	49	displacement, %
Pin holes	22		Saw cut	50	01 saw cut through edge
Grub or teredo holes	23	cross section, %			02 all other saw cuts
Speck	31		Slope of grain	51	run of slope <sup>A</sup>
Honeycomb	32	cross section, %	Wane	52	first digit is number of fourths of width; second is fourths of thickness
Unsound wood or peck	33				
Distorted grain, knot cluster, or burl	34	displacement, %			
Heart stain	35	displacement, %	Falling breaks	53	01, 1/3 or less of width 02, 1/3 to 2/3 of width 03, 2/3 or more of width
Pitch or bark pockets	41	01 for very small 02 for small 03 for medium 04 for large 15 for very large	Brash failure (not defect related)	54	
			Compression wood	55	
			Coarse grain or exceptionally light weight	56	
Shake	42	01 for light, not through 02 for medium, not through 03 for others, not through 11 for light, through 12 for medium, through 13 for others, through	Local grain deviation on wide face (failure initiated in locally severe grain deviation)	60	run of slope (use 00 if less than 1 in 1) <sup>A</sup>
			Local grain deviation on narrow face (failure initiated in locally severe grain deviation)	70	run of slope as above
Seasoning or roller check	43	01 for surface 02 for small, through 03 for medium, through 04 for large, through	Failure at the point where the sticker crossed the specimen in the package during kiln-drying <sup>B</sup>	99	moisture content at point failure

<sup>A</sup> Expressed in inches, corresponds to a 1-in. rise.

<sup>B</sup> Must be used in conjunction with another characteristic.

## X2. BACKGROUND ON USE OF SHORT COMPRESSION PARALLEL TESTS

X2.1 The use of short specimens cut from commercial lengths of lumber raises two questions: (1) how well a person trained in grading could identify the weakest section in a piece of lumber, given two opportunities; and (2) how well the short specimen test results compare to the Test Methods D198 test.

X2.1.1 Research at the USFPL<sup>5</sup> addressed the first question. A number of pieces of 2 by 4 Southern Pine No. 1 and better and No. 3 grades were selected. A lab technician marked the location of the two sections estimated to be the weakest portion of the piece in axial compression. The sections were also

ordered according to which of the two was estimated to be weaker. Then the remainder of the 2 by 4 was marked off into as many test specimens as possible. The sample boards were then cut into short test specimens and tested in axial compression. The results were as follows: (1) given one chance, a technician could identify the weakest section approximately 50 % of the time; (2) given two chances, the technician could identify the weakest section of the piece at least 70 to 75 % of the time. Generally, the predictive ability of the technician was inversely related to the quality of the sample; in the clearer type of material, it was harder to predict where the weakest section was located. The results also showed that, even though the technician predicted the weakest section accurately as little as 70 % of the time given two chances, the difference in fifth

<sup>5</sup> Green, D. W., and Evans, J. W., "Compression Testing of Lumber: A Comparison of Methods," *Journal of Testing and Evaluation*, Vol 20, No. 2, March 1992, pp. 132–138.

percentile estimates with the true weakest specimens was only approximately 5 % or less.

X2.1.2 The second question was addressed by comparative studies at Forintek Canada Corp.<sup>4</sup> and between USFPL and Forintek.<sup>6</sup> The Forintek study<sup>4</sup> was conducted on full-size lumber of No. 2 and better grade, in which the quality was marked for the estimated two weakest sections. The full length of the piece was then tested by Test Methods **D198** procedures.

---

<sup>6</sup> Shelley, B. E., "Testing Machines: Development, Calibration, and Comparative Studies," *Proceedings Workshop on In-Grade Testing of Structural Lumber*, Forest Products Research Society, Madison, WI, April 25–26, 1988, pp. 15–26.

If the piece failed away from the marked sections, the sections were cut out and tested as short sections. The test results indicated that the difference between the two test methods was at most approximately 2 %, with the short specimen test higher.

X2.1.2.1 The comparative studies between Forintek and the USFPL<sup>6</sup> verified the importance of maintaining intermittent lateral supports to yield a slenderness ratio of 17 (Test Methods **D198**, Section 20) for full-length tests rather than continuous support. When the full-length tests were based on this intermittent support, the difference was negligible between these results and those using the estimated weakest short specimen fully supported.

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the ASTM website (www.astm.org/COPYRIGHT/).*