



# Standard Test Method for Shear Viscosity of Coal-Tar and Petroleum Pitches<sup>1</sup>

This standard is issued under the fixed designation D5018; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

---

<sup>ε1</sup> NOTE—SI units formatting was corrected editorially in May 2015.

---

## 1. Scope

1.1 This test method covers the determination of the apparent shear viscosity of coal-tar and petroleum-based pitches having a Mettler softening point (SP) range of approximately 95 °C to 120 °C.

1.2 This test method is applicable only for rotational viscometers.

1.3 Since this test method is based on theoretical grounds, strict adherence to details of the procedure is necessary to comply with the theoretical requirements.

1.4 The values stated in SI units are to be regarded as standard.

1.4.1 *Exception*—The values stated in conventional units (centipoise) are to be regarded as the standard for viscosity measurement only. The SI unit is the pascal second (Pa·s) and one millipascal second (mPa·s) = one centipoise (cps); centipoise is in cgs units.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* Specific hazard statements are given in Section 7.

---

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products, Liquid Fuels, and Lubricants and is the direct responsibility of Subcommittee D02.05 on Properties of Fuels, Petroleum Coke and Carbon Material.

Current edition approved April 1, 2015. Published May 2015. Originally approved in 1989. Last previous edition approved in 2009 as D5018 – 89 (2009). DOI: 10.1520/D5018-89R15E01.

## 2. Referenced Documents

2.1 *ASTM Standards*:<sup>2</sup>

D4296 Practice for Sampling Pitch

E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method

## 3. Summary of Test Method

3.1 The viscosity of a pitch, over the temperature range of about 40 °C to 100 °C above the SP of the material, is determined using a rotational viscometer.

3.2 The recommended specifications herein are for measuring the apparent shear viscosity of binder pitches via a concentric cylinder viscometer. Apparent shear viscosity is the ratio of shear stress to shear rate in a unidirectional simple shear flow field at steady state conditions. A concentric cylinder viscometer is useful for measuring the apparent shear viscosity, provided the sample temperature is adequately controlled, the “end-effects” are negligible, and the gap between rotor/cup is small and remains constant during the test. The extrapolated value of apparent shear viscosity at “zero” shear rate is called shear viscosity.

## 4. Significance and Use

4.1 This test method is useful as one element in establishing the uniformity of shipments.

4.2 Viscosity is also valuable for rheological characterization of binder pitches. Binder pitch imparts consistency to

---

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard’s Document Summary page on the ASTM website.

carbonaceous mixes and affects their resistance to deformation. Binder pitch viscosity is important for assessing mix consistency and for evaluating the ease of mix extrusion or molding into artifacts.

## 5. Apparatus

5.1 *Viscometer*—A rotational viscometer capable of measuring viscosity in the range of about 5 cps to 15 000 cps; the viscometer should be equipped with the appropriate accessories to allow measurements up to about 230 °C. Two viscometers meeting these requirements are the LVT, LVF,<sup>3</sup> or equivalent, and the RV100, RV20,<sup>4</sup> or equivalent.

5.2 *Sample Temperature Control System*—Any device capable of maintaining the sample test temperature within limits of  $\pm 1.0$  °C while allowing viscosity measurements. Examples are the Thermosel System<sup>3</sup> and the TP 24<sup>5</sup> with heater.

5.3 *Thermometer*—ASTM precision thermometer 2C, having a range of  $-5$  °C to 300 °C.

5.4 *Hot Plate*<sup>5</sup>—Any hot plate with adjustable temperature control and surface temperature indication (to prevent sample overheating).

5.5 *Calibration Fluids*<sup>6</sup>—A series of calibrated fluids that cover the viscosity range of approximately 100 cps to 15 000 cps at temperatures up to 150 °C.

## 6. Reagents and Materials

6.1 *Cleaning Solvent*—Any solvent capable of dissolving pitch, (suitable solvents are quinoline or creosote oils).

6.2 *Rinsing Solvents*—Toluene and acetone are used for final rinsing after initial cleaning.

## 7. Safety Hazards

7.1 Fumes of hot pitch or solvents, or both, should be removed from all working areas by means of proper hoods. The working area should be kept free of sparks and flames. Quinoline fumes should not be inhaled, and prolonged contact with skin should be avoided. Toluene is toxic and flammable.

<sup>3</sup> The sole source of supply of the apparatus known to the committee at this time is available from Brookfield Engineering Laboratories, Inc., 240 Cushing St., Stoughton, MA 02072. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee<sup>1</sup>, which you may attend.

<sup>4</sup> The sole source of supply of the apparatus known to the committee at this time is available from Haake Buchler Instruments, Inc., 244 Saddle River Road, Saddle Brook, NJ 07662-6001. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee<sup>1</sup>, which you may attend.

<sup>5</sup> The sole source of supply of the apparatus known to the committee at this time is the Hot plate Model 11-496-3 with 11-496-4 dial thermometer, available from Fisher Scientific, 585 Alpha Drive, Pittsburgh, PA 15238. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee<sup>1</sup>, which you may attend.

<sup>6</sup> Fluids available from Brookfield Engineering Laboratories; Cannon Instrument Co., P.O. Box 16, State College, PA 16804, have been found suitable for this purpose. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee<sup>1</sup>, which you may attend.

## 8. Bulk Sampling

8.1 Take samples from shipments in accordance with Practice [D4296](#). Samples shall be free of foreign substances. Thoroughly mix the sample immediately before removing a representative portion for the determination or for dehydration.

## 9. Sample Preparation

9.1 Ensure sample is dry; if there is visible moisture, dehydrate at 50 °C in a forced-air or vacuum oven until dry, but no longer than 2 h. (Experience has shown that drying at temperatures in excess of 50 °C increases the SP and viscosity of the pitch.)

9.2 Crush dry lumps of pitch to a size of 6 mm to 12 mm.

## 10. Charging Sample Cup

10.1 In a suitable container, or the sample cup, melt pitch with occasional stirring. Overheating of sample must be avoided as loss of volatiles may affect viscosity. (Maximum temperature should not exceed 50 °C above SP. As a guide, the surface temperature of the hot plate surface should not exceed 200 °C.)

10.2 Place rotor in cup and preheat both to approximately the first test temperature.

10.3 Remove rotor and transfer required amount of pitch to the level specified by the manufacturer.

10.4 Re-insert rotor, check that rotor is immersed to specified depth, and install insulating cover.

## 11. Viscometer Calibration

11.1 This step, required only occasionally, is designed to establish that the temperature and viscosity indicated by the appropriate measuring devices are in agreement with known standards.

11.2 Equipment is to be properly leveled and installed in accordance with manufacturer's instructions.

11.3 Use the ASTM thermometer (applying the appropriate stem correction) to correlate pitch temperature (in cup) to temperature controller/indicator. Test temperature is considered to be the actual pitch temperature and not the temperature indicated on the controller.

11.4 Calibrate viscometer using calibration fluids.

11.4.1 Use high- and low-temperature fluids; see [5.5](#).

11.4.2 Calibrate each rotor/cup combination and use them as a paired set.

## 12. Procedure for Viscosity Determination

12.1 The following general principles apply to all viscosity measurements determined by rotational methods:

12.1.1 Maximize rotor diameter.

12.1.2 Minimize gap width between rotor and cup.

12.1.3 Minimize end effects (use longest available rotor).

12.1.4 Prevent viscous heating (due to prolonged rotation of rotor at high revolutions per minute).

12.2 Select the proper rotor/cup combination that covers the anticipated viscosity range. A typical viscosity-temperature

curve for various coal-tar pitches is given in Fig. 1, and a typical spindle number and revolutions per minute relationship for a LV series Brookfield viscometer<sup>4</sup> is given in Table 1. If there is overlap in rotor/cup selection, select the combination that best meets the criteria set forth in 12.1.1 to 12.1.4.

12.3 Determine viscosity from the lowest to the highest test temperatures.

12.4 Turn rotor at low revolutions per minute during heat-up (after sample is melted) and when changing test temperatures.

12.5 Stabilize temperature for a *minimum of 5 min but not more than 15 min* before measuring viscosity.

12.6 Determine viscosity following manufacturer’s procedure. Ensure that the scale reading has stabilized before recording the value; only record values that are between 10 % and 90 % of the maximum scale reading.

TABLE 1 Brookfield Thermosel Spindle Factors LV Series Viscometers<sup>A</sup>

Speed, r/min	Spindle Number		
	18	31	34
60	0.5	5	10
30	1	10	20
12	2.5	25	50
6	5	50	100
3	10	100	200
1.5	20	200	400
0.6	50	500	1000
0.3	100	1000	2000

<sup>A</sup> Viscosity (centipoise) is determined by multiplying the scale reading (0 to 100) by the appropriate spindle factor. If the usable scale readings are 10 % to 90 % of maximum (see 12.6), then the viscosity range for spindles 18, 31, and 34 are 5 to 9000, 50 to 90 000, and 100 to 180 000 centipoise, respectively.

12.7 Increase temperature controller to next higher test temperature and repeat 12.4 through 12.7.

12.8 Record test temperature and corresponding scale readings and convert scale readings to viscosity using appropriate factors supplied by manufacturer or determined by calibration.

12.9 Pitch is generally regarded as a Newtonian liquid (the viscosity is independent of shear rate (rotational velocity or revolutions per minute)). To ensure that the pitch sample is in fact Newtonian, determine the viscosity at different revolutions per minute at a given temperature. If viscosities at different revolutions per minute are different (at same temperature), but are within 10 % of the average of the readings, report the average value. If the viscosities, at different revolutions per minute but the same temperature, differ by more than 10 % from the average, the material is non-Newtonian and the viscosity for each shear rate (revolutions per minute) should be reported.

12.10 Occasionally, the pitch volume in the cup can decrease when heated to higher temperatures due to loss of moisture or entrapped air. Consequently, the rotor will not be completely immersed in pitch and the viscosity at higher temperatures will be lower than the true value. Also, the viscosity at lower temperatures will be inaccurate due to foaming. To ensure that this did not occur, check the level in the cup after the test is completed and the temperature is about 150 °C. If the rotor is not completely immersed, repeat the test taking care to expel any moisture or entrapped air prior to charging the cup. Moisture can be eliminated by drying at 50 °C, see 9.1. Entrapped air can be removed by carefully melting the pitch and stirring gently until no foaming is observed; avoid overheating the pitch, see 10.1. Also, entrapped air can be minimized by avoiding the use of fine pitch particles; use 6 mm × 12 mm sized particles, see 9.2.

13. Cleaning

13.1 After completion of test, cool to about 40 °C above SP, remove rotor and place rotor into a container of quinoline or other high-boiling aromatic solvent (in hood), or wipe rotor using toluene or quinoline.

13.2 Remove cup and pour out pitch; clean with quinoline, or other appropriate solvent, and toluene.

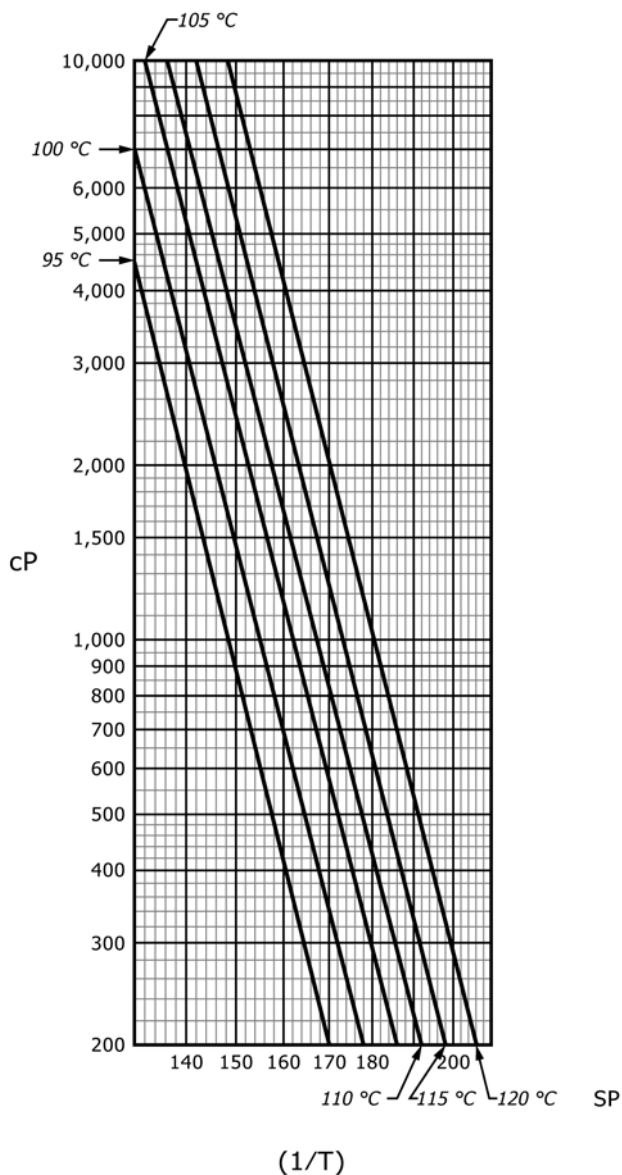


FIG. 1 Viscosity of Coal-Tar Pitch as a Function of Temperature

13.3 After the cup and rotor are clean and cool, rinse both with acetone to remove any oil residue.

#### 14. Report

14.1 Report viscosity, for each test temperature, to the nearest centipoise.

14.2 The data can be reported in simple tabular form or plotted on suitable graph paper. (Usually a plot of log viscosity versus 1/T (Celsius) gives a straight-line relationship.)

#### 15. Precision and Bias

15.1 The precision was determined by an interlaboratory study conducted in accordance with Practice E691. Fourteen laboratories tested four materials (three coal-tar pitches and one petroleum pitch) in the temperature range of 150 °C to 210 °C (150 °C to 230 °C for the petroleum pitch); the viscosities ranged from 12 000 cps to 50 cps. Based on this study, the criteria in 15.1.1 and 15.1.2 shall be used for judging the

acceptability of results (95 % probability) obtained in the aforementioned temperature ranges and in the viscosity range of 50 cps to 12 000 cps:

15.1.1 *Repeatability Limits*—Duplicate values (cps) by the same operator shall not be considered suspect unless the determined viscosities, at a given temperature, differ by more than 12 % of the average of the duplicate determinations.

15.1.2 *Reproducibility Limits*—The values reported by each of two laboratories, representing the arithmetic average of duplicate determinations at a given temperature, shall not be considered suspect unless the reported values (cps) differ by more than 36 % of the average of the four values.

15.2 *Bias*—This test method has no bias with any other standard.

#### 16. Keywords

16.1 coal tar pitch; petroleum pitch; pitch; viscosity

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; http://www.copyright.com/*