



Standard Practice for Flow Rate Adjustment of Personal Sampling Pumps¹

This standard is issued under the fixed designation D5337; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This practice describes the calibration of sampling pumps commonly used for monitoring personal airborne exposures in the work-place.

1.2 This practice includes procedures for describing primary and secondary calibration techniques.

1.3 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*²

[D1356 Terminology Relating to Sampling and Analysis of Atmospheres](#)

2.2 *NIOSH and OSHA Documents:*

[HSM-99-71-31 Personal Sampling Pump for Charcoal Tubes; Final Report](#)³

[NIOSH Manual of Analytical Methods, 4th ed.](#)⁴

[OSHA Analytical Methods Manual](#)⁵

3. Terminology

3.1 For definitions of terms used in this practice, refer to Terminology [D1356](#).

¹ This practice is under the jurisdiction of ASTM Committee D22 on Air Quality and is the direct responsibility of Subcommittee D22.04 on Workplace Air Quality.

Current edition approved Nov. 1, 2016. Published November 2016. Originally approved in 1992. Last previous edition approved in 2011 as D5337 – 11. DOI: 10.1520/D5337-11R16.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ Available from the U.S. Department of Commerce, National Technical Information Service, Port Royal Road, Springfield, VA 22161.

⁴ Centers for Disease Control and Prevention (CDC), National Institute for Occupational Safety and Health (NIOSH), Cincinnati, Ohio (1994); Available from NIOSH Publications, 4676 Columbia Parkway, Cincinnati, Ohio 45226; www.cdc.gov/niosh/nmam.

⁵ Occupational Safety and Health Administration, Salt Lake Technical Center, Salt Lake City, Utah (1985); Available from OSHA Analytical Laboratory, 8660 S. Sandy Parkway, Sandy, UT 84070; www.osha.gov/dts/sltc/methods.

3.2 The term *primary flow-rate calibration*, as used in this practice, does not imply the calibration is traceable to a primary standard, unless the apparatus used in the calibration (burets, stop-watches, etc.) has been demonstrated to be traceable to national or international standards, and that this traceability is established on a routine (generally annual) basis. Traceability of calibration is strongly recommended.

4. Summary of Practice

4.1 A bubble tube meter or electronic near-frictionless pump is used for primary calibration of personal sampling pumps. The practice is applicable to systems using air sampling devices. Provisions are made for both manual and automated bubble meters.

4.2 Secondary calibration procedures for field applications are also included in the practice (see [7.3](#)).

5. Significance and Use

5.1 Most occupational exposure assessment methods require the use of personal sampling pumps to collect air samples at typical workplace sampling rates, with sampling volumes specified by (a) particular procedure(s). The precision and bias of these methods are directly affected by the precision and bias of the pumps used to measure the air volume(s) sampled.

6. Apparatus

6.1 *Burets*, 1-L (for high flow) and 100-mL or 10 mL (for low flow).

6.2 *Manometer*.

6.3 *Rotameter*.

6.4 *Stop Watch*.

6.5 Electronic Bubble Meter or Near-frictionless Piston Flowmeter (alternates), should have traceable calibration (see [3.2](#)).

7. Procedure

7.1 Calibrate the personal sampling pumps before and measure after each day's sampling.

7.2 *Primary Flow-Rate Calibration Device(s)* (as noted in [3.2](#), these are not primary standards unless the apparatus used in the calibration has been demonstrated to be traceable to national and international standards):


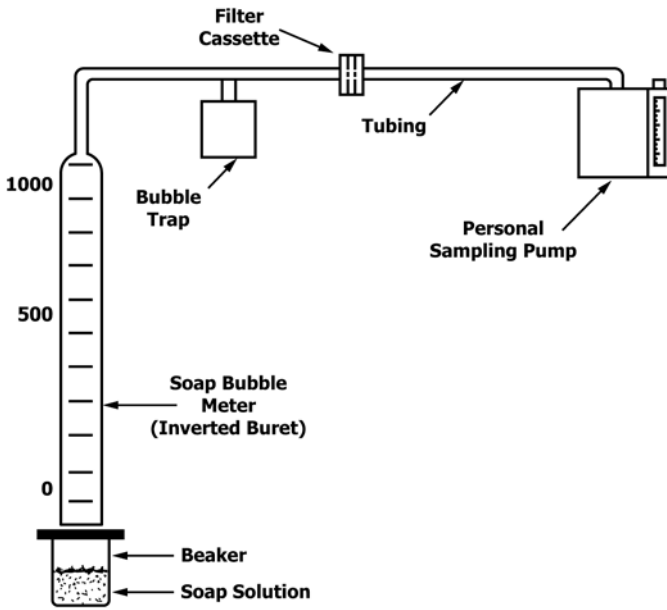


FIG. 1 Calibration Setup for Personal Sampling Pump with Filter Cassette

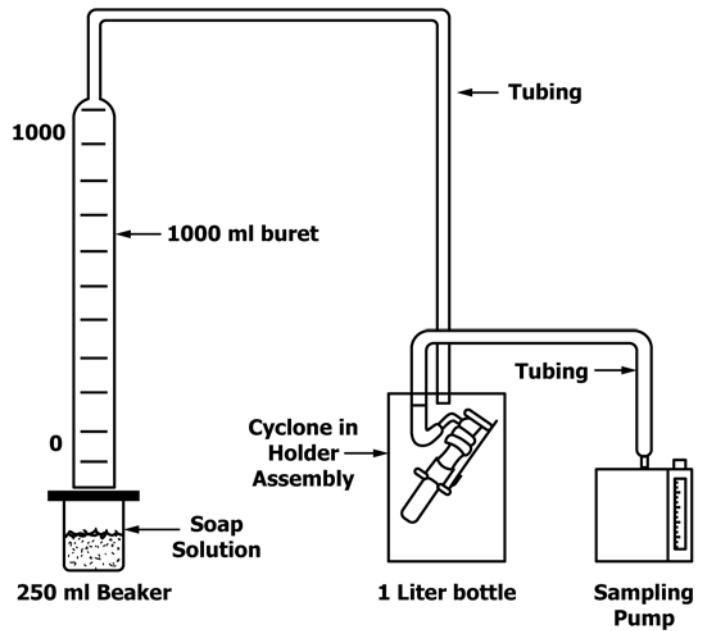

NOTE 1—Other cyclones may require different setups.
 FIG. 3 Calibration Setup for Personal Sampling Pump with a 10-mm Nylon Cyclone Respirable Dust Sampler Using a Bubble Meter

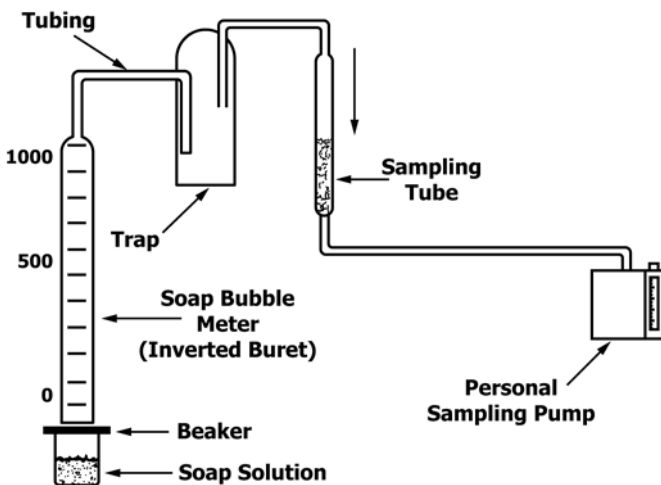


FIG. 2 Calibration Setup for Personal Sampling Pump with Sampling Tube

$$\text{Flow Rate (L/min)} = \frac{\text{Volume (L)}}{\text{Time (min)}} \quad (1)$$

7.2.1.8 If using a pump equipped with a rotameter, record the position of center of the float that corresponds with the flow rate. The rotameter can then be used as an approximate indicator of flow-rate during the sampling period.

7.2.1.9 An automated electronic-bubble flow meter may be used in place of manual types. The flow meter has an electronic timer that measures the time taken for the bubble to move through a defined volume producing a direct read-out of flow-rate.

7.2.2 *Electronic Near-Frictionless Piston Method*—Allow the pump to stabilize and connect to an appropriate sampling train as in 7.3, Figs. 1-3 except that the soap bubble meter is replaced by a near-frictionless piston flow-meter. The flow meter has an electronic timer that measures the time taken for the piston to move through a defined volume producing a direct read-out of flow-rate.

7.3 *Secondary Flow-rate Calibration Devices:*

7.3.1 Set up a calibration apparatus appropriate for the sample collector to be used. See Figs. 1-3.

7.3.2 Place the secondary calibration device (for example, rotameter) in line, between the bubble meter and sampler, connecting the inlet of the secondary calibrator to the outlet of the bubble meter and the outlet of the sampler.

7.3.3 Adjust the pump to the desired flow rate.

7.3.4 Determine the exact flow rate as described in 7.2. Record the calibration flow rate and the corresponding reading on the secondary calibration device.

7.3.5 Calibration over the range of the sampling flow rates is necessary if the secondary sampling pump calibration device is required. Calibrate the secondary calibrator at each flow rate

7.2.1 *Bubble Meter Method:*

7.2.1.1 Allow the pump to run five minutes prior to calibration to stabilize pump.

7.2.1.2 Connect pump to an appropriate sampling train. Sampling trains identical to that used in sampling for sorbent tubes, filter cassettes, and cyclones are shown in Figs. 1-3.

7.2.1.3 Check all connections to insure their integrity.

7.2.1.4 Wet the inside surface of the 1-L buret with the soap solution (use a 100-mL buret for low flow pumps).

7.2.1.5 Turn on the pump and momentarily submerge the opening of the buret into the soap solution to form a bubble.

7.2.1.6 With a stop watch, time the travel of a single film from the zero mark to the calibrated volume mark. Note the time and repeat this procedure at least three times.

7.2.1.7 Calculate the flow rate using the formula:

with the bubble meter. Prepare a calibration graph across the range of flow rates of interest.

7.3.6 Calibrate secondary devices subsequent to shipping from one location to another, or whenever the integrity of the device is questioned.

7.3.7 Once calibrated, the secondary calibration device can be used to replace the bubble meter for calibrating pumps; this is accomplished by attaching the outlet of the calibration device to the inlet of the sampling system.

8. Keywords

8.1 air monitoring; flow rate calibration; personal sampling pumps; sampling and analysis; workplace atmospheres

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>