



Standard Test Method for Color Determination of Plastic Pellets¹

This standard is issued under the fixed designation D6290; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reappraisal. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reappraisal.

1. Scope*

1.1 This test method is intended primarily for the instrumental measurement of the degree of yellowness (or change of degree of yellowness) under daylight illumination of homogeneous, nonfluorescent, nearly-colorless transparent or nearly-white translucent or opaque plastics. The measurement is made on pellets and based on tristimulus values obtained with a spectrophotometer or colorimeter.

1.2 This test method is applicable to the color analysis of plastic pellets. It is possible that each material will have unique characteristics that determine the color values.

1.3 This procedure outlines a method to determine color measurements, such as Yellowness Index, CIE X, Y, Z, and Hunter L, a, b, or CIE L*, a*, b*.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

NOTE 1—There is no known ISO equivalent to this standard.

2. Referenced Documents

2.1 *ASTM Standards:*²

[D883 Terminology Relating to Plastics](#)

[D2244 Practice for Calculation of Color Tolerances and Color Differences from Instrumentally Measured Color Coordinates](#)

[E179 Guide for Selection of Geometric Conditions for Measurement of Reflection and Transmission Properties of Materials](#)

[E284 Terminology of Appearance](#)

[E308 Practice for Computing the Colors of Objects by Using the CIE System](#)

¹ This test method is under the jurisdiction of ASTM Committee D20 on Plastics and is the direct responsibility of Subcommittee D20.40 on Optical Properties.

Current edition approved Nov. 1, 2013. Published November 2013. Originally approved in 1998. Last previous edition approved in 2005 as D6290 - 05^{ε1}. DOI: 10.1520/D6290-13.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

[E313 Practice for Calculating Yellowness and Whiteness Indices from Instrumentally Measured Color Coordinates](#)

[E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

[E1331 Test Method for Reflectance Factor and Color by Spectrophotometry Using Hemispherical Geometry](#)

[E1347 Test Method for Color and Color-Difference Measurement by Tristimulus Colorimetry](#)

[E1349 Test Method for Reflectance Factor and Color by Spectrophotometry Using Bidirectional \(45°:0° or 0°:45°\) Geometry](#)

3. Terminology

3.1 *Definitions*—Refer to Terminologies [D883](#) and [E284](#) for definitions of terms used in this test method.

4. Significance and Use

4.1 Before proceeding with this test method, make reference should be made to the specification of the material being tested. Any test specimen preparation, conditioning, dimensions, or testing parameters, or a combination thereof, covered in the materials specification shall take precedence over those mentioned in this test method. If there are no material specifications, then default conditions apply.

NOTE 2—Some materials, such as polyamide (nylon), can be cooled very differently during the production of the pellets. This variation in the cooling of the pellets can result in different levels of crystallinity in the pellets only. More crystalline nylons will be more opaque than amorphous nylons. This will result in differences in pellet opacity. The pellet shape is independent of the crystallinity of the material. This variation in pellet appearance, due to varying levels of crystallinity, does not affect final properties.

NOTE 3—This test method should not be used for general material specifications.

4.2 This test method describes a technique useful for making color comparisons of resins in pellet form that is fast and convenient as it does not require preparation, such as molding or extruding specimens. The test method shall be used only to compare specimens of similar pellet shape, size, texture, and degree of translucency. For example, compare translucent disc-shaped pellets to translucent disc-shaped pellets, not with opaque, rectangular shaped pellets.

4.3 Exact measurements of resin pellet color are not necessarily directly related to the color of the final cast, molded or extruded product due to the multitude of variables, such as

*A Summary of Changes section appears at the end of this standard

producing variables, methods, and pellet shape and size. Color measurements can be useful for comparing resins in pellet form when all samples are similar in shape and size.

4.4 A three-number tristimulus system is necessary to quantify color completely and precisely. The general method used in this procedure measures color using the CIE Systems described in Practice E308, Test Method D2244, the CIE 1976 (X, Y, Z) system, and, the CIELAB 1976 color space.³

4.5 Individual components of the tristimulus measurement such as CIE Y (Luminance), Hunter L, a, b, or CIE L*, a*, b* values or other useful metrics like yellowness index can be used to describe color attributes of materials. This test method describes a standard procedure on how these measurements are made.

5. Interferences

5.1 Comparisons of color measurements can only be made if the material is the same, the pellet cut, size and shape are essentially the same and the test instrument is the same type and within the same group. (See 6.2 and Section 10 and Tables A and B for instrument differences.)

6. Apparatus

6.1 Choices of apparatus include spectrophotometer, or tristimulus colorimeter, conforming to Guide E179.

6.2 There are several different optical geometries currently being used for measuring color. It is important that similar optical geometries be used if results are to be compared. These are designated as Groups defined as follows:

6.2.1 *Group I*—Spectrophotometer with 45 to 52-mm port with 0/45 directional geometry. See Test Methods E1347 and E1349.

6.2.2 *Group II*—Colorimeter with 31 to 52-mm port with 45/0 directional geometry. See Test Methods E1347 and E1349.

6.2.3 *Group III*—Sphere with minimum of 25-mm port with a nominal 0/diffuse geometry. See Test Methods E1331 and E1347.

6.2.4 *Group IV*—Sphere with minimum of 25-mm port with a nominal diffuse/0 geometry. See Test Methods E1331 and E1347.

6.3 Other optical geometries are potentially used for this test method, they need to be added if being used and brought to our attention as this procedure is being evaluated.

6.4 *Calibrated tiles*, for instrument standardization.

6.5 *Glass (clear)*, specimen cell at least 60-mm (2 1/2-in.) diameter and a minimum of 50-mm depth and black sample cover of sufficient size to prevent external light from affecting the pellet measurement.

NOTE 4—The clear sample holder may be any shape that is larger than

the port with at least 6-mm between the edge of the port and the edge of the sample holder.

7. Procedure

7.1 Standardize the instrument in accordance with the manufacturer's written instructions (usually once per shift).

7.2 Fill the sample cup to the top with pellets.

7.3 Center the pellet filled cup at the sensor port for measurement. Use a centering device if one is provided by the manufacturer.

7.4 Cover the sample cup with an opaque, light exclusion device or cover.

7.5 For Yellowness Index make, the necessary readings of Tristimulus X, Y, Z to determine Yellowness Index as described in Test Method E313 as soon as possible using illuminant "C", specular excluded, and CIE 1931 2° observer.

NOTE 5—Care must be taken not to allow the pellet sample to remain at the measurement port for a long period of time prior to measurement. Light exposure of high intensity may cause yellowness to change, thus altering the test value.

NOTE 6—Many instruments will report the Yellowness Index in accordance with Test Method E313 directly thus no calculations are required for individual Yellowness Index value.

7.5.1 For other measurements, such as Hunter L, a, b or CIE L*, a*, b* make the necessary instrument settings and take the readings.

7.6 Repeat steps 7.2 through 7.5.1 two more times for a total of three results.

8. Calculation

8.1 Determine the average yellowness index, YI, if requested, using the following formula:

$$YI = 100 (C_x X - C_z Z) / Y \quad (1)$$

where:

$C_x = 1.2769$, and

$C_z = 1.0592$.

8.2 Determine the average yellowness index by summing the test values and divide by the number of samples tested.

9. Report

9.1 Report the following information:

9.1.1 Average of the Yellowness Index or other measurements if noted,

9.1.2 Sample identification, such as lot number, source, etc.,

9.1.3 Date test was conducted,

9.1.4 The instrument group or geometry, and

9.1.5 The instrument used including name of manufacturer, model, and serial number.

10. Precision and Bias⁴

10.1 *Precision:*

³ Based upon the *Colorimetry, 2nd ed.*, Publication CIE No. 15.2, Central Bureau of the CIE, Vienna, 1986. Currently available through the U.S. National Committee of the CIE, % Mr. Thomas Lemmons, TLA Lighting Consultants, Inc., 7 Pond St., Salem, MA 01970-4819.

⁴ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D20-1235.

10.1.1 **Table 1** reflects data tested with ten instruments in Group I, and **Table 2** with six instruments in Group II. All data are based on a round robin conducted in 1994-1995 in accordance with Practice **E691**, involving eight materials tested with six test results measured on three days by each laboratory. For each material, pellets were gathered and packaged by one source and the individual packages were sent to each of the laboratories which tested them. Each test result is the value of an individual determination. Each laboratory obtained six test results for each materials. **Table 1A** and **Table 2B** reflect the values as if each test value consisted of an average of three readings. (**Warning**—The following explanations of r and R (10.1.2 through 10.1.4) only are intended to present a meaningful way of considering approximate precision of this test method. It is not appropriate to rigorously apply the data in **Table 1**, **Table 2**, **Table 1A**, and **Table 2A** to acceptance or rejection of material, as those data are specific to the round robin and are not necessarily representative of other lots, conditions, materials, or laboratories. Users of this test method need to apply the principles outlined in Practice **E691** to generate data specific to their laboratory and materials or between specific laboratories. The principles of 10.1.2 through 10.1.4 then would be valid for such data.)

10.1.2 *Concept of r and R* —If S_r and S_R have been calculated from a large enough body of data and for test results that are the result of testing one specimen:

10.1.3 *Repeatability Limit, r (Comparing two test results for the same material, obtained by the same operator using the same equipment on the same day)*—Judge the two test results

TABLE 1 Yellowness Index of Pellets

Material	Apparatus Group I				
	Average	S_r^A	S_R^B	r^C	R^D
Material G	-3.99	0.206	0.495	0.576	1.385
Material B	-0.33	0.130	0.424	0.363	1.188
Material F	-0.133	0.113	0.524	0.317	1.467
Material H	0.538	0.076	0.443	0.214	1.241
Material C	1.539	0.095	0.398	0.267	1.116
Material E	8.82	0.376	1.840	1.052	5.153
Material A	15.8	0.365	0.877	1.023	2.455
Material D	24.6	0.139	0.860	0.390	2.409

TABLE 1A Yellowness Index of Pellets

Material	Estimate for Three Specimens (Apparatus Group I)				
	Average	S_r^A	S_R^B	r^C	R^D
Material G	-3.99	0.092	0.459	0.258	1.286
Material B	-0.33	0.058	0.408	0.162	1.143
Material F	-0.133	0.051	0.514	0.142	1.439
Material H	0.538	0.034	0.438	0.096	1.226
Material C	1.539	0.043	0.389	0.119	1.090
Material E	8.82	0.168	1.809	0.470	5.067
Material A	15.8	0.163	0.813	0.458	2.278
Material D	24.6	0.062	0.851	0.174	2.383

^A S_r is the within-laboratory standard deviation or the indicated material. It is obtained by pooling the within-laboratory standard deviations of the test results from all of the participating laboratories:

$$S_r = [((s_1)^2 + (s_2)^2 - \dots + (s_n)^2)/n]^{1/2}$$

^B S_R is the between-laboratories reproducibility, expressed as standard deviation:

$$S_R = [S_r^2 + S_L^2]^{1/2}$$

where: S_L is the standard deviation of laboratory means.

^C r is the within-laboratory critical interval between two test results = $2.8 \times S_r$.

^D R is the between-laboratories critical interval between two test results = $2.8 \times S_R$.

TABLE 2 Yellowness Index of Pellets

Material	Apparatus Group II				
	Average	S_r^A	S_R^B	r^C	R^D
Material G	-5.32	0.361	1.01	1.01	2.82
Material F	-1.85	0.177	0.838	0.495	2.35
Material H	-1.64	0.138	0.512	0.387	1.43
Material B	-1.61	0.152	0.646	0.425	1.81
Material C	-0.126	0.220	0.507	0.617	1.42
Material E	7.21	0.289	2.20	0.810	6.15
Material A	13.3	0.352	2.01	0.986	5.63
Material D	20.6	0.167	1.45	0.468	4.07

TABLE 2A Yellowness Index of Pellets

Material	Estimate for Three Specimens (Apparatus Group II)				
	Average	S_r^A	S_R^B	r^C	R^D
Material G	-5.32	0.161	0.908	0.452	2.54
Material F	-1.85	0.079	0.823	0.173	2.31
Material H	-1.64	0.062	0.497	0.173	1.39
Material B	-1.61	0.068	0.632	0.190	1.77
Material C	-0.126	0.098	0.467	0.276	1.31
Material E	7.21	0.129	2.18	0.362	6.11
Material A	13.3	0.158	1.98	0.441	5.56
Material D	20.6	0.075	1.44	0.209	4.05

^A S_r is the within-laboratory standard deviation or the indicated material. It is obtained by pooling the within-laboratory standard deviations of the test results from all of the participating laboratories:

$$S_r = [((s_1)^2 + (s_2)^2 - \dots + (s_n)^2)/n]^{1/2}$$

^B S_R is the between-laboratories reproducibility, expressed as standard deviation:

$$S_R = [S_r^2 + S_L^2]^{1/2}$$

where: S_L is the standard deviation of laboratory means.

^C r is the within-laboratory critical interval between two test results = $2.8 \times S_r$.

^D R is the between-laboratories critical interval between two test results = $2.8 \times S_R$.

TABLE 3 Yellowness Index of Pellets

Material	All Apparatus Groups				
	Average	S_r^A	S_R^B	r^C	R^D
Material G	-4.69	1.04	1.45	2.92	4.05
Material F	-1.61	1.06	1.91	2.96	5.36
Material B	-0.979	0.504	1.03	1.41	2.88
Material H	0.014	4.13	4.13	11.6	11.6
Material C	2.08	5.77	5.77	16.2	16.2
Material E	6.51	2.45	3.77	6.87	10.6
Material A	12.7	3.78	4.87	10.6	13.6
Material D	20.7	3.94	5.50	11.0	15.4

TABLE 3A Yellowness Index of Pellets

Material	Estimate for Three Specimens—All Apparatus Groups				
	Average	S_r^A	S_R^B	r^C	R^D
Material G	-4.69	0.466	1.11	1.30	3.10
Material F	-1.61	0.473	1.66	1.33	4.66
Material B	-0.979	0.226	0.925	0.632	2.59
Material H	0.014	1.85	1.85	5.17	5.17
Material C	2.08	2.58	2.58	7.23	7.23
Material E	6.51	1.10	3.07	3.07	8.60
Material A	12.7	1.69	3.50	4.73	9.81
Material D	20.7	1.76	4.23	4.93	4.23

^A S_r is the within-laboratory standard deviation or the indicated material. It is obtained by pooling the within-laboratory standard deviations of the test results from all of the participating laboratories:

$$S_r = [((s_1)^2 + (s_2)^2 - \dots + (s_n)^2)/n]^{1/2}$$

^B S_R is the between-laboratories reproducibility, expressed as standard deviation:

$$S_R = [S_r^2 + S_L^2]^{1/2}$$

where: S_L is the standard deviation of laboratory means.

^C r is the within-laboratory critical interval between two test results = $2.8 \times S_r$.

^D R is the between-laboratories critical interval between two test results = $2.8 \times S_R$.

should be judged not equivalent if they differ by more than the r value for that material.

10.1.4 *Reproducibility Limit, R (Comparing two test results for the same material, obtained by different operators using different equipment in different laboratories)*—Judge the two test results should be judged not equivalent if they differ by more than the *R* value for that material.

10.1.5 Any judgment in accordance with 10.1.1 or 10.1.2 would have an approximate 95 % (0.95) probability of being correct.

10.2 *Bias*—There are no recognized standards by which to estimate bias of this test method.

11. Keywords

11.1 color; pellets; plastics; yellowness; yellowness index

ANNEX

(Mandatory Information)

A1. RR PRODUCTS IDENTIFICATION

A1.1 Identify RR Products as follows:

A1.1.1 *A*—PP Random

A1.1.2 *B*—PP Random

A1.1.3 *C*—PP Impact

A1.1.4 *D*—PP Impact

A1.1.5 *E*—PP Homopolymer

A1.1.6 *F*—LDPE

A1.1.7 *G*—EVA Copolymer

A1.1.8 *H*—HDPE

APPENDIXES

(Nonmandatory Information)

X1. ADDITIONAL INSTRUMENT INFORMATION

X1.1 As discussed in this test method, there are many instruments with different geometries being used to make the measurements described herein. Different instruments give different values so comparison of data can only be done when

similar instruments are used. For example, compare the average values in Table 1 to those in Table 2. Table 3 and Table 3A show the effect the different apparatus have on the test results.

X2. GROUP IDENTIFICATION

X2.1 *Group I*—Spectrophotometers with 45 to 52-mm port and 0/45 circumferential geometry.

X2.2 *Group II*—Colorimeter with 31 to 52-mm port and 45/0 bidirectional.

X2.3 *Group III*—Sphere with 25-mm port with 0/diffuse geometry.

X2.4 *Group IV*—Sphere with 25-mm port with diffuse/0 geometry.

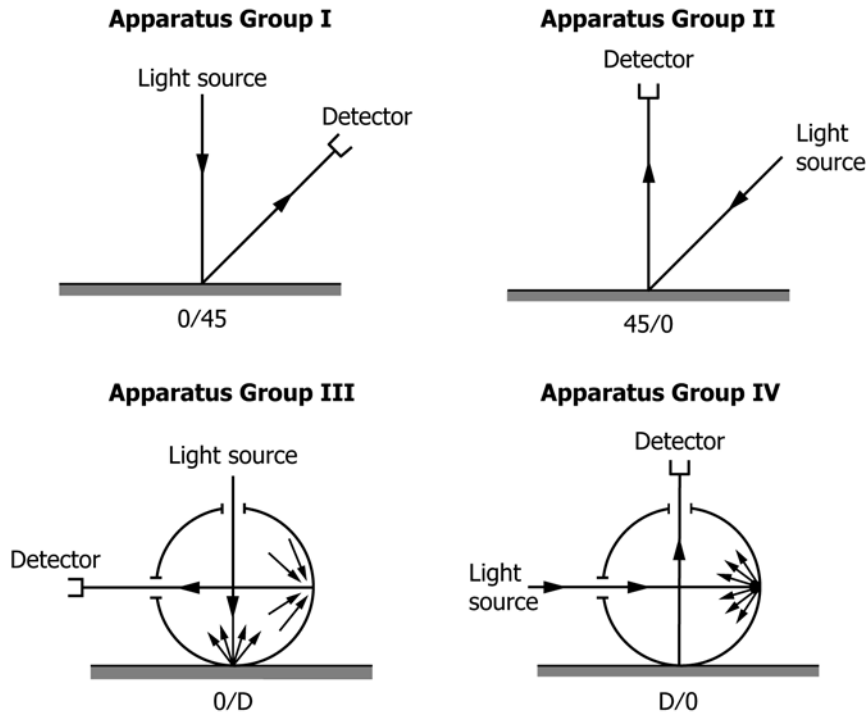


FIG. X1.1 CIE Recommended Illuminating and Viewing Geometries

SUMMARY OF CHANGES

Committee D20 has identified the location of selected changes to this standard since the last issue, D6290 - 05^{e1}, that may impact the use of this standard. (November 1, 2013)

- (1) Reworded ISO statement in **Note 1** in accordance with Guide D4968.
- (2) Guide E179 was reinstated, leave in **2.1** and **6.1**.
- (3) Widened the port size to 31 to 52 mm in **6.2.2** and **X2.2**.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; http://www.copyright.com/