



Designation: D7344 – 17

# Standard Test Method for Distillation of Petroleum Products and Liquid Fuels at Atmospheric Pressure (Mini Method)<sup>1</sup>

This standard is issued under the fixed designation D7344; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope\*

1.1 This test method covers the procedure for the determination of the distillation characteristics of petroleum products and liquid fuels in the range of 20 °C to 400 °C (68 °F to 752 °F) using miniaturized automatic distillation apparatus.

1.2 This test method is applicable to such products as: light and middle distillates, automotive spark-ignition engine fuels, automotive spark-ignition engine fuels containing up to 10 % ethanol, aviation gasolines, aviation turbine fuels, all grades of No. 1 and No. 2 diesel fuels (as described in Specification D975), biodiesel (B100), biodiesel blends up to 30 % biodiesel, special petroleum spirits, pure petrochemical compounds, naphthas, white spirits, kerosenes, furnace fuel oils, and distillate marine fuels.

NOTE 1—The up to 10 % by volume ethanol limit in spark ignition engine fuels (E10) was the range used in the supporting interlaboratory studies. Spark ignition engine fuels containing > 10 % by volume ethanol and up to 20 % by volume ethanol (E20) may be analyzed, however the stated precision and bias does not apply.

1.3 This test method is designed for the analysis of distillate products; it is not applicable to products containing appreciable quantities of residual material.

1.4 The values stated in SI units are to be regarded as the standard. The values given in parentheses are for information only.

1.5 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

1.6 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recom-*

*mendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>2</sup>

D86 Test Method for Distillation of Petroleum Products and Liquid Fuels at Atmospheric Pressure

D323 Test Method for Vapor Pressure of Petroleum Products (Reid Method)

D975 Specification for Diesel Fuel Oils

D1160 Test Method for Distillation of Petroleum Products at Reduced Pressure

D4057 Practice for Manual Sampling of Petroleum and Petroleum Products

D4177 Practice for Automatic Sampling of Petroleum and Petroleum Products

D4953 Test Method for Vapor Pressure of Gasoline and Gasoline-Oxygenate Blends (Dry Method)

D5190 Test Method for Vapor Pressure of Petroleum Products (Automatic Method) (Withdrawn 2012)<sup>3</sup>

D5191 Test Method for Vapor Pressure of Petroleum Products (Mini Method)

D5482 Test Method for Vapor Pressure of Petroleum Products (Mini Method—Atmospheric)

D6300 Practice for Determination of Precision and Bias Data for Use in Test Methods for Petroleum Products and Lubricants

D6708 Practice for Statistical Assessment and Improvement of Expected Agreement Between Two Test Methods that Purport to Measure the Same Property of a Material

### 2.2 Energy Institute Standards:<sup>4</sup>

IP 69 Determination of Vapour Pressure—Reid Method

IP 394 Determination of Air Saturated Vapour Pressure

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee D02 on Petroleum Products, Liquid Fuels, and Lubricants and is the direct responsibility of Subcommittee D02.08 on Volatility.

Current edition approved May 1, 2017. Published June 2017. Originally approved in 2007. Last previous edition approved in 2014 as D7344 – 14. DOI: 10.1520/D7344-17.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>3</sup> The last approved version of this historical standard is referenced on [www.astm.org](http://www.astm.org).

<sup>4</sup> Available from Energy Institute, 61 New Cavendish St., London, WIG 7AR, U.K., <http://www.energyinst.org.uk>.

\*A Summary of Changes section appears at the end of this standard

### 3. Terminology

#### 3.1 Definitions:

3.1.1 *decomposition, n*—of a hydrocarbon, pyrolysis or cracking of a molecule yielding smaller molecules with lower boiling points than the original molecule.

3.1.1.1 *decomposition point, n*—in distillation, the corrected temperature reading that coincides with the first indications of thermal decomposition of the specimen.

3.1.2 *dynamic holdup, n*—in D7344 distillation, amount of material present in the distillation column, and in the condenser during the distillation.

3.1.3 *end point (EP) or final boiling point (FBP), n*—maximum corrected temperature reading obtained during the test.

3.1.4 *initial boiling point (IBP), n*—in D7344 distillation, corrected temperature reading at the instant of the first detection of condensate in the receiver.

3.1.5 *percent evaporated, n*—in distillation, sum of the percent recovered and the percent loss.

3.1.6 *percent loss, n*—in distillation, one hundred minus the percent total recovery.

3.1.6.1 *corrected loss, n*—percent loss corrected for barometric pressure.

3.1.7 *percent recovered, n*—in distillation, the volume of condensate collected relative to the sample charge.

3.1.8 *percent recovery, n*—in distillation, maximum percent recovered relative to the sample charge.

3.1.8.1 *corrected percent recovery, n*—in distillation, the percent recovery, adjusted for the corrected percent loss.

3.1.8.2 *percent total recovery, n*—in distillation, the combined percent recovery and percent residue.

3.1.9 *percent residue, n*—in distillation, the volume of residue relative to the sample charge.

3.1.10 *sample charge, n*—the amount of sample used in a test.

3.1.11 *vapor temperature reading, n*—temperature of the saturated vapor measured in the distillation column below the vapor tube, as determined by the prescribed conditions of the test.

3.1.11.1 *corrected vapor temperature reading, n*—temperature reading, as described in 3.1.11, corrected for barometric pressure.

### 4. Summary of Test Method

4.1 Based on its composition, vapor pressure, expected IBP or expected FBP, or a combination thereof, the sample is placed in one of five groups. Condenser temperature and other operational variables are defined by the group in which the sample falls.

4.2 A specimen of the sample is distilled under prescribed conditions for the group in which the sample falls. The specimen volume for distillation Groups 0 to 3 is 6 mL. For Group 4, the specimen volume is 5.5 mL. The distillation is performed in an automatic, miniaturized distillation apparatus

at ambient pressure under conditions that are designed to provide approximately one theoretical plate fractionation. The vapor temperature readings and volumes of condensate are monitored continuously. After the test, specimen losses and residue are recorded.

4.3 After conclusion of the test, the temperatures are automatically corrected for barometric pressure, using the pressure reading of a built-in pressure transducer. The data are examined for conformance to procedural requirements, such as distillation rates. The test has to be repeated if any specified condition has not been met.

4.4 Test results are commonly expressed as percent volume evaporated or percent volume recovered versus corresponding vapor temperature, either in a table or graphically, as a plot of the distillation curve.

4.5 This test method uses a small specimen volume and miniaturized apparatus which can be portable for field testing.

### 5. Significance and Use

5.1 The distillation (volatility) characteristics of hydrocarbons and other liquids have an important effect on their safety and performance, especially in the case of fuels and solvents. The boiling range gives information on the composition, the properties, and the behavior of the fuel during storage and use. Volatility is the major determinant of the tendency of a hydrocarbon mixture to produce potentially explosive vapors.

5.2 The distillation characteristics are equally important for both automotive and aviation gasolines, affecting starting, warm-up, and tendency to vapor lock at high operating temperatures or high altitude, or both. The presence of high boiling point components in these and other fuels can significantly affect the degree of formation of solid combustion deposits.

5.3 Volatility, as it affects the rate of evaporation, is an important factor in the application of many solvents, particularly those used in paints.

5.4 Distillation limits are often included in petroleum product specifications, in commercial contract agreements, process refinery/control applications, and for compliance to regulatory rules.

5.5 This test method is suitable for setting specifications, for use as an internal quality control tool, and for use in development or research work on hydrocarbon solvents.

5.5.1 This test method gives a broad indication of general purity and can also indicate presence of excessive moisture. It will not differentiate between products of similar boiling range.

### 6. Apparatus

6.1 *Automatic Distillation Apparatus*—The type of apparatus suitable for this test method employs a heat source, a specimen cup, a stainless steel distillation column, a temperature measuring device, a thermoelectrically controlled condenser and receiver system, a thermoelectrically controlled sample introduction and dosing system, and a system to measure and automatically record the vapor temperature, the

associated percent recovered volume in the receiver, the condenser temperature, and the barometric pressure.<sup>5</sup>

6.2 A description of the apparatus is given in **Annex A1**.

6.3 *Sample Introduction and Dosing System*—A system capable to automatically draw sample from a sample container and fill the specimen container cup with a specimen of 6 mL ± 0.05 mL or 5.5 mL ± 0.05 mL.

6.4 *Temperature Measuring Device*—A thermocouple (NiCr-Ni or similar) in stainless steel tube of 1 mm ± 0.02 mm diameter with a response time of  $t(90) = 3\text{ s} \pm 1\text{ s}$  shall be used for measuring the temperature of the vapor. The minimum resolution shall be 0.1 °C (0.2 °F), and the minimum accuracy ±0.1 °C (0.2 °F).

6.5 *Pressure Transducer*—A pressure transducer with a minimum range of 0 kPa to 120 kPa with a minimum resolution of 0.1 kPa shall be used. The minimum accuracy shall be ±0.1 kPa.

6.6 *Balance*, with a minimum range of 25 g and a minimum accuracy of ±3 mg.

6.7 *Pressure Measuring Device for Calibration*, capable of measuring local station pressure with an accuracy and a resolution of 0.1 kPa (1 mm Hg) or better, at the same elevation relative to sea level as the apparatus in the laboratory.

## 7. Reagents and Materials

7.1 *Purity of Reagents*—Use chemicals of at least 99 % purity for quality control checks. Quality control check materials used in this test method are toluene (**Warning**—Flammable and a health hazard) and hexadecane (see Section 10). Unless otherwise indicated, it is intended that all reagents conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society<sup>6</sup> where such specifications are available. Lower purities can be used, provided it is first ascertained that the reagent is of sufficient purity to permit its use without lessening the accuracy of the determination.

NOTE 2—The chemicals in this section are suggested for quality control procedures (see Section 10) and are not used for instrument calibration.

## 8. Sampling, Storage, and Sample Conditioning

8.1 Determine the group characteristics that correspond to the sample to be tested (see **Table 1**). Where the procedure is dependent upon the group, the section headings will be so marked.

### 8.2 Sampling:

<sup>5</sup> The sole source of supply of the apparatus known to the committee at this time is Grabner Instruments, A-1220 Vienna, Dr. Otto Neurathgasse 1, Austria. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,<sup>1</sup> which you may attend.

<sup>6</sup> *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC. For Suggestions on the testing of reagents not listed by the American Chemical Society, see *Annual Standards for Laboratory Chemicals*, BDH Ltd., Poole, Dorset, U.K., and the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD.

**TABLE 1 Group Characteristics**

	Group 0	Group 1	Group 2	Group 3	Group 4
Sample characteristics	Pure	Gasoline	Gasoline	Jet Fuel	Diesel
Distillate type					
Vapor pressure at:					
37.8 °C, kPa			<65.5	<65.5	<65.5
100 °F, psi			<9.5	<9.5	<9.5
(Test Methods <b>D323</b> , <b>D4953</b> , <b>D5190</b> , <b>D5191</b> , <b>D5482</b> , IP 69, or IP 394)					
Distillation:					
IBP	°C >20	≤100	>100	>100	>100
	°F >68	≤212	>212	>212	>212
EP	°C <400	≤250	≤250	>250	>250
	°F <752	≤482	≤482	>482	>482

8.2.1 Only samples that are liquid at room temperature can be tested by this test method.

8.2.2 Sampling shall be done as described in **Table 2** and in accordance with Practice **D4057** or **D4177**, except do not use the “Sampling by Water Displacement” section for fuels containing oxygenates.

8.2.2.1 *Groups 1 and 2*—Collect the sample as described in **8.2.2** at a temperature below 10 °C (50 °F). If this is not possible because, for instance, the product to be sampled is at ambient temperature, the sample shall be drawn into a bottle prechilled to below 10 °C (50 °F), in such a manner that agitation is kept at a minimum. Close the bottle immediately with a tight-fitting closure. (**Warning**—Do not completely fill and tightly seal a cold bottle of sample due to the likelihood of breakage upon warming.)

8.2.2.2 *Groups 0, 3, and 4*—Collect the sample at ambient temperature. After sampling, close the sample bottle immediately with a tight-fitting closure.

8.2.2.3 If the sample received by the testing laboratory has been sampled by others and it is not known whether sampling has been performed as described in **8.2**, the sample shall be assumed to have been so sampled.

8.2.2.4 Follow the manufacturer’s instructions for introducing the test specimen into the measuring chamber.

### 8.3 Sample Storage:

8.3.1 If testing is not to start immediately after collection, store the samples as indicated in **8.3.2** and **8.3.3** and **Table 2**. All samples shall be stored away from direct sunlight or sources of direct heat.

8.3.2 *Groups 1 and 2*—Store the sample at a temperature below 10 °C (50 °F).

NOTE 3—If there are no, or inadequate, facilities for storage below or equal 10 °C (50 °F), the sample may also be stored at a temperature below 20 °C (68 °F), provided the operator ensures that the sample container is tightly closed and leak-free.

8.3.3 *Groups 0, 3, and 4*—Store the sample at ambient or lower temperature.

### 8.4 Sample Conditioning Prior to Analysis:

8.4.1 Samples shall be conditioned to the temperature shown in **Table 2** before opening the sample container.

8.4.1.1 *Groups 1 and 2*—Samples shall be conditioned to a temperature of less than 10 °C (50 °F) before opening the sample container.

**TABLE 2 Sampling, Storage, and Sample Conditioning**

	Group 0	Group 1	Group 2	Group 3	Group 4
Temperature of sample bottle	°C	<10			
	°F	<50			
Temperature of stored bottle	°C ambient	<10 <sup>A</sup>	<10 <sup>A</sup>	ambient	ambient
	°F ambient	<50 <sup>A</sup>	<50 <sup>A</sup>	ambient	ambient
Temperature of sample after conditioning prior to analysis	°C ambient	<10	<10	ambient	ambient
	°F ambient	<50	<50	ambient	ambient
If sample is wet <sup>B</sup>		dry <sup>C</sup>	resample	resample	dry <sup>C</sup>
If sample is still wet <sup>B</sup>		dry <sup>D</sup>	dry <sup>D</sup>		dry <sup>C</sup>

<sup>A</sup> Under certain circumstances, samples may also be stored at temperatures below 20 °C (68 °F). See also 8.3.3.

<sup>B</sup> If sample is known to be wet, resampling may be omitted. Dry sample in accordance with 8.5.2 and 8.5.3.

<sup>C</sup> Dry in accordance with 8.5.3.

<sup>D</sup> Dry in accordance with 8.5.2.

8.4.1.2 *Groups 0, 3, and 4*—Samples shall be conditioned to a temperature not above ambient before opening the sample container.

### 8.5 Wet Samples:

8.5.1 Samples of materials that visibly contain water are not suitable for testing. If the sample is not dry, obtain another sample that is free from suspended water.

8.5.2 *Groups 1, and 2*—If such a sample cannot be obtained, the suspended water can be removed by maintaining the sample at 0 °C to 10 °C (32 °F to 50 °F), adding approximately 10 g of anhydrous sodium sulfate per 100 mL of sample, shaking the mixture for approximately 2 min, and then allowing the mixture to settle for approximately 15 min. Once the sample shows no visible signs of water, use a decanted portion of the sample, maintained between 1 °C and 10 °C (34 °F and 50 °F), for the analysis. Note in the report that the sample has been dried by the addition of a desiccant.

NOTE 4—Suspended water in hazy samples in Groups 1 and 2 can be removed by the addition of anhydrous sodium sulfate and separating the liquid sample from the drying agent by decanting. For Test Method D86, it has been shown that this procedure does not statistically affect the results of the test.<sup>7</sup>

8.5.3 *Groups 0, 3, and 4*—In cases in which a water-free sample is not practical, the suspended water can be removed by shaking the sample with anhydrous sodium sulfate or other suitable drying agent and separating it from the drying agent by decanting. Note in the report that the sample has been dried by the addition of a desiccant.

## 9. Preparation of Apparatus

9.1 Refer to Table 1 and prepare the instrument by choosing the appropriate group in accordance with the manufacturer's instructions.

9.2 Place a specimen cup whose mass has been determined according to the manufacturer's instructions to be known to be at least ±3 mg on the specimen cup support in the apparatus.

<sup>7</sup> Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1455.

## 10. Verification of Calibration and Standardization

10.1 *Temperature Measuring Device*—Verify the calibration of the thermocouple used to monitor the vapor temperature at least every six months, and after the system has been replaced or repaired, against a thermometer which is traceable to National Institute of Standards and Technology (NIST) or national authorities in the country the equipment is used.

10.1.1 The temperature measuring device calibration can be checked by distilling pure toluene (**Warning**—Flammable and a health hazard) in accordance with this test method. The temperature measurement system shall indicate, at 50 % distilled, a temperature of 110.6 °C ± 0.8 °C (231 °F ± 1.5 °F).

10.1.2 To check the temperature measuring device at elevated temperatures, perform a distillation with hexadecane (cetane). The temperature measurement system shall indicate at 50 % distilled a temperature of 281.3 °C ± 1.5 °C (538.5 °F ± 3 °F) under Group 3 and 4 distillation conditions.

NOTE 5—The melting point of n-hexadecane is 18 °C (64.5 °F). If the sample is solid, heat it to about 25 °C (77 °F) and wait until all the material is liquid before starting the test.

10.2 *Pressure Transducer*—Check the calibration of the transducer at intervals of not more than six months, and after the instrument has been repaired. The calibration of the transducer is checked against ambient barometric pressure as measured by the pressure measuring device described in 6.7. If the displayed atmospheric pressure is not equal to the ambient barometric pressure, adjust the transducer control until the appropriate reading is observed. The ambient barometric pressure is the actual station pressure at the location of the tester at the time of measurement. (**Warning**—Many aneroid barometers, such as those used at weather stations and airports, are pre-corrected to give sea level readings. These shall not be used for calibration of the apparatus.)

10.3 *Receiver System*—The percent volume detection system of the apparatus shall have a resolution of 6 µL or better with a maximum error of 18 µL between the 0.3 mL and 6 mL points. The calibration of the assembly shall be verified in accordance with manufacturer's instructions at intervals of not more than six months and after the system has been replaced or repaired.

## 11. Procedure

11.1 Connect the specimen container filling system inlet tubing to the inlet of the apparatus and immerse it in the sample. For samples of Group 1, make provisions to avoid loss of high volatiles in the sample. The overall volume of the sample shall be at least 50 mL for all distillation groups (see Table 1). Follow the manufacturer's instructions for introducing the test specimen into the measuring chamber.

11.2 Regulate the temperatures of the specimen container filling system, the condenser, and the receiver system for the appropriate group of the sample as specified in Table 3. For biodiesel (B100), the condenser and receiver system is regulated to 60 °C ± 0.2 °C.

**TABLE 3 Default Conditions During Test Procedure<sup>A</sup>**

		Group 0	Group 1	Group 2	Group 3	Group 4
Temperature of filling system <sup>A</sup>	°C	10 ± 0.2	10 ± 0.2	10 ± 0.2	10 ± 0.2	40 ± 0.2
	°F	50 ± 0.4	50 ± 0.4	50 ± 0.4	50 ± 0.4	104 ± 0.4
Temperature of condenser <sup>A</sup>	°C	10 ± 0.2	10 ± 0.2	10 ± 0.2	10 ± 0.2	40 ± 0.2
	°F	50 ± 0.4	50 ± 0.4	50 ± 0.4	50 ± 0.4	104 ± 0.4
Temperature of receiver system <sup>A</sup>	°C	10 ± 0.2	10 ± 0.2	10 ± 0.2	10 ± 0.2	40 ± 0.2
	°F	50 ± 0.4	50 ± 0.4	50 ± 0.4	50 ± 0.4	104 ± 0.4
Time from first application of heat to initial boiling point, min		<12	<7	<8	<12	<12
Uniform rate of condensation at 5 % recovered and 95 % recovered, mL/min		≥0.15	≥0.15	≥0.15	≥0.15	≥0.15
Uniform rate of condensation from 10 % recovered to 90 % recovered, mL/min		0.3–0.9	0.3–0.9	0.3–0.9	0.3–0.9	0.3–0.9
Time from 95 % recovered to end point, min		<4	<4	<4	<4	<4
Specimen volume of sample (mL)		6 ± 0.05	6 ± 0.05	6 ± 0.05	6 ± 0.05	5.5 ± 0.05
Mean density of liquid residual, g/ccm		0.72	0.76	0.76	0.86	0.87

<sup>A</sup> The proper temperature will depend upon the wax content of the sample and of its distillation fractions. The test is generally performed using one single temperature. Wax formation in the condenser can be deduced from (a) the presence of wax particles in the distillate, (b) a higher distillation loss than what would be expected based on the initial boiling point of the specimen, (c) an erratic recovery rate and (d) the presence of wax particles during cleaning of the condenser with a lint-free swab. The minimum temperature that permits satisfactory operation shall be used. In some cases involving grade No. 2 fuel oil, Grade No. 2-D diesel fuel oil, gas oils, pure petrochemical compounds, and similar distillates, it may be necessary to hold the condenser, receiver and filling system temperature in the 40 °C to 60 °C (86 °F to 140 °F) range. Also, for very high volatile Group 1 samples, it may be necessary to decrease the filling and receiving temperature to 5 °C (41 °F).

11.3 *Filling*—Following the manufacturer’s instructions, draw in sample, and place a specimen of 6 mL ± 0.05 mL (Groups 0 to 3) or 5.5 mL ± 0.05 mL (Group 4) into the specimen cup.

11.4 *Initial Boiling Point*—Apply heat to the specimen cup and note the start time.

11.5 Regulate the specimen container heating so that the time interval between the first application of heat and the IBP is as specified in **Table 3**. Record the IBP to the nearest 0.1 °C (0.2 °F).

11.6 Continue to regulate the specimen container heating so that the uniform average rate of condensation from 5 % or 10 % recovered to 95 % recovered is 0.6 mL ± 0.3 mL per min, as specified in **Table 3**. (**Warning**—Due to the configuration of the distillation column and the conditions of the test, the vapor and liquid around the temperature sensor are not in thermodynamic equilibrium. The distillation rate will consequently have an effect on the measured vapor temperature. The distillation rate shall, therefore, be kept as constant as possible throughout the test.)

**NOTE 6**—When testing gasoline samples, it is not uncommon to see the condensate suddenly form non-miscible liquid phases and bead up on the temperature sensor and in the neck of the distillation column at a vapor temperature of around 160 °C (320 °F). This may be accompanied by a sharp (about 3 °C (6 °F)) dip in the vapor temperature and a drop in the recovery rate. The phenomenon, which may be due to the presence of trace water in the sample, may last for 10 s to 30 s before the temperature recovers and the condensate starts flowing smoothly again. This point is sometimes colloquially referred to as the Hesitation Point.

11.7 If a decomposition point is observed, discontinue the heating and proceed as directed in **11.13**.

**NOTE 7**—Characteristic indications of thermal decomposition are evolution of fumes and erratic, typically decreasing, temperature readings that occur during the final stages of the distillation.

11.8 In the interval between the IBP and the end of the distillation, record all volumes in the receiving cylinder to the nearest 5 µL, and all temperature readings to the nearest 0.1 °C (0.2 °F).

11.8.1 Record temperature readings at least at every 0.25 % recovered.

11.9 When the percent recovered is approximately 95 %, make a final adjustment of the heat. The time from the 95 %, recovered to the EP (FBP) shall be within the limits prescribed in **Table 3**. If this condition is not satisfied, repeat the test with appropriate modification of the final heat adjustment.

11.10 Observe and record the EP (FBP) as required, and discontinue the heating.

11.11 Allow the distillate to drain into the receiver, after specimen heating has been discontinued. The apparatus shall continually monitor the percent recovered volume until this volume changes by no more than 10 µL in 1 min.

11.12 Record the volume in the receiver, in mL, as the percent recovered volume.

11.13 After the specimen cup has cooled place the cup on a balance and determine the mass of the cup plus residual specimen to the nearest ±3 mg. (**Warning**—Take adequate precautions when removing the sample cup to prevent accidental burns. Remove the cup in accordance with the manufacturer’s instructions.)

11.13.1 If a residue larger than 300 mg is obtained and the distillation was not purposely terminated before the EP, check whether adequate heat was applied towards the end of the distillation and whether conditions during the test conform to those specified in **Table 3**.

11.14 Repeat any distillation that did not meet the requirements described in **11.5** and **11.6**.

NOTE 8—The test method is not designed for the analysis of distillate fuels containing appreciable quantities of residual material (see 1.2).

$$L_c = 0.5 + (L - 0.5) / \{1 + (101.3 - P_k) / 8.00\} \quad (6)$$

$$L_c = 0.5 + (L - 0.5) / \{1 + (760 - P) / 60.0\} \quad (7)$$

## 12. Calculations

12.1 Calculate the percent recovery in accordance with the following equation:

$$R = 100 V_R / V_S \quad (1)$$

where:

$R$  = percent recovery,  
 $V_R$  = recovered volume, in mL (see 11.14), and  
 $V_S$  = sample charge, in mL (see 11.3).

12.2 Calculate the percent residue in accordance with the following equation:

$$R_p = 100 (M_t - M_c) / (\rho_R V_S) \quad (2)$$

where:

$R_p$  = percent residue,  
 $M_t$  = total mass of specimen cup and residual specimen in the cup, as determined in 11.13, in g,  
 $M_c$  = mass of the empty specimen cup, in g,  
 $\rho_R$  = mean density of residual specimen (see Table 3), in g/ccm, and  
 $V_S$  = sample charge, in mL (see 11.3).

12.3 The percent total recovery is the sum of the percent recovery (see 12.1) and the percent residue (see 12.2). Deduct the percent total recovery from 100 to obtain the percent loss.

12.4 Correct temperature readings to 101.3 kPa (760 mm Hg) pressure. Obtain the correction to be applied to each temperature reading by means of the Sydney Young equation as given in Eq 3, Eq 4, or Eq 5, as appropriate.

For Celsius temperatures:

$$C_c = 0.0009 (101.3 - P_k) (273 + t_c) \quad (3)$$

$$C_c = 0.00012 (760 - P) (273 + t_c) \quad (4)$$

For Fahrenheit temperatures:

$$C_f = 0.00012 (760 - P) (460 + t_f) \quad (5)$$

where:

$t_c$  = the observed temperature reading in °C,  
 $t_f$  = the observed temperature reading in °F,  
 $C_c$  and  $C_f$  = corrections to be added algebraically to the observed temperature readings,  
 $P_k$  = barometric pressure, prevailing at the time and location of the test, in kPa, and  
 $P$  = barometric pressure, prevailing at the time and location of the test, in mm Hg.

12.4.1 After applying the corrections and rounding each result to the nearest 0.1 °C (0.2 °F), use the corrected temperature readings in all further calculations and reporting.

NOTE 9—Temperature readings are not corrected to 101.3 kPa (760 mm Hg) when product definitions, specifications, or agreements between the parties involved indicate, specifically, that such correction is not required or that correction shall be made to some other base pressure.

12.5 Correct the actual loss to 101.3 kPa (760 mm Hg) pressure when temperature readings are corrected to 101.3 kPa pressure. The corrected loss,  $L_c$ , is calculated from Eq 6 or Eq 7, as appropriate.

where:

$L$  = observed loss,  
 $L_c$  = corrected loss,  
 $P_k$  = pressure, kPa, and  
 $P$  = pressure, mm Hg.

NOTE 10—Eq 6 and 7 have been derived from the data in Table 7 and Eqs 5 and 6 in Test Method D86-95 and earlier versions. It is probable that Eq 6 and 7 shown were the original empirical equations from which the table and equations in the Test Method D86-95 and earlier versions were derived.

12.5.1 Calculate the corresponding corrected percent recovery in accordance with the following equation:

$$R_c = R + (L - L_c) \quad (8)$$

where:

$L$  = percent loss or observed loss,  
 $L_c$  = corrected loss,  
 $R$  = percent recovery, and  
 $R_c$  = corrected percent recovery.

12.6 To obtain the percent evaporated at a prescribed temperature reading, add the percent loss to each of the observed percent recovered at the prescribed temperature readings, and report these results as the respective percent evaporated, that is:

$$P_e = P_r + L \quad (9)$$

where:

$L$  = observed loss,  
 $P_e$  = percent evaporated, and  
 $P_r$  = percent recovered.

12.7 To report a temperature reading at a prescribed percent evaporated, obtain the desired temperature directly from the database as the temperature closest to and within 0.1 volume % of the prescribed percent evaporated.

NOTE 11—The available instruments perform most procedures described in Sections 11 and 12 automatically.

## 13. Report

13.1 Report the following information:

13.2 Report the barometric pressure to the nearest 0.1 kPa (1 mm Hg).

13.3 Report all volumetric readings in percentages to the nearest 0.1 %, and all temperature readings to the nearest 0.1 °C (0.2 °F).

13.4 After barometric corrections of the temperature readings have been made, the following data require no further calculation prior to reporting: IBP, EP (FBP), decomposition point, and all pairs of corresponding values involving percent recovered and temperature readings.

13.5 It is advisable to base the report on relationships between temperature readings and percent evaporated when the sample is a gasoline, or any other product classified under Group 1, or in which the percent loss is greater than 2.0. Otherwise, the report can be based on relationships between

temperature readings and percent evaporated or percent recovered. Every report must indicate clearly which basis has been used.

13.6 Report if a drying agent, as described in 8.5.2 or 8.5.3, was used.

## 14. Precision and Bias

14.1 *Precision*—The precision of this test method has been determined by the statistical examination of interlaboratory test results.<sup>8</sup>

NOTE 12—The precision has been derived according to the group number in the following fashion. Group 1 and 2 samples are labeled as NOT4, and Group 3 and 4 samples are labeled GRP4.

NOTE 13—Distillation limits are typically not specified for fuel oils of grades Nos. 4, 5, and 6.

NOTE 14—Information on the precision of % evaporated or % recovered at a prescribed temperature can be found in Annex A4.

14.1.1 *Repeatability*—The difference between successive test results obtained by the same apparatus under constant operating conditions on identical test material would, in the long run, in the normal and correct operation of the test method, exceed the following value only in one case in twenty:

Group 0: Refer to Annex A2 for tables of calculated repeatability.

IBP:	$r = T^3 \times 0.0000006265$	valid range: 65 °C – 215 °C
T10:	$r = T^{1.6477} \times 0.0002254$	valid range: 65 °C – 240 °C
T50:	$r = T^{0.81} \times 0.004725$	valid range: 65 °C – 255 °C
T90:	$r = T^{-0.2137} \times 0.6504$	valid range: 65 °C – 255 °C
FBP:	$r = T^{0.9815} \times 0.03547$	valid range: 65 °C – 265 °C

Groups 1 and 2 (NOT4): Refer to Annex A2 for tables of calculated repeatability.

IBP:	$r = 2.46$	valid range: 20 °C – 60 °C
E10:	$r = 1.97$	valid range: 40 °C – 65 °C
E50:	$r = 0.02939 \times (E - 50)$	valid range: 75 °C – 105 °C
E90:	$r = 2.45$	valid range: 145 °C – 165 °C
FBP:	$r = 3.22$	valid range: 170 °C – 200 °C

Group 3 and 4 (GRP4): Refer to Annex A2 for tables of calculated repeatability.

IBP:	$r = 3.57$	valid range: 150 °C – 190 °C
T10:	$r = 0.04782 \times (T - 135)$	valid range: 160 °C – 220 °C
T50:	$r = 0.01926 \times (T - 137)$	valid range: 165 °C – 285 °C
T90:	$r = 0.009911 \times (T - 20)$	valid range: 180 °C – 345 °C
T95:	$r = 0.006461 \times (T + 210)$	valid range: 185 °C – 355 °C
FBP:	$r = 0.01033 \times (T - 37)$	valid range: 200 °C – 370 °C

where:

E = evaporated temperature within valid range prescribed

T = recovered temperature within valid range prescribed

NOTE 15—For naphthas, solvents, and other similar materials where percent recovered are reported and the percent loss is typically less than one percent, the percent recovered temperatures can be considered identical to the percent evaporated temperatures, and precision can be calculated as shown for Group NOT4.

14.1.2 *Reproducibility*—The difference between two single and independent results obtained by different operators working in different laboratories on identical material would, in the long run, in the normal and correct operation of the test method, exceed the following values in only one case in twenty:

Group 0: Refer to Annex A2 for tables of calculated reproducibility.

<sup>8</sup> Supporting data (the results of the 2015 Interlaboratory Cooperative Test Program) have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1855. Contact ASTM Customer Service at service@astm.org.

IBP:	$R = T^3 \times 0.0000007052$	valid range: 65 °C – 215 °C
E10:	$R = T^{1.6477} \times 0.0002509$	valid range: 65 °C – 240 °C
E50:	$R = T^{0.81} \times 0.008968$	valid range: 65 °C – 255 °C
E90:	$R = T^{-0.2137} \times 1.6210$	valid range: 65 °C – 255 °C
FBP:	$R = T^{0.9815} \times 0.06388$	valid range: 65 °C – 265 °C

Group 1 and 2 (NOT4): Refer to Annex A2 for tables of calculated reproducibility.

IBP:	$R = 5.27$	valid range: 20 °C – 60 °C
E10:	$R = 4.68$	valid range: 40 °C – 65 °C
E50:	$R = 0.04536 \times (E - 50)$	valid range: 75 °C – 105 °C
E90:	$R = 3.53$	valid range: 145 °C – 165 °C
FBP:	$R = 4.82$	valid range: 170 °C – 200 °C

Group 3 and 4 (GRP4): Refer to Annex A2 for tables of calculated reproducibility.

IBP:	$R = 5.32$	valid range: 150 °C – 190 °C
T10:	$R = 0.06407 \times (T - 135)$	valid range: 160 °C – 220 °C
T50:	$R = 0.02475 \times (T - 137)$	valid range: 165 °C – 285 °C
T90:	$R = 0.01567 \times (T - 20)$	valid range: 180 °C – 345 °C
T95:	$R = 0.01062 \times (T + 210)$	valid range: 185 °C – 355 °C
FBP:	$R = 0.01667 \times (T - 37)$	valid range: 200 °C – 370 °C

where:

E = evaporated temperature within valid range prescribed

T = recovered temperature within valid range prescribed

NOTE 16—See Note 15.

NOTE 17—Precision was not determined above E50 for one sample of aviation gasoline, because its unique boiling profile would give it undue leverage on the precision estimates. Users are cautioned that the actual precisions for aviation gasoline may differ from these estimates.

NOTE 18—The degrees of freedom associated with the reproducibility estimate from this interlaboratory study for NOT4 samples are 27 for IBP and 25 for E10. These do not meet the minimum requirements of Practice D6300. Users should be aware that the two corresponding reproducibility estimates are not as precise as the others.<sup>10</sup>

14.2 *Bias*—Since there is no accepted reference material suitable for determining bias for the procedure in this test method, bias has not been determined.

14.3 *Relative Bias*—The Degree of Agreement between results by Test Method D7344 and Test Method D86 (automated)—The 2015 interlaboratory study (ILS-1058)<sup>8</sup> was not used to determine the relative bias statements. The relative bias statements are from the 2005 interlaboratory study.<sup>9</sup> Results on the same materials produced by Test Method D7344 and Test Method D86 were assessed in accordance with procedures outlined in Practice D6708.<sup>9</sup> The findings were:

### IBP:

#### NOT4

No bias-correction considered in Practice D6708 can further improve agreement between results from Test Method D7344 and Test Method D86 (automated), for sample types and property ranges studied. Sample-specific bias, as defined in Practice D6708, was observed for some samples.

Differences between results from Test Method D7344 and Test Method D86 (automated), for the sample types and property ranges studied, are expected to exceed the following cross method reproducibility ( $R_{x,y}$ ), as defined in Practice D6708, about 5 % of the time.

Group NOT4: Refer to Annex A3.

<sup>10</sup> Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1793. Contact ASTM Customer Service at service@astm.org.

<sup>9</sup> Supporting data (the results of the 2005 Interlaboratory Cooperative Test Program) have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1621.

*GRP4*

The degree of agreement between results from Test Method D7344 and Test Method **D86** (automated) can be further improved by applying the bias-correction outlined in [Eq 10](#). Sample-specific bias, as defined in Practice **D6708**, was observed for some samples after applying the bias-correction.

$$\text{Bias – corrected } X = \text{predicted } Y = X - 12.4 \text{ } ^\circ\text{C} \quad (10)$$

where:

X = result obtained by Test Method D7344 (this test method), and *bias-corrected* X = predicted Y = result that would have been obtained by Test Method **D86** (automated) on the same sample.

Differences between bias-corrected results from [Eq 10](#) and Test Method **D86**, for the sample types and property ranges studied, are expected to exceed the following cross method reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time.

Group GRP4: Refer to [Annex A3](#).

**T10:**

*NOT4*

The degree of agreement between results from Test Method D7344 and Test Method **D86** (automated) can be further improved by applying the bias-correction outlined in [Eq 11](#). Sample-specific bias, as defined in Practice **D6708**, was observed for some samples after applying the bias-correction.

$$\text{Bias – corrected } X = \text{predicted } Y = X + 3.65 \text{ } ^\circ\text{C} \quad (11)$$

where:

X = result obtained by Test Method D7344 (this test method), and *bias-corrected* X = predicted Y = result that would have been obtained by Test Method **D86** (automated) on the same sample.

Differences between bias-corrected results from [Eq 11](#) and Test Method **D86**, for the sample types and property ranges studied, are expected to exceed the following cross method reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time.

Group NOT4: Refer to [Annex A3](#).

*GRP4*

The degree of agreement between results from Test Method D7344 and Test Method **D86** (automated) can be further improved by applying the bias-correction outlined in [Eq 12](#). Sample-specific bias, as defined in Practice **D6708**, was observed for some samples after applying the bias-correction.

$$\text{Bias – corrected } X = \text{predicted } Y = 0.97 X + 3.97 \text{ } ^\circ\text{C} \quad (12)$$

where:

X = result obtained by Test Method D7344 (this test method), and *bias-corrected* X = predicted Y = result that would have been obtained by Test Method **D86** (automated) on the same sample.

Differences between bias-corrected results from [Eq 12](#) and Test Method **D86**, for the sample types and property ranges studied, are expected to exceed the following cross method reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time.

Group GRP4: Refer to [Annex A3](#).

**T50:**

*NOT4*

No bias-correction considered in Practice **D6708** can further improve agreement between results from Test Method D7344 and Test Method **D86** (automated), for sample types and property ranges studied. Sample-specific bias, as defined in Practice **D6708**, was observed for some samples.

Differences between results from Test Method D7344 and Test Method **D86** (automated), for the sample types and property ranges studied, are expected to exceed the following cross method reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time.

Group NOT4: Refer to [Annex A3](#).

*GRP4*

The degree of agreement between results from Test Method D7344 and Test Method **D86** (automated) can be further improved by applying the bias-correction outlined in [Eq 13](#). Sample-specific bias, as defined in Practice **D6708**, was observed for some samples after applying the bias-correction.

$$\text{Bias – corrected } X = \text{predicted } Y = 0.98 X + 3.21 \text{ } ^\circ\text{C} \quad (13)$$

where:

X = result obtained by Test Method D7344 (this test method), and *bias-corrected* X = predicted Y = result that would have been obtained by Test Method **D86** (automated) on the same sample.

Differences between bias-corrected results from [Eq 13](#) and Test Method **D86** (automated), for the sample types and property ranges studied, are expected to exceed the following cross method reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time.

Group GRP4: Refer to [Annex A3](#).

**T90:**

*NOT4*

No bias-correction considered in Practice **D6708** can further improve agreement between results from Test Method D7344 and Test Method **D86** (automated), for sample types and property ranges studied. Sample-specific bias, as defined in Practice **D6708**, was observed for some samples.

Differences between results from Test Method D7344 and Test Method **D86** (automated), for the sample types and property ranges studied, are expected to exceed the following cross method reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time.

Group NOT4: Refer to [Annex A3](#).

*GRP4*

No bias-correction considered in Practice **D6708** can further improve agreement between results from Test Method D7344 and Test Method **D86** (automated), for sample types and property ranges studied. Sample-specific bias, as defined in Practice **D6708**, was observed for some samples.

Differences between results from Test Method D7344 and Test Method **D86** (automated), for the sample types and property ranges studied, are expected to exceed the following cross method reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time.

Group GRP4: Refer to [Annex A3](#).

**FBP:**

*NOT4*

No bias-correction considered in Practice **D6708** can further improve agreement between results from Test Method D7344 and Test Method **D86** (automated), for sample types and property ranges studied. Sample-specific bias, as defined in Practice **D6708**, was observed for some samples.

Differences between results from Test Method D7344 and Test Method **D86** (automated), for the sample types and property ranges studied, are expected to exceed the following cross method reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time.

Group NOT4: Refer to [Annex A3](#).



**GRP4**

The degree of agreement between results from Test Method D7344 and Test Method D86 (automated) can be further improved by applying the bias-correction outlined in Eq 14. Sample-specific bias, as defined in Practice D6708, was observed for some samples after applying the bias-correction.

$$\text{Bias - corrected } X = \text{predicted } Y = X - 3.81 \text{ } ^\circ\text{C} \quad (14)$$

where:

X = result obtained by Test Method D7344 (this test method), and  
*bias-corrected* X = predicted Y = result that would have been obtained by Test Method D86 (automated) on the same sample.

Differences between bias-corrected results from Eq 14 and Test Method D86 (automated), for the sample types and property ranges studied, are expected to exceed the following cross method reproducibility ( $R_{XY}$ ), as defined in Practice D6708, about 5 % of the time.

Group GRP4: Refer to Annex A3.

NOTE 19—In some cases, stated precision for 10 % ethanol-gasoline blends at the 50 % evaporation point may not be achieved.

NOTE 20—The 2015 interlaboratory study (ILS-1058)<sup>8</sup> was not used to determine relative bias; users are cautioned that the actual relative bias may differ from these estimates.

14.4 The precision statements were derived according to Practice D6300 from a 2015 interlaboratory cooperative test program.<sup>8</sup> Eleven laboratories have participated and analyzed 29 samples comprising specification grade gasolines (some containing up to 10 % ethanol or other oxygenates), specification grade diesel (with a B7, B20, and B30 biodiesel), specification grade heating oil, aviation turbine fuels, aviation gasolines, marine fuels, mineral spirits, and toluene. The temperature range covered was 21 °C to 368 °C. The sample set also included the pure petrochemicals Hexane, Cyclohexane, Nonane, Decane, Dodecane, and Tetradecane (temperature range: 65 °C to 265 °C). Information on the type of samples and their average boiling points are in the research report.<sup>8</sup>

14.5 *Precision (Biodiesel B100)*<sup>10</sup>—The precision of this test method when applied to biodiesel (FAME) as determined by the statistical examination of the interlaboratory test results is as follows:

**TABLE 4 Precision (Biodiesel B100) (°C)**

Recovery	Repeatability (r)	Reproducibility (R)	Range (°C)
IBP	0.66 (X–50)	0.66 (X–50)	155 – 245
5 %	29.4	36.9	290 – 320
10 %	19.5	26.5	305 – 335
20 %	12.8	19.4	325 – 350
30 %	5.35	7.99	330 – 360
40 % to 95 %	0.0736 (X–315)	0.1 (X–315)	335 – 370
FBP	0.395 (X–345)	0.825 (X–345)	345 – 370

14.5.1 *Repeatability*—The difference between successive test results, obtained by the same operator using the same apparatus under constant operating conditions on identical test material, would in the long run, in the normal and correct operation of this test method, exceed the values in Table 4 only in one case in twenty.

14.5.2 *Reproducibility*—The difference between two single and independent test results, obtained by different operators working in different laboratories on identical test material,

would in the long run, in normal and correct operation of this test method, exceed the values in Table 4 only in one case in twenty.

NOTE 21—The degrees of freedom associated with the reproducibility estimate from this interlaboratory study for D7344 biodiesel (B100) precision for FBP are 24. Since the minimum requirement of 30 (in accordance with Practice D6300) is not met, users are cautioned that the actual reproducibility may be significantly different than these estimates.

14.5.3 The precision statements for biodiesel (B100) were derived from a 2012 interlaboratory cooperative test program.<sup>10</sup> The precision and relative bias are applicable only to the biodiesel sample types listed in the research report. A total of nine participating laboratories using various Test Method D1160 automated, automatic, or manual apparatus; and eleven participating laboratories using D7344 apparatus; analyzed blind replicates of eleven sample sets comprised of eight specification grade biodiesel (B100) (derived from soy, canola, tallow and yellow grease), two mixed blends of biodiesel (B100) (soy and tallow), and a mustard oil. The distillation range was from 274 °C to 400 °C. Information on the type of samples and their average boiling points are in the research report.<sup>10</sup>

14.6 *Bias (Biodiesel B100)*—Since there is no accepted reference material suitable for determining the bias for the procedure in this test method, bias has not been determined.

14.7 *Relative Bias (Biodiesel B100)*—The degree of agreement between results by Test Method D7344 and Test Method D1160; results on the same materials produced by Test Method D7344 and Test Method D1160 have been assessed in accordance with procedures outlined in Practice D6708. The findings are:

14.7.1 *For IBP*—Test material property differences cannot be reliably distinguished by either Test Method D7344, or Test Method D1160, or both.

14.7.2 *For T5 to T30 %*—Test material property differences cannot be reliably distinguished by either Test Method D7344, or Test Method D1160, or both.

14.7.3 *For T40 %*—There is an insufficient degree of agreement (correlation) between Test Method D7344 and Test Method D1160.

14.7.4 *For T50 %*—The degree of agreement between results from Test Method D7344 and Test Method D1160, can be further improved by applying correction equation (Eq 15) as listed below. No sample-specific bias, as defined in Practice D6708, was observed after the bias-correction for the materials and property range studied.

$$\text{Bias-corrected } X = \text{predicted } Y = 0.67(X - 346) + 348.8 \quad (15)$$

where:

X = result in °C obtained by Test Method D7344 (this test method), and

*bias-corrected* X = predicted Y = result that would have been obtained by Test Method D1160 on the same sample.

14.7.4.1 Differences between bias-corrected results from Test Method D7344 and Test Method D1160, for the sample types and property ranges studied, are expected to exceed the

following between methods reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time. Between Methods  $R = (0.5 R_X^2 + 0.5 R_Y^2)^{0.5} = (0.00501 (X-315)^2 + 15.1)^{0.5}$

14.7.5 *For T60 %*—The degree of agreement between results from Test Method D7344 and Test Method **D1160**, can be further improved by applying correction equation (Eq 16) as listed below. No sample-specific bias, as defined in Practice **D6708**, was observed after the bias-correction for the materials and property range studied.

$$\text{Bias-corrected } X = \text{predicted } Y = 0.611(X - 346.9) + 349.8 \quad (16)$$

where:

$X$  = result in °C obtained by Test Method D7344 (this test method), and  
*bias-corrected*  $X$  = predicted  $Y$  = result that would have been obtained by Test Method **D1160** on the same sample.

14.7.5.1 Differences between bias-corrected results from Test Method D7344 and Test Method **D1160**, for the sample types and property ranges studied, are expected to exceed the following between methods reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time. Between Methods  $R = (0.5 R_X^2 + 0.5 R_Y^2)^{0.5} = (0.00501 (X-315)^2 + 10.8)^{0.5}$

14.7.6 *For T70 %*—The degree of agreement between results from Test Method D7344 and Test Method **D1160**, can be further improved by applying correction equation (Eq 17) as listed below. No sample-specific bias, as defined in Practice **D6708**, was observed after the bias-correction for the materials and property range studied.

$$\text{bias-corrected } X = \text{predicted } Y = 0.455(X - 347.9) + 350.6 \quad (17)$$

where:

$X$  = result in °C obtained by Test Method D7344 (this test method), and  
*bias-corrected*  $X$  = predicted  $Y$  = result that would have been obtained by Test Method **D1160** on the same sample.

14.7.6.1 Differences between bias-corrected results from Test Method D7344 and Test Method **D1160**, for the sample types and property ranges studied, are expected to exceed the following between methods reproducibility ( $R_{XY}$ ), as defined in Practice **D6708**, about 5 % of the time. Between Methods  $R = (0.5 R_X^2 + 0.5 R_Y^2)^{0.5} = (0.00501 (X-315)^2 + 10.8)^{0.5}$

14.7.7 *For T80 %*—Test material property differences cannot be reliably distinguished by either Test Method D7344, or Test Method **D1160**, or both.

14.7.8 *For T90 %*—Test material property differences cannot be reliably distinguished by either Test Method D7344, or Test Method **D1160**, or both.

14.7.9 *For T95 %*—There is an insufficient degree of agreement (correlation) between Test Method D7344 and Test Method **D1160**.

14.7.10 *For FBP*—Test material property differences cannot be reliably distinguished by either Test Method D7344, or Test Method **D1160**, or both.

## 15. Keywords

15.1 atmospheric distillation; distillation; laboratory distillation; mini method; petroleum products

## ANNEXES

### (Mandatory Information)

#### A1. DESCRIPTION OF APPARATUS

A1.1 *Specimen Cup*—The specimen cup shall be made of metal (copper or aluminum have been found suitable), constructed to the dimensions and tolerances shown in Fig. A1.1.

A1.2 *Distillation, Condenser and Receiver System*—The design of the complete system is shown in Fig. A1.2.

A1.2.1 The electric heater (1) shall be of low heat retention. The power to the electric heater shall be adjustable from 0 to a minimum of 105 W.

A1.2.2 The heater is integrated in a motor driven lift (2). This lift presses the specimen cup against the bottom of the distillation column (3). The cup and the column thus form a distillation flask.


A1.2.3 The distillation column (3) shall be made of stainless steel. The thermocouple vapor temperature sensor (4) shall protrude into the distillation column from above so that the

bottom of the sensor is at the same height as the bottom of the tube connecting to the condenser.

A1.2.4 The condenser (5) shall be made of aluminum or brass. The condenser is open at the top so that the complete system is always at atmospheric pressure. The temperature of the condenser shall be controlled by a thermoelectric element and shall be adjustable from 5 °C to 60 °C (41 °F to 140 °F).


A1.2.5 The receiver system is integrated in the condenser so that condenser and receiver are always at the same temperature. The receiver consists of a meniscus detection system (6) and a variable volume receiver chamber (7) formed by a cylindrical bore hole and a piston driven by a stepper motor (8).

A1.3 *Distillation Column*—The design of the distillation column is shown in Fig. A1.3.

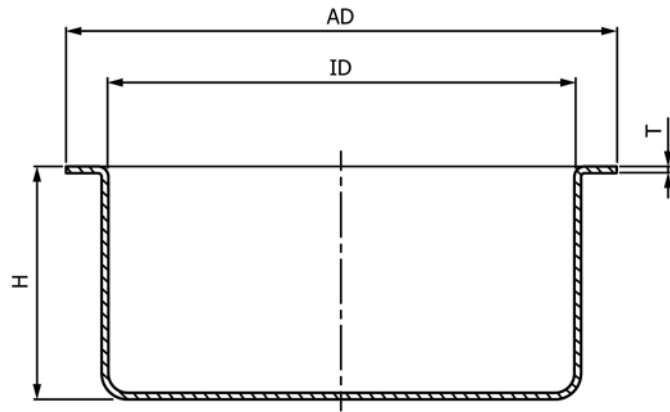


AD =  $33 \pm 0.5$  mm  
ID =  $28.1 \pm 0.05$  mm  
H =  $13.5 \pm 0.1$  mm  
T =  $0.3 \pm 0.03$  mm

FIG. A1.1 Sample Cup

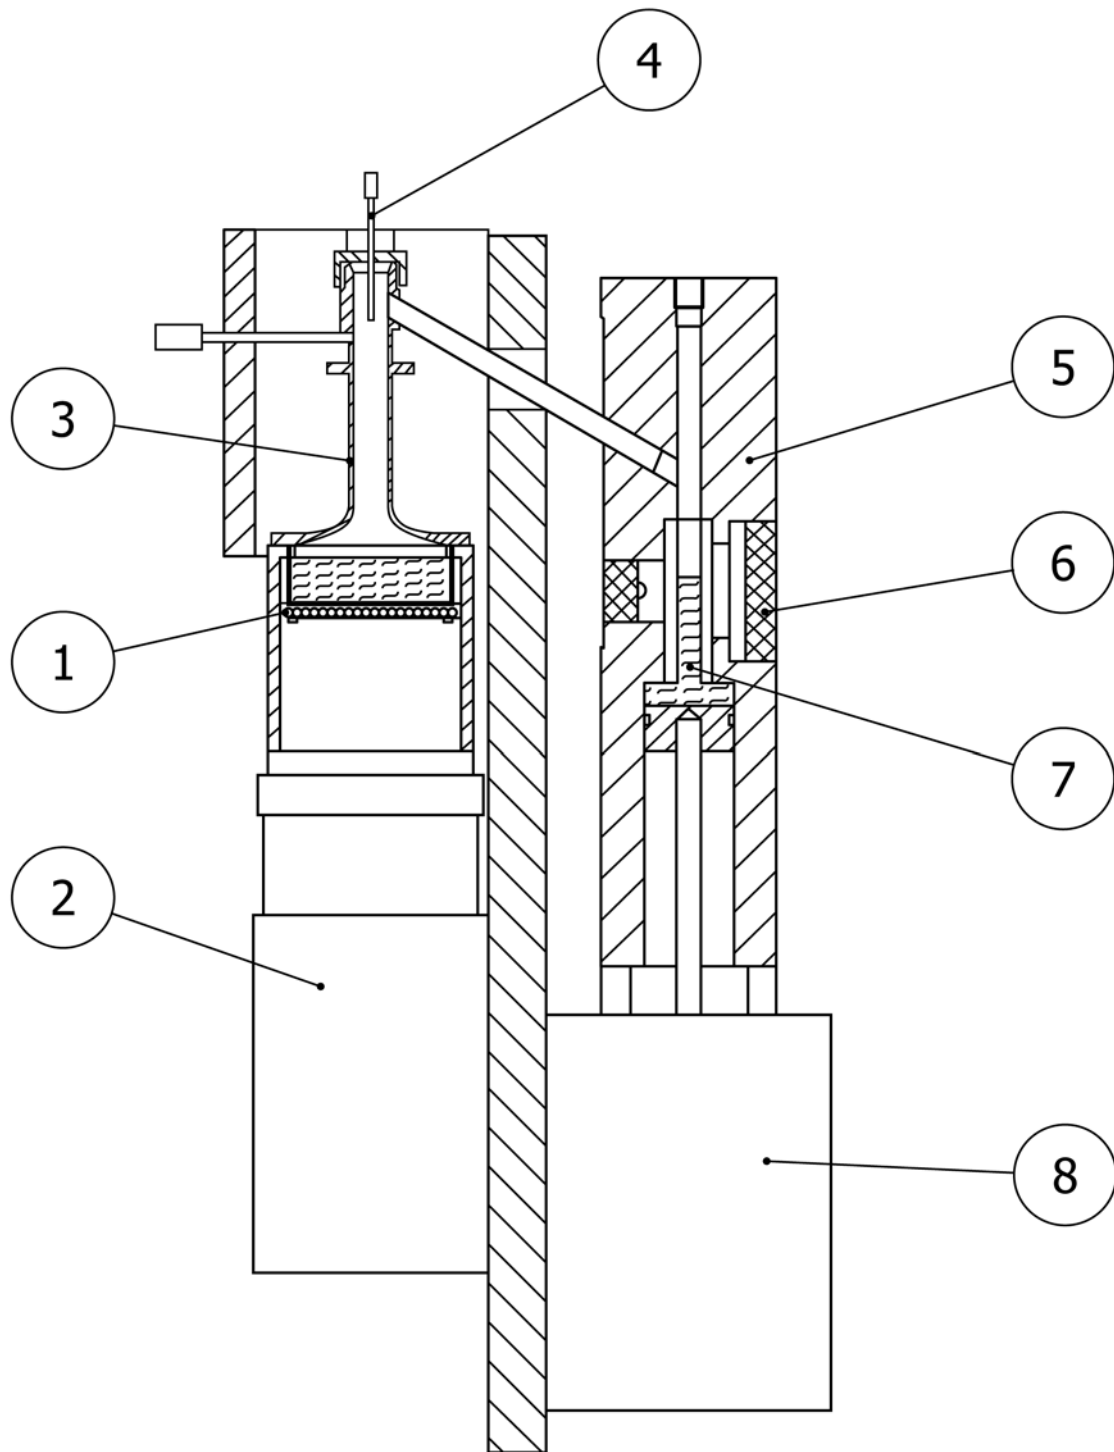

- 1 Electric heater
- 2 Motor driven sample cup lift
- 3 Distillation column
- 4 Vapor temperature sensor
- 5 Condenser
- 6 Meniscus detection system
- 7 Receiver chamber
- 8 Stepper motor

FIG. A1.2 Schematic of Mini Distillation

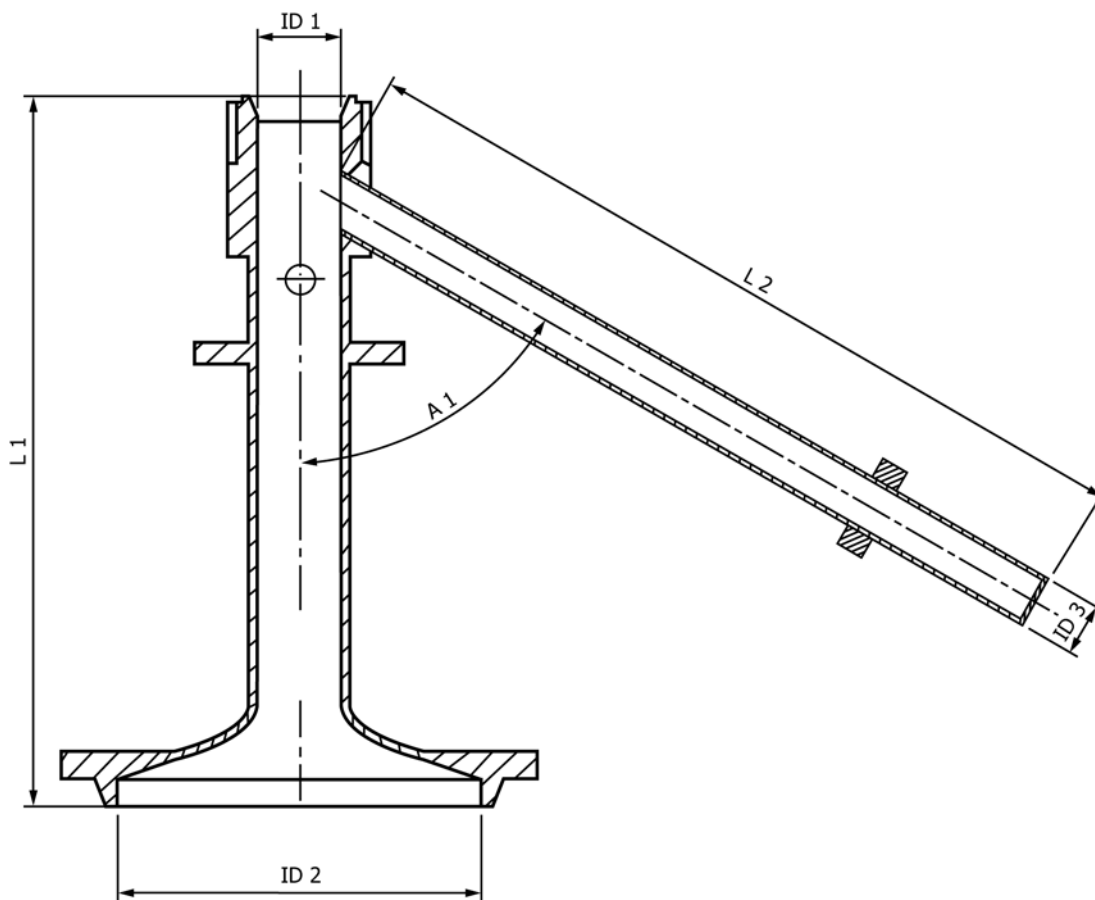

ID 1: 6 mm ± 0.05 mm  
 ID 2: 26 mm  
 ID 3: 3.4 mm  
 L 1: 50.5 mm  
 L 2: 58 mm  
 A 1: 60°

FIG. A1.3 Distillation Column

**A2. PRECISION TABLES FOR REPEATABILITY AND REPRODUCIBILITY**  
 (r = repeatability; R = Reproducibility)

IBP Temp (°C)	IBP_GRP0		IBP Temp (°C)	IBP_GRP0	
	r_Mini	R_Mini		r_Mini	R_Mini
65	0.17	0.19	140	0.00	1.94
70	0.21	0.24	145	1.91	2.15
75	0.26	0.30	150	2.11	2.38
80	0.32	0.36	155	2.33	2.63
85	0.38	0.43	160	2.57	2.89
90	0.46	0.51	165	2.81	3.17
95	0.54	0.60	170	3.08	3.46
100	0.63	0.71	175	3.36	3.78
105	0.73	0.82	180	3.65	4.11
110	0.83	0.94	185	3.97	4.47
115	0.95	1.07	190	4.30	4.84
120	1.08	1.22	195	4.65	5.23
125	1.22	1.38	200	5.01	5.64
130	1.38	1.55	205	5.40	6.08
135	1.54	1.74	210	5.80	6.53
			215	6.23	7.01

IBP Temp (°C)	IBP_NOT4	
	r_Mini	R_Mini
20	2.46	5.27
25	2.46	5.27
30	2.46	5.27
35	2.46	5.27
40	2.46	5.27
45	2.46	5.27
50	2.46	5.27
55	2.46	5.27
60	2.46	5.27

IBP Temp (°C)	IBP_GRP4	
	r_Mini	R_Mini
150	3.57	5.32
155	3.57	5.32
160	3.57	5.32
165	3.57	5.32
170	3.57	5.32
175	3.57	5.32
180	3.57	5.32
185	3.57	5.32
190	3.57	5.32

Recovered 10 % Temp (°C)	T10_GRP0	
	r_Mini	R_Mini
65	0.22	0.24
70	0.25	0.28
75	0.28	0.31
80	0.31	0.34
85	0.34	0.38
90	0.37	0.42
95	0.41	0.46
100	0.44	0.50
105	0.48	0.54
110	0.52	0.58
115	0.56	0.62
120	0.60	0.67
125	0.64	0.72
130	0.69	0.76
135	0.73	0.81
140	0.77	0.86
145	0.82	0.91
150	0.87	0.97
155	0.92	1.02
160	0.97	1.07
165	1.02	1.13
170	1.07	1.19
175	1.12	1.25
180	1.17	1.30
185	1.23	1.36
190	1.28	1.43
195	1.34	1.49
200	1.39	1.55
205	1.45	1.62
210	1.51	1.68
215	1.57	1.75
220	1.63	1.82
225	1.69	1.88
230	1.76	1.95
235	1.82	2.02
240	1.88	2.10

Evaporated 10 % Temp (°C)	E10_NOT4	
	r_Mini	R_Mini
40	1.97	4.68
45	1.97	4.68
50	1.97	4.68
55	1.97	4.68
60	1.97	4.68
65	1.97	4.68

Recovered 10 % Temp (°C)	T10_GRP4	
	r_Mini	R_Mini
160	1.20	1.60
165	1.43	1.92
170	1.67	2.24

Recovered 10 % Temp (°C)	T10_GRP4	
	r_Mini	R_Mini
175	1.91	2.56
180	2.15	2.88
185	2.39	3.20
190	2.63	3.52
195	2.87	3.84
200	3.11	4.16
205	3.35	4.48
210	3.59	4.81
215	3.83	5.13
220	4.06	5.45

Recovered 50 % Temp (°C)	T50_GRP0	
	r_Mini	R_Mini
65	0.14	0.26
70	0.15	0.28
75	0.16	0.30
80	0.16	0.31
85	0.17	0.33
90	0.18	0.34
95	0.19	0.36
100	0.20	0.37
105	0.20	0.39
110	0.21	0.40
115	0.22	0.42
120	0.23	0.43
125	0.24	0.45
130	0.24	0.46
135	0.25	0.48
140	0.26	0.49
145	0.27	0.51
150	0.27	0.52
155	0.28	0.53
160	0.29	0.55
165	0.30	0.56
170	0.30	0.57
175	0.31	0.59
180	0.32	0.60
185	0.32	0.62
190	0.33	0.63
195	0.34	0.64
200	0.35	0.66
205	0.35	0.67
210	0.36	0.68
215	0.37	0.69
220	0.37	0.71
225	0.38	0.72
230	0.39	0.73
235	0.39	0.75
240	0.40	0.76
245	0.41	0.77
250	0.41	0.79
255	0.42	0.80

Evaporated 50 % Temp (°C)	E50_NOT4	
	r_Mini	R_Mini
75	0.73	1.13
80	0.88	1.36
85	1.03	1.59
90	1.18	1.81
95	1.32	2.04
100	1.47	2.27
105	1.62	2.49

Recovered 50 % Temp (°C)	T50_GRP4	
	r_Mini	R_Mini
165	0.54	0.69
170	0.64	0.82
175	0.73	0.94
180	0.83	1.06
185	0.92	1.19
190	1.02	1.31
195	1.12	1.44
200	1.21	1.56
205	1.31	1.68

Recovered 50 %		T50_GRP4	
Temp (°C)	r_Mini	R_Mini	
210	1.41	1.81	
215	1.50	1.93	
220	1.60	2.05	
225	1.69	2.18	
230	1.79	2.30	
235	1.89	2.43	
240	1.98	2.55	
245	2.08	2.67	
250	2.18	2.80	
255	2.27	2.92	
260	2.37	3.04	
265	2.47	3.17	
270	2.56	3.29	
275	2.66	3.42	
280	2.75	3.54	
285	2.85	3.66	

Recovered 90 %		T90_GRP0	
Temp (°C)	r_Mini	R_Mini	
65	0.27	0.66	
70	0.26	0.65	
75	0.26	0.64	
80	0.25	0.64	
85	0.25	0.63	
90	0.25	0.62	
95	0.25	0.61	
100	0.24	0.61	
105	0.24	0.60	
110	0.24	0.59	
115	0.24	0.59	
120	0.23	0.58	
125	0.23	0.58	
130	0.23	0.57	
135	0.23	0.57	
140	0.23	0.56	
145	0.22	0.56	
150	0.22	0.56	
155	0.22	0.55	
160	0.22	0.55	
165	0.22	0.54	
170	0.22	0.54	
175	0.22	0.54	
180	0.21	0.53	
185	0.21	0.53	
190	0.21	0.53	
195	0.21	0.53	
200	0.21	0.52	
205	0.21	0.52	
210	0.21	0.52	
215	0.21	0.51	
220	0.21	0.51	
225	0.20	0.51	
230	0.20	0.51	
235	0.20	0.50	
240	0.20	0.50	
245	0.20	0.50	
250	0.20	0.50	
255	0.20	0.50	

Evaporated 90 %		E90_NOT4	
Temp (°C)	r_Mini	R_Mini	
145	2.45	3.53	
150	2.45	3.53	
155	2.45	3.53	
160	2.45	3.53	
165	2.45	3.53	

Recovered 90 %		T90_GRP4	
Temp (°C)	r_Mini	R_Mini	
180	1.59	2.51	
185	1.64	2.59	
190	1.68	2.66	
195	1.73	2.74	
200	1.78	2.82	

Recovered 90 %		T90_GRP4	
Temp (°C)	r_Mini	R_Mini	
205	1.83	2.90	
210	1.88	2.98	
215	1.93	3.06	
220	1.98	3.13	
225	2.03	3.21	
230	2.08	3.29	
235	2.13	3.37	
240	2.18	3.45	
245	2.23	3.53	
250	2.28	3.60	
255	2.33	3.68	
260	2.38	3.76	
265	2.43	3.84	
270	2.48	3.92	
275	2.53	4.00	
280	2.58	4.07	
285	2.63	4.15	
290	2.68	4.23	
295	2.73	4.31	
300	2.78	4.39	
305	2.82	4.47	
310	2.87	4.54	
315	2.92	4.62	
320	2.97	4.70	
325	3.02	4.78	
330	3.07	4.86	
335	3.12	4.94	
340	3.17	5.01	
345	3.22	5.09	

Recovered 95 %		T95_GRP4	
Temp (°C)	r_Mini	R_Mini	
185	2.55	4.19	
190	2.58	4.25	
195	2.62	4.30	
200	2.65	4.35	
205	2.68	4.41	
210	2.71	4.46	
215	2.75	4.51	
220	2.78	4.57	
225	2.81	4.62	
230	2.84	4.67	
235	2.88	4.73	
240	2.91	4.78	
245	2.94	4.83	
250	2.97	4.89	
255	3.00	4.94	
260	3.04	4.99	
265	3.07	5.04	
270	3.10	5.10	
275	3.13	5.15	
280	3.17	5.20	
285	3.20	5.26	
290	3.23	5.31	
295	3.26	5.36	
300	3.30	5.42	
305	3.33	5.47	
310	3.36	5.52	
315	3.39	5.58	
320	3.42	5.63	
325	3.46	5.68	
330	3.49	5.73	
335	3.52	5.79	
340	3.55	5.84	
345	3.59	5.89	
350	3.62	5.95	
355	3.65	6.00	

FBP		FBP_GRP0	
Temp (°C)	r_Mini	R_Mini	
65	2.13	3.84	
70	2.30	4.13	
75	2.46	4.42	
80	2.62	4.71	

FBP Temp (°C)	FBP_GRP0	
	r_Mini	R_Mini
85	2.78	5.00
90	2.94	5.29
95	3.10	5.58
100	3.26	5.87
105	3.42	6.15
110	3.58	6.44
115	3.74	6.73
120	3.90	7.02
125	4.05	7.30
130	4.21	7.59
135	4.37	7.88
140	4.53	8.16
145	4.69	8.45
150	4.85	8.73
155	5.01	9.02
160	5.17	9.30
165	5.33	9.59
170	5.48	9.88
175	5.64	10.16
180	5.80	10.45
185	5.96	10.73
190	6.12	11.01
195	6.27	11.30
200	6.43	11.58
205	6.59	11.87
210	6.75	12.15
215	6.90	12.44
220	7.06	12.72
225	7.22	13.00
230	7.38	13.29
235	7.53	13.57
240	7.69	13.85
245	7.85	14.14
250	8.01	14.42
255	8.16	14.70
260	8.32	14.99
265	8.48	15.27

FBP Temp (°C)	FBP_GRP4	
	r_Mini	R_Mini
200	1.68	2.72
205	1.74	2.80
210	1.79	2.88
215	1.84	2.97
220	1.89	3.05
225	1.94	3.13
230	1.99	3.22
235	2.05	3.30
240	2.10	3.38
245	2.15	3.47
250	2.20	3.55
255	2.25	3.63
260	2.30	3.72
265	2.36	3.80
270	2.41	3.88
275	2.46	3.97
280	2.51	4.05
285	2.56	4.13
290	2.61	4.22
295	2.67	4.30
300	2.72	4.38
305	2.77	4.47
310	2.82	4.55
315	2.87	4.63
320	2.92	4.72
325	2.98	4.80
330	3.03	4.88
335	3.08	4.97
340	3.13	5.05
345	3.18	5.13
350	3.23	5.22
355	3.28	5.30
360	3.34	5.38
365	3.39	5.47
370	3.44	5.55

FBP Temp (°C)	FBP_NOT4	
	r_Mini	R_Mini
170	3.22	4.82
175	3.22	4.82
180	3.22	4.82
185	3.22	4.82
190	3.22	4.82
195	3.22	4.82
200	3.22	4.82



### A3. BETWEEN METHOD REPRODUCIBILITY

A3.1 2005 precision from RR:D02-1621<sup>9</sup> was used to calculate Between Method Reproducibility found in A3.2.

A3.1.1 The Degree of Agreement between results by Test Method D7344 and Test Method D86 (automated) results on the same materials produced by Test Method D7344 and Test Method D86 were assessed in accordance with procedures outlined in Practice D6708 following the 2005 interlaboratory study.<sup>9</sup> The analysis conducted in the corresponding research program, segregated the samples into two groupings as follows.

A3.1.1.1 NOT4 is the grouping of samples usually covered under Test Method D86 Groups 1, 2, and 3, typically gasoline.

A3.1.1.2 GRP4 is the grouping of samples usually covered under Test Method D86 Group 4, typically No. 1 and No. 2 diesel fuels as described in Specification D975 (diesel), aviation turbine fuel, and marine distillate fuels.

A3.1.1.3 The 2015 interlaboratory study<sup>8</sup> was not used to determine relative bias; users are cautioned that the actual relative bias may differ from these estimates.

**TABLE A3.1 2005 Precision from RR:D02-1621<sup>9</sup>**

Group NOT4:		
IBP:	R = 10.0	valid range: 20 – 80 °C
E10:	R = 7.74	valid range: 30 – 90 °C
E50:	R = 4.36	valid range: 60 – 140 °C
E90:	$R = E^{2.1716} \times 0.000125$	valid range: 110 – 245 °C
FBP:	$R = E \times 0.0736$	valid range: 140 – 260 °C
Group GRP4:		
IBP:	R = 18.6	valid range: 145 – 195 °C
T10:	$R = (T + 139.9) \times 0.016$	valid range: 160 – 265 °C
T50:	$R = T \times 0.014$	valid range: 170 – 295 °C
T90:	$R = T^{2.6197} \times 0.0000145$	valid range: 180 – 340 °C
T95:	R = 6.70	valid range: 260 – 338 °C
FBP:	R = 8.95	valid range: 195 – 365 °C

where:  
E = evaporated temperature within valid range prescribed  
T = recovered temperature within valid range prescribed

#### A3.2 Calculated Between Method Reproducibility:

IBP_NOT4 Temp (°C)	R_xy
25	9.61
30	9.70
35	9.80
40	9.90
45	10.01
50	10.12
55	10.24
60	10.36
65	10.48
70	10.61
75	10.74
80	10.88

IBP_GRP4 Temp (°C)	R_xy
150	16.81
155	16.89
160	16.97
165	17.05
170	17.14
175	17.23
180	17.32
185	17.42
190	17.51
195	17.61
200	17.71
205	17.81
210	17.91
215	18.02
220	18.13
T10_NOT4 Temp (°C)	R_xy
30	6.33
35	6.33
40	6.33
45	6.33
50	6.33
55	6.33
60	6.33
65	6.33
70	6.33
75	6.33
80	6.33
85	6.33
90	6.33
95	6.33
T10_GRP4 Temp (°C)	R_xy
160	4.32
165	4.42
170	4.51
175	4.61
180	4.70
185	4.80
190	4.90
195	4.99
200	5.09
205	5.18
210	5.28
215	5.38
220	5.47
225	5.57
230	5.67
235	5.76
240	5.86
245	5.96
250	6.06
255	6.15
260	6.25
265	6.35

T50_NOT4 Temp (°C)	R_xy
60	4.14
65	4.14
70	4.14
75	4.14
80	4.14
85	4.14
90	4.14
95	4.14
100	4.14
105	4.14
110	4.14
115	4.14
120	4.14

T50_GRP4 Temp (°C)	R_xy
170	2.96
175	2.99
180	3.03
185	3.07
190	3.11
195	3.14
200	3.18
205	3.22
210	3.26
215	3.30
220	3.35
225	3.39
230	3.43
235	3.47
240	3.52
245	3.56
250	3.60
255	3.65
260	3.69
265	3.73
270	3.78
275	3.83
280	3.87
285	3.92
290	3.96

T90_NOT4 Temp (°C)	R_xy
110	4.29
115	4.60
120	4.92
125	5.27
130	5.63
135	6.01
140	6.41
145	6.83
150	7.27
155	7.72
160	8.20
165	8.69
170	9.20
175	9.74
180	10.29
185	10.86
190	11.45
195	12.06
200	12.69
205	13.34
210	14.00

T90_GRP4 Temp (°C)	R_xy
180	3.04
185	3.15
190	3.27
195	3.39
200	3.51

T90_GRP4 Temp (°C)	R_xy
205	3.64
210	3.77
215	3.90
220	4.04
225	4.18
230	4.33
235	4.48
240	4.63
245	4.79
250	4.95
255	5.12
260	5.29
265	5.47
270	5.65
275	5.84
280	6.04
285	6.24
290	6.44
295	6.65
300	6.87
305	7.09
310	7.31
315	7.55
320	7.79
325	8.03
330	8.28
335	8.54
340	8.81

FBP_NOT4 Temp (°C)	R_xy
140	13.72
145	14.09
150	14.46
155	14.84
160	15.21
165	15.59
170	15.97
175	16.36
180	16.74
185	17.13
190	17.52
195	17.91
200	18.30
205	18.69
210	19.09
215	19.48
220	19.88
225	20.28
230	20.68
235	21.08
240	21.48

FBP_GRP4 Temp (°C)	R_xy
190	11.32
195	11.32
200	11.32
205	11.32
210	11.32
215	11.32
220	11.32
225	11.32
230	11.32
235	11.32
240	11.32
245	11.32
250	11.32
255	11.32
260	11.32
265	11.32
270	11.32
275	11.32

FBP_GRP4 Temp (°C)	R <sub>xy</sub>
280	11.32
285	11.32
290	11.32
295	11.32
300	11.32
305	11.32
310	11.32
315	11.32
320	11.32

FBP_GRP4 Temp (°C)	R <sub>xy</sub>
325	11.32
330	11.32
335	11.32
340	11.32
345	11.32
350	11.32
355	11.32
360	11.32

#### A4. PRECISION OF THE VOLUME PERCENT EVAPORATED OR RECOVERED AT A PRESCRIBED TEMPERATURE

A4.1 The precision of the volume % evaporated or recovered at a prescribed temperature for Test Method D7344 were derived according to Practice D6300 from a 2005 interlaboratory program.<sup>9</sup>

A4.1.1 *Precision for Volume % Evaporated for Gasoline:* Consolidated equation for valid range of E70 to E180°C.

$$\text{Mini Dis} = \frac{r}{0.0219(160 - X)} \quad \frac{R}{0.0372(160 - X)}$$

where: X = percent evaporated at the prescribed temperature

A4.1.2 *Precision for Percent Recovered for Diesel (Rxxx):* Equation for valid range of R200 to R300°C.

$$\text{Mini Dis} = \frac{r}{0.01233(200 - X)} \quad \frac{R}{0.01973(200 - X)}$$

where: X = percent recovered at the prescribed temperature

A4.2 *Relative Bias*—Relative bias for both gasoline and diesel samples were examined in relation to D86; the methodology of D6708 was used for these comparisons. The biases were, in general, rather small. Still, they were statistically significant in some cases. It should be noted that D6708 requires ten samples minimum, which is a requirement that is not met for any of these comparisons. Even when the percents evaporated or percents recovered are pooled over the six different temperatures, there are still fewer than ten samples. As a result, we should treat these comparisons as suggestive, rather than definitive.

A4.2.1 *Gasoline Samples*—For Mini Dis, % evaporated, there is a small correctable bias. The preferred equation for predicting D86 results from Mini Dis results is:

$$\%E \text{ by D86} = 1.031 \times \%E \text{ by Mini Dis} - 2.81 \quad (\text{A4.1})$$

where:

%E = volume percent evaporated at the prescribed temperature.

There are also some sample specific biases, which may be treated as random. The between-method reproducibility R<sub>xy</sub> is approximately equivalent to the reproducibility of the Mini Dis method itself.

A4.2.2 *Diesel Samples*—Comparing the Mini Dis method to D86 percent recovered, there is a small correctable bias, plus some small sample-specific biases. The suggested correction is:

$$\%R \text{ by D86} = 1.42 + 0.98 \text{ times } \%R \text{ by Mini Dis} \quad (\text{A4.2})$$

where:

%R = volume percent recovered at the prescribed temperature

The between-method reproducibility R<sub>xy</sub> is approximately equivalent to the reproducibility of the Mini Dis method itself.

A4.2.3 *Diesel Samples T95*—Comparing the mini dis method to D86 for the temperature at 95 % recovered (T95), there appears to be a small correctable bias.

$$\text{D86 T95} = 0.998 \text{ Mini T95} \quad (\text{A4.3})$$

where:

T95 = temperature in degrees Celsius at 95 volume percent recovered.

In addition, some sample-specific biases may be random. The between method reproducibility is about 31 % larger than the root mean square of the two method's reproducibilities.

**SUMMARY OF CHANGES**

Subcommittee D02.08 has identified the location of selected changes to this standard since the last issue (D7344 – 14) that may impact the use of this standard. (Approved May 1, 2017.)

- (1) Revised subsection 1.2. Scope changed to include B30 and pure petrochemical hydrocarbons (Group 0 samples) and clarified furnace and marine fuels.
- (2) Revised subsection 4.1. Changed to include Group 0 samples.
- (3) Revised subsection 4.2. Changed to include Group 0 samples.
- (4) Added new subsection 5.5. Scope to reflect use of Group 0 samples.
- (5) Revised subsection 8, Table 1. Adjusted group characteristics and included Group 0 characteristics.
- (6) Revised subsection 8, Table 2. Added Group 0 characteristics.
- (7) Revised subsection 8.2.2.2. Changed to include Group 0 samples. Additional editorial change.
- (8) Revised subsection 8.3.3. Changed to include Group 0 samples.
- (9) Revised subsection 8.4.1.2. Changed to include Group 0 samples.
- (10) Revised subsection 8.5.3. Changed to include Group 0 samples.
- (11) Revised subsection 11.3. Changed to include Group 0 samples.
- (12) Revised subsection 11, Table 3. Added Group 0 default conditions. Adjusted Group 3 and 4 default conditions.
- (13) Revised subsection 11.9. Changed percentage for final heat adjustment.
- (14) Revised subsection 14.1. Changed precision statement.
- (15) Revised subsection 14.3. Clarified source of between method bias estimates.
- (16) Revised subsection 14.5. Renamed Note 10.
- (17) Revised subsection 14.4. Changed information about ILS sample set. Added caution note for Avgas sample. Added caution note for NOT 4 (gasoline). Added note to clarify use of percent evaporated temperatures for Group 1 and 2 samples and percent recovered temperatures for Group 3 and 4 samples.
- (18) Revised Annex A2. Changed precision calculations.
- (19) Revised Annex A3. Clarified precision used to calculate between method reproducibility.

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; http://www.copyright.com/*