



Standard Practice for Sampling of Liquids in Waste Management Activities Using a Peristaltic Pump¹

This standard is issued under the fixed designation D7353; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This practice covers the use of a peristaltic pump for sampling liquids from multiple depths. It is applicable for a wide range of fluids including: high-viscosity fluids, aggressive and corrosive fluids, high-purity solutions and abrasive fluids. It is especially useful for sampling liquids that require complete isolation from the pump.

1.2 This practice includes the determination of sample depth, pump set up and collecting a sample to be analyzed.

1.3 This practice is not intended to give detailed instructions for running a peristaltic pump or recommend which peristaltic pump to purchase. It instructs the field personnel how to connect the pump and collect a sample.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:²

- D4448 Guide for Sampling Ground-Water Monitoring Wells
- D4687 Guide for General Planning of Waste Sampling
- D4840 Guide for Sample Chain-of-Custody Procedures
- D5681 Terminology for Waste and Waste Management
- D5792 Practice for Generation of Environmental Data Related to Waste Management Activities: Development of Data Quality Objectives
- D5956 Guide for Sampling Strategies for Heterogeneous Wastes
- D6044 Guide for Representative Sampling for Management of Waste and Contaminated Media

¹ This practice is under the jurisdiction of ASTM Committee D34 on Waste Management and is the direct responsibility of Subcommittee D34.01.03 on Sampling Equipment.

Current edition approved Feb. 1, 2013. Published February 2013. Originally approved in 2007. Last previous edition approved in 2007 as D7353 – 07. DOI: 10.1520/D7353-07R13.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For Annual Book of ASTM Standards volume information, refer to the standard's Document Summary page on the ASTM website.

- D6063 Guide for Sampling of Drums and Similar Containers by Field Personnel
- D6232 Guide for Selection of Sampling Equipment for Waste and Contaminated Media Data Collection Activities
- D6250 Practice for Derivation of Decision Point and Confidence Limit for Statistical Testing of Mean Concentration in Waste Management Decisions
- D6311 Guide for Generation of Environmental Data Related to Waste Management Activities: Selection and Optimization of Sampling Design
- D6634 Guide for Selection of Purging and Sampling Devices for Groundwater Monitoring Wells

3. Terminology

3.1 *Definitions:*

3.2 See Terminology D5681.


4. Summary of Practice

4.1 A peristaltic pump is a suction lift pump (see Fig. 1b). A length of polytetrafluoroethylene (PTFE) or other suitable tubing such as Silastic tubing is placed in the liquid at any depth up to 7.6 m (25 ft.) for water or less depending upon the density of the sample being taken. The other end is connected to the piece of flexible tubing which has been threaded around the rotor of the peristaltic pump (see Fig. 1a). A second piece of PTFE or other suitable tubing is connected to the discharge end of the flexible tubing to allow the liquid to be containerized or sampled. One can fill a vacuum-worthy sample container after attaching two tubes to it, one from the top of the pump inlet, and the other from a lower level to the source (see Fig. 1c).

5. Significance and Use

5.1 This practice can be used in sampling drums, tanks, and similar containers and in sampling monitoring and waste wells including small diameter (1 in.) wells. The pump can collect samples from multiple depths. The samples can be high-viscosity fluids, aggressive and corrosive fluids, high-purity solutions and abrasive fluids. The pump can be used to mix samples (see D6063).

5.2 Peristaltic pumps use a vacuum to transport the samples. This vacuum may cause some degassing and loss of volatile

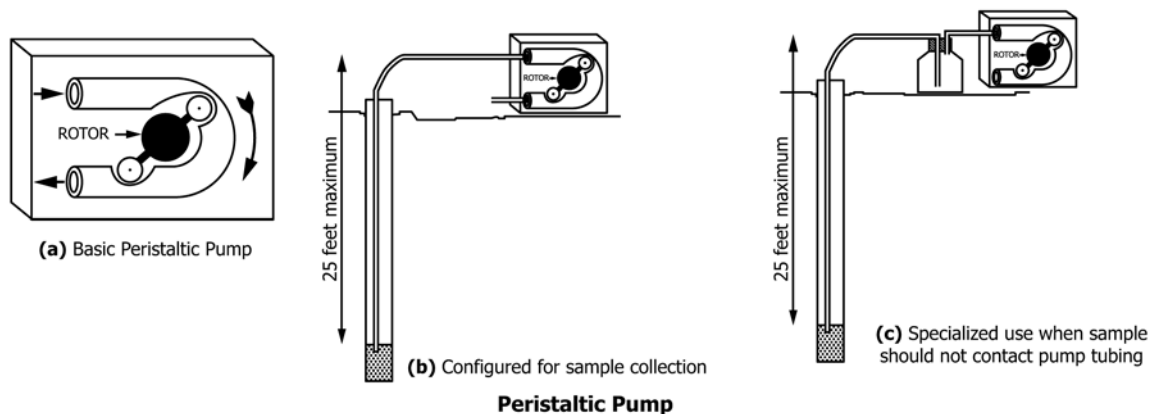

Peristaltic Pump
FIG. 1 Peristaltic Pump

organic compounds (VOCs) from the sample. When precise quantitative data for VOCs and dissolved gases are not required, peristaltic pumps may be used.

5.3 The pump is self-priming, runs dry without damage, and is completely isolated from the pumped fluid. A sample can be taken on the intake or discharge side of the pump.

5.4 Some additional advantages of the peristaltic pump are: decontamination of the pump motor is not necessary and the tubing in the pump is disposable and easy to replace. The pumps can be easily started and stopped and can pump fluids at a wide range of pressures and flow rates.

5.5 The place, quality and quantity, frequency, and time of sampling is dependent upon the decisions that are to be made (see D6250), sampling design (see D6311), the sample, the heterogeneity of the samples (see D5956), how representative the sample is (see D6044), and the parameters to be tested as determined by the data quality objectives (DQOs) (see D5792).

6. Sampling Equipment

6.1 It is recommended that two peristaltic pumps be taken to the site with two pump specific clamps per unit.

NOTE 1—There are many peristaltic pumps on the market from several manufacturers. Consult with the manufacturers to determine the capabilities of each pump for your application.

6.2 Two fully charged batteries (or other applicable batteries or AC/DC converter as required).

6.3 New medical-grade rubber/silicone tubing (Dow-Corning Silastic or equivalent). In corrosive situations, a length of PTFE tubing is used.

6.4 Applicable tubing couplers for discharge and intake as needed.

6.5 Tape measure or water level instrument.

6.6 Waste container.

6.7 Plastic, glass, or other non-reactive containers should be used as specified by the site sampling plan (see Guide D4687).

7. General Sample Collection

7.1 Review the work or sampling plan.

7.2 Check to make sure that the supply of sample containers, labels, ice chest, stop watch or timing device, composite collection container if required, and sampling equipment in place are adequate and correct. There should be sampling forms, or log books, or equivalent for recording field information such as date, time the sample was taken, sampler's name, physical description of the sampling location and any other information which might impact the validity of the sample. The log books, sampling forms, and bottle labels should be signed or initialed.

7.3 Provision should be made for split samples and field quality control samples, such as trip blanks, equipment blanks, and field spikes.

8. Pre-sampling Testing

8.1 Remove the pump cover plate. Slide the tubing through the clamps, position the clamps in their seats, and gently rotate the pump mast to engage the tubing in the pump housing. With the pump mast at the 6:00/12:00 position, the un-pinched tubing should touch the walls of the pump housing (Fig. 1a). A little slack is desirable.

8.2 Tighten each pump clamp and replace the pump cover plate.

8.3 Install the battery and hook up the power lead.

8.4 Insert one end of the tubing into the liquid and the other end into a waste container. The arrow on the pump points to the discharge tube.

8.5 Activate the pump.

8.5.1 Observe the flow of the liquid through the tubing and into the waste container.

8.5.1.1 The system may be checked without liquid by placing a finger over the intake of the sampling system and checking for vacuum.

8.5.2 Vary the pump speeds through the full range.

NOTE 2—It is normal for the pump to be a little sluggish at slow speeds.

8.6 Turn the pump off and switch the tube ends so the discharge tubing end is now the intake tubing end and the discharge tubing end is the intake.

8.6.1 Turn the pump direction switch to reverse the pump mast.

8.7 Repeat 8.5.

8.8 Record the following data in the field log book:

8.8.1 Date and time; pump type, manufacturer, and serial number; battery tracking number, type, and manufacturer; lot number of the tubing; and results of the test.

9. General Peristaltic Sampling Set-ups

9.1 Fig. 1b demonstrates sampling directly from the exit tube after the pump.

9.2 Fig. 1c demonstrates sampling by attaching a sample bottle to the sampling tube from the sample source and a second tube to the intake side of the pump. The sample intake tube reaches almost to the bottom of the sample container while the bottle exit tube reaches just below the bottle cover. The exit tube is placed in the waste container. The pump does not require an air purge between samples since no liquids are in contact with the pump.

9.2.1 If a new sample source is to be sampled, the sampling tube should be replaced or flushed according to the sampling plan.

10. Procedure for Sampling from Wells

10.1 Review the well construction data to determine the screen size, type and depth.

10.2 Prepare the labels, sample bottles, waste containers, and coolers.

10.3 Collect a field blank by pumping de-ionized water or equivalnet through the new tubing. The tubing should have the same lot number as the tubing used to collect the samples.

10.4 Determine the liquid level using a level meter (water level or oil/water interface meter). **Warning**—Peristaltic pumps are not recommended for sampling below 25 ft from the top of the well (see Guide D6634 for sampling devices and Guide D4448 for guidance in sampling ground water monitoring wells).

10.5 *Taking the Samples:*

10.5.1 Lower the intake tubing end to the pre-determined depth to be sampled (Fig. 1b).

10.5.2 Start the pump and purge the system as specified in the sampling plan.

10.5.3 Turn off the pump and lower the exit tube into the sample container.

10.5.4 Turn on the pump.

10.5.5 Fill the labeled sample bottle or bottles to the desired volume, and apply the cap and custody tape if required (see Guide D4840).

10.6 Air-purge the tubing by reversing the pump direction with the exit side of the pump clear of any liquids before sampling the next level. The pump and sampling tube must be clear of any liquid.

10.7 Reverse the pump again and lower the intake tube to the next level if required.

10.8 Repeat the steps in 10.5.

10.9 Record the information in the field log book and preserve the samples.

10.10 If samples are taken on the suction side of the pump according to 9.2 and Fig. 1c, pump reversal and air purging will not be required before moving to a new sample level.

11. Procedure for Sampling From Tanks

11.1 Determine the physical dimensions of each tank to be sampled (height, diameter, length, liquid level or depth, and position/height of pump access point).

11.2 Prepare the intake tubing for installation to the pump by marking depth levels as specified in the sampling plan.

11.3 Determine the distance to the top of the liquid and record the data in the field log book.

11.4 Prepare the sample containers according to the sampling plan. Each bottle should have a label which can be placed on the bottle before or at the time of sampling (see Guide D4840).

11.4.1 Aliquots shall be taken at the pre-designated depths as specified within the sampling plan. The data quality objectives will specify whether the samples shall be handled as discrete or composite samples.

11.4.2 Replicates are prepared by repeating the entire process at each of the specified intervals.

NOTE 3—Vertical tanks and horizontal tanks may need to be sampled differently if volumes at a given level need to be considered. In horizontal cylindrical tanks evenly-spaced depth intervals do not correspond with equal volumes. If a volume to depth relationship is to be maintained, more sample volume needs to be collected in the middle than at the top or bottom of the column to account for extra volume in the middle.

NOTE 4—Special consideration shall be given in the sampling plan procedures to the top and bottom of the tank to ensure that light non-aqueous phase liquid (LNAPL) or dense non-aqueous phase liquids (DNAPL) are not missed in the sampling.

11.5 Lower the calibrated intake tube into the tank to the desired depth and the exit tube into a waste collection container.

11.6 Start the pump and purge the system as specified in the sampling plan before placing the exit tubing into the sample bottle.

11.7 Fill the pre-labeled sample bottle or sample bottles to the desired level. Turn off the pump.

11.8 Cap the bottle and label as required and put on the sample custody seal if required.

11.9 Record the time and other required information on the label (see Guide D4840) and in the field log book.

11.10 Repeat the process until the desired amount of sample has been taken at the required level.

11.11 Take the exit tube out of the sample bottle and air-purge the pump by direction reversal. Once there is no liquid in the system, lower the intake tube to the next level to be sampled. Reverse the pump and repeat 11.6 to 11.9.

11.12 Repeat the process at each level to be sampled.

12. Procedure for Sampling from Drums

12.1 Prepare the pump as outlined in Sections 8 and 9.

12.2 Place the end of the inlet tubing in the drum at a depth from which the sample will be extracted.

12.3 Place the exit end tubing within the drum.

12.4 Turn on the pump and allow at least two volumes of material to flow through the system. If drum mixing using the pump is required, extend the time to meet the requirements of the sampling plan.

12.5 Once the sample is adequately mixed, turn off the pump and place the end of the out let tubing into the appropriate sample container.

12.6 Turn on the pump and fill the labeled sample bottle or bottles to the desired volume, and apply the cap and custody tape if required.

13. Procedure for Sampling Ponds and Lagoons

13.1 While there are many techniques available for sampling ponds or lagoons, the peristaltic pump may be useful

when the sampling requires an average of several aliquots since the pump can be timed to turn on or off at specified intervals (see Guide **D6232**).

13.1.1 Ponds and lagoons can be sampled with a peristaltic pump by the use of a boat.

13.1.2 Ponds and lagoons can be sampled by dropping the intake tube into the liquid backed up behind the weir or overflow dam.

13.1.3 The intake tube can be suspended at the end of a long pole and allowed to be dipped into the pond or lagoon.

13.2 The basic sampling procedure is covered in Sections **8**, **9**, and **10.5**.

14. Keywords

14.1 peristaltic; pump; sampling; waste streams

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the ASTM website (www.astm.org/COPYRIGHT/).