



# Standard Test Method for Condition Monitoring of Phosphate Antiwear Additives in In-Service Petroleum and Hydrocarbon Based Lubricants by Trend Analysis Using Fourier Transform Infrared (FT-IR) Spectrometry<sup>1</sup>

This standard is issued under the fixed designation D7412; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This test method covers monitoring phosphate antiwear additives in in-service petroleum and hydrocarbon based lubricants such as various types of engine oils, hydraulic oils, and other lubricants that are formulated for protection against wear. Typical phosphate antiwear additives include zinc dialkyl-dithiophosphates, trialkyl phosphates and triaryl phosphates.

1.2 This test method uses Fourier Transform Infrared (FT-IR) spectrometry for monitoring of phosphate antiwear additive depletion in in-service petroleum and hydrocarbon based lubricants as a result of normal machinery operation. Monitoring the depletion of phosphate antiwear additives in in-service lubricants can indicate unusual wear or severe operating conditions of the machine. This test method is designed as a fast, simple spectroscopic check for monitoring of phosphate antiwear additives in in-service petroleum and hydrocarbon based lubricants with the objective of helping diagnose the operational condition of the machine based on measuring the level of phosphate antiwear additives in the oil.

1.3 Acquisition of FT-IR spectral data for measuring phosphate antiwear additives in in-service oil and lubricant samples is described in Practice [D7418](#). In this test method, measurement and data interpretation parameters for phosphate antiwear additives using both direct trend analysis and differential (spectral subtraction) trend analysis are presented.

1.4 This test method is based on trending of spectral changes associated with phosphate antiwear additives in in-service petroleum and hydrocarbon based lubricants. Warnings or alarm limits can be set on the basis of a fixed minimum

---

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee [D02](#) on Petroleum Products, Liquid Fuels, and Lubricants and is the direct responsibility of Subcommittee [D02.96](#) on In-Service Lubricant Testing and Condition Monitoring Services.

Current edition approved July 1, 2009. Published August 2009. DOI: 10.1520/D7412-09.

value for a single measurement or, alternatively, can be based on a rate of change of the response measured, see Ref (1).<sup>2</sup>

1.4.1 For direct trend analysis, values are recorded directly from absorption spectra and reported in units of absorbance per 0.1 mm pathlength.

1.4.2 For differential trend analysis, values are recorded from the differential spectra (spectrum obtained by subtraction of the absorption spectrum of the reference oil from that of the in-service oil) and reported in units of 100\*absorbance per 0.1 mm pathlength (or equivalently absorbance units per centimeter).

1.4.3 In either case, maintenance action limits should be determined through statistical analysis, history of the same or similar equipment, round robin tests or other methods in conjunction with the correlation of changes in the level of phosphate antiwear additives to equipment performance.

NOTE 1—It is not the intent of this test method to establish or recommend normal, cautionary, warning or alert limits for any machinery. Such limits should be established in conjunction with advice and guidance from the machinery manufacturer and maintenance group.

1.5 This test method is for petroleum and hydrocarbon based lubricants and is not applicable for ester based oils, including polyol esters or phosphate esters.

1.6 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.6.1 *Exception*—The unit for wave numbers is  $\text{cm}^{-1}$ .

1.7 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

---

<sup>2</sup> The boldface numbers in parentheses refer to a list of references at the end of this standard.

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>3</sup>

- D445** Test Method for Kinematic Viscosity of Transparent and Opaque Liquids (and Calculation of Dynamic Viscosity)
- D2896** Test Method for Base Number of Petroleum Products by Potentiometric Perchloric Acid Titration
- D5185** Test Method for Multielement Determination of Used and Unused Lubricating Oils and Base Oils by Inductively Coupled Plasma Atomic Emission Spectrometry (ICP-AES)
- D6304** Test Method for Determination of Water in Petroleum Products, Lubricating Oils, and Additives by Coulometric Karl Fischer Titration
- D7414** Test Method for Condition Monitoring of Oxidation in In-Service Petroleum and Hydrocarbon Based Lubricants by Trend Analysis Using Fourier Transform Infrared (FT-IR) Spectrometry
- D7415** Test Method for Condition Monitoring of Sulfate By-Products in In-Service Petroleum and Hydrocarbon Based Lubricants by Trend Analysis Using Fourier Transform Infrared (FT-IR) Spectrometry
- D7418** Practice for Set-Up and Operation of Fourier Transform Infrared (FT-IR) Spectrometers for In-Service Oil Condition Monitoring
- E131** Terminology Relating to Molecular Spectroscopy
- E2412** Practice for Condition Monitoring of In-Service Lubricants by Trend Analysis Using Fourier Transform Infrared (FT-IR) Spectrometry

## 3. Terminology

3.1 *Definitions*—For definitions of terms relating to infrared spectroscopy used in this test method, refer to Terminology **E131**. For definition of terms related to in-service oil condition monitoring, refer to Practice **D7418**.

3.2 *machinery health, n*—qualitative expression of the operational status of a machine subcomponent, component, or entire machine, used to communicate maintenance and operational recommendations or requirements in order to continue operation, schedule maintenance, or take immediate maintenance action.

## 4. Summary of Test Method

4.1 This test method uses FT-IR spectrometry to monitor levels of phosphate antiwear additives in in-service petroleum and hydrocarbon based lubricants. The FT-IR spectra of in-service oil samples are collected according to the protocol for either direct trend analysis or differential trend analysis described in Practice **D7418**, and the levels of phosphate antiwear additives are measured using the peak height or area measurements described herein.

## 5. Significance and Use

5.1 Antiwear additives are commonly used in petroleum and hydrocarbon based lubricants to prevent machinery wear by forming a chemical barrier activated by frictional heat. Antiwear additives that are phosphate based can be measured by FT-IR spectroscopy using the phosphate absorption band. Initially, phosphate antiwear additives will decompose and form a protective film by binding to metal surfaces and through oxidative mechanisms, and so a decrease in the level of phosphate antiwear additive relative to that in the new oil is expected during normal machinery operation. Subsequently, significant depletion of phosphate antiwear additives due to oxidation or hydrolysis can occur when the lubricant is subjected to high temperatures and high levels of moisture. This usually occurs prior to the point where the oxidation of the lubricant begins to accelerate—making trending of phosphate antiwear additives a useful indicator of the lubricant's remaining in-service life. Monitoring of phosphate antiwear additive depletion is therefore an important parameter in determining overall machinery health and should be considered in conjunction with data from other tests such as atomic emission (AE) and atomic absorption (AA) spectroscopy for wear metal analysis (Test Method **D5185**), physical property tests (Test Methods **D445**, **D2896**, and **D6304**) and other FT-IR oil analysis methods for oxidation (Test Method **D7414**), sulfate by-products (Test Method **D7415**), nitration, breakdown products and external contaminants (Practice **E2412**), which also assess elements of the oil's condition, see Refs (1-6).

## 6. Interferences

6.1 High levels of glycol and ester based additives, or contaminants, or both, can interfere with the measurement of phosphate antiwear additives.

## 7. Apparatus

7.1 Fourier transform infrared spectrometer equipped with sample cell, filter (optional) and pumping system (optional) as specified in Practice **D7418**.

7.2 *FT-IR Spectral Acquisition Parameters*—Set FT-IR spectral acquisition parameters according to instructions in Practice **D7418**.

## 8. Sampling

8.1 Obtain a sample of the in-service oil and a sample of the reference oil (required only for differential trend analysis) according to the protocol described in Practice **D7418**.

## 9. Preparation and Maintenance of Apparatus

9.1 Rinse, flush, and clean the sample cell, lines and inlet filter according to instructions in Practice **D7418**.

9.2 Monitor cell pathlength as specified in Practice **D7418**.

## 10. Procedure

10.1 Collect a background spectrum according to the procedure specified in Practice **D7418**.

10.2 *Differential Trend Analysis Only*—Collect the absorption spectrum of a reference oil sample according to the procedure specified in Practice **D7418**.

<sup>3</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

10.3 Collect the absorption spectrum of an in-service oil sample according to the procedure specified in Practice D7418.

10.4 *Data Processing*—All data are normalized to a path-length of 0.100 mm according to the procedure specified in Practice D7418.

## 11. Calculation

### 11.1 Calculation of Phosphate Antiwear Value:

11.1.1 *Procedure A (Direct Trend Analysis)*—Phosphate antiwear value by the direct trending method is calculated from the oil sample spectrum using the measurement area and baseline points listed in Table 1. Fig. 1 illustrates the area used in the measurement of phosphate antiwear additives in the spectrum of diesel crankcase oil.

11.1.2 *Procedure B (Differential Trend Analysis)*—Phosphate antiwear value by the differential trending method is calculated from the differential spectrum using a minimum peak height and a two-point baseline (Table 1), giving negative values as the amount of phosphate antiwear additives in the in-service oil relative to that in the reference oil progressively decreases. Fig. 2 illustrates the band used in the measurement of phosphate antiwear additives in the differential spectrum of diesel crankcase oil.

11.2 *Sample Carryover*—To ensure the minimum amount of sample-to-sample cross-contamination or carryover, either a minimum volume of the subsequent sample or a solvent rinse is used to flush out the previous sample. The efficacy of the flushing protocol may be assessed by consecutively analyzing a used oil sample having a low phosphate antiwear level (L1) and an oil having a high phosphate antiwear level (H1) followed by a second run of the oil sample having a low phosphate antiwear level (L2) and then calculating the percent carryover (PC) as follows. The calculated PC should be <5%.

$$PC = [(L2 - L1)/H1] \times 100 \quad (1)$$

where:

L1, H1, and L2 = the values measured for phosphate antiwear additives (using the parameters given in Table 1) for the samples run in the indicated sequence.

## 12. Report

12.1 *Procedure A (Direct Trend Analysis)*—Values are reported in units of absorbance/0.100 mm.

**TABLE 1 Parameters for Measuring Phosphate Antiwear Additives in In-Service Petroleum and Hydrocarbon Based Lubricants**

| Method                                    | Measurement, cm <sup>-1</sup>   | Baseline Point(s), cm <sup>-1</sup> |
|---|---------------------------------|-------------------------------------|
| Procedure A (Direct Trend Analysis)       | Area from 1025 to 960           | Minima 2200 to 1900 and 650 to 550  |
| Procedure B (Differential Trend Analysis) | Minimum height from 1020 to 930 | Two points at 1020 and 930          |

12.2 *Procedure B (Differential Trend Analysis)*—Values are reported in units of absorbance per centimeter (Abs/cm), calculated as follows:

$$\text{Phosphate Antiwear in Abs/cm} \quad (2)$$

$$= \text{Phosphate Antiwear in Abs/0.100 mm} \times 100$$

12.3 *Trending*—Data shall be recorded and reported at selected time intervals during the lubricant’s life. Ideally, phosphate antiwear values would be compared to that of the newly formulated oil and plotted over time to visualize the relative changes in phosphate antiwear additives and to determine when there needs to be an oil change, albeit other parameters may dictate this change earlier. Sampling and reporting time intervals for phosphate antiwear additives are based on the type of machinery and its previous history associated with this parameter.

12.4 *Statistical Analysis and Alarm Limits*—For statistical analysis and setting alarm limits, refer to Practice E2412, Annex A3 on “Distribution Profiles and Statistical Analysis.”

12.5 *Effects of Oil Formulation*—The compositions of various oil formulations can have an effect on the results reported for the phosphate antiwear value, and values from two different oil formulations should not be compared. Results should be interpreted relative to values measured for unused oils of the same formulation or trended directly from the sample history.

## 13. Precision and Bias (Interim)<sup>4</sup>

13.1 *Precision*—The precision of the test method has not yet been determined by a formal interlaboratory study. Preliminary examinations of repeatability have shown that the difference between repetitive results obtained by the same operator in a given laboratory applying the same test method with the same apparatus under constant operating conditions on identical test material within short intervals of time would in the long run, in the normal and correct operation of the test method, exceed the following values only in one case in 20:

repeatability = 0.53 absorbance units/0.100 mm for Procedure A (direct trend analysis)  
 repeatability = 0.57 absorbance units/cm for Procedure B (differential trend analysis)

The reproducibility of this test method is being determined and will be available on or before May 1, 2013.

13.2 *Bias*—The procedures in this test method have no bias because the phosphate antiwear values can be defined only in the terms of the test method and no accepted reference method or value is available.

## 14. Keywords

14.1 condition monitoring; differential trend analysis; direct trend analysis; Fourier transform infrared; FT-IR; hydrocarbon based lubricants; in-service petroleum lubricants; infrared; IR; lubricants; oils; phosphate antiwear

<sup>4</sup> Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:D02-1667.

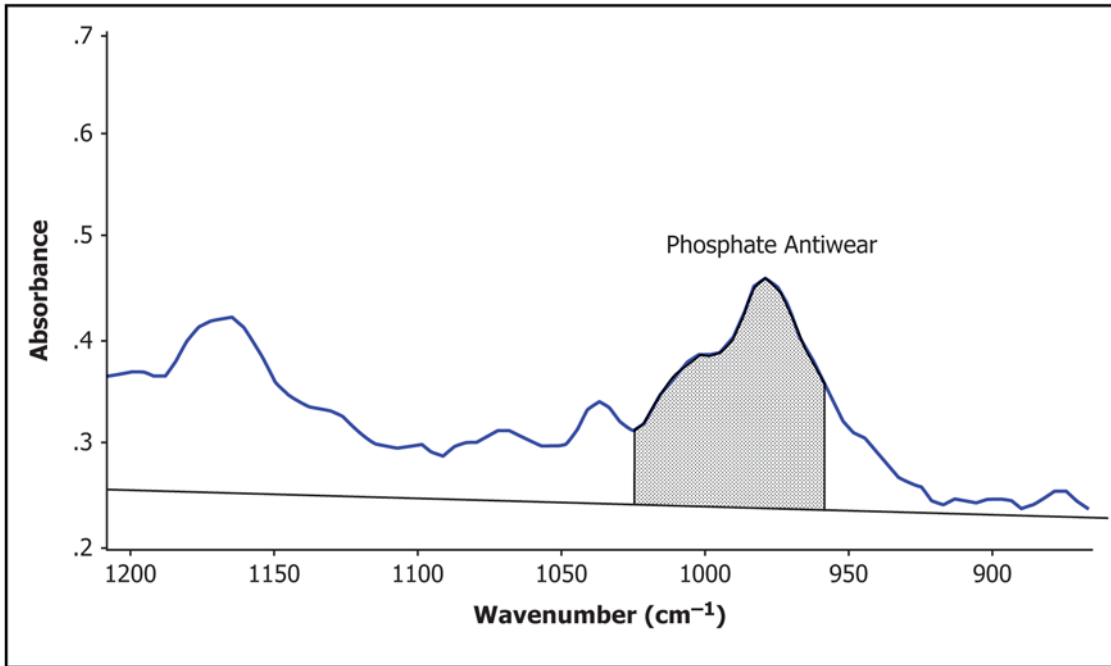


FIG. 1 Phosphate Antiwear Measurement in the Spectrum of a Diesel Crankcase Oil for Direct Trend Analysis (Procedure A)

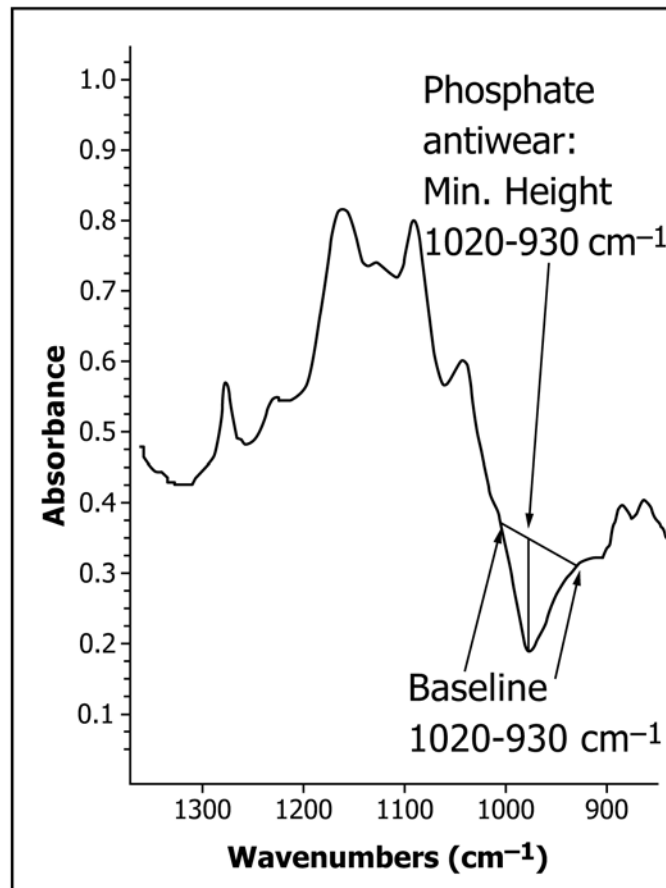


FIG. 2 Phosphate Antiwear Measurement in the Differential Spectrum of a Petroleum Crankcase Lubricant for Differential Trend Analysis (Procedure B)

## REFERENCES

- (1) Toms, L. A., and Toms, A. M., *Machinery Oil Analysis: Methods, Automation & Benefits*, 3rd edition, STLE, 2008.
- (2) Coates, J., and Setti, L., "Infrared Spectroscopy as a Tool for Monitoring Oil Degradation," *Aspects of Lubricant Oxidation*, ASTM Special Technical Publication 916, ASTM International, 1986, pp. 57-78.
- (3) Garry, M., "Applied Interpretation of FT-IR Oil Analysis Results for Improving Predictive Maintenance Programs," Proceedings of the 1992 Joint Oil Analysis Program International Condition Monitoring Conference, *JOAP-TSC*, 1992, pp. 233-254.
- (4) Powell, J., and Compton, D., "Automated FTIR Spectrometry for Monitoring Hydrocarbon-Based Engine Oils," *Lubrication Engineering*, 49, 3, March 1993, pp. 233-239.
- (5) Toms, A., and Powell, J., "Molecular Analysis of Lubricants by FT-IR Spectrometry," *P/PM Technology*, 10, 4, August 1997, pp. 58-64.
- (6) Lukas, M., and Anderson, D., "Laboratory Used Oil Analysis Methods," *CRC/STLE Tribology Data Handbook*, Booser, E., ed., CRC Press, 1997.

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or [service@astm.org](mailto:service@astm.org) (e-mail); or through the ASTM website ([www.astm.org](http://www.astm.org)). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>*