



# Standard Test Method for Nitrite-Nitrate in Water by Nitrate Reductase<sup>1</sup>

This standard is issued under the fixed designation D7781; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This test method is applicable to the determination of nitrate plus nitrite (as nitrogen) in drinking water, surface, saline, wastewater, and ground waters. The applicable range of this test method is from 0.05 to 5 mg/L of nitrogen. The range may be extended upward by dilution of an appropriate aliquot. The 40 CFR Part 136 Method Detection Limit (MDL) is 0.02 mg /L.

1.2 It is the user's responsibility to ensure the validity of this test method for waters of untested matrices. The quality control criteria in Section 17 for method blanks, laboratory control samples, matrix spikes and matrix duplicates must be met.

1.3 The values stated in SI units are regarded as standard. No other units of measurement are included in this standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

D992

D1129 Terminology Relating to Water

D1141 Practice for the Preparation of Substitute Ocean Water

D1193 Specification for Reagent Water

D1254 Method of Test for Nitrite Ion in Water (Withdrawn 1980)<sup>3</sup>

D3867 Test Methods for Nitrite-Nitrate in Water

D5810 Guide for Spiking into Aqueous Samples

D6146 Guide for Monitoring Aqueous Nutrients in Watersheds

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee D19 on Water and is the direct responsibility of Subcommittee D19.05 on Inorganic Constituents in Water.

Current edition approved April 1, 2014. Published May 2014. DOI: 10.1520/D7781-14.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>3</sup> The last approved version of this historical standard is referenced on [www.astm.org](http://www.astm.org).

## 3. Terminology

3.1 *Definitions*—For definitions of terms used in these test methods, refer to Terminology D1129.

3.2 *Definitions of Terms Specific to This Standard:*

3.2.1 *bispecific NaR, n*—nitrate reductase that can use either NADH or NADPH as its electron donor (cofactor).

3.2.2 *discrete analyzer, n*—a programmable, computer-controlled instrument that automates wet-chemical analysis by using one or more robotic arms interfaced to high-precision volumetric dispensers to aspirate and dispense samples, standards, diluents, and reagents.

3.2.3 *Greiss reaction, n*—chemical formation of an azo dye by diazotization of nitrite ion with sulfanilamide and subsequent coupling with *N*-(1-naphthyl)ethylenediamine hydrochloride.

3.2.4 *NADH, n*—nicotinamide adenine dinucleotide, reduced form is a coenzyme found in all living cells.

3.2.5 *NADPH, n*—nicotinamide adenine dinucleotide phosphate, reduced form is a coenzyme found in all living cells; NADP<sup>+</sup> is the oxidizing form and NADPH is the reducing form.

3.2.6 *nitrate reductase (NaR), n*—NADH:NaR (EC1.7.1.1 and CAS 9013-03-0) or bispecific NaR (EC 1.7.1.2 and CAS 9029-27-0) with 1 unit of enzyme activity defined as 1 micromol nitrite produced per minute at 30°C, at pH 7 with NADH (refer to 3.2.4 and 10.2) as an electron donor.

## 4. Summary of Test Method

4.1 *Nitrite-Nitrate Nitrogen*—The sample is mixed with a buffered solution containing NAD(P)H: nitrate reductase (EC 1.7.1.3) and NADH or NADPH to reduce nitrate ion to nitrite ion. The combined nitrite-nitrate (expressed as mg/L NO<sub>3</sub>+NO<sub>2</sub>-N) is determined by diazotizing the total nitrite ion with sulfanilamide and coupling with *N*-(1-naphthyl) ethylenediamine dihydrochloride to form a highly colored azo dye that is measured spectrophotometrically at about 540 nm.

4.2 *Nitrite Nitrogen*—The nitrite ion (expressed as mg/L NO<sub>2</sub>-N) originally present in the sample can be determined separately by carrying out the procedure and omitting the reduction step.

4.3 *Nitrate Nitrogen*—The nitrate ion as nitrogen can be calculated as the difference between the combined nitrate plus nitrite ( $\text{NO}_3 + \text{NO}_2 - \text{N}$ ) and the nitrite ( $\text{NO}_2 - \text{N}$ ):

$$\text{mg/LNO}_3 - \text{N} = \text{mg/L}(\text{NO}_3 + \text{NO}_2 - \text{N}) - \text{mg/L}(\text{NO}_2 - \text{N}) \quad (1)$$

## 5. Significance and Use

5.1 This test method replaces Test Methods **D1254** (Nitrite) and **D992** (Nitrate). The nitrite test method (Test Method **D1254**) used a reagent that is considered to be a potential carcinogen. The nitrate test method (Test Method **D992**) has been shown to have relatively large errors when used in wastewaters and also has greater manipulative difficulties than the test method described herein.

5.2 This test method can be used in place of Test Methods **D3867** (Nitrite-Nitrate). Test Methods **D3867** uses cadmium for the reduction of nitrate to nitrite. Cadmium is considered a toxic metal. Also, the heterogeneous cadmium reductant creates greater difficulty than the reduction described in this test method.

## 6. Interferences

6.1 Turbid samples should be filtered prior to analysis to eliminate particulate interference.

6.2 Sample color that absorbs at wavelengths between 520 and 540 nm interferes with the absorbance measurements. When color is suspect, analyze a sample blank, omitting the *N*-(1-naphthyl)ethylenediamine dihydrochloride from the color reagent.

NOTE 1—The instrumentation described in this standard may automatically correct for some turbidity and sample color. See the instrument manual for further information.

6.3 Certain ions may cause interferences. See **Table 1**.

## 7. Purity of Reagents

7.1 Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents shall conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, when such specifications are available.<sup>4</sup> Other grades may be used, provided it is first ascertained that the reagent is of sufficient high purity to permit its use without lessening the accuracy of the determination.

7.2 *Purity of Water*—Unless otherwise indicated, references to water shall be understood to mean reagent water conforming to Specification **D1193**, Type I or Type II. Other reagent water types may be used, provided it is first ascertained that the water is of sufficiently high purity to permit its use without adversely affecting the bias and precision of these test methods.

## 8. Sampling and Sample Preservation

8.1 Collect the sample in accordance with Guide **D6146**.

<sup>4</sup> *Reagent Chemicals, American Chemical Society Specifications*, American Chemical Society, Washington, DC, [www.chemistry.org](http://www.chemistry.org). For suggestions on the testing of reagents not listed by the American Chemical Society, see the *United States Pharmacopeia and National Formulary*, U.S. Pharmacopeial Convention, Inc. (USPC), Rockville, MD, <http://www.usp.org>.

**TABLE 1 Determination of Nitrate in the Presence of Potential Interferences**

Species	Concentration Added (mg/L)	Unspiked Sample Result (mg/L)	Spiked Sample Results (mg/L)	Spike Added (mg/L)	% Recovery
Cl <sup>-</sup>	500	0.02	0.23	0.200	105
		0.17	2.54	2.50	95
F <sup>-</sup>	500	0.01	0.22	0.200	105
Br <sup>-</sup>	500	<0.01	0.21	0.200	100
		0.15	2.65	2.50	100
PO <sub>4</sub> <sup>-3</sup>	500	0.01	0.22	0.200	105
		0.14	2.54	2.50	96
SO <sub>4</sub> <sup>-2</sup>	500	<0.01	0.21	0.200	105
		0.14	2.53	2.50	96
Fe	500	0.17	2.60	2.50	97
	1.0	<0.01	0.21	0.200	105
Zn	1.0	0.168	2.59	2.50	96
		<0.01	0.22	0.200	110
Al	1.0	0.14	2.64	2.50	100
		<0.01	0.21	0.200	105
BrO <sub>3</sub> <sup>-</sup>	1.0	0.14	2.53	2.50	96
		<0.01	0.22	0.200	110
ClO <sub>2</sub> <sup>-</sup>	1.0	0.17	2.64	2.50	99
		<0.01	0.22	0.200	110
ClO <sub>3</sub> <sup>-</sup>	1.0	0.14	2.54	2.50	96
		0.23	2.45	2.50	89
CHCl <sub>3</sub>	>Miscibility	<0.01	0.21	0.200	105

8.2 When nitrite ion is to be determined separately, analyze within 48 hours after sampling. Even when sterile bottles are used, bacteria naturally present in the water may cause conversion of all or part of nitrite ion to other forms such as nitrate or ammonia. Ammonia and natural amines, which are frequently present in natural waters, may react with nitrites to form nitrogen. If samples are to be stored for 48 h or less, preserve the sample by refrigeration at 2–6°C. If the sample must be stored for more than 48 h, preserve it by the addition of sulfuric acid to pH 2 in addition to refrigeration at 2–6°C.

NOTE 2—Use sulfuric acid for preservation of nitrite-nitrate nitrogen only. Samples for nitrite must be analyzed within 48 hours.

NOTE 3—Sulfuric acid does not necessarily inhibit oxidation and mercury compounds should be avoided to prevent environmental pollution.

NOTE 4—Residual chlorine does not interfere, however, attempts to remove residual chlorine (such as addition of ascorbic acid) interfere by inhibiting reduction of nitrate to nitrite. Do attempt to remove residual chlorine.

## 9. Apparatus

9.1 Automated discrete analysis system (see **3.2.2**).

## 10. Reagents

10.1 *Phosphate Buffer Solution*—Dissolve 3.75 g of potassium dihydrogen phosphate (KH<sub>2</sub>PO<sub>4</sub>), 0.01 g of disodium ethylenediaminetetraacetate dehydrate

**TABLE 2 Example Concentrations of Calibration Standards**

NO <sub>3</sub> -N or NO <sub>2</sub> -N, mg/L	mL of 10 mg/L Standard Solution/100 mL final volume
0.05	0.5
0.1	1.0
0.5	5.0
1.0	10
2.0	20
3.0	30
5.0	50

**TABLE 3 Reduction Efficiency**

NO <sub>3</sub> -N or NO <sub>2</sub> -N, mg/L	mL of 10 mg/L Standard Solution/100 mL final volume
Mean (%)	103
Standard Deviation	4.14
Lower Limit (%)	91
Upper Limit (%)	115

(C<sub>10</sub>H<sub>14</sub>O<sub>8</sub>N<sub>2</sub>Na<sub>2</sub>·2H<sub>2</sub>O), and 1.4 g potassium hydroxide (KOH) in about 500 mL reagent water contained in a 1000 mL volumetric flask, dilute to the mark and mix. Transfer this solution to a screw-cap container and store at 2–6°C. This solution is stable for 6 months.

**10.2 β-nicotinamide adenine dinucleotide, Reduced Form (NADH) Stock Solution (2 mg/mL)**—Dissolve 0.1 g NADH (C<sub>21</sub>H<sub>27</sub>N<sub>7</sub>O<sub>14</sub>P<sub>2</sub>) in 25 mL of reagent water contained in a 50 mL volumetric flask, dilute to the mark and mix. Transfer 1-mL aliquots to 1.5 mL snap-cap colorless polypropylene vials and store at –20°C. Stable for 1 month.

**NOTE 5**—NADH is a hygroscopic white powder that is freely soluble in water. The solids are stable if stored dry and protected from light. Neutral solutions are colorless and stable for 1 week if stored at 4°C, but decompose rapidly under basic or acidic conditions.

**10.3 NADH Working Solution**—Thaw one 1-mL vial of NADH stock (refer to 10.2) and dilute to 10 mL with phosphate buffer (refer to 10.1). This reagent is stable for about 8 hours. Prepare sufficient NADH working solution for the number of samples and standards to be analyzed.

**NOTE 6**—NADH inhibits color formation in the Greiss reaction (refer to 3.2.3). The molar concentration of NADH in the reduction medium should be about twice that of the highest calibration standard.

**10.4 Sulfanilamide (SAN) Reagent (10g/L)**—While stirring constantly add 300 mL of concentrated hydrochloric acid (HCl, 37 % w/v) and 10 g of sulfanilamide (SAN, C<sub>6</sub>H<sub>8</sub>N<sub>2</sub>O<sub>2</sub>S) to about 500 mL reagent water contained in a 1000 mL volumetric flask, dilute to the mark and mix. This solution is stable for about six months when stored in a brown bottle at 20°C.

**10.5 N-(1-naphthyl)ethylenediamine dihydrochloride (NED) Solution (1g/L)**—dissolve 1 g NED (C<sub>10</sub>H<sub>7</sub>NHCH<sub>2</sub>CH<sub>2</sub>NH<sub>2</sub>·2HCl) in about 500 mL reagent water contained in a 1000 mL volumetric flask, dilute to the mark and mix. Transfer to a glass or amber screw-cap container. This solution is stable for 6 months at 20°C.

**10.6 Nitrate Reductase (NaR)**—Follow the manufacturer’s instructions for preparing a solution of 1 unit NaR (refer to 3.2.6) activity per mL of phosphate buffer (refer to section 10.1). Dilute 3 units NaR to 20 mL with phosphate buffer. Store

the solution at 2–6°C, where it is stable for 8 hours. Prepare sufficient NaR for the total number of samples and standards to be analyzed.

**NOTE 7**—For some NaR forms, high phenolic content humic substances (>2 mg dissolved organic carbon/L) have little affect on the NaR activity in the temperature range of 5–15°C, but become increasingly inhibitory in the temperature range of 20–30°C. Humic substances at the operation temperatures specified in this standard do not inhibit other forms of NaR.<sup>5</sup> If humic acids are expected to be present the user must verify reduction efficiency of the NaR is use by analysis of Quality Control checks that approximate the sample matrix.

**10.7 Nitrate Solution, Stock (1000 mg/L NO<sub>3</sub>-N)**—Dry potassium nitrate (KNO<sub>3</sub>) in an oven at 105°C for 24 h. Dissolve 7.218 g in water in about 500 mL reagent water contained in a 1000 mL volumetric flask, dilute to the mark and mix. This solution is stable for up to 2 months with refrigeration. Alternatively, certified nitrate stock solutions are commercially available through chemical supply vendors and may be used.

**10.8 Nitrate Solution, Standard (10 mg/L NO<sub>3</sub>-N)**—Dilute 10 mL of stock nitrate solution (10.7) to 1 L with water and store in a dark bottle. Prepare fresh as needed.

**10.9 Nitrite Solution, Stock (1000 mg/L NO<sub>2</sub>-N)**—Place about 7 g of potassium nitrite (KNO<sub>2</sub>) in a tared 125-mL beaker and dry for about 24 h to a constant weight in a desiccator containing a suitable desiccant. Adjust the weight of the dry potassium nitrite to 6.072 g. Add 50 mL of water to the beaker, stir until dissolved, and transfer quantitatively to a 1000-mL volumetric flask. Dilute to the mark with water store in a sterilized bottle under refrigeration. Prepare fresh as needed. Alternatively, certified nitrite stock solutions are commercially available through chemical supply vendors and may be used.

**NOTE 8**—Potassium nitrite is easily oxidized; use only dry, free flowing white, or yellowish white crystalline powder of this reagent.

**10.10 Nitrite Solution, Standard (10 mg/L NO<sub>2</sub>-N)**—Dilute 10 mL of stock nitrite solution (10.9) to 1 L with water. This solution is unstable; prepare fresh as needed.

## 11. Hazards

**11.1** All reagents and standards should be prepared in volumes consistent with laboratory use to minimize the generation of waste.

## 12. Calibration

**12.1** Using the standard nitrate solution (10.8) prepare calibration standards by using the automated calibration function of the discrete analyzer (3.2.2). Table 2 specifies suggested calibration levels.

**12.2** Prepare at least one calibration standard from the standard nitrite solution (10.10) at the same concentration as one of the nitrate standards to verify the efficiency of the reduction. Verify that reduction efficiency is between 90 and 115 % with each batch of enzyme. See Table 3.

**NOTE 9**—When the sample to be analyzed is saline water, use substitute ocean water (SOW) to prepare the standards (Practice D1141 or a

<sup>5</sup> NaR available from the Nitrate Elimination Company Inc. (NECi), www.nitrate.com, has been found suitable.

commercially available synthetic seawater). Run a reagent water blank in addition to a SOW blank because the reagents used to prepare SOW frequently contain nitrite or nitrate, or both. Adjust this curve for the contaminant level in SOW.

NOTE 10—Most discrete analyzers generate calibration standards and calibration curves automatically. Follow the manufacturer’s instructions for calibrating with individual calibration standards if an automatic calibration function is not available.

12.3 Develop the color and determine the absorbance of each standard as directed in the procedure (13.4.6).

12.4 Prepare a standard curve by plotting the absorbance (or optical density) of each processed calibration standard against its known concentrations. See Fig. 1 for an example of a calibration curve.

12.5 Verify the calibration each day, or before each use with a calibration verification solution (see 17.2.2).

### 13. Conditioning

13.1 *Removal of Interferences*—Remove interferences (Section 6) by the following procedures:

13.2 For turbidity removal, when suspended solids are present, filter the sample through a glass-fiber filter or a 0.45- $\mu\text{m}$  filter. Centrifugation can be used as an option.

13.3 For correction for color interferences, if there is a possibility that the color of the sample might absorb in the photometric range from  $530 \pm 10$  nm, determine the background absorbance.

NOTE 11—Many discrete analyzers automatically compensate for background absorbance and turbidity on each sample. Follow the manufacturer’s instructions.

13.4 Prepare a method in the discrete analyzer software according to the following, or similar, conditions as recommended by the manufacturer:

13.4.1 Dispense 170 microliters of Nitrate Reductase NaR (10.6) plus 10 microliters of sample. Mix.

13.4.2 Add 15 microliters of NADH (10.3). Mix and measure the background absorbance (or optical density).

13.4.3 Incubate 600 seconds at 37°C.

13.4.4 Add 25 microliters of SAN reagent (10.4). Mix and incubate 120 seconds at 37°C.

13.4.5 Add 25 microliters of NED reagent (10.5). Mix and incubate 120 seconds at 37°C.

13.4.6 Measure absorbance (or optical density) at 540 nm.

NOTE 12—When determining nitrite alone, replace NaR reagent (10.6) with Phosphate Buffer (10.1).

NOTE 13—Samples may be reduced manually keeping sample to reagent ratios similar to steps 13.4.1 – 13.4.5. Analyze the reduced sample by Test Methods D3867 without the cadmium column inline.

### 14. Calculation

14.1 Determine the concentration of nitrate or nitrite nitrogen in the samples in milligrams per liter using the computer based data handler provided with the automated discrete analyzer software.

NOTE 14—The discrete analyzer will automatically calculate the net absorbance by subtracting the background absorbance from the measured absorbance of the color developed sample. Use the net absorbance to determine the concentration of nitrogen in the sample.

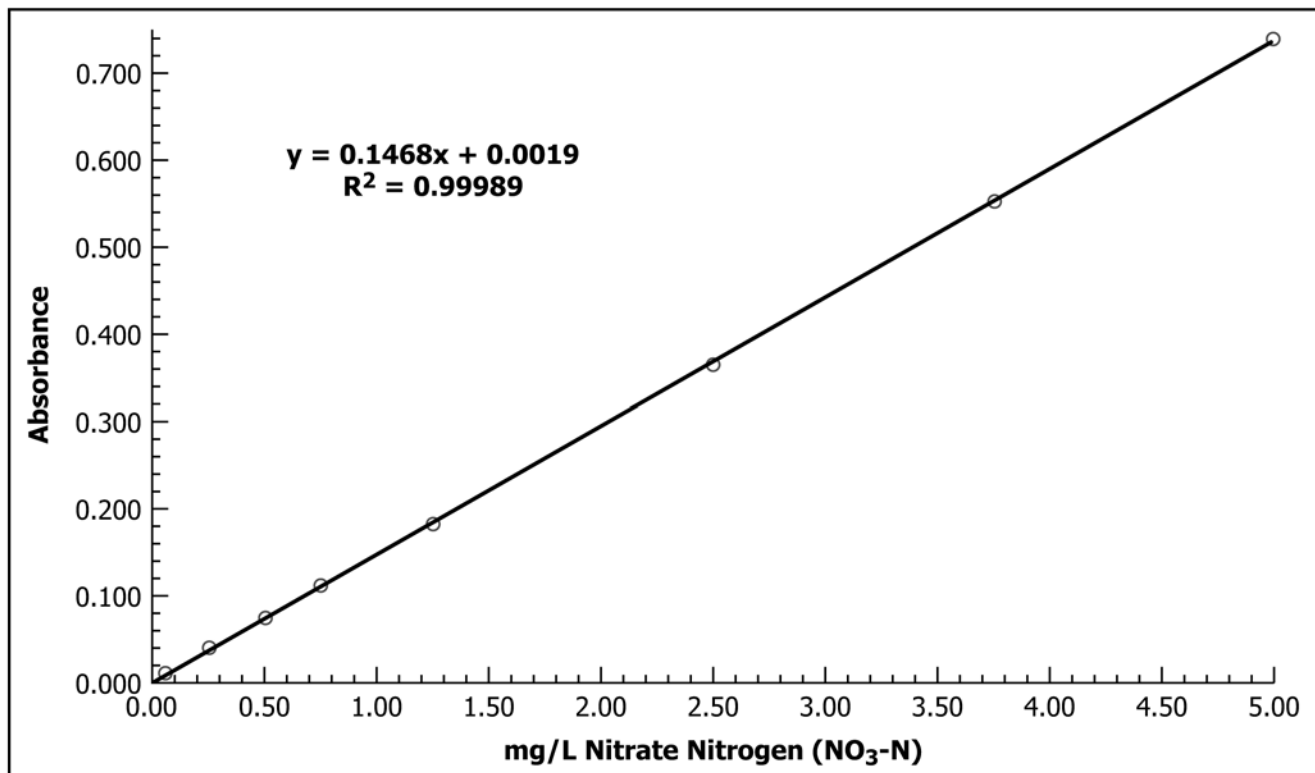


FIG. 1 Example Calibration Curve

**TABLE 4 Precision and Bias for Drinking Water**

Sample Matrix	Mean (mg/L)	Standard Deviation	No. of Laboratories	No. of Results	Multi-laboratory %RSD
High TDS (500 ppm)	0.77	0.02	5	35	2.28 %
High TOC (2 ppm)	1.12	0.02	5	35	1.36 %
ERA #698 WS	6.59	0.17	4	28	2.51 %

**TABLE 5 Overall Spike and Spike Duplicate Data for Drinking Water**

Matrix	Average Spike Recovery (%)	Average RPD (%)
High TDS (500 ppm)	101	2.20
High TOC (2 ppm)	99.5	3.25
ERA #698 WS	98.4	3.99

**TABLE 6 Summary of Nitrate Analysis on Groundwater Samples**

Samples #	Analysis by Cd Reduction (mg NO <sub>3</sub> +NO <sub>2</sub> -N/L)	Analysis by Reductase (mg NO <sub>3</sub> +NO <sub>2</sub> -N/L)	Analysis by Reductase (mg NO <sub>3</sub> +NO <sub>2</sub> -N/L) Non-Preserved
1	0.96	0.94	0.88
2	0.04	0.05	0.06
3	0.32	0.24	0.55
4	0.68	0.68	0.58
5	10.1	11.6	Lost
6	0.75	0.79	0.77
7 <sup>A</sup>	2.5	3.11	2.88

<sup>A</sup> Sample #7 contains sulfide. Sulfide reacts with cadmium forming cadmium sulfide decreasing the efficiency of the reduction.

14.2 Where separate values are required for nitrite-nitrogen and nitrate-nitrogen, calculate the nitrate-nitrogen by subtracting the nitrite-nitrogen from the total nitrate-nitrite nitrogen content.

## 15. Report

15.1 Report the following information:

15.1.1 Report the nitrogen content in milligrams per liter as:

15.1.1.1 Nitrite-Nitrogen (NO<sub>2</sub>-N), mg/L,

15.1.1.2 Nitrate-Nitrogen (NO<sub>3</sub>-N), mg/L, and

15.1.1.3 Combined Nitrate-Nitrite Nitrogen (NO<sub>3</sub>, NO<sub>2</sub>-N), mg/L.

## 16. Precision and Bias

16.1 *Precision and Bias for Drinking and Source Water Matrices:*

16.1.1 Based on the results of five operators in five laboratories, the overall precision and bias for drinking water are shown in Table 4. The precision and bias were obtained on the matrices indicated during an inter-laboratory study; data may not apply to untested matrices.

16.1.2 Inter-laboratory spike recovery and spike sample duplicate (RPD) is shown in Table 5.

16.2 *Precision and Bias for Wastewater Matrices:*

16.2.1 Single laboratory recoveries of known amounts of nitrites-nitrates from reagent water and eleven other selected

**TABLE 7 Single Laboratory Validations of Twelve Matrices**

Matrix	Expected (mg NO <sub>3</sub> -N/L)	Found (mg NO <sub>3</sub> -N/L)	% Recovery
Industrial Effluent	1.03	0.95	93
	5.03	5.19	103
POTW Influent	0.10	0.10	100
	5.00	4.46	93
POTW Effluent	1.48	1.61 (10) <sup>A</sup>	110
	5.48	5.19 (2.7)	95
Septic System	0.12	0.11	93
	5.02	5.34	106
Reagent Water	1.06	1.15	109
	5.06	5.22	103
Tap Water	5.04	4.95	98
Seawater	0.15	0.16	107
	1.05	1.10	105
	5.05	4.71 (10)	93
Monitoring Well	10.6	0.99	93
	5.06	5.07	100
Industrial Effluent 1	1.74	1.77 (4.0)	102
	5.74	5.03 (4.4)	88
Soil Extract	1.74	1.62	88
Industrial Effluent 2	1.78	1.80	103
	5.78	4.92	83
Industrial Effluent 3	2.43	2.50	107
Industrial Effluent 3 (diluted)	1.71	1.73	102
	5.71	5.14	89

<sup>A</sup> RPD = Relative Percent Difference in parentheses.

water matrices are shown in Table 6. A comparison of results by this method and Test Methods D3867 is shown in Table 7.

16.2.2 The overall precision and bias based on ten operators and ten laboratories for selected wastewater matrices is shown in Table 8. Inter-laboratory spike sample recovery and spike sample duplicate (RPD) is shown in Table 9.

16.3 It is the user's responsibility to ensure the validity of this test method for waters of untested matrices.

## 17. Quality Control

17.1 To be certain that analytical values obtained using these test methods are valid and accurate within the confidence limits of the test, the following QC procedures must be followed when analyzing nitrite-nitrate in water.

17.2 *Calibration and Calibration Verification:*

17.2.1 Prior to the analysis of samples, calibrate the instrument using at least four working standards containing concentrations of nitrite-nitrate in water that bracket the expected sample concentration.

17.2.2 Before each analysis, verify the calibration with a mid-range calibration standard (CCV). The result should fall within ±10 % of the known concentration.

17.2.3 If the CCV is not within ±10 %, determine the problem, and recalibrate the instrument.

**TABLE 8 Overall Precision and bias for Wastewater Samples**

Sample Matrix	Mean (mg/L)	Standard Deviation	No. of Laboratories	No. of Results	Single Operator % RSD	Multiple Operator % RSD
WW treatment plant influent	0.03	0.0131	10	30	22.9 %	41.9 %
wastewater treatment plant effluent #1	7.73	0.3181	10	30	1.03 %	4.12 %
wastewater treatment plant effluent #2	0.23	0.0126	10	30	2.92 %	5.46 %
Paper Mill waste stream effluent	0.04	0.0156	10	30	14.9 %	41.7 %
metal finisher wastewater effluent	273	10.234	8	24	24.3 %	3.75 %
commercial laundry wastewater effluent	4.90	0.2123	10	30	13.3 %	4.34 %
ERA #507 Hardness	0.02	0.0144	10	30	36.8 %	61.5 %
Confined Animal Feeding Operation (CAFO) effluent	13.9	0.4623	10	30	12.6 %	3.33 %
Low Nutrient Seawater	0.02	0.0112	10	30	31.7 %	62.1 %

**TABLE 9 Overall Spike and Spike Duplicate Data for Wastewater**

Matrix	Average Spike Recovery (%)	Average RPD (%)
WW treatment plant influent	94.1	3.7
wastewater treatment plant effluent #1	99.7	8.1
wastewater treatment plant effluent #2	97.9	2.7
Paper Mill waste stream effluent	102	1.9
metal finisher wastewater effluent	98.0	15.3
commercial laundry wastewater effluent	101	3.2
ERA #507 Hardness	95.2	5.9
Confined Animal Feeding Operation (CAFO) effluent	91.5	16.6
Low Nutrient Seawater	93.5	1.6

17.2.4 Analyze a CCV standard before each calibration, at the end of each batch, and inter-dispersed at regular intervals (usually after every 20th sample) throughout the analytical run.

17.2.5 CCV results should be within  $\pm 10$  % of the known concentration.

17.2.6 If the CCV is not within 10 % of the known concentration, determine the cause, and repeat analysis of samples that were not bracketed by passing CCV standards.

### 17.3 Initial Demonstration of Laboratory Capability (IDC):

17.3.1 If a laboratory has not performed the test before, or if there has been a major change in the measurement system, for example, new analyst, new instrument, and so forth, a precision and bias study must be performed to demonstrate laboratory capability.

17.3.2 Analyze four replicates of a standard solution prepared from a Certified Independent Reference Material (CRM) containing a mid-range concentration of nitrite-nitrate in water.

The matrix and chemistry of the solution should be equivalent to the solution used in the collaborative study. Each replicate must be taken through the complete analytical test method including any sample preservation and pretreatment steps.

17.3.3 Calculate the mean and standard deviation of the four values and compare to the acceptable ranges provided by the manufacturer of the CRM. Do not use this test method to analyze samples unless the IDC recoveries are within the accepted limits.

### 17.4 Laboratory Control Sample (LCS):

17.4.1 To ensure that the test method is in control, analyze a LCS containing a mid-range concentration of nitrite-nitrate in water with each batch or 10 samples. If large numbers of samples are analyzed in the batch, analyze the LCS after every 10 samples. The LCS must be taken through all of the steps of the analytical method including sample preservation and pretreatment. The result obtained for the LCS shall fall within  $\pm 15$  % of the known concentration.

17.4.2 If the result is not within these limits, analysis of samples is halted until the problem is corrected, and either all the samples in the batch must be reanalyzed, or the results must be qualified with an indication that they do not fall within the performance criteria of the test method.

### 17.5 Method Blank:

17.5.1 Analyze a reagent water test blank with each batch. The concentration of nitrite-nitrate in water found in the blank should be less than 0.5 times the lowest calibration standard. If the concentration of nitrite-nitrate in water is found above this level, analysis of samples is halted until the contamination is eliminated, and a blank shows no contamination at or above this level, or the results must be qualified with an indication that they do not fall within the performance criteria of the test method.

**TABLE 10 Drinking Water Quality Control Acceptance Criteria**

QC Sample	% Recovery	% RPD
CCV	90–110	N/A
LCS	90–110	N/A
MS/MSD	90–110	≤10 %

**TABLE 11 Wastewater Quality Control Acceptance Criteria**

QC Sample	% Recovery	% RPD
CCV/IPR	90–110	≤10 %
LCS/LCSD	85–115	≤15 %
MS/MSD	70–125	≤25 %

### 17.6 Matrix Spike (MS):

17.6.1 To check for interferences in the specific matrix being tested, perform a MS on at least one sample from each batch by spiking an aliquot of the sample with a known concentration of nitrite-nitrate in water and taking it through the analytical method.

17.6.2 The spike concentration plus the background concentration of nitrite-nitrate in water must not exceed the high calibration standard. The spike must produce a concentration in the spiked sample that is 2 to 5 times the nitrite-nitrate in water concentration in the unspiked sample, or 10 to 50 times the detection limit of the test method, whichever is greater.

17.6.3 Calculate the percent recovery of the spike (P) using the following equation:

$$P = 100 \times \frac{[A \times (V_s + V) - (B \times V_s)]}{C \times V} \quad (2)$$

where:

A = nitrite+nitrate concentration (mg/L) in spiked samples,

B = nitrite+nitrate concentration (mg/L) in unspiked samples,

C = nitrite+nitrate concentration (mg/L) in the spiking solution,

$V_s$  = sample volume (mL) used, and

V = added spiking solution volume (mL).

17.6.4 The percent recovery of the spike shall fall within the limits given in **Table 10** for drinking water matrices or **Table 11** for wastewater matrices, or both. If the percent recovery is not within these limits, a matrix interference may be present in the sample selected for spiking. Under these circumstances, one of the following remedies must be employed: the matrix interference must be removed, all samples in the batch must be analyzed by a test method not affected by the matrix interference, or the results must be qualified with an indication that they do not fall within the performance criteria of the test method.

NOTE 15—Acceptable spike recoveries are dependent on the concentration of the component of interest. See Guide **D5810** for additional information.

### 17.7 Duplicate:

17.7.1 To check the precision of sample analyses, analyze a sample in duplicate with each batch. If the concentration of the nitrite-nitrate in water is less than five times the detection limit for the nitrite-nitrate in water, a matrix spike duplicate (MSD) should be used.

17.7.2 Calculate the relative percent difference (RPD) of the duplicate values and compare to the RPD maximum in **Table 10** for drinking water or **Table 11** for wastewater, or both.

17.7.3 If the result exceeds the RPD maximum limit, the batch must be reanalyzed or the results must be qualified with an indication that they do not fall within the performance criteria of the test method.

### 17.8 Independent Reference Material (IRM):

17.8.1 In order to verify the quantitative value produced by the test method, analyze an Independent Reference Material (IRM) submitted as a regular sample (if practical) to the laboratory at least once per quarter. The concentration of the IRM should be in the concentration mid-range for the method chosen. The value obtained must fall within the control limits established by the laboratory.

## 18. Keywords

18.1 nitrate; nitrite; nitrate plus nitrite; discrete analyzer; nitrate reductase; enzyme; cadmium reduction

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the ASTM website (www.astm.org/COPYRIGHT/).*