



Standard Specification for Piston or Plunger Operated Volumetric Apparatus¹

This standard is issued under the fixed designation E1154; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This specification covers requirements, operating conditions, and test methods for piston or plunger operated volumetric apparatus (POVA).

1.2 This specification includes specifications applicable for all types of POVA or those given by the manufacturer. The following precautionary caveat pertains only to the test method portion, Section 13, of this specification: *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 *ASTM Standards:*

E617 Specification for Laboratory Weights and Precision Mass Standards

E898 Test Method of Testing Top-Loading, Direct-Reading Laboratory Scales and Balances

2.2 *ISO Documents:*²

ISO 3534 Statistics—Vocabulary and Symbols

ISO 653 Long Solid-Stem Thermometers for Precision Use

ISO 655 Long Enclosed-Scale Thermometers for Precision Use

ISO 4787 Laboratory Glassware—Volumetric Glassware—Methods for Testing and Use

2.3 *Other Documents*³

OIML R 111-1 Weights of classes E₁, E₂, F₁, F₂, M₁, M₁₋₂, M₂, M₂₋₃ and M₃; Part 1: Metrological and technical requirements

3. Terminology

3.1 Definitions of Terms Specific to This Standard:

¹ This specification is under the jurisdiction of ASTM Committee E41 on Laboratory Apparatus and is the direct responsibility of Subcommittee E41.06 on Weighing Devices.

Current edition approved Dec. 1, 2014. Published January 2015. Originally approved in 1987. Last previous edition approved in 2008 as E1154-89 (2008). DOI: 10.1520/E1154-14.

² Available from American National Standards Institute (ANSI), 25 W. 43rd St., 4th Floor, New York, NY 10036, <http://www.ansi.org>.

³ Available from International Organization of Legal Metrology, 11 rue Turgot, 75009 Paris, France. www.oilm.org/en/

3.1.1 *accuracy*⁴—the accuracy of an instrument is the closeness of agreement between the nominal volume and the mean volume, obtained by applying the test procedure specified in Section 13 of this specification. It is quantified by the inaccuracy of the mean.

3.1.2 *dead volume*—the dead volume is that part of the total liquid volume, held in the operational part of the device, which is not delivered.

3.1.2.1 *Discussion*—The dead volume should not be confused with the dead space of an air displacement instrument.

3.1.3 *disposable*—those parts of an instrument that are intended to be used once only and then discarded. Disposable parts are generally intended for use in applications where sample carryover is intolerable.

3.1.4 *maximum error*—the maximum difference between the nominal volume and any single individual volume obtained by applying the test procedure specified in Section 13 of this Specification.

3.1.5 *maximum expectable error*—with more than 95 % probability, the maximum expectable error is calculated as follows:

$$\pm(1E_T + 2s) \quad (1)$$

where:

E_T = inaccuracy of the mean, and

s = standard deviation from the repeatability test in Section 13.

3.1.6 *nominal volume(s)*—the stated volume(s) for which performance is specified.

3.1.7 *piston or plunger operated volumetric apparatus (POVA)*—the volume of liquid to be measured with POVA is defined by one or more strokes of one or more pistons or plungers. POVA may be operated manually or mechanically (for example, electrically, pneumatically or by hydrostatic pressure).

3.1.7.1 *Discussion*—In the following text the word ‘piston’ means ‘piston or plunger.’

⁴ These definitions apply only in the cases where the distributions are Gaussian.

3.1.8 *precision*⁴—the closeness of agreement between the individual volumes obtained by applying the test procedure specified in this specification. It is quantified by the imprecision.

3.1.8.1 *Discussion*—The test procedure specified gives only a measure of the repeatability (see ISO 3534) under controlled conditions.

3.1.9 *reference temperature*—the temperature at which the instrument is designed to deliver its nominal volume(s).

3.1.9.1 *Discussion*—At that temperature the closest agreement between manufacturer’s performance claims and test results may be expected.

3.1.10 *reference temperature range*—that temperature range for which the tolerances for accuracy are specified.

3.1.11 *reusable*—those parts of an instrument that are meant to be used more than once. As the reusability of some parts can rarely be quantified, any institution or individual who reuses a reusable part must see to its safety and effectiveness. Reusable parts are generally intended for use in applications where sample carryover is tolerable, or can be adequately prevented.

3.1.12 *sample carryover*—that portion of the sample that is retained in the instrument and that may affect subsequent samples.

3.1.13 *stated feature*—any feature claimed by the manufacturer.

3.1.14 *unit of volume*—the millilitre or the microlitre, that are accepted substitutes for the cubic centimetre or cubic millimetre.

3.1.14.1 *Discussion*—It is recommended that volumes should be specified in microlitres up to 999 μL , and in millilitres from 1 mL.

3.1.15 *working range*—that part (of the total range) for which manufacturer’s performance specifications are given.

3.1.16 *working temperature range*—that range of temperatures for which manufacturer’s performance specifications are given.

4. Classification

4.1 *Types of POVA*—Piston or plunger operated volumetric apparatus (POVA) are classified as follows:

4.1.1 *Pipette*—A measuring instrument for the transfer of a predetermined volume of liquid from one vessel to another. It is not connected to a reservoir.

4.1.2 *Dispenser*—A measuring instrument for delivering predetermined volumes of liquid from a reservoir. The reservoir may be integrated with the instrument or connected externally.

4.1.3 *Dilutor*—A measuring instrument for taking up different liquids (for example, sample and diluent) and delivering them in combination so as to comprise a predetermined ratio, or predetermined volumes, or both. The reservoir of diluent may be integrated with the instrument or connected externally.

4.1.4 *Displacement Buret*—A measuring instrument from which the volume delivered is determined by an external indicator. The volume delivered can then be read.

4.2 Types of Displacement:

4.2.1 Displacement with an air interface (“air displacement”). The delivered liquid is displaced by an air interface (indirect action), (see Figs. 1 and 2).

4.2.2 Displacement without an air interface (“positive displacement”). The delivered liquid is displaced either by a liquid interface (indirect action) or by actual contact with the piston (direct action), (see Fig. 3 and Fig. 4).

5. Performance Requirements

5.1 Performance Tolerances:

5.1.1 Performance tolerances specified for POVA are meant to include any thermal drift effect upon the accuracy and precision attributable to hand-transmitted heat during normal use. It is, therefore, important that the instrument being evaluated according to the referenced procedure not be preconditioned (warmed) by recent handling, nor isolated from normal handwarming during the test series (30 or 10 cycles).

5.1.2 Volumetric performance tolerances are not specified in this specification. The manufacturer shall specify the performance tolerances in terms of the accuracy of the mean (\bar{E}_C %) and coefficient of variation (CV_c %). Values shall be given for the minimum and maximum volumes of the working range, as well as for any intermediate volumes in the series 1, 2, 5, 10

5.2 The reference temperature recommended for all POVA is 21.5°C, which is the mid-point of the reference temperature range, (see section 3.1.10). The use of another reference temperature must be stated by the manufacturer.

5.2.1 *Reference Temperature Range*—The reference temperature range for all POVA shall be 19 to 24°C, (see section 3.1.9 and section 3.1.10).

5.3 Removable Parts:

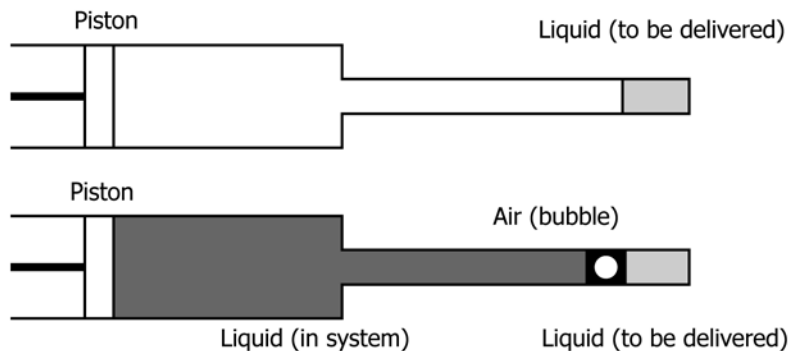


FIG. 1 Displacement With an Air Interface (Air Displacement)


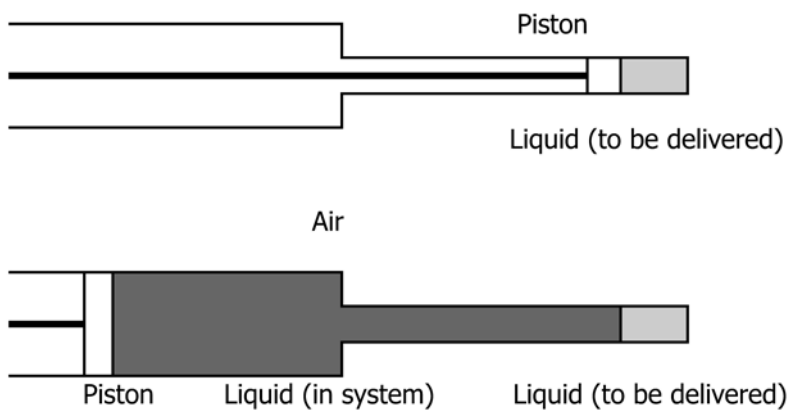


FIG. 2 Displacement Without an Air Interface (Positive Displacement)


PLUNGER POSITIONS

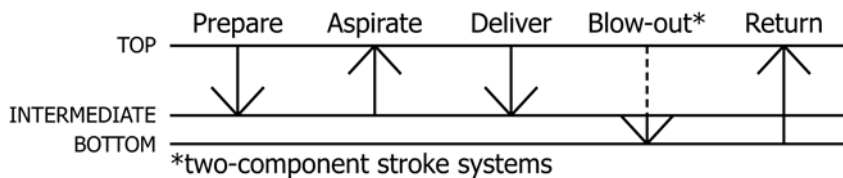

*two-component stroke systems

FIG. 3 Pipetter Mode of Operation (Forward Mode)

PLUNGER POSITIONS

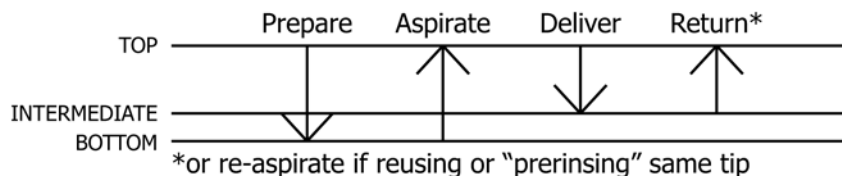

*or re-aspirate if reusing or "prerinsing" same tip

FIG. 4 Pipetter Mode of Operation (Reverse Mode)

5.3.1 The volumetric performance of POVA to be used with removable parts can depend to a large extent on the design, material, and workmanship of those parts. The test procedures described can give information only about the performance of the instruments together with the removable parts actually used.

5.3.2 *Single-Measurement Test*—The single-measurement test requires either 30 or 10 randomly selected removable parts, one for each sample of the series. This test evaluates the instrument's performance and component of imprecision due to the variation of these parts.

5.3.3 *Replicate-Delivery Test*—The replicate delivery test uses one removable part for the 30 or 10 sample series. This test evaluates the instrument's performance and the component of imprecision due to the reuse of this part.

5.4 *Durability*—Any claim by a manufacturer that an instrument is resistant to any defined conditions (for example, sterilization and chemical exposure) shall be understood in such a way that even long term or repeated exposure to those

conditions (as specified by the manufacturer) will not affect the rated performance of the instrument.

6. General Operating Conditions

6.1 *Relationship to Performance*—The specification of operating procedures is critical to the proper functioning of the instruments, and determines their ability to perform within specified tolerances. Changes in the operating mode can dramatically alter the results of analyses. Most instruments are calibrated for certain operating modes; another manner of use may result in a change in the accuracy or precision, or both.

6.2 *Delineation*—It is the manufacturer's responsibility to delineate the modes of operation in instruction manuals and to state for which of the modes the instrument is calibrated.

6.3 *Preparation*—The manufacturer shall provide instructions necessary for the preparation of the instrument for use in particular operating modes (for example, mounting of removable parts, method of volume adjustment, temperature

equation, isothermal requirements, testing of piston action, lubrication, priming, purging or prerinsing information, etc.).

7. Operating Conditions for Pipetters

7.1 Two common modes of operation are in use, the forward mode (sometimes referred to as normal mode), and the reverse mode (usable with two-component stroke mechanism systems only), (see Fig. 3 and Fig. 4).

7.1.1 In general, the precision of the repetitive use of the forward mode relies upon the precise draining by air pressure (in the case of air displacement pipetters) or internal wiping of the pipet barrel or tip (in the case of displacement pipetters). As compared to the reverse mode, the forward mode is relatively insensitive to variations in the speed of the piston or plunger in the dispensing action. Positive displacement instruments with relatively small delivery orifices are generally less sensitive to change in accuracy when handling liquids with high wettability characteristics.

7.1.2 Air displacement pipetters with two-component stroke mechanisms are generally less sensitive than air displacement pipetters with one-stroke mechanisms positive displacement pipetters to errors introduced by slight variations of the dynamics of the liquid interface break at the end of the pipet or pipet tip during the dispensing action, due to the purging action of the air “blow-out” stroke potential.

7.1.3 The use of the reverse mode with two-component stroke mechanism pipetters may be more advantageous when liquids that are difficult to handle in the forward mode are encountered.

7.2 Forward Mode, General Format:

7.2.1 *Preparation*—Pipetter and environment shall be isothermal. Volume settings and the mounting of removable or disposable pipet tips shall be accomplished according to the manufacturer’s directions.

7.2.2 *Aspiration:*

7.2.2.1 Hold the instrument in a vertical position, or as prescribed by the manufacturer.

7.2.2.2 In the case of two-component stroke systems, depress the push button smoothly to the intermediate stop position.

7.2.2.3 In the case of one-component stroke systems, depress the push-button smoothly to the bottom stop position.

7.2.2.4 Immerse the pipet or pipet tip into the liquid to be pipetted to, and maintain it at the following depth:

Volume, μL	Immersion Depth, mm
1 to 100	2 to 3
101 to 1000	2 to 4
1.1 to 10 mL	3 to 6

7.2.2.5 Allow the push-button to move up to the top stop position slowly and smoothly.

7.2.2.6 For air displacement pipetters, observe a wait of 1 s.

7.2.2.7 Withdraw the pipet or pipet tip smoothly by lifting straight up either from the center of the liquid surface in the vessel, or up the sidewall of the vessel.

NOTE 1—No further liquid contact of the pipet or pipet tip is allowed once the liquid interface is broken.

7.2.2.8 Wipe the pipet or pipet tip *only* if there are extraneous droplets. Contact with the orifice of the pipet or pipet tip,

especially with absorbent material, must be avoided, as large components of random or systematic error may be introduced.

7.2.3 *Delivery*—Place the pipet or pipet tip at an angle (10 to 45°, or as prescribed by the manufacturer) against the inside wall of the receiving vessel.

7.2.3.1 For two-component stroke systems, depress the push-button smoothly to the intermediate stop position. After a wait of 1 s, depress the push-button to the bottom stop position as the pipet or pipet tip end is removed from the sidewall by either a sliding action up the wall or a movement away from the wall (“touching off”).

7.2.3.2 For one-component stroke systems, depress the push-button smoothly to the bottom stop position as the pipet or pipet tip end is removed from the sidewall by either a sliding action up the wall, or a movement away from the wall.

7.2.3.3 Allow the push-button to move up to the top stop position.

7.3 Reverse Mode, General Format:

7.3.1 *Preparation*—Prepare in accordance with 7.2.1, forward mode.

7.3.2 *Aspiration*—Aspirate in accordance with 7.2.2, except that the push-button is depressed to the *bottom* stop position prior to pipet tip immersion.

7.3.3 *Delivery:*

7.3.3.1 Place the pipet or pipet tip at an angle (10 to 45°, or as prescribed by the manufacturer) against the inside wall of the receiving vessel.

7.3.3.2 Depress the push-button smoothly to the intermediate stop position.

7.3.3.3 After a 1-s wait, remove the pipet or pipet tip from the sidewall, in accordance with 7.2.3.

7.3.3.4 In the case of the pipet tip being reused, allow the push-button to remain in the intermediate stop position for subsequent immersion for the next pipetting cycle. In the case of the pipet tip to be changed, allow the push-button to return to the top stop position.

NOTE 2—Top and bottom stop positions, as described in the procedures above, are not meant to include auxiliary stroke positions (for example, for tip ejection).

7.4 Prerinsing (Forward Mode):

7.4.1 Prerinsing is the action of precoating the inside of the liquid contracting part(s) with a thin film of the same liquid to be pipetted. It is accomplished by duplicating the exact motion of a forward mode pipetting cycle, except that the liquid is dispensed back into the original vessel, or preferably discarded.

7.4.2 Prerinsing in the forward mode is advantageous when reusing (the same liquid and volume setting only) the pipet or pipet tip for subsequent immediate pipettings. Eliminating the dispensed amount from the first wetting from the sample group formed by subsequent wettings and thus the removal of its value from the calculation of a precision statistic for the group, will result in a more precise distribution.

7.4.3 Prerinsing may also be practiced when a removable pipet tip is to be used only once (for example, when pipetting different liquids), but the increase in time required to accommodate prerinsing each tip reserves this practice for pipetting different liquids which may be especially difficult to handle (for example, different patient sera). The need for prerinsing is

also related to the surface properties of the pipet tip as well as due to the physical characteristics of the liquid(s).

7.5 Positioning the Residual Volume (Reverse Mode)—Positioning the residual volume for the reverse mode is the functional equivalent of prerinsing for the forward mode. It is accomplished by duplicating the exact motion of a reverse mode pipetting cycle, except that the liquid is dispensed back into the original vessel, or preferably discarded, and the push-button kept at the intermediate stop position instead of being allowed to return to the top stop position, when reusing the pipet tip.

7.6 Disposable Pipet Tips—Discarded pipet tips contain liquid residues, particularly when used in the reverse mode. Suitable precautions should be taken with their disposal.

8. Operating Conditions

8.1 Dispensers with Valve(s)—The aspiration tube must be immersed in the reservoir for operation. When the system is filled (free of air bubbles, according to manufacturer’s instructions), the movement of the piston in one direction aspirates liquid. While moving in the opposite direction, the adjusted volume of liquid is dispensed, (see Fig. 5).

8.2 Dispensers Without Valve—When the system is filled (free of air bubbles, according to manufacturer’s instructions), the movement of the piston in one direction aspirates liquid. While moving in the opposite directions, the adjusted volume of liquid is dispensed, (see Fig. 6).

9. Operating Conditions for Dilutors

9.1 During operation the entire system except the end of the probe tube is filled with diluent. Any movement of the piston (V) in the direction (A) aspirates diluent. The diluent is aspirated as follows:

9.1.1 In the case of dilutors with valve(s), through the aspiration tube, (see Fig. 7), and

9.1.2 In the case of dilutors without valve, through the probe tube, (see Fig. 8).

9.2 Any movement of the piston (P) in the direction (A) aspirates sample liquid through the probe tube.

9.3 A movement of the pistons (V) and (P) in the direction (B) expels diluent and sample liquids in the adjusted ratio. Fig. 7 and Fig. 8 show dilutors with two separate pistons. Dilutors may also operate with one piston or with telescopic pistons. For the functioning of a dilutor it is irrelevant whether the

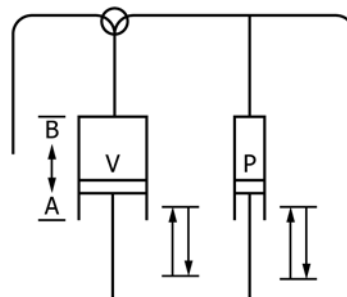


FIG. 6 Dispenser Without Valve

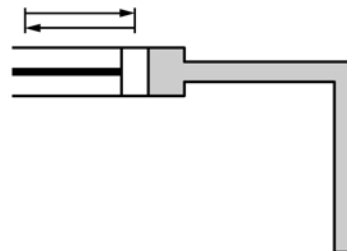


FIG. 7 Dilutor With Valve

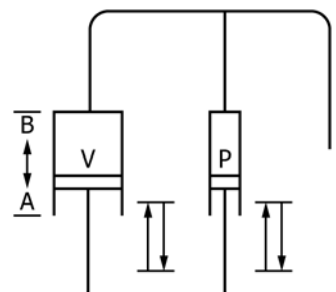


FIG. 8 Dilutor Without Valve

pistons operate in the same direction, and simultaneously, or in opposite directions at different times.

10. Operating Conditions for Displacement Burets

10.1 Burets with Valve(s)—The aspiration tube must be immersed in the reservoir for operation. When the system is filled (free of air bubbles, according to manufacturer’s instructions), the movement of the piston in one direction aspirates liquid. The movement of the piston in the opposite direction expels liquid, after which a reading can be taken, (see Fig. 9).

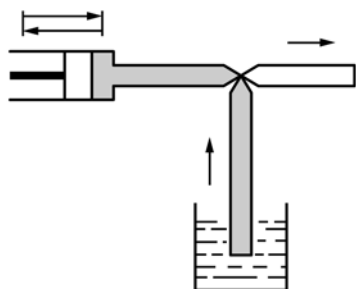


FIG. 5 Dispenser With Valve

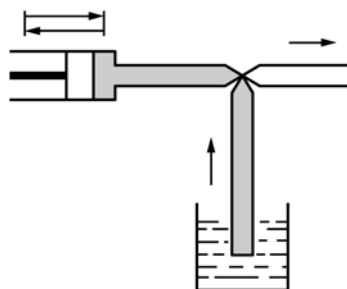


FIG. 9 Burette With Valve

10.2 *Burets Without Valve*—When the system is filled (free of air bubbles, according to manufacturer’s instructions), the movement of the piston in one direction aspirates liquid. The movement of the piston in the opposite direction expels liquid, after which a reading can be taken, (see Fig. 10).

11. Number of Tests and Retests

11.1 *Functional Test*—A functional test (for example, tests for leakage, broken parts, existence of air bubbles, contamination) shall be performed daily.

11.2 *Volumetric Tests:*

11.2.1 An appropriate single or replicate measurement test should also be performed following a change in the source of any removable parts of the delivery system (for example, as indicated by control or lot numbers of pipet tips, or change in dispensing cannulae).

11.2.2 A quick check four sample test measuring accuracy and roughly estimating precision should be performed at least monthly, or more frequently as indicated by the physical condition or extent of use of the apparatus.

11.2.3 A ten sample test measuring both accuracy and precision should be performed on all delivery systems upon introduction to service, following routine and other maintenance, and as otherwise necessary to provide a comprehensive evaluation on at least a quarterly basis.

12. Sample Size

12.1 For purposes of specifying or testing the volumetric performances of a single instrument by the manufacturer, supplier, or testing agent, the procedures specified in Section 13 shall be repeated at least 30 times.

12.2 For control purposes ten replicate measurements may be sufficient.

12.3 For quick checks of accuracy, four replicate measurements are sufficient.

13. Gravimetric Test Method

13.1 *Scope*—These test methods cover the testing of POVA under prescribed conditions.

13.2 *Summary of Method*—The general procedure is based upon the determination of the weighing result of water samples delivered by the instrument. The values are corrected for evaporation, then true mass and volume are calculated simultaneously, based upon the knowledge of the density of water at specific temperatures and corrections for air buoyancy (see ISO 4787).

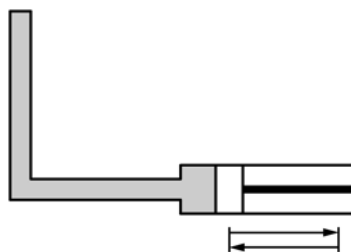


FIG. 10 Burette Without Valve

13.3 *Significance and Use*—These test methods are intended to provide uniform reference procedures that can be used by anyone to assess the errors of instruments. These test methods are recommended for use in the establishing performance claims, in quality control procedures during manufacture, as well as in control checks throughout the working life of an instrument.

13.4 *Apparatus:*

13.4.1 The resolution requirement of the weighing equipment shall be to one tenth of one percent of the water sample weight. The imprecision requirement of the weighing equipment is determined as the standard deviation of at least ten repeated weighings of a metal weight of a mass similar to the mass of the water sample. The minimum requirements for the balance are as shown in Table 1. Balances shall be calibrated and maintained at least annually, and re-calibrated after being moved. Balance calibration shall be checked at least daily. (See Test Method E898 for balance calibration and OIML R 111-1 or Specification E617 for weight requirements.)

13.4.2 *Weighing Vessel*, shall be such that the instrument can be operated according to the manufacturer’s instructions. The total volume of the weighing vessel shall be as small as practicable and preferably smaller than 50 times the volume to be tested. In the case of test volumes smaller than 100 µL, the weighing vessel shall be covered with a cap to avoid excessive errors due to the evaporation of water during weighing, unless conditions such as high ambient relative humidity make this unnecessary. The cap must not come into contact with the liquid.

13.4.2.1 The vessel and cover shall be made of nonporous material.

13.4.2.2 The opening shall be as small as possible. The top edge angle shall be such as not to affect the normal operation of the instrument under test.

13.4.3 *Thermometer*, used for measuring the ambient and water temperature shall show a maximum permissible error of + 0.1°C, for example, thermometer STL/0.1/–5/ + 25 in accordance with ISO 653, or thermometer EL/0.1/–5/ + 25 in accordance with ISO 655.

13.5 *Materials and Environment:*

13.5.1 Water shall be distilled and reasonably free of dissolved air.

13.5.2 *Ambient Test Conditions*—The instruments shall be tested under referenced ambient conditions. The ambient conditions for the tests shall be as follows:

13.5.2.1 The temperatures of the test environment, including the analytical equipment, material, test water, instrument to be evaluated (including removable parts) should be identical,

TABLE 1 Minimum Balance Requirements^A

Test Volume, µL	Sensitivity, mg	Imprecision (s), mg	Weight Class, OIML/ASTM
1 ≤ V ≤ 10	≤ 0.001	≤ 0.002	E ₂ /1
10 < V ≤ 100	≤ 0.01	≤ 0.02	E ₂ /1
100 < V ≤ 1000	≤ 0.1	≤ 0.1	E ₂ /1
1000 < V	≤ 0.1	≤ 0.2	F ₁ /1

^A See 13.4.1.

and as stable as possible ($+ 0.5^{\circ}\text{C}$) at least 2 h prior to and throughout the evaluation period.

13.5.2.2 The relative humidity should be maintained at 45 to 75 %, in order to reduce the evaporation rate and control the buildup of electrostatic potentials. In the immediate weighing area the relative humidity may be increased, but care should then be taken against condensation of water.

13.5.2.3 The balance area shall be reasonably free of vibration and air currents.

13.5.2.4 The ambient air shall be reasonably clean.

13.5.2.5 The lighting shall be of necessary intensity, and glare-free. Diffused light is preferred (direct sunlight must be avoided).

13.5.2.6 The working surface directly in front of the balance should be a dark color and glare-free.

13.5.2.7 The average barometric pressure in the test laboratory shall be known to $+ 25$ m bar.

13.6 Procedures:

13.6.1 *General*—Ensure that all equipment and materials including a sufficient number of removable parts are properly selected and conditioned, the desired volume is set (if applicable) and the electronic balance (if used) has had the warm-up time specified by the manufacturer.

13.6.2 *Pipetters*—Select the following test conditions: pipetting operating mode, option regarding prerinsing or not, whether to reuse or dispose of pipet tips, and a cycle time for procedure.

NOTE 3—The cycle time shall be consistent throughout a series of measurements.

13.6.2.1 Mount removable pipet tip.

13.6.2.2 Measure the temperature of the water to $\leq 0.1^{\circ}\text{C}$ and record it.

13.6.2.3 Place a small amount of water in the weighing vessel (between 2 and 30 sample amounts, or a minimum of 0.5 mL).

13.6.2.4 Place the cap on the weighing vessel, if necessary, and the weighing vessel on the balance pan.

13.6.2.5 While the balance is equilibrating the pipet tip may be prerinsed, and the sample aspirated, according to the operating mode selected.

13.6.2.6 Tare the weighing vessel and record the value, if necessary.

13.6.2.7 Note the time.

13.6.2.8 Deliver the sample according to the operating mode selected and replace the cap, if used.

13.6.2.9 Weigh the weighing vessel and record the time and weighing result.

13.6.2.10 If a series of measurements shall be carried out: repeat 13.6.2.5 through 13.6.2.9 until the desired number of measurements is achieved.

13.6.2.11 Perform a control blank for estimation of evaporation by repeating 13.6.2.6 through 13.6.2.9 exactly as in a normal sample weighing but without actually delivering any liquid to the weighing vessel.

NOTE 4—It is suggested that this evaporation control check be performed at the beginning and end of each series of measurements, and between each group of 10 samples in larger series.

13.6.2.12 Measure the temperature of the water and record a second time.

13.6.2.13 The procedure in 13.6.2.5 through 13.6.2.9 should be performed as quickly as practicable but without compromise to the integrity of the liquid delivery, precision of the technique of the operator, or time intervals.

13.6.3 Dispensers:

13.6.3.1 Measure the temperature of the water to $\leq 0.1^{\circ}\text{C}$ and record.

13.6.3.2 Connect or fill the reservoir and prime the dispenser according to the manufacturer's instructions before equilibrating it for normal use.

13.6.3.3 Place a small amount of water in the weighing vessel (between 2 and 30 sample amounts, or a minimum of 0.5 mL).

13.6.3.4 Place the cap on the weighing vessel, if necessary, and the weighing vessel on the balance pan. Equilibrate the dispenser to normal operation by actuating at least one complete cycle and discarding the first dispensing.

13.6.3.5 Tare the weighing vessel and record the value, if necessary.

13.6.3.6 Note the time.

13.6.3.7 Actuate a complete dispensing cycle to deliver the sample into the weighing vessel and replace the cap, if used.

13.6.3.8 Weigh the weighing vessel and record the time and weighing result.

13.6.3.9 If a series of measurements shall be carried out, the procedure in 13.6.3.5 – 13.6.3.8 are to be repeated until the desired number of measurements is achieved.

13.6.3.10 Perform a control blank for estimation of evaporation by repeating 13.6.3.5 – 13.6.3.8 exactly as in a normal sample weighing but without actually delivering any liquid to the weighing vessel.

NOTE 5—It is suggested that this evaporation control check be performed at the beginning and end of each series of measurements, and between each group of 10 samples in larger series.

13.6.3.11 Measure the temperature of the water and record a second time.

13.6.3.12 The procedure in 13.6.3.5 – 13.6.3.10 should be performed as quickly as possible, but without compromise to the integrity of the liquid delivery, precision of technique of the operator, or time intervals.

13.6.4 Dilutors:

13.6.4.1 In the case of dilutors, parameters to be tested can be as follows: the sample volume, the diluent volume, and the total volume or the dilution ratio, or both.

13.6.4.2 Dilutors can be tested gravimetrically only if there is no interdependence between the sample and diluent volume(s). In this case follow the procedures described for dispensers or pipetters, as appropriate.

13.6.5 *Displacement Burets*—When the buret is filled (free of air bubbles, according to manufacturer's instruction(s)), deliver an amount of liquid which is approximately as large as the volume to be tested into a weighing vessel. Compare the volume(s) actually delivered with the indication(s) of the buret and use the resulting deviation(s) for the calculation(s).

13.7 Calculations:

13.7.1 *General*—The mean volume at the test temperature (\bar{V}_t) shall be calculated from the mean weighing result (\bar{W}) by addition of the mean evaporation (\bar{e}), and conversion of the sum by an appropriate factor incorporating density and buoyancy corrections for water when weighed in air, at the test temperature and pressure, at standard humidity (see Table 2). This calculation need only be performed once in order to calculate the performance statistics.

13.7.2 *Individual Weighings*—The individual weighing result (W_i) in air shall be calculated by subtracting the tare reading from the sample reading.

13.7.3 *Evaporation*—The evaporation (e_i) shall be estimated by subtracting the appropriate balance reading after the control blanks from the reading before each blank (these values should be positive). The mean evaporation (e) shall be calculated as follows from the number of determinations (n_e):

$$e = \sum e_i / n_e \quad (2)$$

13.7.4 *Test Temperature*—The test temperature (t) shall be the average of the two measurements of water temperature, rounded to the nearest 0.5°C.

13.7.5 *Mean Weighing Result*—The mean weighing result (\bar{W}) shall be calculated from the n individual weighings (W_i):

$$\bar{W} = \sum W_i / n \quad (3)$$

13.7.6 *Mean Volume*—The mean volume of the liquid samples (V_t) shall be calculated as follows from the mean weighing result (W) as follows:

$$\bar{V}_t = (W + e) \cdot Z \quad (4)$$

where:

- \bar{e} = mean evaporation loss (mg), and
- Z = conversion factor ($\mu\text{L}/\text{mg}$) incorporating the density of water when buoyed in air, at the test temperature and pressure.

Values of Z for water at various test temperatures are listed in Table 2.

13.7.7 *Inaccuracy of the Mean*—The accuracy of the mean (E_t %) of the apparatus at the test temperature (t) shall be calculated from the nominal volume of the apparatus (V_o) and the calculated mean volume (V_t) as

$$E_t \% = V_t - V_o / V_o \times 100 \quad (5)$$

13.7.8 *Imprecision*—The imprecision, expressed as a percentage (coefficient of variation) shall be calculated from the distribution of individual weighing results (W_i) about their mean (W), which is then corrected for error due to evaporation, as

$$CV\% = s \cdot 100 / W + e \quad (6)$$

where:

- e = mean evaporation
- s = $\frac{\sum (W_i - \bar{W})^2}{n - 1}$
- n = 30 or 10, and
- CV = coefficient of variation.

This statistic measures the total sources of imprecision, including that of the operator, mode of operation and test method, and is thus best used for comparison purposes.

NOTE 6—Volume may be calculated for each weighing result if data processing equipment is available.

13.8 *Precision and Bias:*

13.8.1 *Analytical Error*—The tolerances permitted in this test method for parameters involved in the calculation of V_t (see below) are as follows:

Parameter	Maximum Deviation	Maximum Volume Deviation
water temperature	±0.25°C	0.005 %
air pressure	±27 m bar	0.003 %
air temperature	±2.5°C	0.001 %
relative humidity	±25, - 5 % r.h.	0.0003 %
		Total = 0.01 %

13.8.2 *Hypothesis Test (Bias):*

13.8.2.1 If the critical value of the test result exceeds the values listed below, the instrument evaluated is considered significantly acceptable or rejectable at the listed confidence levels.

13.8.2.2 If the critical value is smaller than the indicated value at the confidence level required, the instrument should be

TABLE 2 Conversion Factor Values of % ($\mu\text{L}/\text{mg}$), As A Function of Temperature and Pressure, for Distilled Water

Temperature, °C	Air pressure, kPa					
	800	853	907	960	1013	1067
15	1.0016	1.0018	1.0019	1.0019	1.0020	1.0020
15.5	1.0018	1.0019	1.0019	1.0020	1.0020	1.0021
16	1.0019	1.0020	1.0020	1.0021	1.0021	1.0022
16.5	1.0020	1.0020	1.0021	1.0022	1.0022	1.0023
17	1.0021	1.0021	1.0022	1.0022	1.0023	1.0023
17.5	1.0022	1.0022	1.0023	1.0023	1.0024	1.0024
18	1.0022	1.0023	1.0024	1.0024	1.0025	1.0025
18.5	1.0023	1.0024	1.0025	1.0025	1.0026	1.0026
19	1.0024	1.0025	1.0025	1.0026	1.0027	1.0027
19.5	1.0025	1.0026	1.0026	1.0027	1.0028	1.0028
20	1.0026	1.0027	1.0027	1.0028	1.0029	1.0029
20.5	1.0027	1.0028	1.0028	1.0029	1.0030	1.0030
21	1.0028	1.0029	1.0030	1.0030	1.0031	1.0031
21.5	1.0030	1.0030	1.0031	1.0031	1.0032	1.0032
22	1.0031	1.0031	1.0032	1.0032	1.0033	1.0033
22.5	1.0032	1.0032	1.0033	1.0033	1.0034	1.0035
23	1.0033	1.0033	1.0034	1.0035	1.0035	1.0036
23.5	1.0034	1.0035	1.0035	1.0036	1.0036	1.0037
24	1.0035	1.0036	1.0036	1.0037	1.0038	1.0038
24.5	1.0037	1.0037	1.0038	1.0038	1.0039	1.0039
25	1.0038	1.0038	1.0039	1.0039	1.0040	1.0041
25.5	1.0039	1.0040	1.0040	1.0041	1.0041	1.0042
26	1.0040	1.0041	1.0042	1.0042	1.0043	1.0043
26.5	1.0042	1.0042	1.0043	1.0043	1.0044	1.0045
27	1.0043	1.0044	1.0044	1.0045	1.0045	1.0046
27.5	1.0044	1.0045	1.0046	1.0046	1.0047	1.0047
28	1.0046	1.0046	1.0047	1.0048	1.0048	1.0049
28.5	1.0047	1.0048	1.0048	1.0049	1.0050	1.0050
29	1.0048	1.0049	1.0050	1.0050	1.0051	1.0052
29.5	1.0050	1.0051	1.0051	1.0052	1.0052	1.0053
30	1.0052	1.0052	1.0053	1.0053	1.0054	1.0055

reevaluated after giving careful consideration to the test conditions, method requirements, selection of operating mode, removable parts and competence of the operator, before a final decision is made.

Confidence Level for (+) Acceptance/ (-) Rejection	Critical Value (Fraction of Tests, CV % value)	
	n = 30	n = 10
50 %	0	0
90 %	±0.24	±0.43
95 %	±0.31	±0.57
99 %	±0.45	±0.87
99.9 %	±0.62	±1.31

Critical values for other confidence levels can be calculated as follows:

$$\pm (t/\sqrt{n}) CV\% \quad (7)$$

where:

t = critical value of Student's for one-tailed test at the significance value desired (commonly available from statistical tables) and

n = 30 or 10.

$$\text{Critical Value} = \frac{d\%}{CV_T\%} = \frac{E_c\% - E_T\%}{CV_T\%} \quad (8)$$

where:

$E_T\%$ = inaccuracy of the mean, %,

$E_c\%$ = claimed inaccuracy of the mean, %, and

$CV_T\%$ = imprecision, %, (see Figs. 11 and 12).

13.8.3 Hypothesis Test (Precision)—If the ratio of the test

result value to the specified tolerance for the precision ($CV_c\%$) exceeds the limits listed below, the combined precisions of the instrument, operator and test method are considered significantly rejectable at the confidence levels listed below. The figures are based upon the assumption that the specification requires 30 samples. Figs. 11 and 12.

Confidence Level for Acceptance/ Rejection	Critical Value of Ratio			
	Acceptance/Rejection n = 30		Acceptance/Rejection n = 10	
50 %	1.00	1.00	1.00	1.00
90 %	0.73	1.37	0.67	1.49
95 %	0.69	1.46	0.62	1.61
98 %	0.64	1.57	0.57	1.76
99 %	0.61	1.65	0.53	1.87

Critical values for other confidence levels can be calculated as $-\rightarrow\sqrt{1/F}$ for acceptance or $-\rightarrow\sqrt{F}$ for rejection.

where:


F = critical value for F for one-tailed test (see accuracy test regarding reevaluation considerations).

14. Product Marking

14.1 The product information shall include all necessary information for use, maintenance, cleaning (sterilizing) of the instrument in question, and all conditions for which performance is specified.


15. Keywords

15.1 dilutor; displacement buret; dispenser; pipette; POVA

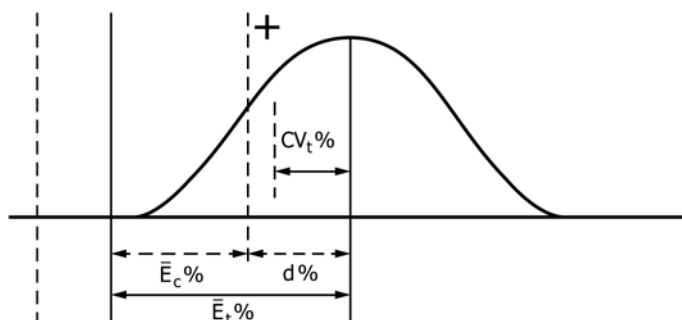

NOTE 1—Critical value is negative.

FIG. 11 Hypothesis Test for Accuracy: Rejection Test

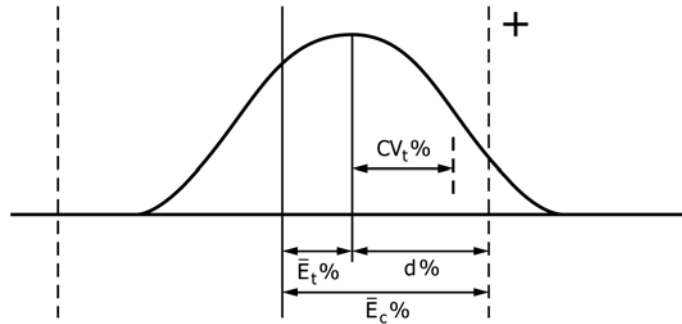

NOTE 1—Critical value is positive.

FIG. 12 Hypothesis Test for Accuracy: Acceptance Test

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; http://www.copyright.com/