



# Standard Test Method for Measuring Fast-Neutron Reaction Rates by Radioactivation of Niobium<sup>1</sup>

This standard is issued under the fixed designation E1297; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This test method describes procedures for measuring reaction rates by the activation reaction  $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$ .

1.2 This activation reaction is useful for monitoring neutrons with energies above approximately 0.5 MeV and for irradiation times up to about 30 years.

1.3 With suitable techniques, fast-neutron reaction rates for neutrons with energy distribution similar to fission neutrons can be determined in fast-neutron fluences above about  $10^{16}\text{ cm}^{-2}$ . In the presence of high thermal-neutron fluence rates ( $>10^{12}\text{ cm}^{-2}\cdot\text{s}^{-1}$ ), the transmutation of  $^{93\text{m}}\text{Nb}$  due to neutron capture should be investigated. In the presence of high-energy neutron spectra such as are associated with fusion and spallation sources, the transmutation of  $^{93\text{m}}\text{Nb}$  by reactions such as  $(n,2n)$  may occur and should be investigated.

1.4 Procedures for other fast-neutron monitors are referenced in Practice E261.

1.5 Fast-neutron fluence rates can be determined from the reaction rates provided that the appropriate cross section information is available to meet the accuracy requirements.

1.6 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.7 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

## 2. Referenced Documents

2.1 *ASTM Standards:*<sup>2</sup>

D1193 Specification for Reagent Water

<sup>1</sup> This test method is under the jurisdiction of ASTM Committee E10 on Nuclear Technology and Applications and is the direct responsibility of Subcommittee E10.05 on Nuclear Radiation Metrology.

Current edition approved Jan. 1, 2013. Published January 2013. Originally approved in 1989. Last previous edition approved in 2008 as E1297 – 08. DOI: 10.1520/E1297-08R13.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

E170 Terminology Relating to Radiation Measurements and Dosimetry

E181 Test Methods for Detector Calibration and Analysis of Radionuclides

E185 Practice for Design of Surveillance Programs for Light-Water Moderated Nuclear Power Reactor Vessels

E261 Practice for Determining Neutron Fluence, Fluence Rate, and Spectra by Radioactivation Techniques

E262 Test Method for Determining Thermal Neutron Reaction Rates and Thermal Neutron Fluence Rates by Radioactivation Techniques

E844 Guide for Sensor Set Design and Irradiation for Reactor Surveillance, E 706 (IIC)

E944 Guide for Application of Neutron Spectrum Adjustment Methods in Reactor Surveillance, E 706 (IIA)

E1005 Test Method for Application and Analysis of Radiometric Monitors for Reactor Vessel Surveillance, E 706 (IIIA)

E1006 Practice for Analysis and Interpretation of Physics Dosimetry Results from Test Reactor Experiments

E1018 Guide for Application of ASTM Evaluated Cross Section Data File, Matrix E706 (IIB)

## 3. Terminology

3.1 *Definitions*—The definitions stated in Terminology E170 are applicable to this test method.

## 4. Summary of Test Method

4.1 High purity niobium is irradiated in a neutron field producing radioactive  $^{93\text{m}}\text{Nb}$  from the  $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$  reaction. The metastable state decays to the ground state by the virtual emission of 30 keV gamma rays that are all internally converted giving rise to the actual emission of orbital electrons followed by X rays.

4.2 Sources of the irradiated niobium are prepared for X ray or liquid scintillation counting.

4.3 The X rays emitted as a result of the decay of  $^{93\text{m}}\text{Nb}$  are counted, and the reaction rate, as defined in Practice E261, is calculated from the decay rate and irradiation conditions.

4.4 The neutron fluence rate may then be calculated from the appropriate spectral-weighted neutron activation cross section as defined by Practice E261.

## 5. Significance and Use

5.1 Refer to Practice E261 for a general discussion of the determination of decay rates, reaction rates, and neutron fluence rates with threshold detectors (1-29).<sup>3</sup> Refer to Practice E1006, Practice E185 and Guide E1018 for the use and application of results obtained by this test method.(30-32)

5.2 The half-life of <sup>93m</sup>Nb is 5730 ± 220 days (33) and has a K X-ray emission probability of 0.1099 ± 0.0025 per decay (33). The K<sub>α</sub> and K<sub>β</sub> X-rays of niobium are at 16.5213–16.152 and 18.618–18.953 keV, respectively. The recommended <sup>93</sup>Nb (n,n')<sup>93m</sup>Nb cross section comes from the IRDF-90 cross section compendium (34), was drawn from the RRDF-98 cross section evaluations (35) and is shown in Fig. 1.

5.3 Chemical dissolution of the irradiated niobium to produce very low mass-per-unit area sources is an effective way to obtain consistent results. The direct counting of foils or wires can produce satisfactory results provided appropriate methods and interpretations are employed. It is possible to use liquid scintillation methods to measure the niobium activity provided the radioactive material can be kept uniformly in solution and appropriate corrections can be made for interfering activities.

5.4 The measured reaction rates can be used to correlate neutron exposures, provide comparison with calculated reaction rates, and determine neutron fluences. Reaction rates can be determined with greater accuracy than fluence rates because of the current uncertainty in the cross section versus energy shape.

5.5 The <sup>93</sup>Nb(n,n')<sup>93m</sup>Nb reaction has the desirable properties of monitoring neutron exposures related to neutron damage of nuclear facility structural components. It has an energy response range corresponding to the damage function of steel

<sup>3</sup> The boldface numbers in parentheses refer to the list of references at the end of this test method.

and has a half-life sufficiently long to allow its use in very long exposures (up to about 40 years). Monitoring long exposures is useful in determining the long-term integrity of nuclear facility components.

## 6. Interferences

6.1 Pure niobium in the forms of foil and wire is available and easily handled as a metal. When thin niobium is irradiated, it may become brittle and fragile, thus requiring careful handling or encapsulation to prevent damage or loss of the niobium. Refer to Guide E844 for the selection, irradiation, and quality control of neutron dosimeters.

6.2 There are some distinct advantages and limitations to three measurement techniques identified in 5.3. It is the responsibility of the user to evaluate these and determine the optimum technique for the situation.

6.2.1 Low mass source X-ray spectrometry advantages include sufficient energy resolution to eliminate other X-ray emissions, stable long life sources, reduced interference fluorescence due to other radionuclides, small and precise background corrections, and minimal X-ray source self-absorption corrections. Limitations are low counting efficiency, complex source preparation, and use of hazardous chemicals.

6.2.2 Direct X-ray spectrometry of metal (foil or wire) sources has the advantages of simple source preparation, stable long life sources, sufficient energy resolution to eliminate other X-ray emissions, small and precise background corrections, and no use of hazardous chemicals. Limitations are low counting efficiency, large X-ray source self-absorption corrections, larger corrections for interference fluorescence due to the other radionuclides, and source geometry control.

6.2.3 Liquid scintillation counting advantages include very high detection efficiency, reproducible source preparation, and no source self absorption corrections. Limitations include specialized calibration techniques to reduce interference from

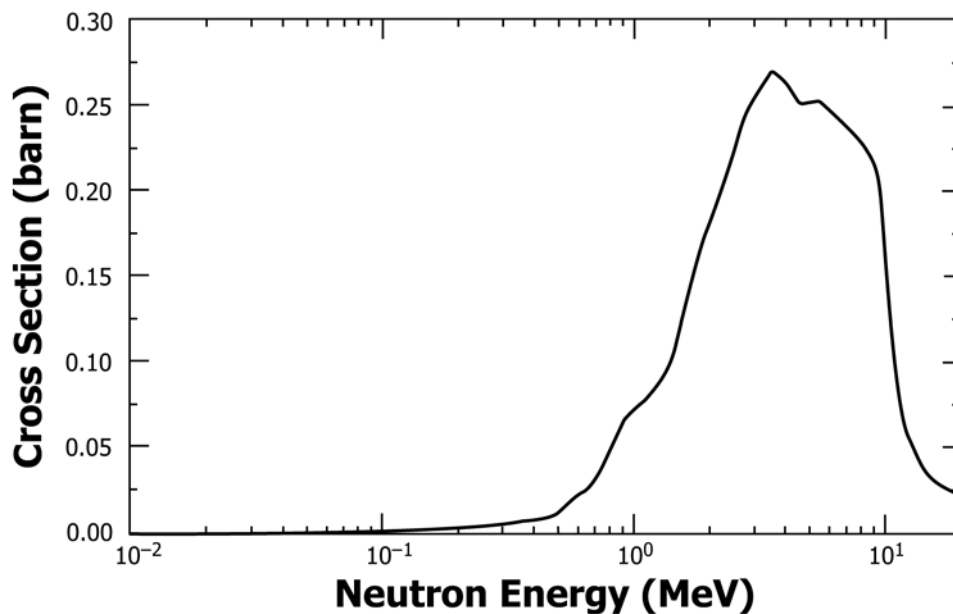


FIG. 1 IRDF-90 Cross Section Versus Energy for the <sup>93</sup>Nb(n,n')<sup>93m</sup>Nb Reaction

other radionuclides, limited source stability, use of hazardous chemicals, and disposal of hazardous chemical waste.

## 7. Apparatus

7.1 *X-ray Spectrometer*, using a Si(Li) detector or a Ge detector and a multichannel pulse-height analyzer. For more information, refer to Test Methods [E181](#) and [E1005](#).

7.2 *Precision Balance*, able to achieve the required accuracy.

7.3 *Beakers*, 50 mL polyethylene; pycnometer (weighing bottle), 50 mL polyethylene; volumetric pipets, 10  $\mu$ L to 5 mL.

7.4 *Gamma Ray Spectrometer*, using a Ge detector and a multichannel pulse-height analyzer. Refer to Test Method [E181](#).

7.5 *Liquid Scintillation Counter*.

## 8. Reagents and Materials

8.1 *Purity of Reagents*—Reagent grade chemicals shall be used in all tests. Unless otherwise indicated, it is intended that all reagents conform to the specifications of the Committee on Analytical Reagents of the American Chemical Society, where such specifications are available.<sup>4</sup> Other grades may be used, provided it is first ascertained that the reagent is of sufficiently high purity to permit its use without lessening the accuracy of the determination.

8.2 *Purity of Water*—Unless otherwise indicated, any water used shall be understood to mean reagent water as defined by Type I of Specification [D1193](#).

8.3 *Hydrofluoric Acid*—Concentrated (32*M*) hydrofluoric acid (HF).

8.4 *Nitric Acid*—Concentrated (16*M*) nitric acid (HNO<sub>3</sub>).

8.5 *Niobium Metal*—The purity of the niobium is important in that no impurities (such as tantalum) should be present to produce long-lived radionuclides that interfere with the <sup>93m</sup>Nb activity determination. To avoid problems from tantalum, the niobium should have the lowest tantalum content possible. Niobium metal in the form of foil and wire with tantalum content of about 5 ppm (parts per million) or less is obtainable and can be used under most conditions. The niobium material should be tested for interfering radioactivity by neutron activation techniques.

8.6 *Encapsulation Material*—The encapsulation material (such as quartz, stainless steel, aluminum, etc.) should be selected to prevent corrosion of the niobium during irradiation and to be compatible with the irradiation environment and post-irradiation handling. If thermal and epithermal neutron filters or shrouds are used, these materials (such as cadmium, tantalum, gadolinium, etc.) must also be compatible with the encapsulation and irradiation environment.

8.7 *Analytical Paper*—Analytical grade filter paper of uniform thickness (about 0.076 cm) and density (about 8 mg cm<sup>-2</sup>). The paper can be cut or obtained precut to the desired size (usually between 0.5 and 1.5 cm diameter) that is compatible with the activity concentration of the solution and the counting conditions. The paper should be able to absorb as much liquid as is necessary and not decompose from the acid. TFE-fluorocarbon rings with an inside diameter matching the outside diameter of the filter paper disks so they fit together with light contact.

8.8 *Support and Cover Materials*—Thin plastic film and plastic tape materials are useful to support and cover the filter paper sources. They should be strong enough to contain the sources and thin enough to minimize attenuation of the X rays.

8.9 *Source Holder*—A source holder must be used to accurately and reproducibly position the sources for the counting geometry to be used. The source holder should be constructed of low density materials such as aluminum or plastic.

8.10 *Liquid Scintillation Materials*—Vials, emulsion scintillant (xylene-based), chelating agent (di-2-ethylhexyl phosphoric acid).

## 9. Procedure

9.1 Determine the size and shape of the niobium sample being irradiated. Consider the convenience in handling and available irradiation space. Ensure that sufficient <sup>93m</sup>Nb activity will be produced to permit accurate radioassay. Typically, samples of 0.2 to 20 mg of niobium may be used, but a preliminary calculation of the expected production of <sup>93m</sup>Nb will aid in selecting the appropriate mass for the irradiation.

9.2 Accurately weigh the niobium sample being irradiated.

9.3 Encapsulate the niobium sample so that it can be retrieved and identified following the irradiation. Record the sample identification, sample weight, and exact details of the encapsulation. Shroud the niobium with neutron filter material if necessary. If the thermal-to-fast neutron fluence rate ratio is high (greater than 5) or the tantalum impurity is high (greater than 10 ppm), use neutron filter materials, if possible.

9.4 Irradiate the niobium samples. Keep an accurate record of the irradiation history including neutron level versus time, starting and ending time of the irradiation, and the periods when the neutron level is zero. Record the spatial position of the sample in the irradiation facility.

9.5 After the irradiation, retrieve and identify the irradiated sample. Take necessary precautions to avoid personnel overexposure to radiation and the spread of radioactive contamination.

9.6 A waiting time between the end of irradiation and the start of counting may be necessary to allow <sup>92m</sup>Nb or <sup>95</sup>Nb, or both, to decay to an insignificant level. Check the samples for activity from contamination by other materials or reactions (see Test Method [E262](#)) and for any material adhering to the sample. Check the weight of the sample. If necessary, clean and reweigh the sample.

9.7 *X-Ray Source Preparation and Counting*:

<sup>4</sup> "Reagent Chemicals, American Chemical Society Specifications," Am. Chemical Soc., Washington, DC. For suggestions on the testing of reagents not listed by the American Chemical Society, see "Reagent Chemicals and Standards," by Joseph Rosin, D. Van Nostrand Co., Inc., New York, NY, and the "United States Pharmacopeia."

9.7.1 If the metal is being dissolved and reduced to a low mass-per-unit area source, dissolve the sample by placing it in a preweighed 50 mL polyethylene or TFE-fluorocarbon (non-wettable) beaker and adding enough concentrated hydrofluoric acid to cover the sample (usually about 1 to 10 mL of HF). Add concentrated nitric acid dropwise to start dissolution; as dissolution slows, add additional drops to maintain a controlled slow rate of dissolution until the entire sample dissolves. After dissolution is complete, bring the final volume of solution to the desired amount by adding distilled water. Weigh the solution in the beaker if mass aliquoting is used. A preweighed polyethylene pycnometer (weighing bottle) is recommended for mass aliquoting. The ratio of the niobium mass to the solution mass determines the concentration of niobium in the solution. When transferring the solution from one container to another, ensure that all of the solution is transferred by using multiple rinses. Use accurately calibrated pipets if volumetric aliquoting is performed.

9.7.2 Deposit the desired amount of the solution on a filter paper disk surrounded by a TFE-fluorocarbon ring to produce a counting source. Deposit the solution on the paper drop-by-drop so the paper does not become saturated but is uniformly wetted. The deposits are allowed to dry by evaporation of the solvent. Gently remove the paper disk from the TFE-fluorocarbon ring. Seal the sources between thin layers of plastic or plastic tape to contain the niobium. Mount the sources on the source holder for the counting geometry being used. Determine and record the amount of niobium in each source.

9.7.3 Count the prepared sources using an X-ray spectrometer with either an Si(Li) or a Ge detector with a beryllium window and designed to count X rays in the energy range between about 5 and 50 keV. Refer to Test Methods E181 and Practice E261. It is assumed that the persons doing the counting are knowledgeable in the operation and use of the counting apparatus and the handling and counting of X-ray sources.

9.7.4 The  $^{93\text{m}}\text{Nb}$  activity can be determined from the K X-ray emission rates by direct comparison to a certified standard of  $^{93\text{m}}\text{Nb}$  prepared and counted under the same conditions. Alternatively, the detection efficiency for the spectrometer system may be determined from other standardized K X-ray sources and applied to the counting of the unknown sources as described in Test Methods E181 and Ref (8).

9.7.5 If the prepared sources contain significant and variable amounts of niobium relative to each other or to the standard source, correction for self-attenuation may be necessary. These corrections can be determined as described in Test Methods E181. The accuracy of these corrections will depend on the uniformity of the distribution of the niobium in the sources. If possible, sources with less than  $1 \text{ mg/cm}^2$  of niobium should be prepared for counting to minimize the self-attenuation of the sources.

### 9.8 Comparison Counting:

9.8.1 If direct counting of metal niobium foils or wires is being done by comparison with appropriate standard sources of  $^{93\text{m}}\text{Nb}$  in the same form and geometry as the unknown sources, or by comparison with certified standards and with appropriate

corrections made for geometry differences, all of the factors that may influence the results must be appropriately controlled. In this approach, the  $^{93\text{m}}\text{Nb}$  emission rate may be compared to that of a fluence standard to produce a fluence relative to that of the standard and the neutron field in which it was irradiated. Fluence standards in the same form as the foils or wires are produced in standardized neutron fields. See Practice E261 for more information.

9.8.2 If foils are counted and compared to standard  $^{93\text{m}}\text{Nb}$  sources of different form and geometry, corrections for self attenuation and geometry are necessary. These corrections may be determined as described in Test Methods E181. The geometry corrections are minimized if the source-to-detector spacing is large. The geometry correction to account for a disk source related to a point source will be less than 2 % if the ratio of the disk radius to the source-to-detector distance is less than 0.2 and the ratio of the detector radius to the source-to-detector distance is less than 0.4. The X-ray attenuation correction for a 0.1 mm thick, 0.63 cm diameter niobium metal foil is about a factor of 1.9. Counting methods are described in 9.7.3.

9.9 When the fluorescence effect of  $^{182}\text{Ta}$  or other activity is not negligible in a niobium neutron monitor source, correction must be made. This correction is determined for the source geometry and niobium quantity being used by experimentally measuring the K X-ray fluorescence rate-per-unit  $^{182}\text{Ta}$  or other activity as a function of niobium mass. The amount of  $^{182}\text{Ta}$  or other activity in the sample is measured by gamma-ray spectrometry (see Test Methods E181), and the correction is determined from the results. If the  $^{182}\text{Ta}$  activity is less than 2 % of the  $^{93\text{m}}\text{Nb}$  activity in a 0.1 mm thick niobium foil, the correction of  $^{182}\text{Ta}$  induced fluorescence will be less than about 5 %. The correction is less for lighter foils and greater for heavier foils.

### 9.10 Liquid Scintillation Counting:

9.10.1 If liquid scintillation counting of the irradiated niobium is being used to determine the  $^{93\text{m}}\text{Nb}$  activity, the niobium must be dissolved (see 9.7.1) and an accurate amount of the niobium placed in the liquid scintillant. Place an accurate and reproducible amount of liquid scintillant, chelating agent, and niobium solution in a standard scintillation vial to form a “cocktail” counting source. In this approach, the  $^{93\text{m}}\text{Nb}$  activity is determined by comparing the liquid scintillation counting rates of an unknown source and a known source or by using the detection efficiency of the counter. Make corrections for the chemical interference changes in the process of light production (quenching).

9.10.2 Prepare the counting source by placing the xylene-based emulsion scintillant<sup>5</sup> along with 10 volume % of chelating agent (di-2-ethylhexyl phosphoric acid, HDEHP) into a standard liquid scintillation counting vial. Add the dissolved niobium solution to the mixture and mix vigorously. This solution will remain in a stable form for about one week.

<sup>5</sup> The sole source of supply of the apparatus known to the committee at this time is Intsa Gel, available from Packard Instrument Co., One State St., Meriden, CT 06450. If you are aware of alternative suppliers, please provide this information to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee,<sup>1</sup> which you may attend.

Keep the amounts of chemicals in all sources (blank, unknown, and known) as constant as possible to minimize quenching differences.

9.10.3 Count the sources as soon as possible following preparation and after temperature equilibrium is established since they are stable only for about one week. Count the sources, blanks, and standards in the same manner and correct them for instrument background. Differences in the quenching can be monitored using the “external source” technique.

9.10.4 If interfering radionuclides are present in the source, the responses to these must be determined and corrections made. Counting in optimized energy windows can be used in conjunction with the responses of the interfering radionuclides to obtain the  $^{93\text{m}}\text{Nb}$  activity. It is assumed that the persons doing the counting are knowledgeable in the operation and use of the counting apparatus, the handling and counting of liquid scintillation sources, and the reduction of liquid scintillation counting data.

## 10. Calculation

10.1 Calculate the reaction rate,  $R_s$ , as follows, assuming the irradiation was at a constant neutron level and there were no interruptions:

$$R_s = \frac{A}{N_o (1 - e^{-\lambda t_i}) (1 - e^{-\lambda t_w})}$$

where:

$A$  = number of  $^{93\text{m}}\text{Nb}$  disintegrations,  $\text{s}^{-1}$ , measured during the counting period and corrected for all interferences,

$N_o$  = number of  $^{93}\text{Nb}$  atoms in the sample,

$\lambda$  = disintegration constant for  $^{93\text{m}}\text{Nb} = 1.40009 \times 10^{-9} \text{ s}^{-1}$ ,

$t_i$  = irradiation time duration, s, and

$t_w$  = elapsed time between the end of irradiation and counting, s.

NOTE 1—If the irradiation is not at a constant neutron level or if the irradiation duration approaches the recommended maximum, corrections will be necessary. Refer to Practice E261 for procedures to make these corrections.

10.2 Refer to Practice E261 and Practice E944 for procedures to determine fast-neutron fluence rate and fluence.

## 11. Report

11.1 Practice E261 describes how data should be reported.

## 12. Precision and Bias

NOTE 2—Measurement uncertainty is described by a precision and bias statement in this standard. Another acceptable approach is to use Type A and B uncertainty components, (34 and 36). This Type A/B uncertainty specification is now used in International Organization for Standardization (ISO) standards and this approach can be expected to play a more prominent role in future uncertainty analyses.

12.1 Disintegration rates of  $^{93\text{m}}\text{Nb}$  from niobium neutron dosimeters can be determined with a bias of  $\pm 2\%$  (1S %) and with a precision of  $\pm 1\%$  (1S %) by use of a  $^{93\text{m}}\text{Nb}$  reference standard. By using a detector calibrated for counting efficiency and the K X-ray emission probability, the disintegration rate can be determined with a bias of  $\pm 3\%$  (1S %) and with a precision of  $\pm 1\%$  (1S %).

12.2 The  $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$  reaction rate can be determined with approximately the same bias and precision as the disintegration rate if the irradiation history is well known.

## 13. Keywords

13.1 activation; activation reaction; cross section; dosimetry; fast neutron monitor; neutron dosimeter; neutron metrology; niobium; pressure vessel surveillance; reaction rate; reaction rate monitor

## REFERENCES

- (1) Hegedus, F., Swiss Report EIR-Bericht Number 195, 1971.
- (2) Lloret, R., *First ASTM-Euratom Symposium on Reactor Dosimetry*, Petten 1975, EUR 5667 E/F, Part 1, p. 747.
- (3) Hegedus, F., Swiss Report EIR-Bericht Number 195, 1971, p. 757.
- (4) Taylor, W. H., *Second ASTM-Euratom Symposium on Reactor Dosimetry*, Palo Alto 1977, NUREG/CP-0004, Vol 2, p. 831.
- (5) Tourwe, H., and Maene N., *Third ASTM-Euratom Symposium on Reactor Dosimetry*, Ispra 1979, EUR 6813, EN-FR, p. 1245.
- (6) Tourwe, H., Taylor, W. H., Reher, D., Vaninbroux, R., Lloret, R., Noltehnus, J. H., Wille, P., and Schweighofer, R., *Fourth ASTM-Euratom Symposium on Reactor Dosimetry*, Gaithersburg 1982, NUREG/CP-0029, p. 401.
- (7) Alberts, W. G., Hollnagel, R., Knauf, K., Matzke, M., and Pessara, W., *Fourth ASTM-Euratom Symposium on Reactor Dosimetry*, Gaithersburg 1982, NUREG/CP-0029, p. 433.
- (8) Hegedus, F., *Fifth ASTM-Euratom Symposium on Reactor Dosimetry*, Geesthacht 1984, “Reactor Dosimetry,” Vol 1, p. 381.
- (9) Gehrke, R. J., Rogers, J. W., and Baker, J. D., *Fifth ASTM-Euratom Symposium on Reactor Dosimetry*, Geesthacht 1984, “Reactor Dosimetry,” Vol 1, p. 391.
- (10) Bars, B., and Karnani, H., *Fifth ASTM-Euratom Symposium on Reactor Dosimetry*, Geesthacht 1984, “Reactor Dosimetry,” Vol 1, p. 319.
- (11) Wille, P., *Fifth ASTM-Euratom Symposium on Reactor Dosimetry*, Geesthacht 1984, “Reactor Dosimetry,” Vol 1, p. 497.
- (12) Strohmaier, B., Togenes, S., and Vonach, H., *Physics Data*, NR 13-2, 1980.
- (13) Gayther, D. B., Murphy, M. C., Randle, K., Taylor, W. H., and Utley, C. A., *Conference on Nuclear Data*, Santa Fe, 1985.
- (14) Vaninbroux, R., *International Journal of Applied Radiation Isotopes*, Vol 34, No. 8, p. 1211.
- (15) Alberts, W. G., Schotzig, U., and Siegert, “Nuclear Data for the Use of Niobium as a Neutron Fluence Monitor,” *Sixth ASTM-Euratom Symposium on Reactor Dosimetry*, Jackson, WY, May 1987, Paper 170.
- (16) Nishizawa, N., Sudo, H., Akiyama, T., and Sugimori, N., “The Preparation of Ultra High Purity Niobium and High Purity Vanadium for Monitoring Neutron Fluence,” *Sixth ASTM-Euratom Symposium on Reactor Dosimetry*, Jackson, WY, May 1987, Paper 273.
- (17) Central Bureau for Nuclear Measurements Reference Material for Reactor Neutron Dosimetry Available for Sale, GE/NI/SP/002/87, Distributed at the Sixth ASTM/Euratom Conference on Reactor Dosimetry.
- (18) Williamson, T. G., Ayers, T. A., Hammersten, W. L., Lamaze, G. P., and Schima, F. J., “ $^{93}\text{Nb}(n,n')$  Cross Section Measurements in Fission Spectrum,” *Sixth ASTM-Euratom Symposium on Reactor*

- Dosimetry*, Jackson, WY, May 1987, Paper 173.
- (19) Williams, J., Cogburn, C., Hodgson, L., Apple, S., McGarry, D., Lamaze, G., Gilliam, D., Grundl, J., Coursey, B., Schima, F., Rogers, J.W., Gehrke, R. J., Baker, J. D., and Wheeler, F. J., "Measurements of Fission Spectrum Averaged Cross Section for the  $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$  Reaction," *Sixth ASTM-Euratom Symposium on Reactor Dosimetry*, Jackson, WY, May 1987, Paper 176.
  - (20) Cogburn, C. O., Hodgson, L. M., and Williams, J. G., "Pressure Vessel Dosimetry at Three PWR Plants Using Niobium Monitors," *Sixth ASTM-Euratom Symposium on Reactor Dosimetry*, Jackson, WY, May 1987, Paper 163.
  - (21) Bars, L. B., Seren, T. O., and Wasastjerna, F., "Experimental and Theoretical Neutron Flux Estimates at the Surveillance Chain, at the Pressure Vessel Inner Surface and in the Cavity of a VVER-440 PWR," *Sixth ASTM-Euratom Symposium on Reactor Dosimetry*, Jackson, WY, May 1987, Paper 159.
  - (22) McCrohon, R., Plested, M., and Fudge, A., "Development in the Use of Niobium for Fast Neutron Metrology," *Sixth ASTM-Euratom Symposium on Reactor Dosimetry*, Jackson, WY, May 1987, Paper 259.
  - (23) Alberts, W. G., and Schneider, W., "Reactor Dosimetry: Standardization of Procedures and Considerations on Further Development of LWR PV Surveillance in the Federal Republic of Germany," *Sixth ASTM-Euratom Symposium on Reactor Dosimetry*, Jackson, WY, May 1987, Paper 403.
  - (24) "Workshop on Neutron Dosimetry With Niobium," chairmen B. Baers, J. W. Rogers, *Proceedings of the Seventh ASTM-EURATOM Symposium on Reactor Dosimetry*, G. Tsotridis, R. Dierckx, and P. D'Hondt, Eds., Kluwer Academic Publishers, Dordrecht, 1992, pp. 928–929.
  - (25) Odano, N., Iwasaki, S., and Sugiyama, K., "Nuclear Model Calculation of Dosimetry Reactions on  $^{93}\text{Nb}$ ," *Reactor Dosimetry, ASTM STP 1228*, pp. 341–348, *Proceedings of the Seventh ASTM-EURATOM Symposium on Reactor Dosimetry*, G. Tsotridis, R. Dierckx, P. D'Hondt, Eds., Kluwer Academic Publishers, Dordrecht, 1992, pp. 928–929.
  - (26) Badikov, S. A., and Zolotarev, K. I., "Evaluation of the  $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$  and  $^{93}\text{Nb}(n,2n)^{92\text{m}}\text{Nb}$  Reactions Cross Sections From Threshold to 30 MeV," *Reactor Dosimetry, ASTM STP 1228*, pp. 694–703, H. Farrar, IV, E. P. Lippincott, J. G. Williams, and D. W. Vehar, Eds., American Society for Testing and Materials, Philadelphia, 1994.
  - (27) Bars, B., and Uusheimo, K., "Experiences with Nb Dosimeters for Neutron Flux Measurements," *Proceedings of the Seventh ASTM-EURATOM Symposium on Reactor Dosimetry*, G. Tsotridis, R. Dierckx, and P. D'Hondt, Eds., Kluwer Academic Publishers, Dordrecht, 1992, pp. 928–929.
  - (28) Freudenreich, W. E., "Experiences with the Reaction  $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$  in Neutron Fluence Monitoring," *Proceedings of the Seventh ASTM-EURATOM Symposium on Reactor Dosimetry*, G. Tsotridis, R. Dierckx, and P. D'Hondt, Eds., Kluwer Academic Publishers, Dordrecht, 1992, pp. 928–929.
  - (29) Williams, T. G., and Chubb, A. C., "Induced X-ray Emission in Niobium Foil Dosimeters," *Proceedings of the Seventh ASTM-EURATOM Symposium on Reactor Dosimetry*, G. Tsotridis, R. Dierckx, and P. D'Hondt, Eds., Kluwer Academic Publishers, Dordrecht, 1992, pp. 928–929.
  - (30) Gritzay, O.O., Rusinko, P.M., Vasylyeva, O.G., "Use of the Reaction  $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$  to Determine Neutron Spectra at Outer PV Surface of WWER-1000 Reactor," *Reactor Dosimetry: Radiation Metrology and Assessment, ASTM STP 1398*, pp. 737–744, J.G. Williams, D.W. Vehar, F.H. Ruddy, D.M. Gilliam, Eds., ASTM International, West Conshohocken, PA, 2001.
  - (31) Tellin, A.I., Ryazanov, D.K., Markina, N.V., "Study of the  $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$  Reaction in Fast Reactor Neutron Spectra," *Proceedings of the 9<sup>th</sup> International Symposium on Reactor Dosimetry*, pp. 698–705, H. Ait Abderrahim, P. D'homdt, B. Osmera, Eds., World Scientific, Singapore, 1998.
  - (32) Greenwood, L.R., Ratner, R.T., Poepfel, K.A., V., "Use of the  $^{93}\text{Nb}(n,n')^{93\text{m}}\text{Nb}$  Reaction for Dosimetry, EBRII, and HFIR Reactors" *Proceedings of the 9<sup>th</sup> International Symposium on Reactor Dosimetry*, pp. 698–705, H. Ait Abderrahim, P.D'homdt, B. Osmera, Eds., World Scientific, singapore, 1998.
  - (33) Update of Xray and Gamma Ray Decay Data Standards for Detector Calibration and Other Applications, Vol. 1: *Recommended Decay Data High Energy Gamma Ray Standards and Angular Correlation Coefficient*. International Atomic Energy Agency, report STI/PUB/1287, Vienna, 2007.
  - (34) "International Reactor Dosimetry File (IRDF-2002)," International Atomic Energy Agency, Nuclear Data Section, Technical Reports Series No. 452, 2006. Document available from URL <http://www.nds.iaea.org/irdf2002/docs/irdf-2002.pdf>
  - (35) Zoloterev, K.i., Ingatyuk, A. V., Mahokhin, V.N., Pashchenko, A.B., RRDF-98 *Russian Reactor Dosimetry File*, Rep. IAEA-NDS-193, Rev. IAEA, Vienna, 2005. URL <http://www.nds-ipen.br/ndpub/libraries2/rrdf98/>
  - (36) B.N. Taylor, C.E. Kuyatt, *Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results*, NIST Technical Note 1297, National Institute of Standards and Technology, Gaithersburg, MD 1994.
  - (37) *Guide in the Expression of Uncertainty in Measurement*, International Organization for Standardization, 1993, ISBN 92-67-10188-9.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or [service@astm.org](mailto:service@astm.org) (e-mail); or through the ASTM website ([www.astm.org](http://www.astm.org)). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>