



# Standard Practice for Reducing the Effect of Variability of Color Measurement by Use of Multiple Measurements<sup>1</sup>

This standard is issued under the fixed designation E1345; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## INTRODUCTION

Recent improvements in the precision and bias of color-measuring instruments have been accompanied by more widespread use of numerical color tolerances based on instrumental measurements. As tighter tolerances are specified, they begin to approach the limits of visual perception. In many cases, the instrument user has found it difficult to prepare and measure specimens with adequate repeatability. This practice provides procedures for reducing variability in the mean results of color measurement by the use of multiple measurements, and it indicates how many measurements are required for a specific reduction.

### 1. Scope

1.1 Reduction of the variability associated with average color or color-difference measurements of object-color specimens is achieved by statistical analysis of the results of multiple measurements on a single specimen, or by measurement of multiple specimens, whichever is appropriate.

1.2 This practice provides a means for the determination of the number of measurements required to reduce the variability to a predetermined fraction of the relevant color or color-difference tolerances.

1.3 This practice is general in scope rather than specific as to instrument or material.

### 2. Referenced Documents

2.1 *ASTM Standards*:<sup>2</sup>

[D2244 Practice for Calculation of Color Tolerances and Color Differences from Instrumentally Measured Color Coordinates](#)

[D3134 Practice for Establishing Color and Gloss Tolerances](#)  
[E178 Practice for Dealing With Outlying Observations](#)

[E284 Terminology of Appearance](#)

[E308 Practice for Computing the Colors of Objects by Using the CIE System](#)

<sup>1</sup> This practice is under the jurisdiction of ASTM Committee E12 on Color and Appearance and is the direct responsibility of Subcommittee E12.04 on Color and Appearance Analysis.

Current edition approved Nov. 1, 2014. Published November 2014. Originally approved in 1990. Last previous edition approved in 2008 as E1345 – 98 (2008) <sup>$\epsilon$ 1</sup>. DOI: 10.1520/E1345-98R14.

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

[E456 Terminology Relating to Quality and Statistics](#)  
[E1164 Practice for Obtaining Spectrometric Data for Object-Color Evaluation](#)

2.2 *Other Standard*:

[SAE J 1545 Recommended Practice for Instrumental Color Difference Measurement for Exterior Finishes, Textiles and Colored Trim](#)<sup>3</sup>

### 3. Terminology

3.1 Definitions of appearance terms in Terminology [E284](#) or statistical terms in Terminology [E456](#) are applicable to this practice.

3.2 *Definitions of Terms Specific to This Standard*:

3.2.1 *box and whisker plot, n*—a nonparametric data analysis diagram that illustrates the 25, 50, and 75 % cumulative distribution of values in a data set (the box) and the expected range of values, defined by distance outside the box ends; see *whiskers*, see [Fig. 1](#).

3.2.2 *extreme value, n*—a single reading, selected from a series of readings, whose value is farther from the nearer box end than 3.0 times the hinge length.

3.2.2.1 *Discussion*—A box and whiskers plot is normally used to find outliers and extreme values. Such values should be eliminated from a series before calculating the series mean, standard deviation, and confidence intervals.

3.2.3 *hinges, n*—the 25 and 75 % cumulative distribution points in a set of readings taken during a measurement.

3.2.3.1 *Discussion*—Hinges represent the values in which

<sup>3</sup> Available from Society of Automotive Engineers (SAE), 400 Commonwealth Dr., Warrendale, PA 15096-0001, <http://www.sae.org>.

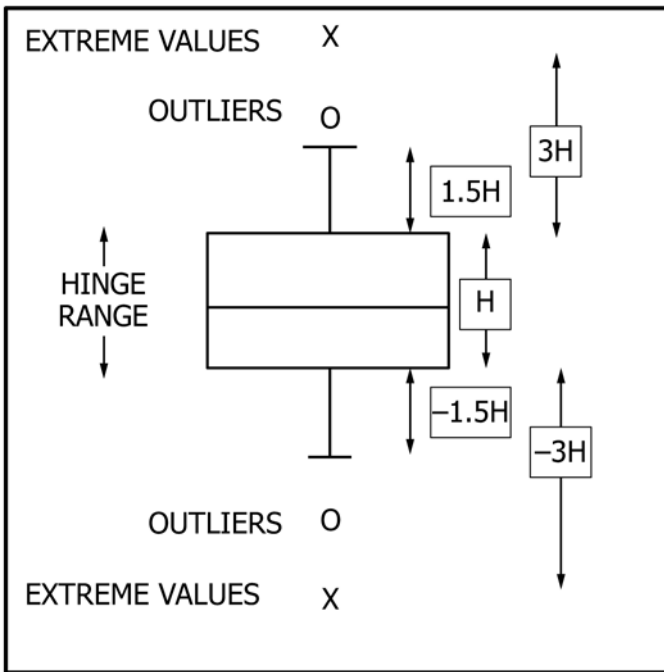


FIG. 1 Schematic Description of a Box and Whisker Plot

25 % of the readings are less than the lower hinge and 75 % of the readings are less than the upper hinge. See also *hinge length*.

3.2.3.2 *Discussion*—Hinges are sometimes called the lower ( $Q_1$ ) and upper ( $Q_3$ ) quartile values.

3.2.4 *hinge length, H, n*—the range of values between the lower and upper hinges.

3.2.4.1 *Discussion*—The hinge length is sometimes called the box width or the interquartile range  $Q_3$  to  $Q_1$ .

3.2.5 *outlier, n*—a single reading, selected from a series of readings, whose value is further from the nearer box end than 1.5 times the hinge length; see 3.2.2.1.

3.2.6 *sampling number, N, n*—number of multiple measurements, or number of multiple specimens, required to reduce the variability of color or color-difference measurement to a desired level.

3.2.7 *standard deviation of color or color-difference measurement, s*—standard deviation of the color scale or color-difference-scale value,  $x_i$ , being considered:

$$s = \left[ \frac{\sum (x_i - x_{avg})^2}{(n - 1)} \right]^{0.5} \quad (1)$$

where:

$x_{avg}$  =  $(\sum x_i)/n$ , and  
 $n$  = the number of replicate measurements made.

3.2.8 *standard deviation of instrument, s<sub>i</sub>, n*—standard deviation of a color-scale or color-difference-scale value due to instrument variability alone:

$$s_i = \left[ \frac{\sum (x_i - x_{avg})^2}{(n - 1)} \right]^{0.5} \quad (2)$$

3.2.9 *standard error of the estimated mean, s<sub>e</sub>, n*—standard deviation of color or color-difference measurement divided by the square root of the sampling number:

$$s_e = s/(N^{0.5}) \quad (3)$$

3.2.10 *standard error goal, s<sub>e,g</sub>, n*—level to which the standard error of the estimated mean is to be reduced.

3.2.11 *tolerance, n*—the upper tolerance limit minus the lower tolerance limit; the total allowable range of the color-scale or color-difference-scale value considered.

3.2.12 *whiskers, n*—lines extending out from the box ends to the largest and smallest observations lying within 1.5 times the hinge length, measured from the box ends.

#### 4. Summary of Practice

4.1 This practice assumes that, for the material under consideration and a specified set of color scales, relevant color or color-difference tolerances have been established (see Practice D3134).

4.2 For convenience, the numerical example in the Appendix uses CIELAB *LCH* (lightness, chroma, hue) color difference scales  $\Delta L^*$ ,  $\Delta C^*_{ab}$ , and  $\Delta H^*_{ab}$  (see Practice D2244 and Practice E308), but this is not meant to be restrictive.

NOTE 1—Some coordinates, such as CIE  $x$ ,  $y$ ,  $Y$ , do not follow the theories of this standard due to excessive colinearity. While it has not been tested, this same colinearity problem may also be observed in 1960  $u$ ,  $v$  and 1976  $u'$ ,  $v'$  coordinates. Table 1 provides a listing of the appropriate and inappropriate color coordinates for use with this practice.

4.3 The successive steps in the procedure are as follows:

4.3.1 Determine the standard deviation of instrument.

4.3.1.1 Screen the measurement data for outliers and extreme values.

4.3.2 Determine the standard deviation of color or color-difference measurement.

4.3.2.1 Screen the measurement data for outliers and extreme values.

4.3.3 Determine the standard error of the estimated mean for a sampling number of one.

4.3.4 Determine the final sampling number that reduces the standard error of the estimated mean to less than the standard error goal for each scale value.

4.3.5 Determine the final standard error goal values.

NOTE 2—When the standard error of the estimated mean for a sampling number of one is larger than a specified fraction of the tolerance or a specified multiple of the standard deviation of instrument for any of the three color-difference-scale values, a sampling number greater than one is required.

4.4 *Screening for and Elimination of Outliers and Extreme Values in Measured Data:*

TABLE 1 Appropriate and Inappropriate Color Coordinates for Use in This Practice

| Color Coordinates | Appropriate | Inappropriate |
|-------------------|-------------|---------------|
| CIE Yxy           |             | ✓             |
| CIE LCH           | ✓           |               |
| CIE LAB           | ✓           |               |
| CIE LUV           | ✓           |               |
| CIE LuV           |             | ✓             |

**TABLE 2 Official Values for  $T$  (One-Sided Test) for Outliers**

| Number of Observations<br>$n$ | Upper 0.1 % Significance Level | Upper 1.0 % Significance Level |
|-------------------------------|--------------------------------|--------------------------------|
| 3                             | 1.155                          | 1.155                          |
| 4                             | 1.499                          | 1.492                          |
| 5                             | 1.780                          | 1.749                          |
| 6                             | 2.011                          | 1.944                          |
| 7                             | 2.201                          | 2.097                          |
| 8                             | 2.358                          | 2.221                          |
| 9                             | 2.492                          | 2.323                          |
| 10                            | 2.606                          | 2.410                          |
| 11                            | 2.705                          | 2.485                          |
| 12                            | 2.791                          | 2.550                          |
| 13                            | 2.867                          | 2.607                          |
| 14                            | 2.935                          | 2.659                          |
| 15                            | 2.997                          | 2.705                          |

4.4.1 *Box and whisker test*—This test is best carried out by computer. Many programs for the box and whisker technique are available.<sup>4</sup>

4.4.1.1 Order the readings from lowest to highest value. The reading whose value is half way between the minimum and maximum values is the median. Fig. 1 illustrates the following steps.

4.4.1.2 The reading whose value is just less than 75 % of the other readings is the lower hinge. The readings whose value is just higher than 75 % of the other readings is the upper hinge. The difference between these two is the hinge length  $H$ .

4.4.1.3 If the smallest value of any reading is less than the lower hinge value minus 1.5 times the hinge length, it may be considered an outlier. Likewise, if the largest value of any reading is greater than the upper hinge value plus 1.5 times the hinge length, it may be considered an outlier.

4.4.1.4 If the smallest (largest) value of any reading is less (greater) than the lower (upper) hinge value minus (plus) 3.0 times the hinge length, it may be considered an extreme value.

4.4.2 *Practice E178 Procedure*—The test for outliers in Practice E178 is constructed from the sample mean  $X_{avg}$ , and the standard deviation  $s$ .

4.4.2.1 Order the readings from lowest to highest value.

4.4.2.2 Calculate the following two statistics,  $T_l$  for the lowest value, and  $T_n$  for the highest value in a set of  $n$  ordered readings as follows:

$$T_l = \frac{(x_{avg} - x_1)}{s} \quad (4)$$

$$T_n = \frac{(x_n - x_{avg})}{s} \quad (5)$$

4.4.2.3 Compare the values of  $T_l$  ( $T_n$ ) to critical values in Table 2. If  $T_l$  ( $T_n$ ) is larger than the critical value for  $n$  readings at the 1 % level of significance. Reading 1 ( $n$ ) may be considered an outlier.

NOTE 3—Table 2 contains critical values for series of up to 15 readings and for 0.1 and 1 % significance levels. For other significance levels and larger datasets, see Table 1 of Practice E178.

4.4.2.4 If  $T_l$  ( $T_n$ ) is larger than the critical value for  $n$  readings at the 1 % level of significance, Readings 1 ( $n$ ) may be considered an extreme value.

4.4.3 If any outliers or extreme values were found, consider carefully whether they should be dropped or retained. Drop those readings not considered to be part of the desired dataset, by whatever consistent criteria are accepted. See 5.3.

4.4.4 Recalculate the mean, standard deviation and confidence limits of the remaining dataset.

## 5. Significance and Use

5.1 This practice should be used whenever measured color-scale or color-difference-scale values are to be compared to an established tolerance. In this way it can be demonstrated quantitatively that the sampling and measurement procedures are adequate to allow an unambiguous decision as to whether or not the mean results are within tolerance.

5.2 This practice is based on portions of SAE J 1545, as it applies to painted or plastic automotive parts. It is generally applicable to object colors in various materials. Textured materials, such as textiles, may require special consideration (see SAE J 1545 and STP 15D Manual on Presentation of Data and Control Chart Analysis<sup>5</sup>).

5.3 While Practice E178 deals with outliers, it does not include definitions relating to the box and whisker technique. The definition of an outlier is operational and a little vague because there is still considerable disagreement about what constitutes an outlier. In any normally distributed population, there will be members that range from minus to plus infinity. Theoretically, one should include any member of the population in any sample based on estimates of the population parameters. Practically, including a member that is found far from the mean within a small sample, most members of which are found near the mean, will introduce a systematic bias into the estimate of the population parameters (mean, standard deviation, standard error). Such a bias is in direct contrast with the goal of this practice, namely, to reduce the effects of variability of measurement. For the purposes of this practice, no distinction is made between errors of sampling and members of the tails of the distribution. Practice E178 has several methods and significance tables to attempt to differentiate between these two types of extreme values.

## 6. Procedure

6.1 Determine the standard deviation of instrument,  $s_i$ , by carrying out the appropriate color measurement at least 10 times ( $n = 10$ ) when using a stable product standard as the specimen, without removing or disturbing the specimen between measurements. Calculate  $s_i$  by the use of Eq 2. This determination should be carried out for each color scale used and for each product with a new color; however,  $s_i$  is unlikely to change appreciably over relatively extended periods.

6.1.1 Screen the measurement data for outliers and extreme values following 4.4.1 – 4.4.4.

<sup>4</sup> See for example, Schaefer, R. L. and Anderson, R. B., *The Student Edition of Minitab*, Addison-Wesley, New York, 1989.

<sup>5</sup> Available from ASTM International Headquarters 100 Barr Harbor Drive, West Conshohocken, PA 19428.

6.2 Select maximum allowable values of the standard error of the estimated mean, as a fraction of the tolerance and as a multiple of the standard deviation of instrument. In the absence of specified values of these quantities, use those recommended in SAE J 1545: 0.1 times the tolerance and  $2s_i$ . These values are used in [Appendix X1](#).

NOTE 4—This practice assumes that all measurements are subject to the central limit theorem of mathematical statistics, so that as the number of replicate or repeat measurements becomes large, the distribution of values is described by the standard normal distribution. It has been shown,<sup>6,7</sup> however, that averages of large numbers of measurements of a verification standard on a properly maintained spectrophotometer are not approximated by the standard normal distribution. As a result, tests anchored to  $s_i$  may exhibit a significance or a power dependence different from that which is expected.

6.3 Determine the standard deviation of color or color-difference measurement,  $s$ , by making the appropriate measurement at least 10 times ( $n = 10$ ), as follows:

6.3.1 To assess the variability within a single specimen, measure the same specimen at ten or more randomly selected different areas of the specimen.

6.3.1.1 Screen the measurement data for outliers and extreme values following [4.4.1 – 4.4.4](#).

6.3.2 To assess the variability among specimens, measure at least ten replicate specimens.

6.3.2.1 Screen the measurement data for outliers and extreme values following [4.4.1 – 4.4.4](#).

6.4 Determine the standard error of the estimated mean,  $s_e$ , for a sampling number of one, using [Eq 3](#). Note that for  $N = 1$ ,  $s_e = s$ . Use the larger of the values of  $s$  determined in [6.3.1](#) or [6.3.2](#).

6.5 Compare the value of  $s_e$  to 0.1 times the tolerance and to  $2s_i$  for each of the three color or color-difference scales used. When in any of the three cases  $s_e$  exceeds  $2s_i$  or 0.1 times the tolerance, multiple measurements are required ( $N > 1$ ). Whether these should be multiple measurements of a single specimen or measurements of multiple (replicate) specimens is determined by whether the value of  $s$  from [6.3.1](#) or [6.3.2](#) is greater.

<sup>6</sup> Marcus, R. T., and Billmeyer, F. W., Jr., “Statistical Study of Color-Measuring Instruments,” *Applied Optics*, Vol 13, 1974, pp. 1519–1530.

<sup>7</sup> Billmeyer, F. W., Jr., and Alessi, P. J., “Assessment of Color-Measuring Instruments,” *Color Research and Application*, Vol 6, 1981, pp. 195–202.

6.6 Determine the value of the standard error goal,  $s_{e,g}$ , as the greater of  $2s_i$  or 0.1 times the tolerance, for each color or color-difference scale used.

6.7 Calculate the sampling number required to meet the criteria of  $s_{e,g}$  as follows:

6.7.1 For each color or color-difference scale, calculate  $N$  by the following rearrangement of [Eq 3](#):

$$N = (s/s_{e,g})^2 \quad (6)$$

6.7.2 Round any fractional values of  $N$  to the next larger whole number.

6.7.3 Select the largest of the rounded values of  $N$  as the final sampling number.

6.8 Using the final value of  $N$  from [6.7.3](#), calculate the final standard error goal for each color scale by use of [Eq 3](#).

## 7. Report

7.1 Report the final sampling number from [6.7.3](#) and the final standard error goal for each color scale from [6.8](#), in addition to the quantities required in the report of the test method used.

## 8. Precision and Bias

8.1 *Precision and Bias of Final Sampling Number,  $N$* —Since  $N$  has been rounded up to the next larger whole number, its precision is  $\pm 1$  unit and its maximum bias is  $+ 1$  unit.

8.2 *Precision and Bias of Final Standard Error Goals,  $s_{e,g}$* :

8.2.1 The calculations of this practice can affect the precision of  $s_{e,g}$  due to roundoff. To minimize this error, one more significant figure should be carried in the calculations than is required by the precision and bias statement of the test method used.

8.2.2 The calculations of this practice should introduce no bias into  $s_{e,g}$ .

8.2.3 To the quantities of [8.2.1](#) should be added any contribution to precision or bias resulting from the test method used.

## 9. Keywords

9.1 color; color difference; color measurement; color tolerances

**APPENDIX**
**(Nonmandatory Information)**
**X1. CALCULATION OF THE FINAL SAMPLING NUMBER AND THE FINAL STANDARD ERROR OF THE ESTIMATED MEAN**
**TABLE X1.1**

| Section | Quantity  | Color-Difference Scale |                   |                   |
|---------|---|------------------------|-------------------|-------------------|
|         |   | $\Delta L^*$           | $\Delta C^*_{ab}$ | $\Delta H^*_{ab}$ |
| 6.1     | Instrument standard deviation, $s_i$                  | 0.1                    | 0.1               | 0.1               |
| 6.2     | Least significant scale-value interval, $2s_i$        | 0.2                    | 0.2               | 0.2               |
|         | Upper tolerance limit                                 | + 2.0                  | + 1.0             | + 0.5             |
|         | Lower tolerance limit                                 | -2.0                   | -1.0              | -0.5              |
|         | Tolerance   | 4.0                    | 2.0               | 1.0               |
|         | 0.1 times the tolerance                               | 0.4                    | 0.2               | 0.1               |
| 6.3     | Standard deviation, $s$                               | 0.45                   | 0.35              | 0.15              |
| 6.4     | Standard error of estimated mean, $s_e$ , for $N = 1$ | 0.45                   | 0.35              | 0.15              |
| 6.6     | Standard error goal, $s_{e,g}$                        | 0.4                    | 0.2               | 0.2               |
| 6.7.1   | Sampling number, $N$                                  | 1.27                   | 3.06              | 0.56              |
| 6.7.2   | Rounded sampling number                               | 2                      | 4                 | 1                 |
| 6.7.3   | Final sampling number                                 | 4                      | 4                 | 4                 |
| 6.8     | Final standard error goal                             | 0.23                   | 0.18              | 0.08              |

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>