



Designation: E2214 – 17

Standard Practice for Specifying and Verifying the Performance of Color-Measuring Instruments¹

This standard is issued under the fixed designation E2214; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

INTRODUCTION

Recent advances in optics, electronics and documentary standard have resulted in a proliferation of instruments for the measurement of color and appearance of materials and objects. These instruments possess very good performance but there has been little progress toward standardizing the terminology and procedures to quantify that performance. Therefore, the commercial literature and even some documentary standards are a mass of confusing terms, numbers and specifications that are impossible to compare or interpret.

Two recent papers in the literature, have proposed terms and procedures to standardize the specification, comparison and verification of the level of performance of a color-measuring instrument.^{2,3} Following those procedures, those specifications can be compared to product tolerances. This becomes important so that instrument users and instrument makers can agree on how to compare or verify, or both, that their instruments are performing in the field as they were designed and tested in the factory.

1. Scope

1.1 This practice provides standard terms and procedures for describing and characterizing the performance of spectral and filter based instruments designed to measure and compute the colorimetric properties of materials and objects. It does not set the specifications but rather gives the format and process by which specifications can be determined, communicated and verified.

1.2 This practice does not describe methods that are generally applicable to visible-range spectroscopic instruments used for analytical chemistry (UV-VIS spectrophotometers). ASTM Committee E13 on Molecular Spectroscopy and Chromatography includes such procedures in standards under their jurisdiction.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

1.4 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

2. Referenced Documents

2.1 *ASTM Standards:*⁴

[D2244 Practice for Calculation of Color Tolerances and Color Differences from Instrumentally Measured Color Coordinates](#)

[E284 Terminology of Appearance](#)

[E1164 Practice for Obtaining Spectrometric Data for Object-Color Evaluation](#)

¹ This practice is under the jurisdiction of ASTM Committee E12 on Color and Appearance and is the direct responsibility of Subcommittee E12.04 on Color and Appearance Analysis.

Current edition approved May 1, 2017. Published July 2017. Originally approved in 2002. Last previous edition approved in 2016 as E2214 – 16. DOI: 10.1520/E2214-17.

² Ladson, J., "Colorimetric Data Comparison of Bench-Top and Portable Instruments," *AIC Interim Meeting, Colorimetry*, Berlin, 1995.

³ Rich, D., "Standardized Terminology and Procedures for Specifying and Verifying the Performance of Spectrocolorimeters," *AIC Color 97 Kyoto*, Kyoto, 1997.

⁴ For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

2.2 Other Documents:

ISO VIM International Vocabulary of Basic and General Terms in Metrology (VIM)⁵

NIST Technical Note 1297 Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results⁶

3. Terminology

3.1 Definitions of appearance terms in Terminology **E284** are applicable to this practice.

3.2 Definitions of metrology terms in ISO, International Vocabulary of Basic and General Terms in Metrology (VIM) are applicable to this practice.

3.3 Definitions of Terms Specific to This Standard:

3.3.1 *colorimetric spectrometer, n*—spectrometer, one component of which is a dispersive element (such as a prism, grating or interference filter or wedge or tunable or discrete series of monochromatic sources), that is normally capable of producing as output colorimetric data (such as tristimulus values and derived color coordinates or indices of appearance attributes) as well as the underlying spectral data from which the colorimetric data are derived.

3.3.2 *inter-instrument agreement, n*—the closeness of agreement between the results of measurements in which two or more instruments from the same manufacturer and model are compared.

3.3.3 *inter-model agreement, n*—the closeness of agreement between the results of measurements in which two or more instruments from different manufacturers, or of different but equivalent design, are compared.

3.3.3.1 *Discussion*—Modern instruments have such high precision that small differences in geometric and spectral design can result in significant differences in the performance of two instruments. This can occur even though both instruments exhibit design and performance bias which are well within the expected combined uncertainty of the instrument and within the requirements of any international standard.

3.3.4 *mean color difference from the mean, MCDM, n*—a measure of expectation value of the performance of a color-measuring instrument.

3.3.4.1 *Discussion*—MCDM calculates the average color difference between a set of readings and the average of that set of readings. $MCDM = \text{average}(\Delta E_i(\text{average}(Lab) - Lab_i))$, for $i = 1$ to N readings. Any standard color difference or color tolerance equation can be used as long as the report clearly identifies the equation being used (see Practice **D2244**).

4. Summary of Practice

4.1 This practice defines standardized terms for the most common instrument measurement performance parameters (repeatability, reproducibility, inter-instrument agreement,

inter-model instrument agreement, accuracy) and describes a set of measurements and artifacts, with which both the producers and users of color-measuring instruments verify or certify the specification and performance of color-measuring instruments. Following this practice can improve communications between instrument manufacturers and instrument users and between suppliers and purchasers of colored materials.

5. Significance and Use

5.1 In today's commerce, instrument makers and instrument users must deal with a large array of bench-top and portable color-measuring instruments, many with different geometric and spectral characteristics. At the same time, manufacturers of colored goods are adopting quality management systems that require periodic verification of the performance of the instruments that are critical to the quality of the final product. The technology involved in optics and electro-optics has progressed greatly over the last decade. The result has been a generation of instruments that are both more affordable and higher in performance. What had been a tool for the research laboratory is now available to the retail point of sale, to manufacturing, to design and to corporate communications. New documentary standards have been published that encourage the use of colorimeters, spectrophotometers, and colorimetric spectrometers in applications previously dominated by visual expertise or by filter densitometers.⁷ Therefore, it is necessary to determine if an instrument is suitable to the application and to verify that an instrument or instruments are working within the required operating parameters.

5.2 This practice provides descriptions of some common instrumental parameters that relate to the way an instrument will contribute to the quality and consistency of the production of colored goods. It also describes some of the material standards required to assess the performance of a color-measuring instrument and suggests some tests and test reports to aid in verifying the performance of the instrument relative to its intended application.

6. Instrument Performance Parameters

6.1 *Repeatability*—is generally the most important specification in a color-measuring instrument. Colorimetry is primarily a relative or differential measurement, not an absolute measurement. In colorimetry, there is always a standard and a trial specimen. The standard may be a real physical specimen or it may be a set of theoretical target values. The trial is usually similar to the standard in both appearance and spectral nature. Thus, industrial colorimetry is generally a test of how well the instrument repeats its readings of the same or nearly the same specimen over a period of minutes, hours, days, and weeks.

6.1.1 The ISO VIM defines repeatability as a measure of the random error of a reading and assumes that the sample standard deviation is an estimate of repeatability. Repeatability is further defined as the standard deviation of a set of measurements taken over a specified time period by a single operator, on a

⁵ ISO/IDE/OIML/BIPM, *International Vocabulary of Basic and General Terms in Metrology* International Organization for Standardization, Geneva, Switzerland, 1984.

⁶ TaylorBarry N., and Kuyatt, Chris E., *Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Results* NIST Technical Note 1297, U. S. Government Printing Office, Washington, D. C., 1984.

⁷ ISO 13655 Spectral Measurement and Colorimetric Computation for Graphic Arts Images, International Organization for Standardization, Geneva, Switzerland.

single instrument with a single specimen. This definition is similar to that in Terminology E284, except that the ISO explicitly defines the metric of “closeness of agreement” as the sample standard deviation. Since color is a multidimensional property of a material, repeatability should be reported in terms of the multidimensional variance–covariance matrix.

6.1.2 The time period over which the readings are collected must be specified and is often qualitatively described as “short,” “medium,” or “long.” The definitions of these time frames do not overlap. This is intentional, providing clearly defined milestones in the temporal stability of test results.

6.1.2.1 For the purposes of colorimetry, “short” is normally the time required to collect a set of 30 readings, taken as fast as the instrument will allow. The actual time will vary as a function of lamp and power supply characteristics but should be less than one hour.

6.1.2.2 “Medium” term is normally defined as, at least the period of one work shift (8 h) but less than three work shifts (one day).

6.1.2.3 “Long” term is open ended but is often described as any set readings taken over a period of at least 4 to 8 weeks. The longest known reported study described readings taken over a period of 3¼ years.⁸

6.2 *Reproducibility* is the second most important specification in a color-measuring instrument. According to Terminology E284, reproducibility is the closeness of agreement of the results of measurements in which one or more of the measurement parameters have been systematically changed. Thus the sample is different, the procedures or instrument are different, or the time frame is very long. The increase of disorder over a very long time changes the instrument systematically and the set of readings really compares a “young” instrument with an “old” instrument.

6.2.1 The ISO VIM defines reproducibility as the closeness of agreement of the results of measurements in which either the time frame is very long, in which the operator changes, the instrument changes, or the measurement conditions change. ISO again recommends estimating this with a standard deviation. Reproducibility is further defined as the standard deviation of a set of measurements taken over a specified period of time by a single operator, on a single instrument with a single specimen. This definition is similar to that in Terminology E284, except that the ISO again, explicitly defines the metric of “closeness of agreement” as the sample standard deviation. Again, since color is a multidimensional property of a material, reproducibility should be reported in terms of the multidimensional variance–covariance matrix.

6.2.2 The time period over which the readings are collected must be specified. For the purposes of colorimetry, “long” term repeatability is the most common and important type of reproducibility. Repeatability and reproducibility have traditionally been evaluated in colorimetry by comparing the color differences of a set of readings to a single reading or to the average of the set of readings.

6.3 *Inter-Instrument Agreement*, as defined in 3.3.2, describes the reproducibility between two or more instruments, of identical design. The ISO has no definition or description of such a concept. This is because in most test results, a method or instrument dependent bias can be assessed. In this situation, such a test measures the consistency of the design and manufacturing process. Within the technical description of the standard geometric and spectral parameters for the measurement of diffuse reflectance factor and color, a significant amount of latitude exists. This latitude results in a random amount of bias. For a given design, a manufacturer may reduce the random bias, often to a level less than the stability of reference materials. The most common form of test for inter-model instrument agreement is pairwise color difference assessment of a series of specimens. Various parameters are reported in the literature including the average color difference, the maximum color difference, the typical color difference, the RMS color difference or the MCDM mean color difference from the mean, taking the average of all instruments as the standard and the other as the test instrument. Using pairs of instruments and materials one can derive a multivariate confidence interval against the value 0.0 difference and then test individual components to determine which attribute (lightness, chroma, hue) are the significant contributors to the differences between instruments. If a group of instruments are being tested then a multivariate analysis of variance (MANOVA) can be performed to test the agreement of the means of the instrument.

6.4 *Inter-Model Agreement*, as defined in 3.3.3, describes the reproducibility between two or more instruments of differing design. The latitude within the standard geometric and spectral parameters described in the preceding paragraph is at a maximum when the designs differ. The systematic bias may increase by factors of from 5 to 10 because of the increased latitude. Standardizing laboratories will report either the algebraic differences between measurement results or the ratio of the measurement values between two labs. The former will be a normal statistical variable if the measurement values are normally distributed, and the latter will be distributed as a ratio of normally distributed variables. This distribution can be estimated from the multivariate variance–covariance matrix. Using pairs of instruments and materials one can derive a multivariate confidence interval against the value 0.0 difference and then test individual components to determine which attribute (lightness, chroma, hue) are the significant contributors to the differences between instruments. If a group of instruments are being tested then a multivariate analysis of variance (MANOVA) can be performed to test the agreement of the means of the instrument.

6.5 *Accuracy*, while occasionally critical, is generally the least significant parameter in characterizing the performance of a color-measuring instrument. ISO defines accuracy as the conformance of a series of readings to the accepted or true value. In modern colorimetry, the volume of the total combined uncertainty around the accepted value is often many times larger than volume of visual acceptability of the products whose color is being quantified. Therefore, an “accurate” color measurement may result in an unacceptable product color. There are two scales in a spectrophotometer that can be

⁸ Rich, D. C., Battle, D., Malkin, F., Williamson, C., Ingleson, A., “Evaluation of the Long-Term Repeatability of Reflectance Spectrophotometers,” *Spectrophotometry, Luminescence and Colour: Science and Compliance*, C. Burgess and D. G. Jones, eds., Elsevier, Amsterdam, 1995.

assigned nominal values and tested against standard values. They are the radiometric scale and the wavelength scale.

6.5.1 The wavelength scale includes the sampling position (centroid wavelength) and the sampling window width (spectral bandwidth). These parameters are normally tested against physical standards of wavelength based on fundamental phenomena, such as discharge lamps or laser lines. In very abridged instruments it may not be possible to test directly against such a physical standard, so either material standards are used, such as holmium oxide or didymium oxide glasses or pairs of sharp-cutting filter glasses, or a scanning monochromator are characterized against physical standards. In the case of the monochromator, the output intensity is equalized and scanned across the input to the abridged spectrometer to resolve the location of the wavelength centroid at each sampling point in the abridged spectrum.

6.5.2 Radiometric scale accuracy is more difficult to evaluate since it involves three aspects: the zero level, white level, and the linearity between the two levels. White level can be tested by direct comparison to a primary standard of reflectance or transmittance and the result reported as \pm the expanded uncertainty at a stated confidence level, as described in NIST Technical Note 1297. The expanded uncertainty is the combined uncertainty of the white plaque and the instrument under test combined in quadrature at the 95 % confidence level and multiplied by the appropriate coverage factor. The exact methods for propagating the uncertainty in a reflectance factor measurement into the color coordinates is still a matter of some dispute. Methods have been proposed in the literature but are not widely accepted and used.⁹

6.5.3 The black level only needs to be tested to show that the optical zero is less than some minimum value, since it is impossible to define the optical zero except in terms of the noise floor of the spectrometer or colorimeter. The results of measurements of near black materials (black glass of known refractive index or a suitably designed black trap) shall show results that are less than some upper limit. For example, the zero level ≤ 0.025 %.

6.5.4 Finally, linearity must be specified in a testable way. If the spectrometer is linear then at any wavelength, plots of the measured values versus the standard values of a set of neutral samples should lie on a line passing through the origin with a slope of 1.0. Unfortunately, it is possible to fit a line by least squares to a higher order function (having some errors positive and some negative) and obtain a slope of 1.0. Estimating the slope of the line passing through all points will not identify that kind of non-linearity. To avoid this, standardizing laboratories and some analytical instruments use the addition-of-radiance method, either with two sources or with a double aperture apparatus to generate a signal and a 2 \times signal into the spectrometer that can be adjusted to cover the radiometric range of the spectrometer. Since commercial colorimeters are not easily configured with such devices, the use of neutral plaques or neutral filters is the best compromise.

7. Procedures

7.1 Repeatability shall be measured by placing a white plaque at the measurement port of a recently standardized instrument and making replicate readings of the plaque without moving the plaque. For short-term repeatability, at least 30 readings shall be collected as fast as the instrument allows. The quantity of reading (30 or more) depends upon the desired level of confidence in the results and the time required to acquire that number of readings. For very slow instruments, the costs of performing even 30 measurements may be very high, in those cases a lower number of readings may be adequate if the variance-covariance is adequately characterized. For medium term repeatability, at least 60 readings shall be collected, uniformly spread out over an 8-h period, with at least 60 s between readings. Use of a white plaque is recommended because the radiometric random noise is generally highest near the upper end of the scale of diffuse reflectance. A noise level of a few hundredths of a percent is expected at a 90 % reflectance while the noise level may be a few thousandths of a percent at 4 % reflectance. Spectrally selective (colored) standards are not recommended as they tend to confound the radiometric noise with temperature and mechanical sensitivity in a way that is not representative of the general performance of the instrument. Often, a light gray plaque may be substituted for the white plaque when an instrument is never used to measure very light or white specimens as the gray level may result in values for repeatability that are more representative of typical materials. Measurements of medium, dark or black specimens will not generally add any useful information since the radiometric noise level tends to be proportional to the signal and the noise will be lost inside the resolution limit of the spectrometer.

7.1.1 The basic measurement values of a colorimetric spectrometer are the set of reflectance factors and those of a filter colorimeter are the tristimulus values. Those variables are the most closely related to a normal statistical random variable. The reported repeatability shall be either twice the univariate standard deviation of at least three, widely separated reflectance factors, $\Delta R_\lambda(2\sigma)$, ($\lambda = 440 \text{ nm}, 560 \text{ nm}, 660 \text{ nm}$) that are returned from the instrument, or if the reflectance factors are not available, then twice the univariate standard deviation of the individual tristimulus values $\{\Delta X(2\sigma), \Delta Y(2\sigma), \Delta Z(2\sigma)\}$. Since the variance (standard deviation) of closely spaced spectral reflectance factors or tristimulus values are generally, not independent, it will be necessary to report the multivariate variance-covariance matrix instead of the square root of the variance for each measurement point. If the set of univariate standard deviations (multiple reflectance factors or multiple tristimulus values) must be reduced to a single dimension, then it is recommended that a weighted standard deviation be reported, the weight being proportional to the sum of the standard observer functions [$weight = (\bar{x}_i + \bar{y}_i + \bar{z}_i)$] or the variances of the tristimulus values themselves ($\sigma_x^2 + \sigma_y^2 + \sigma_z^2$).

7.1.1.1 If an estimate of expected color difference is desired, then it can be reported using the multivariate variance-covariance matrix which will be a three dimensional ellipsoid for tristimulus data or color coordinate data. **Annex A1** shows

⁹ Fairchild, M. D., and Reniff, L., "Propagation of Random Errors in Spectrophotometric Colorimetry," *Color Research & Application*, Vol. 16, 1991, p. 360.

the steps required to compute the precision of color differences or the significance of a mean color difference.

7.1.1.2 It is also acceptable to report the repeatability in ranges. For example, one value for wavelengths less than 460 nm, a second value for wavelengths between 460 nm and 640 nm and a third value for wavelengths greater than 640 nm, using the appropriate number of wavelengths in the computation of the multivariate confidence volume.

7.2 Reproducibility shall be measured by collecting readings on a set of at least 10 material standards, including both neutral and chromatic samples. It is important to standardize the instrument before each measurement series. Long term repeatability involves daily measurement of the standard for a period of at least 30 days.

NOTE 1—This shall be 30 measurement days, not 30 calendar days.

7.2.1 Reproducibility shall be reported as either two times the univariate standard deviation of the 30 readings of the reflectance factor $\Delta R_i(2\sigma)$ at the same three wavelengths or as twice the univariate standard deviation of the tristimulus values $\{\Delta X(2\sigma), \Delta Y(2\sigma), \Delta Z(2\sigma)\}$. However, keep in mind that ΔX , ΔY and ΔZ are generally correlated and not independently distributed. Again, to compensate for correlation between tristimulus values or to provide statistics based on uniform color spaces, the reproducibility shall be computed and reported as described in [Annex A1](#).

7.3 Accuracy has to be independently tested on each of the two scales, wavelength and radiometric. The wavelength scale has the advantage that there are physical standards of wavelength that can be utilized by some colorimetric spectrometers. Procedures for verifying the wavelength scale, bandwidth and radiometric scale are described in Practice [E1164](#). Specific additional procedures are given here.

7.3.1 The wavelength scale includes the sampling position (centroid wavelength) and the sampling window width (bandwidth). These are normally tested against physical standards of wavelength such as a discharge lamp or laser line. In very abridged instruments it may not be possible to test directly against a physical standard, so one of two options may be exercised. In option 1, a material standard is used, such as holmium oxide or didymium oxide glasses. In option 2, a modern, digital, direct scanning monochromator is characterized against physical sources and the output intensity is equalized and scanned across the input to the abridged spectrometer.

7.3.2 It is recommended that for sampling frequencies of fewer than 16 points across the visible region (400 nm to 700 nm) the wavelength accuracy and bandwidth or filter fit, be tested and reported at each sampling point. Small numbers of spectral samples are usually more independent and have wider spectral windows making each sample point more critical. For sampling frequencies of 16 or more points it is recommended to report the wavelength scale conformance and bandwidth at three specific wavelengths (450 nm \pm 0.x nm, 550 nm \pm 0.x nm, 650 nm \pm 0.x nm) with bandwidths of ($bw \pm 0.x$ nm). Here the tolerances are twice the sample standard deviation for at

least 10 replicate determinations of the wavelength scale. If there is a significant bias in the scale position, then that shall be reported as well.

7.3.2.1 As indicated in [6.5.2](#), the radiometric scale accuracy is more difficult to assess. White level must be tested by direct comparison to a primary standard of reflectance or transmittance obtained from a suitable standardizing laboratory. The result shall be reported along with the expanded uncertainty, as described in [6.5.2](#).

7.3.2.2 The results of the measurements of the white level can be reported as 100 % \pm U %. Using white ceramic plaques with luminous reflectance factors (Y) of 85 or greater, the 100 % level expanded uncertainty will be in the range of ± 0.3 % or the uncertainty of the primary standard, whichever is larger. NPL currently cites uncertainties of ± 0.5 % (2σ) and NIST cites uncertainties of ± 0.3 % (2σ) on white primary standards of reflectance.

7.3.2.3 As indicated in [6.5.3](#), the black level needs only to be tested to the extent to show that the optical zero is less than some value. The results of measurements of a near black material or a black trap shall be less than 0.0005 (that is, 0.05 %).


7.3.2.4 As indicated in [6.5.4](#), the linearity must be evaluated using neutral standards. The five neutral BCRA tiles, the three grays (Pale, Mid, Deep) and the White and Black are recommended for this.¹⁰ The plaques must have standard values assigned to them. Lines are to be passed through each sequential pair of the measured points. The slopes of each line segment shall be compared to the expected value of 1.0. [Fig. 1](#) illustrates that the readings from the five BCRA neutral tiles create four intermediate linear regions. If lines are passed through each of these and the slopes of each compared then differential non-linearities will be seen. Plot or tabulate the results for each line segment: the accepted values for the slope (always 1.0); the measured values for the slopes; and the percent difference between the two. The report shall include the maximum absolute difference \pm combined uncertainty in the slope due to uncertainty in the accepted values and the measured values.

7.4 Between Instrument Agreement must report whether the test is for inter-model instrument agreement or inter-instrument agreement. The two types of reproducibility are tested in a similar manner but the results are evaluated quite differently. The difference between these two parameters can be as large as an order of magnitude.

7.4.1 To estimate this reproducibility calculate the mean CIELAB component differences between the readings of a set of at least 10 BCRA tiles plus white and black plaques. The measurement conditions (temperature, humidity, etc.) shall be specified and corrected to standard conditions via the NPL table, reproduced in [Annex A2](#).¹¹ As observed in [Fig. 2](#), the distribution of a set of color difference (ΔE) determinations

¹⁰ BCRA tiles are produced by Lucideon Ltd. (previously CERAM Research), Queens Road, Penkhull, Stoke-on-Trent, ST4 7LQ, England. The tiles are available for various vendors in the USA and UK.

¹¹ Verrill, J. F., Compton, J. A., and Malkin, F., *Applied Optics*, Vol. 25, 1986, p. 3011.

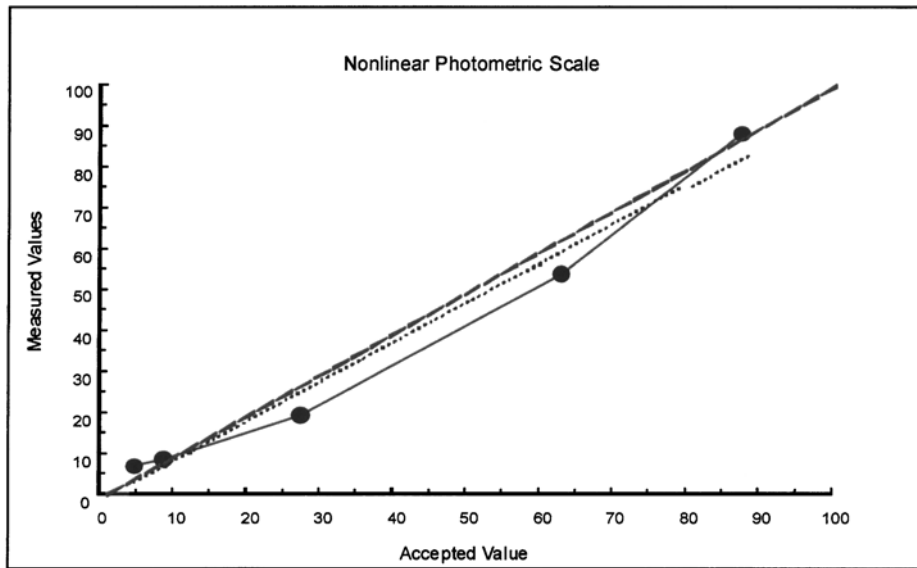

NOTE 1—Solid line is ideal, dotted line show zero and a scale error, and points show nonlinear scale.

FIG. 1 Nonlinear Photometric Scale

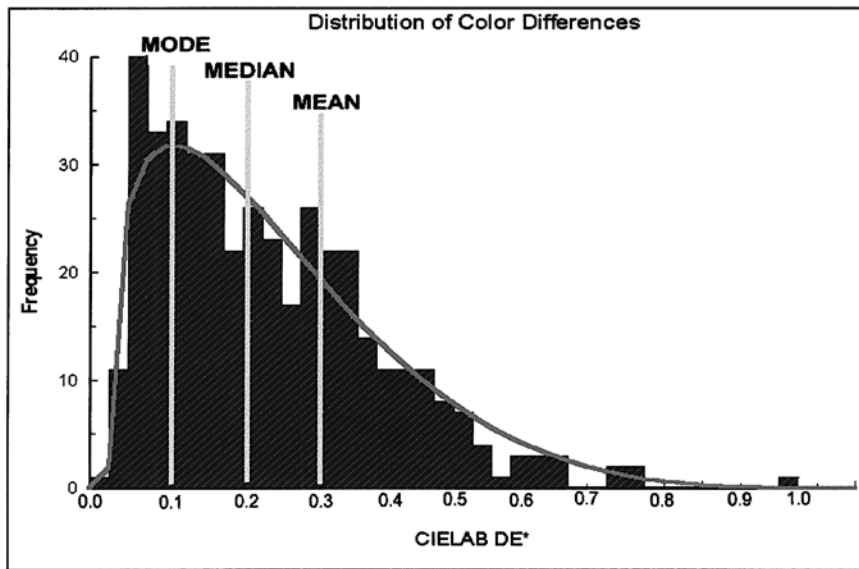


FIG. 2 Comparison of a Large Number of Color Differences Showing Positive Skew Distribution

does not follow a bell curve but a curve related to the Chi distribution, as described by Hotelling.¹²

7.4.1.1 For this positively skewed distribution, if the univariate MODE is reported, then the estimate is highly optimistic, influenced by the easily characterized neutral samples. On the other hand, if the univariate MEDIAN is used then fully half of the readings are above and half below the modal color difference. Finally, the mean (arithmetic average) is highly influenced by the largest color differences in the tail of the distribution. The maximum of the readings is highly dependent on the sample character and the measurement

conditions—the maximum will be large for difficult to measure specimens and small for easily characterized specimens.

7.4.2 Spectral ratios or spectral differences can be used to quantify the spectral and radiometric differences between instruments, but geometric differences are confounded with the radiometric differences and thus provide additional information only for inter-model instrument agreement or for comparison of spectrally non-selective specimens.¹³

7.4.3 The most appropriate and conservative estimate of the expected difference between the two instruments is the 3D

¹² Hotelling, H., "The Generalization of the Student's Ratio," *Annals of Mathematical Statistics*, Vol. 2, 1931, pp. 360-378.

¹³ Robertson, A. R., *Advances in Standards and Methodology in Spectrophotometry*, Burgess, C., and Mielenz, K. D., eds., Elsevier, Amsterdam, 1987, pp. 277-286.

ellipsoidal confidence interval on the joint distribution of measurements from the two instruments. If an estimate of the dispersion of the color differences is required, then compute the variance-covariance matrix and report this or the individual component contributions are described in [Annex A1](#). Replicate readings at different times can provide an even better estimate of the expected performance of the instruments under test. The test can be extended to multiple instruments with complete generality, creating a multivariate analysis of variance (MANOVA) problem. The solution of that comparison is

beyond the scope of this standard but can be found in most elementary textbooks on multivariate analysis and in any good statistical software package.

8. Keywords

8.1 color; instrumental measurement-color/light; inter-instrument; inter-model; light-transmission and reflection; reflectance; reflectance and reflectivity; spectrophotometry; spectrophotometry

ANNEXES

(Mandatory Information)

A1. MULTIVARIATE ANALYSIS OF COLOR READINGS

A1.1 Estimates of the Mean Vector and Variance Matrix

A1.1.1 Given a set of n color readings, either repeatability or reproducibility readings of a single specimen expressed in terms of CIELAB color coordinates (L^* , a^* , b^*), compute the following:

$$\text{cov}(L^*, a^*) = \frac{1}{n-1} \sum (L_i^* - \bar{L}^*) \cdot (a_i^* - \bar{a}^*)$$

$$\bar{L}^* = \frac{1}{n} \sum L_i^*, \bar{a}^* = \frac{1}{n} \sum a_i^*, \bar{b}^* = \frac{1}{n} \sum b_i^*$$

$$\text{var}(L^*) = \frac{1}{n-1} \sum (L_i^* - \bar{L}^*)^2$$

$$\text{var}(a^*) = \frac{1}{n-1} \sum (a_i^* - \bar{a}^*)^2$$

$$\text{var}(b^*) = \frac{1}{n-1} \sum (b_i^* - \bar{b}^*)^2$$

$$\text{cov}(L^*, b^*) = \frac{1}{n-1} \sum (L_i^* - \bar{L}^*) \cdot (b_i^* - \bar{b}^*)$$

$$\text{cov}(a^*, b^*) = \frac{1}{n-1} \sum (a_i^* - \bar{a}^*) \cdot (b_i^* - \bar{b}^*)$$

A1.1.2 The mean vector is given by:

$$w = \begin{bmatrix} \bar{L}^* \\ \bar{a}^* \\ \bar{b}^* \end{bmatrix}$$

A1.1.3 The variance-covariance matrix is given by:

$$V = \begin{bmatrix} \text{var}(L^*) & \text{cov}(L^*, a^*) & \text{cov}(L^*, b^*) \\ \text{cov}(L^*, a^*) & \text{var}(a^*) & \text{cov}(a^*, b^*) \\ \text{cov}(L^*, b^*) & \text{cov}(a^*, b^*) & \text{var}(b^*) \end{bmatrix}$$

A1.2 Application of Multivariate Analysis to Colorimetry

A1.2.1 As stated in [7.1.1](#) of the main text, the tristimulus values X , Y , Z measured by spectrophotometers have distributions that are close to normal. Because the colorimetric errors are small, derived values such as L^* , a^* , b^* will also be tightly enough constrained so the deviations in L^* , a^* , b^* are approximately linearly related to those of X , Y , Z and hence also close to normally distributed. Accordingly, random errors of func-

tions of L^* , a^* , b^* can be propagated by means of partial derivatives, as will be done in this Annex.

A1.2.2 For colorimetric measurements that are normally distributed, standard deviations and critical values can be derived from the mean vector (w) and the variance-covariance matrix (V). The mean vector and variance matrix can be calculated for a set of individual readings, as shown above, or for a set of color difference readings (Batch-Standard). The variance-covariance matrix is the same whether calculated from individual readings, or from individual readings with a common standard value subtracted. Standard deviations for coordinates are as given in [Table A1.1](#).

A1.2.3 CIELAB components ΔL^* , Δa^* , Δb^* , and derived differences ΔC^* , Δh^* , and ΔH^* are also one-dimensional comparisons. Hence, repeatability and reproducibility are expressible by a standard deviation. For derived differences ΔC^* , Δh^* , and ΔH^* , the standard deviations can be derived from the variance-covariance matrix of (ΔL^* , Δa^* , Δb^*).

A1.2.4 The CIELAB color difference ΔE^* is an intrinsically trivariate measure. If ΔE^* equals zero, then all other component differences are zero. Repeatability and reproducibility, in terms of ΔE^* , is not a standard deviation but is the root mean square value.

A1.3 Example Calculations

A1.3.1 Raw data table.

$$\bar{L}^*_{Std} = 98.04, \bar{a}^*_{Std} = -0.02, \bar{b}^*_{Std} = 1.78$$

Sample Number	ΔL^*	Δa^*	Δb^*
1	-0.82	-0.02	0.36
2	-0.89	-0.01	0.37
3	-0.73	-0.04	0.36
4	-0.91	-0.08	0.35
5	-0.91	-0.16	0.36
6	-0.63	0.02	0.31
7	-0.64	-0.01	0.35
8	-0.81	-0.02	0.35
9	-0.60	-0.08	0.45
10	-0.68	-0.01	0.38
11	-0.61	0.00	0.38
12	-0.71	-0.07	0.40

Sample Number	ΔL^*	Δa^*	Δb^*
13	-0.93	0.03	0.33
14	-0.99	0.02	0.27
15	-0.70	-0.09	0.41
16	-0.87	-0.01	0.34
17	-0.79	-0.01	0.38
18	-0.78	-0.09	0.39
19	-0.67	-0.05	0.43
20	-0.74	-0.04	0.38
Averages	-0.771	-0.036	0.368

Component	Repeatability (2s)
-----------	--------------------

ΔL^*	$2\sqrt{v_{11}} = 0.235$
--------------	--------------------------

Δa^*	$2\sqrt{v_{22}} = 0.094$
--------------	--------------------------

Δb^*	$2\sqrt{v_{33}} = 0.080$
--------------	--------------------------

$$\Delta h_{ab}^* = 2 \frac{180}{\pi} \sqrt{(\bar{b}^2 v_{22} + \bar{a}^2 v_{33} - 2\bar{a}\bar{b}v_{23})/\bar{C}^4} = 2.5^\circ$$

$$\Delta H_{ab}^* = 2\sqrt{(\bar{b}^2 v_{22} + \bar{a}^2 v_{33} - 2\bar{a}\bar{b}v_{23})/\bar{C}^2} = 0.093$$

$$\Delta C_{ab}^* = 2\sqrt{(\bar{a}^2 v_{22} + \bar{b}^2 v_{33} + 2\bar{a}\bar{b}v_{23})/\bar{C}^2} = 0.082$$

$$\Delta E_{ab}^* = 2\sqrt{v_{11} + v_{22} + v_{33}} = 0.266$$

A1.3.2

$$\overline{\Delta H^*} = \frac{-0.02 \cdot 2.148 - 1.78 \cdot (-0.056)}{\sqrt{(2.1487 \cdot 1.7801 + (-0.056) \cdot (-0.02) + 2.148 \cdot 1.78)/2}} = 0.029$$

$$\bar{L}_{Trial}^* = 98.04 + (-0.771) = 97.27$$

$$\bar{a}_{Trial}^* = -0.02 + (-0.036) = -0.056$$

$$\bar{b}_{Trial}^* = 1.78 + (0.368) = 2.148$$

$$\overline{\Delta E^*} = \sqrt{(-0.771)^2 + (-0.036)^2 + (0.368)^2} = 0.86$$

$$\overline{\Delta C^*} = \sqrt{(-0.056)^2 + (2.148)^2} - \sqrt{(-0.02)^2 + (1.78)^2} = 0.37$$

$$\Delta h_{ab}^* = \text{atan} \frac{2.148}{-0.056} - \text{atan} \frac{1.78}{-0.02} = 0.85^\circ$$

$$\text{var}(\Delta L^*) = v_{11} = \frac{1}{20-1} \sum (\Delta L_i^* - \overline{\Delta L^*})^2 = 0.013805$$

$$\text{var}(\Delta a^*) = v_{22} = \frac{1}{20-1} \sum (\Delta a_i^* - \overline{\Delta a^*})^2 = 0.002225$$

$$\text{var}(\Delta b^*) = v_{33} = \frac{1}{20-1} \sum (\Delta b_i^* - \overline{\Delta b^*})^2 = 0.001620$$

$$\begin{aligned} \text{cov}(\Delta L^*, \Delta a^*) &= v_{12} = v_{21} = \frac{1}{20-1} \sum (\Delta a_i^* - \overline{\Delta a^*}) \cdot (\Delta L_i^* - \overline{\Delta L^*}) \\ &= -0.000114 \end{aligned}$$

$$\begin{aligned} \text{cov}(\Delta L^*, \Delta b^*) &= v_{13} = v_{31} = \frac{1}{20-1} \sum (\Delta b_i^* - \overline{\Delta b^*}) \cdot (\Delta L_i^* - \overline{\Delta L^*}) \\ &= 0.002741 \end{aligned}$$

$$\begin{aligned} \text{cov}(\Delta a^*, \Delta b^*) &= v_{23} = v_{32} = \frac{1}{20-1} \sum (\Delta a_i^* - \overline{\Delta a^*}) \cdot (\Delta b_i^* - \overline{\Delta b^*}) \\ &= 0.001000 \end{aligned}$$

$$w = \begin{bmatrix} -0.771 \\ -0.036 \\ 0.368 \end{bmatrix}$$

$$V = \begin{bmatrix} 0.013805 & -0.000114 & 0.002741 \\ -0.000114 & 0.002225 & -0.001000 \\ 0.002741 & -0.001000 & 0.001620 \end{bmatrix}$$

A1.3.3 Using the formulas in **Table A1.1**, we compute repeatability (2s) of each of the color difference components.

A1.4 Inter-Instrument Agreement

A1.4.1 Inter-instrument agreement is tested using the Hotelling T^2 statistic for comparing two sets of multivariate observations. Calculate first the mean vectors and covariance matrices w_1, V_1, w_2, V_2 . The test statistic is

$$T^2 = \frac{n_1 n_2}{n_1 + n_2} (w_1 - w_2)' V^{-1} (w_1 - w_2)$$

where:

$$V = \frac{(n_1 - 1)V_1 + (n_2 - 1)V_2}{n_1 + n_2 - 2}$$

is the pooled variance-covariance matrix.

A1.4.2 The critical region for the test statistic is related to the F distribution with $(3, n_1 + n_2 - 4)$ degrees of freedom.

$$T^2 > \frac{3(n_1 + n_2 - 2)}{n_1 + n_2 - 4} F_{0.95}(3, n_1 + n_2 - 4)$$

A1.4.3 When a significant difference between instruments is found, confidence intervals for the difference in terms individual color components are useful to evaluate the components contributing to the difference. These are

$$\begin{aligned} \overline{\Delta L_1^*} - \overline{\Delta L_2^*} \pm t_{0.975} (n_1 + n_2 - 2) \sqrt{v_{11}(1/n_1 + 1/n_2)} \\ \overline{\Delta a_1^*} - \overline{\Delta a_2^*} \pm t_{0.975} (n_1 + n_2 - 2) \sqrt{v_{22}(1/n_1 + 1/n_2)} \\ \overline{\Delta b_1^*} - \overline{\Delta b_2^*} \pm t_{0.975} (n_1 + n_2 - 2) \sqrt{v_{33}(1/n_1 + 1/n_2)} \end{aligned}$$

where v_{11}, v_{22}, v_{33} are the diagonal elements of the pooled variance-covariance matrix V , and $t_{0.975}(n_1+n_2-2)$ is the 0.975 or two-sided 95 % percentile of the Student's t distribution with (n_1+n_2-2) degrees of freedom.

TABLE A1.1 Formulas for Coordinate Standard Deviations

NOTE 1—As tabulated here, the arctangent formula for h as a function of a* and b*, tan⁻¹(b*/a*), is a shorthand for a four-quadrant arctangent that has the range [0, 360] degrees. Computation of h or of Δh* is recommended only outside the 0.1-radius domain about a*, b* = 0. The following pseudo-code applies.

if b* = 0 then
 h = 90 – 90 sign(a*)
 else
 h = 180 – (180/π) tan⁻¹(a*/b*) – 90 sign(b*)

NOTE 2—The formula for ΔH*_{ab} is valid only when neither of the compared chroma values is zero. ΔH*_{ab} = 0 when either C = 0 or C₀ = 0.

Color Coordinate	Formula	Standard Deviation (s)
ΔL*	$L - L_0$	$\sqrt{V_{11}}$
Δa*	$a - a_0$	$\sqrt{V_{22}}$
Δb*	$b - b_0$	$\sqrt{V_{33}}$
Δh* _{ab}	$\frac{180}{\pi} \left[\tan^{-1}\left(\frac{b}{a}\right) - \tan^{-1}\left(\frac{b_0}{a_0}\right) \right]$	$\sqrt{\delta^* V \delta}$ $\delta = \begin{bmatrix} \partial h^*/\partial L \\ \partial h^*/\partial a \\ \partial h^*/\partial b \end{bmatrix} = \frac{180}{\pi} \begin{bmatrix} 0 \\ -b^*/C^{*2} \\ a^*/C^{*2} \end{bmatrix}$
ΔH* _{ab}	$\frac{a_0 b - b_0 a}{\sqrt{(C C_0 + a a_0 + b b_0)/2}}$	$\sqrt{\delta^* V \delta}$ $\delta = \begin{bmatrix} \partial \Delta H^*/\partial L \\ \partial \Delta H^*/\partial a \\ \partial \Delta H^*/\partial b \end{bmatrix} = \begin{bmatrix} 0 \\ -b^*/C^* \\ a^*/C^* \end{bmatrix}$
ΔC* _{ab}	$\sqrt{a^2 + b^2} - \sqrt{a_0^2 + b_0^2}$	$\sqrt{\delta^* V \delta}$ $\delta = \begin{bmatrix} \partial C^*/\partial L \\ \partial C^*/\partial a \\ \partial C^*/\partial b \end{bmatrix} = \begin{bmatrix} 0 \\ a^*/C^* \\ b^*/C^* \end{bmatrix}$
ΔE* _{ab}	$\sqrt{(\Delta L^*)^2 + (\Delta a^*)^2 + (\Delta b^*)^2}$	root mean square $= \sqrt{V_{11} + V_{22} + V_{33}}$

A2. TEMPERATURE DEPENDENCE OF BCRA CERAMIC TILES

A2.1 The NPL and CERAM have studied the temperature sensitivity of the Ceramic Colour Standards, Series II and have published the following tables of changes in the CIELAB coordinates for a 10°C rise in ambient temperature or the temperature at the surface of the tile.

A2.2 To correct a color measurement to a specific temperature use the following equation:

$$C_{CORRECTED} = C_{MEASURED} + \left(\Delta T_C \times \frac{T_C - T_M}{10} \right)$$

Where C_{CORRECTED} is the corrected color coordinates (L*, a*, b*), C_{MEASURED} is the measured color coordinate, ΔT_C is the thermochromic coefficient from either Table A2.1 or Table A2.2, T_M is the temperature at which the measurement was

made, and T_C is the temperature to which the color measurement is to be corrected.

Example: Suppose the Yellow tile had been measured at 22.5° C using (8°/t) geometry and resulted in the following CIELAB values (D65/1964) L* = 83.50, a* = 1.73, b* = 77.17. Correct the readings to a standard temperature of 25°C. The calculations are thus:

$$L^* = 83.50 + \left(-0.27 \times \frac{(25 - 22.5)}{10} \right) = 83.43$$

$$a^* = 1.73 + \left(0.70 \times \frac{(25 - 22.5)}{10} \right) = 1.91$$

$$b^* = 77.17 + \left(-0.11 \times \frac{(25 - 22.5)}{10} \right) = 77.14$$

TABLE A2.1 Changes for 10°C Rise in Temperature for Illuminant D65 and the 1964 Standard Observer when Measured with 8°/t (Specular Component Included) Geometry

Tile Color	ΔL^*	Δa^*	Δb^*	ΔE^*
Pale Grey	-0.03	-0.02	0.02	0.04
Mid Grey	-0.03	-0.02	0.04	0.05
Difference Grey	-0.04	0.04	0.03	0.06
Deep Grey	0.00	0.01	0.00	0.01
Deep Pink	-0.10	-0.44	-0.19	0.48
Red	-0.37	-0.71	-0.61	1.01
Orange	-0.45	0.56	-0.66	0.97
Yellow	-0.27	0.70	-0.11	0.76
Green	-0.18	0.66	-0.04	0.68
Difference Green	-0.18	0.69	-0.05	0.72
Cyan	-0.10	0.31	0.01	0.32
Deep Blue	0.00	-0.04	0.05	0.06

TABLE A2.2 Changes for 10°C Rise in Temperature for Illuminant D65 and the 1964 Standard Observer when Measured with 0°/d (Specular Component Excluded) Geometry

Tile Color	ΔL^*	Δa^*	Δb^*	ΔE^*
Pale Grey	-0.03	-0.02	0.03	0.04
Mid Grey	-0.03	-0.03	0.04	0.06
Difference Grey	-0.04	0.04	0.03	0.07
Deep Grey	0.00	0.01	0.00	0.01
Deep Pink	-0.13	-0.48	-0.23	0.55
Red	-0.55	-0.54	-0.83	1.13
Orange	-0.49	0.65	-0.67	1.06
Yellow	-0.29	0.74	0.02	0.79
Green	-0.20	0.75	-0.03	0.77
Difference Green	-0.20	0.77	-0.03	0.80
Cyan	-0.12	0.34	0.00	0.36
Deep Blue	0.01	-0.09	0.08	0.12

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>