



Standard Practice for Calibration of Fixed-Cell Differential Scanning Calorimeters¹

This standard is issued under the fixed designation E2603; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This practice covers the calibration of fixed-cell differential scanning calorimeters over the temperature range from -10 to $+120^{\circ}\text{C}$.

1.2 The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* Specific precautionary statements are given in Section 7.

2. Referenced Documents

2.1 *ASTM Standards:*²

[E473 Terminology Relating to Thermal Analysis and Rheology](#)

[E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

[E967 Test Method for Temperature Calibration of Differential Scanning Calorimeters and Differential Thermal Analyzers](#)

[E968 Practice for Heat Flow Calibration of Differential Scanning Calorimeters](#)

[E1142 Terminology Relating to Thermophysical Properties](#)

3. Terminology

3.1 Specific technical terms used in this practice are defined in Terminologies [E473](#) and [E1142](#), including *differential scanning calorimeter*, *enthalpy*, *Kelvin*, and *transformation temperature*.

¹ This practice is under the jurisdiction of ASTM Committee [E37](#) on Thermal Measurements and is the direct responsibility of Subcommittee [E37.09](#) on Microcalorimetry.

Current edition approved May 1, 2015. Published August 2015. Originally approved in 2008. Last previous edition approved in 2008 as E2603 – 08. DOI: 10.1520/E2603-15.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

4. Summary of Practice

4.1 This practice covers calibration of fixed-cell differential scanning calorimeters. These calorimeters differ from another category of differential scanning calorimeter in that the former have generally larger sample volumes, slower maximum temperature scan rate capabilities, provision for electrical calibration of heat flow, and a smaller range of temperature over which they operate. The larger sample cells, and their lack of disposability, make inapplicable the calibration methods of Practices [E967](#) and [E968](#).

4.2 This practice consists of heating the calibration materials in aqueous solution at a controlled rate through a region of known thermal transition. The difference in heat flow between the calibration material and a reference material, both relative to a heat reservoir, is monitored and continuously recorded. A transition is marked by the absorption or release of energy by the specimen resulting in a corresponding peak in the resulting curve.

4.3 The fixed-cell calorimeters typically, if not always, have electrical heating facilities for calibration of the heat-flow axis. Despite the use of resistance heating for calibration, a chemical calibration serves to verify the correct operation of the calibration mechanism and the calorimeter. The thermal denaturation of chicken egg white lysozyme is used in this practice for verification of the proper functioning of the instrument's systems. The accuracy with which the denaturation enthalpy of chicken egg white lysozyme is currently known, $\pm 5\%$, is such that it should be rare that a calorimeter provides a value outside that established in the literature for this reference material.

5. Significance and Use

5.1 Fixed-cell differential scanning calorimeters are used to determine the transition temperatures and energetics of materials in solution. For this information to be accepted with confidence in an absolute sense, temperature and heat calibration of the apparatus or comparison of the resulting data to that of known standard materials is required.

5.2 This practice is useful in calibrating the temperature and heat flow axes of fixed-cell differential scanning calorimeters.

6. Apparatus

6.1 Apparatus shall be:

6.1.1 *Differential Scanning Calorimeter (DSC)*, capable of heating a test specimen and a reference material at a controlled rate and of automatically recording the differential heat flow between the sample and the reference material to the required sensitivity and precision.

6.1.2 *DSC Test Chamber*, composed of:

6.1.2.1 A device(s) to provide uniform controlled heating or cooling of a specimen and reference to a constant temperature or at a constant rate within the applicable temperature range of this method.

6.1.2.2 A temperature sensor to provide an indication of the specimen temperature to ± 0.01 K.

6.1.2.3 Differential sensors to detect a heat flow (power) difference between the specimen and reference with a sensitivity of $\pm 0.1 \mu\text{W}$.

6.1.3 A *Temperature Controller*, capable of executing a specific temperature program by operating the furnace(s) between selected temperature limits at a rate of temperature change of 0.01 K/min to 1 K/min constant to ± 0.001 K/min or at an isothermal temperature constant to ± 0.001 K.

6.1.4 A *Data Collection Device*, to provide a means of acquiring, storing, and displaying measured or calculated signals, or both. The minimum output signals required for DSC are heat flow, temperature, and time.

6.1.5 *Containers*, that are inert to the specimen and reference materials and that are of suitable structural shape and integrity to contain the specimen and reference in accordance with the specific requirements of this test method. These containers are not designed as consumables. They are either an integral part of the instrument, whether or not user-removable for replacement or, in some implementations, are removable and reusable. Container volumes generally range from 0.1 ml to 1 ml, depending on the instrument's manufacture.

6.2 *Analytical Balance*, capable of weighing to the nearest 0.1 mg, for preparation of solutions.

6.3 *UV spectrophotometer or UV/Vis spectrophotometer*, capable of scanning the UV spectrum in a region about 280 nm.

6.4 *Reagents*:

6.4.1 *Phosphatidylcholines*, 1,2-ditridecanoyl-*sn*-glycero-3-phosphocholine (DTPC) CAS Number 71242-28-9 and 1,2-ditetradecanoyl-*sn*-glycero-3-phosphocholine (DLPC) CAS Number 91742-11-9 are the minimum required.

6.4.2 *Aqueous buffer solutions*, 0.01 Molar, pH 7 aqueous solution of $\text{Na}_2\text{HPO}_4 - \text{NaH}_2\text{PO}_4$ and 0.1 Molar, pH (2.4 \pm 0.1) aqueous solution of HCl + glycine.

6.4.3 *Chicken egg white lysozyme*.

7. Precautions

7.1 This practice assumes linear temperature indication. Care must be taken in the application of this practice to ensure that calibration points are taken sufficiently close together so that linear temperature indication may be approximated.

8. Calibration Materials

8.1 Phosphatidylcholines: 1,2-ditridecanoyl-*sn*-glycero-3-phosphocholine (DTPC) CAS Number 71242-28-9; and 1,2-ditetradecanoyl-*sn*-glycero-3-phosphocholine (DLPC) CAS

Number 91742-11-9. Purities are to be 0.99 or better. Additional calibration materials are listed in **Table 1**.

8.1.1 Aqueous suspensions of the phosphatidylcholines are prepared as follows. Weighed amounts of a 0.01 Molar, pH 7 solution of the buffer $\text{Na}_2\text{HPO}_4 - \text{NaH}_2\text{PO}_4$ and DTPC are combined so to give a solution of 1 mass percent of the phosphatidylcholine. This procedure is repeated for DLPC. The solutions are heated in a hot water bath to 5 K above the transition temperatures. A vortex mixer is used to shake the solutions at their respective temperatures until the lipid appears to have been completely suspended. The solutions may be stored in a refrigerator until use for up to a week.

8.2 Chicken egg white lysozyme with purity of at least 95 % mass percent.

8.2.1 Weighed amounts of the lysozyme and of a 0.1 M HCl – glycine buffer at pH = (2.4 \pm 0.1) are combined to obtain a solution of approximately 3 mass percent.

8.2.2 The concentration of lysozyme in this solution is calculated from UV absorbance at a wavelength of 280 nm, using a 1 cm cell and the optical density of 2.65 for a 1 mg mL⁻¹ solution.

8.2.2.1 Fill a 1 cm optical cell with buffer solution and another 1 cm cell with the lysozyme solution. Follow the instrument's directions for establishing baseline, and if needed, calibration of the absorbance scale. Insert both of the filled cells in the UV spectrometer if the spectrometer is a dual beam instrument. Scan through the 280 nm region and note the absorbance at 280 nm. If the spectrometer is a single beam instrument, the buffer is measured first, then the lysozyme solution is measured and the difference in the recorded absorbances is used to calculate the concentration. Concentration is calculated as:

$$c = A / (2.65 \text{ mL mg}^{-1})$$

where:

A = absorbance, and

c = concentration in mg mL⁻¹.

NOTE 1—Different concentrations may be used between 1 and 10 mass percent, the concentration used shall be included in the report.

9. Procedure

9.1 *Two Point Temperature Calibration*:

9.1.1 Determine the apparent transition temperature for each calibration material, as described in **Table 1**.

9.1.1.1 Fill the clean specimen cell with the phosphatidylcholine suspension, according to the usual method specified for

TABLE 1 Melting Temperature of Calibration Material

NOTE 1—The uncertainties for the temperatures are ± 0.1 K.

Calibration Material	Melting Temperature	
	°C	K
1,2-ditridecanoyl- <i>sn</i> -glycero-3-phosphocholine (DTPC)	13.25	286.4
1,2-ditetradecanoyl- <i>sn</i> -glycero-3-phosphocholine (DMPC)	23.75	296.9
1,2-dihexadecanoyl- <i>sn</i> -glycero-3-phosphocholine (DPPC)	41.45	314.6
1,2-dioctadecanoyl- <i>sn</i> -glycero-3-phosphocholine (DSPC)	54.85	328.0
1,2-dieicosanoyl- <i>sn</i> -glycero-3-phosphocholine (DAPC)	65.05	338.2
1,2-didocosanoyl- <i>sn</i> -glycero-3-phosphocholine (DBPC)	73.35	346.5
1,2-ditetradecanoyl- <i>sn</i> -glycero-3-phosphocholine (DLPC)	80.55	353.7

the instrument. Fill the reference cell with buffer solution that was used to prepare the phosphatidylcholine suspension.

9.1.1.2 Equilibrate the calorimeter approximately 10 K to 15 K below the expected transition temperature from **Table 1**.

9.1.1.3 Heat each calibration material at the desired scan rate through the transition until the baseline is reestablished above the transition. Record the resulting thermal curve.

NOTE 2—Temperature scale calibration may be affected by temperature scan rate and by the time-constant of the instrument.

9.1.2 From the resultant curve, measure the temperature for the maximum of the heat flow, T_p . See **Fig. 1**.

9.1.3 Using the apparent transition temperatures thus obtained, calculate the slope (S) and intercept (I) of the calibration **Eq 1** (see Section 10). The slope and intercept values reported should be mean values from duplicate determinations based on separate specimens.

9.2 One-Point Temperature Calibration:

9.2.1 If the slope value (S) previously has been determined in **9.1** (using the two-point calibration calculation in **10.2**) to be sufficiently close to 1.0000, a one-point calibration procedure may be used.

NOTE 3—If the slope value differs by only 1 % from linearity (that is, $S < 0.9900$ or $S > 1.0100$), a 0.5 K error will be produced if the test temperature differs by 50 K from the calibration temperature.

9.2.2 Select a calibration material from **Table 1**. The calibration temperature should be centered as close as practical within the temperature range of interest.

9.2.3 Determine the apparent transition temperatures of the calibration material using steps **9.1.1.1 – 9.1.1.3**.

9.2.4 Using the apparent transition temperature thus obtained, calculate the intercept (I) of the calibration equation using all available decimal places. The value reported should be a mean value based upon duplicate determinations on separate specimens.

9.3 Enthalpy Calibration:

9.3.1 If recommended by the instrument manufacturer, perform an electrical calibration per the manufacturer’s directions.

9.3.2 Determine the enthalpy of transition for the lysozyme solution.

9.3.2.1 Fill the sample cell with the lysozyme + buffer solution and fill the reference cell with the HCl-glycine buffer solution—taking care that no air bubbles are retained in either of the cells.

9.3.2.2 Equilibrate the calorimeter near room temperature, following equilibration the temperature of the calorimeter is ramped at 60 K/h until a sufficient baseline is established beyond the transition peak.

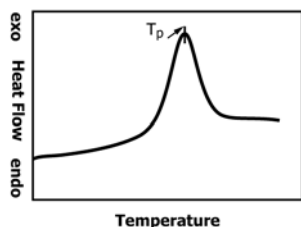


FIG. 1 Example Showing the Temperature of Maximum Heat Flow

NOTE 4—Slower scan rates shall not be used in this step due to potential aggregation of the denatured protein.

9.3.2.3 The enthalpy of the denaturation is calculated by integration, using a two-state transition baseline. This enthalpy is then divided by the mass of sample in the cell. The mass of sample in the cell, m , is calculated as:

$$m = v c$$

where:

v = the volume of the measuring cell in milliliters.

NOTE 5—A two state model refers to a model that assumes the denaturation reaction proceeds from a single native state to a single denatured state. Although the denaturation reaction involves a transition between one manifold of states to another manifold of states, the two-state model adequately represents the average behavior for this protein. The heat capacity of the solution with the native state protein is often significantly different from the heat capacity of the solution with the denatured protein. A two-state transition baseline is one that employs a heat capacity calculated from the thermodynamic progression from one state to the next and the heat capacities of the aqueous solution of the two states of the protein.

9.3.2.4 A second enthalpy of denaturation is calculated using a two-state model and the van’t Hoff equation, which is built into the software packages of most fixed-cell calorimeters.

NOTE 6—Using the two state model, the equations: $Q(T) = \Delta H \cdot x(T)$ $K(T) = x/(1-x)$ define the temperature dependence of the observed curve, if the enthalpy is defined by the van’t Hoff relation: $d \ln K/dT = \Delta H/RT^2$, where Q is the integrated enthalpy observed, ΔH is the enthalpy change for the two-state reaction, K is the equilibrium constant for the reaction, R is the gas constant, x is the fraction of reactant converted to product and T is temperature. The model can be fitted to the curve of apparent heat capacity against temperature. Failure of the two state model occurs from precipitation reactions or other reactions that inhibit a reverse reaction in the thermodynamic equilibrium.

9.4 If practical, adjustment to the temperature scale of the instrument should be made so that temperatures are accurately indicated directly.

10. Calculation

10.1 For the purposes of this procedure, it is assumed that the relationship between observed temperature (TO) and actual specimen temperature (T) is a linear one governed by the following equation:

$$T = TO \times S + I \tag{1}$$

where:

S and I = the slope and intercept, respectively. (See **10.2** for the values for S and I , used in **Eq 1**.)

NOTE 7—For some instruments, the assumption of a linear relation between observed and actual specimen temperature may not hold. Under such conditions, calibration temperatures sufficiently close together shall be used so that the instrument calibration is achieved with a series of linear relations.

10.2 Two-Point Calibration:

10.2.1 Using the standard temperature values taken from **Table 1** and the corresponding observed temperatures taken from experimental **9.1.2**, calculate the slope and intercept using the following equations:

$$S = (TS_1 - TS_2)/(TO_1 - TO_2) \tag{2}$$

$$I = [(TO_1 \times TS_2) - (TS_1 \times TO_2)]/(TO_1 - TO_2) \tag{3}$$

where:

S = slope (nominal value = 1.00),

I = intercept,

TS_1 = reference transition temperature for Standard 1 taken from [Table 1](#),

TS_2 = reference transition temperature for Standard 2 taken from [Table 1](#),

TO_1 = observed transition temperature for Standard 1 determined in [Section 9](#), and

TO_2 = observed transition temperature for Standard 2 observed in [Section 9](#).

NOTE 8— I has the same units (that is, °C or K) as TS_1 , TS_2 , TO_1 , and TO_2 which are consistent with each other. The value for I will be different depending upon the units used. S is a dimensionless number whose value is independent of the units of I and T .

10.2.2 S should be calculated to four significant figures and I should be calculated retaining all available decimal places.

10.3 *One-Point Calibration*—If the slope value determined above is sufficiently close to 1.000, only the intercept need be determined through a one-point calibration procedure.

$$I = TS_1 - TO_1 \quad (4)$$

10.4 Using the determined values for S and I , [Eq 1](#) may be used to calculate the actual specimen transition temperature (T) from an observed transition temperature (TO). Values of T may be rounded to the nearest 0.1°C.

11. Report

11.1 The report shall include the following:

11.1.1 Complete identification and description of the reference materials used including source and purity,

11.1.2 Description of the instrument used for tests,

11.1.3 Statement of the concentrations, pH, and temperature program,

11.1.4 Results of the calibration procedure including values for slope and intercept. Values of S and I shall be reported to the nearest 0.0001.

12. Precision and Bias

12.1 Within laboratory variability may be described using the repeatability value (r) obtained by multiplying the repeatability relative standard deviation by 2.8. The repeatability value estimates the 95 % confidence limit. That is, two results from the same laboratory should be considered suspect (at the 95 % confidence level) if they differ by more than the repeatability value.

12.2 The between laboratory variability may be described using the reproducibility value (R) obtained by multiplying the relative reproducibility standard deviation by 2.8. The reproducibility value estimates the 95 % confidence limit. That is, results obtained by two different laboratories should be considered suspect (at the 95 % confidence level) if they differ by more than the reproducibility value.

12.3 Bias is the difference between the mean value obtained and an accepted reference value for the same material.

12.4 *Precision—Temperature:*

12.4.1 An intralaboratory study was conducted in 1991³ that included seven samples characterized by a single instrument for the within laboratory repeatability of the transition temperature of a series of seven dialkylphosphocholines. This intralaboratory study was conducted elsewhere and does not correspond to ASTM interlaboratory study protocols. Regardless, it gives intralaboratory repeatability estimates based upon a modified treatment of the data similar to Practice [E691](#).⁴

12.4.2 The within laboratory standard deviation was found to be 0.053 K.

12.4.3 The within laboratory repeatability value was found to be 0.15 K.

12.5 *Bias—Temperature:*

12.5.1 The purpose of this standard is to determine the bias in a measurement.

12.5.2 As an example, the bias determined for three materials was found to be −0.24 K, 0.19 K, and 3.2 K.

12.6 *Precision—Enthalpy:*

12.6.1 An interlaboratory study was conducted in 1991⁵ on chicken egg white lysozyme that involved six laboratories and six different models of DSC (laboratories operated more than one model of DSC). This interlaboratory study was conducted elsewhere and does not correspond to the ASTM interlaboratory study protocols of Practice [E691](#). Regardless, the data from five of the laboratories reported in that study may be treated by a modified Practice [E691](#) procedure where the values were weighted for the number of differing number of replicates.⁴

12.6.2 The within laboratory repeatability relative standard deviation was found to be 3.2 %.

12.6.3 The within laboratory repeatability value was found to be 9.0 %.

12.6.4 The between laboratory relative reproducibility standard deviation was found to be 4.4 %.

12.6.5 The between laboratory reproducibility value (R) was found to be 12 %.

12.7 *Bias—Enthalpy:*

12.7.1 The purpose of this standard is to determine the bias in a measurement.

12.7.2 As an example, the accepted value for the enthalpy of transition is 403 kJ/mol.

12.7.3 The mean value for the denaturation of chicken egg white lysozyme is observed to be 405 kJ/mol.

12.7.4 These two values indicate no observable bias in this measurement based upon $R = 12$ %.

³ Schwarz, F. P., "Biological Thermodynamic Data for the Calibration of Differential Scanning Calorimeters: Dynamic Temperature Data on the Gel to Liquid Crystal Phase Transition of Dialkylphosphatidylcholine in Water Suspensions," *Thermochimica Acta*, Vol 177, No. 1, 1991, p. 285–303.

⁴ Supporting data have been filed at ASTM International Headquarters and may be obtained by requesting Research Report RR:E37-1046. Contact ASTM Customer Service at service@astm.org.

⁵ Hinz, H. J., and Schwarz, F. P., "Measurement and Analysis of Results Obtained on Biological Substances with Differential Scanning Calorimetry," *Pure and Applied Chemistry*, Vol 73, No. 4, 2001, p. 745–759.

13. Keywords

13.1 calibration; differential scanning calorimetry; transition temperature

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>