



Designation: E2928/E2928M – 17

# Standard Practice for Examination of Drillstring Threads Using the Alternating Current Field Measurement Technique<sup>1</sup>

This standard is issued under the fixed designation E2928/E2928M; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon ( $\epsilon$ ) indicates an editorial change since the last revision or reapproval.

## 1. Scope

1.1 This practice describes procedures to be followed during alternating current field measurement examination of drillstring threads on tubulars used for oil and gas exploration and production for detection and, if required, sizing of service-induced surface breaking discontinuities transverse to the pipe.

1.2 This practice is intended for use on threads in any metallic material.

1.3 This practice does not establish acceptance criteria. Typical industry practice is to reject these connections on detection of a confirmed crack.

1.4 While the alternating current field measurement technique is capable of detecting discontinuities in these connections, supplemental surface NDT methods such as magnetic particle testing for ferrous metals and penetrant testing for non-ferrous metals may detect more discontinuities.

1.5 *Units*—The values stated in either inch-pound units or SI units are to be regarded separately as standard. The values stated in each system might not be exact equivalents; therefore, each system shall be used independently of the other. Combining values from the two systems may result in nonconformance with the standard.

1.6 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

1.7 *This international standard was developed in accordance with internationally recognized principles on standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.*

<sup>1</sup> This practice is under the jurisdiction of ASTM Committee E07 on Nondestructive Testing and is the direct responsibility of Subcommittee E07.07 on Electromagnetic Method.

Current edition approved June 1, 2017. Published June 2017. Originally approved in 2013. Last previous edition approved in 2013 as D2928/D2928M–13. DOI: 10.1520/E2928\_E2928M–17.

## 2. Referenced Documents

### 2.1 ASTM Standards:<sup>2</sup>

E543 Specification for Agencies Performing Nondestructive Testing

E1316 Terminology for Nondestructive Examinations

E2261 Practice for Examination of Welds Using the Alternating Current Field Measurement Technique

### 2.2 ASNT Standards<sup>3</sup>

SNT-TC-1A Personnel Qualification and Certification in Nondestructive Testing

ANSI/ASNT-CP-189 Standard for Qualification and Certification of Nondestructive Testing Personnel

### 2.3 ISO Standard:<sup>4</sup>

ISO 9712 Non-Destructive Testing: Qualification and Certification of NDT Personnel

## 3. Terminology

3.1 For definitions of terms relating to this practice refer to Terminology E1316, Section A, Common NDT terms, and Section C, Electromagnetic testing. The following definitions are specific to the alternating current field measurement technique:

### 3.2 Definitions:

3.2.1 *detector*—one or more coils or elements used to sense or measure a magnetic field; also known as a receiver.

3.2.2 *exciter*—a device that generates a time varying electromagnetic field, usually a coil energized with alternating current (AC); also known as a transmitter.

3.2.3 *uniform field*—as applied to nondestructive testing with magnetic fields, the area of uniform magnetic field over the surface of the material under examination produced by a parallel induced alternating current, which has been passed

<sup>2</sup> For referenced ASTM standards, visit the ASTM website, [www.astm.org](http://www.astm.org), or contact ASTM Customer Service at [service@astm.org](mailto:service@astm.org). For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

<sup>3</sup> Available from American Society for Nondestructive Testing (ASNT), P.O. Box 28518, 1711 Arlingate Ln., Columbus, OH 43228-0518, <http://www.asnt.org>.

<sup>4</sup> Available from International Organization for Standardization (ISO), ISO Central Secretariat, BIBC II, Chemin de Blandonnet 8, CP 401, 1214 Vernier, Geneva, Switzerland, <http://www.iso.org>.

through the testpiece and is observable beyond the direct coupling of the exciting coil.

### 3.3 Definitions of Terms Specific to This Standard:

3.3.1 *alternating current field measurement system*—the electronic instrumentation, software, probes, and all associated components and cables required for performing an examination using the alternating current field measurement technique.

3.3.2 *box*—the female thread in a drillstring connection.

3.3.3 *B<sub>x</sub>*—the x component of the magnetic field, parallel to the thread root, the magnitude of which is proportional to the current density set up by the electric field.

3.3.4 *B<sub>z</sub>*—the z component of the magnetic field normal to the examined pipe surface, the magnitude of which is proportional to the lateral deflection of the induced currents in the plane of that surface.

3.3.5 *configuration data*—standardization data and instrumentation settings for a particular probe stored in a computer file.

3.3.6 *data sample rate*—the rate at which data is digitized for display and recording, in data points per second.

3.3.7 *longitudinal*—following from the above definition, a longitudinal discontinuity is parallel to the pipe axis and therefore perpendicular to the scan direction.

3.3.8 *operational standardization block*—a reference standard with specified artificial notches, used to confirm the operation of the system.

3.3.9 *pin*—the male thread in a drillstring connection.

3.3.10 *satellite signals*—*B<sub>x</sub>* and *B<sub>z</sub>* signals observed when the probe passes a discontinuity in an adjacent thread root.

3.3.11 *surface plot*—for use with array probes. This type of plot has one component of the magnetic field plotted over an area, typically as a color contour plot or 3-D wire frame plot.

3.3.12 *time base plots*—these plot the relationship between *B<sub>x</sub>* or *B<sub>z</sub>* values with time.

3.3.13 *transverse*—as is normal in drilling, the terms transverse and longitudinal are defined in reference to the pipe axis. Therefore, a transverse discontinuity is parallel to the thread and hence to the scan direction. This is different to the situation for weld inspection, covered in Guide E2261.

3.3.14 *X-Y Plot*—an X-Y graph with two orthogonal components of magnetic field plotted against each other.

NOTE 1—Different equipment manufacturers may use slightly different terminology. Reference should be made to the equipment manufacturer's documentation for clarification.

## 4. Summary of Practices

4.1 In a basic alternating current field measurement system, a small probe is moved around the thread root. The probe contains an exciter coil, which induces an AC magnetic field in the material surface aligned to the direction of the thread root. This, in turn, causes alternating current to flow across the threads. The depth of penetration of this current varies with material type and frequency but is typically 0.004 in. [0.1 mm] deep in magnetic materials and 0.08 to 0.3 in. [2 to 7 mm] deep in non-ferrous materials. Any surface breaking discontinuities

within a short distance of either side of the scan line at this location will interrupt or disturb the flow of the alternating current. Measurement of the absolute quantities of the two major components of the surface magnetic fields (*B<sub>x</sub>* and *B<sub>z</sub>*) determines the severity of the disturbance (see Fig. 1) and thus the severity of the discontinuity. Discontinuity sizes, such as crack length and depth, can be estimated from the values of these quantities or the physical locations of key points, or both, selected from the *B<sub>x</sub>* and *B<sub>z</sub>* traces along with the standardization data and instrument settings from each individual probe. This discontinuity sizing can be performed automatically using system software. Discontinuities essentially perpendicular to the thread may be detected (in ferritic metals only) by the flux leakage effect.

4.2 Configuration data is loaded at the start of the examination. System sensitivity and operation is verified using an operation standardization block. System operation is checked and recorded prior to and at regular intervals during the examination. This can be accomplished using discontinuity-sizing tables in the system software. Data is recorded in a manner that allows archiving and subsequent recall for each thread. Evaluation of examination results may be conducted at the time of examination or at a later date. The examiner generates an examination report detailing complete results of the examination.

## 5. Significance and Use

5.1 The purpose of the alternating current field measurement method is to evaluate threads for surface breaking discontinuities such as fatigue cracks running along the thread root. The examination results may then be used to determine the fate of the tool. This may involve re-examination by an alternative technique, immediate scrapping of the tool, or reworking to remove discontinuities (beyond the scope of this

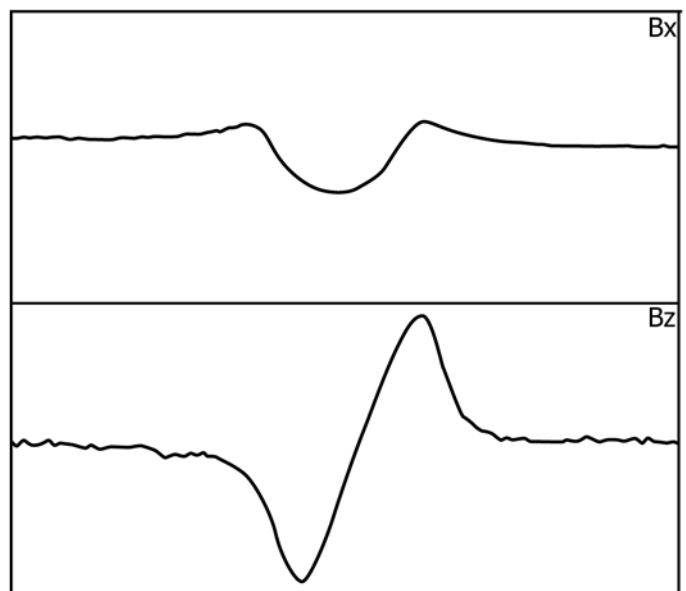


FIG. 1 Example *B<sub>x</sub>* and *B<sub>z</sub>* Traces as a Probe Passes Over a Crack (The orientation of the traces may differ depending upon the instrumentation.)

practice). This practice is not intended for the examination of threads for non-surface breaking discontinuities.

## 6. Basis of Application

6.1 *Personnel Qualification*—if specified in the contractual agreement, personnel performing examinations to this practice shall be qualified in accordance with a nationally or internationally recognized NDT personnel qualification practice or standard such as ANSI/ASNT-CP-189, SNT-TC-1A, ISO 9712, or a similar document and certified by the employer or certifying agent, as applicable. The practice or standard used and its applicable revision shall be identified in the contractual agreement between the using parties

6.2 *Qualification of Nondestructive Evaluation Agencies*—if specified in the contractual agreement, NDT agencies shall be qualified and evaluated as described in Specification E543, with reference to sections on electromagnetic examination. The applicable edition of Specification E543 shall be specified in the contractual agreement.

## 7. Job Scope and Requirements

7.1 The following items may require agreement by the examining party and their client and should be specified in the purchase document or elsewhere:

7.1.1 Location and type of threaded component to be examined, design specifications, degradation history, previous nondestructive examination results, maintenance history, process conditions, and specific types of discontinuities that are required to be detected, if known.

7.1.2 The maximum recommended probe scan speed is to be stated by the manufacturer. However, detection of smaller discontinuities requires a slower probe scan speed or cleaning of surface, or both.

7.1.3 Size, material grade and type, and configuration of threads to be examined.

7.1.4 A thread numbering or identification system.

7.1.5 Extent of examination, for example: complete or partial coverage, which threads and to what extent.

7.1.6 Type of alternating current field measurement instrument and probe; and description of operations standardization block used, including such details as dimensions and material.

7.1.7 Required thread cleanliness.

7.1.8 Environmental conditions, equipment and preparations that are the responsibility of the client; common sources of noise that may interfere with the examination, such as motor drive for rotary table.

7.1.9 Complementary methods or techniques may be used to obtain additional information.

7.1.10 Acceptance criteria to be used in evaluating discontinuities.

7.1.11 Disposition of examination records and reference standards.

7.1.12 Format and outline contents of the examination report.

## 8. Interferences

8.1 This section describes items and conditions, which may compromise the alternating current field measurement technique.

### 8.2 *Material Properties:*


8.2.1 Although there are unlikely to be permeability differences in a ferromagnetic material between different parts of a thread, if a probe is scanned across a permeability change such as an area of residual magnetism, this may produce indications which could be similar to those from a discontinuity. Differentiation between a discontinuity signal and a permeability change signal can be achieved by comparing scans from neighboring threads. The signal from a discontinuity will die away quickly. If there is no significant change in indication amplitude two or more threads away along the pipe axis then the indication is likely due to the permeability changes in the component.

### 8.3 *Magnetic State:*

8.3.1 *Demagnetization*—It must be ensured that the surface being examined is in a low magnetization state, or that any magnetization is uniform over the surface. Therefore the procedure followed with any previous magnetic technique developed must include demagnetization of the surface, or ensuring that connections are magnetically saturated. This is because areas of remnant magnetization, particularly where the leg of a magnetic particle examination yoke was sited, can produce loops in the X-Y plot, which may sometimes be confused with a discontinuity indication.

### 8.4 *Thread Geometry:*

8.4.1 When a probe scans away from the shoulder of a pin connection, the  $B_x$  indication value will decrease with little change in the  $B_z$  value. In the representative plot of Fig. 2, this appears as a drop in the X-Y plot. The  $B_x$  indication value will also decrease as a probe approaches the open end of a thread (pin or box).

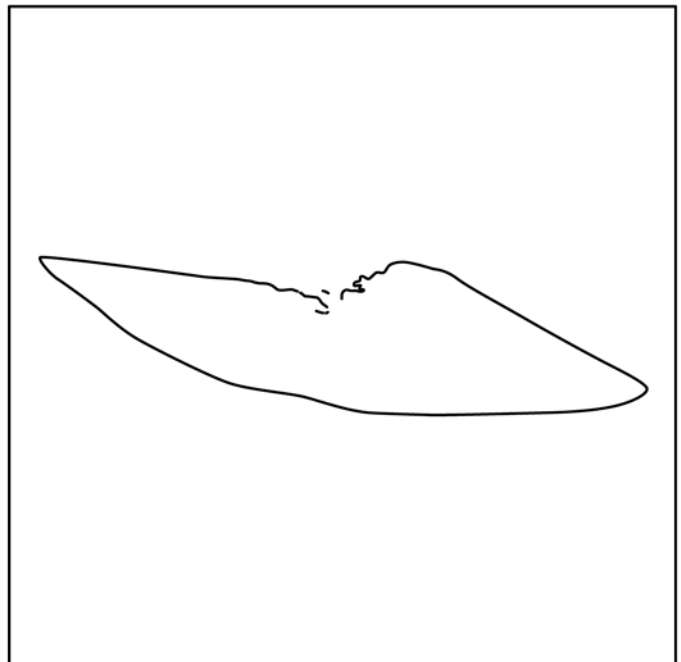

**FIG. 2 Example X-Y Plot Produced by Plotting the  $B_x$  (vertical) and  $B_z$  (horizontal) Together (The orientation of the plot may differ depending upon the instrumentation.)**

### 8.5 Crack Geometry Effects:

8.5.1 Since the effect of a discontinuity on the signals can be detected some distance away, “satellite” signals are observed as the probe passes one thread (or two threads) away from a sufficiently-large discontinuity. The satellite signals will be smaller than the main discontinuity signal, and symmetrically spaced one thread revolution either side. Care should be taken not to classify these signals as additional discontinuities.

8.5.2 A large discontinuity may jump across a thread crown from one root to the neighboring one. This causes a sudden rise in  $B_x$  signal where the discontinuity leaves the root, and a sudden decrease in  $B_x$  signal at the same place in the neighboring thread where the discontinuity enters the root.

8.5.3 *Line Contact*—when contacts occur across a discontinuity then minor loops occur within the main X-Y plot loop produced by the discontinuity. This can be differentiated from adjacent multiple discontinuities when there will be a number of separate loops, each returning to the background level.

8.5.4 *Longitudinal Discontinuities*—in the unlikely event that a discontinuity exists parallel to the pipe axis then the  $B_x$  may rise instead of fall and the  $B_z$  signal will remain the same as for a short transverse discontinuity. The X-Y plot will then go upwards instead of down in the representative plot of Fig. 2. The extent of this flux leakage signal above the surface is related to the opening of the discontinuity, so it may not be seen for tightly closed discontinuities.

### 8.6 Instrumentation:

8.6.1 The operator should be aware of indicators of noise, saturation or signal distortion particular to the instrument being used. Special consideration should be given to the following concerns:

8.6.1.1 The excitation frequency of operation should be chosen to maximize discontinuity sensitivity whilst maintaining acceptable noise levels.

8.6.1.2 Saturation of electronic components is a potential problem in alternating current field measurement because signal amplitude can increase rapidly as a probe is scanned into tight angle geometry, such as a shoulder on a pin. This could cause the  $B_x$  indication to rise above the top of the range of the A/D converter in the instrument. Data acquired under saturation conditions are not acceptable and appear as a flattening of the  $B_x$  response in the representative plots of Fig. 1 at the maximum possible signal value. If saturation conditions are observed, the equipment gain should be reduced until the  $B_x$  value no longer appears to saturate and the examination repeated. After adjusting the equipment gain, an equipment operation check as described in 11.2 is recommended, except that the loop size will be smaller. Note that this gain adjustment does not affect the discontinuity sizing capability.

8.6.2 *Instrument Induced Phase-Offset*—The measurements of magnetic field are at a chosen and fixed phase so that unlike during conventional eddy current examination the phase angle does not need to be considered. The phase is selected at manufacture of the probes and is stored in the probe file and is automatically configured by the instrument.

## 9. Alternating Current Field Measurement System

### 9.1 Instrumentation

9.1.1 The electronic instrumentation shall be capable of energizing the exciter at one or more frequencies appropriate to the thread material. The apparatus shall be capable of measuring the  $B_x$  and  $B_z$  magnetic field amplitudes at each frequency. The instrument will be supplied with a processor, either internally, or in the form of a portable personal computer (PC) that has sufficient system capabilities to support the alternating current field measurement software, which will be suitable for the instrument and probes in use and the examination requirements. The software provides control of the instrumentation including set-up, data acquisition, data display, data analysis and data storage. The software provides algorithms for sizing the discontinuities (see Section 14). The software runs on the processor and, on start up, all communications between the processor and the instrument are automatically checked. When the software starts up, it automatically sets up the instrument connected in the correct mode for alternating current field measurement examination. Configuration data for each probe is stored either on the processor or on the probe and is transmitted to the instrument whenever a probe is selected or changed. This configuration data may include different settings dependent on the thread type and size being examined. For non-magnetic materials, if configuration data is not available from the equipment manufacturer, a standardization may be performed on reference blocks prior to the material examination. Equipment operation is also checked by scanning over a standardization block (see 11.2.2). Once the instrumentation is set up for a particular probe, the software can be used to start and stop data acquisition. During data acquisition at least two presentations of the data are presented on the display screen in real time (see 4.1). Data from the probe is displayed against time (with Fig. 1 as an example) and also as an X-Y plot (with Fig. 2 as an example). The data from the probe can also be displayed against position (see Fig. 1) if an encoder is used with the probe. Depending upon equipment type, manual or automatic position markers may be incorporated with the data. Once collected the data can be further analyzed offline using the software to allow, for example, discontinuity sizing (see Section 14) or annotation for transfer to examination reports. The software also provides facilities for all data collected to be electronically stored for subsequent review or reanalysis, printing or archiving.

### 9.2 Driving Mechanisms:

9.2.1 Ideally, the pipe is placed on a rotary rig such that the pipe can be rotated about its own axis, allowing the probe to move down the axis. In this way, the complete thread can be examined without having to move the probe around the pipe, thus avoiding twisting of the probe cable. Alternatively, if the pipe cannot be rotated, an array probe can be used to examine the complete thread in one turn of the probe.

### 9.3 Probes:

9.3.1 The probes selected should be appropriate for the form of examination to be carried out dependent on thread size, geometry, size of detectable discontinuity and component material.

9.3.1.1 *Universal Thread Probe*—used with interchangeable shoes that are each designed to fit a particular thread size and type. It is important to select the correct shoe for the thread to be examined to avoid excessive lift-off or probe rock, and probe wear.

9.3.1.2 *Array Probe*—made up of a number of elements; each element is sensitive to a discrete section of the thread (typically a single root, but may be part of a root for large threads). The array probe is generally used for scanning a complete thread in one full rotation. The probe may have interchangeable scrapers to fit a particular thread size. In this case, it is important to select the correct scrapers for the thread to be examined to avoid excessive lift-off or probe rock, and probe wear.

#### 9.4 Data Displays:

9.4.1 The data display should include  $B_x$  and  $B_z$  indications as well as an X-Y plot.

9.4.2 When multi-element array probes are being used, the facility to produce color contour maps or 3-D wire frame plots representing peaks and troughs should be available.

#### 9.5 Excitation Mechanism:

9.5.1 The degree of uniformity of the magnetic field applied to the material under examination is determined by the equipment manufacturer. The geometry of the notches used in the operation standardization block and the discontinuity sizing model must be consistent with the excitation field.

## 10. Alternating Current Field Measurement Standardization Blocks

### 10.1 Artificial Notches for the Operation Standardization Block:

10.1.1 The operation standardization block has specific artificial discontinuities. It is used to check that the instrument and probe combination is functioning correctly. It may also be used for standardization of the equipment for nonmagnetic materials. Unless otherwise specified by the client or equipment manufacturer, the artificial discontinuities for the operation standardization block are elliptical notches. The notch geometry will be specified by the equipment manufacturer to be consistent with the crack size estimation model. Typical notch dimensions are as follows:


10.1.1.1 Notch in Thread Sample—An elliptical notch placed in a thread root, near to the pin shoulder, with dimensions of at least 0.6 by 0.06 in. [15 by 1.5 mm] to give a suitably large signal for comparison with that expected. (Fig. 3)

10.1.1.2 Notch in plate with a groove to mimic a thread root, if no thread sample is available—An elliptical notch placed in the groove, at least 4 in. [100 mm] from an edge, with dimensions of at least 0.6 by 0.06 in. [15 by 1.5 mm]. (Fig. 4)


10.1.2 These notches shall be less than 0.020 in. [0.50 mm] wide.

10.1.3 The standardization block may contain additional notches, for example smaller notches to indicate sensitivity. In this case, they shall be at least 0.75 in. [19 mm] from any other notch in both longitudinal and transverse directions.

10.1.4 Artificial discontinuity depths are specified by giving the deepest point of the discontinuity. Discontinuity depths

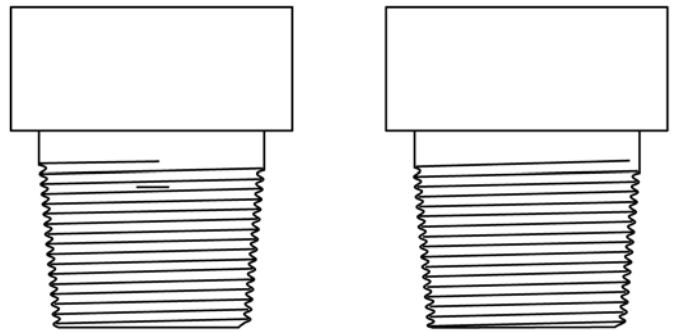

**FIG. 3 Pin Thread Sample Serial Number XXX Showing Size and Location of Reference Notch (Plan View and Side View. Not to Scale)**

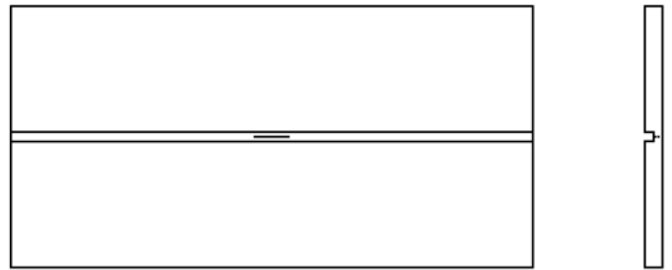

**FIG. 4 Flat Plate Sample Serial Number XXX Showing Size and Location of Reference Notch (Plan View and Side View. Not to Scale)**

shall be accurate to within  $\pm 10\%$  of the depth specified, measured, and documented. The discontinuity length shall be accurate to within  $\pm 0.040$  in. [ $\pm 1.00$  mm] of the dimension specified.

### 10.2 Materials Other than Ferritic Steel:

10.2.1 If the technique is to be used on materials other than ferritic steel, then it may be necessary to standardize the probes on this material. If configuration data are not available from the equipment manufacturer, refer to manufacturer's instructions.

NOTE 2—If this is not done then the sizes of the indications may be too small (so that small discontinuities may be missed) or too large (so that spurious indications may be called), or the  $B_x$  indication may saturate making the examination invalid. This standardization is done using a notch of reasonable size located at a thread root of a representative sample. The gain settings are altered, either automatically or manually according to equipment type, until a loop of reasonable size is produced in the X-Y plot while background noise indications are kept low. When the technique is to be used to size the depths of discontinuities detected in material for which configuration data is unavailable, then a standardization block should be manufactured from the material with at least two notches of differing depth. This provides an adjustment coefficient that modifies the estimated depth from the sizing model.

10.3 Standardization blocks having artificial or simulated discontinuities for threads in materials other than carbon steel shall not be used for discontinuity characterization unless the signals from the artificial discontinuities can be demonstrated to be similar to the signals for discontinuities detected. To be considered similar, a direct comparison should be performed between responses to the simulated discontinuities and real cracks. This comparison should involve at least one limited sizing trial or a probability of detection (POD) study.

#### 10.4 *Manufacture and Care of the Operation Standardization Blocks:*

10.4.1 *Drawings*—for each operation standardization block and standard, there shall be a drawing that includes the as-built measured notch dimensions, material type and grade, and the serial number of the actual operation standardization block.

10.4.2 *Serial Number*—each operation standardization block shall be identified with a unique serial number and stored so that it can be obtained and used for reference when required.

10.4.3 *Notch Spacing*—the notches should be positioned to avoid overlapping of indications and interference from end effects.

10.4.4 Proper machining practices shall be used to avoid excessive cold-working, over-heating, and undue stress and permeability variations.

10.4.5 Blocks should be stored and shipped so as to prevent mechanical damage.

### 11. Equipment Operation Check

#### 11.1 *Instrument Settings:*

11.1.1 *Operating Frequency*—The standard operating frequency depends upon the equipment to be used and typically is in the range of 5 to 50 kHz. The operating frequency should be chosen according to manufacturers' recommendations. Generally a lower frequency is best for ferritic steel or higher conductivity non-ferritic metals, a higher frequency is best for lower conductivity non-ferritic metals. A higher operating frequency will also give better sensitivity on good surfaces. If the system available is not capable of operating at the frequency described by this practice, the inspector shall declare to the client that conditions of reduced sensitivity may exist.

11.1.2 *Standardization*—The configuration data, especially for magnetic materials, may be supplied by the manufacturer. If not, the equipment may need to be standardized. Standardization is performed by loading manufacturer supplied configuration data for the nearest equivalent material, performing standardization measurements, and saving the resulting data and instrument settings as user configuration data. The standardization measurements are performed using the appropriate operation standardization block (see 10.1). The probe is placed so the sensors lie at the bottom of the thread root, with the nose of the probe parallel to the thread. The probe is then scanned across the operation standardization block and over a reference notch as specified by the equipment manufacturer. The signal for the scanned notch is then selected and the gain is adjusted manually or automatically based on the measured signal and a reference signal for the discontinuity. Care must be used to ensure that the reference notch is the same as the discontinuity for the reference signal. This information can then be saved as user configuration data.

#### 11.2 *Test System Check and Procedure:*

11.2.1 The test system shall consist of an alternating current field measurement instrument, a PC (if required), the probe and the operation standardization block.

11.2.2 The equipment operation check will be performed using the appropriate operation standardization block (see 10.1). The probe is placed so the sensors lie at the bottom of the thread root, with the nose of the probe parallel to the thread.

The probe is then scanned across the operation standardization block and over a reference notch as specified by the equipment manufacturer, producing a standardized data plot. Discontinuity indications are created when (1) the background level  $B_x$  value is reduced and then returns to the nominal background level (see Fig. 1), and this is associated with (2) a peak or positive (+ve) indication followed by a trough or negative (-ve) indication (or a trough followed by a peak, depending on direction of scan) in the  $B_z$  values. The resultant effect of the changes in  $B_x$  and  $B_z$  is a loop in the X-Y plot shown, for example, as the downward loop of Fig. 2. The presence of a discontinuity is confirmed when all three of these indications are present, that is, changes in the  $B_x$  and the  $B_z$  values and a loop in the X-Y plot. The loop should fill approximately 50 % of the  $B_x$  direction and 175 % of the  $B_z$  direction of the X-Y plot (that is, the loop is larger than the display in the  $B_z$  direction).

11.2.2.1 If the loop signal size differs from that expected from the operation standardization block, then the instrument and probe settings should be checked. Each probe should have a unique probe file, the validity of which has been checked against the discontinuity sizing tables. The instrument settings can be checked using the software package.

11.2.3 Each alternating current field measurement unit and probe to be used during the examination should be checked with the operation standardization block. If the correct loop signal sizes cannot be obtained within a specified margin (for example 10 %), then there is a fault with the system, which will have to be determined. Do not use for examination unless standardization validity is confirmed within the specified margin.

#### 11.3 *Frequency of System Checks:*

11.3.1 The system should be checked with all of the probes to be used during the examination prior to examining the first thread.

11.3.2 System operation should be checked at least every four hours with the probe in use or at the end of the examination shift. If the discontinuity responses from the operation standardization block have changed by a specified margin (for example, 10 %), the threads examined since the last operations standardization block check shall be re-examined after following the procedure in 11.2.

### 12. Procedure

12.1 Clean the thread surface to remove all grease, drilling mud and other deposits. Visually examine the thread for signs of damage that may impede or damage the probe, and for corrosion pitting that may affect the signals.

12.2 Following the guidelines in 9.3, select a suitable probe for the examination task, then, using the installed software, select a data file and a probe file. For a universal thread probe, fit the shoe appropriate for the thread to be examined.

12.2.1 For the box end, the probe is placed at the start of the thread with the sensors located in the root as close as possible to the thread start (farthest away from open end of pipe) at a suitable datum. This would typically be the thread run-out. A datum line is marked on the outside of the pipe adjacent to the center-line of the probe.

12.2.2 For the pin end, the probe is placed at the start of the thread with the sensors located in the root as close as possible to the thread start (farthest away from the end of the pipe) at a suitable datum. This would typically be the thread run-out. A datum line is marked on the shoulder adjacent to the center-line of the probe.

12.2.3 The pipe is then rotated if possible (by motor or by hand), or the probe is moved, such that the probe moves around the thread towards the open end of the pipe. A marker is placed in the data every rotation of the pipe, when the marked datum line passes the probe center-line. Discontinuity indications are created when the following three points are indicated:

12.2.3.1 The background level  $B_x$  value is reduced and then returns to the nominal background level, Fig. 1.

12.2.3.2 This is associated with a peak, or positive (+ve) indication followed by a trough, or negative (-ve) indication (or a trough followed by a peak, depending on direction of scan) in the  $B_z$  values, Fig. 1.

12.2.3.3 The resultant effect of the changes in  $B_x$  and  $B_z$  is a downward loop in the X-Y plot, which is shown as a downward loop in the example plot of Fig. 2.

12.2.4 The presence of a discontinuity is confirmed when all three of these indications are present, that is, the  $B_x$ , the  $B_z$  and a loop in the X-Y plot. Note that discontinuities of significant size will produce satellite indications one or more revolutions either side of the location of the discontinuity.

12.2.5 Analysis of data should be undertaken only after data is collected from the complete thread. To aid analysis, a restricted section of data should be selected by zooming in on part of the time axis (for example, one revolution of the pipe), then moving through the data in stages.

### 12.3 Compensation for Material Differences:

12.3.1 To compensate for the small differences in readings caused by variations in permeability, conductivity or geometry for a given material, the data may be centered on the display area. For larger differences, the equipment settings should be adjusted or a more suitable probe configuration should be used, or both, in accordance with the manufacturer's instructions.

12.4 Size and record all discontinuity indications as described in Section 14, as applicable.

12.5 Note areas of limited sensitivity, using indications from the operation standardization block as an indicator of discontinuity detectability.

12.6 Using a discontinuity characterization standard, evaluate relevant indications in accordance with acceptance criteria specified by the client, if applicable.

12.7 If desired, examine selected areas using an appropriate complementary method or technique to obtain more information, adjusting results where appropriate.

12.8 Compile and present a report to the client.

## 13. Examination Considerations

### 13.1 Scanning Speed:

13.1.1 The scanning speed is chosen using the appropriate data sampling rate to obtain reasonable fidelity with the details of the scanned object given the length of the shortest discon-

tinuity required to be found. A typical scan speed is 2 in./s [50 mm/s]. This will produce a regular scan on the display screen. If short discontinuity-like signals are found, then the area should be reexamined with a slower scan speed. The length and speed of scanning will govern the data-sampling rate selected. With the introduction of faster software or hardware, it is possible to select respective data sampling rates to produce faster scanning rates.

13.1.2 Acquire and record data from the operation standardization block at the selected examination speed.

13.1.3 Acquire and record data from the threads to be examined. Maintain as uniform a probe speed as possible throughout the examination to produce repeatable indications.

### 13.2 Scanning Direction:

13.2.1 The probe should always be scanned parallel to the thread root and this will give recognizable indications from transverse discontinuities as shown in Figs. 1 and 2. Scanning in this direction will also give recognizable, but different, indications in the unlikely event of longitudinal discontinuities parallel to the pipe axis. The operator should be familiar with these types of indications.

## 14. Discontinuity Sizing Procedure

14.1 When requested by the client, the sizing of any confirmed service-related defects may be performed as described herein using measurements taken of the  $B_x$  signatures plus the distance between terminal peak/trough of the  $B_z$  signature, as measured on the component.

### 14.2 Length:

14.2.1 Once an area containing a discontinuity has been located, a repeat scan is taken through the discontinuity. The amplitude of the signal shall be compared with that seen during the initial detection scan to ensure it is the same. This is to avoid mistakenly sizing from a smaller satellite signal in an adjacent thread root, which would result in a large underestimate of depth. The length of the discontinuity is determined by locating the extreme ends of the discontinuity using the peak (+ve) and trough (-ve)  $B_z$  locations. These positions are just inside the actual ends of the discontinuity. Markers are placed on the component at these two locations and the distance between the markers measured by a tape or ruler. This  $B_z$  length is used with the discontinuity sizing tables to determine the true length and depth of the discontinuity. Alternatively, the length of the detected discontinuity may be measured directly by the system software using a position encoder.

### 14.3 Depth:

14.3.1 The depth of the discontinuity is calculated using the  $B_x$  minimum and  $B_x$  background values and the  $B_z$  length of the discontinuity measured from the  $B_z$  data. Once these values have been put into the software, then the discontinuity depth will be estimated using the discontinuity sizing table.

## 15. Report

15.1 *Reporting Requirements*—a list of reporting requirements is given in Table 1. Reference should be made to the Client reporting requirements (7.1.4). The items listed below

**TABLE 1 Reporting Requirements**

NOTE 1—The data report sheets generated by the alternating current field measurement examination will be specifically designed with the system and current examination requirements in mind. The essential information contained on a data sheet will include:

General Information	
Date	
Operator's Name	
Probe Operator	
Component ID Number	
File Number	
Equipment used	
Scanning Data	
Filename	
Page Number	
Position on Thread	
Probe Number	
Probe Direction	
Tape Position	
Examination Summary	
Detailed Record of Indications / Anomalies	
Filename	
Page Number	
Position on Thread	
Start of Discontinuity (Tape reference)	
End of Discontinuity (Tape reference)	
Length of Discontinuity (inches/millimetres)	
Remarks	
Diagram/Drawing of component under examination	

should be included in the examination report. All information below should be archived, whether or not it is required in the report.

15.1.1 Owner, location, type and serial number of component examined.

15.1.2 Size, material type and grade, and configuration of threads examined.

15.1.3 Thread numbering system.

15.1.4 Extent of examination, for example, areas of interest, complete or partial coverage, which threads and other parts, and to what length.

15.1.5 The names and qualifications of personnel performing the examination.

15.1.6 Models, types, and serial numbers of the components of the alternating current field measurement system used, including all probes.

15.1.7 For the initial data acquisition from the operation standardization block, a complete list of all relevant instrument settings and parameters used, such as operating frequencies, and probe speed. The list shall enable settings to be referenced to each individual thread examined.

15.1.8 Serial numbers of all of the operations standardization blocks used.

15.1.9 Brief outline of all techniques used during the examination.

15.1.10 A list of all areas not examinable or where limited sensitivity was obtained. Where possible, indicate factors that may have limited sensitivity.

NOTE 3—Factors that influence sensitivity to discontinuities include but are not limited to: operating frequency, instrument noise, instrument filtering, digital sample rate, probe speed, coil configuration, probe travel noise and interference described in Section 8.

15.1.11 If applicable, specific information about techniques and depth sizing for each discontinuity.

15.1.12 Acceptance criteria used to evaluate discontinuities.

15.1.13 A list of discontinuities as specified in the purchasing agreement.

15.1.14 Complementary examination results that influenced interpretation and evaluation.

15.2 Record data and system settings in a manner that allows archiving and later recall of all data and system settings for each thread. Throughout the examination, data shall be recorded and retained for later retrieval per customer requirements, or in the absence of customer requirements, per company practice.

15.2.1 *Report form.* An example report form is shown in Fig. 5.

## 16. Keywords

16.1 alternating current field measurement; drillstring; electromagnetic examination; ferromagnetic material; non-magnetic material; root; thread



# ACFM Test Report

Report on ACFM non-destructive testing

## GENERAL INSPECTION PAGE REPORT


**Component:**

**Test Date:**

**Test Time:**

**Filename:**

**File Page ID:** 2 (6 pages total)

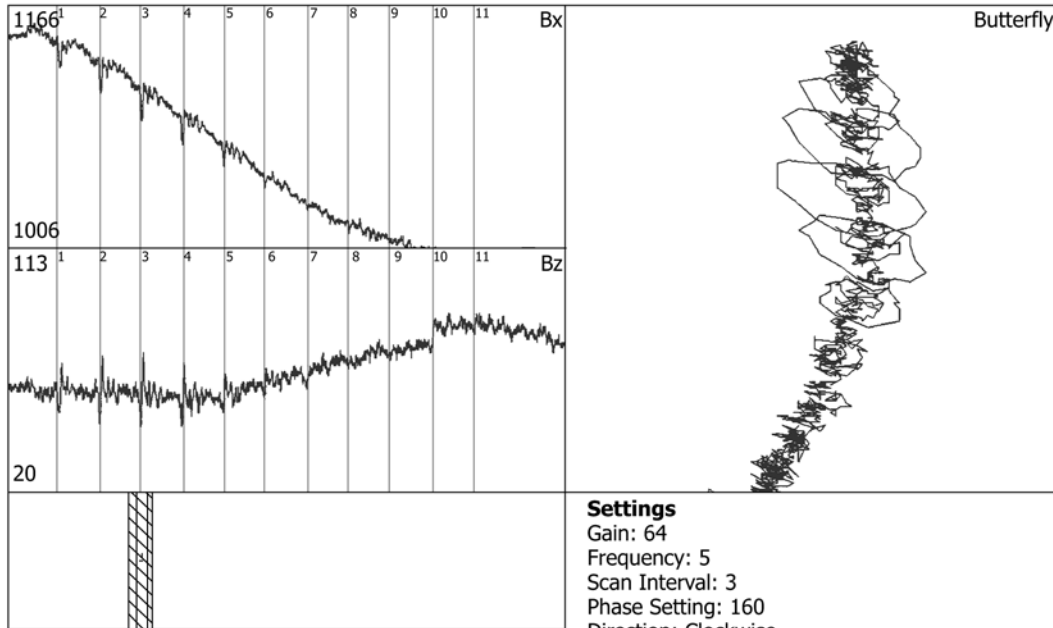

**Region Key**

▨ Defect   ▨ Other

**Settings**

Gain: 64  
 Frequency: 5  
 Scan Interval: 3  
 Phase Setting: 160  
 Direction: Clockwise  
 Data Field: X Field  
 Start Posn (mm): 0  
 Scalings: Default

**Defects**

	Len	Depth
1:	24 mm	0.5 mm

**Notes**

Downhole end - defect detected on 3rd thread

Probe: Universal Thread Probe - 5 kHz  
 Serial Number:  
 Configuration: Ferritic Steel

Operator:  
 Prepared by Signature:  
 Date:

FIG. 5 Example Alternating Current Field Measurement Report

*ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.*

*This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.*

*This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or [service@astm.org](mailto:service@astm.org) (e-mail); or through the ASTM website ([www.astm.org](http://www.astm.org)). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>*