



Standard Test Method for Thickness Measurement of Flexible Packaging Material¹

This standard is issued under the fixed designation F2251; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This test method covers the measurement of thickness of flexible packaging materials using contact micrometers.

1.2 The Precision and Bias statement for this test method was developed using both handheld and bench top micrometers with foot sizes ranging from 4.8 to 15.9 mm ($\frac{3}{16}$ to $\frac{5}{8}$ in.).

1.3 The values stated in either SI units or inch-pound units are to be regarded separately as standard. The values stated in each system may not be exact equivalents; therefore, each system shall be used independently of the other. Combining values from the two systems may result in non-conformance with the standard.

1.4 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.*

2. Referenced Documents

2.1 ASTM Standards:²

[D374 Test Methods for Thickness of Solid Electrical Insulation](#) (Withdrawn 2013)³

[D5947 Test Methods for Physical Dimensions of Solid Plastics Specimens](#)

[D6988 Guide for Determination of Thickness of Plastic Film Test Specimens](#)

[E171 Practice for Conditioning and Testing Flexible Barrier Packaging](#)

[E691 Practice for Conducting an Interlaboratory Study to Determine the Precision of a Test Method](#)

¹ This test method is under the jurisdiction of ASTM Committee F02 on Flexible Barrier Packaging and is the direct responsibility of Subcommittee F02.20 on Physical Properties.

Current edition approved Aug. 1, 2013. Published October 2013. Originally approved in 2003. Last previous edition approved in 2008 as F2251 – 03 (Reapproved 2008). DOI: 10.1520/F2251-13.

² For referenced ASTM standards, visit the ASTM website, www.astm.org, or contact ASTM Customer Service at service@astm.org. For *Annual Book of ASTM Standards* volume information, refer to the standard's Document Summary page on the ASTM website.

³ The last approved version of this historical standard is referenced on www.astm.org.

2.2 ANSI/ASQ Standards:⁴

[ANSI/ASQC Z1.4 Sampling Procedures and Tables for Inspection by Attributes](#)

[ANSI/ASQC Z1.9 Sampling Procedures and Tables for Inspection by Variables](#)

3. Terminology

3.1 Definitions:

3.1.1 *bench micrometer*—tabletop measurement system using a dead weight or spring.

3.1.2 *foot*—the moving component of the micrometer that comes in contact with the sample.

4. Significance and Use

4.1 This test method provides a means for measuring a thickness dimension. Accurate measurement of thickness can be critical to meeting specifications and characterizing process, product, and material performance.

4.2 This test method does not address acceptability criteria. These need to be jointly determined by the user and producer of the product. Repeatability and reproducibility of measurement is shown in the Precision and Bias section. Attention should be given to the inherent variability of materials being measured as this can affect measurement outcome.

5. Apparatus

5.1 Mechanical gage, suitable for measuring thickness:

5.1.1 The thickness gage may be either a bench or hand-held mechanical model.

5.1.2 The gage should be capable of accurately measuring in increments of 2.5 μm (0.0001 in.).

5.1.3 The foot size and foot pressure should be known and identified. Because of the compressibility of different materials it is important when comparing results between different laboratories that the size of the foot and pressure be the same. Refer to Guide [D6988](#) for further guidance on foot pressures.

5.1.4 It is recommended that a calibration be performed on the apparatus used and certified to a recognized industry standard such as National Institute of Standards and Technology (NIST).

⁴ Available from American National Standards Institute (ANSI) 25 W. 43rd St., 4th Floor, New York, NY 10036.

NOTE 1—Test Methods [D5947](#) and [D374](#) give guidance on methods for checking calibration and parallelism.

6. Sampling

6.1 The number of samples tested should be adequate to be predictive of performance. Caution should be taken when eliminating samples with defects as this can bias results.

6.2 See ANSI/ASQC Z1.4 or Z1.9 for guidance on sampling plans and practices.

7. Conditioning

7.1 Conditioning of the samples will depend on the material under evaluation. If conditioning before testing is appropriate, normal, and desirable, refer to Specification [E171](#) for guidance.

8. Procedure

8.1 Review applicable specifications, drawings, or procedures. Specify unit of measure to be used and directions related to precision requirements (for example, measure to nearest 0.0001 in., round up or down to nearest 1 μm , and so forth).

8.2 Clean the micrometer contact area (foot and anvil).

8.3 Verify that the micrometer reads 0.0 μm (0.00000 in.) when no specimen is present.

8.4 Place sample to be measured between the gage foot and anvil. The foot and anvil must be maintained in a parallel state. The sample must be placed such that the measurement location is parallel to the gage foot and anvil. The sample should lay flat and smooth without wrinkles, creases or folds. Material should not be under tension when measured.

8.5 Release foot and allow reading to stabilize.

8.6 Read thickness on gauge readout or face.

9. Report

9.1 Report the following information:

9.1.1 Lot number and source of material, date, time, location and operator of test and complete identification of materials being tested.

9.1.2 Any conditioning of the materials.

9.1.3 The apparatus used to measure the thickness, including the foot size and foot pressure.

9.1.4 Any and all deviations from standard.

TABLE 1 Description of Equipment used in Round Robin Studies

NOTE 1—Force ranges from instruments are specified from 10 to 150 g. Exceptions include bench top model at 15.875 mm (0.625 in.) rated at 7.3 psi with a dead weight load of 1033 g and 6.35 mm (0.25 in.) handheld is rated at a force between 600 to 1000 g.

Diameter	Foot Size, mm	Foot Size, in.	Type	Make
	4.7752	0.188	Bench	Mitutuoyo
	4.7752	0.188	Bench	Mitutuoyo
	4.7752	0.188	Bench	Mitutuoyo
	6.35	0.250	Handheld	Mitutuoyo
	6.35	0.250	Bench	Mitutuoyo
	9.525	0.375	Bench	Ono Sokki
	9.525	0.375	Handheld	Precision Material
	9.525	0.375	Handheld	Mitutuoyo
	15.875	0.625	Bench	TMI

9.1.5 The sampling plan and number of specimens tested along with test results should at a minimum include mean, range and standard deviation.

10. Precision and Bias

10.1 *Precision*—A research report⁵ describes a round robin conducted in 2002 in accordance with Practice [E691](#), involving seven laboratories measuring eight specimens. Ten different pieces of equipment were used to collect information. Equipment used and foot sizes are listed in [Table 1](#). Measurements taken included use of micrometers in 0.0001 in. divisions. Statistical summaries of repeatability (within a laboratory) and reproducibility (between laboratories) are listed in [Tables 2 and 3](#). All test results are expressed in SI units of measure.

10.2 Concept of “*r*” and “*R*” in [Tables 2 and 3](#)—If S_r and S_R have been calculated from a large enough body of data, and for test results that are averages from three tests on one specimen for each test result, then the following applies:

10.3 Repeatability “*r*” is the interval representing the critical difference between two test results for the same material, obtained by the same operator using the same equipment on the same day in the same laboratory. Two test results shall be judged to be not equivalent if they differ by more than the “*r*” value for that material.

⁵ A research report is available from ASTM International Headquarters. Request RR:F02-1018.

TABLE 2 Summary of Interlaboratory Results by Measurement Set

Part	Avg Thickness		Repeatability, Std Dev, s_r		Reproducibility, Std Dev, s_R		95 % Repeatability, Limit, r		95 % Reproducibility, Limit, R	
	mm	mils	mm	mils	mm	mils	mm	mils	mm	mils
G: 0.48 mil PET	0.012954	0.5100	0.001008	0.0397	0.002197	0.0865	0.00282	0.1111	0.006152	0.2422
A: 2 mil PE	0.053679	2.1133	0.000881	0.0347	0.002691	0.1059	0.00247	0.0971	0.007534	0.2966
B: 2.5 mil PET/PE	0.06405	2.5217	0.000489	0.0192	0.001915	0.0754	0.00137	0.0539	0.005361	0.2111
H: 2.94 mil Calibration Feeler Gage	0.074083	2.9167	0.001316	0.0518	0.00152	0.0598	0.00369	0.1451	0.004255	0.1675
F: 42# Uncoated Medical Paper	0.090678	3.5700	0.000733	0.0289	0.001943	0.0765	0.00205	0.0808	0.00544	0.2142
D: 4.2 mil PET/PE/FOIL/PE	0.10994	4.3283	0.000811	0.0319	0.001966	0.0774	0.00227	0.0894	0.005505	0.2167
E: Uncoated 1073B Tyvek	0.143722	5.6583	0.00164	0.0645	0.009781	0.3851	0.00459	0.1807	0.027387	1.0782
C: 10 mil EVA/SURLYN/EVA	0.260181	10.2433	0.001222	0.0481	0.002596	0.1022	0.00342	0.1347	0.007268	0.2862
Average			0.001069	0.0421	0.004001	0.1575	0.00299	0.1178	0.011204	0.4411

TABLE 3 Summary of Interlaboratory Averaged Results

Repeatability (within a laboratory) standard deviation (s_r)	0.001069 mm (0.0421 mils)
95 % repeatability limit (r)	0.00299 mm (0.1178 mils)
Reproducibility (between laboratories) standard deviation (s_R)	0.004001 mm (0.1575 mils)
95 % reproducibility limit (R)	0.011204 mm (0.4411 mils)

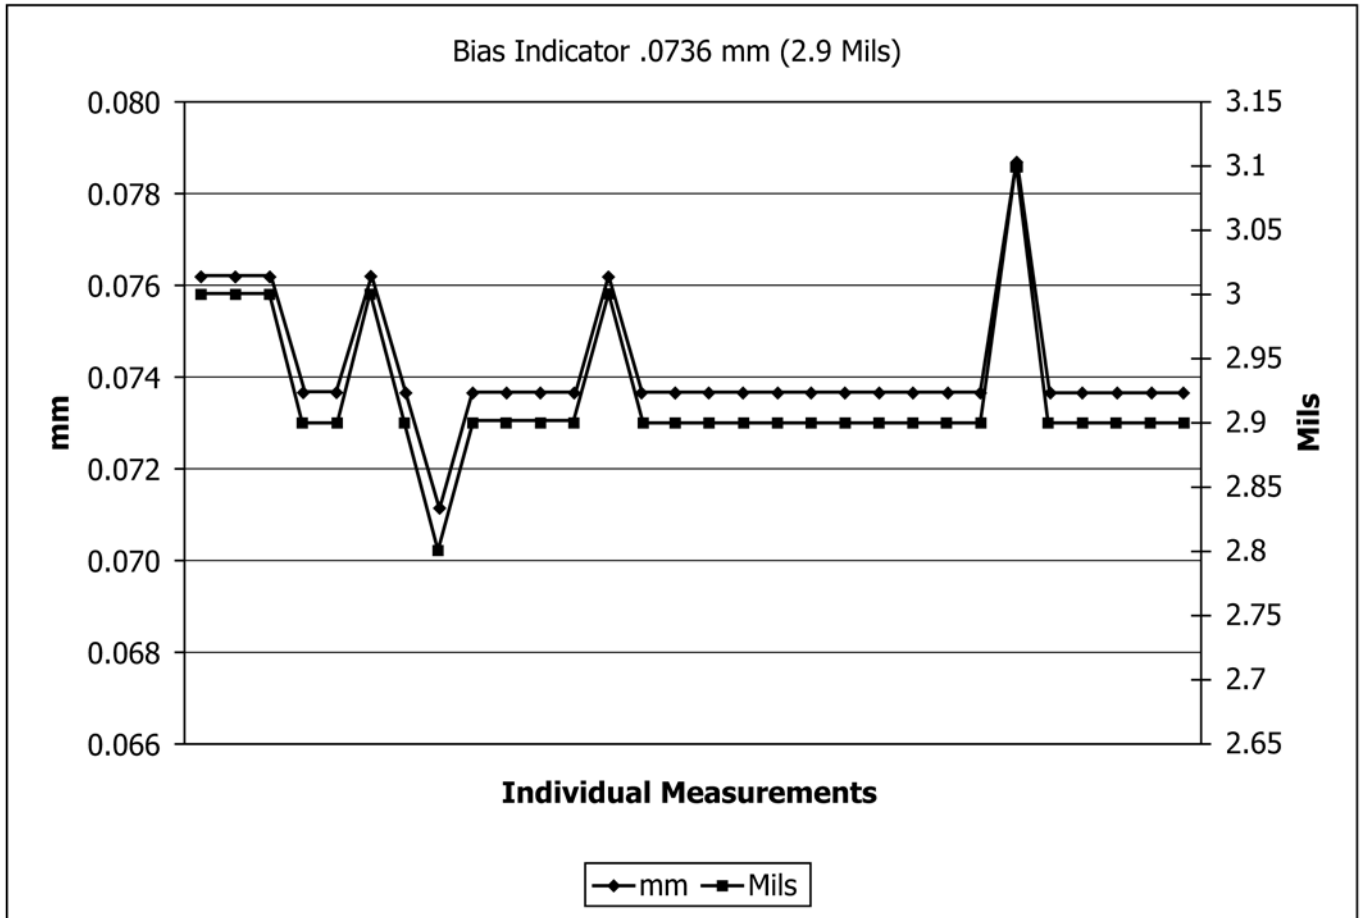


FIG. 1

10.4 Reproducibility “ R ” is the interval representing the critical difference between two test results for the same material, obtained by different operators using different equipment in different laboratories, not necessarily on the same day. Two test results shall be judged to be not equivalent if they differ by more than the “ R ” value for that material.

10.5 Any judgment in accordance with 10.3 or 10.4 will have approximately 95 % (0.95) probability of being correct.

10.6 *Bias*—Bias gage measures to 0.0736 mm (2.94 mils) per NIST calibration testing. Micrometer measurements collected to 0.1 mils precision. Analysis is based upon a 2.9 mil target. The chart in Fig. 1 does not indicate a consistent bias.

11. Keywords

11.1 dimension; micrometer; thickness measurement

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; <http://www.copyright.com/>