



Standard Practice for Sampling Gas Blow Down Systems and Components for Particulate Contamination by Automatic Particle Monitor Method¹

This standard is issued under the fixed designation F327; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This practice describes how to connect, prepare, and sample pressurized gas systems (having up to 19.1-mm (0.75-in.) diameter lines) for particulate contamination by using an automatic monitor.

1.2 The values stated in MKS units are to be regarded as the standard. The values given in parentheses are for information only.

1.3 *This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety and health practices and determine the applicability of regulatory limitations prior to use.* For hazard statements, see Section 5.

2. Terminology

2.1 Definitions:

2.1.1 *downstream terminal point*—the point in a gas system from which gas is fed into a further system or component, usually the designated “sample port.”

2.1.2 *filtered gas system*—a gas system that is equipped with required filtration devices to furnish gas that is suitably clean for the intended application.

2.1.3 *purge*—to flush a gas supply system or component with a regulated flow of gas.

2.1.4 *sample port*—the designated point in a gas system or component from which a representative gas sample may be taken.

3. Summary of Practice

3.1 The pressurized gas system or component and the apparatus are prepared in accordance with the requirements of the users sample analysis procedure. The sensing unit of the

¹ This practice is under the jurisdiction of ASTM Committee E21 on Space Simulation and Applications of Space Technology and is the direct responsibility of Subcommittee E21.05 on Contamination.

Current edition approved May 1, 2015. Published June 2015. Originally approved in 1972. Last previous edition approved in 2008 as F327 – 08. DOI: 10.1520/F0327-08R15.

automatic particle monitor is connected to the designated sample port which is under purge condition. The system flow-rate is adjusted to the sample flow rate requirement. All the gas passing through the sensing unit is monitored for particulate contamination until the required sample volume has been analyzed.

4. Apparatus

4.1 *Automatic Monitor*, with sensor that sizes and counts all entering fluid in accordance with the users requirements for pressure, flow, temperature, and accuracy.

4.2 *Filtered Gas System*—See Fig. 1.

4.3 *Stop Watch or Timer*, with a + 1, – 0-s resolution.

4.4 *Miscellaneous Fittings*, as needed for sampling point adaption, cleaned and packaged within system contamination requirements.

4.5 *Connecting Lines*, cleaned and packaged within system contamination requirements.

4.6 *Flowmeter*, calibrated for the sample port fluid, flow, and temperature requirements.

5. Hazards

5.1 Personnel must stand clear of exiting gas.

5.2 Ear protection must be used when gas flow approaches sonic velocity.

5.3 All lines and associated system components must be connected and operated within the requirements of recognized safety codes.

6. Procedure

6.1 Establish a minimum continuous purge pressure of 6.89 kPa (1 psig) gage or 2.83 dm³/min (0.1 ft³/min), flow from the filtered gas pressure supply.

6.2 Connect one end of a suitable connecting line to the purge outlet of 6.1, and then connect the other end to the inlet of the component or system to be sampled.

NOTE 1—If the system to be sampled is already connected to the filtered gas pressure supply, then establish the purge as noted in 6.1.

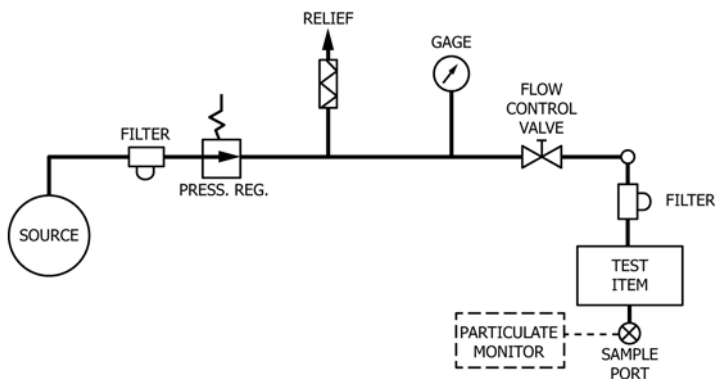


FIG. 1 Filtered Gas System

6.3 Connect a suitable connecting line from the sample port to the inlet of the automatic monitor sensing device. (When no sample port is designated, use the down-stream terminal point from which purge gas is flowing.)

6.4 Increase the purge to one of the following:

6.4.1 8.49-dm³/min (0.3-ft³/min) flow,

6.4.2 34.5-kPa (5-psig) gage pressure, or

6.4.3 5 % of system operating pressure when this pressure is less than 34.5-kPa (5-psig) gage.

6.5 Surge Pressure Cleaning:

6.5.1 Quickly increase the continuous purge pressure for a 5-s duration, three times at 1-min intervals in accordance with one of the following:

6.5.1.1 To 689.5-kPa (100-psig) gage pressure,

6.5.1.2 To 113.2-dm³/min (4.0-ft³/min) flow,

6.5.1.3 70 % of system operating pressure when this operating pressure is below 689.5 kPa (100 psig) gage.

6.5.1.4 In accord with a given system operation requirement, but not to exceed the rated pressure of the sensing unit.

6.5.2 Reduce the purge pressure to the level in 6.4 after each surge pressure application of 6.5.1 (that is during 1-min interval).

6.6 Connect a flowmeter to the outlet of the automatic monitor sensor and adjust the flow versus time to achieve a

required sample volume within the capability of the sensor. Remove the flowmeter after adjusting the flow.

6.7 Set automatic monitor display to zero.

6.8 Simultaneously begin automatic particulate counting, sizing and timing of volumetric flow.

6.9 Record particulate contamination counts on the monitor display for the required sample volume.

6.10 Adjust the continuous purge to the level in 6.4.

6.11 Evaluate results and if requirements of contamination levels are acceptable, disconnect the monitor and secure the system in accordance with the user's requirements.

6.12 If results are rejected, repeat 6.5 – 6.12.

7. Precision

7.1 Each testing agency has the responsibility of judging the acceptability of its own results. The precision of the results is a function of the procedures (Note 2), facilities utilized, as well as compliance to the recommended industry state-of-the-art practices in cleanliness. Reproducible analysis determinations by different users can be achieved only with identical facilities and trained conscientious personnel.

NOTE 2—Every effort should be made to eliminate outside contamination during operations.

ASTM International takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM International Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, at the address shown below.

This standard is copyrighted by ASTM International, 100 Barr Harbor Drive, PO Box C700, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (www.astm.org). Permission rights to photocopy the standard may also be secured from the Copyright Clearance Center, 222 Rosewood Drive, Danvers, MA 01923, Tel: (978) 646-2600; http://www.copyright.com/