

**Steel and iron —
Determination of total
silicon content —
Gravimetric method
(ISO 439:1994)**

ICS 77.080.01

National foreword

This British Standard is the UK implementation of EN ISO 439:2010. It is identical to ISO 439:1994. It supersedes BS 6200-3.26.1:1995 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee ISE/102, Methods of chemical analysis for Iron and Steel.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 May 2010

© BSI 2010

ISBN 978 0 580 69258 1

Amendments/corrigenda issued since publication

Date	Comments

EUROPEAN STANDARD

EN ISO 439

NORME EUROPÉENNE

EUROPÄISCHE NORM

April 2010

ICS 77.080.01

English Version

Steel and iron - Determination of total silicon content - Gravimetric method (ISO 439:1994)

Aciers et fontes - Dosage du silicium total - Méthode
gravimétrique (ISO 439:1994)

Stahl und Eisen - Bestimmung des Gesamtsiliziumgehaltes
- Gravimetrisches Verfahren (ISO 439:1994)

This European Standard was approved by CEN on 18 March 2010.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

The text of ISO 439:1994 has been prepared by Technical Committee ISO/TC 17 “Steel” of the International Organization for Standardization (ISO) and has been taken over as EN ISO 439:2010 by Technical Committee ECISS/TC 102 “Methods of chemical analysis for iron and steel” the secretariat of which is held by SIS.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by October 2010, and conflicting national standards shall be withdrawn at the latest by October 2010.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and the United Kingdom.

Endorsement notice

The text of ISO 439:1994 has been approved by CEN as a EN ISO 439:2010 without any modification.

Steel and iron — Determination of total silicon content — Gravimetric method

1 Scope

This International Standard specifies a gravimetric method for the determination of the total silicon content in steel and iron.

The method is applicable to silicon contents between 0,10 % (*m/m*) and 5,0 % (*m/m*) (see note 1).

NOTE 1 For samples containing molybdenum, niobium, tantalum, titanium, tungsten, zirconium or high levels of chromium, the results are less precise than for unalloyed steels (see annex A).

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 377-2:1989, *Selection and preparation of samples and test pieces of wrought steels — Part 2: Samples for the determination of the chemical composition.*

ISO 385-1:1984, *Laboratory glassware — Burettes — Part 1: General requirements.*

ISO 648:1977, *Laboratory glassware — One-mark pipettes.*

ISO 1042:1983, *Laboratory glassware — One-mark volumetric flasks.*

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods.*

ISO 5725:1986, *Precision of test methods — Determination of repeatability and reproducibility for a standard test method by inter-laboratory tests.*

3 Principle

Attack of a test portion by hydrochloric and nitric acids.

Conversion of acid-soluble silicon compounds to hydrated silicon dioxide by evaporation with perchloric acid until white fumes appear. Filtration of the hydrated silicon dioxide and acid-insoluble silicon compounds, ignition to form impure silicon dioxide and then weighing.

Treatment of the ignited residue with hydrofluoric and sulfuric acids, followed by ignition and weighing.

4 Reagents

During the analysis, unless otherwise stated, use only reagents of recognized analytical grade and grade 2 water as specified in ISO 3696.

4.1 Hydrochloric acid, ρ about 1,19 g/ml.

4.2 Hydrochloric acid, ρ about 1,19 g/ml, diluted 1 + 1.

4.3 Hydrochloric acid, ρ about 1,19 g/ml, diluted 1 + 19.

4.4 Nitric acid, ρ about 1,40 g/ml, diluted 3 + 1.

4.5 Hydrofluoric acid, ρ about 1,14 g/ml.

4.6 Perchloric acid, ρ about 1,67 g/ml (see note 2).

NOTE 2 Perchloric acid (ρ about 1,54 g/ml) may also be used.

4.7 Sulfuric acid, ρ about 1,83 g/ml, diluted 1 + 1.

5 Apparatus

All volumetric glassware shall be class A, in accordance with ISO 385-1, ISO 648 or ISO 1042, as appropriate.

Ordinary laboratory apparatus, and

5.1 Platinum crucibles, of capacity approximately 30 ml.

5.2 Muffle furnace, adjustable from 800 °C up to 1 100 °C.

5.3 Filter paper, medium-texture, of known low ash content.

6 Sampling

Carry out sampling in accordance with ISO 377-2 or appropriate national standards for steel and iron.

7 Procedure

WARNING — Perchloric acid vapour may cause explosions in the presence of ammonia, nitrous fumes or organic matter in general. All evaporations must be carried out in fume cupboards suitable for use with perchloric acid.

7.1 Test portion

Use millings or drillings of a maximum thickness of 0,2 mm.

According to the presumed silicon content, weigh, to the nearest 1 mg, the following mass (m_0) of the test portion:

- a) for silicon contents between 0,10 % (m/m) and 0,50 % (m/m): $m_0 \approx 5$ g;
- b) for silicon contents between 0,50 % (m/m) and 2,5 % (m/m): $m_0 \approx 2,5$ g;
- c) for silicon contents between 2,5 % (m/m) and 5,0 % (m/m): $m_0 \approx 1$ g.

7.2 Blank test

In parallel with the determination and following the same procedure, carry out a blank test using the same quantities of all the reagents.

7.3 Determination

7.3.1 Acid attack of the test portion and formation of hydrated silicon dioxide

Place the test portion (7.1) in a beaker of acid-resistant glass of suitable capacity.

Add 30 ml of hydrochloric acid (4.1), and then gently heat the beaker covered with a watch glass until the reaction ceases. Oxidize by careful addition of 15 ml of nitric acid (4.4). When the fairly violent reaction ceases, rinse the watch glass with a little hot water and collect the washings in the beaker. Add a volume of perchloric acid (4.6) as indicated in table 1.

Table 1

Mass of test portion (7.1) g	Volume of perchloric acid (4.6) ml	
	$\rho = 1,67$ g/ml	$\rho = 1,54$ g/ml
5	60	75
2,5	40	50
1	25	35

WARNING — Perchloric acid (4.6) must be added cautiously in small portions, especially when a 5 g test portion has been taken, in order to avoid boiling over, due to a very violent reaction.

Heat the uncovered beaker slightly until the attack is complete and then increase the rate of heating. As soon as the first white perchloric acid fumes appear, cover the beaker with the watch glass and continue fuming for about 20 min. Allow to cool, carefully moisten with 5 ml of hydrochloric acid (4.1) (see note 3), heat slightly, dilute with 100 ml of water at 70 °C to 80 °C and heat again until the salts are dissolved (taking care not to allow the solution to boil).

NOTE 3 For samples containing high chromium contents, more than 5 ml of hydrochloric acid (4.1) should be added to reduce the hexavalent chromium.

7.3.2 Filtration and washing

With a rubber-tipped glass rod, detach any hydrated silicon dioxide or acid-insoluble silicon compounds

that may be adhering to the beaker and filter immediately through a filter paper (5.3) containing a little filter-paper pulp of the same quality.

Wash the beaker and the filter with hot hydrochloric acid (4.3), transferring the hydrated silicon dioxide and acid-insoluble silicon compounds to the filter, and complete the washing, first with hot hydrochloric acid (4.2) and then with cold water until the iron salts are completely eliminated (see note 4).

NOTE 4 The filter should be washed thoroughly in order to avoid popping and loss of residue due to perchloric acid during ignition.

7.3.3 Recovery of silicon compounds in the filtrate

Transfer the filtrate and the washings to the beaker previously used for the attack, evaporate them by heating until dense white fumes of perchloric acid are evolved, and maintain a steady refluxing of acid on the walls of the beaker for about 20 min. Moisten and dilute according to the procedure specified in 7.3.1, then filter through a second filter paper (5.3) and wash according to the procedure specified in 7.3.2.

7.3.4 Ignition, volatilization of silicon dioxide and weighing

Put the two filters and their contents together in a platinum crucible (5.1). Heat at between 500 °C and 600 °C until the filters are completely incinerated, then cover the crucible partially with a platinum cover and ignite in the muffle furnace (5.2) at 1 100 °C for 30 min to 45 min, depending on the quantity of silicon dioxide, for samples containing molybdenum, until a constant mass is obtained.

Allow to cool, add approximately 2 ml of sulfuric acid (4.7) to the crucible, heat carefully and continue heating until the sulfuric acid fumes are completely eliminated. Then ignite in the muffle furnace at 800 °C to constant mass.

Allow to cool in a desiccator and weigh the crucible and its contents (mass in grams: m_1).

Then moisten the ignited silicon dioxide with a few drops of sulfuric acid (4.7) (see note 5), add approximately 5 ml of hydrofluoric acid (4.5), evaporate to dryness and continue heating until the sulfuric acid fumes are completely eliminated.

NOTE 5 If molybdenum, niobium, tantalum, titanium, tungsten or zirconium are present, add 2 ml of sulfuric acid (4.7) in order to avoid any partial volatilization of the fluorides of these elements.

Complete the ignition in the muffle furnace at 800 °C for 10 min.

Allow to cool in a desiccator, then weigh the crucible and its contents (mass in grams: m_2).

8 Expression of results

8.1 Method of calculation

The silicon content, w_{Si} , expressed as a percentage by mass, is given by the equation

$$w_{\text{Si}} = 0,467\ 4 \times \frac{(m_1 - m_2) - (m_3 - m_4)}{m_0} \times 100$$

$$= 46,74 \times \frac{(m_1 - m_2) - (m_3 - m_4)}{m_0}$$

where

m_0 is the mass, in grams, of the test portion (7.1);

m_1 is the mass, in grams, of the crucible and the impure silicon dioxide;

m_2 is the mass, in grams, of the crucible and residue after volatilization of the silicon dioxide;

m_3 is the mass, in grams, of the crucible and the impure silicon dioxide in the blank test;

m_4 is the mass, in grams, of the crucible and residue after volatilization of the silicon dioxide in the blank test;

0,467 4 is the Si/SiO₂ coefficient.

Express the results to the second decimal place.

8.2 Precision

A planned trial of this method was carried out by 26 laboratories, using nine levels of total silicon contents, each laboratory making three determinations of total silicon content on each level (see notes 6 and 7).

The test samples used and mean results obtained are listed in table A.1.

The results obtained were treated statistically in accordance with ISO 5725.

The data obtained showed a logarithmic relationship between total silicon content and repeatability (r) and reproducibility (R and R_w) of the test results (see note 8) as summarized in table 2. The graphical representation of the data is shown in figure B.1.

Table 2

Total silicon content % (m/m)	Repeatability <i>r</i>	Reproducibility	
		<i>R</i>	<i>R_w</i>
0,10	0,010 5	0,013 9	0,010 5
0,20	0,013 8	0,019 3	0,014 8
0,50	0,019 8	0,030 0	0,023 3
1,00	0,025 9	0,041 9	0,032 9
2,00	0,034 0	0,058 5	0,046 5
5,00	0,048 7	0,090 9	0,073 4

NOTES

6 Two of the three determinations were carried out under repeatability conditions as defined in ISO 5725; i.e. one operator, same apparatus, identical operating conditions, same calibration, and a minimum period of time.

7 The third determination was carried out at a different time (on a different day) by the same operator as in note 6, using the same apparatus with a new calibration.

8 From the two values obtained on day 1, the repeatability (*r*) and reproducibility (*R*) were calculated using the procedure specified in ISO 5725. From the first value obtained on day 1 and the value obtained on day 2, the within-laboratory reproducibility (*R_w*) was calculated.

9 Test report

The test report shall include the following information:

- a) all information necessary for the identification of the sample, the laboratory and the date of analysis;
- b) the method used by reference to this International Standard;
- c) the results, and the form in which they are expressed;
- d) any unusual features noted during the determination;
- e) any operation not specified in this International Standard, or any optional operation which may have influenced the results.

Annex A (informative)

Additional information on the international cooperative tests

Table 2 was derived from the results of international analytical trials carried out in 1991 on eight steel samples and one iron sample in 11 countries involving 26 laboratories.

The results of the trials were reported in document ISO/TC 17/SC 1 N 934, April 1992. The graphical representation of the precision data is given in annex B.


The test samples used are listed in table A.1.

Table A.1

Sample	Total silicon content % (m/m)			Precision data		
	Certified	Found		Repeatability <i>r</i>	Reproducibility	
		$\bar{w}_{Si,1}$	$\bar{w}_{Si,2}$		<i>R</i>	<i>R_w</i>
BCS 460/1 (low alloy steel) [0,066Nb]	0,098	0,097 3	0,097 2	0,007 6	0,010 3	0,007 8
BCS 220/2 (tool steel) [5Cr, 0,3Co, 5Mo, 2V, 7W]	0,19	0,194	0,192	0,024 9	0,032 4	0,022 6
JSS 030-6 (unalloyed steel)	0,26	0,255	0,255	0,013 4	0,016 3	0,015 7
ECRM 292-1 (stainless steel) [18Cr, 10Ni, 0,6Nb]	0,402	0,404	0,403	0,021 8	0,043 4	0,026 4
BCS 410/2 (low alloy steel) [1,7Cr, 2Ni, 0,4Mo, 0,4V]	1,10	1,090	1,091	0,015 0	0,024 6	0,020 6
ECRM 481-1 (cast iron) [1Ni, 0,05Mg]	2,29	2,284	2,289	0,028 0	0,052 0	0,042 0
BCS 206/3 (high Si, P steel) [3Si, 1,6P]	3,17	3,155	3,152	0,055 9	0,082 9	0,069 5
ECRM F 114-1 (high Si steel)	4,0 ¹⁾	4,012	4,014	0,068 2	0,077 6	0,083 9
CE 034 (silicon steel)	5,18	5,152	5,149	0,037 4	0,115	0,068 7
$\bar{w}_{Si,1}$, general mean within a day						
$\bar{w}_{Si,2}$, general mean between days						
1) Non-certified value.						

Annex B (informative)

Graphical representation of precision data

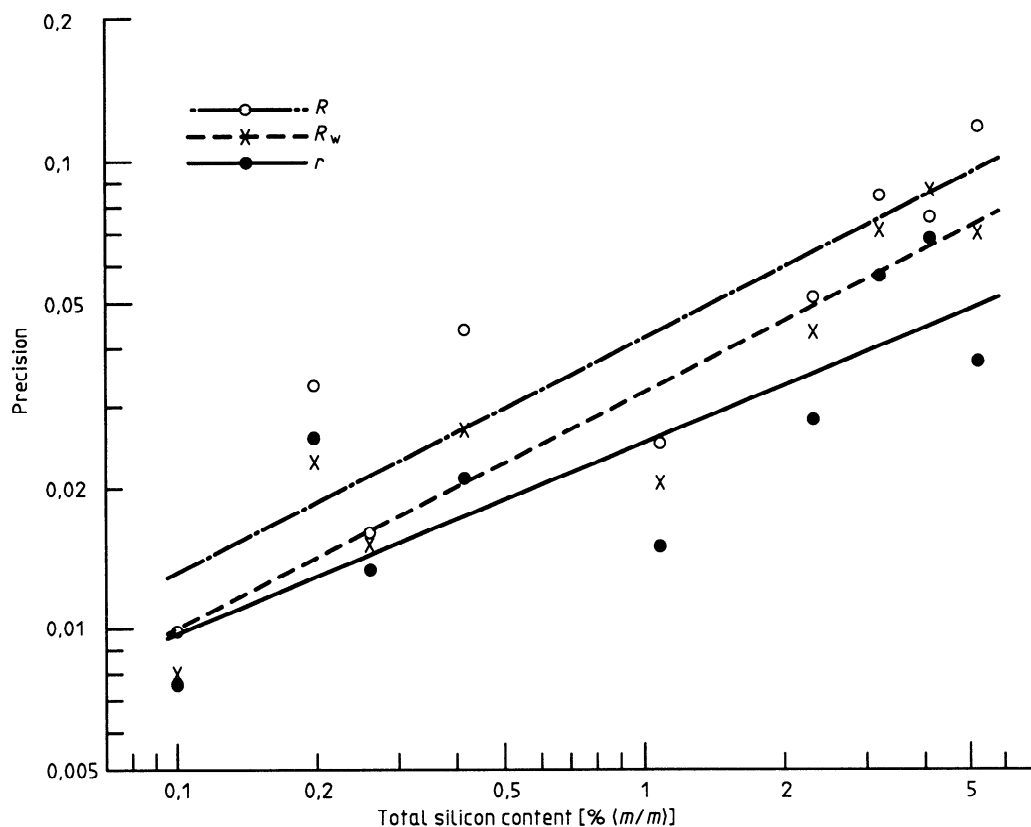

$$\lg r = 0,391\ 8 \lg \bar{w}_{\text{Si},1} - 1,586$$

$$\lg R_w = 0,498\ 1 \lg \bar{w}_{\text{Si},2} - 1,482$$

$$\lg R = 0,480\ 5 \lg \bar{w}_{\text{Si},1} - 1,377$$

where

$\bar{w}_{\text{Si},1}$ is the average silicon content, expressed as a percentage by mass, obtained within a day;

$\bar{w}_{\text{Si},2}$ is the average silicon content, expressed as a percentage by mass, obtained between days.

Figure B.1 — Logarithmic relationship between total silicon content (\bar{w}_{Si}) and repeatability (r) or reproducibility (R and R_w)

BSI - British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001 Email: orders@bsigroup.com You may also buy directly using a debit/credit card from the BSI Shop on the Website <http://www.bsigroup.com/shop>

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact Information Centre. Tel: +44 (0)20 8996 7111 Fax: +44 (0)20 8996 7048 Email: info@bsigroup.com

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002 Fax: +44 (0)20 8996 7001 Email: membership@bsigroup.com

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsigroup.com/BSOL>

Further information about BSI is available on the BSI website at <http://www.bsigroup.com>.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright and Licensing Manager. Tel: +44 (0)20 8996 7070 Email: copyright@bsigroup.com