

Geometrical Product Specifications (GPS) — Dimensional measuring equipment — Design and metrological characteristics of mechanical dial gauges

ICS 17.040.30

THESE ARE THE ONLY TWO

EUROPEAN STANDARD

EN ISO 463

NORME EUROPÉENNE

EUROPÄISCHE NORM

March 2006

ICS 17.040.30

English Version

**Geometrical Product Specifications (GPS) - Dimensional
measuring equipment - Design and metrological characteristics
of mechanical dial gauges (ISO 463:2006)**

Spécification géométrique des produits (GPS) -
Instruments de mesure dimensionnel: Comparateurs
mécaniques à cadran - Caractéristiques de conception et
caractéristiques métrologiques (ISO 463:2006)

Geometrische Produktspezifikation (GPS) -
Längenmessgeräte - Konstruktionsmerkmale und
messtechnische Merkmale für mechanische Messuhren
(ISO 463:2006)

This European Standard was approved by CEN on 23 January 2006.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

Foreword

This document (EN ISO 463:2006) has been prepared by Technical Committee ISO/TC 213 "Dimensional and geometrical product specifications and verification" in collaboration with Technical Committee CEN/TC 290 "Dimensional and geometrical product specification and verification", the secretariat of which is held by AFNOR.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by September 2006, and conflicting national standards shall be withdrawn at the latest by September 2006.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

Endorsement notice

The text of ISO 463:2006 has been approved by CEN as EN ISO 463:2006 without any modifications.

Contents

Page

Foreword.....	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions.....	1
4 Design characteristics.....	2
4.1 General.....	2
4.2 Dimensions.....	2
4.3 Dial and pointer.....	5
4.4 Revolution counting device.....	6
4.5 Contact element	6
4.6 Zero adjustment.....	6
4.7 Movable limit indicators	7
4.8 Design characteristics (manufacturer's specification).....	7
5 Metrological characteristics	7
5.1 MPE and MPL for a number of metrological characteristics	7
5.2 Contact element	8
5.3 Measuring forces	8
6 Proving conformance with specification	8
6.1 General.....	8
6.2 Measurement standards for calibration of metrological characteristics.....	8
7 Marking	8
Annex A (informative) Example diagram of errors of indication	9
Annex B (informative) Example data sheet for mechanical dial gauges	10
Annex C (informative) Calibration of metrological characteristics	11
Annex D (informative) Relation to the GPS matrix model	12
Bibliography	14

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 463 was prepared by Technical Committee ISO/TC 213, *Dimensional and geometrical product specifications and verification*.

This first edition of ISO 463 cancels and replaces ISO/R 463:1965, which has been technically revised.

Introduction

This International Standard is a geometrical product specification (GPS) standard and is to be regarded as a general GPS standard (see ISO/TR 14638). It influences the chain link 5 of the chains of standards on size, distance, form of a line independent of datum, form of a line dependent of datum, form of a surface independent of datum, form of a surface independent of datum, orientation, location, circular run-out and total run-out in the general GPS matrix.

For more detailed information of the relation of the standard to other standards and the GPS matrix model see Annex D.

Geometrical Product Specifications (GPS) — Dimensional measuring equipment — Design and metrological characteristics of mechanical dial gauges

1 Scope

This International Standard specifies the most important design and metrological characteristics of mechanical dial gauges.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 14253-1, *Geometrical Product Specifications (GPS) — Inspection by measurement of workpieces and measuring equipment — Part 1: Decision rules for proving conformance or non-conformance with specifications*

ISO/TS 14253-2, *Geometrical Product Specifications (GPS) — Inspection by measurement of workpieces and measuring equipment — Part 2: Guide to the estimation of uncertainty in GPS measurement, in calibration of measuring equipment and in product verification*

ISO 14978:2006, *Geometrical Product Specification (GPS) — General concepts and requirement for GPS measuring equipment*

ISO/IEC Guide 98-3, *Uncertainty of measurement — Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*

ISO/IEC Guide 99, *International vocabulary of metrology — Basic and general concepts and associated terms (VIM)*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 14253-1, ISO/TS 14253-2, ISO 14978, VIM and the following apply.

3.1

mechanical dial gauge

measuring instrument in which the axial displacements of a plunger are transmitted and magnified by suitable mechanical means to a pointer which rotates in front of an analog circular scale

NOTE It may also be provided with a revolution-counting device, e.g. in which a pointer rotates in front of a scale which indicates the number of revolutions of the pointer or the axial displacement of the plunger.

4 Design characteristics

4.1 General

The general design and workmanship shall be such that the performance of the dial gauge complies with the requirements of this International Standard unless otherwise specified by the manufacturer.

The design and rigidity of the dial gauge shall be such that the freedom of movement of the plunger is not impaired by clamping the stem of the instrument, providing that such clamping is applied to the minimum extent necessary to achieve a stable mounting. Where alternative methods of mounting are used, e.g. attaching the lug on the back plate, the design and rigidity of that mounting shall be such that the performance is not impaired.

4.2 Dimensions

The dial gauge shall conform to the dimensions specified in Figures 1, 2 and Table 1 to ensure interchangeability.

Table 1 — Main dimensions

Values in millimetres



Size classification	Bezel diameter D_1				
	30	40	60	80	100
Range of bezel diameter D_1 ^a	28 to 36	37 to 50	51 to 70	71 to 89	90 to 115
Stem diameter D_2	8 h6	8 h6	8 h6	8 h6	8 h6
Contact element outside diameter D_3	≤ 7,5	≤ 7,5	≤ 7,5	≤ 7,5	≤ 7,5
Thread size D_4	M2,5-6H	M2,5-6H	M2,5-6H	M2,5-6H	M2,5-6H
Thread size D_5	M2,5-6g	M2,5-6g	M2,5-6g	M2,5-6g	M2,5-6g
Clamp diameter D_6 ^b	28 h6	28 h6	28 h6	28 h6	28 h6
Stem length L_1	≥ 8,5	≥ 10	≥ 12	≥ 15,5	≥ 9,5
Length L_2 ^c	≤ 12	≤ 28	≤ 34	d	d
Thread length L_3	≤ 5	≤ 5	≤ 5	≤ 5	≤ 5
Thread length L_4	≥ 6	≥ 6	≥ 6	≥ 6	≥ 6
Contact distance, centreline to back, L_5	≤ 10	≤ 10	≤ 10	≤ 10	≤ 10

^a Actual bezel diameter equals width.

^b The clamp diameter D_6 is optional.

^c Plunger pressed in.


^d Depending on the measuring range.

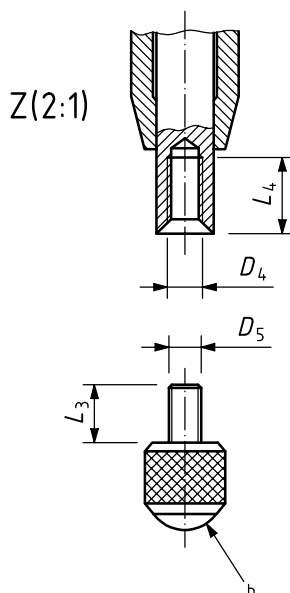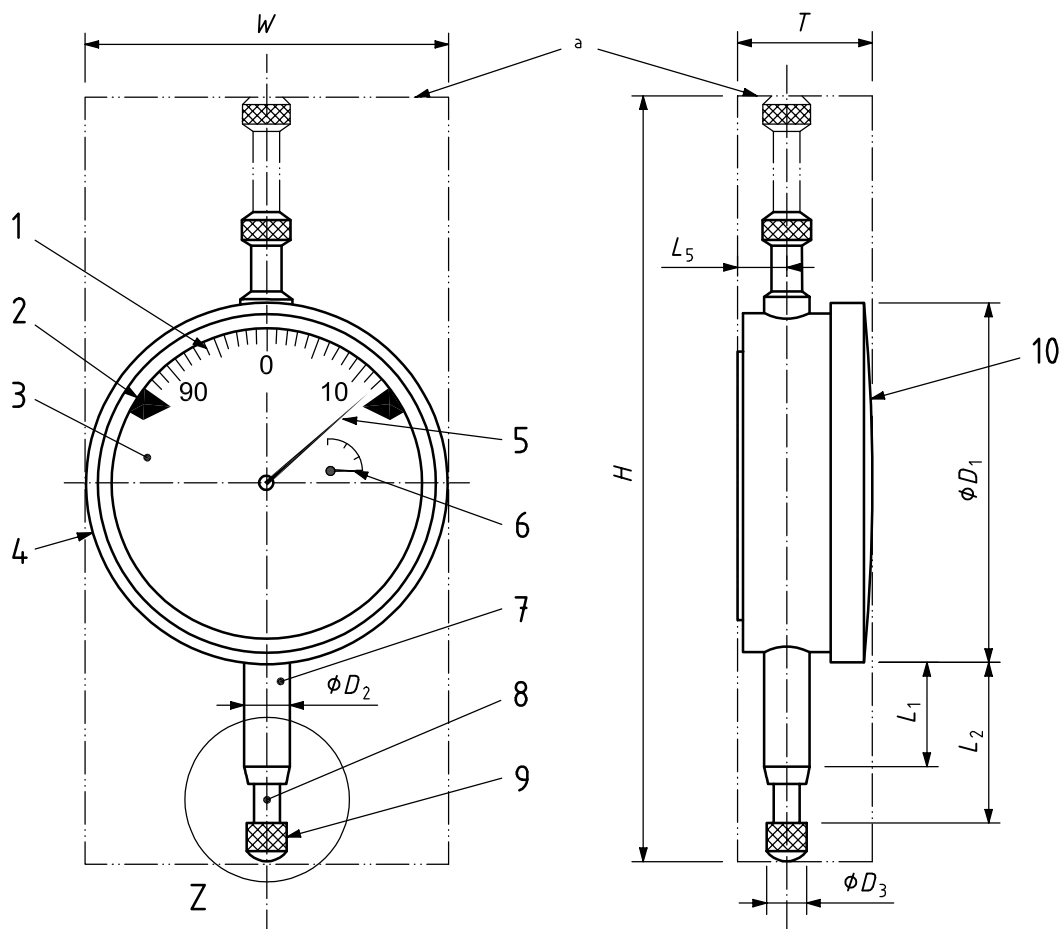

Key

- | | | | |
|-------------------|------------------------------|-------------------|---------------------------|
| 1 scale | 4 bezel | 7 stem | 10 dial cover |
| 2 limit indicator | 5 pointer | 8 plunger | a Maximum required space. |
| 3 dial | 6 revolution counting device | 9 contact element | b Measuring face. |

Figure 1 — Nomenclature and general design of dial gauge

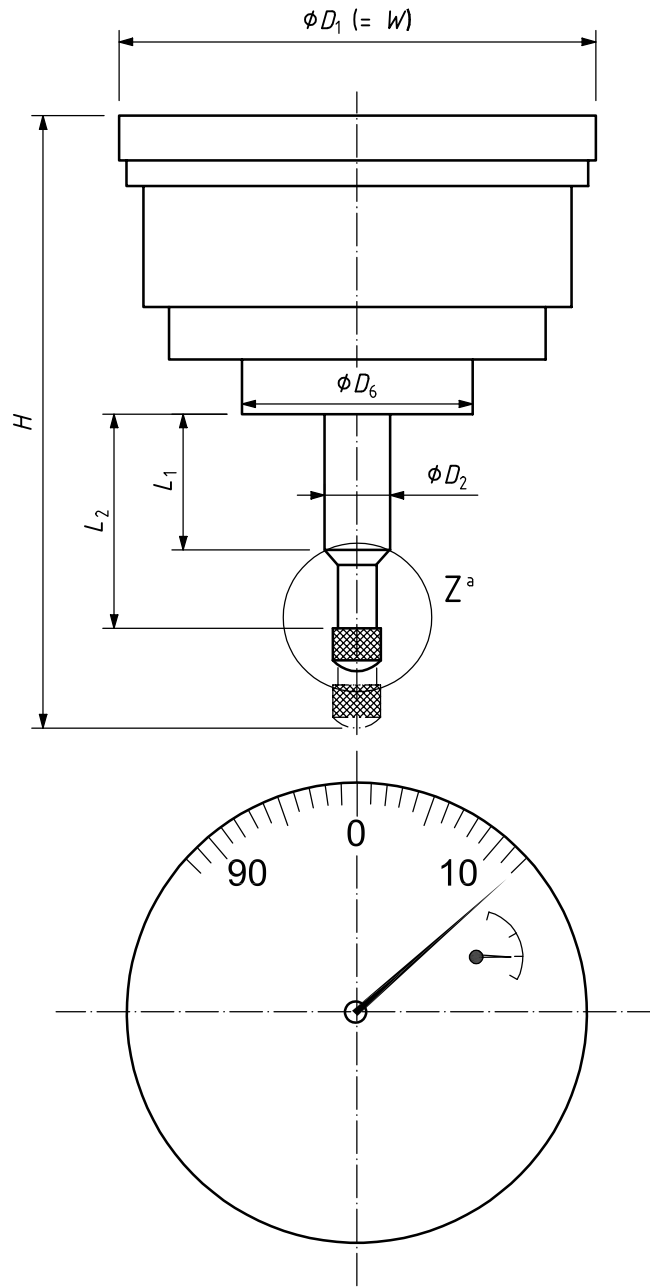

^a See Figure 1.

Figure 2 — Nomenclature and general design of dial gauge with plunger at rear

4.3 Dial and pointer

The circular scale shall be graduated in scale intervals. The scale interval and its unit shall be clearly identified. Two examples of scale layouts are shown in Figure 3 (scale interval: 0,01 mm, 0,001 mm).

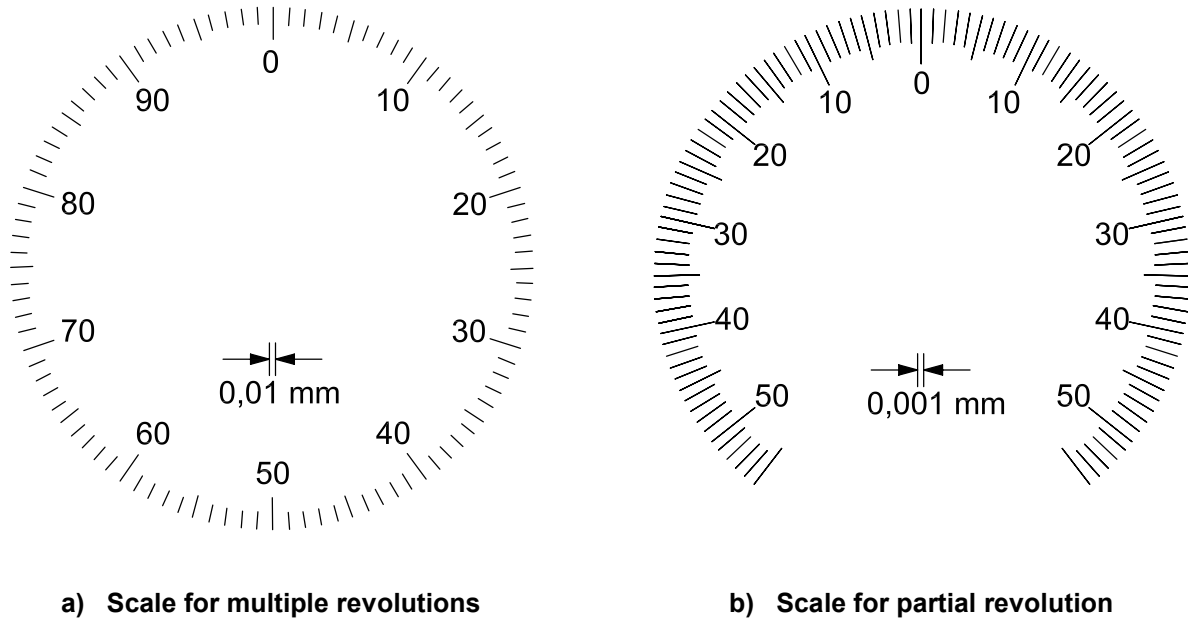


Figure 3 — Examples of scale layouts


The pointer shall move in a clockwise direction when the plunger is pressed into the gauge.

For dial gauges with more than one pointer revolution [dial layout according to Figure 3 a)]:

- When the long pointer is in the position of rest and the zero mark on the dial is at 12 o'clock, the pointer shall lie at least 1/10th of the scale range in an anticlockwise position (pre-span). Travel beyond the measuring range (post-span) shall be not less than 1/10th of the scale range [see Figure 4 a)].

For dial gauges with less than one pointer revolution [dial layout according to Figure 3 b)]:

- When the plunger is in the position of rest, the pointer shall lie at least 3 scale intervals in an anticlockwise position (pre-span). The post-span (travel beyond the measuring range) shall be such that the pointer does not reach the position which it has in the position of rest. But the post-span shall be at least 3 scale intervals [see Figure 4 b)].

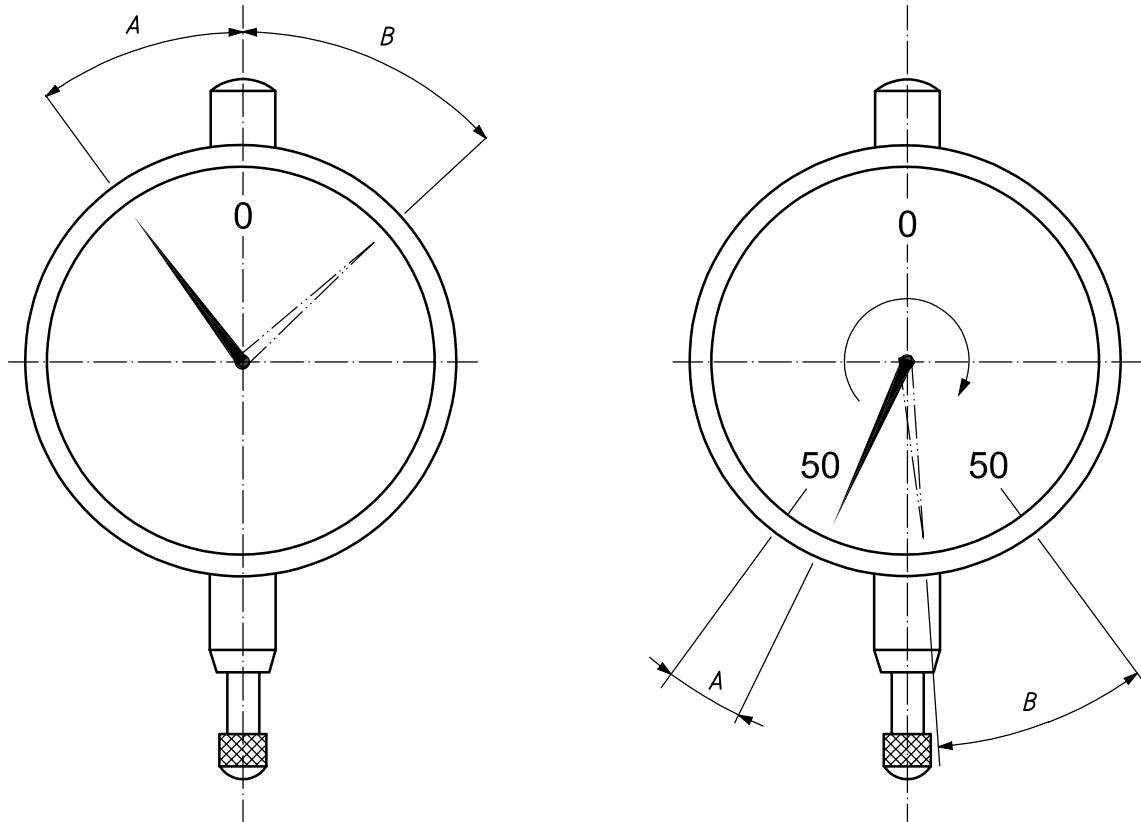

a) Dial gauge with multiple revolutions

b) Dial gauge with partial revolution

Key

- A pre-span
- B post-span

Figure 4 — Examples of pre-span and post-span

4.4 Revolution counting device

When a revolution counting device is provided, its pointer shall indicate the appropriate division on its scale when the pointer is at 12 o'clock on each of its revolutions.

4.5 Contact element

The contact element shall be replaceable. It shall have a wear-resistant measuring surface and shall be of suitable form and surface finish (see Figure 1).

4.6 Zero adjustment

Each dial gauge shall be provided with a reliable means of resetting the gauge to zero that cannot be unintentionally displaced (other than by the application of excessive force), e.g. through provision of setting a locking device such as a clamp or by frictional resistance.

4.7 Movable limit indicators

Limit indicators, where provided shall not unduly impair visibility of the scale markings (see Figure 1).

4.8 Design characteristics (manufacturer's specification)

As a minimum requirement the manufacturer shall specify at least the information set out in Table 2 (see Annex B).

Table 2 — Design characteristics

Characteristic			
Maximum required space	Width	W	mm
	Thickness	T	
	Height	H	
Measuring range			
Scale interval			
Presence of	plunger lifting device	Yes/No	
	attachment mounting and type ^a	Yes/No	
	fluid and dust protection	(Code IP)/No	
	plunger shock protection	Yes/No	
^a To be defined by the manufacturer.			

5 Metrological characteristics

5.1 MPE and MPL for a number of metrological characteristics

Maximum permissible error MPE is the extreme value of an error of a metrological characteristic permitted by the specification.

Maximum permissible limit MPL is the extreme value of a metrological characteristic permitted by the specification.

AC1 The manufacturer shall specify MPE and MPL information for the dial gauge metrological characteristics given in Table 3. For the purposes of verification after the sale, customers are free to define their own values for MPEs and MPLs, according to their company needs. Unless otherwise specified by the manufacturer, the static response of the dial gauge shall comply with these hysteresis and repeatability of error of indication MPE/MPL values at any position within the measuring range and at any orientation of the dial gauge (see Table 3). **AC1**

Table 3 — Metrological characteristics



Characteristic		MPE or MPL
Hysteresis of error of indication ^a		μm
Repeatability of error of indication		
Errors of indication over a range of	any 1/10 revolution	
	any 1/2 revolution	
	one revolution	
	the measuring range	
Measuring force	maximum	N
	minimum	
	hysteresis	
NOTE For the indication of the numerical values of the MPE and MPL, the data sheet given in Annex B can be used.		
^a The discrimination is nearly half the hysteresis.		

5.2 Contact element

The contact element and its metrological characteristics shall be appropriate for the intended measuring task.

5.3 Measuring forces

Measuring forces shall be given as the maximum measuring force, the minimum measuring force and the hysteresis of the measuring force.

The measuring force characteristics are based on a two-sided specification given in ISO 14978 :2006, 7.5.5. 

6 Proving conformance with specification

6.1 General

For proving conformance/non-conformance with specification, ISO 14253-1 applies. Uncertainty evaluation shall be performed according to ISO/TS 14253-2 and GUM.

6.2 Measurement standards for calibration of metrological characteristics

Measurement standards shall be used in accordance with the applicable International Standards.

7 Marking


The dial gauge shall be marked with serialized alpha-numeric identification.

Any marking shall be easily readable and permanent and shall be placed on the surface of the dial gauge such that it will not impair the metrological quality of the equipment.

Annex A (informative)

Example diagram of errors of indication

Figure A.1 shows an example of a diagram of errors of indication. This is a simplified data set (for data points) in order to illustrate the characteristics of the dial gauge. See also ISO 14978:—, Clause 7.

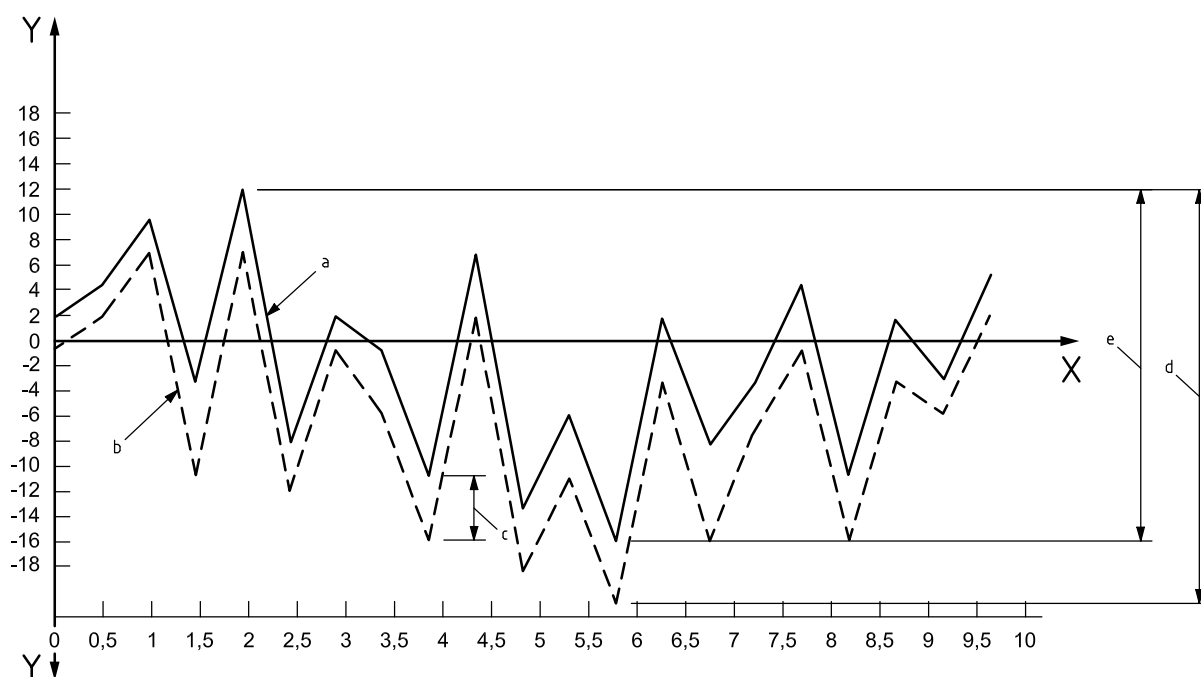

Key

X nominal value
Y error of indication

- a Error curve (plunger outward movement).
- b Error curve (plunger inward movement).
- c Hysteresis at one particular nominal value.
- d Error of indication (maximum) in both directions of plunger (floating zero).
- e Error of indication in one direction of plunger.

Figure A.1 — Diagram of errors of indication

Annex B (informative)

Example data sheet for mechanical dial gauges

This data sheet is intended for communication between technical experts and the purchasing department of the same company.

Name of equipment:

Detailed requirements:

(scale layout, contact element, protection against fluid and dust, shock protection, lifting device, attachment mounting and type, etc.)

Accessories:

Possible suppliers/manufacturers:

Price range (optional):

Additional requirements:

(e.g. inspection report, calibration certificate)

The design and metrological characteristics refer to ISO 463.

Design characteristics

Overall dimensions:

Thickness, *T*: mm Width, *W*: mm Height, *H*: mm

Measuring range: mm

Scale interval: mm

Metrological characteristics

Hysteresis of indication (MPE) μm Repeatability of indication (MPE) μm

Errors (MPE) of indication over a range of:

any 1/10 revolution μm
any 1/2 revolution μm
1 revolution μm
the measuring range μm

Measuring forces (MPL)

maximum N
minimum N
hysteresis N

MPE and MPL in the following orientations:

any vertical horizontal

Company

Department..... Person responsible Date

Annex C (informative)

Calibration of metrological characteristics

The methods should evaluate the performance of the instrument within its measuring range using both directions of displacement of the plunger.

It is essential that the dial gauge be held rigidly in a fixture which is undisturbed by the operating force of the instrument itself.

The global calibration of a sufficient number of scale points over the measuring range will necessitate a large number of readings to be taken. When it is considered that the intended use of the dial gauge does not warrant global calibration, partial calibration or task-related calibration should be considered.

For the determination of the indication errors according to Table 3, a suitable number of intervals are necessary which are dependent on the scale interval and the measuring range or the used measuring range. By these values calibration curves with fixed or floating zeros can be recorded. The MPE-function for the characteristics is given as only one two-sided specification with the constant symmetrical limits USL and LSL as the MPE for the measuring range (see AC_2 ISO 14978:2006 AC_2 , Figure 9).

It is possible to perform a modified global calibration with a reduced number of scale points by using a suitable sampling technique but this will result in an increase in the uncertainty of measurement.

Annex A shows an example of a diagram (with a very small number of scale points) of errors of indication (calibration curve) and hysteresis band of a dial gauge where zero was fixed at the lower limit of the measuring span.

By means of these measuring values the errors for various measured lengths over the measuring range could be calculated (see AC_2 ISO 14978:2006 AC_2 , Figure 7), i.e. the dial gauge is also used with floating zero indicating measuring equipment (see AC_2 ISO 14978:2006, 7.2.3). AC_2

Annex D (informative)

Relation to the GPS matrix model

For full details about the GPS matrix model see ISO/TR 14638.

D.1 Information about this International Standard and its use

This International Standard provides the most important design and metrological characteristics of mechanical dial gauges.

ISO 463 specifies the most important metrological and design characteristics of mechanical dial gauges. Only those design characteristics which are critical to interchangeability have been assigned requirement values. The metrological characteristics are not subject to requirement values as it is the philosophy that the values of these characteristics are matters of the manufacturer and/or user. However, ISO 463 provides definition of the metrological characteristics and states those metrological characteristics for which the manufacturer shall state a MPE or MPL value.

D.2 Position in the GPS matrix model

This International Standard is a general GPS standard, which influences the chain link 5 of the chains of standards on size, distance, form of a line independent of datum, form of a line dependent of datum, form of a surface independent of datum, form of a surface dependent of datum, orientation, location, circular run-out and total run-out in the general GPS matrix, as graphically illustrated in Figure D.1

Global GPS standards						
General GPS standards						
Chain link number	1	2	3	4	5	6
Size						
Distance						
Radius						
Angle						
Form of a line independent of datum						
Form of a line dependent of datum						
Form of a surface independent of datum						
Form of a surface dependent of datum						
Orientation						
Location						
Circular run-out						
Total run-out						
Datums						
Roughness profile						
Waviness profile						
Primary profile						
Surface imperfections						
Edges						

**Fundamental
GPS
standards**

Figure D.1 — GPS matrix

D.3 Related standards

The related standards are those of the chains of standards indicated in Figure D.1.

Bibliography

- [1] ISO/TR 14638:1995, *Geometrical product specification (GPS) — Masterplan*
- [2] IEC 60529:2001, *Degrees of protection provided by enclosures (IP Code)*

BSI - British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001 Email: orders@bsigroup.com You may also buy directly using a debit/credit card from the BSI Shop on the Website <http://www.bsigroup.com/shop>

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact Information Centre. Tel: +44 (0)20 8996 7111 Fax: +44 (0)20 8996 7048 Email: info@bsigroup.com

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002 Fax: +44 (0)20 8996 7001 Email: membership@bsigroup.com

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsigroup.com/BSOL>

Further information about BSI is available on the BSI website at <http://www.bsigroup.com>

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright and Licensing Manager. Tel: +44 (0)20 8996 7070 Email: copyright@bsigroup.com