

# Plastics — Determination of the viscosity of polymers in dilute solution using capillary viscometers

Part 1: General principles (ISO  
1628-1:2009)

ICS 83.080.01

## National foreword

This British Standard is the UK implementation of EN ISO 1628-1:2009+A1:2012. It supersedes BS EN ISO 1628-1:2009 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee PRI/21, Testing of plastics.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

**Compliance with a British Standard cannot confer immunity from legal obligations.**

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 July 2009

© The British Standards Institution 2012.  
Published by BSI Standards Limited 2012

ISBN 978 0 580 74406 8

### Amendments/corrigenda issued since publication

Date	Comments
31 July 2012	Implementation of ISO amendment 1:2012 with CEN endorsement A1:2012: Subclause 9.1, paragraph four amended

ICS 83.080.01

English Version

Plastics - Determination of the viscosity of polymers in dilute solution using capillary viscometers - Part 1: General principles (ISO 1628-1:2009)

Plastiques - Détermination de la viscosité des polymères en solution diluée à l'aide de viscosimètres à capillaires - Partie 1: Principes généraux (ISO 1628-1:2009)

Kunststoffe - Bestimmung der Viskosität von Polymeren in verdünnter Lösung durch ein Kapillarviskosimeter - Teil 1: Allgemeine Grundlagen (ISO 1628-1:2009)

This European Standard was approved by CEN on 12 January 2009.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION  
COMITÉ EUROPÉEN DE NORMALISATION  
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: Avenue Marnix 17, B-1000 Brussels

## **Foreword**

This document (EN ISO 1628-1:2009) has been prepared by Technical Committee ISO/TC 61 "Plastics" in collaboration with Technical Committee CEN/TC 249 "Plastics" the secretariat of which is held by NBN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by August 2009, and conflicting national standards shall be withdrawn at the latest by August 2009.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN ISO 1628-1:1998.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and the United Kingdom.

### **Endorsement notice**

The text of ISO 1628-1:2009 has been approved by CEN as a EN ISO 1628-1:2009 without any modification.

## **Foreword to amendment A1**

This document (EN ISO 1628-1:2009/A1:2012) has been prepared by Technical Committee ISO/TC 61 "Plastics" in collaboration with Technical Committee CEN/TC 249 "Plastics" the secretariat of which is held by NBN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by January 2013, and conflicting national standards shall be withdrawn at the latest by January 2013.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

### **Endorsement notice**

The text of ISO 1628-1:2009/Amd 1:2012 has been approved by CEN as a EN ISO 1628-1:2009/A1:2012 without any modification.

## Contents

Page

Foreword.....	iv
<b>1</b> <b>Scope</b> .....	<b>1</b>
<b>2</b> <b>Normative references</b> .....	<b>1</b>
<b>3</b> <b>Definitions</b> .....	<b>1</b>
<b>4</b> <b>Principle</b> .....	<b>5</b>
<b>5</b> <b>Apparatus</b> .....	<b>5</b>
<b>6</b> <b>Solutions</b> .....	<b>8</b>
<b>7</b> <b>Temperature of measurement</b> .....	<b>9</b>
<b>8</b> <b>Procedure</b> .....	<b>9</b>
<b>9</b> <b>Expression of results</b> .....	<b>10</b>
<b>10</b> <b>Test report</b> .....	<b>11</b>
<b>Annex A</b> (normative) <b>Cleaning of apparatus</b> .....	<b>12</b>
<b>Annex B</b> (normative) <b>Notes on sources of error</b> .....	<b>13</b>
<b>Bibliography</b> .....	<b>16</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 1628-1 was prepared by Technical Committee ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical-chemical properties*.

This third edition cancels and replaces the second edition (ISO 1628-1:1998), of which it constitutes a minor revision intended primarily to correct an error in Subclause 9.1, paragraph 4 (starting: "The intrinsic viscosity shall be calculated from"), where, in line 2, "intrinsic-viscosity values" has been replaced by "inherent-viscosity" values.

ISO 1628 consists of the following parts, under the general title *Plastics – Determination of the viscosity of polymers in dilute solution using capillary viscometers*:

- *Part 1: General principles*
- *Part 2: Poly(vinyl chloride) resins*
- *Part 3: Polyethylenes and polypropylenes*
- *Part 4: Polycarbonate (PC) moulding and extrusion materials*
- *Part 5: Thermoplastic polyester (TP) homopolymers and copolymers*
- *Part 6: Methyl methacrylate polymers*

# Plastics – Determination of the viscosity of polymers in dilute solution using capillary viscometers –

## Part 1: General principles

### 1 Scope

This part of ISO 1628 defines the general conditions for the determination of the reduced viscosity, intrinsic viscosity and  $K$ -value of organic polymers in dilute solution. It defines the standard parameters that are applied to viscosity measurement, and can be used to develop standards for measuring the viscosities in solution of individual types of polymer. It can also be used to measure and report the viscosities of polymers in solution for which no separate standards exist.

### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3105:1994, *Glass capillary kinematic viscometers – Specifications and operating instructions*

ISO 3205, *Preferred test temperatures*

ISO 80000-1, *Quantities and units – Part 1: General*<sup>1)</sup>

ISO 80000-4, *Quantities and units – Part 4: Mechanics*

### 3 Definitions

#### 3.1 Dimensions and units

The dimensions of properties defined in this part of ISO 1628 are expressed in terms of L for length, M for mass and T for time in accordance with ISO 80000-1, while the units appropriate to the properties are given in ISO 80000-1 and ISO 80000-4.

#### 3.2 Definitions applicable to any liquid

##### 3.2.1

##### **viscosity**

viscosity of a fluid sheared between two parallel plates, one of which moves relative to the other in uniform rectilinear motion in its own plane, defined by the Newton equation

---

1) To be published. (Revision of ISO 31-0:1992)

$$\tau = \eta \dot{\gamma} \quad (1)$$

where

$\tau$  is the shear stress;

$\eta$  is the viscosity;

$\dot{\gamma}$  is the velocity gradient or rate of shear, given by  $\frac{dv}{dz}$  where  $v$  is the velocity of one plane relative to the other and  $z$  the coordinate perpendicular to the two planes

NOTE 1 The dimensions of viscosity are  $ML^{-1}T^{-1}$ .

NOTE 2 The units of viscosity are Pa·s.

NOTE 3 For practical use, the sub-multiple  $10^{-3}$  Pa·s is more convenient.

NOTE 4 Viscosity is usually taken to mean “Newtonian viscosity”, in which case the ratio of shearing stress to velocity gradient is constant. In non-Newtonian behaviour, which is the usual case with high-polymer solutions, the ratio varies with the shear rate. Such ratios are often called “apparent viscosities” at the corresponding shear rate.

### 3.2.2 viscosity/density ratio kinematic viscosity

$\nu$   
ratio defined by the equation

$$\nu = \frac{\eta}{\rho} \quad (2)$$

where  $\rho$  is the density of the fluid at the temperature at which the viscosity is measured

NOTE 1 The dimensions of kinematic viscosity are  $L^2T^{-1}$ .

NOTE 2 The units of kinematic viscosity are  $m^2 \cdot s^{-1}$ .

NOTE 3 For practical use, the sub-multiple  $10^{-6} m^2 \cdot s^{-1}$ , i.e.  $mm^2 \cdot s^{-1}$ , is more convenient.

## 3.3 Definitions applicable to polymer solutions

### 3.3.1 relative viscosity

$\eta_r$   
ratio of the viscosity of the polymer solution (of stated concentration)  $\eta$  and the viscosity of the pure solvent  $\eta_0$ , at the same temperature:

$$\eta_r = \frac{\eta}{\eta_0} \quad (3)$$

NOTE 1 Also known as viscosity ratio.

NOTE 2 The ratio has no dimensions.



### 3.3.2

#### relative viscosity increment

viscosity ratio minus one:

$$\left(\frac{\eta}{\eta_0}\right) - 1 = \frac{\eta - \eta_0}{\eta_0} \quad (4)$$

NOTE 1 Also known as viscosity ratio increment and specific viscosity.

NOTE 2 The increment has no dimensions.

### 3.3.3

#### reduced viscosity

*I*

ratio of the viscosity ratio increment to the polymer concentration *c* in the solution:

$$I = \frac{\eta - \eta_0}{\eta_0 c} \quad (5)$$

NOTE 1 Also known as viscosity number.

NOTE 2 The dimensions of reduced viscosity are L<sup>3</sup>M<sup>-1</sup>.

NOTE 3 The units of reduced viscosity are m<sup>3</sup>/kg.

NOTE 4 For practical use, the sub-multiple 10<sup>-3</sup> m<sup>3</sup>/kg, i.e. cm<sup>3</sup>/g, is more convenient and the commonly quoted numerical values for reduced viscosity (viscosity number) use these practical units.

NOTE 5 The reduced viscosity is usually determined at low concentration (less than 5 kg/m<sup>3</sup>, i.e. 0,005 g/cm<sup>3</sup>), except in the case of polymers of low molar mass, for which higher concentrations may be necessary.

### 3.3.4

#### inherent viscosity

ratio of the natural logarithm of the viscosity ratio to the polymer concentration in the solution:

$$\frac{\ln\left(\frac{\eta}{\eta_0}\right)}{c} \quad (6)$$

NOTE 1 Also known as logarithmic viscosity number.

NOTE 2 The dimensions and units are the same as those given in 3.3.3.

NOTE 3 The inherent viscosity is usually determined at low concentration (less than 5 kg/m<sup>3</sup>, i.e. 0,005 g/cm<sup>3</sup>), except in the case of polymers of low molar mass, for which higher concentrations may be necessary.

**3.3.5**  
**intrinsic viscosity**

$[\eta]$   
limiting value of the reduced viscosity or of the inherent viscosity at infinite dilution:

$$[\eta] = \lim_{c \rightarrow 0} \left( \frac{\eta - \eta_0}{\eta_0 c} \right) \tag{7}$$

$$[\eta] = \lim_{c \rightarrow 0} \frac{\ln \left( \frac{\eta}{\eta_0} \right)}{c}$$

NOTE 1 Also known as limiting viscosity number.

NOTE 2 The dimensions and units are the same as those given in 3.3.3.

NOTE 3 The effect of the shear rate on the functions defined in 3.3.1 to 3.3.5 has been neglected, since this effect is usually negligible for values of the reduced viscosity, inherent viscosity and intrinsic viscosity less than 0,5 m<sup>3</sup>/kg, i.e. 500 cm<sup>3</sup>/g. Strictly speaking, all these functions should be defined at the limiting (preferably infinitely small) value of the shear rate.

**3.3.6**  
**K-value**

constant, independent of the concentration of the polymer solution and peculiar to the polymer sample, which is a measure of the average degree of polymerization:

$$K\text{-value} = 1\,000k \tag{8}$$

NOTE 1 According to H. Fikentscher<sup>[2]</sup>,  $k$  is calculated as follows:

$$\lg \eta_r = \left( \frac{75k^2}{1 + 150kc} + k \right) 100c$$

and therefore

$$k = \frac{1,5 \lg \eta_r - 1 + \sqrt{1 + \left( \frac{2}{c} + 2 + 1,5 \lg \eta_r \right) 1,5 \lg \eta_r}}{150 + 300c} \tag{9}$$

where

$\eta_r = \frac{\eta}{\eta_0}$  = the viscosity ratio (see 3.3.1);

$c$  is the concentration, in 10<sup>3</sup> kg/m<sup>3</sup>, i.e. g/cm<sup>3</sup>.

NOTE 2 A limiting viscosity number  $[\eta]_k$  can be calculated from  $k$ :

$$[\eta]_k = 230,3 \left( 75k^2 + k \right)$$

## 4 Principle

The data needed for the evaluation of the functions defined in 3.3 are obtained by means of a capillary-tube viscometer. The efflux times of a given volume of solvent  $t_0$  and of solution  $t$  are measured at fixed temperature and atmospheric-pressure conditions in the same viscometer. The efflux time of a liquid is related to its viscosity by the Poiseuille-Hagenbach-Couette equation:

$$v = \frac{\eta}{\rho} = Ct - \left( \frac{A}{t^2} \right) \quad (10)$$

where

- $v$  is the viscosity/density ratio (see 3.2.2);
- $C$  is a constant of the viscometer;
- $A$  is a parameter of the kinetic-energy correction;
- $\rho$  is the density of the liquid;
- $t$  is the efflux time.

For the purposes of this part of ISO 1628, the kinetic energy correction  $\left( \frac{A}{t^2} \right)$  shall be regarded as negligible when it is less than 3 % of the viscosity of the solvent. Hence Equation (10) can be reduced to

$$v = \frac{\eta}{\rho} = Ct \quad (11)$$

Moreover, if the solution concentrations are limited so that the solvent density  $\rho_0$  and that of the solution  $\rho$  differ by less than 0,5 %, the viscosity ratio  $\frac{\eta}{\eta_0}$  will be given by the so-called "efflux time ratio"  $\frac{t}{t_0}$ .

The need for these constraints, and the consequences of not observing them, is developed in Annex B.

## 5 Apparatus

### 5.1 Capillary viscometer, of the suspended-level Ubbelohde type.

The use of a viscometer having the dimensions given in Figure 1 or 2 is strongly recommended. Furthermore, it is strongly recommended that the size of the viscometer be chosen from among those listed in Table 1. The choice is determined by the viscosity/density ratio of the solvent at the temperature of the measurement, as indicated in Table 1. The next-smaller viscometer can also be used.


Other types of viscometer listed in ISO 3105 can be used, provided they give results equivalent to those given by the particular size of Ubbelohde viscometer chosen on the basis of the criteria specified in the preceding paragraph. In cases of dispute, an Ubbelohde viscometer shall be used.

With automated apparatus, fitted with special timing devices, it may be possible to obtain equivalent results with larger sizes of capillary than those listed for the appropriate solvent viscosity/density ratio in Table 1.

### 5.2 Viscometer holder, suitable to hold the viscometer firmly in the thermostatic bath (5.3) in the vertical position.



Dimensions in millimetres

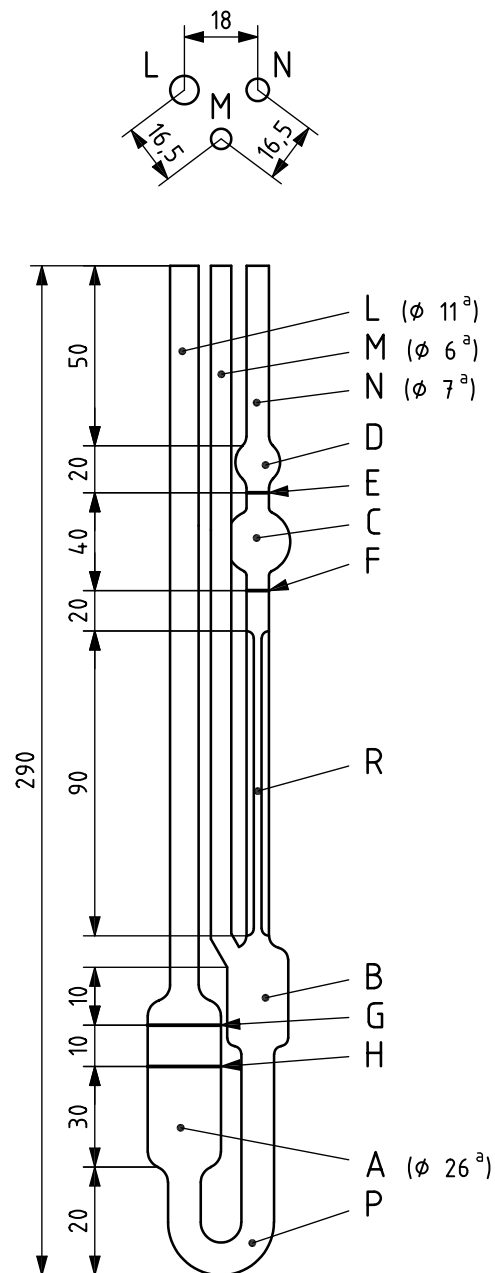

Graduation marks: E and F

Filling marks: G and H

<sup>a</sup> Internal diameter.

Figure 2 – DIN Ubbelohde viscometer

#### 5.4 Temperature-measuring device.

A liquid-in-glass “total immersion” thermometer, reading to 0,05 °C in the range in which it will be used and in a known state of calibration, is suitable. Other thermometric devices of at least equal precision may be used.

#### 5.5 Timing device.

Any timing device may be used providing that it can be read to 0,1 s and that its speed is constant to 0,1 % over 15 min.

Table 1 – Ubbelohde viscometers recommended for the determination of the dilute-solution viscosity of polymers

Viscosity/density ratio of solvent at temperature of measurement  mm <sup>2</sup> ·s <sup>-1</sup>	Ubbelohde conforming to ISO 3105:1994, Table B.4		DIN Ubbelohde conforming to ISO 3105:1994, Table B.9	
	Size No.	Diameter of capillary mm ± 2 %	Size No.	Diameter of capillary mm ± 2 %
0,15 to 0,30	0	0,24	0	0,36
0,31 to 0,50	0C	0,36	0c	0,47
0,51 to 0,75	0B	0,46	0a	0,53
0,76 to 1,50	1	0,58	I	0,63
1,51 to 2,50	1C	0,77	Ic	0,84
2,51 to 5,00	1B	0,88	Ia	0,95
5,01 to 15,00	2	1,03	II	1,13

## 6 Solutions

### 6.1 Preparation

The dissolution of the test sample of polymer in the solvent shall give a “true” solution, essentially free of microgels and associated macromolecules. Polymer degradation shall also be minimized. For these reasons, it is necessary for the dissolution procedure to be exactly defined and it is recommended that the following factors be specified:

- the solvent and its pretreatment, if any;
- the apparatus and the method of agitation;
- the temperature range within which the system is maintained during the preparation of the solution;
- the time interval necessary for the complete dissolution of the polymer without degradation, or at constant degradation;
- the stabilizer and/or the protective atmosphere used;
- the conditions of filtration of the solution, if applicable.

### 6.2 Concentration

Where no standard exists, careful consideration shall be given to the choice of solvent and the solution concentration. The solution concentration shall be chosen so that the ratio of the efflux time of the solution to the efflux time of the solvent is at least 1,2 and less than 2,0.

NOTE A lower limit of 1,2 is necessary to ensure sufficient precision of the measured difference in efflux times. The upper limit of 2,0 is necessary because, at higher molecular masses, there can be shear effects and non-linearity of the viscosity number in relation to concentration.

More than one concentration can therefore be used for a given polymer/solvent system, depending on the molecular mass of the polymer under test.

The concentration is preferably expressed in kg/m<sup>3</sup> of solution or as the multiple 10<sup>3</sup> kg/m<sup>3</sup>, i.e. g/cm<sup>3</sup>.

## 7 Temperature of measurement

The temperature shall be chosen with due regard to sufficient solubility and other technical requirements, but kept constant for any particular polymer/solvent system. The temperature tolerance shall be specified. A temperature of  $25\text{ °C} \pm 0,05\text{ °C}$  shall be chosen whenever possible. If another temperature is used, it shall be chosen from the values recommended in ISO 3205 and stated in the test report.

## 8 Procedure

### 8.1 General

Measure the efflux times for the solution and the solvent successively in the same viscometer, using the procedure described in 8.2 and 8.3.

### 8.2 Preparing and charging the viscometer

Maintain the bath at the specified test temperature.

Charge the dry, clean viscometer (for the cleaning procedure, see Annex A) by tilting it about  $30^\circ$  from the vertical and pouring sufficient liquid through tube L (see Figure 1 or 2) so that, when the viscometer is returned to the vertical, the meniscus is between the filling marks G and H. Avoid trapping air bubbles in the viscometer. The initial filling may be carried out away from the bath.

Mount the viscometer in a holder in the bath, ensuring that tube N is vertical. Allow time for the charged viscometer to reach the temperature of the bath. Usually 15 min will suffice if the measurement is to be made at  $25\text{ °C}$ . At higher temperatures, longer times may be necessary. Unnecessary delays should be avoided as it is found that the most consistent results are obtained shortly after temperature equilibrium is attained with a freshly charged viscometer.

This procedure shall also be followed when a measured amount of solvent is added to a solution, already contained in the viscometer, in order to create a more dilute solution for additional determinations. The additional solvent shall be maintained at the specified test temperature prior to use.

In automated equipment, the viscometer is fixed in the vertical position within a temperature-controlled bath and the apparatus is designed to fill the viscometer with liquid in this position. The bath shall be maintained at the specified test temperature and an equilibration time selected in accordance with paragraph 3 of this subclause.

### 8.3 Efflux time measurement (refer to Figure 1 or 2)

Close tube M and apply suction to tube N, or pressure to tube L, until the liquid reaches a level about 5 mm above mark E. Hold the liquid at this level by closing tube N.

Open tube M so that the liquid drops away from the lower end of capillary tube R.

When the liquid is clear of the end of the capillary and the lower end of tube M, open tube N. Measure the efflux time to the nearest 0,2 s as the time taken for the bottom of the meniscus to pass from the top edge of mark E to the top edge of mark F. For polymer solutions containing small amounts of finely divided pigments, e.g. carbon black, it may be necessary to view the top of the meniscus. Where large concentrations of pigments are involved, it may be necessary to centrifuge the solution before proceeding.

The opening and closing of the tubes may be carried out conveniently by means of taps or clips on clean flexible tubing attached to the ends of the tubes, making sure that no fluff or other contaminant enters the tube.

The first flow shall not be taken into account for measuring the efflux time. Repeat the measurement of efflux time immediately, without emptying or recharging, until two successive efflux times agree to within 0,25 %. Take the mean of these two values as the efflux time.

If two successive determinations of the mean efflux time of the solvent differ by more than 0,4 s, clean the viscometer (see Annex A).

The efflux time for any “new” solution, created by the addition of solvent to an existing solution held in the viscometer, shall be determined as a separate liquid, in accordance with this procedure.

## 9 Expression of results

### 9.1 Reduced viscosity and intrinsic viscosity

Results are preferably expressed as a reduced viscosity.

The reduced viscosity  $I$ , in the units  $10^{-3} \text{ m}^3/\text{kg}$ , i.e.  $\text{cm}^3/\text{g}$ , is calculated from the equation

$$I = \frac{t - t_0}{t_0 c} \quad (12)$$

where

- $t$  is the efflux time of the solution, in seconds;
- $t_0$  is the efflux time of the solvent, in seconds, through the same viscometer;
- $c$  is the concentration, expressed as  $10^3 \text{ kg}/\text{m}^3$ , i.e.  $\text{g}/\text{cm}^3$ .

The results can also be expressed as an intrinsic viscosity  $[\eta]$ , for example in order to compare copolymers of different average molecular masses for which it has been necessary to use different concentrations (see 6.2).

The intrinsic viscosity shall be calculated from the values of inherent viscosity or reduced viscosity obtained for concentrations  $c_1, c_2, c_3 \dots$ , in the approximate ratio 1:2:3 ..., by a graphical method consisting of plotting the inherent-viscosity values or the reduced-viscosity values (on the ordinate axis) against the concentration (on the abscissa) and extrapolating the curve to zero concentration. The intrinsic viscosity is read off the ordinate axis.

NOTE It is recommended that the method of least squares be used for analysing the experimental values.

The intrinsic viscosity  $[\eta]$  can also be calculated from one value of the reduced viscosity, for instance by the following equation:

$$[\eta] = \frac{I}{1 + k'cI} \quad (13)$$

where  $k'$  is an experimental constant, usually between 0,2 and 0,3, which must be determined previously by measuring the reduced viscosity at two different concentrations and applying the equation

$$k' = \frac{I_2 - I_1}{I_1 I_2 (c_2 - c_1)} \quad (14)$$

In the calculation of  $k'$ , it may be preferable to use several concentrations and plot  $I$  against  $c$ , drawing a straight line through the points and selecting two positions on this line to give values for substitution in the equation for  $k'$ .



## 9.2 *K*-value

The *K*-value can be calculated from the relationship

$$K\text{-value} = 1\,000k \quad (15)$$

where *k* is defined by the equations given in 3.3.6.

## 10 Test report

The test report shall contain the following particulars:

- a) a reference to this part of ISO 1628 and the particular standard for the polymer tested, if one exists;
- b) all details necessary for identification of the material tested, including type, source and manufacturer's code number;
- c) the concentration of material in the solution used, a description of the solvent and details of the preparation of the solution;
- d) details of the viscometer used;
- e) the temperature of the test;
- f) the test results;
- g) the date of the test.

## Annex A (normative)

### Cleaning of apparatus

It is essential that all apparatus coming into contact with the liquid under test is scrupulously clean. Any impurities, such as dust, traces of liquid or filaments in the viscometer, will cause false results to be obtained.

Before the test, clean the viscometer and all other apparatus used (glass vessels, pipettes, sintered-glass filters, rubber tubing, etc.). A suitable detergent may be adequate. Aqua regia (3 volumes concentrated hydrochloric acid and 1 volume concentrated nitric acid) may be required to remove inorganic residues from the glassware, and a suitable solvent may be required to remove oil and grease. Following this, dry the glass apparatus and then clean it with specially prepared chromic acid solution. Leave this solution in contact with the glassware overnight at a minimum temperature of 20 °C. For more active cleaning, warm the chromic acid gently on a water bath.

Remove the chromic acid and rinse at least five times with distilled or deionized water. Dry in an electric oven at a temperature no higher than 100 °C or rinse at least five times with acetone that has been distilled, dried and filtered, drying the apparatus with a slow stream of filtered dry air or, preferably, with a vacuum line.

Between successive determinations of the efflux times of samples of a similar nature, the viscometer may be cleaned by draining and thoroughly rinsing with a suitable volatile solvent that has been distilled and filtered. Dry the apparatus with a slow stream of filtered dry air, with a vacuum line, or in an electric oven at a temperature no higher than 100 °C. The effectiveness of the cleaning can be checked by establishing that the efflux times with a given solvent and viscometer remain constant.

If the next solution to be measured is of a polymer of the same type and of similar viscosity, it is permissible to drain the viscometer, wash it with the next solution to be measured and then fill it with a further quantity of this solution.

It is recommended that viscometers used for silicone fluids and fluorocarbons be reserved exclusively for use with these fluids and that these viscometers be subject to calibration checks at frequent intervals. Great care shall be taken to ensure that these fluids do not contaminate other apparatus, either directly or indirectly.

**WARNING – Particular care should be taken when using aqua regia and chromic acid. Chromic acid is toxic. Appropriate action should also be taken to ensure the safe disposal of these acids. Goggles and protective gloves should be worn. Any splashes should be washed off the skin immediately with plenty of cold water. Inhalation of the vapours should be avoided.**

## Annex B (normative)

### Notes on sources of error

#### B.1 General

Guidance is given in this part of ISO 1628 on the determination of the viscometric properties of polymers in dilute solution as defined in Clause 3. The measurement of these properties can usually be carried out with better reproducibility than that attained in absolute measurements of viscosity since many of the instrumental errors are approximately the same for both solvent and solution, and are effectively cancelled.

#### B.2 Principle of measurements

The relative viscosity and the other parameters defined in Clause 3 are calculated from the efflux times of solution and solvent. The liquid flows, under the force of gravity, through the capillary of a suspended-level Ubbelohde viscometer. The efflux times are taken to be proportional to the viscosity/density ratio of the fluids (see Clause 4). This is equivalent to stating that the kinetic energy and other errors are negligible and that the density of the solvent differs negligibly from the density of the solutions.

#### B.3 Sources of error

The most important sources of error in capillary viscometry are related to

- a) surface tension;
- b) capillary end effects;
- c) drainage effects;
- d) viscous heat effects;
- e) deviation of the viscometer from the vertical;
- f) hydrostatic head variations;
- g) losses by evaporation;
- h) errors in the measurement of the concentration and efflux time;
- i) shear effects;
- j) errors in temperature stability and measurement;
- k) kinetic energy.

Fortunately, most of these effects can be considered negligible for the proposed procedures. Errors due to surface tension, end effects and drainage effects are quite small in tests with organic solvents in the Ubbelohde viscometer, when relative measurements of viscosity are concerned<sup>[3],[4]</sup>. Viscous heat effects are negligible when the capillary viscometer is operated by gravity. Errors due to deviation from the vertical and variations in the hydrostatic head are usually very small with this type of viscometer.

Solvent losses by evaporation and concentration errors depend on the particular test procedure and have to be taken into account.

The solvent efflux time should preferably be at least 70 s in order to measure it reproducibly, but it should not be longer than about 200 s in order to avoid long efflux times for the corresponding solutions.

The effect of shear rate can be serious, since polymer solutions are often non-Newtonian<sup>[5],[6]</sup>. Strictly speaking, the measurements should be carried out at very low shear rates, but in the usual procedures the shear rate is as high as 1 000 s<sup>-1</sup> or more. Fortunately, it can be shown<sup>[7],[8],[9]</sup> that shear rate effects are very small unless the molar mass of the polymer is higher than 10<sup>6</sup> g/mol, which seldom happens with commercial polymers. Furthermore, it would be impractical to take account of shear rate effects for the purposes of international standardization, and a better approach is to define the tolerance of the viscometer dimensions in such a way that the shear rate is closely reproducible in different laboratories testing the same polymer sample.

It may be concluded that the most important source of error in the measurements is the kinetic-energy term. Its value can be considerable. For example, it is approximately 15 % for chloroform in a standard Ubbelohde viscometer having a capillary diameter of 0,58 mm. The resultant error in the reduced viscosity can be of the order of 30 % and, for special work outside the scope of this part of ISO 1628, it might be appropriate to include a kinetic-energy correction.

#### B.4 Choice of viscometers

Since it is impractical to introduce a kinetic-energy correction into international standardization, it is necessary to choose the viscometer in such a way that

- a) either the kinetic-energy term is negligible;
- b) or it is constant and reproducible in different laboratories.

It can be shown that the second condition cannot be realized easily. In fact, the maximum fractional hydrostatic pressure  $X$  spent in kinetic energy is given approximately by the equation

$$X = \frac{R^4 h g}{64 L^2 \nu^2} \quad (\text{B.1})$$

where

- $R$  is the radius of the capillary;
- $h$  is the hydrostatic head;
- $g$  is the acceleration due to gravity;
- $L$  is the length of the capillary;
- $\nu$  is the viscosity/density ratio.

It is important to note in Equation (B.1) that the efflux time and the reservoir volume by themselves do not influence the value of  $X$ .

For standard glass capillaries with diameters between 0,3 mm and 1,0 mm, the tolerance limits for the diameter<sup>[10],[11]</sup> are usually  $\pm 0,02$  mm, corresponding to approximately  $\pm 30$  % and  $\pm 8$  %, respectively, of the value of  $X$ , whereas the mean hydrostatic head  $h$  is 120 mm  $\pm$  10 mm and the capillary length  $L$  is 90 mm  $\pm$  9 mm, corresponding to approximately  $\pm 30$  % of the value of  $X$ . The conclusion is that, unless the normal tolerances on standard capillaries are severely restricted, the kinetic-energy term cannot be made reproducible. It is therefore necessary to choose viscometers which minimize it.

In this part of ISO 1628, the maximum permitted value of  $X$  is fixed at 0,03 (approximately 4 % to 6 % of the reduced viscosity).

From Equation (B.1), it can be seen that, at fixed values of  $h$  and  $L$ , the critical parameter which defines the magnitude of  $X$  is the ratio  $R^2/\nu$ .

By inserting

$$h = 120 \text{ mm},$$

$$L = 90 \text{ mm}$$

and

$$X < 0,03$$

in Equation (B.1), a relationship between the maximum capillary radius to be used and the value of  $\nu$  is obtained:

$$R^2 < 0,111\nu \quad (\text{B.2})$$

or, for the diameter,

$$D^2 < 0,444\nu \quad (\text{B.3})$$

where  $R$  and  $D$  are in mm and  $\nu$  is in  $\text{mm}^2\text{-s}^{-1}$ .

It will be noted that Equation (B.3) is dependent on the particular values ascribed to the mean hydrostatic head and the capillary length. These will vary between various designs of viscometer and, in particular, are slightly different for the Ubbelohde and DIN Ubbelohde versions.

Equation (B.3) permits calculation of the maximum theoretical diameter that could be used for a solvent whose viscosity/density ratio  $\nu$  is known at the temperature of measurement. It follows that, in order to determine the properties of polymers described in this part of ISO 1628, the viscosity/density ratio for the solvent chosen must be known. Table B.1 gives values at 25 °C for several of the established solvents for polymers, together with the calculated theoretical maximum capillary diameter for the Ubbelohde viscometer.

Equation (B.3) has also been used to select the recommended sizes of Ubbelohde and DIN Ubbelohde viscometers given in Table 1. Other appropriate series of viscometers and sizes can be identified by substituting the relevant values into Equation (B.1).

**Table B.1 – Examples of viscosity/density ratios for established polymer solvents, and the corresponding maximum theoretical capillary diameters**

Solvent	Viscosity/density ratio at 25 °C	Maximum theoretical capillary diameter from Equation (B.3)
	$\text{mm}^2\text{-s}^{-1}$	mm
Cyclohexanone	2,10	0,97
Dichloromethane	0,33	0,38
<i>m</i> -Cresol (meta-cresol)	13,10	2,41
Trichloromethane	0,36	0,40

## Bibliography

- [1] *Compendium of macromolecular nomenclature*, METANOMSKI, W.V., IUPAC and Blackwell Scientific Publications, 1991
- [2] FIKENTSCHER, H., *Cellulosechemie*, **13**, pp. 58-64 (1932)
- [3] ONYON, P.F., in *Techniques of polymer characterisation*, ed. by ALLEN, P.W., Butterworths, London, 1959
- [4] CRAGG, L.H., and VAN OENE, H., *Can. J. Chem.*, **39**, 203 (1961)
- [5] PASSAGLIA, E., YOUNG, J.T., and WEGEMER, N.J., *J. Polymer Sci.*, **47**, 333 (1960)
- [6] LOHMANDER, U. *Makromol. Chem.* **72**, 159 (1964)
- [7] KRIGBAUM, W.R., and FLORY, P.J., *J. Polymer Sci.*, **11**, 37 (1953)
- [8] CRAGG, L.H., STONES, R.H., and DUMITRU, T.E., *J. Polymer Sci.*, **13**, 167 (1954)
- [9] MERRIL, E.W., MICKLEY, H.S., RAM, A., and PERKINSON, G., *Trans. Soc. Rheol.*, **5**, 237 (1961) and **6**, 119 (1962)
- [10] ASTM D 446, *Standard Specifications and Operating Instructions for Glass Capillary Kinematic Viscometers*
- [11] BS 188, *Methods for the determination of the viscosity of liquids*



# British Standards Institution (BSI)

BSI is the independent national body responsible for preparing British Standards and other standards-related publications, information and services. It presents the UK view on standards in Europe and at the international level.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

## Revisions

British Standards and PASs are periodically updated by amendment or revision. Users of British Standards and PASs should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using British Standards would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Similarly for PASs, please notify BSI Customer Services.

**Tel: +44 (0)20 8996 9001 Fax: +44 (0)20 8996 7001**

BSI offers BSI Subscribing Members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of British Standards and PASs.

**Tel: +44 (0)20 8996 7669 Fax: +44 (0)20 8996 7001**

**Email: [plus@bsigroup.com](mailto:plus@bsigroup.com)**

## Buying standards

You may buy PDF and hard copy versions of standards directly using a credit card from the BSI Shop on the website [www.bsigroup.com/shop](http://www.bsigroup.com/shop). In addition all orders for BSI, international and foreign standards publications can be addressed to BSI Customer Services.

**Tel: +44 (0)20 8996 9001 Fax: +44 (0)20 8996 7001**

**Email: [orders@bsigroup.com](mailto:orders@bsigroup.com)**

In response to orders for international standards, BSI will supply the British Standard implementation of the relevant international standard, unless otherwise requested.

## Information on standards

BSI provides a wide range of information on national, European and international standards through its Knowledge Centre.

**Tel: +44 (0)20 8996 7004 Fax: +44 (0)20 8996 7005**

**Email: [knowledgecentre@bsigroup.com](mailto:knowledgecentre@bsigroup.com)**

BSI Subscribing Members are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.

**Tel: +44 (0)20 8996 7002 Fax: +44 (0)20 8996 7001**

**Email: [membership@bsigroup.com](mailto:membership@bsigroup.com)**

Information regarding online access to British Standards and PASs via British Standards Online can be found at

**[www.bsigroup.com/BSOL](http://www.bsigroup.com/BSOL)**

Further information about British Standards is available on the BSI website at **[www.bsigroup.com/standards](http://www.bsigroup.com/standards)**

## Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained. Details and advice can be obtained from the Copyright & Licensing Department.

**Tel: +44 (0)20 8996 7070**

**Email: [copyright@bsigroup.com](mailto:copyright@bsigroup.com)**

## BSI

389 Chiswick High Road London W4 4AL UK

Tel +44 (0)20 8996 9001

Fax +44 (0)20 8996 7001

[www.bsigroup.com/standards](http://www.bsigroup.com/standards)