

# Metallic materials — Vickers hardness test —

## Part 3: Calibration of reference blocks

The European Standard EN ISO 6507-3:2005 has the status of a British Standard

ICS 77.040.10

## National foreword

This British Standard is the official English language version of EN ISO 6507-3:2005. It is identical with ISO 6507-3:2005. It supersedes BS EN ISO 6507-3:1998 which is withdrawn.

The UK participation in its preparation was entrusted by Technical Committee ISE/NFE/4, Mechanical testing of metals, to Subcommittee ISE/NFE/4/5, Indentation hardness testing, which has the responsibility to:

- aid enquirers to understand the text;
- present to the responsible international/European committee any enquiries on the interpretation, or proposals for change, and keep UK interests informed;
- monitor related international and European developments and promulgate them in the UK.

A list of organizations represented on this subcommittee can be obtained on request to its secretary.

### Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the *BSI Catalogue* under the section entitled “International Standards Correspondence Index”, or by using the “Search” facility of the *BSI Electronic Catalogue* or of British Standards Online.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

**Compliance with a British Standard does not of itself confer immunity from legal obligations.**

### Summary of pages

This document comprises a front cover, an inside front cover, the EN ISO title page, the EN ISO foreword page, the ISO title page, pages ii to iv, pages 1 to 9 and a back cover.

The BSI copyright notice displayed in this document indicates when the document was last issued.

### Amendments issued since publication

Amd. No.	Date	Comments

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 20 January 2006

© BSI 20 January 2006

English Version

**Metallic materials - Vickers hardness test - Part 3: Calibration of  
reference blocks (ISO 6507-3:2005)**

Matériaux métalliques - Essai de dureté Vickers - Partie 3:  
Etalonnage des blocs de référence (ISO 6507-3:2005)

Metallische Werkstoffe - Härteprüfung nach Vickers - Teil  
3: Kalibrierung von Härtevergleichsplatten (ISO 6507-  
3:2005)

This European Standard was approved by CEN on 14 December 2005.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION  
COMITÉ EUROPÉEN DE NORMALISATION  
EUROPÄISCHES KOMITEE FÜR NORMUNG

**Management Centre: rue de Stassart, 36 B-1050 Brussels**

# EN ISO 6507-3:2005

## Foreword

This document (EN ISO 6507-3:2005) has been prepared by Technical Committee ISO/TC 164 "Mechanical testing of metals" in collaboration with Technical Committee ECISS/TC 1 "Steel - Mechanical testing", the secretariat of which is held by AFNOR.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by June 2006, and conflicting national standards shall be withdrawn at the latest by June 2006.

This document supersedes EN ISO 6507-3:1997.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

## Endorsement notice

The text of ISO 6507-3:2005 has been approved by CEN as EN ISO 6507-3:2005 without any modifications.

INTERNATIONAL  
STANDARD

**ISO**  
**6507-3**

Third edition  
2005-12-15

---

---

**Metallic materials — Vickers hardness  
test —**

Part 3:  
**Calibration of reference blocks**

*Matériaux métalliques — Essai de dureté Vickers —  
Partie 3: Étalonnage des blocs de référence*



Reference number  
ISO 6507-3:2005(E)



<b>Contents</b>		Page
<b>Foreword</b> .....		iv
<b>1</b>	<b>Scope</b> .....	<b>1</b>
<b>2</b>	<b>Normative references</b> .....	<b>1</b>
<b>3</b>	<b>Manufacture of reference blocks</b> .....	<b>1</b>
<b>4</b>	<b>Calibration machine</b> .....	<b>2</b>
<b>5</b>	<b>Calibration procedure</b> .....	<b>4</b>
<b>6</b>	<b>Number of indentations</b> .....	<b>4</b>
<b>7</b>	<b>Uniformity of hardness</b> .....	<b>4</b>
<b>8</b>	<b>Marking</b> .....	<b>5</b>
<b>9</b>	<b>Validity</b> .....	<b>5</b>
<b>Annex A (informative) Uncertainty of the mean hardness value of hardness-reference blocks</b> .....		<b>6</b>
<b>Bibliography</b> .....		<b>9</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 6507-3 was prepared by Technical Committee ISO/TC 164, *Mechanical testing of metals*, Subcommittee SC 3, *Hardness testing*.

This third edition cancels and replaces the second edition (ISO 6507-3:1997), which has been technically revised.

ISO 6507 consists of the following parts, under the general title *Metallic materials — Vickers hardness test*:

- *Part 1: Test method*
- *Part 2: Verification and calibration of testing machines*
- *Part 3: Calibration of reference blocks*
- *Part 4: Tables of hardness values*



# Metallic materials — Vickers hardness test —

## Part 3: Calibration of reference blocks

### 1 Scope

This part of ISO 6507 specifies a method for the calibration of reference blocks to be used for the indirect verification of Vickers hardness testing machines, as specified in ISO 6507-2.

The method is applicable only for indentations with diagonals  $\geq 0,020$  mm.

### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 376:2004, *Metallic materials — Calibration of force-proving instruments used for the verification of uniaxial testing machines*

ISO 4287:1997, *Geometrical Product Specifications (GPS) — Surface texture: Profile method — Terms, definitions and surface texture parameters*

ISO 6507-1:2005, *Metallic materials — Vickers hardness test — Part 1: Test method*

ISO 6507-2:2005, *Metallic materials — Vickers hardness test — Part 2: Verification and calibration of testing machines*

### 3 Manufacture of reference blocks

**3.1** The block shall be specially manufactured for use as a hardness-reference block.

NOTE Attention is drawn to the need to use a manufacturing process which will give the necessary homogeneity, stability of structure and uniformity of surface hardness.

**3.2** Each metal block to be calibrated shall be of a thickness not less than 5 mm.

**3.3** The reference blocks shall be free of magnetism. It is recommended that the manufacturer shall ensure that the blocks, if made of steel, have been demagnetized at the end of the manufacturing process.

**3.4** The maximum deviation in flatness of the test and support surfaces shall not exceed 0,005 mm. The maximum error in parallelism shall not exceed 0,010 mm in 50 mm.

**3.5** The test surface shall be free from scratches which interfere with the measurement of the indentations. The surface roughness  $R_a$  shall not exceed 0,000 05 mm for the test surface and 0,000 8 mm for the bottom surface. The sampling length  $l$  shall be 0,80 mm (see ISO 4287:1997, 3.1.9).

**3.6** To verify that no material has been subsequently removed from the reference block, its thickness at the time of calibration shall be marked on it, to the nearest 0,01 mm, or an identifying mark shall be made on the test surface [see 8.1 e)].

## 4 Calibration machine

**4.1** In addition to fulfilling the general requirements specified in ISO 6507-2, the calibration machine shall also meet the requirements of 4.2 to 4.7.

**4.2** The calibration machine shall be verified directly at intervals not exceeding 12 months.

Direct verification involves

- a) verification of the test force;
- b) verification of the indenter;
- c) verification of the measuring device;
- d) verification of the testing cycle; if this is not possible, at least the force versus time behaviour.

**4.3** The instruments used for verification and calibration shall be traceable to national standards.

**4.4** Each test force shall be measured using an elastic proving device (or ISO 376:2004, Class 0.5 or better), or by another method having the same or better accuracy. This measurement shall agree with the nominal value to within  $\pm 0,1$  % for normal and low-force hardness, and to within  $\pm 0,5$  % for microhardness.

**4.5** The indenter shall meet the following requirements:

- a) The four faces of the square-based diamond pyramid shall be highly polished, free from surface defects, and flat within 0,000 3 mm.
- b) The angle between the opposite faces of the vertex of the diamond pyramid shall be  $136^\circ \pm 0,1^\circ$ .

The angle between the axis of the diamond pyramid and the axis of the indenter-holder (normal to the seating surface) shall be less than  $0,3^\circ$ .

- c) The point of the diamond indenter shall be examined with a high-power measuring microscope or preferably with an interference microscope and, if the four faces do not meet at a point, the line of junction between opposite faces shall comply with the values in Table 1.

**Table 1**

Ranges of test force, $F$ N	Maximum permissible length of the line of junction, $a$ mm
$F \geq 49,03$	0,001
$1,961 \leq F < 49,03$	0,000 5
$0,098 07 \leq F < 1,961$	0,000 25

- d) It shall be verified that the quadrilateral which would be formed by the intersection of the faces with a plane perpendicular to the axis of the diamond pyramid has angles of  $90^\circ \pm 0,2^\circ$  (see Figure 1).

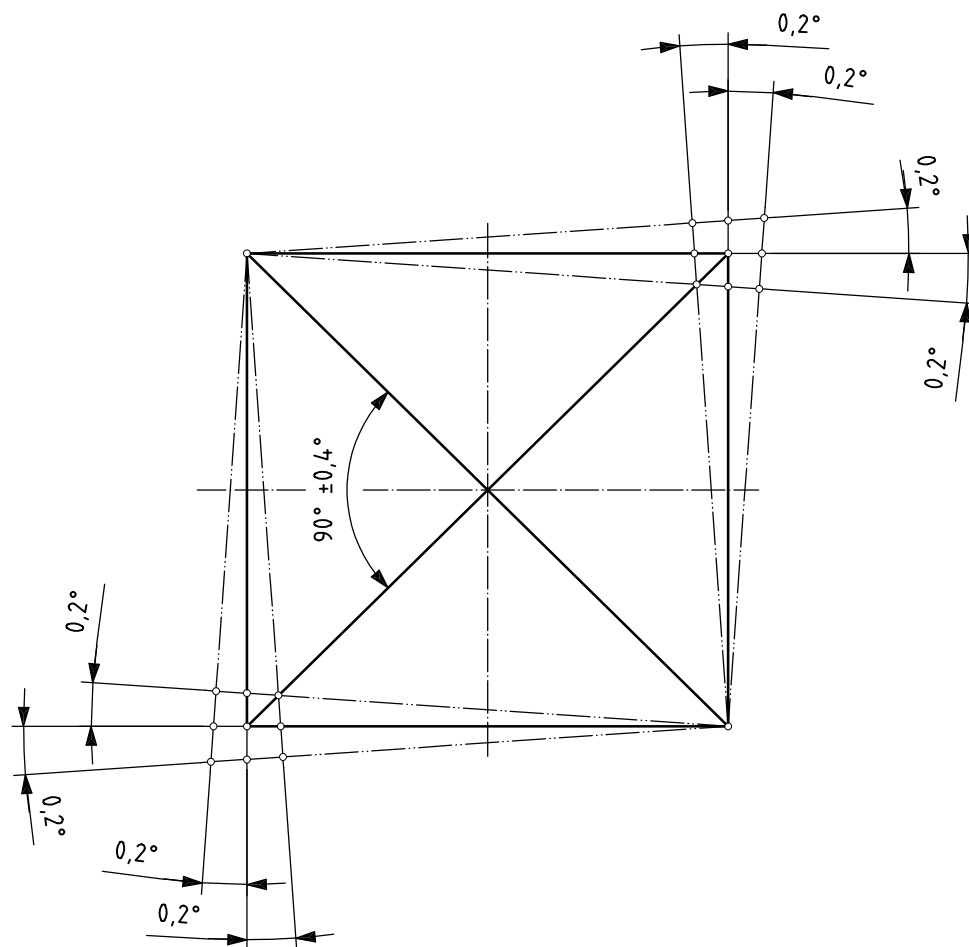


Figure 1 — Permissible difference of the sectional planes of the square form

4.6 The resolution required of the measuring device depends on the size of the smallest indentation to be measured.

The scale of the measuring device shall be graduated to permit estimation of the diagonals of the indentation in accordance with Table 2.

Table 2

Diagonal length, $d$ mm	Resolution of the measuring device	Maximum permissible error
$d \leq 0,040$	0,000 1 mm	0,000 2 mm
$0,040 < d \leq 0,200$	0,25 % of $d$	0,5 % of $d$
$d > 0,200$	0,000 5 mm	0,000 1 mm

The measuring device shall be verified by measurements made on an object micrometer at a minimum of five intervals over each working range.

The maximum permissible error shall not exceed the values given in Table 2.

## 5 Calibration procedure

The reference blocks shall be calibrated in a calibration machine as described in Clause 4, at a temperature of  $(23 \pm 5) ^\circ\text{C}$ , using the general procedure specified in ISO 6507-1.

During calibration, the thermal drift should not exceed  $1 ^\circ\text{C}$ .

The time from the initial application of force until the full test force is reached, and the approach velocity of the indenter, shall meet the requirements given in Table 3.

The duration of application of the test force shall be 13 s to 15 s.

For microhardness testing, the maximum allowable vibrational acceleration reaching the calibration machine shall be  $0,005 g_n$  ( $g_n$  equals the standard acceleration of free fall:  $g_n = 9,806 65 \text{ m/s}^2$ ).

Table 3

Ranges of test force, $F$ N	Time for application of the test force s	Approach velocity of the indenter mm/s
$F < 1,961$	$\leq 10$	0,05 to 0,2
$1,961 \leq F < 49,03$	$\leq 10$	0,05 to 0,2
$F \geq 49,03$	6 to 8	0,05 to 1

## 6 Number of indentations

On each reference block, five indentations shall be made, uniformly distributed over the test surface.

For microhardness tests and to reduce the measurement uncertainty, more than 5 indentations should be made. It is recommended to make 10, 15 or 25 indentations on 5 locations on the reference block.

## 7 Uniformity of hardness

7.1 Let  $d_1, d_2, d_3, d_4, d_5$ , be the arithmetic mean values of the measured diagonals, arranged in increasing order of magnitude, and

$$\bar{d} = \frac{d_1 + d_2 + d_3 + d_4 + d_5}{5} \quad (1)$$

The non-uniformity  $U$  of the block under the particular conditions of calibration is characterized by the difference

$$U = d_5 - d_1 \quad (2)$$

and is expressed as a percentage  $U_{\text{rel}}$ , as

$$U_{\text{rel}} = \frac{100 \times (d_5 - d_1)}{\bar{d}} \quad (3)$$

7.2 The maximum permissible value of non-uniformity  $U_{rel}$  of a reference block is given in Table 4.

**Table 4**

Hardness of block	Maximum permissible value of non-uniformity $U_{rel}$ , %		
	< HV 0,2	≤ HV 0,2 to ≤ HV 5	HV 5 to HV 100
≤ 225 HV <sup>a</sup>	4,0 or 0,001 mm <sup>b</sup>	3,0	2,0
> 225 HV		2,0	1,0

<sup>a</sup> For hardness values < 150 HV, the maximum permissible value of non-uniformity shall be 8 % or 0,001 mm, whichever is greater.  
<sup>b</sup> Whichever is greater.

7.3 The determination of the uncertainty of measurement of hardness reference blocks is given in Annex A.

## 8 Marking

8.1 Each reference block shall be marked with the following particulars:

- arithmetic mean of the hardness values found in the calibration test, for example 249 HV 30;
- name or mark of the supplier or manufacturer;
- serial number;
- name or mark of the calibrating agency;
- thickness of the block, or an identifying mark on the test surface (see 3.6);
- year of calibration, if not indicated in the serial number.

8.2 Any mark put on the side of the block shall be the right way up when the test surface is the upper face.

8.3 Each delivered reference block shall be accompanied with a document giving at least the following information:

- a reference to this part of ISO 6507;
- identity of the block;
- date of calibration;
- arithmetic mean of the hardness values and the value characterizing the non-uniformity of the block;
- information about the location of the reference indentation, together with the mean measured diagonal length.

## 9 Validity

The reference block is only valid for the scale for which it was calibrated.

The calibration validity should be limited to a duration of 5 years. Attention is drawn to the fact that, for Al- and Cu-alloys, the calibration validity could be reduced to 2–3 years.

## Annex A (informative)

### Uncertainty of the mean hardness value of hardness-reference blocks

The metrological chain necessary to define and disseminate hardness scales is shown in Figure D.1 in ISO 6507-1:2005.

#### A.1 Direct verification of the hardness-calibration machine

##### A.1.1 Calibration of the test force

See ISO 6507-2:2005, Annex C.

##### A.1.2 Calibration of the optical measuring device

See ISO 6507-2:2005, Annex C.

##### A.1.3 Verification of the indenter

See ISO 6507-2:2005, Annex C.

##### A.1.4 Verification of the test cycle

See ISO 6507-2:2005, Annex C.

#### A.2 Indirect calibration of the hardness-calibration machine

NOTE In this Annex, the index "CRM (Certified Reference Material)" means, according to the definitions of the hardness testing standards, "Hardness Reference Block".

By the indirect verification with primary hardness-reference blocks, the overall function of the hardness calibration machine is checked and the repeatability, as well as the deviation of the hardness-calibration machine from the actual hardness value, are determined.

The uncertainty of measurement of the indirect calibration of the hardness-calibration machine follows from the equation:

$$u_{CM} = \sqrt{u_{CRM-P}^2 + u_{xCRM-1}^2 + u_{CRM-D}^2 + u_{ms}^2} \quad (A.1)$$

where

$u_{CRM-P}$  is the calibration uncertainty of the primary hardness-reference block, according to the calibration certificate for  $k = 1$ ;

$u_{xCRM-1}$  is the standard deviation of the hardness-calibration machine due to its repeatability;

$u_{CRM-D}$  is the hardness change of the primary hardness-reference block since its last calibration due to drift;

$u_{ms}$  is the uncertainty due to the resolution of the hardness-calibration machine.

EXAMPLE

Primary hardness-reference block: 400,1 HV 30  
 Uncertainty of measurement of the primary hardness-reference block ( $k = 1$ )  $u_{\text{CRM}} = \pm 2,5$  HV  
 Time drift of the primary hardness-reference block  $u_{\text{CRM-D}} = 0$   
 Resolution of the measurement system  $\delta_{\text{ms}} = 0,1 \mu\text{m}$

Table A.1 — Results of the indirect verification

No.	Measured indentation diagonal $d$ mm	Calculated hardness value $H$ HV <sup>a</sup>
1	0,373 4 <sub>max</sub>	399,0 <sub>min</sub>
2	0,373 0	399,9
3	0,372 5 <sub>min</sub>	400,9 <sub>max</sub>
4	0,372 8	400,3
5	0,372 9	400,3
Mean value	0,372 92	400,1
Standard deviation $s_{x\text{CRM-1}}$	0,000 33	0,70
Standard uncertainty of measurement $u_{x\text{CRM-1}}$	0,000 17	0,36

<sup>a</sup> HV: Vickers hardness.

$$u_{x\text{CRM-1}} = \frac{t \cdot s_{x\text{CRM-1}}}{\sqrt{n}} = 0,36 \tag{A.2}$$

( $t = 1,14$  for  $n = 5$ )

Table A.2 — Budget of uncertainty of measurement

Quantity $X_i$	Estimated value $x_i$	Standard uncertainty of measurement $u(x_i)$	Distribution type	Sensitivity coefficient $c_i$	Uncertainty contribution $u_i (H)$
$u_{\text{CRM}}$	400,1 HV 30	2,5 HV	Normal	1,0	2,5 HV
$u_{x\text{CRM-1}}$	0 HV	0,36 HV	Normal	1,0	0,36 HV
$u_{\text{ms}}$	0 HV	0,1 $\mu\text{m} =$ 0,000 1 mm	Rectangular	2 146,0 <sup>a</sup>	0,06 HV
$u_{\text{CRM-D}}$	0 HV	0 HV	Triangular	1,0	0 HV
Combined uncertainty of measurement $u_{\text{CM}}$					2,53 HV

HV: Vickers hardness.

<sup>a</sup> The sensitivity coefficient follows from:  
 $c = \partial H / \partial d = 2(HV/d)$  (A.3)

for  $H = 400,1$  HV,  $d = 0,372 92$  mm.

### A.3 Uncertainty of measurement of hardness-reference blocks

The uncertainty of measurement of hardness-reference blocks follows from the equation:

$$u_{\text{CRM}} = \sqrt{u_{\text{CM}}^2 + u_{x\text{CRM}-2}^2} \quad (\text{A.4})$$

where

$u_{\text{CRM}}$  is the calibration uncertainty of hardness-reference blocks;

$u_{x\text{CRM}-2}$  is the standard deviation due to the inhomogeneity of the hardness distribution on the hardness-reference block;

$u_{\text{CM}}$  see Equation (A.1).

**Table A.3 — Determination of the inhomogeneity of the hardness-reference block**

No.	Measured indentation diagonal $d$ mm	Calculated hardness value $H_{\text{CRM}}$ HV <sup>a</sup>
1	0,373 6 <sub>max</sub>	398,6 <sub>min</sub>
2	0,373 1	399,6
3	0,372 3 <sub>min</sub>	401,4 <sub>max</sub>
4	0,372 5	400,9
5	0,373 1	399,6
Mean value	0,372 92	400,0
Standard deviation $s_{x\text{CRM}-2}$	0,000 52	1,12

<sup>a</sup> HV: Vickers hardness.

Standard uncertainty of CRM:

$$u_{x\text{CRM}-2} = \frac{t \cdot s_{x\text{CRM}-2}}{\sqrt{n}} \quad (\text{A.5})$$

with  $t = 1,14$  and  $n = 5$ :

$$u_{x\text{CRM}-2} = 0,58 \text{ HV}$$

**Table A.4 — Uncertainty of measurement of the hardness-reference block**

Hardness of hardness-reference block $H_{\text{CRM}}$ HV <sup>a</sup>	Inhomogeneity of the hardness-reference block $u_{x\text{CRM}-2}$ HV	Uncertainty of measurement of primary hardness-calibration machine $u_{\text{CM}}$ HV	Expanded calibration uncertainty of hardness-reference block $U_{\text{CRM}}$ HV
400,1	0,57	2,53	5,18

<sup>a</sup> HV: Vickers hardness.

with

$$U_{\text{CRM}} = 2\sqrt{u_{\text{CM}}^2 + u_{x\text{CRM}-2}^2} \quad (\text{A.6})$$



## Bibliography

- [1] SAWLA, A. *Uncertainty of measurement in the verification and calibration of the force measuring systems of testing machines*, Proceedings of the Asia-Pacific symposium on measurement of force, mass and torque (APMF), Tsukuba, Japan, November 2000
- [2] WEHRSTEDT, A., PATKOVSKY, I. *News in the field of standardization about verification and calibration of materials testing machines*, May 2001, EMPA Academy 2001
- [3] GABAUER, W. *Manual codes of practice for the determination of uncertainties in mechanical tests on metallic materials, The estimation of uncertainties in hardness measurements*, Project No. SMT4-CT97-2165, UNCERT COP 14:2000
- [4] POLZIN, T., SCHWENK, D. Method for Uncertainty Determination of Hardness Testing; PC File for Determination, *Materialprüfung* **44** (2002) 3, pp. 64-71

---

---

## **BSI — British Standards Institution**

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

### **Revisions**

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover.  
Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

### **Buying standards**

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001.  
Fax: +44 (0)20 8996 7001. Email: [orders@bsi-global.com](mailto:orders@bsi-global.com). Standards are also available from the BSI website at <http://www.bsi-global.com>.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

### **Information on standards**

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre.  
Tel: +44 (0)20 8996 7111. Fax: +44 (0)20 8996 7048. Email: [info@bsi-global.com](mailto:info@bsi-global.com).

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.  
Tel: +44 (0)20 8996 7002. Fax: +44 (0)20 8996 7001.  
Email: [membership@bsi-global.com](mailto:membership@bsi-global.com).

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsi-global.com/bsonline>.

Further information about BSI is available on the BSI website at <http://www.bsi-global.com>.

### **Copyright**

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright & Licensing Manager.  
Tel: +44 (0)20 8996 7070. Fax: +44 (0)20 8996 7553.  
Email: [copyright@bsi-global.com](mailto:copyright@bsi-global.com).