

BS EN ISO 6508-2:2015



BSI Standards Publication

Metallic materials — Rockwell hardness test

Part 2: Verification and calibration of testing machines and indenters

bsi.

...making excellence a habit.™

National foreword

This British Standard is the UK implementation of EN ISO 6508-2:2015. It supersedes BS EN ISO 6508-2:2005 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee ISE/101/5, Indentation hardness testing.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2015.
Published by BSI Standards Limited 2015

ISBN 978 0 580 79169 7

ICS 77.040.10

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 March 2015.

Amendments/corrigenda issued since publication

Date	Text affected
------	---------------

English Version

Metallic materials - Rockwell hardness test - Part 2: Verification and calibration of testing machines and indenters (ISO 6508-2:2015)

Matériaux métalliques - Essai de dureté Rockwell - Partie 2: Vérification et étalonnage des machines d'essai et des pénétrateurs (ISO 6508-2:2015)

Metallische Werkstoffe - Härteprüfung nach Rockwell - Teil 2: Überprüfung und Kalibrierung der Prüfmaschinen und Eindringkörper (ISO 6508-2:2015)

This European Standard was approved by CEN on 10 January 2015.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

CEN-CENELEC Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

This document (EN ISO 6508-2:2015) has been prepared by Technical Committee ISO/TC 164 "Mechanical testing of metals" in collaboration with Technical Committee ECISS/TC 101 "Test methods for steel (other than chemical analysis)" the secretariat of which is held by AFNOR.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by September 2015, and conflicting national standards shall be withdrawn at the latest by September 2015.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN ISO 6508-2:2005.

According to the CEN-CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

Endorsement notice

The text of ISO 6508-2:2015 has been approved by CEN as EN ISO 6508-2:2015 without any modification.

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 General conditions	1
4 Direct verification of the testing machine	2
4.1 General.....	2
4.2 Calibration and verification of the test force.....	2
4.3 Calibration and verification of the depth-measuring system.....	2
4.4 Calibration and verification of the testing cycle.....	3
4.5 Calibration and verification of the machine hysteresis.....	3
5 Indirect verification of the testing machine	4
5.1 General.....	4
5.2 Procedure.....	4
5.3 Repeatability.....	5
5.4 Bias.....	6
5.5 Uncertainty of measurement.....	7
6 Calibration and verification of Rockwell hardness indenters	7
6.1 General.....	7
6.2 Diamond indenter.....	7
6.2.1 General.....	7
6.2.2 Direct calibration and verification of the diamond indenter.....	7
6.2.3 Indirect verification of diamond indenters.....	8
6.3 Ball indenter.....	9
6.3.1 Direct calibration and verification of the ball indenter.....	9
6.3.2 Indirect verification of the ball holder assembly.....	11
6.4 Marking.....	11
7 Intervals between direct and indirect calibrations and verifications	11
8 Verification report	12
Annex A (normative) Repeatability of testing machines	13
Annex B (informative) Uncertainty of measurement of the calibration results of the hardness testing machine	15
Bibliography	24

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO ISO/TC 164, *Mechanical testing of metals*, Subcommittee SC 3, *Hardness testing*.

This third edition cancels and replaces the first edition (ISO 6508-2:2005), which has been technically revised.

ISO 6508 consists of the following parts, under the general title *Metallic materials — Rockwell hardness test*:

- *Part 1: Test method*
- *Part 2: Verification and calibration of testing machines and Indenters*
- *Part 3: Calibration of reference blocks*

Metallic materials — Rockwell hardness test —

Part 2:

Verification and calibration of testing machines and indenters

1 Scope

This part of ISO 6508 specifies two separate methods of verification of testing machines (direct and indirect) for determining Rockwell hardness in accordance with ISO 6508-1:2015, together with a method for verifying Rockwell hardness indenters.

The direct verification method is used to determine whether the main parameters associated with the machine function, such as applied force, depth measurement, and testing cycle timing, fall within specified tolerances. The indirect verification method uses a number of calibrated reference hardness blocks to determine how well the machine can measure a material of known hardness.

The indirect method may be used on its own for periodic routine checking of the machine in service.

If a testing machine is also to be used for other methods of hardness testing, it shall be verified independently for each method.

This part of ISO 6508 is applicable to stationary and portable hardness testing machines.

Attention is drawn to the fact that the use of tungsten carbide composite for ball indenters is considered to be the standard type of Rockwell indenter ball. Steel indenter balls may continue to be used only when complying with ISO 6508-1:2015, Annex A.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 376, *Metallic materials — Calibration of force-proving instruments used for the verification of uniaxial testing machines*

ISO 6507-1, *Metallic materials — Vickers hardness test — Part 1: Test method*

ISO 6508-1:2015, *Metallic materials — Rockwell hardness test — Part 1: Test method*

ISO 6508-3:2015, *Metallic materials — Rockwell hardness test — Part 3: Calibration of reference blocks*

3 General conditions

Before a Rockwell hardness testing machine is verified, the machine shall be checked to ensure that it is properly set up and operating in accordance with the manufacturer's instructions.

Especially, it should be checked that the test force can be applied and removed without shock, vibration, or overload and in such a manner that the readings are not influenced.

4 Direct verification of the testing machine

4.1 General

4.1.1 Direct verification involves calibration and verification of the following:

- a) test forces;
- b) depth-measuring system;
- c) testing cycle;
- d) machine hysteresis test.

4.1.2 Direct verification should be carried out at a temperature of (23 ± 5) °C. If the verification is made outside of this temperature range, this shall be reported in the verification report.

4.1.3 The instruments used for calibration shall be traceable to national standards.

4.1.4 An indirect verification according to [Clause 5](#) shall be performed following a successful direct verification.

4.2 Calibration and verification of the test force

4.2.1 Each preliminary test force, F_0 , (see [4.2.4](#)) and each total test force, F , used (see [4.2.5](#)) shall be measured, and, whenever applicable, this shall be done at not less than three positions of the plunger spaced throughout its range of movement during testing. The preliminary test force shall be held for at least 2 s.

4.2.2 Three readings shall be taken for each force at each position of the plunger. Immediately before each reading is taken, the plunger shall be moved in the same direction as during testing.

4.2.3 The forces shall be measured by one of the following two methods:

- by means of a force-proving device according to ISO 376 class 1 or better and calibrated for reversibility;
- by balancing against a force, accurate to $\pm 0,2$ %, applied by means of calibrated masses or by another method having the same accuracy.

Evidence should be available to demonstrate that the output of the force-proving device does not vary by more than 0,2 % in the period 1 s to 30 s following a stepped change in force.

4.2.4 The tolerance on each measurement of the preliminary test force, F_0 , (before application and after removal of the additional test force, F_1) shall be $\pm 2,0$ %, see Formula (B.2) The range of all force measurements (highest value minus lowest value) shall be $\leq 1,5$ % of F_0 .

4.2.5 The tolerance on each measurement of the total test force, F , shall be $\pm 1,0$ %. The range of the force measurements (highest value minus lowest value) shall be $\leq 0,75$ % of F .

4.3 Calibration and verification of the depth-measuring system

4.3.1 The depth-measuring system shall be calibrated by making known incremental movements of the indenter or the indenter holder.

4.3.2 The instrument or gauge blocks used to verify the depth-measuring system shall have a maximum expanded uncertainty of 0,000 3 mm when calculated with a 95 % confidence level.

4.3.3 Calibrate the testing machine's depth measurement system at not less than four evenly spaced increments covering the full range of the normal working depth measured by the testing machine. For this purpose, the working depth is 0,25 mm for regular Rockwell scales (A, C, D, B, E, F, G, H, K), and 0,1 mm for superficial Rockwell scales (N, T).

4.3.4 Some testing machines have a long-stroke depth measuring system where the location of the working range of the depth measuring system varies to suit the sample. This type of testing machine shall be able to electronically verify that the depth measuring device is continuous over the full range. These types of testers shall be verified using the following steps:

- a) At the approximate top, midpoint, and bottom of the total stroke of the measuring device, verify the depth measurement system at no less than four evenly spaced increments of approximately 0,05 mm at each of the three locations.
- b) Operate the actuator over its full range of travel to monitor whether the displacement measurement is continuous. The displacement indication shall be continuously indicated over the full range.

4.3.5 The depth-measuring system shall correctly indicate within $\pm 0,001$ mm for the scales A to K and within $\pm 0,000 5$ mm for scales N and T, i.e. within $\pm 0,5$ of a scale unit, over each range.

4.4 Calibration and verification of the testing cycle

4.4.1 The testing cycle is to be calibrated by the testing machine manufacturer at the time of manufacture and when the testing machine undergoes repair which may have affected the testing cycle. Calibration of the complete testing cycle is not required as part of the direct verification at other times, see [Table 10](#).

4.4.2 The testing cycle shall conform to the testing cycle defined in ISO 6508-1:2015.

4.4.3 For testing machines that automatically control the testing cycle, the measurement uncertainty ($k = 2$) of the timing instrument used to verify the testing cycle shall not exceed 0,2 s. It is recommended that the measured times for the testing cycle, plus or minus the measurement uncertainty ($k = 2$) of the calibration measurements, not exceed the timing limits specified in ISO 6508-1:2015.

4.4.4 For testing machines that require the user to manually control the testing cycle, the testing machine shall be verified to be capable of achieving the defined testing cycle.

4.5 Calibration and verification of the machine hysteresis

4.5.1 The machine shall be checked to ensure that the readings are not affected by a hysteretic flexure of testing machine components (e.g. frame, specimen holder, etc.) during a test. The influence of any hysteresis behaviour shall be checked by making repeated hardness tests using a spherical indenter of at least 10 mm diameter, bearing directly against the specimen holder or through a spacer such that no permanent deformation occurs. A parallel block placed between the indenter holder and the specimen holder may be used instead of a blunt indenter. The material of the blunt indenter and of the spacer or parallel block shall have a hardness of at least 60 HRC.

4.5.2 Perform repeated Rockwell tests using the setup defined in [4.5.1](#). The tests shall be conducted using the Rockwell scale with the highest test force that is used during normal testing. Repeat the hysteresis verification procedure for a maximum of 10 measurements and average the last three tests.

4.5.3 The average of the last three tests shall indicate a hardness number of $(130 \pm 1,0)$ Rockwell units when the regular Rockwell ball scales B, E, F, G, H, and K are used, or within $(100 \pm 1,0)$ Rockwell units when any other Rockwell scale is used.

5 Indirect verification of the testing machine

5.1 General

5.1.1 Indirect verification involves the calibration and verification of the testing machine by performing tests on reference blocks.

5.1.2 Indirect verification should be carried out at a temperature of (23 ± 5) °C by means of reference blocks calibrated in accordance with ISO 6508-3:2015. If the verification is made outside of this temperature range, this shall be reported in the verification report.

5.2 Procedure

5.2.1 For the indirect verification of a testing machine, the following procedures shall be applied.

The testing machine shall be verified for each scale for which it will be used. For each scale to be verified, reference blocks from each of the hardness ranges given in [Table 1](#) shall be used. The hardness values of the blocks shall be chosen to approximate the limits of the intended use. It is recommended to perform the same test cycle used when the reference blocks were calibrated.

Only the calibrated surfaces of the test blocks are to be used for testing.

5.2.2 On each reference block, a minimum of five indentations, made in accordance with ISO 6508-1:2015, shall be uniformly distributed over the test surface and each hardness number observed to within 0,2 HR of a scale unit. Before making these indentations, at least two preliminary indentations shall be made to ensure that the machine is working freely and that the reference block, the indenter, and the specimen holder are seating correctly. The results of these preliminary indentations shall be ignored.

Table 1 — Hardness ranges for different scales

Rockwell hardness scale	Hardness range of reference block	Rockwell hardness scale	Hardness range of reference block
A	20 to 40 HRA 45 to 75 HRA 80 to 95 HRA	K	40 to 60 HRKW 65 to 80 HRKW 85 to 100 HRKW
B	10 to 50 HRBW 60 to 80 HRBW 85 to 100 HRBW	15N	70 to 77 HR15N 78 to 88 HR15N 89 to 94 HR15N
C	10 to 30 HRC 35 to 55 HRC 60 to 70 HRC	30N	42 to 54 HR30N 55 to 73 HR30N 74 to 86 HR30N
D	40 to 47 HRD 55 to 63 HRD 70 to 77 HRD	45N	20 to 31 HR45N 32 to 61 HR45N 63 to 77 HR45N

Rockwell hardness scale	Hardness range of reference block	Rockwell hardness scale	Hardness range of reference block
E	70 to 77 HREW 84 to 90 HREW 93 to 100 HREW	15T	67 to 80 HR15TW 81 to 87 HR15TW 88 to 93 HR15TW
F	60 to 75 HRFW 80 to 90 HRFW 94 to 100 HRFW	30T	29 to 56 HR30TW 57 to 69 HR30TW 70 to 82 HR30TW
G	30 to 50 HRGW 55 to 75 HRGW 80 to 94 HRGW	45T	10 to 33 HR45TW 34 to 54 HR45TW 55 to 72 HR45TW
H	80 to 94 HRHW 96 to 100 HRHW		

5.3 Repeatability

5.3.1 For each reference block, let $H_1, H_2, H_3, H_4, \dots, H_n$ be the values of the measured hardness arranged in increasing order of magnitude.

The repeatability range, r , of the testing machine in Rockwell units, under the particular verification conditions, is determined by Formula (1):

$$r = H_n - H_1 \quad (1)$$

The mean hardness value of all indentations \bar{H} is defined according to Formula (2):

$$\bar{H} = \frac{H_1 + H_2 + H_3 + H_4 + \dots + H_n}{n} \quad (2)$$

where

$H_1, H_2, H_3, H_4, \dots, H_n$ are the hardness values corresponding to all the indentations;

n is the total number of indentations.

5.3.2 The repeatability range of the testing machine being verified shall be considered satisfactory if it satisfies the conditions given in [Table 2](#). Permissible repeatability is presented graphically in [Figures A.1](#) and [A.2](#).

Table 2 — Permissible repeatability range and bias of the testing machine

Rockwell hardness scale	Hardness range of the reference block	Permissible bias Rockwell units b	Permissible repeatability range of the testing machine ^a r
A	20 to 75 HRA > 75 to 95 HRA	± 2 HRA $\pm 1,5$ HRA	$\leq 0,02 (100 - \bar{H})$ or 0,8 HRA Rockwell units ^b

^a \bar{H} is the mean hardness value.

^b The one with a greater value becomes the permissible repeatability range of the testing machine.

NOTE The requirements for permissible repeatability range, r , and/or permissible bias, b , might be different in ASTM E 18.

Rockwell hardness scale	Hardness range of the reference block	Permissible bias Rockwell units <i>b</i>	Permissible repeatability range of the testing machine ^a <i>r</i>
B	10 to 45 HRBW > 45 to 80 HRBW > 80 to 100 HRBW	±4 HRBW ±3 HRBW ±2 HRBW	≤ 0,04 (130 - \bar{H}) HRBW Rockwell units
C	10 to 70 HRC	±1,5 HRC	≤ 0,02 (100 - \bar{H}) or 0,8 HRC Rockwell units ^b
D	40 to 70 HRD > 70 to 77 HRD	±2 HRD ±1,5 HRD	≤ 0,02 (100 - \bar{H}) or 0,8 HRD Rockwell units ^b
E	70 to 90 HREW > 90 to 100 HREW	±2,5 HREW ±2 HREW	≤ 0,04 (130 - \bar{H}) HREW Rockwell units
F	60 to 90 HRFW > 90 to 100 HRFW	±3 HRFW ±2 HRFW	≤ 0,04 (130 - \bar{H}) HRFW Rockwell units
G	30 to 50 HRGW > 50 to 75 HRGW > 75 to 94 HRGW	±6 HRGW ±4,5 HRGW ±3 HRGW	≤ 0,04 (130 - \bar{H}) HRGW Rockwell units
H	80 to 100 HRHW	±2 HRHW	≤ 0,04 (130 - \bar{H}) HRHW Rockwell units
K	40 to 60 HRKW > 60 to 80 HRKW > 80 to 100 HRKW	±4 HRKW ±3 HRKW ±2 HRKW	≤ 0,04 (130 - \bar{H}) HRKW Rockwell units
15N, 30N, 45N	All ranges	±2 HR-N	≤ 0,04 (100 - \bar{H}) or 1,2 HR-N Rockwell units ^b
15T, 30T, 45T	All ranges	±3 HR-TW	≤ 0,06 (100 - \bar{H}) or 2,4 HR-TW Rockwell units ^b

^a \bar{H} is the mean hardness value.

^b The one with a greater value becomes the permissible repeatability range of the testing machine.

NOTE The requirements for permissible repeatability range, *r*, and/or permissible bias, *b*, might be different in ASTM E 18.

5.4 Bias

5.4.1 The bias, *b*, of the testing machine in Rockwell units, under the particular calibration conditions, is expressed by the following formula:

$$b = \bar{H} - H_{\text{CRM}} \quad (3)$$

where

\bar{H} is the mean hardness value, from Formula (2);

H_{CRM} is the certified hardness of the reference block used.

5.4.2 The bias of the testing machine shall not exceed the values given in [Table 2](#).

5.5 Uncertainty of measurement

A method to determine the uncertainty of measurement of the calibration results of the hardness testing machines is given in [Annex B](#).

6 Calibration and verification of Rockwell hardness indenters

6.1 General

6.1.1 Indenter calibrations and verifications should be carried out at a temperature of (23 ± 5) °C. If the verification is made outside of this temperature range, this shall be reported in the verification report.

6.1.2 The instruments used for calibration and verifications shall be traceable to national standards.

6.2 Diamond indenter

6.2.1 General

To verify the reliable performance of the spheroconical diamond indenter in conformance with this part of ISO 6508, a direct and an indirect calibration and verification shall be carried out on each indenter.

6.2.2 Direct calibration and verification of the diamond indenter

6.2.2.1 The surfaces of the diamond cone and spherical tip shall be polished for a penetration depth of 0,3 mm and shall blend in a smooth tangential manner. Both surfaces shall be free from surface defects.

6.2.2.2 The verification of the shape of the indenter can be made by direct measurement or optically. The verification shall be made at not less than four unique equally spaced axial planes (for example, at 0°, 45°, 90°, 135°). Measurement with a collimator device is also acceptable. In this case, the measurements should be carried out at least in four central angles and the central angle of 120° shall be included.

The location where the spherical tip and the cone of the diamond blend together will vary depending on the values of the tip radius and cone angle. Ideally for a perfect indenter geometry, the blend point is located at 100 µm from the indenter axis measured along a line normal to the indenter axis. To avoid including the blend area in the measurement of the tip radius and cone angle, the portion of the diamond surface between 80 µm and 120 µm may be ignored.

6.2.2.3 The instruments used to verify the shape of the diamond indenter shall have the following maximum expanded uncertainty when calculated with a 95 % confidence level:

- angle: 0,1°;
- radius: 0,005 mm.

6.2.2.4 The diamond cone shall have an included angle of $(120 \pm 0,35)$ °.

6.2.2.5 The tip of the indenter shall be spherical. Its mean radius shall be determined from at least four single values, measured in the axial section planes defined in [6.2.2.2](#). Each single value shall be within

(0,2 ± 0,015) mm. The mean value shall be within (0,2 ± 0,01) mm. Local deviations from a true radius shall not exceed 0,002 mm.

6.2.3 Indirect verification of diamond indenters

6.2.3.1 The hardness values given by the testing machine depend not only on the dimensions of the tip radius and cone angle, but also on the surface roughness and the position of the crystallographic axes of the diamond, and the seating of the diamond in its holder. To examine these influences, an indirect verification of the performance of the diamond indenter shall be accomplished by making a series of tests on reference blocks that meet the requirements of ISO 6508-3:2015 and comparing the results against a calibration diamond indenter that meets the requirements of ISO 6508-3:2015, 4.3.

This indirect verification shall be performed using a calibration machine that meets the relevant paragraphs of ISO 6508-3:2015, Clause 4, in accordance with the procedure described in ISO 6508-3:2015, Clause 5.

Diamond indenters may be certified for use for either

- only the regular Rockwell diamond scales, or
- only the superficial Rockwell diamond scales, or
- both the regular and superficial Rockwell diamond scales, or
- any singular or limited combination of diamond scales.

NOTE It might be necessary to use a diamond indenter on a reduced number of test scales due to force limitations, such as a side cut diamond indenter for testing gear tooth profiles, or other considerations.

6.2.3.2 The reference blocks used for this indirect verification shall be chosen at the hardness levels given in [Tables 3, 4, 5, 6, or 7](#) depending on the scales for which the indenter is to be certified. When verifying diamond indenters to be used on a limited number of scales, use the reference blocks defined in [Table 5](#) for the HRC scale and/or the appropriate scale row(s) in [Table 7](#) for any other diamond scale.

NOTE The alternate hardness levels given in [Table 4](#) are provided to accommodate indenters calibrated to other International Standards. It is believed that calibrations conducted to [Table 3](#) or [Table 4](#) will yield equivalent results.

Table 3 — Hardness levels for diamond indenters used for Rockwell regular and superficial scales (A, C, D, and N)

Scale	Nominal hardness	Ranges
HRC	23	20 to 26
HRC	55	52 to 58
HR45N	43	40 to 46
HR15N	91	88 to 94

Table 4 — Alternate hardness levels for diamond indenters used for Rockwell regular and superficial scales (A, C, D, and N)

Scale	Nominal hardness	Ranges
HRC	25	22 to 28
HRC	63	60 to 65
HR30N	64	60 to 69
HR15N	91	88 to 94

Table 5 — Hardness levels for diamond indenters to be used for Rockwell regular scale testing only (A, C, and D)

Scale	Nominal hardness	Ranges
HRC	25	22 to 28
HRC	63	60 to 65

Table 6 — Hardness levels for diamond indenters to be used for Rockwell superficial scale testing only (N)

Scale	Nominal hardness	Ranges
HR15N	91	88 to 94
HR30N	64	60 to 69
HR45N	25	22 to 29

Table 7 — Hardness levels for diamond indenters to be used for limited scale testing

Scale	High nominal hardness	High hardness range	Low nominal hardness	Low hardness range
HRA	83	81 to 84	63	61 to 65
HRD	73	70 to 75	44	41 to 46
HR15N	91	88 to 94	72	70 to 74
HR30N	80	77 to 82	46	43 to 49
HR45N	70	66 to 72	25	22 to 29

6.2.3.3 The testing shall be carried out in accordance with ISO 6508-1:2015 using the following procedure.

For each block, the mean hardness value of three indentations made using the indenter to be verified shall not differ from the mean hardness value of three indentations obtained with the calibration indenter by more than $\pm 0,8$ Rockwell units. The indentations made with the indenter to be verified and with the calibration indenter should be adjacent to each other on each block.

6.3 Ball indenter

Ball indenters normally consist of a spherical ball and a separate appropriately designed holder. Single-piece spherically tipped indenters are allowed, provided the surface of the indenter that makes contact with the test piece meets the size, shape, finish, and hardness requirements defined in [6.3.1](#), and it meets the performance requirements defined in [6.3.2](#)

6.3.1 Direct calibration and verification of the ball indenter

6.3.1.1 The balls shall be polished and free from surface defects.

6.3.1.2 The user shall either measure the balls to ensure that they meet the following requirements, or shall obtain balls from a supplier certifying that the following conditions are met. For the purpose of verifying the size, density, and the hardness of the balls, at least one ball selected at random from a batch shall be tested. The balls verified for hardness shall be discarded.

6.3.1.3 The diameter, measured at no less than three positions, shall not differ from the nominal diameter by more than the tolerance given in [Table 8](#).

Table 8 — Tolerances for the different ball diameters

Rockwell hardness scale	Ball diameter mm	Tolerance mm
B	1,587 5	±0,003 5
F	1,587 5	±0,003 5
G	1,587 5	±0,003 5
T	1,587 5	±0,003 5
E	3,175	±0,004
H	3,175	±0,004
K	3,175	±0,004

6.3.1.4 The characteristics of the tungsten carbide composite balls shall be as follows:

- Hardness: The hardness shall be no less than 1 500 HV, when determined using a test force of at least 4,903 N (HV 0,5) in accordance with ISO 6507-1. The ball may be tested directly on this spherical surface or by sectioning the ball and testing on the ball interior. An example for HV 10 is given in [Table 9](#).
- Density: $\rho = (14,8 \pm 0,2) \text{ g/cm}^3$.

The following chemical composition is recommended:

- tungsten carbide (WC): balance;
- total other carbides: 2,0 %;
- cobalt (Co): 5,0 % to 7,0 %.

6.3.1.5 The hardness of steel balls shall be no less than 750 HV, when determined using a test force of 98,07 N in accordance with ISO 6507-1 (see [Table 9](#)).

NOTE Hardened steel balls are only used when performing tests on thin sheet metal according to ISO 6508-1:2015, Annex A.

Table 9 — Values of the mean diagonal (HV10) for the determination of the hardness of the ball indenters

Ball diameter mm	Maximum value of the mean diagonal made on the spherical surface of the ball with a Vickers indenter at 98,07 N (HV10) mm	
	Hardened steel ball	Tungsten carbide composite ball
3,175		0,109
1,587 5	0,150	0,107

6.3.2 Indirect verification of the ball holder assembly

6.3.2.1 The B, E, F, G, H, K, T scale hardness values given by the testing machine depends not only on the dimensions of the ball indenter, but also on the seating and alignment of the ball in its holder. To examine these influences, an indirect verification of the performance of the ball indenter assembly shall be done by making a series of tests on a reference block that meets the requirements of ISO 6508-3:2015, using a tester that meets the requirements of this part of ISO 6508, following the procedures defined in ISO 6508-1:2015.

6.3.2.2 Perform at least three tests on at least one HRBW scale (or the scale with the highest test force that the indenter is going to be used to perform) test block.

6.3.2.3 The mean hardness value of three indentations made using the ball holder assembly to be verified shall not differ from the certified hardness value of the test block by more than the permissible bias defined in [Table 2](#).

6.4 Marking

6.4.1 All diamond indenters and ball holder assemblies shall be serialized. When it is not practical to mark the serial number on the indenter due to size limitations, the serial number shall be marked on the container.

6.4.2 Diamond indenters with limited range of use shall be appropriately marked. For example, diamond indenters certified for use on the superficial N scale only may be marked with an N and diamonds certified for use on the regular A, C, and D scales only may be marked with a C.

7 Intervals between direct and indirect calibrations and verifications

7.1 The schedules for the direct verification of Rockwell hardness testing machines are given in [Table 10](#).

7.2 Indirect verification shall be performed at least once every 12 months and after a direct verification has been performed. For high-use machines, a smaller interval might be appropriate.

7.3 If an indirect verification has not been performed within 13 months, a direct verification shall be performed before the tester can be used (see [Table 10](#)).

Table 10 — Direct verifications of hardness testing machines

Requirements of verification	Force	Measuring system	Test cycle	Machine hysteresis	Indenter ^a
before setting to work first time	x	x	x	x	x
after dismantling and reassembling, if force, measuring system or test cycle are affected	x	x	x	x	
failure of indirect verification ^b	x	x	(x) ^c	x	
indirect verification > 13 months ago	x	x	(x) ^c	x	

^a In addition, it is recommended that the diamond indenter be directly verified after two years of use.

^b Direct verification of these parameters may be carried out sequentially (until the machine passes indirect verification) and is not required if it can be demonstrated (e.g. by tests with a reference indenter) that the indenter was the cause of the failure.

^c At minimum, verify the duration of the total test forces.

8 Verification report


A verification report is required for the direct and indirect verifications of testing machines and indenters. The verification report certificate shall at minimum include the following information:

- a) a reference to this part of ISO 6508, i.e. ISO 6508-2;
- b) method of verification (direct and/or indirect);
- c) identification data for the hardness testing machine, or indenter/ball holder;
- d) means of verification (reference blocks, elastic proving devices, etc.);
- e) Rockwell hardness scale(s) verified;
- f) diamond scale indenter reports shall indicate the scale(s) the indenter is certified to perform;
- g) verification temperature, if the verification was carried out outside of $(23 \pm 5) ^\circ\text{C}$;
- h) result obtained;
- i) date of verification and reference to the verification institution;
- j) uncertainty of the verification result. Examples are indicated in [Annex B](#).

Annex A (normative)

Repeatability of testing machines


The permissible repeatability of testing machines is presented graphically in [Figures A.1](#) and [A.2](#).

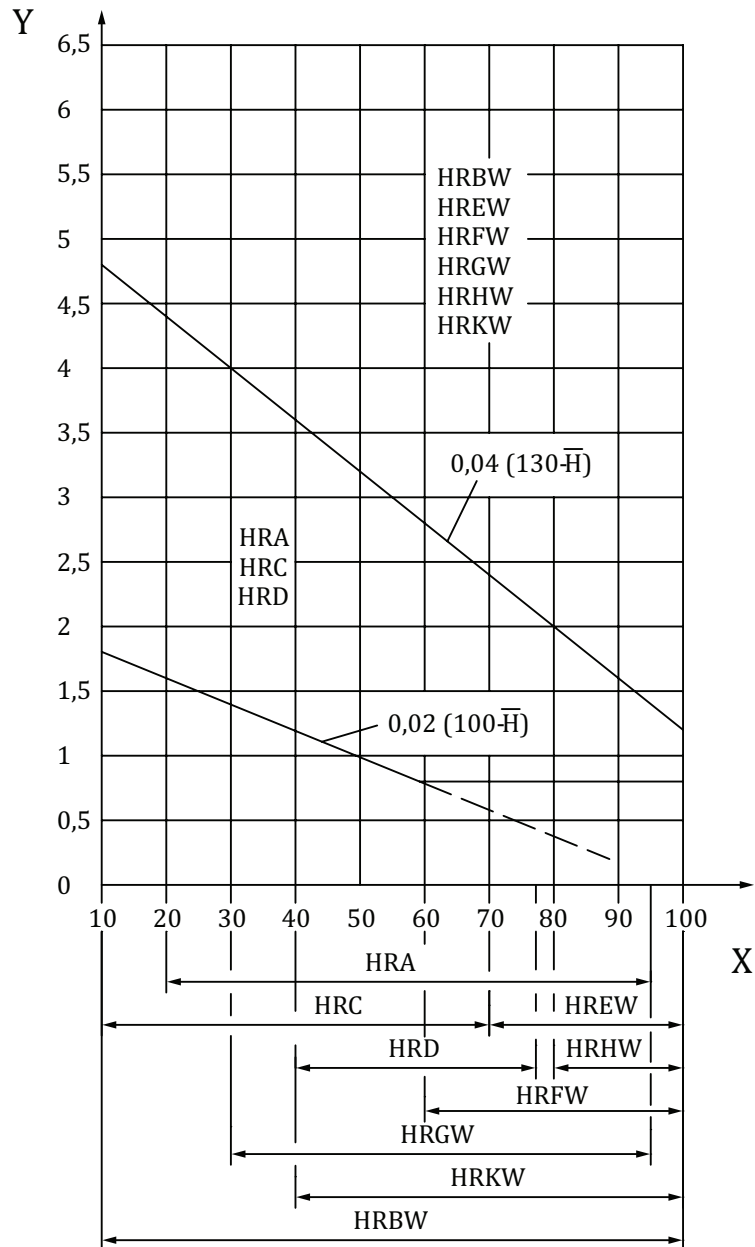

Key

- X Rockwell hardness
- Y repeatability of testing machines

Figure A.1 — Rockwell hardness (scales A, B, C, D, E, F, G, H, and K)

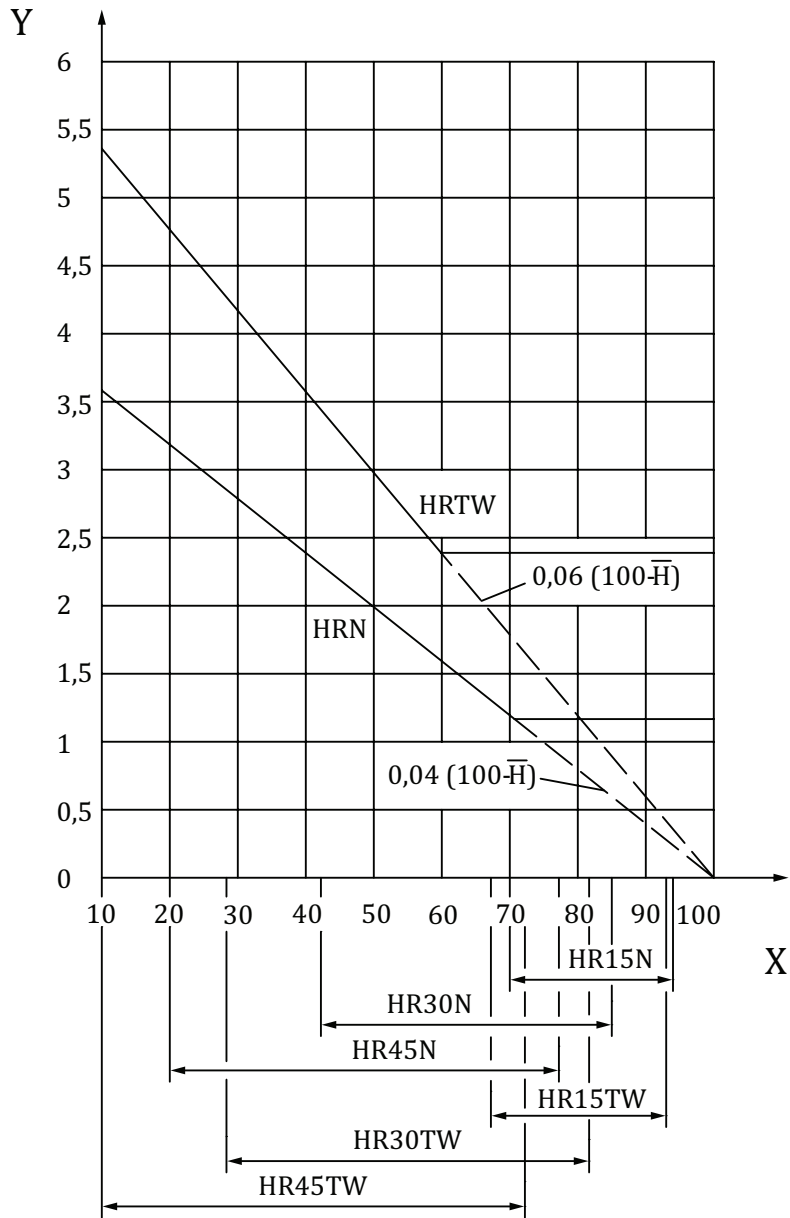

Key

- X Rockwell hardness
- Y repeatability of testing machines

Figure A.2 — Rockwell superficial hardness (scales N and T)

Annex B (informative)

Uncertainty of measurement of the calibration results of the hardness testing machine

B.1 General

Measurement uncertainty analysis is a useful tool to help determine sources of error and to understand differences between measured values. This annex gives guidance on uncertainty estimation, but the methods contained are for information only, unless specifically instructed otherwise by the customer. The criteria specified in this part of ISO 6508 for the performance of the testing machine have been developed and refined over a significant period of time. When determining a specific tolerance that the machine needs to meet, the uncertainty associated with the use of measuring equipment and/or reference standards has been incorporated within this tolerance and it would therefore be inappropriate to make any further allowance for this uncertainty by, for example, reducing the tolerance by the measurement uncertainty. This applies to all measurements made when performing a direct or indirect verification of the machine. In each case, it is simply the measured value resulting from the use of the specified measuring equipment and/or reference standards that is used to assess whether or not the machine complies with this part of ISO 6508. However, there can be special circumstances where reducing the tolerance by the measurement uncertainty is appropriate. This should only be done by agreement of the parties involved.

B.2 Direct verification — Uncertainty of calibration of machine components

B.2.1 Uncertainty of calibration of the test force

For the direct calibration of force, the difference ΔF between each individual measurement of force applied by the hardness machine and the corresponding force value indicated by the reference instrument is calculated and reported. The direct verification verifies whether each ΔF is within the specified maximum permissible limits. Consequently, the following is a procedure to calculate the uncertainties of the ΔF values with respect to the true value of force specified by the test. The combined relative standard uncertainty of the test force calibration is calculated according to Formula (B.1):

$$u_F = \sqrt{u_{FRS}^2 + u_{FHTM}^2 + u_{ms}^2} \quad (\text{B.1})$$

where

- u_{FRS} is the relative uncertainty of measurement of the force transducer (from calibration certificate);
- u_{FHTM} is the relative standard uncertainty of the test force generated by the hardness testing machine;
- u_{ms} is the relative uncertainty of measurement due to the resolution of the measuring system.

The uncertainty of measurement of the reference instrument, force transducer, is indicated in the corresponding calibration certificate. Influence quantities like the following should be considered for critical applications:

- temperature dependence;

- long-term stability;
- interpolation deviation.

Depending on the design of the force transducer, the rotational position of the transducer related to the indenter axis of the hardness testing machine should be considered.

NOTE The metrological chain necessary to define and disseminate hardness scales is shown in ISO 6508-1:2015, Figure I.1.

EXAMPLE Direct verification of the applied force of the testing machine.

Calibration value of the force transducer (force to be measured): $F_{RS} = 1\,471,0\text{ N}$

Expanded uncertainty of measurement of the force transducer: $U_{FRS} = 0,12\% (k = 2)$ (from calibration certificate)

Resolution of the force indicating instrument: $\delta_{ms} = 0,1\text{ N}$

$$\Delta F_{rel} = 100 \times \frac{F - F_{RS}}{F_{RS}} \quad (\text{B.2})$$

$$u_{FRS} = \frac{U_{FRS}}{2} \quad (\text{B.3})$$

$$u_{FHTM} = 100 \times \frac{s_{F,i}}{\bar{F}} \times t \quad (\text{B.4})$$

where $s_{F,i}$ is the standard deviation of the test-force indication values in the i -th height position.

$$u_{ms} = 100 \times \frac{\delta_{ms}}{2\sqrt{3}} \times \frac{1}{F_{RS}} \quad (\text{B.5})$$

Table B.1 — Results of the test force calibration

Number of height position for test force calibration	Force indication 1	Force indication 2	Force indication 3	Mean value \bar{F}	Standard deviation $s_{F,i}$
	F_1	F_2	F_3		
	N	N	N		
1	1 471,5	1 471,9	1 471,7	1 471,7	0,200
2	1 472,1	1 472,3	1 472,7	1 472,4	0,306
3	1 472,2	1 473,5	1 471,3	1 472,3	1,106

The following example calculations will use values of the force indication 1 at the height position 3 from [Table B.1](#). See [Table B.2](#).

From the given direct verification parameters and [Table B.1](#):

$$\Delta F_{rel} = 100 \times \frac{1472,2 - 1471,0}{1471,0} = 0,08\% \quad (\text{for force indication 1 at the height position 3})$$

$$u_{FRS} = \frac{U_{FRS}}{2} = 0,06\%$$

$$u_{FHTM} = 100 \times \frac{s_{F,i}}{\bar{F}} \times t = 100 \times \frac{1,106}{1472,3} \times 1,32 = 9,9 \times 10^{-2}\% \quad (\text{for three readings, } t = 1,32)$$

$$u_{\text{ms}} = 100 \times \frac{\delta_{\text{ms}}}{2\sqrt{3}} \times \frac{1}{F} = 100 \times \frac{0,1}{2\sqrt{3}} \times \frac{1}{1471,0} = 2,0 \times 10^{-3} \%$$

**Table B.2 — Calculation of the uncertainty of measurement of the test force
(for force indication 1 at the height position 3 from [Table B.1](#))**

Quantity	Estimated value	Relative limit values	Distribution type	Relative standard measurement uncertainty	Sensitivity coefficient	Relative standard measurement uncertainty symbol	Relative uncertainty contribution
X_i	x_i	a_i		$u(x_i)$	c_i		u_i
Force transducer indication	1 471,0 N		Normal	$6,0 \times 10^{-2} \%$	1	u_{FRS}	$6,0 \times 10^{-2} \%$
Generated test force	1 471,0 N	1,0 %	Normal	$9,9 \times 10^{-2} \%$	1	u_{FHTM}	$9,9 \times 10^{-2} \%$
Measurement system resolution			Rectangular	$2,0 \times 10^{-3} \%$	1	u_{ms}	$2,0 \times 10^{-3} \%$
Relative combined standard uncertainty, u_{F}							$1,2 \times 10^{-1} \%$
Relative expanded uncertainty of measurement, U_{F} ($k = 2$)							$2,3 \times 10^{-1} \%$

The above calculations must be done for all force measurements.

[Table B.3](#) shows the relative deviation of one test force measurement (1 471 N force indication 1; height 3) and the corresponding expanded relative uncertainty of the test force deviation, ΔF_{rel} . There can be circumstances where the user needs to account for the relative expanded uncertainty of the test force deviation, U_{F} , generated by the hardness testing machine when determining compliance with the maximum permissible relative deviation of the test force. In [Table B.3](#), a value of ΔF_{max} is also calculated as follows:

$$\Delta F_{\text{max}} = |\Delta F_{\text{rel}}| + U_{\text{F}} \quad (\text{B.6})$$

which includes the expanded relative uncertainty of the test force. In this case, the value of ΔF_{max} , rather than the force deviation value, ΔF_{rel} , is compared to [4.2.5](#) to determine compliance.

Table B.3 — Calculation of the relative deviation of one test force measurement and the expanded relative uncertainty of the test force measurement

Relative deviation of test force [force indication 1; height 3] ΔF_{rel}	Expanded combined relative uncertainty of the test force U_{F}	Relative deviation of test force combined with the expanded relative uncertainty of the test force ΔF_{max}
0,08 %	0,23 %	0,31 %

B.2.2 Uncertainty of depth-measuring system

For the direct verification of depth-measuring system, the difference ΔL between each individual measurement of depth measured by the hardness machine and the corresponding depth value indicated by the reference instrument is calculated and reported. The direct verification verifies whether each ΔL is within specified maximum permissible limits. Consequently, the following is a procedure to calculate

the uncertainties of the ΔL values with respect to the true value of the depth. The combined standard uncertainty of the reference instrument for the depth-measuring system is calculated as follows:

$$u_L = \sqrt{u_{LRS}^2 + u_{ms}^2 + u_{LHTM}^2} \quad (B.7)$$

where

u_{LRS} is the uncertainty of measurement of the depth calibration device (reference standard) from the calibration certificate for $k = 1$;

u_{ms} is the uncertainty of measurement due to the resolution of the measuring system;

u_{LHTM} is the standard uncertainty of measurement of the hardness testing machine.

The uncertainty of measurement of the reference instrument for the depth-measuring system, the depth calibration device, is indicated in the corresponding calibration certificate. It is assumed that quantities, such as the following, do not exert an essential influence on the uncertainty of measurement of the depth calibration device:

- temperature dependence;
- long-term stability;
- interpolation deviation.

EXAMPLE Direct verification of the depth measuring system of the testing machine for the A to K scales.

Expanded uncertainty of measurement of depth calibration system: $U_{LRS} = 0,000\ 2\ \text{mm}$ ($k = 2$) (from calibration certificate)

Resolution of the depth-measuring system: $\delta_{ms} = 0,5\ \mu\text{m}$

Three measurements of depth are made at each of five intervals of depth as shown in [Table B.4](#).

$$\Delta L = L - L_{RS} \quad (B.8)$$

$$u_{LRS} = \frac{U_{LRS}}{2} \quad (B.9)$$

$$u_{LHTM} = s_{L,i} \times t \quad (B.10)$$

where $s_{L,i}$ is the standard deviation of the depth indication values for the i -th depth interval.

$$u_{ms} = \frac{\delta_{ms}}{2\sqrt{3}} \quad (B.11)$$

Table B.4 — Results of the calibration of the depth-measuring system

Rated value of the depth-measuring system	Depth measurement 1	Depth measurement 2	Depth measurement 3	Standard deviation
L_{RS}	$L_1 (\Delta L_1)$	$L_2 (\Delta L_2)$	$L_3 (\Delta L_3)$	$s_{L,i}$
mm	mm	mm	mm	mm
0,050	0,050 5 (+0,000 5)	0,050 5 (+0,000 5)	0,050 0 (0,000 0)	$2,9 \times 10^{-4}$
0,100	0,100 5 (+0,000 5)	0,100 0 (0,000 0)	0,100 5 (+0,000 5)	$2,9 \times 10^{-4}$
0,150	0,150 5 (+0,000 5)	0,150 5 (+0,000 5)	0,150 0 (0,000 0)	$2,9 \times 10^{-4}$
0,200	0,200 5 (+0,000 5)	0,200 5 (+0,000 5)	0,200 5 (+0,000 5)	0
0,250	0,250 5 (+0,000 5)	0,250 5 (+0,000 5)	0,250 0 (0,000 0)	$2,9 \times 10^{-4}$

The following example calculations will use values of the depth measurement 1 at the 0,050 mm depth interval from [Table B.4](#). See [Table B.5](#).

From the given direct verification parameters and [Table B.4](#):

$$u_{LRS} = \frac{U_{LRS}}{2} = 0,0001 \text{ mm}$$

$$u_{LHTM} = s_{L,i} \times t = 2,9 \times 10^{-4} \times 1,32 = 3,8 \times 10^{-4} \text{ mm} \quad (\text{for three readings, } t = 1,32)$$

$$u_{ms} = \frac{1}{2\sqrt{3}} \times \delta_{ms} = 1,4 \times 10^{-4} \text{ mm}$$

**Table B.5 — Calculation of the uncertainty of measurement of the measuring system
(for depth measurement 1 at the 0,050 mm depth interval from Table B.4)**

Quantity	Estimated value	Limit value	Distribution type	Standard measurement uncertainty	Sensitivity coefficient	Standard measurement uncertainty symbol	Uncertainty contribution
X_i	X_i	a_i		$u(x_i)$	c_i		u_i
	mm	mm		mm			mm
Depth measurement: calibration device	0,050	$1,5 \times 10^{-4}$	Normal	$1,0 \times 10^{-4}$	1	u_{LRS}	$1,0 \times 10^{-4}$
Depth measurement: testing machine	0,050	$1,0 \times 10^{-3}$ (A to K scales)	Normal	$3,8 \times 10^{-4}$	1	u_{LHTM}	$3,8 \times 10^{-4}$
Measurement system resolution		$0,5 \times 10^{-4}$	Rectangular	$1,4 \times 10^{-4}$	1	u_{ms}	$1,4 \times 10^{-4}$
Combined uncertainty of measurement, u_L , mm							$4,2 \times 10^{-4}$
Expanded uncertainty of measurement, U_L ($k = 2$), mm							$8,4 \times 10^{-4}$

The above calculations must be repeated for all depth measurements.

Table B.6 shows the deviation of one depth measurement ΔL (depth measurement 1; 0,050 mm depth interval) and the corresponding expanded uncertainty of the depth measurement deviation. There can be circumstances where the user needs to account for the expanded uncertainty of the depth measurement deviation generated by the hardness testing machine when determining compliance with the maximum permissible deviation of the depth measurement. In Table B.6, a value of ΔL_{max} is also calculated as follows:

$$\Delta L_{max} = |\Delta L| + U_L \quad (B.12)$$

which includes the expanded uncertainty of the depth measurement deviation. In this case, the value of ΔL_{max} , rather than the depth deviation value, ΔL , is compared to 4.3.4 to determine compliance. In the example given in Table B.6, ΔL_{max} exceeds the maximum permissible deviation of the depth measurement of $\pm 0,001$ mm for the scales A to K.

**Table B.6 — Calculation of the maximum deviation of one depth measurement
and the expanded uncertainty of the depth measurement
(for depth measurement 1 at the 0,050 mm depth interval from Table B.4)**

Depth interval	Deviation of the depth measurement	Expanded uncertainty of depth measurement	Deviation of depth measurement combined with the expanded uncertainty of the depth measurement
L_{RS}	ΔL	U_L	ΔL_{max}
0,050 mm	0,000 5 mm	0,000 84 mm	0,001 34 mm

B.2.3 Verification of the indenter

The indenter, consisting of indenter tip and holder, cannot be verified or calibrated on site. A valid calibration certificate from an accredited calibration laboratory shall exist which states the geometry of the indenter (see [Clause 6](#)).

B.2.4 Verification of the test cycle

In [4.4](#), the permissible deviation for every section of the test cycle is stipulated as $\pm 0,5$ s. While measuring with a usual time measuring system (stopwatch), the uncertainty of measurement can be indicated as 0,1 s. Therefore, an estimation of the uncertainty of measurement is not necessary.

B.3 Indirect verification — Uncertainty of calibration of testing machine

B.3.1 Uncertainty of the bias of the testing machine

NOTE In this Annex, the index “CRM (Certified Reference Material)” means, according to the definitions of the hardness testing standards, “Hardness Reference Block”.

By indirect verification with CRMs, the overall function of the hardness testing machine is checked. The repeatability of the hardness testing machine and the deviation of the hardness testing machine’s measurement of hardness from the true hardness value are determined. For the indirect verification of the hardness testing machine, the difference, or bias, b , between the average hardness of the CRM measured by the hardness machine and the corresponding certified value of the CRM is calculated and reported. The indirect verification verifies whether the bias is within specified maximum permissible limits. Consequently, the following is a procedure to calculate the uncertainty of the bias value of the hardness machine measurement with respect to the true average hardness of the CRM. This process is based on the results from indirect verification and is applicable for the calibration of the machine in Rockwell units using CRMs.

The uncertainty of the measurement of the bias of the hardness testing machine from the indirect verification follows from Formula (B.13):

$$u_{\text{HTM}} = \sqrt{u_{\text{CRM}}^2 + u_{\text{HCRM}}^2 + u_{\text{ms}}^2} \quad (\text{B.13})$$

where

- u_{CRM} is a contribution to the measurement uncertainty due to the calibration uncertainty of the certified value of the CRM according to the calibration certificate for $k = 1$;
- u_{HCRM} is a contribution to the measurement uncertainty due to the lack of measurement repeatability of the hardness testing machine and the hardness nonuniformity of the CRM, calculated as the standard deviation of the mean of the hardness measurements when measuring the CRM;
- u_{ms} is a contribution to the measurement uncertainty due to the resolution of the hardness testing machine.

EXAMPLE Indirect verification of the Rockwell C scale (approximately 45 HRC) of the testing machine.

Hardness reference block (CRM):	$H_{\text{CRM}} = 45,4$ HRC
Expanded uncertainty of the certified value of the CRM: (certificate)	$U_{\text{CRM}} = 0,5$ HRC (from calibration certificate)
Resolution of the hardness testing machine:	$\delta_{\text{ms}} = 0,1$ HRC

Five HRC measurements are made on the CRM as shown in [Table B.7](#).

$$b = \bar{H} - H_{\text{CRM}} \quad (\text{B.14})$$

$$u_{\text{CRM}} = \frac{U_{\text{CRM}}}{2} \quad (\text{B.15})$$

$$u_{\text{H}} = \frac{t \cdot s_{\text{H}}}{\sqrt{n}} \quad (\text{B.16})$$

$$u_{\text{ms}} = \frac{\delta_{\text{ms}}}{2\sqrt{3}} \quad (\text{B.17})$$

Table B.7 — Results of the indirect verification

No.	Measured hardness value <i>H</i> , HRC ^a
1	46,4 _{max}
2	46,1
3	45,3 _{min}
4	45,7
5	45,8
Mean value, \bar{H}	45,9
Standard deviation, s_{H}	0,42
^a HRC: Rockwell C hardness scale.	

From the given indirect verification parameters and [Table B.7](#):

$$b = \bar{H} - H_{\text{CRM}} = 45,9 - 45,4 = 0,5 \text{ HRC}$$

$$u_{\text{CRM}} = \frac{U_{\text{CRM}}}{2} = 0,25 \text{ HRC}$$

For $n = 5$, $t = 1,14$,

$$u_{\text{H}} = \frac{t \cdot s_{\text{H}}}{\sqrt{n}} = \frac{1,14 \times 0,42}{\sqrt{5}} = 0,21 \text{ HRC}$$

$$u_{\text{ms}} = \frac{1}{2\sqrt{3}} \times \delta_{\text{ms}} = 0,03 \text{ HRC}$$

B.3.2 Budget of uncertainty of indirect calibration/verification measurement (See Table B.8)

Table B.8 — Budget of uncertainty of measurement

Quantity	Estimated value	Distribution type	Standard uncertainty of measurement	Sensitivity coefficient	Standard measurement uncertainty symbol	Uncertainty contribution
X_i	x_i		$u(x_i)$	c_i		u_i
Certified value of CRM	45,4 HRC	Normal	0,25 HRC	1,0	u_{CRM}	0,25 HRC
Hardness machine measurement	45,4 HRC	Normal	0,21 HRC	1,0	u_H	0,21 HRC
Hardness machine resolution	0 HRC	Rectangular	0,03 HRC	1,0	u_{ms}	0,03 HRC
Combined uncertainty of bias value, u_{HTM}						0,33 HRC
Expanded uncertainty of bias value, $U_{HTM} (k = 2)$						0,66 HRC

Table B.9 shows the bias value, b , and the corresponding expanded uncertainty of the bias measurement, U_{HTM} . There can be circumstances where the user needs to account for the expanded uncertainty of the bias measurement generated by the hardness testing machine when determining compliance with the maximum permissible deviation of the bias. In Table B.9, a value of ΔH_{HTMmax} also calculated as follows:

$$\Delta H_{HTMmax} = |b| + U_{HTM} \quad (B.18)$$

which includes the expanded uncertainty of the bias. In this case, the value of ΔH_{HTMmax} , rather than the bias value, b , is compared to Table 2 to determine compliance.

Table B.9 — Maximum deviation of the hardness testing machine including the uncertainty of measurement

Measured hardness on the hardness testing machine	Deviation of the testing machine when calibrating with the reference block	Expanded uncertainty of bias value	Maximum deviation of the testing machine including uncertainty of bias value
H	b	U_{HTM}	ΔH_{HTMmax}
45,9 HRC	0,5 HRC	0,66 HRC	1,16 HRC

Bibliography

- [1] SAWLA A. *Uncertainty of measurement in the verification and calibration of the force measuring systems of testing machines*. Proceedings of the Asia-Pacific symposium on measurement of force, mass and torque (APMF), Tsukuba, Japan, November 2000
- [2] WEHRSTEDT A., & PATKOVSKY I. News in the field of standardization about verification and calibration of materials testing machines, May 2001. EMPA Academy, 2001
- [3] GABAUER W. *Manual codes of practice for the determination of uncertainties in mechanical tests on metallic materials, The estimation of uncertainties in hardness measurements*, Project No. SMT4-CT97-2165, UNCERT COP 14:2000
- [4] POLZIN T., & SCHWENK D. Method for Uncertainty Determination of Hardness Testing; PC File for Determination, *Materialprüfung* **44** (2002) 3, pp. 64-71.
- [5] ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*
- [6] ISO/IEC 17011, *Conformity assessment — General requirements for accreditation bodies accrediting conformity assessment bodies*

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com



...making excellence a habit.™