

BS EN ISO 6508-3:2015



BSI Standards Publication

# Metallic materials — Rockwell hardness test

Part 3: Calibration of reference blocks

**bsi.**

...making excellence a habit.™

**National foreword**

This British Standard is the UK implementation of EN ISO 6508-3:2015. It supersedes BS EN ISO 6508-3:2005 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee ISE/101/5, Indentation hardness testing.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2015.  
Published by BSI Standards Limited 2015

ISBN 978 0 580 79171 0

ICS 77.040.10

**Compliance with a British Standard cannot confer immunity from legal obligations.**

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 March 2015.

**Amendments/corrigenda issued since publication**

Date	Text affected
------	---------------

---

English Version

## Metallic materials - Rockwell hardness test - Part 3: Calibration of reference blocks (ISO 6508-3:2015)

Matériaux métalliques - Essai de dureté Rockwell - Partie 3:  
Étalonnage des blocs de référence (ISO 6508-3:2015)

Metallische Werkstoffe - Härteprüfung nach Rockwell - Teil  
3: Kalibrierung von Härtevergleichsplatten (ISO 6508-  
3:2015)

This European Standard was approved by CEN on 10 January 2015.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION  
COMITÉ EUROPÉEN DE NORMALISATION  
EUROPÄISCHES KOMITEE FÜR NORMUNG

**CEN-CENELEC Management Centre: Avenue Marnix 17, B-1000 Brussels**

## **Foreword**

This document (EN ISO 6508-3:2015) has been prepared by Technical Committee ISO/TC 164 "Mechanical testing of metals" in collaboration with Technical Committee ECISS/TC 101 "Test methods for steel (other than chemical analysis)" the secretariat of which is held by AFNOR.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by September 2015, and conflicting national standards shall be withdrawn at the latest by September 2015.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN ISO 6508-3:2005.

According to the CEN-CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

### **Endorsement notice**

The text of ISO 6508-3:2015 has been approved by CEN as EN ISO 6508-3:2015 without any modification.

# Contents

Page

<b>Foreword</b> .....	<b>iv</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Manufacture of reference blocks</b> .....	<b>1</b>
<b>4 Calibration machine and calibration indenter</b> .....	<b>2</b>
4.1 General.....	2
4.2 Calibration machine.....	2
4.3 Calibration diamond indenter.....	2
4.4 Calibration ball indenter.....	4
<b>5 Calibration procedure</b> .....	<b>4</b>
<b>6 Number of indentations</b> .....	<b>5</b>
<b>7 Uniformity of hardness</b> .....	<b>5</b>
<b>8 Marking</b> .....	<b>6</b>
<b>9 Calibration certificate</b> .....	<b>7</b>
<b>10 Validity</b> .....	<b>7</b>
<b>Annex A (normative) Uniformity of reference blocks</b> .....	<b>8</b>
<b>Annex B (informative) Uncertainty of the mean hardness value of hardness-reference blocks</b> .....	<b>10</b>
<b>Annex C (normative) Requirements for reference diamond indenters</b> .....	<b>16</b>
<b>Bibliography</b> .....	<b>17</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 164, *Mechanical testing of metals*, Subcommittee SC 3, *Hardness testing*.

This third edition cancels and replaces the second edition (ISO 6508-3:2005), which has been technically revised.

ISO 6508 consists of the following parts, under the general title *Metallic materials — Rockwell hardness test*:

- *Part 1: Test method*
- *Part 2: Verification and calibration of testing machines and indenters*
- *Part 3: Calibration of reference blocks*

# Metallic materials — Rockwell hardness test —

## Part 3: Calibration of reference blocks

### 1 Scope

This part of ISO 6508 specifies a method for the calibration of reference blocks to be used for the indirect and daily verification of Rockwell hardness testing machines, as specified in ISO 6508-2:2015.

Attention is drawn to the fact that the use of hard metal for ball indenters is considered to be the standard type of Rockwell indenter ball. Steel indenter balls can be used only when complying with ISO 6508-1:2015, Annex A.

### 2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 376, *Metallic materials — Calibration of force-proving instruments used for the verification of uniaxial testing machines*

ISO 6508-1:2015, *Metallic materials — Rockwell hardness test — Part 1: Test method*

ISO 6508-2:2015, *Metallic materials — Rockwell hardness test — Part 2: Verification and calibration of testing machines and indenters*

### 3 Manufacture of reference blocks

**3.1** The block shall be specially manufactured for use as a hardness-reference block.

**NOTE** Attention is drawn to the need to use a manufacturing process, which will give the necessary homogeneity, stability of structure, and uniformity of surface hardness.

**3.2** Each hardness reference block shall be of a thickness not less than 6 mm. To minimize the effect of hardness change with increasing number of indents, thicker blocks should be used.

**3.3** The reference blocks shall be free of magnetism. It is recommended that the manufacturer ensure that the blocks, if made of steel, have been demagnetized at the end of the manufacturing process (before calibration).

**3.4** The deviation from surface flatness of the top and bottom surfaces shall be  $\leq 0,01$  mm. The bottom of the blocks shall not be convex. The deviation from parallelism of the top and bottom surfaces shall be  $\leq 0,02$  mm per 50 mm.

**3.5** The test surface and lower surface shall be free from damage, such as notches, scratches, oxide layers, etc., which can interfere with the measurement of the indentations. The surface roughness,  $R_a$ , shall not exceed 0,000 3 mm for the test surface and 0,000 8 mm for the bottom surface. Sampling length is  $l = 0,8$  mm (see ISO 4287:1997, 3.1.9).

3.6 To verify that no material is subsequently removed from the reference block, the thickness at the time of calibration shall be marked on it, to the nearest 0,1 mm, or an identifying mark shall be made on the test surface [see [8.1 e](#)].

## 4 Calibration machine and calibration indenter

### 4.1 General

4.1.1 Calibrations and verifications of Rockwell calibration machines and calibration indenters shall be carried out at a temperature of  $(23 \pm 5)$  °C.

4.1.2 The instruments used for calibration shall be traceable to national standards.

### 4.2 Calibration machine

4.2.1 In addition to fulfilling the general conditions specified in ISO 6508-2:2015, Clause 3, the calibration machine shall also meet the requirements given in [4.2.2](#), [4.2.3](#), [4.2.4](#), [4.2.5](#), and [4.2.6](#).

4.2.2 The machine shall be directly verified in intervals not exceeding 12 months. Direct verification involves calibration and verification of the following:

- a) test force;
- b) measuring system;
- c) testing cycle; if this is not possible, at least the force versus time behaviour.

4.2.3 The test force shall be measured by means of an elastic proving device (according to ISO 376) class 0,5 or better and calibrated for reversibility, or by another method having the same or better accuracy.

Evidence should be available to demonstrate that the output of the force-proving device does not vary by more than 0,1 % in a period of 1 s to 30 s, following a stepped change in force.

4.2.4 Each test force shall be measured and shall agree with the nominal preliminary test force,  $F_0$ , to within  $\pm 0,2$  % and the nominal total test force,  $F$ , to within  $\pm 0,1$  %.

4.2.5 The measuring system shall have a resolution of  $\pm 0,000 1$  mm and a maximum expanded uncertainty of  $0,000 2$  mm, when calculated with a confidence level of 95 % over its working range.

4.2.6 The testing cycle shall be timed with an uncertainty less than  $\pm 0,5$  s and shall conform to the testing cycle of [Clause 5](#).

### 4.3 Calibration diamond indenter

4.3.1 The geometric shape and performance of calibration diamond indenters shall be calibrated as defined below. Direct verification of the geometric shape shall be made before first use and at a frequency of no greater than five years. Verification of the indenter performance, as specified in [4.3.3](#), shall be made before first use and at a frequency of no greater than 12 months.

4.3.2 The diamond indenter shall be measured on at least eight unique axial section planes equidistant from each other (e.g. the eight cross-sections will be spaced approximately  $22,5^\circ$  apart at  $0^\circ$ ,  $22,5^\circ$ ,  $45^\circ$ ,  $67,5^\circ$ ,  $90^\circ$ ,  $112,5^\circ$ ,  $135^\circ$ ,  $157,5^\circ$ ), and shall meet the following requirements:



- a) The cone angle shall be measured adjacent to the blend. The diamond cone shall have a mean included angle of  $(120 \pm 0,1)^\circ$ . In each measured axial section, the included angle shall be  $(120 \pm 0,17)^\circ$ .
- b) The mean deviation from straightness of the generatrix of the diamond cone adjacent to the blend shall not exceed 0,000 5 mm over a minimum length of 0,4 mm. In each measured section, the deviation shall not exceed 0,000 7 mm.
- c) The radius of the spherical tip of the diamond shall be measured adjacent to the blend. The tip shall have a mean radius of  $(0,200 \pm 0,005)$  mm. In each measured section, the radius shall be within  $(0,200 \pm 0,007)$  mm and local deviations from a true radius shall not exceed 0,002 mm.

NOTE The tip of the diamond indenter is usually not truly spherical, but often varies in radius across its surface. Depending on the crystallographic orientation of the diamond stone with respect to the indenter axis, diamond tends to preferentially polish away more easily or with more difficulty at the tip, producing an increasingly flat or sharp surface in the central indenter axis region. The sphericity of the diamond tip can be better evaluated by measuring multiple measurement windows of varying width. The measurement window would be bounded by widths measured along a line normal to the indenter axis. For example, the following window sizes can be evaluated:

- between  $\pm 80 \mu\text{m}$  from the indenter axis;
  - between  $\pm 60 \mu\text{m}$  from the indenter axis;
  - between  $\pm 40 \mu\text{m}$  from the indenter axis.
- d) The surfaces of the cone and the spherical tip shall blend in a smooth tangential manner. The location where the spherical tip and the cone of the diamond blend together will vary depending on the values of the tip radius and cone angle. Ideally for a perfect indenter geometry, the blend point is located at 100  $\mu\text{m}$  from the indenter axis measured along a line normal to the indenter axis. To avoid including the blend area in the measurement of the tip radius and cone angle, the portion of the diamond surface between 90  $\mu\text{m}$  and 110  $\mu\text{m}$  should be ignored.
  - e) The inclination of the axis of the diamond cone to the axis of the indenter holder (normal to the seating surface) shall be within  $0,3^\circ$ .

**4.3.3** Calibration diamond indenters shall be performance verified by performing comparison tests with reference diamond indenter(s) that meet the requirements of [Annex C](#). Calibration diamond indenters can be verified for use on either regular or superficial Rockwell diamond scales or both. The test blocks used for the comparison testing shall meet the requirements of [Clause 3](#) and be calibrated at the hardness levels given in [Table 1](#), [Table 2](#), [Table 3](#), or [Table 4](#), depending on the scales for which the indenter is verified. The testing shall be carried out in accordance with ISO 6508-1:2015.

NOTE The alternate hardness levels given in [Table 2](#) are provided to accommodate indenters calibrated to other International Standards. It is believed that calibrations conducted to [Table 1](#) or [Table 2](#) will yield equivalent results.

For each block, the mean hardness value of three indentations made using the calibration diamond indenter to be verified shall not differ from the mean hardness value of three indentations obtained with a reference diamond indenter by more than  $\pm 0,4$  Rockwell units. The indentations made with the calibration diamond indenter to be verified and with the reference diamond indenter should be adjacent.

**Table 1 — Hardness levels for indenters to be used for calibrating Rockwell regular and superficial scale test blocks (A, C, D, and N)**

Scale	Nominal hardness	Ranges
HRC	23	20 to 26
HRC	55	52 to 58
HR45N	43	40 to 46
HR15N	91	88 to 94

**Table 2 — Alternate hardness levels for indenters to be used for calibrating Rockwell regular and superficial scale test blocks (A, C, D, and N)**

Scale	Nominal hardness	Ranges
HRC	25	22 to 28
HRC	63	60 to 65
HR30N	64	60 to 69
HR15N	91	88 to 94

**Table 3 — Hardness levels for indenters to be used for calibrating Rockwell regular scale test blocks only (A, C, and D)**

Scale	Nominal hardness	Ranges
HRC	25	22 to 28
HRC	45	42 to 50
HRC	63	60 to 65
HRA	81	78 to 84

**Table 4 — Hardness levels for indenters to be used for calibrating Rockwell superficial scale test blocks only (N)**

Scale	Nominal hardness	Ranges
HR15N	91	88 to 94
HR30N	64	60 to 69
HR30N	46	42 to 50
HR45N	25	22 to 29

#### 4.4 Calibration ball indenter

**4.4.1** The calibration tungsten carbide composite ball shall be replaced at a frequency no greater than 12 months.

**4.4.2** Calibration tungsten carbide composite balls shall meet the requirements of ISO 6508-2:2015, with the exception of the following tolerances for the ball diameter:

- $\pm 0,002$  mm for the ball of diameter 1,587 5 mm;
- $\pm 0,003$  mm for the ball of diameter 3,175 mm.

### 5 Calibration procedure

**5.1** The reference blocks shall be calibrated in a calibration machine as described in [Clause 4](#), at a temperature of  $(23 \pm 5)$  °C, using the general procedure described in ISO 6508-1:2015.

During calibration, the thermal drift should not exceed 1 °C.

**5.2** The velocity of the indenter, when it comes into contact with the surface, shall not exceed 1 mm/s.

The velocity of the indenter, when it comes into contact with the surface, should not exceed 0,3 mm/s for undamped systems.

**5.3** Bring the indenter into contact with the test surface and apply the preliminary test force,  $F_0$ , without shock or vibration and without oscillation or overload of the test force. The application time,  $T_a$ , of the preliminary test force,  $F_0$ , shall not exceed 2 s.

The duration,  $T_p$ , of the preliminary test force,  $F_0$ , shall be equal to  $(3 \pm 1)$  s, as shown in Formula (1):

$$T_p = T_a/2 + T_{pm} = (3 \pm 1) \text{ s} \quad (1)$$

where

$T_p$  is the preliminary test force time;

$T_a$  is the application time of preliminary test force;

$T_{pm}$  is the duration time of preliminary test force prior to measuring the initial indentation depth.

For testing machines that apply the preliminary test force in less than 1 s ( $T_a$ ),  $T_p$  can be calculated as being equal to  $T_{pm}$ .

**5.4** Bring the measuring system to its datum position, and without shock, vibration, oscillation, or overload, apply the additional test force,  $F_1$ .

For the regular Rockwell scale tests, apply the additional test force,  $F_1$ , in  $7_{-6}^{+1}$  s. For all HRN and HRTW Rockwell superficial test scales, apply the additional test force,  $F_1$ , in less than or equal to 4 s. During the final stage of the indentation process (approximately in the range of  $0,8 F$  to  $0,99 F$ ), the indentation speed should be in the range of 0,015 mm/s to 0,04 mm/s.

**5.5** The duration of the application of the total force,  $F$ , shall be equal to  $(5 \pm 1)$  s.

**5.6** The final reading shall be made  $(4 \pm 1)$  s after removing the additional test force,  $F$ , and returning to the preliminary test force,  $F_0$ .

## 6 Number of indentations

On each reference block, at least five indentations shall be made, uniformly distributed over the test surface. The arithmetic mean of the hardness values characterizes the hardness value of the block.

To reduce the measurement uncertainty, more than five indentations should be made.

## 7 Uniformity of hardness

**7.1** For each reference block, let  $H_1, H_2, H_3, H_4, \dots, H_n$  be the values of the measured hardness, arranged in increasing order of magnitude.

The mean hardness value of all the indentations is defined according to Formula (2):

$$\bar{H} = \frac{H_1 + H_2 + H_3 + H_4 + \dots + H_n}{n} \quad (2)$$

where

$H_1, H_2, H_3, H_4, \dots, H_n$  are the hardness values corresponding to all the indentations arranged in increasing order of magnitude;

$n$  is the total number of indentations.

The non-uniformity,  $R$ , of the block in Rockwell units, under the particular conditions of calibration, is characterized by Formula (3):

$$R = H_n - H_1 \quad (3)$$

7.2 The maximum permissible value of non-uniformity,  $R$ , of a reference block in Rockwell units is given in [Table 5](#) and is graphically presented in [Figure A.1](#) and [Figure A.2](#).

**Table 5 — Maximum permissible value of non-uniformity**

Rockwell hardness scale	Maximum permissible value of non-uniformity, $R^a$
A	0,015 (100 - $\bar{H}$ ) or 0,4 HRA Rockwell units
B	0,020 (130 - $\bar{H}$ ) or 1,0 HRBW Rockwell units
C	0,010 (100 - $\bar{H}$ ) or 0,4 HRC Rockwell units
D	0,010 (100 - $\bar{H}$ ) or 0,4 HRD Rockwell units
E	0,020 (130 - $\bar{H}$ ) or 1,0 HREW Rockwell units
F	0,020 (130 - $\bar{H}$ ) or 1,0 HRFW Rockwell units
G	0,020 (130 - $\bar{H}$ ) or 1,0 HRGW Rockwell units
H	0,020 (130 - $\bar{H}$ ) or 1,0 HRHW Rockwell units
K	0,020 (130 - $\bar{H}$ ) or 1,0 HRKW Rockwell units
15N, 30N, 45N	0,020 (100 - $\bar{H}$ ) or 0,6 HR-N Rockwell units
15T, 30T, 45T	0,030 (100 - $\bar{H}$ ) or 1,2 HR-TW Rockwell units

<sup>a</sup> The greater of the two values shall apply.

7.3 The uncertainty of measurement of the hardness reference blocks shall be calculated. An example method is given in [Annex B](#).

## 8 Marking

8.1 Each reference block shall be marked with the following:

- arithmetic mean of the hardness values found in the calibration test. For example, 66,3 HRC;
- name or mark of the supplier or manufacturer;
- serial number;
- name or mark of the calibration agency;
- thickness of the block, or an identifying mark on the test surface (see [3.6](#));
- year of calibration, if not indicated in the serial number.

8.2 Any mark put on the side of the block shall be upright when the test surface is the upper face.

## 9 Calibration certificate

9.1 Each delivered reference block shall be accompanied with a document giving at least the following information:

- a) reference to this part of ISO 6508 (i.e. ISO 6508-3);
- b) identity of the block;
- c) date of calibration;
- d) individual calibration results;
- e) arithmetic mean of the hardness values;
- f) value characterizing the non-uniformity of the block (see [7.1](#));
- g) statement of uncertainty.

## 10 Validity

The hardness reference block is only valid for the scale for which it was calibrated.


The calibration validity should be limited to a duration of five years. Attention is drawn to the fact that, for Al-alloys and Cu-alloys, the calibration validity could be reduced to two years to three years.

The calibration result is only valid for the reference block at the time of calibration. The hardness of the block can be changed by repeated test on the block and attention must be drawn to the fact that it might not be negligible when the number of indentation is large.

## Annex A (normative)

### Uniformity of reference blocks


Maximum permissible values of non-uniformity,  $R$ , in Rockwell units are given in [Figure A.1](#) and [Figure A.2](#).

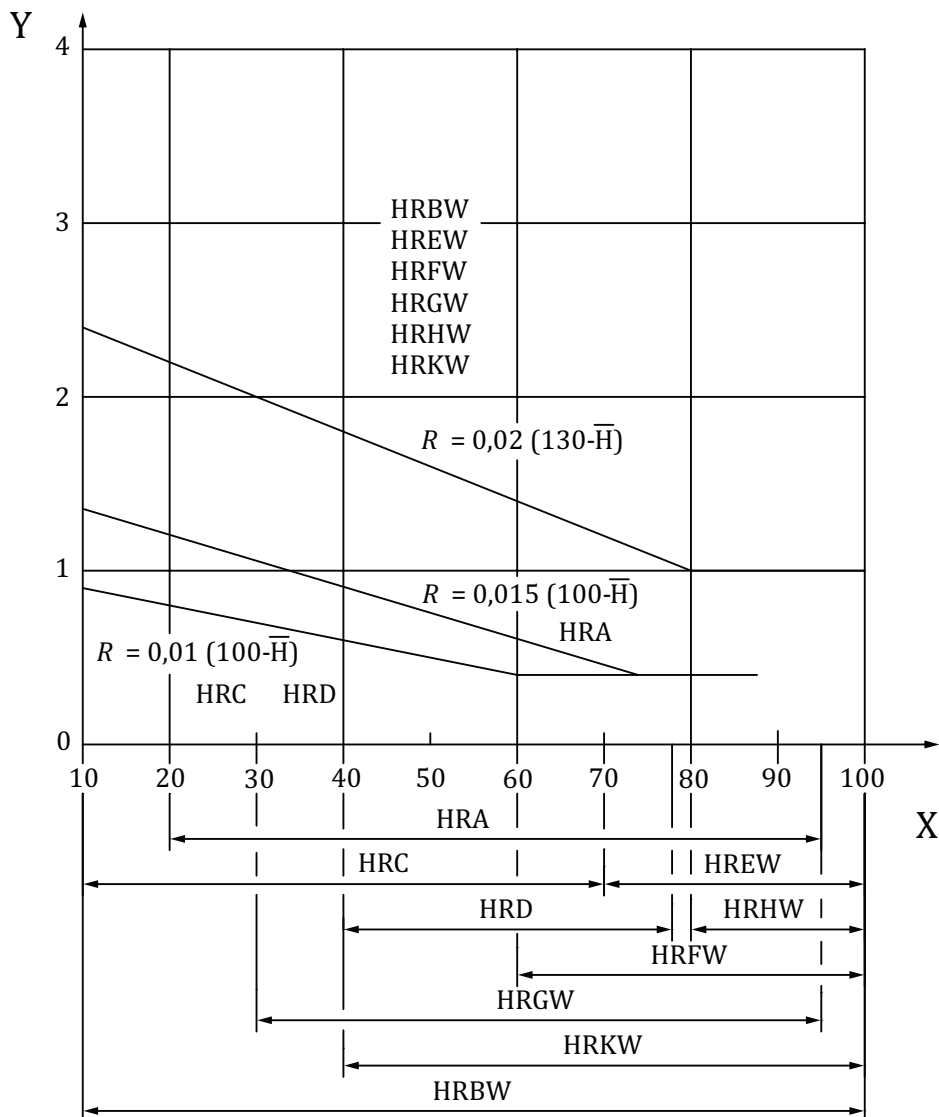

**Key**

- X Rockwell hardness
- Y non-uniformity,  $R$

**Figure A.1 — Rockwell hardness (scales A, B, C, D, E, F, G, H, and K)**

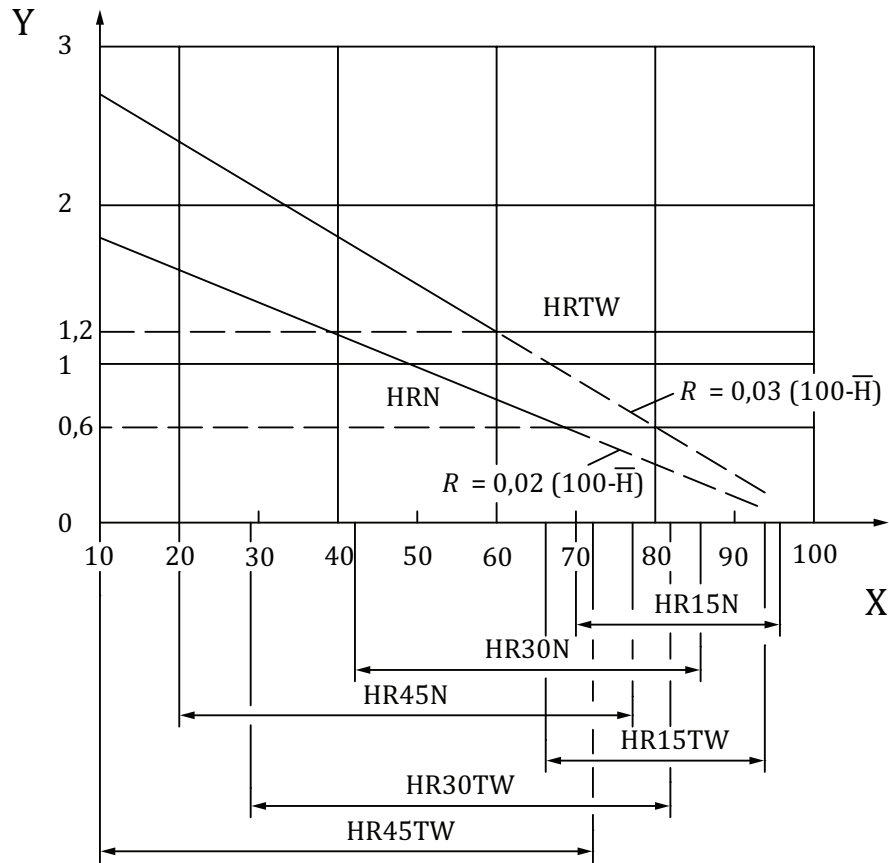

**Key**

- X Rockwell hardness
- Y non-uniformity,  $R$

**Figure A.2 — Rockwell superficial hardness (scales N and T)**

## **Annex B** **(informative)**

### **Uncertainty of the mean hardness value of hardness-reference blocks**

#### **B.1 General**

Measurement uncertainty analysis is a useful tool to help determine sources of error and to understand differences between measured values. This Annex gives guidance on uncertainty estimation, but the methods contained are for information only, unless specifically instructed otherwise by the customer. The criteria specified in this International Standard for the calibration requirements of the reference block have been developed and refined over a significant period of time. When determining a specific tolerance that the reference block needs to meet, the uncertainty associated with the use of measuring equipment has been incorporated within this tolerance and therefore, it would be inappropriate to make any further allowance for this uncertainty, for example, by reducing the tolerance by the measurement uncertainty. This applies to all measurements associated with the manufacture and calibration of the reference blocks and also to all measurements made when performing a verification of the calibration machine. In each case, it is simply the measured value resulting from the use of the specified measuring equipment that is used to assess compliance with this International Standard. However, there might be special circumstances where reducing the tolerance by the measurement uncertainty is appropriate. This should only be done by agreement of the parties involved.

NOTE The metrological chain necessary to define and disseminate hardness scales is shown in ISO 6508-1:2015, Figure I.1.

#### **B.2 Direct verification - uncertainty of calibration of machine components**

##### **B.2.1 Calibration and verification of the test force**

See ISO 6508-2:2015, Annex B.

##### **B.2.2 Calibration and verification of the depth-measuring device**

See ISO 6508-2:2015, Annex B.

##### **B.2.3 Verification of the indenter**

See ISO 6508-2:2015, Annex B.

##### **B.2.4 Verification of the test cycle**

See ISO 6508-2:2015, Annex B.

#### **B.3 Indirect verification - uncertainty of calibration of calibration machine**

NOTE 1 In this Annex, the index “CRM-P (certified reference material-primary)” means “primary hardness reference block”.

NOTE 2 The result of indirect verification is used for the evaluation of the uncertainty of calibration of the hardness calibration machine.



By indirect verification with primary hardness-reference blocks, the overall function of the hardness-calibration machine is checked. The repeatability of the hardness-calibration machine and the deviation of the hardness-calibration machine's measurement of hardness from the true hardness value are determined. For the indirect verification of the hardness-calibration machine, the difference, or bias,  $b_{\text{HCM}}$ , between the average hardness of the primary hardness-reference block measured by the hardness-calibration machine and the corresponding certified value of the primary hardness-reference block is calculated and reported. The indirect verification verifies whether the bias is within specified maximum permissible limits. Consequently, the following is a procedure to calculate the uncertainty of the bias value of the hardness-calibration machine measurement with respect to the true average hardness of the primary hardness-reference block.

The uncertainty of the measurement of the bias of the hardness-calibration machine is calculated from the indirect verification results using Formula (B.1):

$$u_{\text{HCM}} = \sqrt{u_{\text{CRM-P}}^2 + u_{\text{HCRM-P}}^2 + u_{\text{ms}}^2} \quad (\text{B.1})$$

where

$u_{\text{CRM-P}}$  is a contribution to the measurement uncertainty due to the calibration uncertainty of the certified value of the primary hardness-reference block, according to the calibration certificate for  $k = 1$ ;

$u_{\text{HCRM-P}}$  is a contribution to the measurement uncertainty due to the lack of measurement repeatability of the hardness-calibration machine and the hardness non-uniformity of the primary hardness-reference block, calculated as the standard deviation of the mean of the hardness measurements when measuring the primary hardness-reference block;

$u_{\text{ms}}$  is a contribution to the measurement uncertainty due to the resolution of the hardness-calibration machine.

**EXAMPLE** Indirect verification of the Rockwell C scale ( $\sim 45$  HRC) of the hardness-calibration machine.

Primary-hardness reference block (CRM-P)  $H_{\text{CRM-P}} = 45,40$  HRC

Expanded uncertainty of the certified value of the CRM-P  $U_{\text{CRM-P}} = 0,24$  HRC (from calibration certificate)

Resolution of the hardness-calibration machine  $\delta_{\text{ms}} = 0,01$  HRC

Five HRC measurements are made on the CRM-P, as shown in [Table B.1](#).

$$b_{\text{HCM}} = \bar{H} - H_{\text{CRM-P}} \quad (\text{B.2})$$

$$u_{\text{CRM-P}} = \frac{U_{\text{CRM-P}}}{2} \quad (\text{B.3})$$

$$u_{\text{HCRM-P}} = \frac{t \times s_{\text{HCRM-P}}}{\sqrt{n}} \quad (\text{B.4})$$

$$u_{\text{ms}} = \frac{\delta_{\text{ms}}}{2\sqrt{3}} \quad (\text{B.5})$$

where

$s_{\text{HCRM-P}}$  is the standard deviation of the indirect verification measurements.

**Table B.1 — Results of the indirect verification**

No.	Measured hardness value $H$ , HRC
1	45,65
2	45,52
3	45,51
4	45,58
5	45,61
Mean value, $\bar{H}$	45,57
Standard deviation, $s_{\text{HCRM-P}}$	0,059
Standard uncertainty of measurement, $u_{\text{HCRM-P}}$	0,030
HRC Rockwell C scale hardness.	

From the given indirect verification parameters and [Table B.1](#):

$$b_{\text{HCM}} = \bar{H} - H_{\text{CRM}} = (45,57 - 45,40) \text{ HRC} = 0,17 \text{ HRC}$$

$$u_{\text{CRM-P}} = \frac{U_{\text{CRM-P}}}{2} = 0,12 \text{ HRC}$$

For  $n = 5$ ,  $t = 1,14$

$$u_{\text{HCRM-P}} = \frac{t \times s_{\text{HCRM-P}}}{\sqrt{n}} = \frac{1,14 \times 0,059}{\sqrt{5}} = 0,030 \text{ HRC}$$

$$u_{\text{ms}} = \frac{1}{2\sqrt{3}} \times \delta_{\text{ms}} = 0,003 \text{ HRC}$$

**Table B.2 — Budget of uncertainty of measurement Bias**

Quantity $X_i$	Estimated value $x_i$	Standard uncertainty of measurement $u(x_i)$	Distribution type	Sensitivity coefficient $c_i$	Standard measurement uncertainty symbol	Uncertainty contribution $u_i(H)$
Certified value of CRM-P	45,40 HRC	0,12 HRC	Normal	1,0	$u_{\text{CRM-P}}$	0,120 HRC
Hardness calibration machine measurement	45,40 HRC	0,030 HRC	Normal	1,0	$u_{\text{HCRM-P}}$	0,030 HRC
Hardness calibration machine resolution	0 HRC	0,003 HRC	Rectangular	1.0	$u_{\text{ms}}$	0,003 HRC
Combined uncertainty of bias value, $u_{\text{HCM}}$						0,124 HRC
Expanded uncertainty of bias value, $U_{\text{HCM}} (k = 2)$						0,247 HRC
HRC Rockwell C scale hardness.						

## B.4 Uncertainty of the certified value of hardness-reference blocks

### B.4.1 General

The combined expanded uncertainty of the measurement of a calibrated hardness-reference block is calculated using Formula (B.6):

$$U_{\text{CRM}} = k \times \sqrt{u_{\text{HCRM}}^2 + u_{\text{ms}}^2 + u_{\text{HCM}}^2} \quad (\text{B.6})$$

When measurements made using the hardness-calibration machine are not corrected for bias,  $b_{\text{HCM}}$ , then the certified value of the calibrated hardness-reference block,  $\bar{H}_{\text{CRM}}$ , and the associated uncertainty are calculated using Formula (B.7):

$$\bar{H}_{\text{CRM}} \pm (U_{\text{CRM}} + |b_{\text{HCM}}|) \quad (\text{B.7})$$

When measurements made using the hardness-calibration machine are corrected for bias,  $b_{\text{HCM}}$ , then the certified value of the calibrated hardness-reference block,  $\bar{H}_{\text{CRM}}$  and the associated uncertainty are calculated using Formula (B.8):

$$(\bar{H}_{\text{CRM}} - b_{\text{HCM}}) \pm U_{\text{CRM}} \quad (\text{B.8})$$

where

$u_{\text{HCRM}}$  is a contribution to the measurement uncertainty due to the lack of measurement repeatability of the hardness-calibration machine and the non-uniformity of the CRM block being calibrated;

$u_{\text{ms}}$  is a contribution to the measurement uncertainty due to the resolution of the hardness-calibration machine;

$u_{\text{HCM}}$  is a contribution to the measurement uncertainty due to the standard uncertainty of the bias,  $b_{\text{HCM}}$ , measurement generated by the hardness-calibration machine [this value is reported as a result of the indirect verification defined above, see Formula (B.1)];

$b_{\text{HCM}}$  is the bias between the average hardness of the primary hardness-reference block measured by the hardness-calibration machine and the corresponding certified value of the primary hardness-reference block.

#### EXAMPLE

Bias of hardness-calibration machine (~ 45 HRC)  $b_{\text{HCM}} = 0,17$  HRC

Combined standard uncertainty of bias value (~ 45 HRC)  $u_{\text{HCM}} = 0,124$  HRC

Resolution of the hardness-calibration machine  $\delta_{\text{ms}} = 0,01$  HRC

Five calibration HRC measurements are made on the hardness-reference block, as shown in [Table B.3](#).

$$u_{\text{HCRM}} = \frac{t \times s_{\text{HCRM}}}{\sqrt{n}} \quad (\text{B.9})$$

$$u_{\text{ms}} = \frac{\delta_{\text{ms}}}{2\sqrt{3}} \quad (\text{B.10})$$

**Table B.3 — Results of the calibration of the hardness-reference block**

No.	Measured hardness value, $H$ , HRC
1	43,22
2	43,30
3	43,23
4	43,37
5	43,40
Mean value, $\bar{H}_{CRM}$	43,30
Standard deviation, $s_{HCRM}$	0,081
HRC Rockwell C scale hardness.	

From the given indirect verification parameters and [Table B.3](#):

$$u_{HCRM} = \frac{t \times s_{HCRM}}{\sqrt{n}} = \frac{1,14 \times 0,081}{\sqrt{5}} = 0,041 \text{ HRC}$$

$$u_{ms} = \frac{1}{2\sqrt{3}} \times \delta_{ms} = 0,003 \text{ HRC}$$

#### B.4.2 Budget of uncertainty of certified value of hardness-reference blocks

**Table B.4 — Budget of uncertainty of measurement**

Quantity $X_i$	Estimated value $x_i$	Distribution type	Standard uncertainty of measurement $u(x_i)$	Sensitivity coefficient $c_i$	Standard measurement uncertainty symbol	Uncertainty contribution $u_i$
Hardness calibration machine measurement	43,30 HRC	Normal	0,041 HRC	1,0	$u_{HCRM}$	0,041 HRC
Hardness calibration machine resolution	0 HRC	Rectangular	0,003 HRC	1,0	$u_{ms}$	0,003 HRC
Hardness calibration machine bias	0,17 HRC	Normal	0,124 HRC	1,0	$u_{HCM}$	0,124 HRC
Standard uncertainty of certified value of a calibrated hardness-reference block, $u_{CRM}$						0,131 HRC
Expanded uncertainty of certified value of a calibrated hardness-reference block, $U_{CRM} (k = 2)$						0,261 HRC

**Table B.5 — Uncertainty of certified value of the hardness-reference block**

	<b>Certified value of hardness reference block</b>	<b>Expanded uncertainty of measurement</b> $U_{\text{CRM}}$	<b>Hardness calibration machine bias</b> $b_{\text{HCM}}$	<b>Expanded uncertainty of certified value of hardness-reference block</b>
$\bar{H}_{\text{CRM}(\text{Uncorr})}$ Uncorrected	43,30 HRC $(\bar{H}_{\text{CRM}})$	0,26 HRC	0,17 HRC	0,43 HRC $(U_{\text{CRM}} +  b_{\text{HCM}} )$
$\bar{H}_{\text{CRM}(\text{Corr})}$ Corrected	43,10 HRC $(\bar{H}_{\text{CRM}} - b_{\text{HCM}})$	0,26 HRC	0,17 HRC	0,26 HRC $(U_{\text{CRM}})$
HRC Rockwell C scale hardness.				

## Annex C (normative)

### Requirements for reference diamond indenters

**C.1** Reference diamond indenters shall comply with [4.3.2](#) and the following additional requirements.

**C.2** Reference diamond indenters shall be performance verified by comparison tests with national reference diamond indenters. The national reference diamond indenter is the indenter or indenters being recognized as the national reference indenter(s) of the National Metrology Institute. Reference blocks shall be tested at the hardness levels given in [Table 1](#), [Table 2](#), [Table 3](#), or [Table 4](#), depending on the scales for which the reference diamond indenter is certified. The testing shall be carried out in accordance with ISO 6508-1:2015.

**C.3** For each block, the mean hardness value of five indentations made using the reference diamond indenter to be verified shall not differ from the mean hardness value of five indentations obtained with a national reference diamond indenter by more than  $\pm 0,4$  Rockwell units. The indentations made with the reference diamond indenter and with the national Reference diamond indenter should be adjacent.

## Bibliography

- [1] ISO 4287:1997, *Geometrical Product Specifications (GPS) — Surface texture: Profile method — Terms, definitions and surface texture parameters*
- [2] ISO/IEC 17011, *Conformity assessment — General requirements for accreditation bodies accrediting conformity assessment bodies*
- [3] ISO/IEC 17025, *General requirements for the competence of testing and calibration laboratories*
- [4] POLZIN T., & SCHWENK D. Method for Uncertainty Determination of Hardness Testing; PC File for Determination, *Materialprüfung* **44** (2002) 3, pp. 64-71
- [5] SAWLA A. *Uncertainty of measurement in the verification and calibration of the force measuring systems of testing machines*. Proceedings of the Asia-Pacific symposium on measurement of force, mass and torque (APMF), Tsukuba, Japan, November 2000
- [6] WEHRSTEDT A., & PATKOVSKY I. News in the field of standardization about verification and calibration of materials testing machines, May 2001. EMPA Academy, 2001
- [7] GABAUER W. *Manual codes of practice for the determination of uncertainties in mechanical tests on metallic materials, The estimation of uncertainties in hardness measurements*, Project No. SMT4-CT97-2165, UNCERT COP 14:2000







# British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

## About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

## Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at [bsigroup.com/standards](http://bsigroup.com/standards) or contacting our Customer Services team or Knowledge Centre.

## Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at [bsigroup.com/shop](http://bsigroup.com/shop), where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

## Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to [bsigroup.com/subscriptions](http://bsigroup.com/subscriptions).

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

**PLUS** is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit [bsigroup.com/shop](http://bsigroup.com/shop).

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email [bsmusales@bsigroup.com](mailto:bsmusales@bsigroup.com).

## BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

## Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

## Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

## Useful Contacts:

### Customer Services

**Tel:** +44 845 086 9001

**Email (orders):** [orders@bsigroup.com](mailto:orders@bsigroup.com)

**Email (enquiries):** [cservices@bsigroup.com](mailto:cservices@bsigroup.com)

### Subscriptions

**Tel:** +44 845 086 9001

**Email:** [subscriptions@bsigroup.com](mailto:subscriptions@bsigroup.com)

### Knowledge Centre

**Tel:** +44 20 8996 7004

**Email:** [knowledgecentre@bsigroup.com](mailto:knowledgecentre@bsigroup.com)

### Copyright & Licensing

**Tel:** +44 20 8996 7070

**Email:** [copyright@bsigroup.com](mailto:copyright@bsigroup.com)



...making excellence a habit.™