

# Natural gas — Determination of mercury —

## Part 1: Sampling of mercury by chemisorption on iodine

The European Standard EN ISO 6978-1:2005 has the status of a  
British Standard

ICS 75.060

## National foreword

This British Standard is the official English language version of EN ISO 6978-1:2005. It is identical with ISO 6978-1:2003. Together with BS ISO 6978-2 and -3, it supersedes BS 7678:1993 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee PTI/15, Natural gas and gas analysis, which has the responsibility to:

- aid enquirers to understand the text;
- present to the responsible international/European committee any enquiries on the interpretation, or proposals for change, and keep UK interests informed;
- monitor related international and European developments and promulgate them in the UK.

A list of organizations represented on this committee can be obtained on request to its secretary.

### Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the *BSI Catalogue* under the section entitled “International Standards Correspondence Index”, or by using the “Search” facility of the *BSI Electronic Catalogue* or of British Standards Online.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

**Compliance with a British Standard does not of itself confer immunity from legal obligations.**

### Summary of pages

This document comprises a front cover, an inside front cover, the EN ISO title page, the EN ISO foreword page, the ISO title page, pages ii to v, a blank page, pages 1 to 16, an inside back cover and a back cover.

The BSI copyright notice displayed in this document indicates when the document was last issued.

### Amendments issued since publication

Amd. No.	Date	Comments
16103	January 2006	Renumbers BS ISO 6978-1:2003 as BS EN ISO 6978-1:2005

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 17 December 2003

© BSI 16 February 2006

ISBN 0 580 43103 7

ICS 75.060

English version

## Natural gas — Determination of mercury — Part 1: Sampling of mercury by chemisorption on iodine (ISO 6978-1:2003 )

Gaz naturel — Détermination de la teneur en mercure —  
Partie 1: Echantillonnage de mercure par chimisorption sur  
iode (ISO 6978-1:2003)

Erdgas — Bestimmung von Quecksilber — Teil 1:  
Probenahme von Quecksilber durch Chemisorption an Iod  
(ISO 6978-1:2003)

This European Standard was approved by CEN on 17 April 2005.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION  
COMITÉ EUROPÉEN DE NORMALISATION  
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

## Foreword

The text of ISO 6978-1:2003 has been prepared by Technical Committee ISO/TC 193, Natural gas, of the International Organization for Standardization (ISO) and has been taken over as EN ISO 6978-1:2005 by CMC.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by November 2005, and conflicting national standards shall be withdrawn at the latest by November 2005.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

### Endorsement notice

The text of ISO 6978-1:2003 has been approved by CEN as EN ISO 6978-1:2005 without any modifications.

INTERNATIONAL  
STANDARD

**ISO**  
**6978-1**

First edition  
2003-10-15

---

---

**Natural gas — Determination of  
mercury —**

Part 1:  
**Sampling of mercury by chemisorption  
on iodine**

*Gaz naturel — Détermination de la teneur en mercure —*

*Partie 1: Échantillonnage de mercure par chimisorption sur iode*



Reference number  
ISO 6978-1:2003(E)



## Contents

Page

Foreword .....	iv
Introduction .....	v
1 Scope.....	1
2 Normative references .....	1
3 Terms and definitions .....	2
4 Principle .....	2
5 Apparatus.....	2
6 Reagents .....	9
7 Sampling .....	10
7.1 General .....	10
7.2 Sampling procedure (see Figures 1 and 2).....	11
7.3 Sample treatment .....	12
8 Mercury determination .....	13
8.1 Transfer of mercury to AAS or AFS instrument.....	13
8.2 Calibration.....	13
8.3 Blank test .....	13
9 Calculation .....	14
10 Precision .....	15
10.1 General .....	15
10.2 Repeatability and reproducibility .....	15
10.3 Uncertainty.....	15
11 Test report.....	15
Bibliography .....	16

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 6978-1 was prepared by Technical Committee ISO/TC 193, *Natural gas*, Subcommittee SC 1, *Analysis of natural gas*.

This first edition of ISO 6978-1, together with ISO 6978-2, cancels and replaces ISO 6978:1992, which has been technically revised.

ISO 6978 consists of the following parts, under the general title *Natural gas — Determination of mercury*:

- *Part 1: Sampling of mercury by chemisorption on iodine*
- *Part 2: Sampling of mercury by amalgamation on gold/platinum alloy*



## Introduction

Natural gases may contain considerable amounts of mercury, which are generally present in the elemental form. Gases with high mercury content have to be purified to avoid the condensation of mercury during processing and transport as well as to be compliant with the demands of gas sales contracts. Low mercury concentrations are specified when natural gas is to be liquefied. This is to avoid severe corrosion problems, for instance in aluminium heat exchangers of liquefaction plants.

Since the presence of hydrocarbons, in particular aromatic hydrocarbons present in low concentrations in almost every natural gas, interferes in the determination of mercury by atomic absorption spectrometry (AAS) or atomic fluorescence spectrometry (AFS), mercury cannot be determined directly in natural gas. Therefore, prior to the analytical determination, mercury has to be collected and separated from aromatic hydrocarbons.

The purpose of the determination of the mercury content can be

- to monitor gas quality,
- to monitor the operation of gas treatment plants for mercury removal.

Several methods for the collection or enrichment of mercury from natural gas have been developed. The collection of mercury from dry natural gas normally poses no particular problem. However, care should be taken when sampling mercury from natural gases under nearly condensing conditions (see ISO 6570).

The two parts of ISO 6978 describe the principles of sampling and specify the general requirements for methods for sampling mercury and for determining total mercury in pipeline quality natural gas. This part of ISO 6978 specifies a method of sampling mercury by chemisorption on iodine-impregnated silica gel whereas Part 2 specifies a method of sampling mercury by amalgamation on gold/platinum alloy thread.



# Natural gas — Determination of mercury —

## Part 1: Sampling of mercury by chemisorption on iodine

**WARNING** — The use of this part of ISO 6978 may involve hazardous materials, operations and equipment. This part of ISO 6978 does not purport to address all of the safety problems, associated with its use. It is the responsibility of the user of this part of ISO 6978 to establish appropriate safety and health practices and to determine the applicability or regulatory limitations prior to use.

### 1 Scope

This part of ISO 6978 specifies a method for the determination of total mercury content in natural gas using a sampling method at pressures up to 40 MPa by chemisorption on iodine-impregnated silica gel. This sampling method is suitable for the determination of mercury contents within the range of 0,1 µg/m<sup>3</sup> to 5 000 µg/m<sup>3</sup> in natural gas. This method is applicable to sampled gas volumes containing less than 20 mg hydrogen sulfide (absolute content) and less than a total liquid hydrocarbon condensate of 10 g/m<sup>3</sup> under the sampling conditions. The collected mercury is determined by measuring the absorbance or fluorescence of mercury vapour at 253,7 nm.

NOTE ISO 6978-2 gives a sampling method suitable for the determination of mercury content of pipeline natural gas by amalgamation of mercury on gold/platinum alloy thread at atmospheric pressure for the range of mercury from 0,01 µg/m<sup>3</sup> to 100 µg/m<sup>3</sup> and for sampling at high pressure (up to 8 MPa) from 0,001 µg/m<sup>3</sup> to 1 µg/m<sup>3</sup>.

### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 6570, *Natural gas — Determination of potential hydrocarbon liquid content — Gravimetric methods*

ISO 10715, *Natural gas — Sampling guidelines*

ISO 14111, *Natural gas — Guidelines to traceability in analysis*

ISO 14532, *Natural gas — Vocabulary*

*Guide to the expression of uncertainty in measurement (GUM)*, BIPM, IEC, IFCC, ISO, IUPAC, IUPAP, OIML

AISI Steel Code<sup>1)</sup>

---


1) Available from the American Iron and Steel Institute, c/o James McCarl, 131 Huron Drive, Carnegie, PA 15106, USA.

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 14532 apply.

### 4 Principle

The gas is passed through a glass tube containing silica gel impregnated with iodine. Mercury (Hg) present in the gas as elemental mercury or organic mercury compounds [e.g. dimethyl mercury,  $\text{Hg}(\text{CH}_3)_2$ , or diethyl mercury,  $\text{Hg}(\text{C}_2\text{H}_5)_2$ ] is chemisorbed:



The mercury iodide ( $\text{HgI}_2$ ) formed is then dissolved in an ammonium iodide/iodine solution ( $\text{NH}_4\text{I}/\text{I}_2$ ) in the laboratory. Hydrocarbon condensates are removed by vacuum stripping at this stage. Mercury, present in the form of a water-soluble complex, is determined by reducing aliquot portions of this solution with alkaline tin(II) solution to elemental mercury. The mercury is stripped from the solution by an inert gas and the mercury vapour is transferred to a cold vapour atomic absorption spectrometer (AAS) or atomic fluorescence spectrometer (AFS) for measurement at 253,7 nm. Calibration for the final mercury determination is performed in the same way using an aqueous mercury standard solution which is matrix-matched to the sample.

Unless otherwise specified, gas volumes are expressed in cubic metres ( $\text{m}^3$ ) at 273,15 K and 1 013,25 hPa.

### 5 Apparatus

The parameters influencing the measurement shall be traceable to national or International Standards. The uncertainty of the volume measurement (volume, temperature and pressure of the gas as well as ambient air pressure) directly contributes to the uncertainty of the determined mercury content of the gas. Therefore suitable measuring equipment, calibrated against a commonly accepted reference, shall be used to minimize the uncertainty of the volume measurement to less than 1 %.

**5.1 Sampling apparatus** [see Figure 1 a) for sampling up to 10 MPa and Figure 1 b) for up to 40 MPa], comprising the following:

**5.1.1 High-pressure sampling cell** (see Figure 1 with details given in Figure 2), made of NiMo16Cr15W (material no. 2.4819 in accordance with the Steel Code), which includes a temperature gauge and a pressure gauge and the following components.

**5.1.1.1 Acid-washed glass wool.**

**5.1.1.2 Sampling tube** (see Figure 1 with details given in Figure 3), made of borosilicate glass and fitted with a screw cap.

Fit the sampling tube (Figure 3) first with a layer, 0,5 cm thick, of acid-washed glass wool (5.1.1.1) to retain the absorbent. Then fill the tube with 4,00 g of iodine-laden silica gel (6.2.3) to obtain a 5 cm absorption layer. Then add another layer, 0,5 cm thick, of glass wool (5.1.1.1) to retain the top of the absorbent layer. Close the tube with a screw cap.

**5.1.2 Temperature gauges or thermometers** (see Figure 1 with details given in Figure 2).

**5.1.3 Pressure gauges** (see Figure 1 with details given in Figure 2).

**5.1.4 Pressure relief valves** (see Figure 1) which are either

- a) **electrically heated**, for sampling pressure up to 10 MPa [see Figure 1 a)], or
- b) **coupled with a heat exchanger** (5.1.5), for sampling pressure up to 40 MPa [see Figure 1 b)].

When positioned in a hazardous area, the electrically heated pressure relief valve shall comply with local safety regulations.

**5.1.5 Heat exchanger** [see Figure 1 b)], with sufficient capacity to heat sample and bypass gas to 90 °C.

When positioned in a hazardous area, the heat exchanger shall comply with local safety regulations.

**5.1.6 Gas meter** (see Figure 1), equipped with a thermometer (5.1.2) and a pressure gauge (5.1.3).

**5.1.7 Barometer**, required for measuring the ambient air pressure.

**5.2 Glass apparatus for dissolution** (see Figure 4), for the dissolution of mercury iodide and consisting of the following.

**5.2.1 Reservoir**, for the solution.

**5.2.2 Graduated receiver**.

**5.2.3 Stop cocks**.

**5.2.4 Three-way valve**.

**5.3 Glass apparatus for charging of silica gel with iodine** (see Figure 5), comprising the following.

**5.3.1 Round bottom flask**, of 2 l capacity.


**5.3.2 Gas inlet tube**.

**5.3.3 Air filter**, filled with a suitable absorbent, such as sulfur-impregnated activated charcoal, to remove mercury from the air.

**5.4 Cold vapour atomic absorption spectrometer (AAS) or atomic fluorescence spectrometer (AFS)**.

A cold vapour technique AAS with background correction capability or an AFS with a mercury unit, capable of detecting at least 1 ng Hg, standard laboratory equipment and polyvinyl acetate (PVA) hoses are required. However, hoses of other suitable plastic material, such as polytetrafluoroethylene (PTFE) or polyamide (PA), may be used.


It is essential to make sure that the flowrate transporting the mercury through the analytical system remains constant.

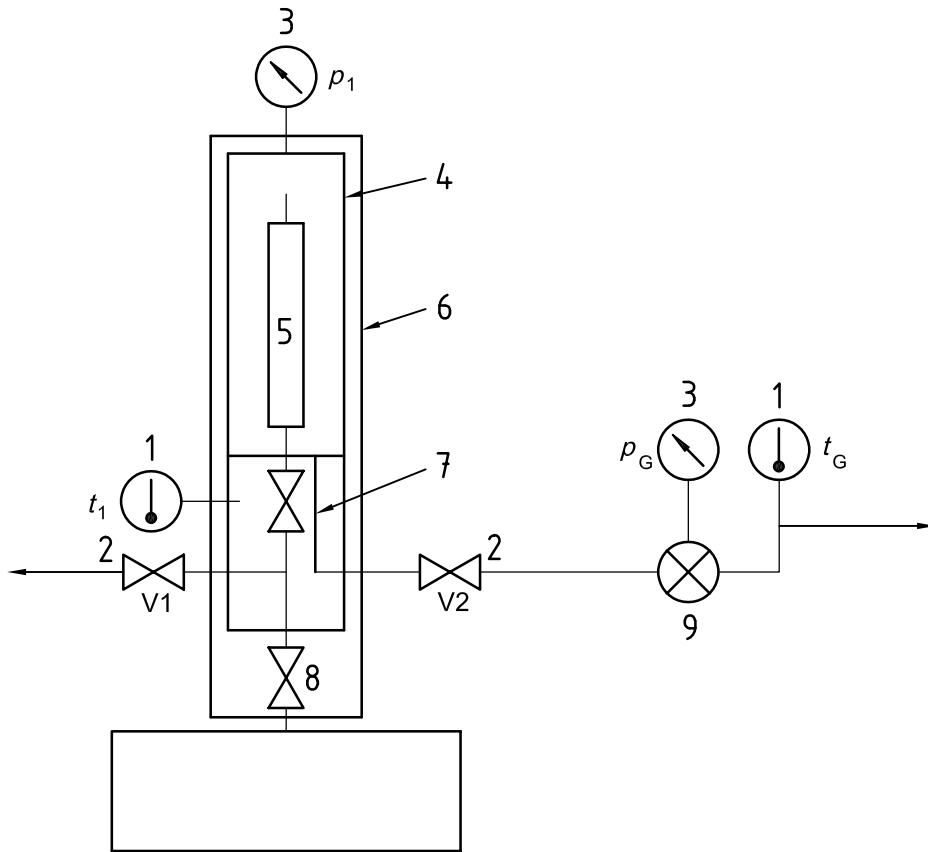

a) Apparatus for pressures up to 10 MPa

**Key**

- |   |                                   |   |                |
|---|-----------------------------------|---|----------------|
| 1 | temperature gauges ( $t_1, t_G$ ) | 6 | insulation     |
| 2 | pressure relief valves (V1, V2)   | 7 | cell valve     |
| 3 | pressure gauges ( $p_1, p_G$ )    | 8 | sampling valve |
| 4 | high-pressure sampling cell       | 9 | gas meter      |
| 5 | sampling tube                     |   |                |

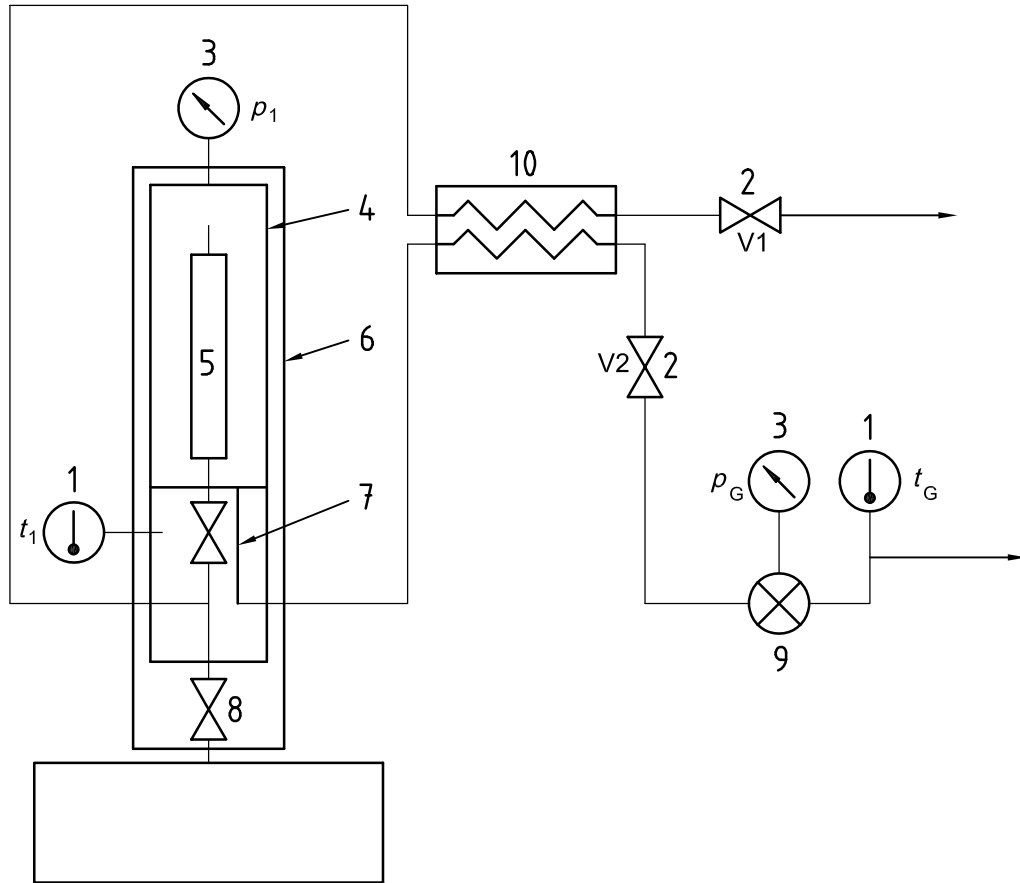


b) Apparatus for pressures up to 40 MPa

**Key**

- |   |                                      |    |                |
|---|--------------------------------------|----|----------------|
| 1 | temperature gauges ( $t_1$ , $t_G$ ) | 6  | insulation     |
| 2 | pressure relief valves (V1, V2)      | 7  | cell valve     |
| 3 | pressure gauges ( $p_1$ , $p_G$ )    | 8  | sampling valve |
| 4 | high-pressure sampling cell          | 9  | gas meter      |
| 5 | sampling tube                        | 10 | heat exchanger |

NOTE See 7.2.

**Figure 1 — High pressure sampling apparatus**

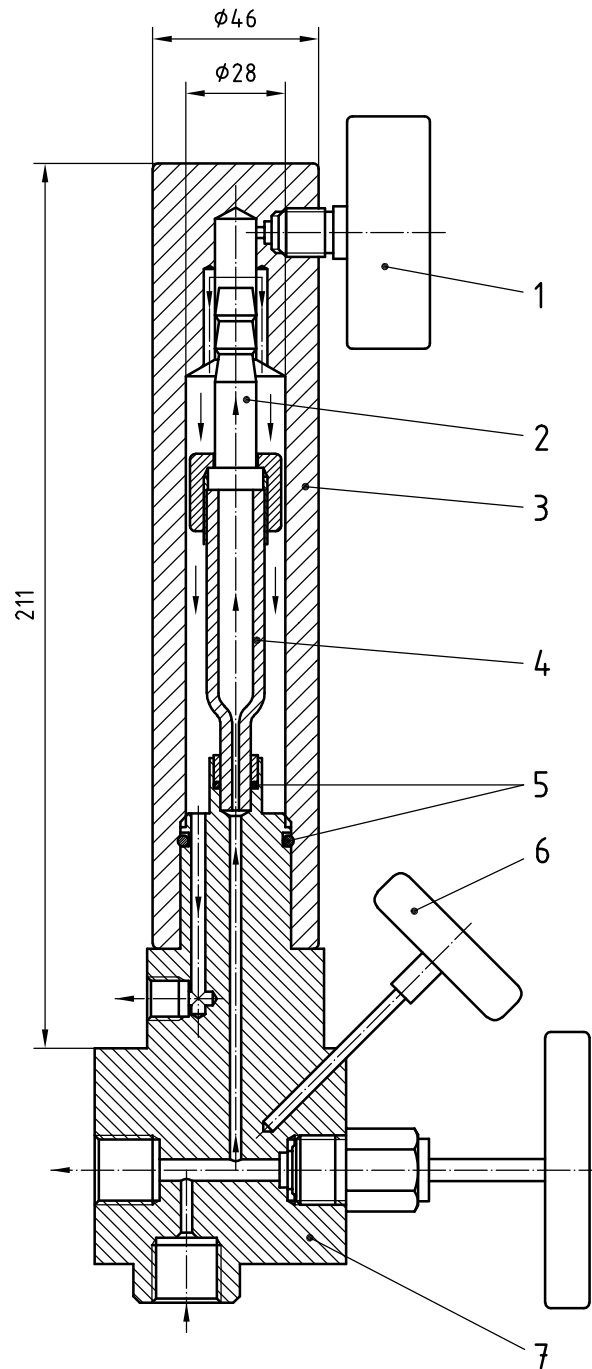

**Key**


- |                           |   |
|---------------------------|---|
| 1 pressure gauge          | 5 O-ring                                    |
| 2 connection tube         | 6 temperature gauge                         |
| 3 high-pressure cell body | 7 bottom part of cell with integrated valve |
| 4 sampling tube           |   |

NOTE See 7.2.

**Figure 2 — High-pressure sampling cell**




Dimensions in millimetres

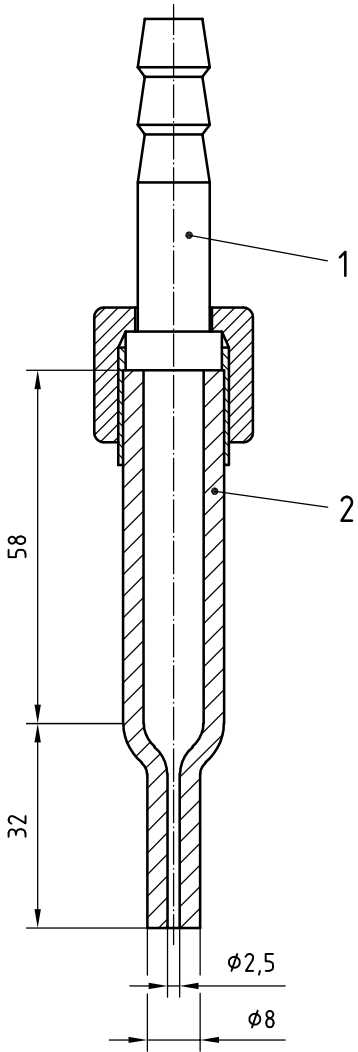

- Key**  
1 connection tube  
2 sampling tube

NOTE See 7.2.

Figure 3 — Sampling tube (borosilicate glass)

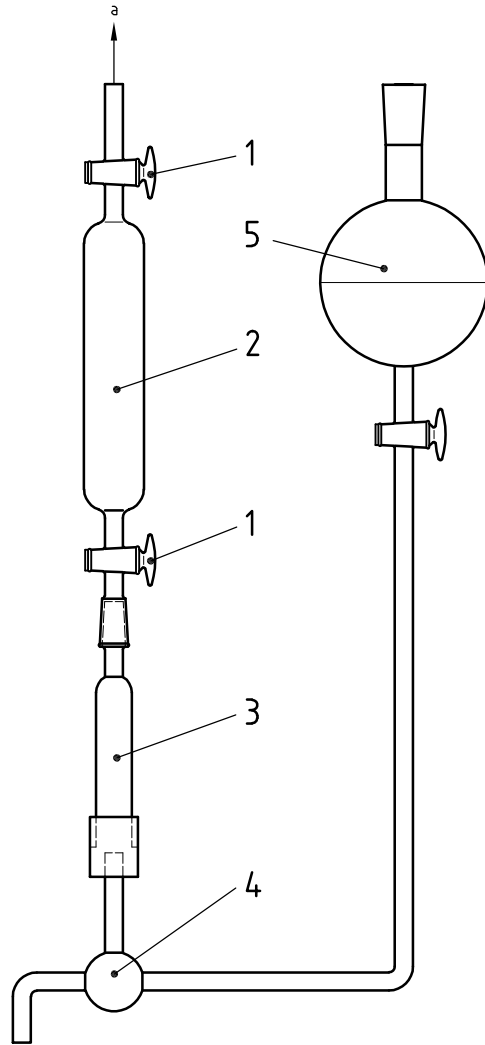


**Key**

- 1 stop cock
- 2 graduated receiver
- 3 sampling tube
- 4 three-way valve
- 5 round-bottom reservoir

a To vacuum.

**Figure 4 — Glass apparatus for dissolution**

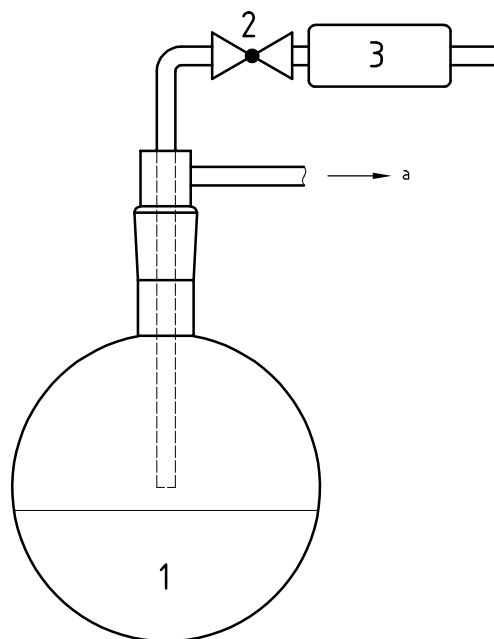**Key**

- 1 round-bottom flask (2 l)
- 2 glass valve
- 3 air filter, filled with activated carbon
- a To vacuum.

**Figure 5 — Glass apparatus for charging silica gel with iodine**

## 6 Reagents

**6.1 Water**, distilled, containing less than 1 µg/l of Hg.

**6.2 Reagents for chemisorption.**

**6.2.1 Iodine** ( $I_2$ ).

**6.2.2 *n*-Pentane.**

**6.2.3 Iodine-laden silica gel**, having a grain size of 0,2 mm to 0,5 mm and prepared as follows.

In a 2-l round bottom flask (5.3.1), dissolve 12 g of iodine (6.2.1) in 1 l of *n*-pentane (6.2.2). To this solution, add 0,5 kg silica gel in portions under swirling. After a reaction time of some 30 min, fit the flask with the assembly shown in Figure 5 featuring an air filter (5.3.3), filled with sulfur-impregnated activated charcoal or another suitable absorbent material. By drawing air through the filter and flask and occasionally swirling the flask contents, gradually evaporate the *n*-pentane. Finally, evaporate the remaining *n*-pentane at a reduced pressure of approximately 30 hPa by closing the glass valve for a short time. Do not remove *n*-pentane completely so as to avoid evaporating the iodine. Keep the  $I_2$ -laden silica gel in a brown ground-glass container to protect it against light. It then has a shelf life of more than 6 months.

**6.3. Reagents for dissolution.****6.3.1 Iodine** ( $I_2$ ).**6.3.2 Ammonium iodide** ( $NH_4I$ ).**6.3.3 Ammonium iodide solution**,  $c(NH_4I) = 1 \text{ mol/l}$ .**6.3.4 Ammonium iodide/iodine** ( $NH_4I/I_2$ ) **reagent solution**, prepared by first dissolving 10 g of iodine in 1 l of the  $NH_4I$  solution (6.3.3), then diluting this solution tenfold with water (6.1).

Keep both the  $NH_4I/I_2$  reagent solution and the  $NH_4I$  solution in brown flasks to protect them against light. Both solutions then have a shelf life of more than 6 months.

**6.4 Reagents for reduction solution.****6.4.1 Potassium hydroxide** (KOH) **solution**, 15 % by mass.**6.4.2 Tin(II) chloride** ( $SnCl_2$ ).**6.4.3 Reduction solution**, prepared by dissolving, in portions and stirring, 5 g of tin(II) chloride (6.4.2) into 95 g of the potassium hydroxide solution (6.4.1).

This solution may have to be filtered and has a maximum shelf life of two days.

**6.5 Calibration solutions.****6.5.1 Mercury stock solution**, mass concentration  $\rho(Hg) = 1,000 \text{ g/l}$ , traceable to a national or international primary standard in accordance with ISO 14111.**6.5.2 Mercury calibration solution**, prepared by diluting the mercury stock solution (6.5.1) with the  $NH_4I/I_2$  solution (6.3.4) to an appropriate mass concentration suitable for the working range of the instrumentation.

The mercury calibration solution, when kept in brown flasks, will be stable for more than one year.

**7 Sampling**

**DANGER — Mercury presents a health hazard if incorrectly handled. Avoid inhalation of the vapour.**

**SAFETY PRECAUTIONS — Sampling shall follow all relevant safety regulations in accordance with ISO 10715. All the equipment used should comply with the specific local safety regulations.**

**7.1 General****7.1.1 Precautions**

In natural gas, mercury is found at extremely low concentration levels. Consequently, to determine mercury at such low levels, it is necessary to take certain precautions in order to obtain reliable results. Such trace analysis is strongly affected by the following:

- the sorption of mercury by the sampling equipment, resulting in false, lower levels of mercury;
- background mercury contamination within the equipment and chemicals or of the air in the laboratory, resulting in false, higher levels of mercury.

Therefore, it is necessary to check all the equipment and chemicals used in the method prior to use.

Mercury is easily sorbed by most materials commonly available for sampling. Therefore, to obtain acceptable results, use quartz glass, borosilicate glass and stainless steel. Depending on the length of the lines, the material used and the flowrate, preconditioning of the sampling system is recommended. For the transfer of mercury vapour to the spectrometer, polyvinyl acetate (PVA) hose connections are recommended. However, other suitable plastics, for instance polytetrafluoroethylene (PTFE) or polyamide (PA), may be used.

### 7.1.2 Conditions for representative sampling

For general aspects of natural gas sampling, see ISO 10715.

Due to the sorption phenomena mentioned in 7.1.1, only perform direct sampling.

Purge the sampling system (sample probe and sampling valve) prior to sampling so as to remove any deposits or impurities. Avoid any excessive purging because it can possibly cause the sampling valve to freeze as a result of gas expansion (Joule-Thomson effect).

The sampling and transfer lines should be as short as possible.

It is strongly recommended to use a fast loop to bypass the sorption tube. This guarantees high gas velocity in the sampling system (sample probe and sampling valve) and minimizes any sorption phenomena.

### 7.1.3 Sampling at high pressure

High-pressure sampling (above atmospheric pressure) allows a rather large volume of gas to be passed through the sampling tube in a short time without changing the pressure and temperature of the gas. This may also prevent retrograde condensation of hydrocarbons. Heat exchangers are required to heat the gas prior to pressure reduction so that the gas sample volume can be measured accurately; the bypass should be reintroduced either to a low-pressure pipeline or to a flared and/or vented outlet for safety reasons.

### 7.1.4 Applicability

This sampling method is suitable for the determination of mercury content in the range of 0,1  $\mu\text{g}/\text{m}^3$  to 5 000  $\mu\text{g}/\text{m}^3$  in natural gas. The sampled gas volume shall contain less than 20 mg hydrogen sulfide ( $\text{H}_2\text{S}$ ) (absolute content) and less than 10  $\text{g}/\text{m}^3$  liquid hydrocarbon condensate determined in accordance with ISO 6570 under the sampling conditions.

## 7.2 Sampling procedure (see Figures 1 and 2)

Carry out direct sampling (i.e. discontinuously) in accordance with ISO 10715 at operating pressure.

Open the sampling valve (see Figure 1) to blow out any deposits or impurities. Take care to prevent excessive blowing out, otherwise the Joule-Thomson effect can cause the valve to ice up.

Keep the sample line to the high-pressure sampling cell (see Figure 1) as short as possible to prevent losses by adsorption on the inside surface of the sampling line as well as by a temperature drop.

Connect the bottom part of the high-pressure sampling cell (see Figure 2) in such a way so as to fix it in a vertical position. If tube connections are required, use stainless steel tubing.

After replacing the screw cap on the sampling tube (see Figure 3) by a connecting tube, insert the sampling tube into the bottom part of the cell (see Figure 2), where it is sealed by an O-ring. Screw the high-pressure cell body (see Figure 2) onto the bottom part and tighten it by hand (O-ring seal).

To prevent condensation and icing-up of the pressure relief valves (see Figure 1), heat the pressure relief valve [for sampling pressure up to 10 MPa, see Figure 1 a)], or heat the gas using a heat exchanger [see Figure 1 b)] upstream to the pressure relief valves, which are connected by two lines (NiMo16Cr15W steel, material No. 2.4819 as specified by the Steel Code, or PTFE-coated high-pressure hoses) to the high-pressure sampling cell [for sampling pressure up to 40 MPa, see Figure 1 b)].

When the temperature of the heated relief valves has reached approximately 50 °C, or the temperature  $t_2$  of the heat exchanger has reached approximately 90 °C, gradually open the sampling valve and the pressure relief valve V1 (see Figure 1). Depending on the diameter and length of the sampling line and the upstream pressure, adjust the volumetric flow from the system through the bypass to 10 m<sup>3</sup>/h.

The sampling nozzle with the sampling valve (see Figure 1) and the bottom part of the cell (see Figure 2) become heated to the temperature of the gas. Measure the temperature  $t_1$  using the temperature gauge (see Figure 1). When a constant temperature has been reached (i.e. the measured drift is less than 2 K/10 min), begin sampling.

Pressurize the sampling cell, by gradually opening the cell valve (see Figure 1). Take care not to open the valve too quickly, as this may cause the sampling tube to burst.

Then check the system for tightness by performing a bubble leak test. Replace the O-ring in the bottom part of the cell, if it leaks. If the gas temperature is higher than the ambient temperature during sampling, insulate the entire high-pressure sampling cell and the sampling valve including the sampling nozzle with adequate insulation material.

It is recommended to carry out the procedure once before sampling begins to pre-heat the sampling cell. Discard the sampling tube used for this purpose.

Take a pressure reading  $p_1$  at the pressure gauge (see Figure 1).

Record the initial value  $V_i$  at the gas meter (see Figure 1), then adjust the pressure relief valve V2 to give the following gas flow:

- for system pressures of  $p > 6,0$  MPa      gas flow = 6 m<sup>3</sup>/h to 8 m<sup>3</sup>/h
- for system pressures of  $p \leq 6,0$  MPa      gas flow = numerical value of  $p$  in m<sup>3</sup>/h

Take readings at the gas meter for the gas temperature  $t_G$  and the gauge pressure  $p_G$  at regular intervals. At minimum, take readings at the beginning and at the end of sampling.

At the same time, take a reading at the barometer of the ambient pressure  $p_a$ .

Once the required sampling volume (0,15 m<sup>3</sup> to 2 m<sup>3</sup>) has passed through the system, gradually close the cell valve (see Figure 1) and take the final reading  $V_f$  at the gas meter.

After each sampling procedure, replace the sampling tube with a new, clean tube as quickly as possible so as to avoid heat loss.

If the absorption layer inside the sampling tube is almost fully discoloured during the sampling, i.e. the iodine has evaporated or the sampling tube is saturated, insert a new sampling tube and repeat the procedure using a smaller sample volume.

### 7.3 Sample treatment

Fix the sampling tube in the dissolution apparatus (see Figure 4). Evacuate the sampling tube through the upper stop cock of the graduated 50 ml receiver using a vacuum pump and keeping the three-way valve closed. After closing the lower stop cock of the graduated receiver, open the three-way valve to allow all the silica gel in the sampling tube to come into full contact with the NH<sub>4</sub>I/I<sub>2</sub> solution fed from the round-bottom reservoir.

Slightly open the lower stop cock of the graduated receiver so as to draw the NH<sub>4</sub>I/I<sub>2</sub> solution into the graduated receiver. Allow 50 ml of this solution to flow through the sampling tube into the receiver within approximately 10 min.

During this process, keep the upper stop cock of the graduated receiver connected to the vacuum pump open. Owing to the vacuum still present, the absorbed hydrocarbons are mostly evaporated, avoiding any adverse effect on subsequent testing.

Close both stop cocks of the graduated receiver and the three-way valve and remove the connections. Shake the receiver containing the  $\text{NH}_4\text{I}/\text{I}_2$  solution a few times and transfer the contents to a brown sample flask.

## 8 Mercury determination

**WARNING — Mercury presents a health hazard if incorrectly handled. Avoid inhalation of the vapour.**

### 8.1 Transfer of mercury to AAS or AFS instrument

Perform the analytical determination using an AAS (5.4) with background correction capability or an AFS (5.4) instrument with a reduction unit. Batch, flow injection and continuous flow methods may be used as specified in the following procedure.

Pour 20 ml of a potassium hydroxide solution (6.4.1) and 20 ml of water (6.1) into the reduction receptacle of the mercury unit of the AAS or AFS instrument. Then add 10  $\mu\text{L}$  to 1 000  $\mu\text{L}$  of the sample solution. Ensure the mercury content remains within the linear range of the AAS or AFS. Dilute samples with a higher mercury content with the  $\text{NH}_4\text{I}/\text{I}_2$  solution (6.3.4).

Add 1,25 ml of the reduction solution (6.4.3) in order to reduce the mercury complex to elemental mercury. Strip off the mercury with inert gas and use the AAS or AFS instrument for detection. When using the flow injection and continuous flow system, use the same reduction solution. The presence of condensate in the solution may influence the mercury determination unless background correction is used with AAS.

### 8.2 Calibration

Calibrate the integrator of the AAS or AFS instrument by analysing known amounts of mercury calibration solution (6.5.2) in the same way as described in 8.1.

Repeat this procedure until the relative standard deviation for three consecutive measurements is less than 3 %. At least two calibrations at different levels within the measuring range are necessary for a first order calibration curve passing through the origin and at least three calibrations for curves not passing through the origin.

The appropriate response factor for the measured signal of the sample is derived from the calibration curve.

The measured signal for the mercury calibration solution may be used to construct control charts for the purpose of indicating whether the equipment and the method are working satisfactorily.

### 8.3 Blank test

Reagents used can contain traces of mercury. Correct the values of the sample by subtracting a blank from the determined total mercury. Check the blank value for each new batch of reagents used. Use the same procedure as described in 7.3 and 8.1 using at least three unused sampling tubes. The blank should contain less than 1  $\mu\text{g}/\text{l}$  of Hg in the final solution used for the determination specified in 8.1.

## 9 Calculation

Calculate the mass, expressed in nanograms, of mercury,  $m_{\text{Hg}}$ , collected on the sampling tube using Equation (1):

$$m_{\text{Hg}} = \frac{A \times V_1}{R_f \times V_2} \quad (1)$$

where

$A$  is the integrated signal, expressed in arbitrary units, indicated by the AAS or AFS;

$R_f$  is the response factor, expressed in arbitrary units per nanogram, derived from the calibration curve;

$V_1$  is the volume, expressed in millilitres, of the total sample solution;

$V_2$  is the volume, expressed in millilitres, of the measured sample solution.

Correct the mass of mercury for reagent contribution using Equation (2):

$$m_{\text{Hg,corr}} = m_{\text{Hg}} - m_{\text{blank}} \quad (2)$$

where

$m_{\text{Hg,corr}}$  is the corrected mass, expressed in nanograms, of mercury in the sample;

$m_{\text{blank}}$  is the mass, expressed in nanograms, of mercury in the blank, calculated according to Equation (1).

Calculate the gas volume sampled, expressed in litres,  $V_G$ , at 273,15 K and 1 013,25 hPa using Equation (3):

$$V_G = \frac{(V_f - V_i) \times (p_a + p_G) T_N}{p_N (T_N + t_G)} \quad (3)$$

where

$V_f$  is the final volume reading, expressed in litres, of the gas meter;

$V_i$  is the initial volume reading, expressed in litres, of the gas meter;

$p_a$  is the ambient air pressure, expressed in hectopascals;

$p_G$  is the gauge pressure, expressed in hectopascals, of the gas meter (averaged for duration of sampling);

$t_G$  is the gas temperature, expressed in degrees Celsius, inside the gas meter (averaged for duration of sampling);

$T_N$  is the normal temperature equal to 273,15 K;

$p_N$  is the normal pressure equal to 1 013,25 hPa.

Calculate the mercury content as mass concentration,  $\beta_{\text{Hg}}$ , expressed in nanograms per litre (ng/l), and equal to micrograms per cubic metre ( $\mu\text{g}/\text{m}^3$ ) at normal conditions according to Equation (4):

$$\beta_{\text{Hg}} = \frac{m_{\text{Hg,corr}}}{V_G} \quad (4)$$



## 10 Precision

### 10.1 General

The precision of the method, as obtained by statistical examination of interlaboratory test results, is as follows.

### 10.2 Repeatability and reproducibility

#### 10.2.1 Repeatability

Little statistical data is available. However, it is expected that replicate test results, obtained by the same operator with the same apparatus under constant operating conditions on identical test gas would be expected to be  $\pm 3\%$  (95 % confidence limits).

#### 10.2.2 Reproducibility

Little statistical data is available. However, it is expected that two single and independent replicate results, obtained by different operators working in different laboratories on identical test gas, under normal and correct operation of the test method, would be expected to be  $\pm 7\%$  (95 % confidence limits).

### 10.3 Uncertainty

The uncertainty based on interlaboratory comparison of measurements of the amount of mercury in the sample solution is typically better than  $\pm 20\%$ , including both bias and uncertainty of measurement.

## 11 Test report

The test report shall include the following information:

- a reference to this part of ISO 6978, i.e. ISO 6978-1.
- the date and time of sampling;
- the place where the sample was taken;
- the conditions of the sampled gas, e.g. temperature, pressure, throughput;
- the sampling method;
- the analytical method (AAS or AFS instrument);
- the total mercury content, expressed in micrograms per cubic metre ( $\mu\text{g}/\text{m}^3$ ), with calculated uncertainty in accordance with the GUM;
- the calibration data;
- the corresponding blank measurement;
- any unusual features noted during sampling and determination.

## Bibliography

- [1] ISO 6978-2:2003, *Natural gas — Determination of mercury — Part 2: Sampling of mercury by amalgamation on gold/platinum alloy*



---

---

## BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

### Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover.  
Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

### Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001.  
Fax: +44 (0)20 8996 7001. Email: [orders@bsi-global.com](mailto:orders@bsi-global.com). Standards are also available from the BSI website at <http://www.bsi-global.com>.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

### Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre.  
Tel: +44 (0)20 8996 7111. Fax: +44 (0)20 8996 7048. Email: [info@bsi-global.com](mailto:info@bsi-global.com).

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.  
Tel: +44 (0)20 8996 7002. Fax: +44 (0)20 8996 7001.  
Email: [membership@bsi-global.com](mailto:membership@bsi-global.com).

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsi-global.com/bsonline>.

Further information about BSI is available on the BSI website at <http://www.bsi-global.com>.

### Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright & Licensing Manager.  
Tel: +44 (0)20 8996 7070. Fax: +44 (0)20 8996 7553.  
Email: [copyright@bsi-global.com](mailto:copyright@bsi-global.com).