

BS EN ISO 10819:2013

Incorporating corrigendum August 2015



BSI Standards Publication

**Mechanical vibration and
shock — Hand-arm vibration —
Measurement and evaluation
of the vibration transmissibility
of gloves at the palm of the
hand**

bsi.

...making excellence a habit.™

National foreword

This British Standard is the UK implementation of EN ISO 10819:2013. It supersedes BS EN ISO 10819:1997 which is withdrawn.

The UK participation in its preparation was entrusted by Technical Committee GME/21, Mechanical vibration, shock and condition monitoring, to Subcommittee GME/21/6, Mechanical vibration, shock and condition monitoring - Human exposure to mechanical vibration and shock.

A list of organizations represented on this subcommittee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2015.

Published by BSI Standards Limited 2015

ISBN 978 0 580 84205 4

ICS 13.160; 13.340.40; 17.160

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 July 2013.

Amendments/corrigenda issued since publication

Date	Text affected
31 August 2015	Implementation of CEN Correction Notice 7 August 2013: the Foreword now contains information regarding the background of the project

English Version

Mechanical vibration and shock - Hand-arm vibration - Measurement and evaluation of the vibration transmissibility of gloves at the palm of the hand (ISO 10819:2013)

Vibrations et chocs mécaniques - Vibrations main-bras -
Mesurage et évaluation du facteur de transmission des
vibrations par les gants à la paume de la main (ISO
10819:2013)

Mechanische Schwingungen und Stöße - Hand-Arm-
Schwingungen - Verfahren für die Messung und Bewertung
der Schwingungsübertragung von Handschuhen in der
Handfläche (ISO 10819:2013)

This European Standard was approved by CEN on 29 May 2013.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

This document (EN ISO 10819:2013) has been prepared by Technical Committee ISO/TC 108 "Mechanical vibration, shock and condition monitoring" in collaboration with Technical Committee CEN/TC 231 "Mechanical vibration and shock" the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by January 2014, and conflicting national standards shall be withdrawn at the latest by January 2014.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN ISO 10819:1996.

This document has been prepared under a mandate given to CEN by the European Commission and the European Free Trade Association, and supports essential requirements of EU Directive.

For relationship with EU Directive, see informative Annex ZA, which is an integral part of this document.

The main changes to the first edition EN ISO 10819:1996 are stronger criteria for antivibration gloves and the addition of a method for measuring the material thickness.

To place anti-vibration gloves on the market of the European Union (EU), manufacturers or their authorised representatives established within the EU shall make sure that they cover all Basic Health and Safety Requirements (BHSRs) applicable to their products under the foreseeable conditions of use for which such Personal Protective Equipment (PPE) is intended (EU Directive 89/686/EEC on PPE). If the relevant harmonized European Standards do not cover all applicable BHSRs they have, in addition to the application of these standards, to assess the conformity to those BHSRs not covered by using other relevant technical specifications and test methods.

This European Standard EN ISO 10819 is intended to confirm the vibration reducing properties of gloves placed on the EU market as anti-vibration gloves.

To mark anti-vibration gloves with the CE conformity mark they must also satisfy the BHSRs of the PPE Directive using harmonised European Standards, such as EN 388 and EN 420. As such, manufacturers or their authorised representatives established within the EU shall make an application for type-examination to an approved inspection body (notified body).

According to the CEN-CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

Endorsement notice

The text of ISO 10819:2013 has been approved by CEN as EN ISO 10819:2013 without any modification.

Annex ZA
(informative)
**Relationship between this European Standard and the Essential
Requirements of EU Directive 89/686/EEC**

This European Standard has been prepared under a mandate given to CEN by the European Commission and the European Free Trade Association to provide one means of conforming to Essential Requirements of the New Approach Directive 89/686/EEC on Personal protective equipment.

Once this standard is cited in the Official Journal of the European Union under that Directive and has been implemented as a national standard in at least one Member State, compliance with the normative clauses of this standard confers, within the limits of the scope of this standard, a presumption of conformity with the corresponding Essential Requirements of that Directive and associated EFTA regulations.

WARNING Other requirements and other EU Directives may be applicable to the products falling within the scope of this standard.

Contents

Page

Foreword	v
Introduction	vi
1 Scope	1
2 Normative references	1
3 Terms and definitions	2
4 Symbols and abbreviations	2
5 Measuring principle and equipment	3
5.1 General principle and setup.....	3
5.2 Measuring equipment.....	4
5.3 Vibration excitation system.....	7
6 Measurement conditions and procedure	8
6.1 Measurement conditions.....	8
6.2 Vibration signal.....	10
6.3 Test procedure.....	11
7 Evaluation of results	13
7.1 Calculation of transmissibility.....	13
7.2 Bare palm adaptor vibration transmissibility.....	15
7.3 Uncorrected glove vibration transmissibility.....	16
7.4 Corrected glove vibration transmissibility.....	16
8 Calculation of statistical values	17
8.1 General.....	17
8.2 One-third-octave vibration transmissibility.....	17
8.3 Frequency-weighted vibration transmissibility.....	18
9 Criteria for designating gloves as antivibration gloves	18
9.1 General.....	18
9.2 Vibration transmissibility of the gloves.....	18
9.3 Construction of the gloves.....	19
10 Test report	21
Annex A (informative) Examples of handles with force and acceleration measuring systems	23
Bibliography	26

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2, www.iso.org/directives.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received, www.iso.org/patents.

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

The committee responsible for this document is ISO/TC 108, *Mechanical vibration, shock and condition monitoring*, Subcommittee SC 4, *Human exposure to mechanical vibration and shock*.

This second edition cancels and replaces the first edition (ISO 10819:1996), of which it constitutes a technical revision. The main changes are stronger criteria for antivibration gloves and the addition of a method for measuring the material thickness.

Introduction

Because of the growing demand to reduce health risks associated with exposure to hand-transmitted vibration, gloves with vibration-reducing materials are often used to attenuate vibration transmitted to the hands. These gloves normally provide little reduction in hand-transmitted vibration at frequencies below 150 Hz. Some gloves can increase the vibration transmitted to the hands at these low frequencies. Gloves with vibration-reducing materials that meet the requirements of this International Standard to be classified as an antivibration glove can be expected to reduce hand-transmitted vibration at frequencies above 150 Hz. These gloves can reduce but not eliminate health risks associated with hand-transmitted vibration exposure.

Field observations indicate that gloves with vibration-reducing materials can result in positive and negative health effects. Positive health effects can occur with gloves that reduce finger tingling and numbness and that keep the hands warm and dry. Negative health effects can occur with gloves that increase the vibration transmitted to the hands at low frequencies and that increase hand and arm fatigue because they increase the hand grip effort required to control a vibrating machine.

Gloves tested in accordance with the requirements of this International Standard are evaluated in a controlled laboratory environment. The actual vibration attenuation of a glove in a work environment can differ from that measured in a controlled laboratory environment.

Vibration transmissibility measurements made in accordance with the requirements of this International Standard are performed only at the palm of the hand. The transmission of vibration to the fingers is not measured. When evaluating the effectiveness of a glove with a vibration-reducing material used to reduce vibration transmitted to the hand, vibration transmission to the fingers should also be assessed. However, research subsequent to the publication of this International Standard is needed to develop a measurement procedure that can be used to measure the vibration transmissibility of gloves at the fingers.

The measurement procedure specified in this International Standard only addresses glove properties that can reduce health risks associated with hand-transmitted vibration in work environments. It does not address glove properties necessary to reduce other hand-related health and safety risks in work environments.

The measurement procedure specified in this International Standard can also be used to measure the vibration transmissibility of a material that is being evaluated for use to cover a handle of a machine or for potential use in a glove.

Mechanical vibration and shock — Hand-arm vibration — Measurement and evaluation of the vibration transmissibility of gloves at the palm of the hand

WARNING — This International Standard defines a screening test procedure for measuring the vibration transmission through gloves with an embedded vibration-reducing material. Many factors not addressed in this International Standard can influence the transmission of vibration through these gloves. Therefore, use the vibration transmissibility values obtained in accordance with this International Standard with caution in the assessment of the vibration-reducing effects of gloves.

1 Scope

This International Standard specifies a method for the laboratory measurement, data analysis, and reporting of the vibration transmissibility of a glove with a vibration-reducing material that covers the palm, fingers, and thumb of the hand. This International Standard specifies vibration transmissibility in terms of vibration transmitted from a handle through a glove to the palm of the hand in one-third-octave frequency bands with centre frequencies of 25 Hz to 1 250 Hz.

The measurement procedure specified in this International Standard can also be used to measure the vibration transmissibility of a material that is being evaluated for use to cover a handle of a machine or for potential use in a glove. However, results from this test cannot be used to certify that a material used to cover a handle meets the requirements of this International Standard to be classified as an antivibration covering. A material tested in this manner could later be placed in a glove. When this is the case, the glove needs to be tested in accordance with the measurement procedure of this International Standard and needs to meet the vibration attenuation performance requirements of this International Standard in order to be classified as an antivibration glove.

NOTE ISO 13753[1] defines a method for screening materials used for vibration attenuation on the handles of machines and for gloves.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 2041, *Mechanical vibration, shock and condition monitoring — Vocabulary*

ISO 5349-1, *Mechanical vibration — Measurement and evaluation of human exposure to hand-transmitted vibration — Part 1: General requirements*

ISO 5805, *Mechanical vibration and shock — Human exposure — Vocabulary*

ISO 8041, *Human response to vibration — Measuring instrumentation*

IEC 61260, *Electroacoustics — Octave-band and fractional-octave-band filters*

EN 388, *Protective gloves against mechanical risks*

EN 420, *Protective gloves — General requirements and test methods*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 2041, ISO 5805 and the following apply.

3.1 glove vibration transmissibility
ratio of the acceleration measured on the palm adaptor of the gloved hand to the acceleration measured on the instrumented handle

Note 1 to entry: Glove vibration transmissibility values greater than 1 indicate that the glove amplifies the vibration, and values lower than 1 indicate that the glove attenuates the vibration.

4 Symbols and abbreviations

The following symbols and abbreviations are used.

$a_{h(Pb)}(f_i)$	unweighted r.m.s. acceleration measured on the bare adaptor in the i th one-third-octave band
$a_{h(Pbx,y,z)}(f_i)$	value of $a_{h(Pb)}(f_i)$ on three mutually orthogonal axes, respectively
$a_{h(Pg)}(f_i)$	unweighted r.m.s. acceleration measured on the palm adaptor of the gloved hand in the i th one-third-octave band
$a_{h(Pgx,y,z)}(f_i)$	value of $a_{h(Pg)}(f_i)$ on three mutually orthogonal axes, respectively
$a_{h(S)}(f_i)$	unweighted r.m.s. acceleration for spectrum S in the i th one-third-octave band
$a_{hw(S)}(f_i)$	frequency-weighted r.m.s. acceleration for spectrum S in the i th one-third-octave band
$a_R(f_i)$	unweighted r.m.s. acceleration measured at the reference position on the handle in the i th one-third-octave band
$C_{V,T}(f_i)$	coefficient of variation for the corrected handle-gloved hand transmissibility in the i th one-third-octave band
$C_{V,T}(S)$	coefficient of variation for the handle-gloved ISO-weighted hand transmissibility for spectrum S
f_i	centre frequency of the i th one-third-octave band
H	subscript representing one-third-octave frequency bands from 200 Hz to 1 250 Hz
i_L	frequency band number of the lowest one-third-octave band associated with each spectrum S according to Table 2
i_U	frequency band number of the uppermost one-third-octave band associated with each spectrum S according to Table 2
M	subscript representing one-third-octave frequency bands from 25 Hz to 200 Hz
S	spectrum, $S = S_M$ or S_H
$s_T(f_i)$	standard deviation for the corrected handle-gloved hand transmissibility in the i th one-third-octave band
$s_T(S)$	standard deviation for the handle-gloved ISO-weighted hand transmissibility for spectrum S
$T_b(f_i)$	handle-adaptor bare adaptor transmissibility in the i th one-third-octave band
$T_g(f_i)$	handle-gloved hand transmissibility in the i th one-third-octave band

$T_{b(S)}$	handle-adaptor bare adaptor ISO weighted transmissibility for spectrum S
$T_{g(S)}$	uncorrected handle-gloved hand ISO weighted transmissibility for spectrum S
$T(f_i)$	corrected handle-gloved hand transmissibility in the i th one-third-octave band
$T_{(S)}$	corrected handle-gloved ISO weighted hand transmissibility for spectrum S
$\bar{T}(f_i)$	mean value for the corrected handle-gloved hand transmissibility in the i th one-third-octave band
$\bar{T}_{(S)}$	mean value for the handle-gloved ISO-weighted hand transmissibility for spectrum S
W_{hi}	ISO frequency-weighting factor specified in ISO 5349-1 for the i th one third-octave frequency band associated with each spectrum S

5 Measuring principle and equipment

5.1 General principle and setup

The method specified in this International Standard is used to measure the vibration input to a gloved hand that is transmitted through the glove at the palm of the hand, which grips and pushes on an instrumented handle. The glove vibration transmissibility (3.1) measured at the palm is used as an index to judge the vibration-reducing effectiveness of the glove. A vibration excitation system (normally an electromechanical shaker) shall be used to generate the required vibration input. The vibration in the direction of the excitation shall be simultaneously measured at the middle point of the top of the instrumented handle (see [Annex A](#)) and between the palm of the hand and glove by means of a palm adaptor. The adaptor shall contain an accelerometer and shall be placed inside the glove between the hand and handle. To compensate for the frequency response of the palm adaptor, the glove vibration transmissibility is calculated as the ratio of the vibration transmissibility values at the palm of the hand with a glove, as measured with the palm adaptor, divided by the corresponding transmissibility values associated with the bare palm adaptor attached to the handle.

A schematic drawing of a recommended vibration measurement setup is shown in [Figure 1](#). The acceleration at the reference point in the instrumented handle, $a_R(f_i)$, and the vibration at the palm of the hand, $a_{h(Pb)}(f_i)$ or $a_{h(Pg)}(f_i)$, shall be measured simultaneously. [Annex A](#) shows examples of instrumented handles. The diameter of that part of the instrumented handle that is clasped by the hand shall be $(40 \pm 0,5)$ mm.

The values of the grip and feed forces shall be displayed continuously so the test subject can continually monitor them and consistently apply the required grip and feed forces throughout a test.

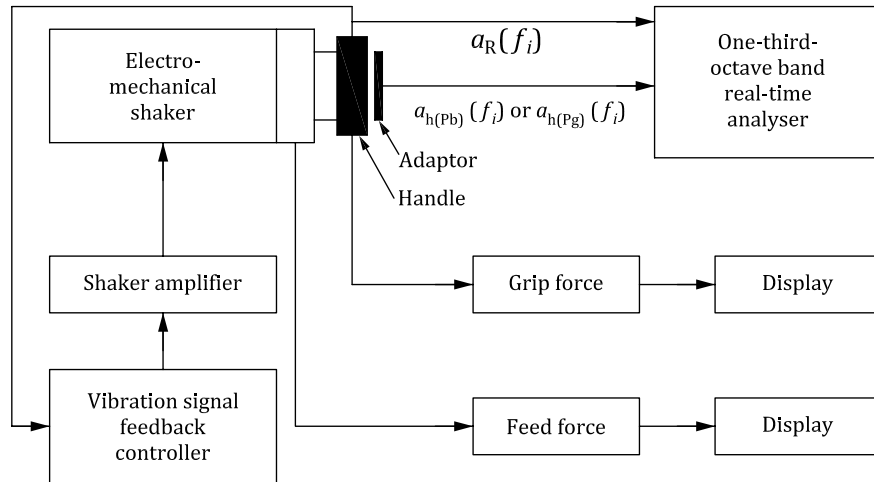


Figure 1 — Schematic diagram for measurement of glove vibration transmissibility

5.2 Measuring equipment

5.2.1 General requirements

A minimum of a two-channel, one-third-octave band real-time frequency analyser and two accelerometers are required.

The elements of the measuring chain shall fulfill the requirements of ISO 8041.


5.2.2 Transducer mounting

5.2.2.1 Mounting at the reference point in the handle

A single-axis accelerometer shall be embedded within the top surface of the test handle that will be in contact with the palm adaptor. The accelerometer shall be placed near the centre of the length of the handle, and its measurement axis shall be parallel to the vibration excitation axis. The exact location of the accelerometer shall be marked on the surface of the handle.

5.2.2.2 Mounting for measurement at the palm of the hand

To measure vibration at the palm of the hand, a palm adaptor shall be used that contains an accelerometer (may be a single axis or triaxial accelerometer) with the dimensions and shape shown in [Figure 2](#). Its mass, which includes the mass of the accelerometer, shall not exceed 15 g. The palm adaptor shall be made of a rigid material, such as wood or hard plastic.

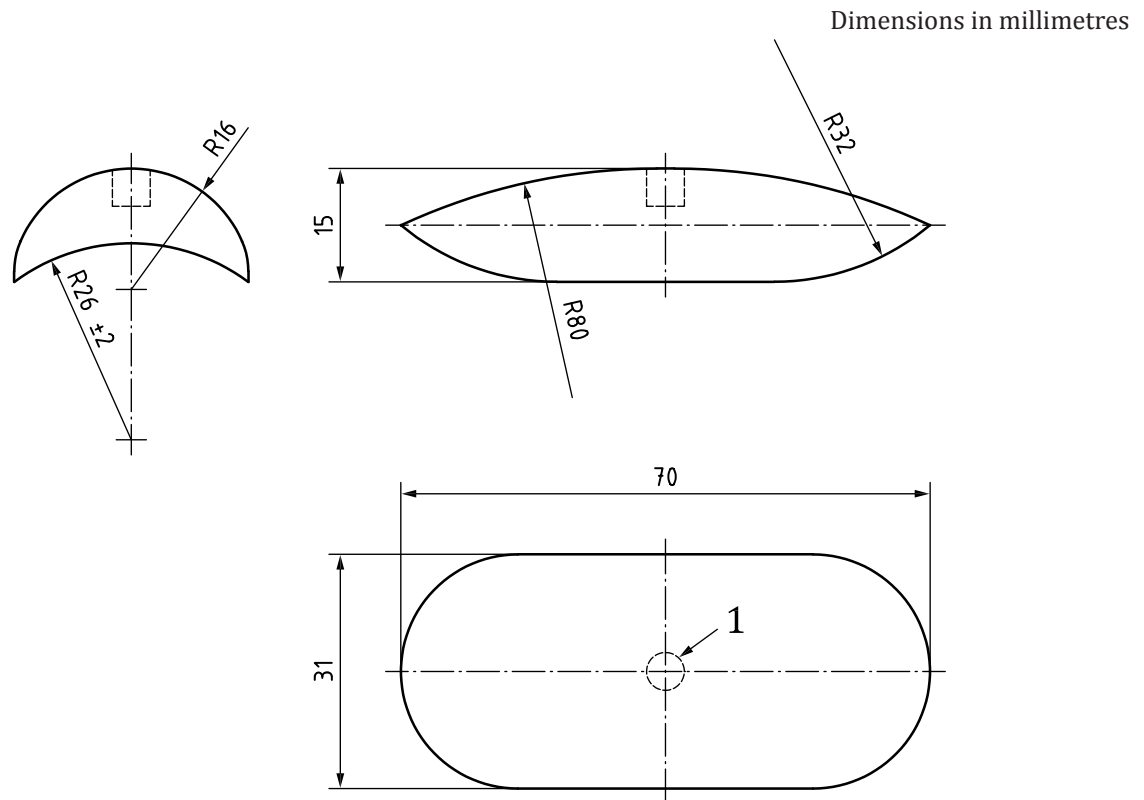

Key

1 accelerometer location

NOTE Unless otherwise specified, all tolerances are $\pm 0,5$ mm.

Figure 2 — Adaptor for holding the accelerometer in the palm of the hand

To ensure measurement accuracy, the calibration consistency of the two accelerometers installed in the handle and the palm adaptor, respectively, shall be checked by affixing the adaptor to the test handle with a contact force of (80 ± 10) N. The adaptor shall be positioned on the surface of the handle as close as possible to the accelerometer installed on the handle (see [Annex A](#)), and the adaptor shall be aligned with the vibration axis of the handle. The palm adaptor shall be held in place by means of a lightweight elastic element (e.g. rubber bands). The measured bare palm adaptor vibration transmissibility shall be within the amplitude range of 0,95 to 1,05 over the one-third-octave frequency range of 25 Hz to 1 250 Hz.


Care should be taken to ensure that the palm adaptor has solid contact with the test handle along a single straight line that runs the length of the adaptor. Deviations from unity transmissibility in excess of ± 5 % can occur when the palm adaptor, which has a radius greater than the test handle radius, does not have good contact with the test handle.

5.2.3 Frequency analyses

Frequency analyses in one-third-octave frequency bands shall be conducted. The one-third-octave band filters shall fulfill the requirements for one-third-octave filters specified in IEC 61260, class 1.

5.2.4 Grip force measuring system

Grip force is the force used to grip the handle along the axis of vibration (see ISO 15230[2]). It is measured according to the scheme shown in [Figure 3](#).

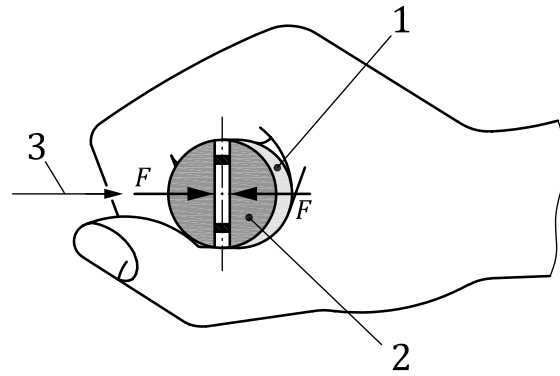

Key

- | | | | |
|---|---------|----------|-------------------|
| 1 | adaptor | 3 | axis of vibration |
| 2 | handle | <i>F</i> | force |

Figure 3 — Grip force to be measured

The grip force shall be measured using the instrumented handle (refer to [Annex A](#)). The grip force measurement system shall fulfill the following requirements:

- a) dynamic range: 10 N to 80 N;
- b) resolution: better than 2 N;
- c) measuring errors: less than 4 N;
- d) integration time for visual display: 0,25 s to 0,50 s.

5.2.5 Feed force measuring system

Feed force means the horizontal force that pushes toward the vibration excitation system along the axis of vibration (see ISO 15230[2]).

The feed force shall be measured using a horizontal force measurement device, which may be a force plate installed on an adjustable platform where the subject stands during the experiment (see [Figure 4](#)) or a force measurement system built into the instrumented handle (refer to [Annex A](#)). The feed force measuring system shall fulfill the following requirements:

- a) dynamic range: 10 N to 80 N;
- b) resolution: better than 2 N;
- c) measuring errors: less than 4 N;
- d) integration time for visual display: 0,25 s to 0,50 s.

6 Measurement conditions and procedure

6.1 Measurement conditions

6.1.1 Test subjects

Five adults with hand sizes between 7 and 10, as specified by EN 420, shall serve as test subjects. The test subjects shall use their dominant hand for the glove vibration transmissibility tests.

6.1.2 Test gloves

Five separate gloves of the same type shall be tested (one glove for each test subject).


6.1.3 Test conditions

For the measurements, the following conditions shall be observed.

- a) Grip force — the grip force shall be displayed continuously. The test subject shall maintain the grip force at (30 ± 5) N throughout the test period.
- b) Feed force — the feed force shall be displayed continuously. The test subject shall maintain the feed force at (50 ± 8) N throughout the test period.
- c) Room temperature — vibration measurements shall take place at a room temperature of (20 ± 5) °C, and the room temperature shall be reported.
- d) Humidity — the relative humidity shall be below 70 % and shall be reported.
- e) Conditioning of gloves — the gloves to be tested shall be stored at the temperature specified in c) for at least 30 min and worn by a test subject for at least 3 min before the test procedure is started.
- f) Fitting of gloves — the size of the gloves shall be chosen according to EN 420.
- g) Vibration measurement averaging time — the averaging time for the vibration tests shall be a minimum of 30 s.

6.1.4 Test subject's posture

The test subject shall clasp the handle with the palm adaptor as shown in [Figure 5](#) for the glove vibration transmissibility tests. The operator shall stand upright on a horizontal surface (floor or platform) as shown in [Figure 4](#). The forearm shall be directed along the axis of vibration. The elbow shall form an angle of $90^\circ \pm 15^\circ$. The elbow shall not touch the body during the measurements. The wrist shall be bent between 0° (neutral) and 40° (dorsal bending) maximum.

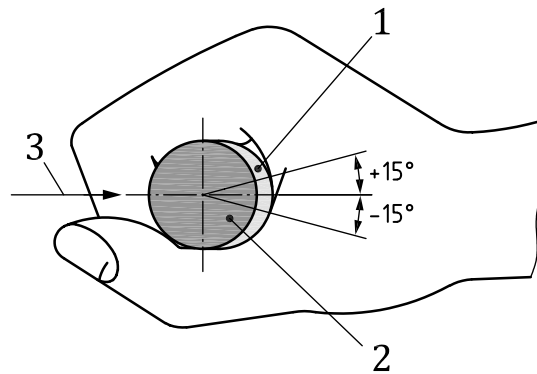

Key

- | | | | | | |
|---|---------|---|--------|---|-------------------|
| 1 | adaptor | 2 | handle | 3 | axis of vibration |
|---|---------|---|--------|---|-------------------|

Figure 5 — Position of hand with handle and adaptor


6.1.5 Position of the palm adaptor in glove vibration transmissibility tests

6.1.5.1 General

The palm adaptor shall be positioned in the gloved hand relative to the handle as shown in [Figure 5](#). The axis of the accelerometer embedded in the adaptor should not deviate from the axis of vibration by more than $\pm 15^\circ$. One of the following procedures shall be used to minimize measurement error associated with misalignment of the palm adaptor on the handle: method 1 with a single axis accelerometer, method 2 with a triaxial accelerometer, or method 1 with a triaxial accelerometer as specified in method 2.

6.1.5.2 Method 1: single axis accelerometer

Place a slit in the seam of the glove between the thumb and index finger so that the palm adaptor can be visually positioned between the palm of the hand and the top of the handle. To facilitate this alignment, place visible marks, as shown in [Figure 6](#), on the top centres of the palm adaptor and the handle.

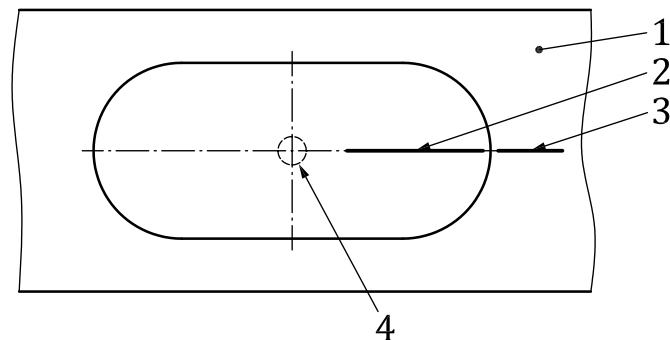


Key

- | | | | |
|---|-----------------------------------|---|-----------------------------|
| 1 | handle | 3 | mark — top centre of handle |
| 2 | mark — top centre of palm adaptor | 4 | accelerometer location |

Figure 6 — Palm adaptor alignment on top of handle

6.1.5.3 Method 2: triaxial accelerometer

Embed a miniature triaxial accelerometer in place of the single axis accelerometer in the palm adaptor ([Figure 7](#)). The palm adaptor acceleration value is the root-sum-squares of the measured acceleration values on the three mutually orthogonal axes shown in [Figure 7](#) [refer to Formulae (3) and (6)].

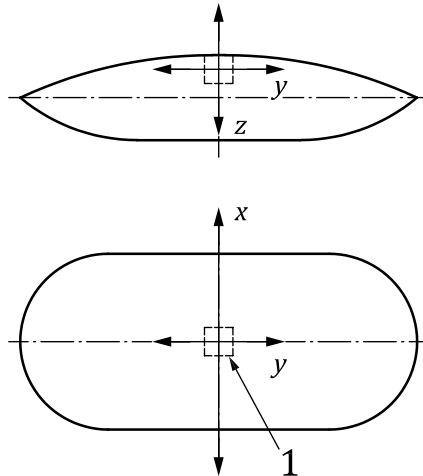


Key

1 accelerometer location x, y, z three mutually orthogonal measurement axes

Figure 7 — Triaxial accelerometer location in palm adaptor

6.2 Vibration signal


The vibration signal measured at the handle is a band-limited random vibration signal. The first part of the signal spectrum (from 25 Hz to 250 Hz) is a constant-velocity (0,012 8 m/s) spectrum. The second part (from 315 Hz to 1 600 Hz) is a ramp-down spectrum. The entire spectrum shall fulfil the requirements specified in [Table 1](#) and [Figure 8](#). The acceleration power spectral density (PSD) is expressed as mean square acceleration per unit frequency bandwidth in $(\text{m/s}^2)^2/\text{Hz}$. The corresponding one-third-octave band acceleration values of the acceleration signal are listed in [Table 1](#) and shown in [Figure 9](#). The frequency-weighted acceleration value of the band-limited random vibration signal is $(4,82 \pm 0,50) \text{ m/s}^2$.

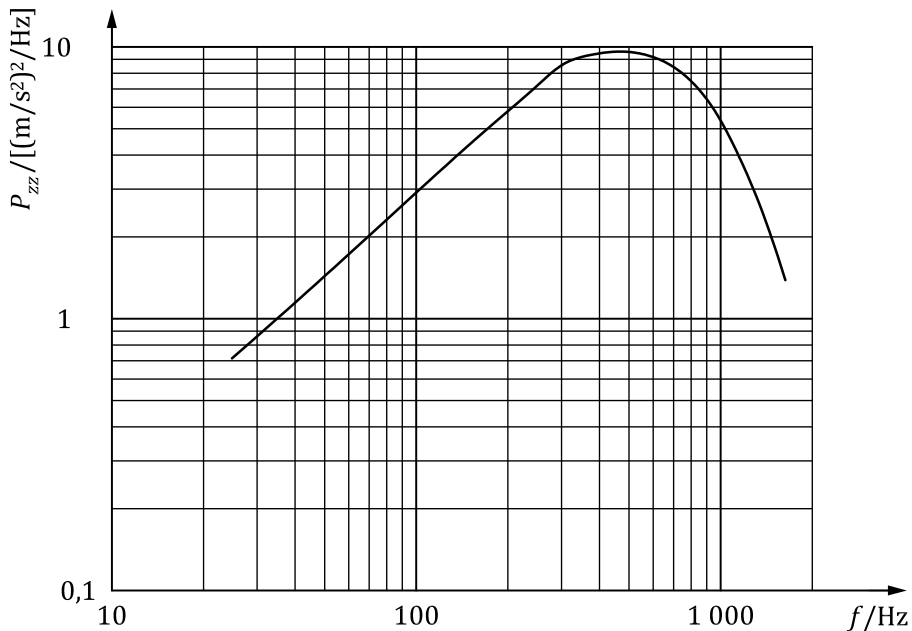

Key

P_{zz} accelerometer power spectral density f frequency

Figure 8 — Handle acceleration power spectral density spectrum

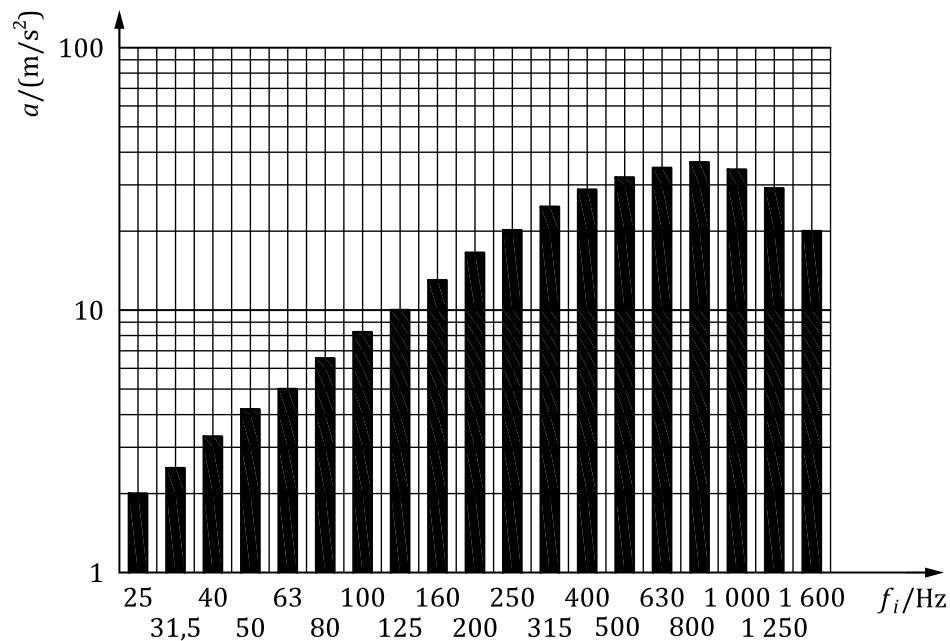

Key

a acceleration f_i one-third-octave-band centre frequency

Figure 9 — One-third-octave band handle acceleration values

6.3 Test procedure

6.3.1 Preparation

The following steps shall be carried out before starting the vibration measurements:

- a) calibrate the accelerometers and measurement system (in accordance with ISO 8041);
- b) condition the gloves as described in 6.1.3 e);
- c) instruct the tests subjects with regard to the test posture in 6.1 and conduct trials so that the test subjects learn to control the feed and grip forces described in 6.1.3 a) and b);
- d) check and adjust the vibration signal to achieve the vibration signal in 6.2.

6.3.2 Measurements with the bare adaptor

One-third-octave band bare palm adaptor acceleration measurements shall be carried out with the palm adaptor attached to the test handle as specified in 5.2.2.2. The hand shall not be used to clasp the test handle with adaptor during these measurements. The one-third-octave band unweighted acceleration values at the handle, $a_R(f_i)$, and on the bare adaptor, $a_{h(Pb)}(f_i)$, shall be measured simultaneously and used to calculate the adaptor transmissibility between the adaptor and handle as specified in 7.2.

If the one-third-octave band bare adaptor transmissibility associated with the unweighted accelerations in any one-third-octave band between 25 Hz and 1 250 Hz is outside the range of 0,95 to 1,05, consider the measurements to be invalid.

Table 1 — Required handle acceleration values

Frequency	Acceleration PSD value	Acceleration tolerance in the one-third octave band	One-third-octave acceleration value
f_i	P_{zz}	dB	m/s ²
Hz	(m/s ²) ² /Hz		
25	0,709	±2	1,98
31,5	0,893	±1	2,45
40	1,134	±1	3,22
50	1,417	±1	4,10
63	1,786	±1	4,85
80	2,268	±1	6,38
100	2,835	±1	8,20
125	3,543	±1	9,81
160	4,535	±1	12,53
200	5,669	±1	16,00
250	7,087	±1	20,14
315	8,521	±1	23,79
400	9,179	±1	28,19
500	9,179	±1	31,59
630	8,555	±1	33,96
800	7,069	±1	35,19
1000	4,994	±1	33,35
1250	2,905	+2 -∞	28,37
1600	1,324	+3 -∞	19,58
Unweighted acceleration			90,19
Frequency-weighted acceleration			4,82
Frequency-weighted acceleration tolerance			± 0,50

6.3.3 Measurements with gloved hand

Using the same adaptor as in 6.3.2, one-third-octave band gloved hand acceleration measurements shall be carried out with each test subject. The one-third-octave band unweighted accelerations obtained at the handle, $a_R(f_i)$, and on the adaptor, $a_{h(Pg)}(f_i)$, shall be measured simultaneously and used to calculate the gloved hand transmissibility as specified in 7.3.

6.3.4 Measurements with resilient material

If the measurement method specified in this International Standard is used to measure the vibration transmissibility of a resilient material, a piece of the material shall be wrapped around the full circumference of the handle. The resilient material shall be attached to the handle with double-sided adhesive tape or other similar adhesive material so the resilient material can be stably held on the handle. The resilient material shall be applied to the handle so as not to preload the grip force transducer in the handle. The resilient material shall then be clasped with the hand with the adaptor placed between the palm of the hand and the material.

6.3.5 Required number of tests

The required number of tests is:

- a) bare palm adaptor vibration transmissibility tests: one test for the adaptor at the beginning of the test day;
- b) glove vibration transmissibility tests: three separate tests for each of the five test subjects.

For each vibration transmissibility test for each test subject, there shall be a minimum 3 min rest period between each test.

If the gloved-hand vibration transmissibility tests for the five test subjects occur over multiple test sessions spread over multiple days, the bare adaptor tests shall be repeated at the beginning of each test day.

7 Evaluation of results

7.1 Calculation of transmissibility

7.1.1 General

Figure 10 is a flow diagram for the bare adaptor and glove vibration transmissibility measurements and the calculations of the mean corrected transmissibility values and related standard deviations and coefficients of variation.

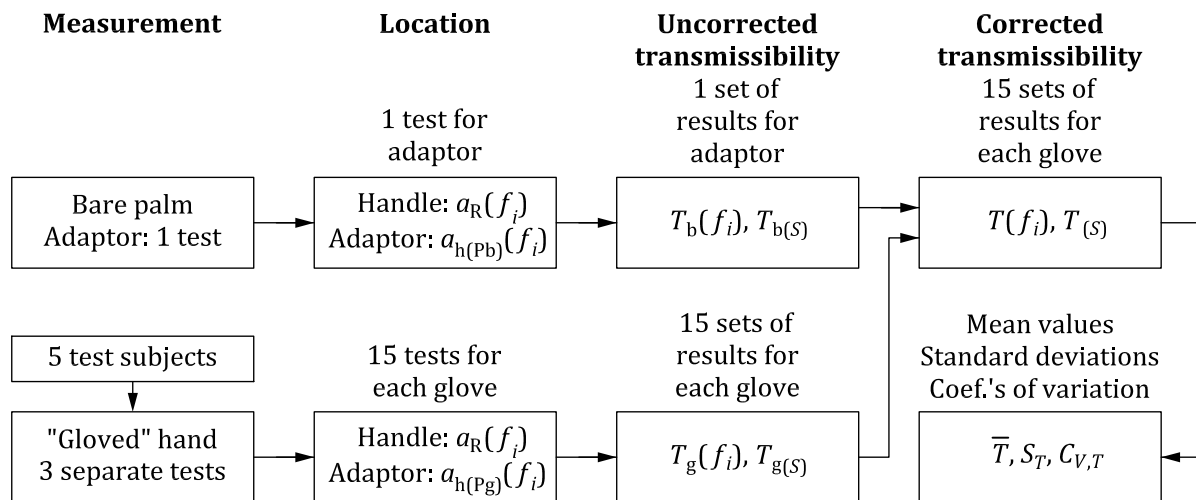


Figure 10 — Flow diagram for determining the mean corrected transmissibility values, standard deviations and coefficients of variation

7.1.2 One-third-octave frequency ranges

The range of one-third-octave centre frequencies for the vibration spectra S_M and S_H shall be:

- a) vibration frequency range Δf_M : 25 Hz to 200 Hz;
- b) vibration frequency range Δf_H : 200 Hz to 1 250 Hz.

7.1.3 Frequency-weighted acceleration values

The frequency-weighted acceleration value, $a_{hw(S)}(f_i)$, in the i th one-third-octave frequency band shall be obtained from:

$$a_{hw(S)}(f_i) = a_{h(S)}(f_i) W_{hi} \quad (1)$$

where

- $a_{h(S)}(f_i)$ is the measured acceleration value in the i th one-third-octave band;
- f_i is the one-third-octave centre frequency for the i th one-third-octave band;
- W_{hi} is the ISO frequency weighting value specified in ISO 5349-1 for the i th one-third-octave frequency band — values for W_{hi} are given in [Table 2](#).

NOTE For the spectrum S_M , S is substituted by M and for the spectrum S_H , S is substituted by H in Formula (1).

Table 2 — Frequency weighting factors W_{hi} for hand-transmitted vibration for conversion of one-third-octave band magnitudes to frequency-weighted magnitudes

Frequency band number	Nominal value of band centre frequency	Weighting factor
i	f_i	W_{hi}
	Hz	
14	25	0,647
15	31,5	0,519
16	40	0,411
17	50	0,324
18	63	0,256
19	80	0,202
20	100	0,160
21	125	0,127
22	160	0,101
23	200	0,079 9
24	250	0,063 4
25	315	0,050 3
26	400	0,039 8
27	500	0,031 4
28	630	0,024 5
29	800	0,018 6
30	1 000	0,013 5
31	1 250	0,008 94

7.2 Bare palm adaptor vibration transmissibility

7.2.1 One-third-octave vibration transmissibility

The bare adaptor vibration transmissibility, $T_b(f_i)$, for the i th one-third-octave band shall be calculated from:

$$T_b(f_i) = \frac{a_{h(\text{Pb})}(f_i)}{a_R(f_i)} \quad (2)$$

where $a_{h(\text{Pb})}(f_i)$ and $a_R(f_i)$ are defined in 6.3.2.

If method 2 in 6.1.5.3 is used to measure $a_{h(\text{Pb})}(f_i)$:

$$a_{h(\text{Pb})}(f_i) = \sqrt{a_{h(\text{Pb}x)}^2(f_i) + a_{h(\text{Pb}y)}^2(f_i) + a_{h(\text{Pb}z)}^2(f_i)} \quad (3)$$

where (refer to Figure 7)

- $a_{h(\text{Pb}x)}(f_i)$ is the value of $a_{h(\text{Pb})}(f_i)$ on the x -axis;
- $a_{h(\text{Pb}y)}(f_i)$ is the value of $a_{h(\text{Pb})}(f_i)$ on the y -axis;
- $a_{h(\text{Pb}z)}(f_i)$ is the value of $a_{h(\text{Pb})}(f_i)$ on the z -axis.

7.2.2 Frequency-weighted vibration transmissibility

The frequency-weighted bare adaptor vibration transmissibility, $T_{b(S)}$, for the S_M and S_H vibration spectra shall be calculated from:

$$T_{b(S)} = \frac{\sqrt{\sum_{i=i_L}^{i_U} [a_{h(\text{Pb})}(f_i) W_{hi}]^2}}{\sqrt{\sum_{i=i_L}^{i_U} [a_R(f_i) W_{hi}]^2}} \quad (4)$$

where

- $a_{h(\text{Pb})}(f_i)$, $a_R(f_i)$ are defined in 6.3.2;
- W_{hi} is defined in Table 2;
- i_L is 14 for $S = S_M$ and 23 for $S = S_H$ (see Table 2);
- i_U is 23 for $S = S_M$ and 31 for $S = S_H$ (see Table 2).

NOTE For the spectrum S_M , S is substituted by M and for the spectrum S_H , S is substituted by H in Formula (4).

7.3 Uncorrected glove vibration transmissibility

7.3.1 One-third-octave vibration transmissibility

The uncorrected glove vibration transmissibility, $T_g(f_i)$, for the i th one-third-octave band shall be calculated from:

$$T_g(f_i) = \frac{a_{h(Pg)}(f_i)}{a_R(f_i)} \quad (5)$$

where $a_{h(Pg)}(f_i)$ and $a_R(f_i)$ are defined in [6.3.3](#).

If method 2 in [6.1.5.3](#) is used to measure $a_{h(Pg)}(f_i)$:

$$a_{h(Pg)}(f_i) = \sqrt{a_{h(Pgx)}^2(f_i) + a_{h(Pgy)}^2(f_i) + a_{h(Pgz)}^2(f_i)} \quad (6)$$

where (refer to [Figure 7](#))

- $a_{h(Pgx)}(f_i)$ is the value of $a_{h(Pg)}(f_i)$ on the x -axis;
- $a_{h(Pgy)}(f_i)$ is the value of $a_{h(Pg)}(f_i)$ on the y -axis;
- $a_{h(Pgz)}(f_i)$ is the value of $a_{h(Pg)}(f_i)$ on the z -axis.

7.3.2 Frequency-weighted vibration transmissibility

The frequency-weighted uncorrected glove vibration transmissibility, $T_g(S)$, for the S_M and S_H vibration spectra shall be calculated from:

$$T_g(S) = \frac{\sqrt{\sum_{i=i_L}^{i_U} [a_{h(Pg)}(f_i) W_{hi}]^2}}{\sqrt{\sum_{i=i_L}^{i_U} [a_R(f_i) W_{hi}]^2}} \quad (7)$$

where

- $a_{h(Pg)}(f_i)$, $a_R(f_i)$ are defined in [6.3.3](#);
- W_{hi} is defined in [Table 2](#);
- i_L is 14 for $S = S_M$ and 23 for $S = S_H$ (see [Table 2](#));
- i_U is 23 for $S = S_M$ and 31 for $S = S_H$ (see [Table 2](#)).

NOTE For the spectrum S_M , S is substituted by M and for the spectrum S_H , S is substituted by H in Formula (7).

7.4 Corrected glove vibration transmissibility

7.4.1 One-third-octave vibration transmissibility

The corrected glove vibration transmissibility, $T(f_i)$, for the i th one-third-octave band shall be calculated from:

$$T(f_i) = \frac{T_g(f_i)}{T_b(f_i)} \quad (8)$$

7.4.2 Frequency-weighted vibration transmissibility

The frequency-weighted corrected glove vibration transmissibility, $T_{(S)}$, shall be calculated from:

$$T_{(S)} = \frac{T_{g(S)}}{T_{b(S)}} \quad (9)$$

NOTE For the spectrum S_M , S is substituted by M and for the spectrum S_H , S is substituted by H in Formula (9). The associated frequency ranges are given in 7.1.2.

8 Calculation of statistical values

8.1 General

The statistical values presented in this clause shall be calculated and reported for all vibration transmissibility tests for each individual test subject (three tests each) and for all five test subjects (15 tests in total).

8.2 One-third-octave vibration transmissibility

The mean value, $\bar{T}(f_i)$, for each corrected one-third-octave vibration transmissibility value is given by:

$$\bar{T}(f_i) = \frac{1}{N} \sum_{j=1}^N T_j(f_i) \quad (10)$$

where

$N = 3$ (three tests for each test subject); or

$N = 15$ (five test subjects with three tests each);

$T_j(f_i)$ are the corrected one-third-octave glove vibration transmissibility values for each individual test.

The standard deviation, $s_T(f_i)$, for the one-third-octave vibration transmissibility values is given by:

$$s_T(f_i) = \sqrt{\frac{1}{N-1} \sum_{j=1}^N [T_j(f_i) - \bar{T}(f_i)]^2} \quad (11)$$

The coefficient of variation, $C_{V,T}(f_i)$, for the one-third-octave vibration transmissibility values is given by:

$$C_{V,T}(f_i) = \frac{s_T(f_i)}{\bar{T}(f_i)} \quad (12)$$

The mean values, standard deviations and coefficients of variation shall be reported

- a) for each individual test subject ($N = 3$); and
- b) for all five test subjects combined ($N = 15$)

for the one-third-octave bands with centre frequencies from 25 Hz to 1 250 Hz.

8.3 Frequency-weighted vibration transmissibility

The mean value, $\bar{T}_{(S)}$, for the corrected frequency-weighted glove vibration transmissibility values is given by:

$$\bar{T}_{(S)} = \frac{1}{N} \sum_{j=1}^N T_{(S)j} \quad (13)$$

where

$N = 3$ (three tests for each test subject); or

$N = 15$ (five test subjects with three tests each);

$T_{(S)j}$ are the corrected frequency-weighted glove vibration transmissibility values for each individual test.

NOTE For the spectrum S_M , S is substituted by M and for the spectrum S_H , S is substituted by H in Formula (13). The associated frequency ranges are given in [7.1.2](#).

The standard deviation, $s_{T(S)}$, for the frequency-weighted transmissibility values is given by:

$$s_{T(S)} = \sqrt{\frac{1}{N-1} \sum_{j=1}^N [T_{(S)j} - \bar{T}_{(S)}]^2} \quad (14)$$

The coefficient of variation, $C_{V,T(S)}$, for the frequency-weighted transmissibility values is given by:

$$C_{V,T(S)} = \frac{s_{T(S)}}{\bar{T}_{(S)}} \quad (15)$$

The mean values, standard deviations and coefficients of variation shall be reported:

- a) for each individual test subject ($N = 3$); and
- b) for all five test subjects combined ($N = 15$)

for $T_{(M)}$ and $T_{(H)}$.

9 Criteria for designating gloves as antivibration gloves

9.1 General

To be designated as an *antivibration glove* according to this International Standard, all the requirements specified in [9.2](#) and [9.3](#) shall be fulfilled.

9.2 Vibration transmissibility of the gloves

The gloved hand mean values $\bar{T}_{(H)}$ and $\bar{T}_{(M)}$ shall meet the requirements:

$$\bar{T}_{(H)} \leq 0,60$$

and

$$\bar{T}_{(M)} \leq 0,90$$

9.3 Construction of the gloves

9.3.1 Glove vibration-reducing material thickness

9.3.1.1 Glove vibration-reducing material thickness in the palm

The thickness of vibration-reducing material placed in the palm section of the glove should not be greater than 8 mm.

NOTE The use of a glove with an embedded vibration-reducing material generally reduces the hand grip strength associated with gripping a machine handle. This requires a greater grip effort to achieve the same level of machine control as is achieved with bare hand operation of the machine. Increased hand-transmitted vibration reduction can often be achieved with thicker vibration-reducing materials. However, a trade-off needs to be made between this increased vibration reduction and the potential negative effects of the thicker materials associated with increased grip effort, reduced finger dexterity and hand comfort, and reduced control while operating a machine.

9.3.1.2 Glove vibration-reducing material in the thumb and fingers

The same vibration-reducing material shall be placed in the palm section and the finger and thumb sections of the glove. The vibration-reducing material shall cover the complete palm area of the hand and shall cover the three phalanges of each finger and the two phalanges of the thumb. The thickness of vibration-reducing material placed in the fingers and thumb sections of the glove shall be equal to or greater than 0,55 times the thickness of the vibration-reducing material placed in the palm section of the glove.

NOTE An antivibration glove that meets the vibration transmissibility requirements of this International Standard can also potentially be too stiff, bulky, and uncomfortable to wear and use if the same thickness of vibration-reducing material is used in the palm section and the finger and thumb sections of the glove. Using a thinner vibration-reducing material of the same type used in the palm section in the finger and thumb sections of a glove increases finger dexterity and hand comfort associated with the use of the glove. The potential negative effects of the thinner material with respect to vibration transmitted to the fingers is minimal and is offset by the increased dexterity and comfort experienced when wearing and using the glove.

9.3.2 Measurement of the thickness of the glove vibration-reducing material

9.3.2.1 General

The thickness of the vibration-reducing material in the palm and finger sections of a glove shall be measured as follows.

9.3.2.2 Measurement setup


The measurement setup for measuring the thickness of the glove vibration-reducing material is shown in [Figure 11](#). The thickness measurement should be made on a flat bench top. Place a $(6 \pm 0,6)$ mm thick sheet of polymethylmethacrylate (PMMA) or other similar material on the surface of the bench top. This is the measurement surface. Machine a uniform cylindrical measurement mass which shall have the following specifications:

- a) material: aluminium (density $2\,700\text{ kg/m}^3$);
- b) diameter, D : (80 ± 4) mm;
- c) thickness, δ_1 : (25 ± 2) mm;
- d) mass: (350 ± 35) g.

The circumferential position of the measurement locations can be conveniently selected based on the location of the measurement mass on the vibration-reducing material.

The purpose of the sheet of PMMA or other similar material is to provide on a typical bench top a smooth flat surface on which to perform the measurements specified in [9.3.2](#). If the measurements

are performed on a smooth flat granite, slate or other similar surface, this sheet may not be necessary. When placed on the palm or fingers of a glove, the disc may extend beyond the boundaries of the palm or fingers of the glove.

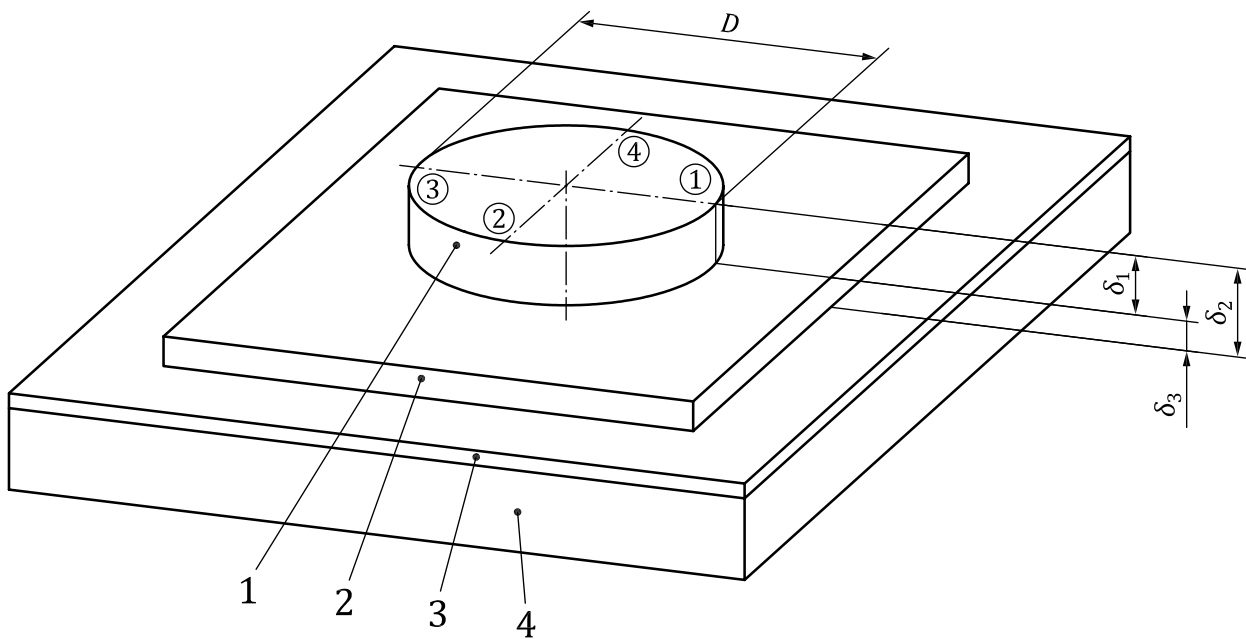

Key			
1	measurement mass	①, ②, ③, ④	measurement locations around the top of the measurement mass
2	vibration-reducing material	D	diameter of the measurement mass
3	polymethylmethacrylate sheet	δ_1	measurement mass thickness
4	flat bench top	δ_2	$\delta_2 = \delta_1 + \delta_3$
		δ_3	vibration-reducing material thickness

Figure 11 — Example of a measurement setup for measuring the glove vibration-reducing material thickness

9.3.2.3 Measurement procedure

The thickness of the glove vibration-reducing material in the palm and finger sections shall be measured as follows.

- a) If the vibration-reducing material is an insert placed into the glove, remove the vibration-reducing material from the glove or use a sample of the vibration-reducing material that has been received from the glove manufacturer or supplier.
- b) If the vibration-reducing material is integrated into the covering of the palm, finger and thumb sections on the palm-side of the glove, the thickness measurement shall include the entire integrated material from the palm side of the glove.
- c) Place the glove vibration-reducing material on the surface of the sheet of PMMA or other similar material and the measurement mass on top of the centre of the palm section or on top of a minimum of three finger elements of the finger section of the vibration-reducing material.
- d) Measure the distance between the top of the measurement mass and the surface of the sheet of PMMA or other similar material, δ_2 , at four locations around the top of the measurement mass that shall be separated by angles of $90^\circ \pm 5^\circ$ to within $\pm 0,1$ mm (see [Figure 11](#)).

- e) Calculate the thickness of the vibration-reducing material, δ_3 , at the four measurement locations, using Formula (16):

$$\delta_{3i} = \delta_{2i} - \delta_1 \quad (16)$$

where $i = 1, 2, 3, 4$.

- f) Calculate the average thickness of the vibration-reducing material, using Formula ((17):

$$\bar{\delta}_3 = \frac{1}{4} \sum_{i=1}^4 \delta_{3i} \quad (17)$$

$\bar{\delta}_3$ shall be the reported thickness of the vibration-reducing material in the palm and finger sections.

- g) It may be difficult to use the measurement setup in [Figure 11](#) to measure the thickness of the thumb element of the glove vibration-reducing material. When this is the case, the thumb element shall be visually inspected to verify that its thickness is similar to the thickness of the four finger elements.

9.3.3 Lacks (gap) between the palm and thumb sections of glove vibration-reducing material

9.3.3.1 General

Antivibration gloves may be fabricated in which the vibration-reducing material placed in the thumb section of the gloves is not directly connected to the adjacent vibration-reducing material placed in the palm section. When this is the case, the following requirements shall be met.

9.3.3.2 Vibration-reducing material covering in the palm area between the index finger and thumb

The area of the palm directly between the index finger and the thumb shall be covered by vibration-reducing material that is part of the vibration-reducing material in the palm section of the gloves.

9.3.3.3 Lacks (gap) between the thumb and palm vibration-reducing material

The lacks (gap) between the thumb section and adjacent palm section vibration-reducing material should not be greater than the thickness of the palm section vibration-reducing material along the length of the lacks.

9.3.3.4 Securing of the vibration-reducing material in the thumb

The thumb section vibration-reducing material shall be secured in the thumb section of the gloves so that the material does not slip or move out of position during normal use of the gloves.

9.3.4 Requirements within the European Union

Gloves that are designated as antivibration gloves according to this International Standard that will be used in workplace environments in the European Union are also required to meet the minimal requirements for mechanical risks specified in EN 388.

10 Test report

The glove manufacturer or supplier shall provide the following information, which shall be included in the test report.

- Description of glove material(s) or fabric(s) used in the palm, finger and thumb sections of the glove that comes into contact with the handles and other parts of a vibrating machine or the surface of a vibrating work piece.

- Description of material(s) or fabric(s) used on the dorsal sections of the glove.
- Description of the vibration-reducing material placed in the glove [include trademark(s) and brand name(s) associated with the vibration-reducing material, if used].
- A picture (in jpeg, tiff or other accepted electronic picture format) of the vibration-reducing material used in the glove.
- Thicknesses of the vibration-reducing material used in the palm, finger and thumb sections of the glove.
- A sample of the glove vibration-reducing material (or permission to disassemble one of the gloves sent for testing) so the thickness measurements specified in [9.3.2](#) can be made.
- Description of other relevant properties of materials or fabrics used in the glove (e.g. outer glove materials or fabrics that are resistant to cutting and slashing, are flame resistant, have improved wear and durability properties). Identify by name the types of these materials [with trademark(s) or brand name(s)].

The test report shall contain at least the following information:

- a) the details of the institute, laboratory or other responsible organization which carried out the test;
- b) the date of the test;
- c) the name and address of the glove manufacturer;
- d) the model or type and condition (new or used) of the glove;
- e) a description of the samples tested (size, mass, left or right, colour);
- f) a description of the testing equipment;
- g) the method 1 or 2 in [6.1.5.2](#) or [6.1.5.3](#) that was used for the vibration transmissibility tests;
- h) the measuring conditions (temperature and relative humidity in the test area);
- i) vibration attenuation results:
 - 1) corrected gloved hand frequency-weighted arithmetic mean vibration transmissibility, standard deviation and coefficient of variation values for the Δf_M and Δf_H frequency ranges for each individual test subject and for all five test subjects combined,
 - 2) corrected gloved hand arithmetic mean vibration transmissibility, standard deviation and coefficient of variation values for the one-third-octave bands with centre frequencies of 25 Hz to 1 250 Hz for each individual test subject and for all five test subjects combined.

NOTE Standard deviation and coefficient of variation values for $T_{(M)}$ and $T_{(H)}$ are calculated and reported as required in [8.3](#). Currently there is no clear guidance as to what constitutes acceptable values for these terms. Standard deviation and coefficient of variation values obtained from glove vibration transmissibility tests conducted in accordance with the requirements of this International Standard will be collected and evaluated. It is anticipated that the results of this evaluation will give guidance as to how to more appropriately select test subjects for glove vibration transmissibility tests conducted in accordance with the requirements of this International Standard.

Annex A (informative)

Examples of handles with force and acceleration measuring systems

Two examples of test handles with force and acceleration measuring systems are shown in [Figures A.1](#) and [A.2](#). [Figure A.1](#) shows a grip force measuring system while [Figure A.2](#) includes both a feed force and a grip force measuring system.


The first resonance frequency of these handles is usually in the range of 1,6 kHz to 2,1 kHz depending on the cap material and the tightness of the screws that hold the handle together.

NOTE 1 Only one charge amplifier is required for the two piezoelectric force transducers because their signals can be input to the same amplifier for the total grip force measurement.

NOTE 2 Because any piezoelectric force transducer has some zero-drift during its use, a reset of the charge amplifier before each test is recommended to ensure the accuracy of the force measurement.

NOTE 3 The accelerometer can be firmly attached to the handle base using a hard adhesive.


Dimensions in millimetres

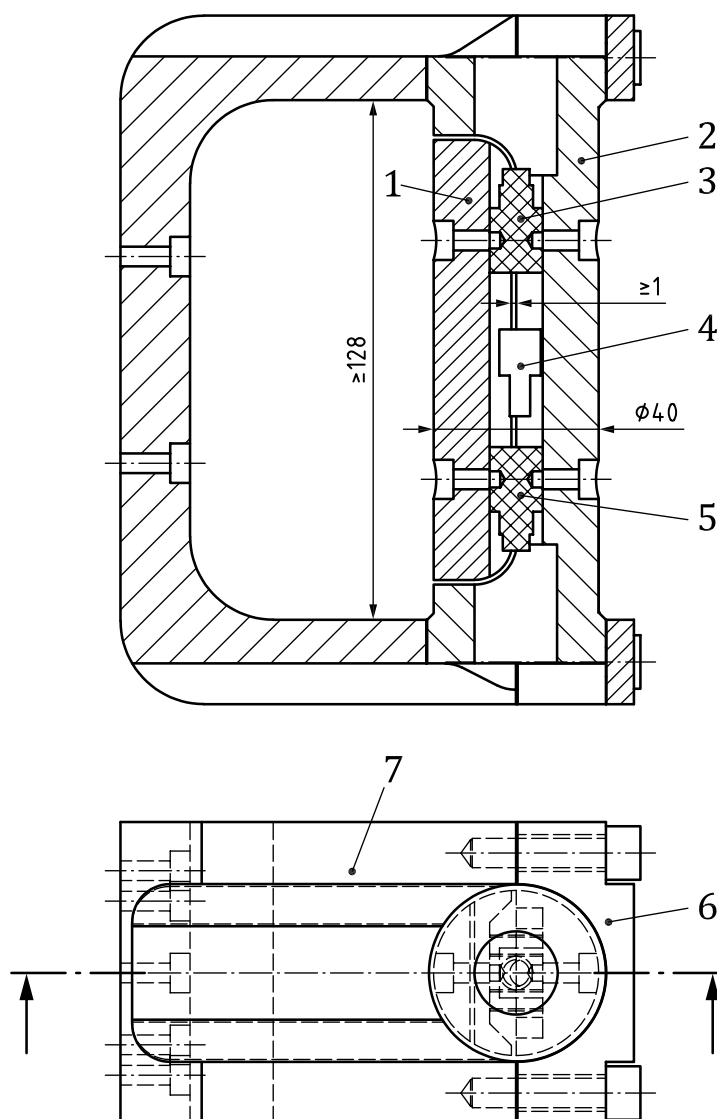

Key

- | | | | |
|---|---|---|---------------------------|
| 1 | measurement cap, aluminium or magnesium | 5 | force transducer |
| 2 | handle base, aluminium | 6 | fixture clamp, aluminium |
| 3 | force transducer | 7 | handle fixture, aluminium |
| 4 | accelerometer attached to base using cyanoacrylate glue or stud | | |

Figure A.1 — Example 1 of a handle with grip force measuring system

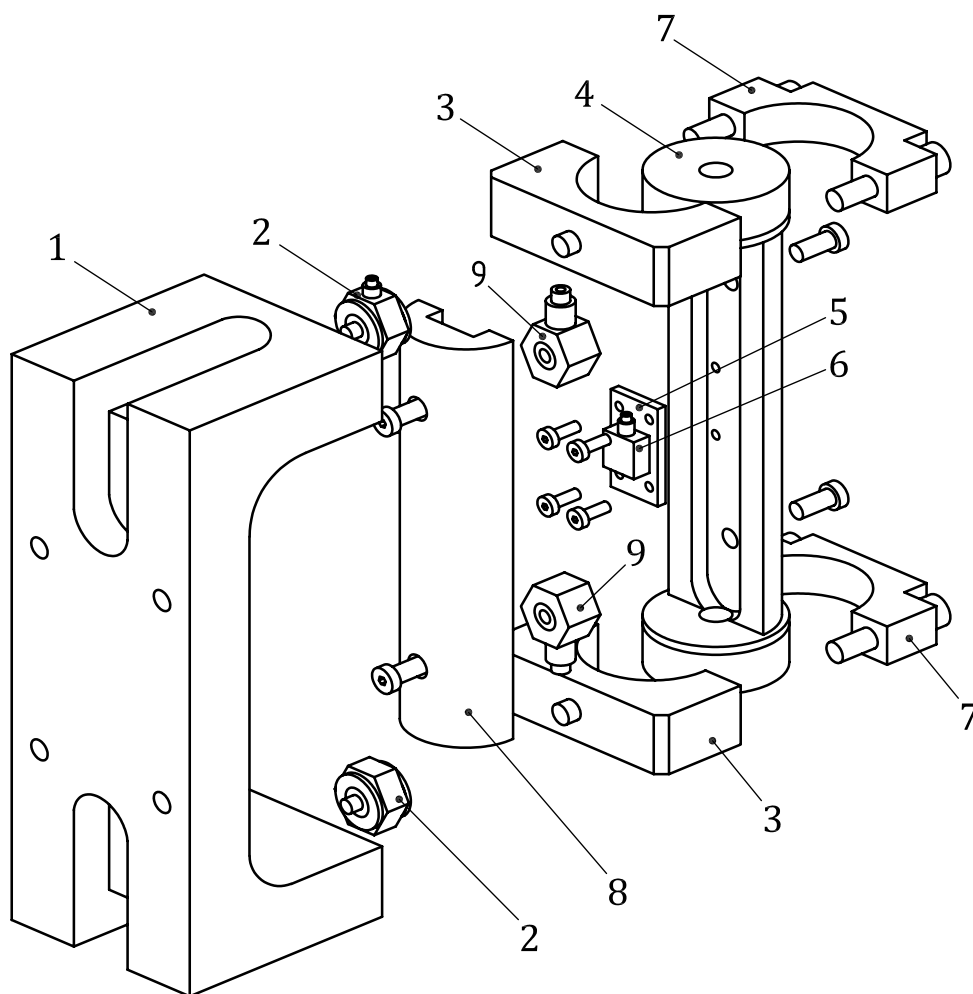

Key

- | | | | | | |
|---|-----------------------|---|----------------------------|---|----------------------------------|
| 1 | base, aluminium | 4 | handle \varnothing 40 mm | 7 | front bracket |
| 2 | feed force transducer | 5 | accelerometer base | 8 | handle cover \varnothing 40 mm |
| 3 | rear bracket | 6 | accelerometer | 9 | grip force transducer |

Figure A.2 — Example 2 of a handle with feed and grip force measuring systems

Bibliography

- [1] ISO 13753, *Mechanical vibration and shock — Hand–arm vibration — Method for measuring the vibration transmissibility of resilient materials when loaded by the hand–arm system*
- [2] ISO 15230, *Mechanical vibration and shock — Coupling forces at the man–machine interface for hand-transmitted vibration*
- [3] ALDIEN Y., WELCOME D.E., RAKHEJA S., DONG R.G., BOILEAU P.-É. Contact pressure distribution at hand-handle interface: Role of hand forces and handle size. *Int. J. Ind. Ergon.* 2005, **35** pp. 267–286
- [4] BOILEAU P.E., BOUTIN J., RAKHEJA S., DONG R.G. Critical evaluation of a laboratory test procedure for measuring the vibration transmissibility of gloves. *Proceedings of the 37th UK Conference on Human Responses to Vibration*, Dept. of Human Sciences, Loughborough University, UK, 2002, pp. 106–117
- [5] DONG R.G., RAKHEJA S., SMUTZ W.P., SCHOPPER A.W., WU J.Z. Evaluating anti-vibration performance of a glove using total effective transmissibility. *Int. J. Ind. Ergon.* 2002, **30** pp. 33–48
- [6] DONG R.G., MCDOWELL T.W., WELCOME D.E., BARKLEY J., WARREN C., WASHINGTON B. Effects of hand–tool coupling conditions on the isolation effectiveness of air bladder anti-vibration gloves. *J. Low Freq. Noise Vibrat. Act. Contr.* 2004, **23** pp. 231–248
- [7] DONG R.G., MCDOWELL T.W., WELCOME D.E., WARREN C., WU J.Z., RAKHEJA S. Analysis of anti-vibration gloves mechanism and evaluation methods. *J. Sound Vibrat.* 2009, **321** pp. 435–453
- [8] GRIFFIN M.J. Evaluating the effectiveness of gloves in reducing hazards hand-transmitted vibration. *Occup. Environ. Med.* 1998, **55** pp. 340–348
- [9] MARCOTTE P., ALDIEN Y., BOILEAU P.-É., RAKHEJA S., BOUTIN J. Effect of handle size and hand-handle contact force on the biodynamic response of the hand–arm system under z_h -axis vibration. *J. Sound Vibrat.* 2005, **283** pp. 1071–1091
- [10] REYNOLDS D.D., & WOLF E. Evaluation of antivibration glove test protocols associated with the revision of ISO 10819. *Indust. Health (Jpn)* 2005, **43**, pp. 556–565. Available (viewed 2013-01-13) at: www.jniosh.go.jp/en/indu_hel/pdf/43-3-21.pdf

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com



...making excellence a habit.™