

# Starch and derived products — Heavy metals content —

## Part 2: Determination of mercury content by atomic absorption spectrometry

The European Standard EN ISO 11212-2:1997 has the status of a  
British Standard

ICS 67.180.20

## National foreword

This British Standard is the English language version of EN ISO 11212-2:1997. It is identical with ISO 11212-2:1997 and implements it as the UK national standard.

This British Standard has been produced to fulfil BSI's obligation to implement all European Standards but, because of the absence of interest in the UK in the subject concerned, there has been no UK participation in the preparation of EN ISO 11212-2.

Any queries relating to the EN should be directed to BSI, quoting the reference AW/100.

### Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the BSI Standards Catalogue under the section entitled "International Standards Correspondence Index", or using the "Find" facility of the BSI Standards Electronic Catalogue. A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

**Compliance with a British Standard does not of itself confer immunity from legal obligations.**

### Summary of pages

This document comprises a front cover, an inside front cover, pages i and ii, the EN ISO title page, page 2, the ISO title page, page ii, pages 1 to 4 and a back cover.

This standard has been updated (see copyright date) and may have had amendments incorporated. This will be indicated in the amendment table on the inside front cover.

### Amendments issued since publication

Amd. No.	Date	Comments

This British Standard, having been prepared under the direction of the Consumer Products and Services Sector Board, was published under the authority of the Standards Board and comes into effect on 15 May 1997

© BSI 02-1999

ISBN 0 580 27457 8

---

---

# Contents

	Page
National foreword	Inside front cover
Foreword	2
Foreword	ii
Text of ISO 11212-2	1

---



---

ICS 67.180

Descriptors: See ISO document

English version

Starch and derived products — Heavy metals  
content — Part 2: Determination of mercury  
content by atomic absorption spectrometry  
(ISO 11212-2:1997)

Amidons, féculés et produits dérivés — Teneur  
en métaux lourds — Partie 2: Détermination de  
la teneur en mercure par spectrométrie  
d'absorption atomique (ISO 11212-2:1997)

Stärke und Stärkederivate —  
Schwermetallgehalt — Teil 2: Bestimmung des  
Quecksilbergehaltes durch  
Atomabsorptionsspektrometrie  
(ISO 11212-2:1997)

This European Standard was approved by CEN on 1997-02-28. CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

The European Standards exist in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

**CEN**

European Committee for Standardization  
Comité Européen de Normalisation  
Europäisches Komitee für Normung

**Central Secretariat: rue de Stassart, 36 B-1050 Brussels**

**Foreword**

The text of the International Standard ISO 11212-2:1997 has been prepared by Technical Committee ISO/TC 93 “Starch (including derivatives and by-products)” in collaboration with CEN/CS.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by September 1997, and conflicting national standards shall be withdrawn at the latest by September 1997.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and the United Kingdom.

**Endorsement notice**

The text of the International Standard ISO 11212-2:1997 was approved by CEN as a European Standard without any modification.

**Contents**

	Page
Foreword	2
1 Scope	1
2 Definition	1
3 Principle	1
4 Reagents	1
5 Apparatus	1
6 Procedure	2
7 Expression of results	3
8 Precision	3
9 Test report	3
Annex A (normative) Result of interlaboratory test	4
Figure 1 — Digestion apparatus	2
Table A.1 — Interlaboratory test on corn starch	4

INTERNATIONAL  
STANDARD

ISO  
11212-2

First edition  
1997-03-15

---

---

**Starch and derived products — Heavy  
metals content —**

**Part 2:**

**Determination of mercury content by atomic  
absorption spectrometry**

*Amidons, fécules et produits dérivés — Teneur en métaux lourds —*

*Partie 2: Détermination de la teneur en mercure par spectrométrie  
d'absorption atomique*



Reference number  
ISO 11212-2:1997(E)

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

International Standard ISO 11212-2 was prepared by Technical Committee ISO/TC 93, *Starch (including derivatives and by-products)*.

ISO 11212 consists of the following parts, under the general title *Starch and derived products — Heavy metals content*.

- *Part 1: Determination of arsenic content by atomic absorption spectrometry;*
- *Part 2: Determination of mercury content by atomic absorption spectrometry;*
- *Part 3: Determination of lead content by atomic absorption spectrometry with electrothermal atomization;*
- *Part 4: Determination of cadmium content by atomic absorption spectrometry with electrothermal atomization.*

Annex A of this part of ISO 11212 is for information only.

**Descriptors:** Starches, food starch, chemical analysis, determination of content, heavy metals, mercury, atomic absorption spectrometric method.



## 1 Scope

This part of ISO 11212 specifies a method for the determination of the mercury content of starch, including derivatives and by-products, by atomic absorption spectrometry with cold-vapour generation.

The cold-vapour generators currently available use very different techniques; it is thus impossible to propose a comprehensive method likely to ensure the attainment of satisfactory results on all types of apparatus. Each analyst should therefore optimize the conditions of use of his/her own apparatus on the basis of general or particular instructions.

## 2 Definition

For the purposes of this part of ISO 11212, the following definition applies.

### 2.1

#### mercury content

quantity of mercury determined in accordance with the conditions specified in this method and expressed as mercury (Hg), in micrograms per kilogram of the product as received

## 3 Principle

Wet digestion of the organic matrix. Reduction of mercury ( $\text{Hg}^{2+}$ ) to metallic mercury by hydrogen resulting from the action of sodium borohydride (or tin(II) chloride) on hydrochloric acid.

Entrainment of the mercury vapour by a flow of gas and determination of monoatomic mercury vapour by atomic absorption spectrometry in a quartz cell.

Measurement of the absorbance at a wavelength of 253,7 nm.

Determination of the concentration of mercury in the sample by means of a calibration curve.

## 4 Reagents

Use only reagents of recognized analytical grade and distilled water or water of equivalent purity.

**4.1 Nitric acid** ( $\rho_{20} = 1,38 \text{ g/ml}$ ).

**4.2 Hydrogen peroxide**, 30 % (V/V) solution.

**4.3 Sodium borohydride solution**

Prepare a solution at the concentration recommended in the instructions for use of the cold-vapour generator (5.3).

**4.4 Tin(II) chloride solution**

Prepare a solution at the concentration recommended in the instructions for use of the cold-vapour generator (5.3).

**4.5 Hydrochloric acid solution**

Prepare a solution at the concentration recommended in the instructions for use of the cold-vapour generator (5.3).

**4.6 Mercury standard solution**, 1 g/l.

Standard solutions are commercially available at this concentration. These solutions may be prepared by weighing and dissolving the salt or metal of known purity.

**4.7 Calibration solutions**

Before each series of measurements, prepare from the standard mercury solution (4.6) at least five calibration solutions covering the range of concentrations to be determined. 100 ml of each calibration solution shall contain 7,5 ml of nitric acid (4.1).

## 5 Apparatus

All the glassware used shall be previously washed by means of suitable products (such as nitric acid) and rinsed with distilled water to eliminate any trace of mercury.

Use ordinary laboratory apparatus and, in particular, the following.

**5.1 Digestion apparatus** (see Figure 1), made of borosilicate glass and consisting of three elements terminating with conical ground joints (5.1.1 to 5.1.3).

**5.1.1 Soxhlet extraction tube**, of capacity 200 ml, equipped with a stopcock and a lateral tube connected directly to the flask (5.1.3).

**5.1.2 Cooling apparatus**, 35 cm long, connected to the top of the Soxhlet extraction tube (5.1.1).

**5.1.3 Round-bottom flask**, of capacity 250 ml, connected to the lower part of Soxhlet extraction tube (5.1.1).

When the stopcock is open, the device is under reflux; when it is closed the Soxhlet extraction tube (5.1.1) retains the condensed water and acid vapours.

**5.2 Atomic absorption spectrometer**, consisting of five elements (5.2.1 to 5.2.5).

**5.2.1 High-resolution monochromator**, allowing a 0,2 nm bandwidth slit.

**5.2.2 Correcting device** for non-specific absorption.

**5.2.3 Measuring and photoelectric reception device**, with a response time not exceeding about 10 ms.

**5.2.4 Detector and signal processing system**, allowing recording of the maximum and/or integrated absorbance signal.

**5.2.5 Mercury discharge lamp or mercury hollow cathode lamp.**

**5.3 Generator of cold mercury vapour**, allowing the generation of cold mercury vapour as well as its transport to a measuring cell whose wavelength is adapted to the spectrometer, and equipped with an automatic sampling device which is necessary to obtain good repeatability and to reduce the risk of contamination.

**5.4 Pipettes and micropipettes**, of suitable capacity.

**5.5 Analytical balance.**

## 6 Procedure

**WARNING** — Mercury is highly toxic and is a very volatile element. It is thus necessary to verify the tightness of the ground joints and of the tap and to avoid any overheating at digestion in order to prevent any loss of mercury vapour.

### 6.1 Preparation of test sample

Thoroughly homogenize the sample.

### 6.2 Digestion

Use the digestion apparatus described in 5.1.

Weigh, to the nearest 1 mg, about 5 g of the test sample into the flask (5.1.3). Add 27,5 ml of nitric acid (4.1) and 1 ml of hydrogen peroxide (4.2). Distil under reflux for 4 h leaving the stopcock open. Turn the stopcock off, continue heating and distil until about  $20 \text{ ml} \pm 1 \text{ ml}$  of liquid are recovered in the extraction tube (5.1.1). Stop heating and allow the flask to cool. Separate the flask from the extraction tube. Add 20 ml of water to the digested residue in the flask, bring to the boil for a few minutes, stop heating and allow to cool. Transfer the solution to a 100 ml volumetric flask, dilute to the mark with distilled water and stir.

**NOTE** To reach the required precision, the tin(II) chloride or the gold amalgam enrichment technique can be used as reducing agent.

### 6.3 Blank test

Perform digestion under the same conditions as in 6.2, replacing the test portion by 5 ml of water.

### 6.4 Determination of the calibration curve

Carry out the analysis of the diluted calibration solutions (4.7) with reference to the instructions for use of the cold-vapour generator (5.3) by adding the recommended quantities of tin(II) chloride solution (4.4) and sodium borohydride solution (4.3). Measure the absorbance of each calibration solution at a wavelength of 253,7 nm using the spectrometer (5.2).

Draw the calibration curve by plotting the mercury concentrations of the calibrations solutions, expressed in micrograms per litre, as the abscissa against the corresponding values of the signal, read either in maximum absorbance or in integrated absorbance, as the ordinate. The calibration curve shall be periodically checked depending on the length of the series of analyses.

### 6.5 Determination

Measure the absorbance of the test samples under the same conditions as the calibration solutions and compare the results with the previously plotted calibration curve.

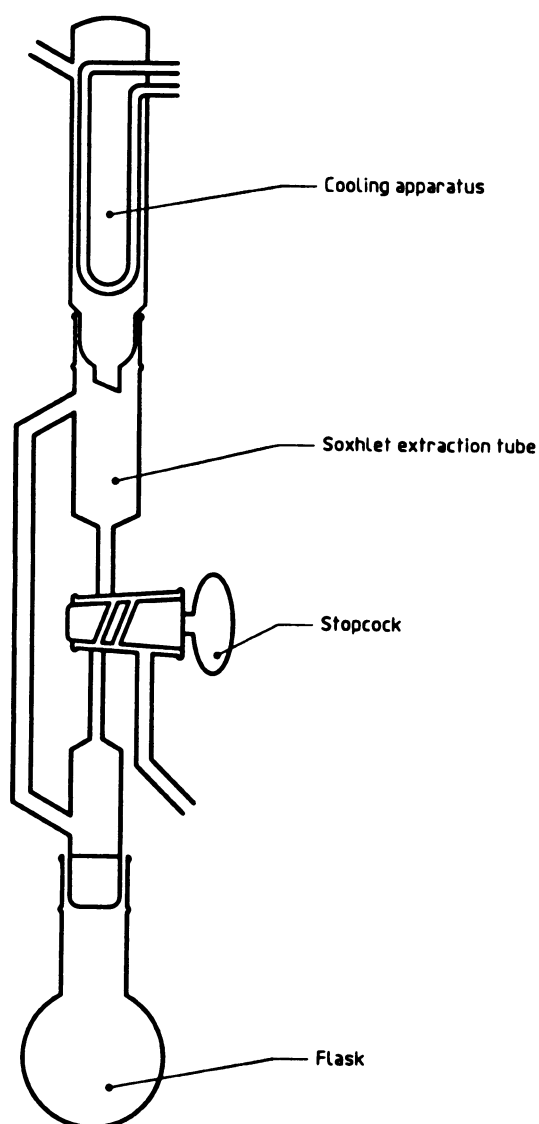


Figure 1 — Digestion apparatus

## 7 Expression of results

With reference to the calibration curve, determine the concentrations corresponding to the signals of the test portion and the blank. The mercury concentration of the sample,  $w$ , expressed in micrograms per kilogram of the product as received, is given by the equation:

$$w = \frac{(\rho_1 - \rho_0) \times 100}{m}$$

where

- $\rho_1$  is the numerical value of the mercury concentration, in micrograms per litre, of the test solution (6.2) read from the calibration curve (6.4);
- $\rho_0$  is the numerical value of the mercury concentration, in micrograms per litre, of the blank test solution (6.3) read from the calibration curve (6.4);
- $m$  is the numerical value of the mass, in grams, of the test portion (6.2).

NOTE When strictly following this method, the quantification limit can reach 20 µg/kg.

## 8 Precision

Details of an interlaboratory test on the precision of the method are summarized in Annex A. The values derived from the interlaboratory test may not be applicable to analyte concentration ranges and matrices other than those given in Annex A.

### 8.1 Repeatability

The absolute difference between two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, will not exceed the repeatability limit  $r$  deduced from Table A.1 in more than 5 % of cases.

### 8.2 Reproducibility

The absolute difference between two single test results, obtained using the same method on identical test material in different laboratories with different operators using different equipment, will not exceed the reproducibility limit  $R$  deduced from Table A.1 in more than 5 % of cases.

## 9 Test report

The test report shall specify:

- the method in accordance with which sampling was carried out, if known;
- the method used;
- the test result(s) obtained; and
- if the repeatability has been checked, the final quoted result obtained.

It shall also mention all operating details not specified in this part of ISO 11212, or regarded as optional, together with details of any incidents which may have influenced the test result(s).

The test report shall include all information necessary for the complete identification of the sample.

**Annex A (informative)**  
**Results of interlaboratory test**

An interlaboratory test at the international level was carried out by 12 laboratories in 1993. The statistical results indicated in Table A.1 were determined in accordance with ISO 5725<sup>1)</sup>.

**Table A.1 — Interlaboratory test on corn starch**

Parameter	Sample <sup>a</sup>		
	LC	HC	VHC
No. of laboratories retained after eliminating outliers	7	8	8
No. of outliers (laboratories)	5	5	5
No. of accepted results	28	31	32
Mean mercury content (µg/kg)	49,4	98,5	161,5
Repeatability standard deviation, $s_r$ (µg/kg)	5,4	10,7	11,7
Repeatability limit, $r = 2,8 \times s_r$ (µg/kg)	15,2	30,3	33,2
Reproducibility standard deviation, $s_R$ (µg/kg)	18,7	43,4	71,8
Reproducibility limit, $R = 2,8 \times s_R$ (µg/kg)	53,0	122,9	203,2
<sup>a</sup> Com starch with LC: low content HC: high content VHC: very high content			

<sup>1)</sup> ISO 5725:1986, *Precision of test methods — Determination of repeatability and reproducibility for a standard test method by inter-laboratory tests* (now withdrawn), was used to obtain the precision data.



---

---

# BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

## Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

## Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

## Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre. Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: 020 8996 7002. Fax: 020 8996 7001.

## Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager. Tel: 020 8996 7070.