

BS EN ISO 11358-1:2014



BSI Standards Publication

Plastics — Thermogravimetry (TG) of polymers

Part 1: General principles

bsi.

...making excellence a habit.™

National foreword

This British Standard is the UK implementation of EN ISO 11358-1:2014. It supersedes BS EN ISO 11358:1997 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee PRI/21, Testing of plastics.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2014. Published by BSI Standards Limited 2014

ISBN 978 0 580 77735 6

ICS 83.080.01

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 July 2014.

Amendments issued since publication

Date	Text affected
------	---------------

EUROPEAN STANDARD

EN ISO 11358-1

NORME EUROPÉENNE

EUROPÄISCHE NORM

July 2014

ICS 83.080.01

Supersedes EN ISO 11358:1997

English Version

Plastics - Thermogravimetry (TG) of polymers - Part 1: General principles (ISO 11358-1:2014)

Plastiques - Thermogravimétrie (TG) des polymères - Partie 1: Principes généraux (ISO 11358-1:2014)

Kunststoffe - Thermogravimetrie (TG) von Polymeren - Teil 1: Allgemeine Grundsätze (ISO 11358-1:2014)

This European Standard was approved by CEN on 28 June 2014.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

CEN-CENELEC Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

This document (EN ISO 11358-1:2014) has been prepared by Technical Committee ISO/TC 61 "Plastics" in collaboration with Technical Committee CEN/TC 249 "Plastics" the secretariat of which is held by NBN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by January 2015, and conflicting national standards shall be withdrawn at the latest by January 2015.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN ISO 11358:1997.

According to the CEN-CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

Endorsement notice

The text of ISO 11358-1:2014 has been approved by CEN as EN ISO 11358-1:2014 without any modification.

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	2
5 Apparatus	2
6 Test specimen preparation	2
6.1 General.....	2
6.2 Test specimens from finished products.....	3
6.3 Test specimen conditioning.....	3
6.4 Test specimen mass.....	3
7 Calibration	3
7.1 Mass calibration.....	3
7.2 Temperature calibration.....	3
8 Procedure	4
8.1 General.....	4
8.2 Temperature scanning mode.....	4
8.3 Isothermal mode.....	5
9 Expression of results	5
9.1 Graphical representation.....	5
9.2 Determination of increase in mass.....	5
9.3 Determination of loss in mass.....	6
10 Test report	8

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: Foreword - Supplementary information

The committee responsible for this document is ISO/TC 61, *Plastics*, Subcommittee SC 5, *Physical chemical properties*.

This first edition of ISO 11358-1 cancels and replaces ISO 11358:1997, which has been technically revised.

The main changes are:

- a) addition of ISO 472 to the Normative references clause and removal of definitions specified therein;
- b) revision of apparatus specifications.

ISO 11358 consists of the following parts, under the general title *Plastics — Thermogravimetry (TG) of polymers*:

- *Part 1: General principles*
- *Part 2: Determination of activation energy*
- *Part 3: Determination of the activation energy using the Ozawa-Friedman plot and analysis of the reaction kinetics*

Plastics — Thermogravimetry (TG) of polymers —

Part 1: General principles

1 Scope

This part of ISO 11358 specifies general conditions for the analysis of polymers using thermogravimetric techniques. It is applicable to liquids or solids. Solid materials may be in the form of pellets, granules or powders. Fabricated shapes reduced to appropriate specimen size may also be analysed by this method.

Thermogravimetry can be used to determine the temperature(s) and rate(s) of decomposition of polymers, and to measure at the same time the amounts of volatile matter, additives and/or fillers they contain.

The thermogravimetric measurements may be carried out in dynamic mode (mass change versus temperature or time under programmed conditions) or isothermal mode (mass change versus time at constant temperature).

Thermogravimetric measurements may also be carried out using different testing atmospheres, e.g. to separate decomposition in an inert atmosphere from oxidative degradation.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 291, *Plastics — Standard atmospheres for conditioning and testing*

ISO 472, *Plastics — Vocabulary*

ISO 11357-1, *Plastics — Differential scanning calorimetry (DSC) — Part 1: General principles*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 472 and the following apply.

3.1

dynamic mass-change determination

technique for recording the variation of the mass of a test specimen with temperature T which is changing at a programmed rate

3.2

isothermal mass-change determination

technique for recording the variation of the mass of a test specimen with time t at constant temperature T

3.3

Curie temperature

temperature at which a ferromagnetic material passes from the ferromagnetic state to the paramagnetic state or vice versa

4 Principle

A test specimen is heated at specified rates with a controlled temperature programme, and the change in mass is measured as a function of temperature. Alternatively, the specimen is kept at a given constant temperature and the change in mass is measured as a function of time over a given period.

During measurement the test specimen is held in a controlled inert or oxidising atmosphere.

In general, the reactions which cause the mass of a test specimen to change are decomposition or oxidation reactions or the volatilisation of a component. The change in mass is recorded as a thermogravimetric (TG) curve.

The change in mass of a material as a function of temperature and the extent of this change are indicators of the thermal stability of the material. TG data can therefore be used to evaluate the relative thermal stability of polymers of the same generic family and polymer-polymer or polymer-additive interactions, using measurements made under the same test conditions.

NOTE TG data may be used for process control, process development and material evaluation. Long-term thermal stability is a complex function of service and environmental conditions. TG data alone may not be able to describe the long-term thermal stability of a polymer.

5 Apparatus

A number of commercial instruments suitable for thermogravimetric measurements are available. The basic apparatus consists of the following.

5.1 Thermobalance, meeting the following requirements:

- capability to generate constant heating and cooling rates suitable for intended measurements;
- capability to maintain the test temperature constant (to within $\pm 0,3$ K or less for the duration of measurement);
- capability to maintain a constant purge gas flow rate controllable to within ± 10 % over a range of flow rates (e.g. 10 ml/min to 150 ml/min);
- temperature and mass range in line with experimental requirements;
- recording device capable of automatically recording the measured curve of mass versus temperature and time;
- measurement of temperature signals with an accuracy of ± 2 K or better;
- measurement of time with an accuracy of ± 1 s or better;
- measurement of mass with an accuracy of ± 20 μg or better.

5.2 Purge gas, dry air or oxygen (oxidizing conditions) or a suitable inert gas with an oxygen content of 0,001 % by volume or less (non-oxidizing conditions). In either case, the water content of the purge gas shall be less than 0,001 % by mass.

6 Test specimen preparation

6.1 General

Test specimens may be liquids or solids. Solids may be in the form of powders, pellets, granules or cut pieces. For finished products, the test specimen shall be in the form normally found in use.

6.2 Test specimens from finished products

Cut the test specimen to appropriate size for the specimen holder. Microtomes or razor blades are suitable for this purpose.

NOTE Test specimen size and shape are generally dependent on the sample holder. Surface area affects the overall results. For instance, in comparing a test specimen of large surface area with a test specimen of smaller surface area, both having the same mass, the smaller surface area test specimen normally changes at a slower rate.

6.3 Test specimen conditioning

Unless otherwise specified in a material specification or product standard, test specimens shall be conditioned, prior to measurement, at one of the standard atmospheres specified in ISO 291, or by any other method specified by agreement between the interested parties.

6.4 Test specimen mass

Preferably, the mass of the test specimen shall be in the range of 10 mg to 100 mg.

7 Calibration

7.1 Mass calibration

Without any gas flow through the thermobalance (to prevent any disturbance through buoyancy and/or convection effects), calibrate the thermobalance as follows, using calibrated masses in the range of 10 mg to 100 mg:

Record the temperature at which the mass calibration was carried out.

Zero the thermobalance. Place the calibration weight on the thermobalance and measure the corresponding mass change. If necessary, adjust the thermobalance so that the measured mass is equal to the calibration mass.

If mass calibration is done by procedures included in the instrument control software or by external service providers a valid calibration certificate may be acceptable to demonstrate adequate mass calibration.

7.2 Temperature calibration

Carry out the temperature calibration using the same atmosphere, rate of gas flow and heating rate as shall be used in the procedure specified in [Clause 8](#).

If the thermobalance is not coupled with another thermoanalytical method, use the following procedure.

- a) Choose two or more calibration materials with a Curie temperature near the temperature range to be examined. If possible, choose the calibration materials in such a way that the temperature range to be examined lies between the Curie temperatures of two of them.
- b) Start heating at the same heating rate as will be used in the procedure specified in [Clause 8](#) and carry out a calibration based on the start temperature T_A , mid-point temperature T_C and end temperature T_B for the Curie temperature transition.

NOTE 1 The Curie point is the temperature at which a ferromagnetic material becomes paramagnetic on heating. The effect is reversible. Applying a magnetic field (e.g. by placing a strong magnet below the furnace) exerts a downward force on the ferromagnetic sample. This creates an apparent increase of weight which is lost upon heating the sample above its Curie temperature.

NOTE 2 Certified calibration materials traceable to metrology laboratories should be preferably used. Suitable calibration materials may be available via instrument manufacturers or National Metrology Institutes.

If the thermobalance is combined with a DSC (differential scanning calorimetry) detector, it is recommended that the thermobalance is temperature-calibrated using procedures specified in corresponding standards, e.g. ISO 11357-1 for DSC.

NOTE 3 The melting point of a calibration material is defined as the intercept of the extrapolated baseline and the tangent to the slope of the endotherm at the point of inflection of the curve (the so-called onset temperature).

NOTE 4 Calibration is the most critical stage in obtaining reliable thermogravimetry data; the relationship between the temperature sensor, specimen geometry and type of atmosphere, including the rate of gas flow, will affect the calibration of the measurement system.

NOTE 5 The rate of mass loss is dependent upon the rate of oxidation of the test specimen, and therefore dependent in part upon the atmosphere and rate of gas flow to which it is exposed. It is therefore important to use the same atmosphere and rate of gas flow in the calibration as in the procedure specified in [Clause 8](#).

8 Procedure

8.1 General

Depending on the measurement requirements a suitable instrument setup has to be chosen. Two modes can be used: temperature scanning (see [8.2](#)) and isothermal (see [8.3](#)).

NOTE 1 A change in buoyancy and convection occurs in the thermobalance when the gas flow is operating. Even if there is no actual change in mass, an apparent change in mass is observed and the accuracy of mass measurement is reduced. It is recommended that a preliminary run without the test specimen is carried out at the same heating rate and gas-flow rate as in the actual test in order to observe the apparent change in mass. The precision of the mass measurement cannot be better than that obtained from the preliminary test.

NOTE 2 A change of gas is possible during the determination. In this case, it will be necessary to use the same flow rate. In addition, it is recommended that gases with similar densities are used in order to obtain a similar buoyancy effect. If gases of similar densities cannot be used, it may be necessary to make a buoyancy correction.

NOTE 3 When using multiple gases, it is important that the distances between the gas sources and the instrument are as short as possible to minimize the lag-time due to line purging.

Select the gas flow rate.

Adjust the zero point of the thermobalance including sample holder using the same purge gas and flow rate as to be used for the sample measurement.

Place the sample holder containing the test specimen on the thermobalance. Start the gas flow and record the initial mass, unless the following paragraph applies.

For investigations under a strictly inert atmosphere, either evacuate the thermobalance with a vacuum pump and then fill or purge with the inert gas to be used for measurement for at least 10 min at the same flow rate to be used for measurement before recording the mass.

8.2 Temperature scanning mode

Set the temperature programme to be followed, which shall be as specified by the referring standard, if applicable.

The programme shall include the initial and final temperatures, the duration of the isothermals at these temperatures, and the rates of heating between programmed temperatures, and the purge gas(es) to be used for the different programme steps.

Start the measurement programme and record the thermogravimetric curve.

8.3 Isothermal mode

Start the instrument, running at its maximum heating rate in order to reach the specified temperature as quickly as possible.


9 Expression of results

9.1 Graphical representation

Present the thermogravimetry data obtained in the form of a mass or mass change versus time or temperature curve. Determine specific temperatures and masses from the TG curve using the procedures specified in 9.2 and 9.3.

9.2 Determination of increase in mass

Determine the maximum mass, m_{\max} , from the curve. A typical mass gain curve is shown in [Figure 1](#).

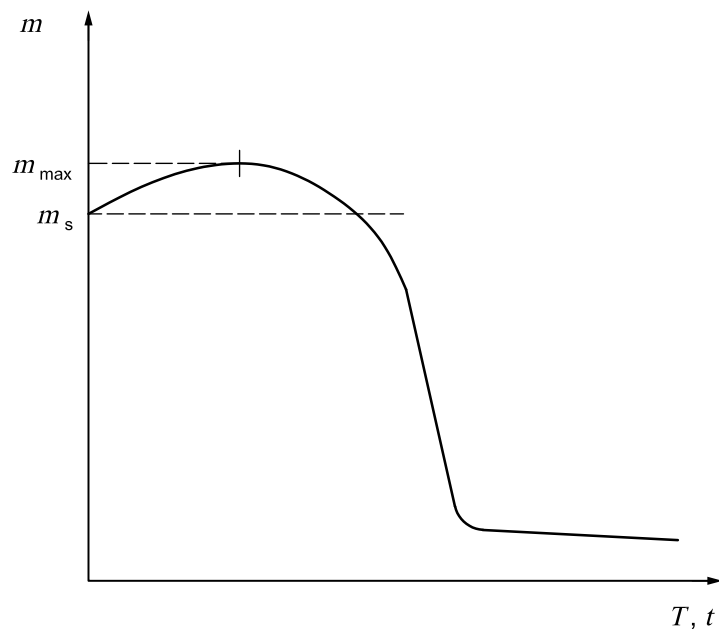

Key

m mass
 T temperature
 t time

Figure 1 — Example of a TG curve showing an increase in mass

Calculate the mass gain, m_g , expressed as a percentage, using Formula (1):

$$m_g = \frac{m_{\max} - m_s}{m_s} \times 100 \quad (1)$$

where


m_{\max} is the maximum mass, in milligrams;

m_s is the mass at the starting temperature, in milligrams.

NOTE An increase in mass according to 9.2 is observed in exceptional cases only where absorption of purge gas components occurs.

9.3 Determination of loss in mass

9.3.1 Single-stage decrease in mass (see Figure 2)

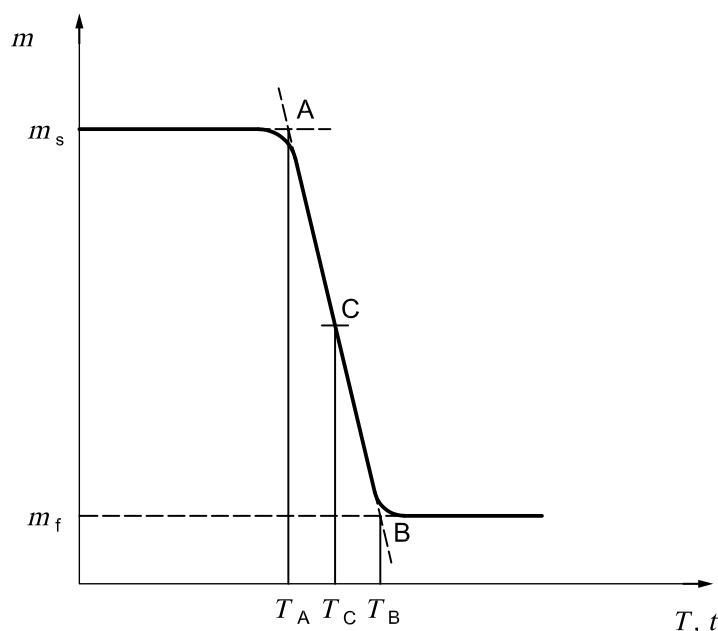

Key

m	mass	A	starting point
T	temperature	B	end point
t	time	C	mid-point

Figure 2 — Example of a TG curve showing a single-stage decrease in mass

From the TG curve, determine points A, B and C, where:

- A is the starting point — the point of intersection of the starting-mass baseline and the tangent to the TG curve at the point of maximum gradient;
- B is the end point — the point of intersection of the final-mass baseline and the tangent to the TG curve at the point of maximum gradient;
- C is the mid-point — the point of intersection of the TG curve with the temperature at which both baselines are equidistant.

Determine masses m_s and m_f and temperatures T_A , T_B and T_C corresponding to points A, B and C.

Calculate the mass loss m_l , expressed as a percentage, using Formula (2):


$$m_l = \frac{m_s - m_f}{m_s} \times 100 \quad (2)$$

where

m_f is the mass, in milligrams, at the end point B;

m_s is the mass, in milligrams, at the starting point A.

9.3.2 Multi-stage decrease in mass (see [Figure 3](#))

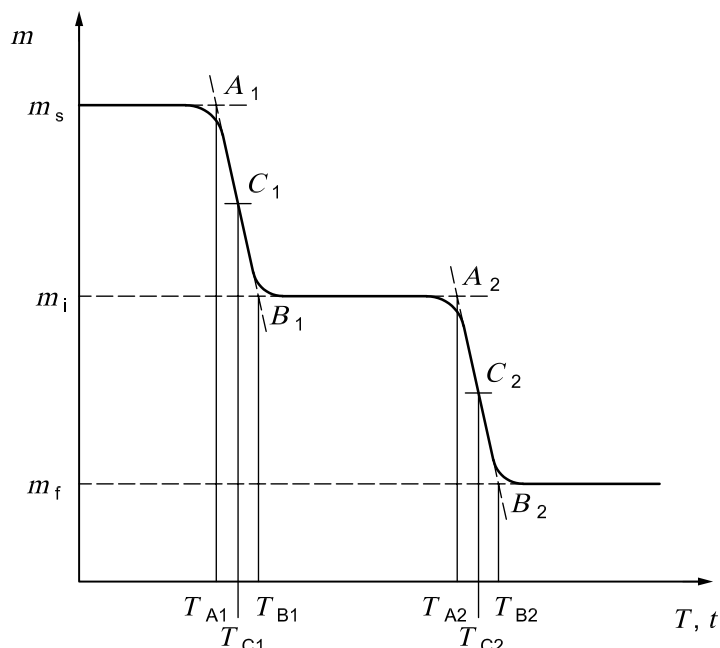

Key

m mass

T temperature


t time

Figure 3 — Example of a TG curve showing a multi-stage decrease in mass

Determine points A_1 , B_1 , C_1 , A_2 , B_2 , C_2 , and so on (if there are more than two stages) as described in [9.3.1](#).

Determine masses m_s , m_i and m_f and temperatures T_{A1} , T_{B1} , T_{C1} , T_{A2} , T_{B2} , T_{C2} , and so on, corresponding to these points.

If the TG curve does not indicate constant mass in the part of the curve between the primary and secondary stage (see [Figure 4](#)), the point of intersection of the tangent to this part of the curve at the point of minimum gradient and the tangent to the first-stage part of the curve at the point of maximum gradient shall be taken as end point of the first stage B_1 and the point of intersection of this minimum-gradient tangent and the maximum-gradient tangent to the second-stage part of the curve shall be taken as starting point of the second stage A_2 . The mass m_i shall be taken as the mid-point between m_{B1} and m_{A2} .

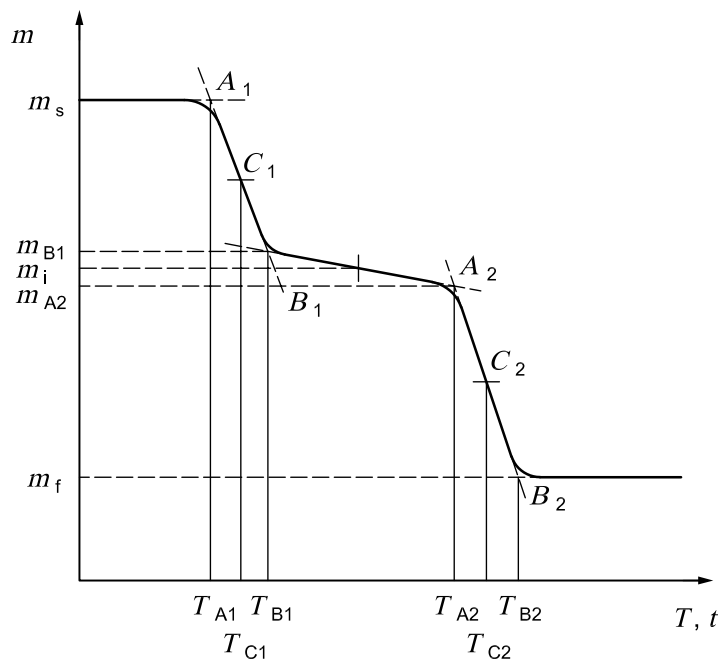

Key

- m mass
- T temperature
- t time

Figure 4 — Example of a TG curve showing a multi-stage decrease in mass where constant mass is not reached between reactions

Calculate the first loss in mass, m_{11} , expressed as a percentage, using Formula (3):

$$m_{11} = \frac{m_s - m_i}{m_s} \times 100 \tag{3}$$

where m_i is the mass, in milligrams, at the first end temperature.

Calculate the second loss in mass, m_{12} , expressed as a percentage, using Formula (4):

$$m_{12} = \frac{m_i - m_f}{m_s} \times 100 \tag{4}$$

Calculate any further losses in mass the same way.

9.3.3 Determination of residue

Calculate the mass of the residue, m_r , expressed as a percentage, using Formula (5)

$$m_r = \frac{m_f}{m_s} \times 100 \tag{5}$$

10 Test report

The test report shall include the following information:

- a) a reference to this part of ISO 11358 (i.e. ISO 11358-1);
- b) all details necessary for complete identification of the material analysed;

- c) the form and dimensions (if applicable) of the test specimen;
- d) the mass of the test specimen;
- e) details of the conditioning of the test specimen prior to the test;
- f) the type of thermobalance used;
- g) the specimen holder size and material of construction;
- h) the type of temperature sensor used and the position (inside or outside the specimen holder);
- i) the atmosphere and gas-flow rate used;
- j) the rate of temperature increase (programmed heating) or isothermal temperature used;
- k) the temperature at which the mass calibration was carried out;
- l) the material(s) used for temperature calibration;
- m) the thermogravimetric diagram;
- n) the mass gain and/or mass loss(es) calculated in [9.2](#), [9.3.1](#) and [9.3.2](#), as applicable;
- o) the residue calculated in [9.3.3](#);
- p) the mass change temperatures T_{A1} , T_{B1} , T_{C1} determined in [9.3.1](#) and [9.3.2](#);
- q) any observations regarding equipment, test conditions or test specimen behaviour;
- r) the date of the test.

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com



...making excellence a habit.™