

Water quality —

Determination of nitrite nitrogen and nitrate nitrogen and the sum of both by flow analysis (CFA and FIA) and spectrometric detection

The European Standard EN ISO 13395:1996 has the status of a British Standard

ICS 13.060

Committees responsible for this British Standard

The preparation of this British Standard was entrusted by Technical Committee EH/3, Water quality, to Subcommittee EH/3/2, Physical, chemical and biochemical methods, upon which the following bodies were represented:

British Agrochemicals Association Ltd.
 British Ceramic Research
 British Gas plc
 British Soft Drinks Association Ltd.
 Chemical Industries' Association
 Convention of Scottish Local Authorities
 Department of the Environment (Her Majesty's Inspectorate of Pollution)
 Department of the Environment (Water Directorate)
 Department of Trade and Industry (Laboratory of the Government Chemist)
 GAMBICA (BEAMA) Ltd.
 Industrial Water Society
 National Rivers Authority
 Royal Society of Chemistry
 Soap and Detergent Industry Association
 Society of Chemical Industry
 Swimming Pool and Allied Trades Association Ltd.
 Water Companies Association
 Water Research Centre
 Water Services Association of England and Wales

This British Standard, having been prepared under the direction of the Health and Environment Sector Board, was published under the authority of the Standards Board and comes into effect on 15 November 1996

© BSI 10-1998

The following BSI references relate to the work on this standard:
 Committee reference EH/3/2
 Draft for comment 94/501676 DC

ISBN 0 580 26092 5

Amendments issued since publication

Amd. No.	Date	Comments

Contents

	Page
Committees responsible	Inside front cover
National foreword	ii
<hr/>	
Foreword	2
1 Scope	3
2 Normative references	3
3 Principle	3
4 Reagents	3
5 Apparatus	6
6 Checking the flow system	7
7 Sampling and sample preparation	7
8 Interferences	7
9 Procedure	7
10 Evaluation	9
11 Expression of results	9
12 Precision	9
13 Test report	13
<hr/>	
Annex A (informative) Examples of flow injection systems (5.1) for the determination of nitrite(N) and nitrite/nitrate(N)	14
Annex B (informative) Examples of continuous flow systems (5.2) for the determination of nitrate(N) and nitrite/nitrate(N)	15
Annex C (informative) Example of a continuous flow system (so-called "macroflow") (5.2) for the determination of 0,2 mg/l to 2 mg/l nitrite/nitrate(N)	16
Annex D (informative) Bibliography	17
<hr/>	
Figure A.1	14
Figure B.1	15
Figure C.1	16
<hr/>	
Table 1 — Options for preparing the solutions C and B in Figure A.1, Figure B.1 and Figure C.1	4
Table 2 — Preparation of the calibration solutions for nitrite(N)	5
Table 3 — Preparation of the calibration solutions for nitrite/nitrate(N)	6
Table 4 — Statistical data for the determination of nitrite(N) with flow injection analysis (FIA)	10
Table 5 — Statistical data for the determination of nitrite(N) with continuous flow analysis (CFA)	11
Table 6 — Statistical data for the determination of nitrite/nitrate(N) with flow injection analysis (FIA)	12
Table 7 — Statistical data for the determination of nitrite/nitrate(N) with continuous flow analysis (CFA)	13
<hr/>	
List of references	Inside back cover
<hr/>	

National foreword

This British Standard has been prepared by Subcommittee EH/3/2 and is the English language version of EN ISO 13395:1996 *Water quality — Determination of nitrite nitrogen and nitrate nitrogen and the sum of both by flow analysis (CFA and FIA) and spectrometric detection* published by the European Committee for Standardization (CEN). It is identical with ISO 13395:1996 published by the International Organization for Standardization (ISO).

NOTE The tests described in this British Standard should only be carried out by suitably qualified persons with an appropriate level of chemical expertise. Standard chemical procedures should be followed throughout.

Cross-references

Publication referred to	Corresponding British Standard
ISO 3696:1987	BS EN ISO 3696:1995 <i>Water for analytical laboratory use. Specification and test methods</i> BS EN 25667 <i>Water quality. Sampling</i>
ISO 5667-1:1980	Part 1:1994 <i>Guidance on the design of sampling programmes</i>
ISO 5667-2:1991	Part 2:1993 <i>Guidance on sampling techniques</i>
ISO 5667-3:1994	BS 6068 <i>Water quality</i> Part 6 <i>Sampling</i> Section 6.3:1996 <i>Guidance on the preservation and handling of samples</i>
ISO 6777:1984	BS EN 26777:1993 <i>Water quality. Physical, chemical and biochemical methods. Determination of nitrite: molecular absorption spectrometric method</i>

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

Summary of pages

This document comprises a front cover, an inside front cover, pages i and ii, the EN title page, pages 2 to 18, an inside back cover and a back cover.

This standard has been updated (see copyright date) and may have had amendments incorporated. This will be indicated in the amendment table on the inside front cover.

ICS:13.060.00

Descriptors: Water, quality, water pollution, water tests, chemical analysis, determination of content, nitrogen, nitrates, nitrites.

English version

Water quality — Determination of nitrite nitrogen and nitrate nitrogen and the sum of both by flow analysis (CFA and FIA) and spectrometric detection

Qualité de l'eau — Détermination de l'azote nitreux et de l'azote nitrique et de la somme des deux par analyse en flux (CFA et FIA) et détection spectrométrique

(ISO 13395:1996)

This European Standard was approved by CEN on 1996-06-09. CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

CEN

European Committee for Standardization
Comité Européen de Normalisation
Europäisches Komitee für Normung

Central Secretariat: rue de Stassart 36, B-1050 Brussels

Foreword

The text of the International Standard ISO 13395:1996 has been prepared by Technical Committee ISO/TC 147, Water quality, in collaboration with Technical Committee CEN/TC 230, Water analysis, the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by January 1997 and conflicting national standards shall be withdrawn at the latest by January 1997.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

1 Scope

This International Standard specifies a method for the determination of nitrite(N) (see note 2), nitrate(N) or the sum of both [nitrite/nitrate(N)], in various types of waters (such as ground, drinking, surface, and waste waters) in mass concentrations ranging from 0,01 mg/l to 1 mg/l for nitrite(N) and from 0,2 mg/l to 20 mg/l for nitrite/nitrate(N), both in the undiluted sample. The range of application can be changed by varying the operating conditions.

NOTE 1 Seawater may be analysed with changes in respect to sensitivity and adaptation of the carrier solution and calibration solutions to the salinity of the samples.

NOTE 2 The following concise terms are used in the text of this International Standard:

nitrite(N):	(mass concentration of) nitrite, expressed as nitrogen
nitrate(N):	(mass concentration of) nitrate, expressed as nitrogen
nitrite(N)/nitrate(N):	(mass concentration of) the sum of nitrite(N) and nitrate(N)

2 Normative references

The following standards contain provisions which, through reference in this text, constitute provisions of this International Standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this International Standard are encouraged to investigate the possibility of applying the most recent editions of the standards indicated below. Members of IEC and ISO maintain registers of currently valid International Standards.

ISO 3696:1987, *Water for analytical laboratory use — Specification and test methods*.

ISO 5667-1:1980, *Water quality — Sampling — Part 1: Guidance on the design of sampling programmes*.

ISO 5667-2:1991, *Water quality — Sampling — Part 2: Guidance on sampling techniques*.

ISO 5667-3:1994, *Water quality — Sampling — Part 3: Guidance on the preservation and handling of samples*.

ISO 6777:1984, *Water quality — Determination of nitrite — Molecular absorption spectrometric method*.

3 Principle

3.1 Sum of nitrite(N) and nitrate(N), nitrite/nitrate(N)

With flow injection analysis (FIA), the sample is fed into a continuously flowing buffer solution (carrier stream) by means of an injection valve, or, with continuous flow analysis (CFA) being applied, it is continuously mixed with this buffer solution.

Nitrate in the sample is reduced with metallic cadmium to nitrite^[4]. Then, a phosphoric acid reagent solution that is also flowing continuously is admixed. Nitrite that is initially present and nitrite resulting from the reduction of nitrate will diazotize sulfanilamide in acid solution to the diazonium salt which is then coupled with *N*-(1-naphthyl)ethylenediamine to form a red dye ^{[5][6][7]}.

Waste containing cadmium in liquid or solid form shall be removed appropriately.

3.2 Nitrite(N)

Nitrite(N) is determined, omitting the cadmium reduction, directly by the above-mentioned diazotization and coupling reaction^[8]. The chemical reactions of the nitrite are identical with those in the manual procedure (see ISO 6777).

3.3 Nitrate(N)

The mass concentration of nitrate(N) is given by the difference: nitrite/nitrate(N) – nitrite(N).

4 Reagents

If not stated otherwise, only reagents of recognized analytical grade and water according to grade 1 of ISO 3696 shall be used. The blank value of the reagents shall be checked regularly (see 9.3).

4.1 *Phosphoric acid* (H₃PO₄), ρ = 1,71 g/ml.

4.2 *Sulfanilamide* (4-aminobenzenesulfonamide, C₆H₈N₂O₂S).

4.3 *N*-(1-naphthyl)ethylenediaminedihydrochloride [*N*-(1-naphthyl)-1,2-diaminoethanedihydrochloride], C₁₂H₁₆N₂Cl₂].

4.4 *Sodium nitrite* (NaNO₂), dried to constant mass at, for example, 150 °C.

4.5 *Potassium nitrate* (KNO₃), dried to constant mass at, for example, 150 °C.

4.6 *Imidazole* (C₃H₄N₂), for synthesis, or alternatively **ammonium chloride** (NH₄Cl), dried to constant mass at 105 °C (see note 3).

4.7 *Hydrochloric acid I* (HCl) concentrated, w = 37 %.

4.8 Hydrochloric acid II, $c(\text{HCl}) = 1 \text{ mol/l}$.

4.9 Copper sulfate solution I,
 $\rho(\text{CuSO}_4 \cdot 5\text{H}_2\text{O}) = 2,5 \text{ g/l}$; this solution is stable.

4.10 Copper sulfate solution II,
 $\rho(\text{CuSO}_4 \cdot 5\text{H}_2\text{O}) = 20 \text{ g/l}$; this solution is stable.

4.11 Polyethyleneglycol dodecyl ether
 $[\text{HO} - (\text{CH}_2\text{CH}_2 - \text{O})_n - \text{C}_{12}\text{H}_{21}]$,
 surfactant, $\theta = 33 \text{ }^\circ\text{C}$ to $41 \text{ }^\circ\text{C}$, solution, $w = 30 \%$.
 The solution is stable for approximately 4 weeks.

4.12 Cadmium granulate (Cd), grain size, for example 0,3 mm to 1,5 mm (a minimum reduction capacity of 90 % shall be reached; see **5.1** and **5.2**).

4.13 Imidazole stock solution, $c = 0,25 \text{ mol/l}$.

Dissolve, in a beaker of nominal capacity 1 litre, 17,0 g of imidazole (**4.6**) in approximately 900 ml of water.

While stirring with a magnetic stirrer, add hydrochloric acid I (**4.7**) and adjust, with the help of a pH electrode, the pH to **7.5**.

Transfer to a volumetric flask, of nominal capacity 1 000 ml, and dilute to volume with water. The solution is stable for 4 weeks if kept in a brown glass bottle at room temperature.

4.14 Buffer solution

Mix 100 ml of the imidazole stock solution (**4.13**) with 100 μl of copper sulfate solution I (**4.9**).

Prepare the solution freshly before use.

NOTE 3 Alternatively an ammonium buffer solution can be used, for example:

85 g of ammonium chloride (NH_4Cl) should be dissolved in water and diluted to a volume of 1 000 ml, and the pH should be adjusted to approximately 7,5.

4.15 Carrier or dilution solutions, C and B in Figure A.1, Figure B.1 and Figure C.1.

Table 1 shows some well-known options for preparing these solutions.

Prepare the solutions, containing the surfactant (**4.11**), freshly before use.

Prior to use, solutions C and B for FIA shall be degassed, for example by membrane filtration (vacuum).

Table 1 — Options for preparing the solution C and B in Figure A.1, Figure B.1 and Figure C.1

Method	Parameter	Content of solution C (see Figure A.1, Figure B.1 and Figure C.1)	Contents of solution B (see Figure A.1, Figure B.1 and Figure C.1)
FIA	Nitrite	Water	Water ^a Buffer (4.14) ^a No solution B ^a
	Nitrite/nitrate	Buffer (4.14)	Buffer (4.14)
CFA	Nitrite	"C" is not necessary	Water ^{a,b} Buffer (4.14) ^{a,b} No solution B ^{a,b}
	Nitrite/nitrate	"C" is not necessary	Buffer (4.14) ^b

^a Three different alternatives.
^b If, in the case of CFA, water or buffer (4.14) is used as solution B and 1 ml of surfactant (4.11) per 1 litre of solution is added. If solution B is omitted, the surfactant (4.11) has to be added to the reagent solution R₁ (4.17, see Figure A.1, Figure B.1 and Figure C.1).

4.16 Buffered copper sulphate solution

Mix 20 ml of the copper sulfate solution II (**4.10**) and 20 ml of the imidazole stock solution (**4.13**) in a beaker of nominal capacity 50 ml.

Prepare the solution freshly before use.

4.17 Reagent solution, R₁ (in Figure A.1, Figure B.1 and Figure C.1).

Dissolve, in a volumetric flask of nominal capacity 500 ml, 5 g of sulfanilamide (**4.2**), 0,5 g of *N*-(1-naphthyl)ethylenediaminedihydrochloride (**4.3**) in water, add 50 ml of phosphoric acid (**4.1**), and dilute to volume.

Stored in a brown glass bottle, the solution is stable for at least one week.

NOTE 4 For the preparation of this reagent solution, hydrochloric acid (**4.7**, **4.8**) may be used instead of phosphoric acid, provided equivalent performance characteristics are obtained. The solutions of sulfanilamide (**4.2**) and *N*-(1-naphthyl)ethylenediaminedihydrochloride (**4.3**) can also be made separately and dosed into the equipment by different lines.

Prior to use, solution R₁ for FIA shall be degassed, for example by membrane filtration (vacuum).

4.18 Nitrite(N) stock solution, $\rho_N = 100$ mg/l.

Dissolve 492,6 mg of sodium nitrite (4.4) in water, in a volumetric flask of nominal capacity 1 000 ml, and dilute to volume.

This solution is stable for at least 2 weeks if kept in a stoppered glass bottle at 4 °C.

4.19 Nitrite(N) solution I, $\rho_N = 20$ mg/l.

Pipette 20 ml of the stock solution (4.18) into a volumetric flask of nominal capacity 100 ml, and dilute to volume with water.

Prepare the solution freshly before use.

4.20 Nitrite(N) solution II, $\rho_N = 1$ mg/l.

Pipette 1 ml of the stock solution (4.18) into a volumetric flask of nominal capacity 100 ml, and dilute to volume with water.

Prepare the solution freshly before use.

4.21 Nitrate(N) solution I, $\rho_N = 200$ mg/l.

Dissolve 144,4 mg of potassium nitrate (4.5) in water, in a volumetric flask of nominal capacity 100 ml, and dilute to volume.

The solution is stable for at least 1 month.

4.22 Nitrate(N) solution II, $\rho_N = 20$ mg/l.

Pipette 10 ml of the nitrate solution I (4.21) into a volumetric flask of nominal capacity 100 ml, and dilute to volume with water.

Prepare the solution freshly before use.

4.23 Calibration solutions

The calibration solutions are prepared by diluting the respective solutions described in 4.19 to 4.22.

These solutions may be used in any combination for the preparation of calibration solutions for the determination of nitrite(N), nitrite/nitrate(N) or nitrate(N). At least five calibration standards per working range are recommended.

The following working ranges are provided:

For nitrite(N): Working range II:
0,01 mg/l to 0,1 mg/l
Working range I:
0,1 mg/l to 1,0 mg/l

For nitrite/nitrate(N): Working range II:
0,2 mg/l to 2 mg/l
Working range I: 2 mg/l
to 20 mg/l

Proceed, for example, as recommended in Table 2 and Table 3 (if 10 standards are used).

All calibration solutions shall be prepared immediately before measurement.

Table 2 — Preparation of the calibration solutions for nitrite(N)

Nitrite(N) concentration mg/l	Volume of nitrite(N) solution II (4.20) diluted with water to 100 ml ml	Nitrite(N) concentration mg/l	Volume of nitrite(N) solution I (4.19) diluted with water to 200 ml ml
0,01	1	0,1	1
0,02	2	0,2	2
0,03	3	0,3	3
0,04	4	0,4	4
0,05	5	0,5	5
0,06	6	0,6	6
0,07	7	0,7	7
0,08	8	0,8	8
0,09	9	0,9	9
0,10	10	1,0	10

Table 3 — Preparation of the calibration solutions for nitrite/nitrate(N)

Nitrate(N) concentration mg/l	Volume of nitrate(N) solution II (4.22) diluted with water to 100 ml ml	Nitrate(N) concentration mg/l	Volume of nitrate(N) solution I (4.21) diluted with water to 100 ml ml
0,2	1	2	1
0,4	2	4	2
0,6	3	6	3
0,8	4	8	4
1,0	5	10	5
1,2	6	12	6
1,4	7	14	7
1,6	8	16	8
1,8	9	18	9
2,0	10	20	10

5 Apparatus

Usual laboratory apparatus and

5.1 Flow injection system (FIA), normally comprising the following components (see Figure A.1).

- Reagent reservoirs.
- Low pulsation pump.
- Suitable pump tubing, if required.
- Sample injector with an injection volume of 10 µl to 300 µl.
- If nitrite/nitrate(N) or nitrate(N) is to be determined: cadmium reductor with a minimum reduction efficiency of 90 %, e.g. packed cadmium column with granulate (4.12), of internal diameter 4,0 mm, for example, and minimum length 5 cm.
- Transport tubes and reaction coils of internal diameter 0,5 mm to 0,8 mm, with tube connections and T-connections of chemically inert plastics.
- Dialysis cell, if required, with, for example, a cellulose membrane, suitable for the predilution of the sample or the elimination of interfering compounds.

NOTE 5 The dialysis cell should be placed after the injector (see Figure A.1). The carrier solution C may serve as a donor and also as a recipient solution. The flow rates of these two streams should be equal.

- Photometric detector with flow cell, wavelength range 520 nm to 560 nm.
- Recording unit (e.g. strip chart recorder, integrator or printer/plotter). In general, peak height signals are evaluated.
- Autosampler, if required.

5.2 Continuous flow analysis (CFA), normally comprising the following components (see Figure B.1):

- Autosampler or any other device allowing a reproducible application of the sample.
- Reagent reservoirs.
- Low pulsation pump with suitable, chemically inert pump tubes.
- If nitrite/nitrate(N) or nitrate(N) is to be determined: cadmium reductor with a minimum reduction efficiency of 90 %, e.g. cadmium tube ^[10] of internal diameter 1,1 mm or cadmium column (see 5.1).
- Manifold with highly reproducible gas-bubble feeding (nitrogen is recommended), sample and reagent feeding, with appropriate transport systems and connection assemblies of chemically inert plastics or metal. The application of the cadmium reductor requires oxygen-free gas. Before entering the cadmium column the flow stream has to be debubbled, if air is used for segmenting the flow stream.
- Dialysis cell, if required, with, for example, a cellulose membrane, suitable for the predilution of the sample or the elimination of interfering compounds.
- Photometric detector with flow cell, wavelength range 520 nm to 560 nm.
- Recording unit (e.g. strip chart recorder, integrator or printer/plotter). In general, peak height signals are evaluated.

NOTE 6 Figure B.1 describes two flow systems with an internal diameter of approximately 1 mm. Figure C.1 shows a flow system (for the determination of nitrite/nitrate(N) with an internal diameter of 2,2 mm.

5.3 Volumetric flasks, of nominal capacity 100 ml, 500 ml and 1 000 ml.

5.4 Pipettes, of nominal capacity 100 µl, 1 ml to 10 ml, 20 ml, 50 ml and 100 ml.

5.5 Beakers, of nominal capacity 25 ml, 50 ml and 1 litre.

5.6 Syringe, of nominal capacity 25 ml.

5.7 Membrane filter assembly, with membrane filters of pore size 0,45 µm.

5.8 pH electrode

6 Checking the flow system

A calibration solution (4.23) with a nitrite(N) concentration of 0,05 mg/l, or a nitrate(N) concentration of 1 mg/l, measured in the system (FIA or CFA, respectively) which is adjusted to the lower working range, should give an absorbance of at least 0,04 per 10 mm path length.

NOTE 7 If the photometric detector (see 5.1 or 5.2) does not give any absorbance readings, the absorbance may then be determined by comparing with an external absorbance-measuring photometer.

7 Sampling and sample preparation

Before use, all containers coming into contact with the sample shall be cleaned thoroughly with water and shall be rinsed several times with the samples. (See ISO 5667-3.)

If only nitrite is to be determined, collect the sample in a glass or polyethylene bottle and analyse it at once. Proceed in the same way, if nitrate is to be determined and if the nitrite(N) concentration is at least in the same working range as the nitrate(N) concentration.

If only nitrite/nitrate(N) is to be determined, or nitrate(N) in samples with nitrite(N) concentrations below the respective nitrite/nitrate(N) working range, sample containers made of polyalkylene and polytetrafluoroethylene (PTFE) are also suitable. Acidify these samples with hydrochloric acid (4.7 and 4.8) to approximately pH 2, store at 2 °C to 5 °C and analyse within 24 h.

As an exception, the samples may be stored in the freezer at approximately – 20 °C for 8 d, provided the applicability of this preservation has previously been checked.

Provided that significant loss of nitrate/nitrite is excluded, filtration of the sample is necessary if it contains particulate matter of a particle size > 0,1 mm (risk of clogging the transport tubes).

8 Interferences

8.1 Interferences of a general nature

Nitrite cannot be stabilized and shall immediately be analysed (see clause 7).

Particulate matter present in the sample may lead to clogging of the transport tubes and will interfere with the photometric measurement. Larger particles (> 0,1 mm) can be removed by membrane filtration, smaller particles can be removed suitably by dialysis.

In order to remove an interfering organic matrix (compounds with a higher molar mass), the sample may be dialysed, if need be in an online process. As an alternative, the sample may be filtered through activated carbon, provided changes of the nitrite or nitrate mass concentration in the sample can be ruled out.

The self-absorption of the sample can be compensated by measuring, in addition to the sample signal (9.5), the signal of the sample without the admixture of the reagents. In this case, the difference of the two responses is used for the evaluation (according to clause 10).

Prior to the measurement, dilute samples with a total salt concentration of > 30 g/l.

8.2 Interference with the reduction of nitrate to nitrite

Interferences may occur if the sample, after the admixture of the buffer solution, does not reach a pH of 6,5 to 7,5. This may happen with strongly acid, basic or buffered samples. In this event, the sample shall, prior to the measurement, be treated appropriately with bases or acids so as to reach the above mentioned pH in the solution streaming through the cadmium reductor (see 5.1 and 5.2).

8.3 Interferences with the formation of the azo dye

Surfactant concentrations > 10 mg/l may interfere with the determination; this interference can be prevented by a dialysis of the sample, if need be in the online process. (See [9] in annex D.)

9 Procedure

9.1 Preparation, activation and checking of the cadmium reductor

9.1.1 Cadmium column with granulate

Place a sufficient quantity of the cadmium granulate (4.12) to fill the column (see 5.1) in a beaker (5.5) of nominal capacity 25 ml. Stir with hydrochloric acid II (4.8) until the surface of the granulates shows a metallic shine.

Remove the acid by washing with water.

Decant the water and stir the granulate twice for approximately 2 min with copper sulfate solution II (4.10). The surface of the granulate will turn black.

Decant and carefully wash with water.

Fill the column with the granulate, avoiding air bubbles and large cavities, and stopper the ends of the column (e.g. with glass wool).

Assemble the column in the flow system, and activate the reductor by applying nitrate(N) solution I (4.21) or II (4.22) three times.

Repeatedly measure the calibration solution (4.23) which has, for the respective working range, the highest permissible nitrite/nitrate(N) concentration (2 mg/l or 20 mg/l, respectively), until stable results are obtained.

NOTE 8 The cadmium column can be stored, free from air bubbles, in the imidazole stock solution (4.13). Prior to re-use, the column should be stabilized and activated as described above.

9.1.2 Cadmium tube

Using the syringe (5.6), aspirate approximately 5 ml of the buffered copper sulfate solution (4.16) into the cadmium tube (see 5.2) and allow to react for 5 min. Repeat the procedure, avoiding air bubbles.

Using the syringe, aspirate approximately 20 ml of imidazole stock solution (4.13) through the tube and allow to react, avoiding air bubbles.

Assemble the column in the flow system, activate and stabilize as described in 9.1.1.

NOTE 9 The cadmium tube can be stored, free from air bubbles, in the imidazole stock solution (4.13). Prior to measurement, stabilize or treat, if required, (see 9.1.3) with buffered copper sulfate solution (4.16).

9.1.3 Checking the reduction capacity [applies to the nitrate(N) or the nitrite/nitrate(N) determination only]

Sequentially analyse a nitrate(N) and a nitrite(N) solution with a nitrogen mass concentration of 2 mg/l each for the nitrite/nitrate(N) working range II, or of 20 mg/l each for the nitrite/nitrate(N) working range I, and compare the measured values obtained.

Transport reagent solutions (4.17) through the flow system with a built-in cadmium reductor and allow the baseline to stabilize.

For example, to check the nitrite/nitrate(N) working range I, use the nitrite(N) solution I (4.19) and the nitrate(N) solution II (4.22).

If the measured value for nitrate(N) is less than 90 % of the measured nitrite(N) value, appropriate measures according to 9.1.1 and 9.1.2 shall be taken to obtain a reduction capacity of at least 90 %.

Check the reduction capacity again, prior to the analysis of each series of samples.

9.2 Preparation for measurement

Assemble the flow system according to the method of determination desired (FIA or CFA, determination of nitrite/nitrate(N) or nitrite(N); see Figure A.1, Figure B.1 and Figure C.1).

Prior to measurement of nitrite, continuously run the reagent solutions for approximately 10 min through the flow system. For the determination of nitrite/nitrate(N), run the reagent solutions through the system for approximately 10 min without the Cd reductor and after that for approximately 10 min with the Cd reductor. Record and zero the base absorbance.

The system is ready when the baseline no longer shows any drift. A satisfactory signal-noise relation should be obtained. Then perform the reaction steps in the sequence of 9.3 to 9.5.

9.3 Monitoring the blank of the reagents

Allow the baseline to stabilize.

Instead of the buffer solution B (4.15) and the reagent solution R₁ (4.17) transport water for 2 min and record changes in the measuring signal.

If the absorbance changes by more than 0,015 per 10 mm path length, either the water being used or the reagent solutions may be contaminated. Take appropriate measures to eliminate the interference.

Then transport the reagent solutions again.

9.4 Calibration

Select the respective working range for nitrite(N) or nitrite/nitrate(N) and prepare the calibration solutions (4.23) for the selected working range. Each working range requires its own calibration.

Calibrate by sequentially adding the calibration solutions and the blank solution.

Prior to the calibration, zero the instrument, if necessary following the manufacturer's instructions.

Determine the measured values from the calibration solutions used while following the manufacturer's instructions, as long as they do not contradict the specifications of this International Standard.

The test conditions for the calibration and the measurement of samples (9.5) are the same. The magnitude of the measuring signal is proportional to the mass concentration of nitrite(N) or nitrite/nitrate(N). Establish the regression line for the measuring series obtained.

The following general equation is satisfied:

$$y = b p_N + a \quad \dots(1)$$

where

- y is the measured value, in terms of instrument-related units (e.g. peak height in millimetres or millivolts);
- b is the slope of the calibration function, in instrument-related units litre per milligram;
- ρ_N is the mass concentration, in milligrams per litre, of nitrite(N) or nitrite/nitrate(N);
- a is the ordinate intercept of the calibration function, in terms of instrument-related units.

9.5 Sample measurement

Analyse the samples, pretreated according to clause 7, in the same manner as the calibration solutions (4.23), with the flow system (FIA, see 5.1 and Figure A.1; CFA, see 5.2 and Figure B.1 and Figure C.1).

If the mass concentrations to be determined exceed the validity range of the selected working range, dilute the sample or analyse it using the other working range.

Check the validity of the calibration function in the respective working range after each sample series, but at the latest after the measurement of 10 to 20 samples, using one calibration solution each for the lower and upper third of the respective working range. Check the reduction capacity (9.1.3) again or make a new calibration (9.4), if necessary. After measurement, store the cadmium reductor in an imidazole solution that is free from oxygen (see notes 8 or 9).

10 Evaluation

Determine the mass concentration of the determinand in the measuring solution using the measured value obtained as described in 9.5, from the calibration function [equation (1), 9.4].

For the evaluation use the appropriate function. Do not extrapolate beyond the working range selected.

Calculate ρ_N using equation (2):

$$\rho_N = \frac{y-a}{b} \quad \dots(2)$$

where

- ρ_N is the mass concentration, in milligrams per litre, of nitrite(N) or nitrite/nitrate(N) in the sample;

y , a and b are as defined in equation (1).

11 Expression of results

Report the results to a maximum of two significant figures.

EXAMPLES

Nitrite(N):	$2,9 \times 10^{-1}$ mg/l
Nitrate(N):	3,0 mg/l
Nitrite/nitrate(N)	4,1 mg/l

12 Precision

The statistical data in Table 4 to Table 7 were established in an interlaboratory trial, carried out in November 1991^[11]:

Table 4 — Statistical data for the determination of nitrite(N) with flow injection analysis (FIA)

Sample No.	Type of matrix	<i>l</i>	<i>n</i>	<i>o</i> %	<i>x</i> _{corr} mg/l	\bar{x} mg/l	RR %	<i>s</i> _r mg/l	VC _r %	<i>s</i> _R mg/l	VC _R %
1	Potable water ^{ab}	15	55	0	0,030	0,030	101	0,000 8	2,67	0,001 6	5,41
2		15	49	11	0,090	0,089	99,1	0,000 8	0,90	0,001 5	1,73
3		15	54	5,3	0,300	0,301	100	0,004 1	1,36	0,015 0	4,98
4		15	49	11	0,900	0,898	99,8	0,006 5	0,72	0,033 8	3,76
5	Industrial waste water ^{cb}	15	55	0	0,030	0,033	109	0,002 0	6,06	0,004 4	13,6
6		15	54	1,8	0,090	0,092	102	0,003 0	3,26	0,005 4	5,88
7		15	53	3,6	0,300	0,296	98,8	0,005 2	1,76	0,025 1	8,48
8		15	53	3,6	0,900	0,912	101	0,006 1	0,67	0,084 6	9,28
9	Standard solutions ^{db}	15	50	9,1	0,030	0,030	101	0,000 6	2,00	0,001 2	3,92
10		15	55	3,5	0,090	0,091	102	0,001 6	1,76	0,004 3	4,73
11		15	55	3,5	0,300	0,302	101	0,004 1	1,36	0,014 0	4,65
12		15	48	13	0,900	0,900	100	0,007 2	0,80	0,028 1	3,13

l is the number of laboratory sets

n is the number of outlier-free individual analytical values

o is the relative portion of the outliers

*x*_{corr} is the correct value, by convention

\bar{x} is the total mean

RR is the recovery rate

*s*_r is the repeatability standard deviation

VC_r is the repeatability coefficient of variation

*s*_R is the reproducibility standard deviation

VC_R is the reproducibility coefficient of variation

^a Drinking water, spiked with nitrite or nitrate solution.

^b Drinking water, waste water, as well as the spiked solutions, were stabilized with 2 ml/l each of chloroform and were shipped in separate bottles to the participants of the interlaboratory trial.

^c Industrial waste water, spiked with nitrite or nitrate solution in the participant's laboratory. In addition, the waste water contained 14 g/l of chloride and a COD of 1 400 mg/l.

^d Water as in 2), spiked with nitrite or nitrate solution in the participant's laboratory.

Table 5 — Statistical data for the determination of nitrite(N) with continuous flow analysis (CFA)

Sample No.	Type of matrix	<i>l</i>	<i>n</i>	<i>o</i> %	x_{corr} mg/l	\bar{x} mg/l	RR %	s_r mg/l	VC_r %	s_R mg/l	VC_R %
1	Potable water ^{ab}	11	42	0	0,030	0,031	102	0,001 7	5,48	0,002 6	8,43
2		11	42	0	0,090	0,092	102	0,002 3	2,50	0,005 6	6,12
3		11	39	2,5	0,300	0,307	102	0,005 5	1,79	0,035 4	11,6
4		11	30	25	0,900	0,910	101	0,006 4	0,70	0,017 3	1,90
5	Industrial waste water ^{cb}	11	33	21	0,030	0,035	117	0,001 5	4,29	0,003 8	10,8
6		11	41	0	0,090	0,104	115	0,008 9	8,56	0,014 2	13,7
7		11	36	10	0,300	0,327	109	0,005 1	1,56	0,023 4	7,16
8		11	40	0	0,900	0,969	108	0,014 4	1,49	0,094 0	9,70
9	Standard solutions ^{db}	11	39	7,1	0,030	0,031	102	0,001 8	5,81	0,002 5	8,21
10		11	42	0	0,090	0,090	100	0,005 0	5,56	0,007 6	8,46
11		11	40	0	0,300	0,307	102	0,004 0	1,30	0,029 8	9,73
12		11	36	10	0,900	0,907	101	0,014 3	1,58	0,055 0	6,07

l is the number of laboratory sets

n is the number of outlier-free individual analytical values

o is the relative portion of the outliers

x_{corr} is the correct value, by convention

\bar{x} is the total mean

RR is the recovery rate

s_r is the repeatability standard deviation

V_r is the repeatability coefficient of variation

s_R is the reproducibility standard deviation

V_R is the reproducibility coefficient of variation

^a Drinking water, spiked with nitrite or nitrate solution.

^b Drinking water, waste water, as well as the spiked solutions, were stabilized with 2 ml/l each of chloroform and were shipped in separate bottles to the participants of the interlaboratory trial.

^c Industrial waste water, spiked with nitrite or nitrate solution in the participant's laboratory. In addition, the waste water contained 14 g/l of chloride and a COD of 1 400 mg/l.

^d Water as in 2), spiked with nitrite or nitrate solution in the participant's laboratory.

Table 6 — Statistical data for the determination of nitrite/nitrate(N) with flow injection analysis (FIA)

Sample No.	Type of matrix	<i>l</i>	<i>n</i>	<i>o</i> %	x_{corr} mg/l	\bar{x} mg/l	RR %	s_r mg/l	VC_r %	s_R mg/l	VC_R %
1	Potable water ^{ab}	15	56	0	3,230	3,295	102	0,039 1	1,19	0,149 1	4,52
2		15	56	1,8	3,790	3,888	103	0,041 1	1,06	0,144 7	3,72
3		15	57	0	6,000	6,155	103	0,085 0	1,38	0,250 0	4,06
4		15	46	15	12,60	12,67	101	0,195 8	1,55	0,336 1	2,65
5	Industrial waste water ^{cb}	15	52	5,5	0,530	0,550	104	0,016 9	3,07	0,050 0	9,09
6		15	52	5,5	1,090	1,107	102	0,015,3	1,38	0,081 1	7,33
7		15	56	1,8	3,300	3,261	98,8	0,035 0	1,07	0,255 2	7,83
8		15	50	7,4	9,900	10,04	101	0,107 4	1,07	0,465 9	4,64
9	Standard solutions ^{db}	15	48	11	0,530	0,533	101	0,006 6	1,24	0,023 5	4,40
10		15	52	5,5	1,090	1,098	101	0,018 1	1,65	0,035 7	3,25
11		15	52	8,8	3,300	3,261	98,8	0,066 3	2,03	0,181 9	5,58
12		15	41	24	9,900	9,948	101	0,071 6	0,72	0,191 7	1,93

l is the number of laboratory sets

n is the number of outlier-free individual analytical values

o is the relative portion of the outliers

x_{corr} is the correct value, by convention

\bar{x} is the total mean

RR is the recovery rate

s_r is the repeatability standard deviation

VC_r is the repeatability coefficient of variation

s_R is the reproducibility standard deviation

VC_R is the reproducibility coefficient of variation

^a Drinking water, spiked with nitrite or nitrate solution.

^b Drinking water, waste water, as well as the spiked solutions, were stabilized with 2 ml/l each of chloroform and were shipped in separate bottles to the participants of the interlaboratory trial.

^c Industrial waste water, spiked with nitrite or nitrate solution in the participant's laboratory. In addition, the waste water contained 14 g/l of chloride and a COD of 1 400 mg/l.

^d Water as in 2), spiked with nitrite or nitrate solution in the participant's laboratory.

Table 7 — Statistical data for the determination of nitrite/nitrate(N) with continuous flow analysis (CFA)

Sample No.	Type of matrix	<i>l</i>	<i>n</i>	<i>o</i> %	x_{corr} mg/l	\bar{x} mg/l	RR %	s_r mg/l	VC_r %	s_R mg/l	VC_R %
1	Potable water ^{ab}	10	36	0	3,230	3,321	103	0,082 2	2,48	0,133 5	4,02
2		10	36	0	3,790	3,945	104	0,075 9	1,92	0,165 0	4,18
3		10	36	0	6,000	6,117	102	0,165 5	2,70	0,385 3	6,30
4		10	30	21	12,60	12,94	103	0,229 5	1,77	0,344 8	2,66
5	Industrial waste water ^{cb}	10	36	0	0,530	0,576	109	0,042 6	740	0,116 8	20,3
6		10	32	11	1,090	1,112	102	0,047 6	4,28	0,111 9	10,1
7		10	34	5,6	3,300	3,401	103	0,077 6	2,28	0,139 5	4,10
8		10	34	11	9,900	10,16	103	0,167 0	1,64	0,638 7	6,29
9	Standard solutions ^{db}	10	34	5,6	0,530	0,521	98,2	0,022 5	4,32	0,045 6	8,75
10		10	30	17	1,090	1,060	97,2	0,039 3	3,71	0,053 4	5,04
11		10	29	19	3,300	3,222	97,6	0,088 7	2,75	0,099 2	3,08
12		10	26	32	9,900	10,00	101	0,100 9	1,01	0,158 9	1,59

l is the number of laboratory sets

n is the number of outlier-free individual analytical values

o is the relative portion of the outliers

x_{corr} is the correct value, by convention

\bar{x} is the total mean

RR is the recovery rate

s_r is the repeatability standard deviation

VC_r is the repeatability coefficient of variation

s_R is the reproducibility standard deviation

VC_R is the reproducibility coefficient of variation

^a Drinking water, spiked with nitrite or nitrate solution.

^b Drinking water, waste water, as well as the spiked solutions, were stabilized with 2 ml/l each of chloroform and were shipped in separate bottles to the participants of the interlaboratory trial.

^c Industrial waste water, spiked with nitrite or nitrate solution in the participant's laboratory. In addition, the waste water contained 14 g/l of chloride and a COD of 1 400 mg/l.

^d Water as in 2), spiked with nitrite or nitrate solution in the participant's laboratory.

13 Test report

The test report shall contain the following information:


- a reference to this International Standard;
- identity of the water sample;
- specification of the procedure applied (CFA or FIA);
- description of the sample pretreatment;
- description of the type of instrument or of the flow conditions;
- expression of the results according to clause 11;

g) precision and trueness of the results, if available;

h) any deviation from this method and all events which may have influenced the result.

Annex A (informative)

Examples of flow injection systems (5.1) for the determination of nitrite(N) and nitrite/nitrate(N)

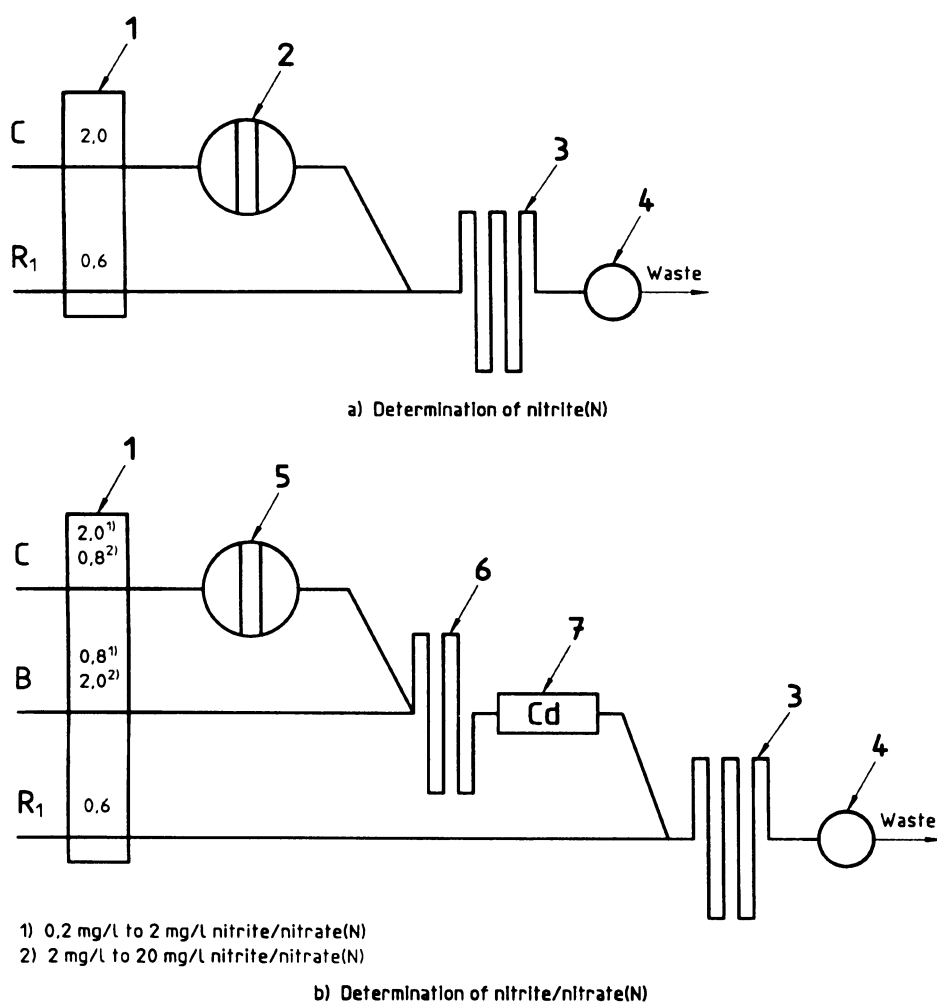

1) 0.2 mg/l to 2 mg/l nitrite/nitrate(N)
 2) 2 mg/l to 20 mg/l nitrite/nitrate(N)

Key

- | | | | |
|----------------|---|---|---|
| B | Buffer solution (4.14, 4.15) | 4 | Detector (1 cm)
520 nm to 560 nm |
| C | Carrier solution (4.15) | 5 | Injector |
| R ₁ | Reagent solution (4.17) | | 10 µl to 40 µl [2 mg/l to 20 mg/l nitrite/nitrate(N)]
100 µl [0,2 mg/l to 2 mg/l nitrite/nitrate(N)] |
| 1 | Pump (flow rate in ml/min) | 6 | Reaction coil
l 30 cm/ø int. 0,5 mm |
| 2 | Injector | 7 | Cadmium reductor
e.g. Cd column
l 5 cm/ø int. 4 mm |
| | 100 µl [0,1 mg/l to 1,0 mg/l nitrite(N)]
300 µl [0,01 mg/l to 0,1 mg/l nitrite(N)] | | |
| 3 | Reaction coil
l 90 cm/ø int. 0,5 mm | | |

Figure A.1

Annex B (informative)

Examples of continuous flow systems (5.2) for the determination of nitrate(N) and nitrite/nitrate(N)

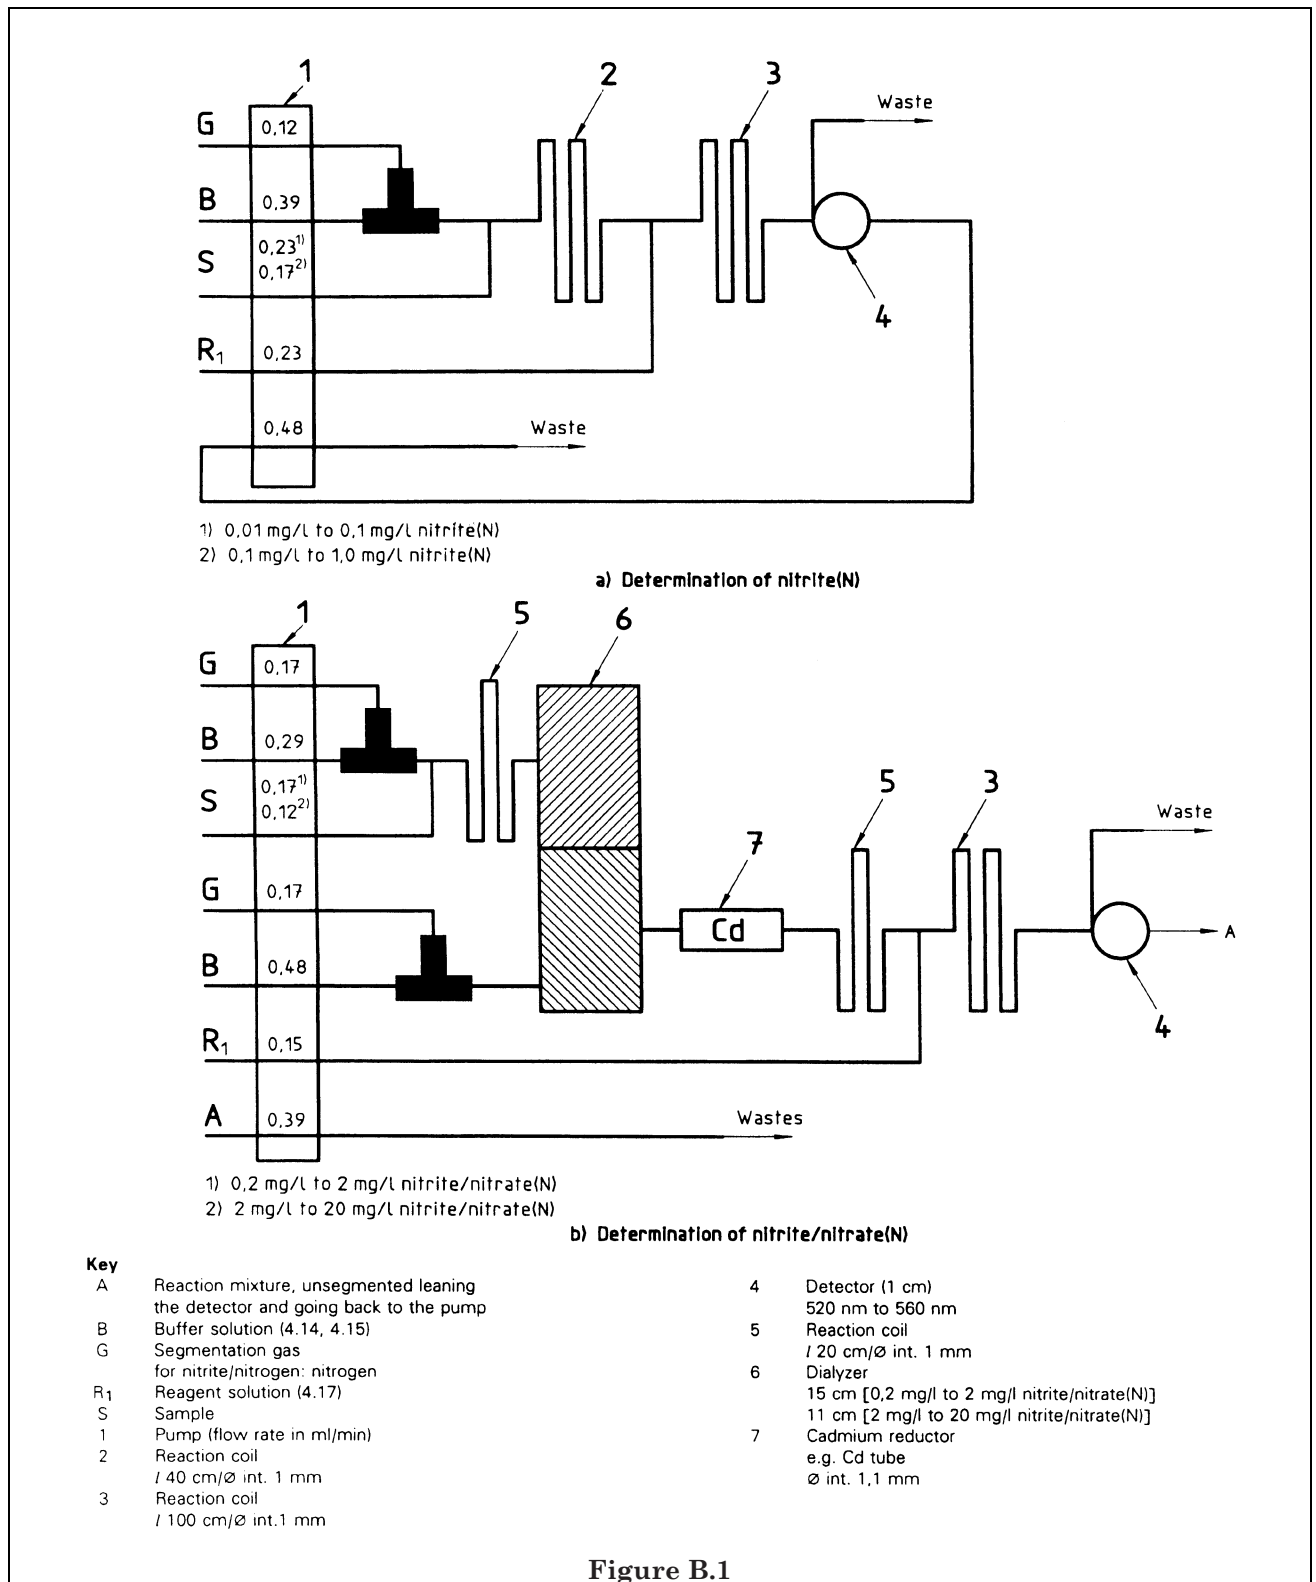


Figure B.1

Annex C (informative)

Example of a continuous flow system (so-called "macroflow") (5.2) for the determination of 0,2 mg/l to 2 mg/l nitrite/nitrate(N)

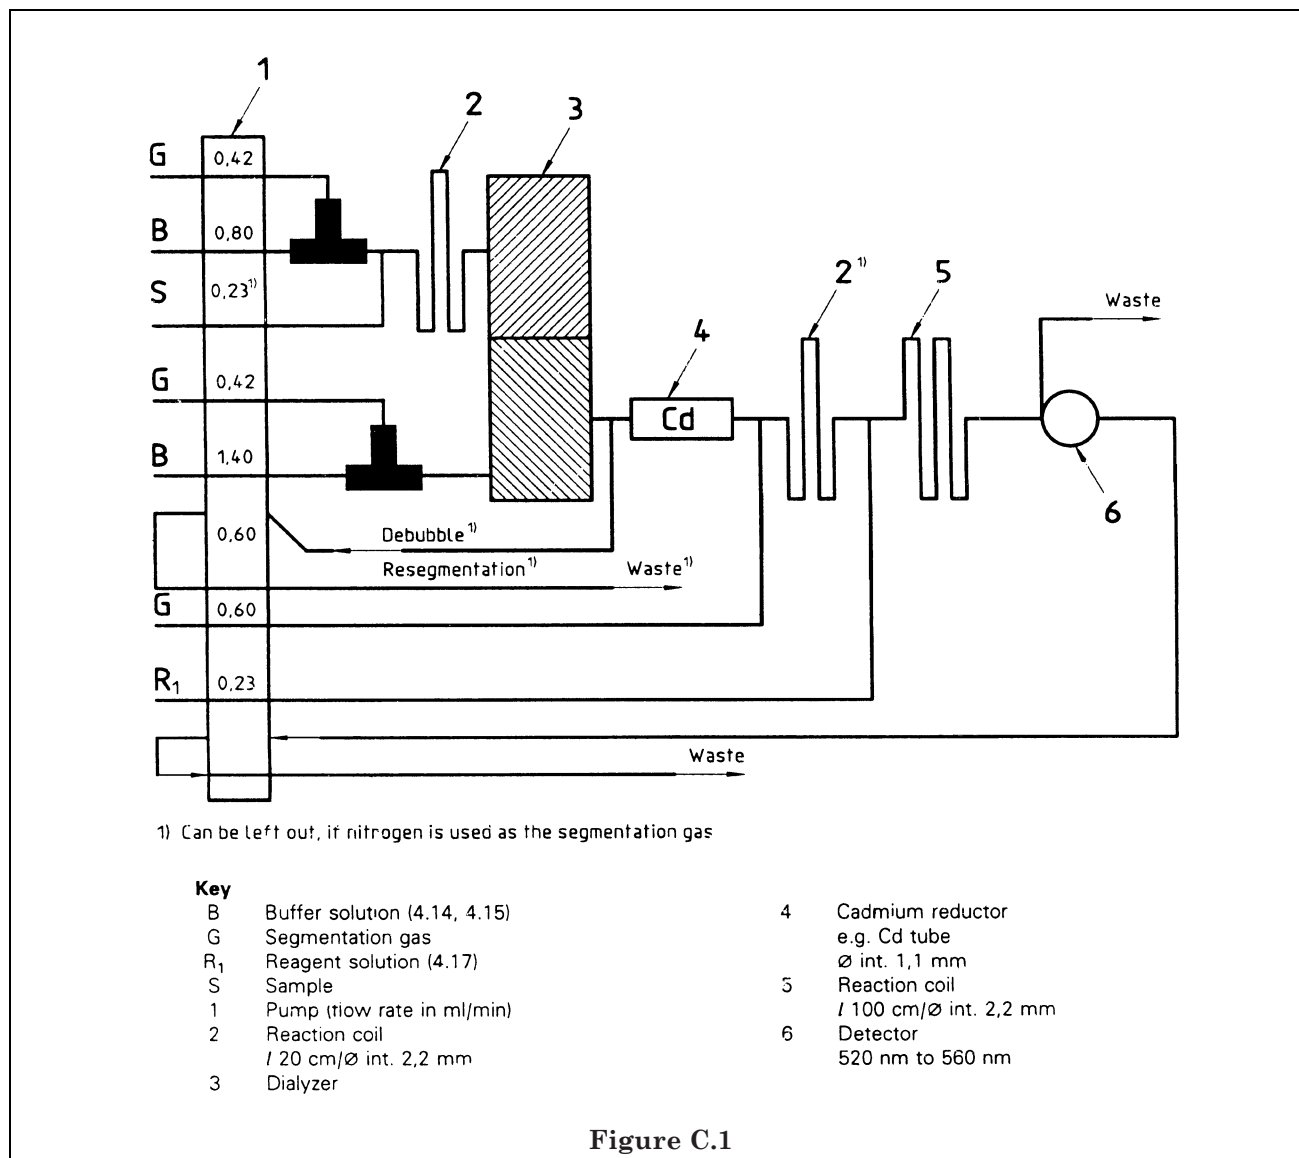


Figure C.1

Annex D (informative)

Bibliography

- [1] RUZICKA, J. and HANSEN, E.H. *Flow Injection Analysis*. Wiley & Sons (2nd Edition), (1988).
- [2] MÖLLER, J. *Flow Injection Analysis, Analytiker Taschenbuch*, Bd. 7 (Springer Verlag (1988), pp. 199-275; and Karlberg B. and Pacey G.E. *Flow Injection Analysis – A Practical Guide*. Elsevier, Amsterdam (1989).
- [3] SKEGGS, L.T. *Anal. Chem.* **38(6)** (1966), 31 A.
- [4] NYDAHL, F. *Talanta* **23** (1976), pp 349-357.
- [5] GINE, M.F., BERGAMIN, H., ZAGATTO, E.A.G. and REIS, B.F. *Anal. Chimica Acta*, **114** (1980), pp. 191-197.
- [6] VAN STADEN, J.F., JOUBERT, A.E. and VAN VLIET, H.R. *Fresen. Z. Anal. Chem.* **325** (1986), pp. 150-152.
- [7] L'Association française de normalisation (AFNOR), NF T 90-012 *Essais des eaux — Dosage des nitrates et des nitrites — Méthode automatique par spectrométrie d'absorption moléculaire*, décembre 1987.
- [8] SHINN, M.B. *Industr. Eng. Chem., Anal. Ed.* **13** (1941), p. 33.
- [9] NORWITZ, G. and KELIHER, P.N. *Analyst* **110** (1985), p. 689 and *Analyst* **111** (1986), p. 1033.
- [10] FOX, J.B. *Anal. Chem.* **51** (1979), p. 1493.
- [11] WINTER, B. and PAPKE, G. *Laborpraxis* **16** (1992), p. 804.

List of references

See national foreword.

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre. Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: 020 8996 7002. Fax: 020 8996 7001.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager. Tel: 020 8996 7070.