

Milk and milk products — Determination of nitrate and nitrite contents —

Part 1: Method using cadmium reduction and spectrometry

The European Standard EN ISO 14673-1:2004 has the status of a
British Standard

ICS 67.100.10

National foreword

This British Standard is the official English language version of EN ISO 14673-1:2004. It is identical with ISO 14673-1:2004. It supersedes BS EN ISO 14673-1:2001 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee AW/5, Milk and milk products, which has the responsibility to:

- aid enquirers to understand the text;
- present to the responsible international/European committee any enquiries on the interpretation, or proposals for change, and keep the UK interests informed;
- monitor related international and European developments and promulgate them in the UK.

A list of organizations represented on this committee can be obtained on request to its secretary.

Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the *BSI Catalogue* under the section entitled “International Standards Correspondence Index”, or by using the “Search” facility of the *BSI Electronic Catalogue* or of British Standards Online.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

Summary of pages

This document comprises a front cover, an inside front cover, the EN ISO title page, the EN ISO foreword page, the ISO title page, pages ii to v, a blank page, pages 1 to 13, the Annex ZA page, an inside back cover and a back cover.

The BSI copyright notice displayed in this document indicates when the document was last issued.

Amendments issued since publication

Amd. No.	Date	Comments
15079 Corrigendum No. 1	18 March 2004	Corrected EN ISO foreword page and incorporating the Annex ZA

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 25 February 2004

© BSI 18 March 2004

English version

Milk and milk products - Determination of nitrate and nitrite contents - Part 1: Method using cadmium reduction and spectrometry (ISO 14673-1:2004)

Lait et produits laitiers - Détermination des teneurs en nitrates et en nitrites - Partie 1: Méthode par réduction au cadmium et spectrométrie (ISO 14673-1:2004)

Milch und Milchprodukte - Bestimmung des Nitrat- und Nitritgehaltes - Teil 1: Verfahren mit Cadmiumreduktion und Spektrometrie (ISO 14673-1:2004)

This European Standard was approved by CEN on 2 February 2004.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

CORRECTED 2004-02-25

Foreword

This document (EN ISO 14673-1:2004) has been prepared by Technical Committee ISO/TC 34 "Agricultural food products" in collaboration with Technical Committee CEN/TC 302 "Milk and milk products - Methods of sampling and analysis", the secretariat of which is held by NEN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by August 2004, and conflicting national standards shall be withdrawn at the latest by August 2004.

This document supersedes EN ISO 14673-1:2001.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

Endorsement notice

The text of ISO 14673-1:2004 has been approved by CEN as EN ISO 14673-1:2004 without any modifications.

NOTE Normative references to International Standards are listed in Annex ZA (normative).

INTERNATIONAL
STANDARD

ISO
14673-1

IDF
189-1

Second edition
2004-02-01

**Milk and milk products — Determination
of nitrate and nitrite contents —**

Part 1:

**Method using cadmium reduction and
spectrometry**

*Lait et produits laitiers — Détermination des teneurs en nitrates et en
nitrites —*

Partie 1: Méthode par réduction au cadmium et spectrométrie



Reference numbers
ISO 14673-1:2004(E)
IDF 189-1:2004(E)

Contents

Page

Foreword.....	iv
1 Scope.....	1
2 Normative references	1
3 Terms and definitions	2
4 Principle	2
5 Reagents	2
6 Apparatus.....	4
7 Sampling	5
8 Preparation of test sample	5
8.1 Dried milk and dried whey.....	5
8.2 Caseins and caseinates.....	5
8.3 Cheese.....	6
8.4 Whey cheese	6
9 Procedure.....	6
9.1 Preparation of the copperized cadmium column	6
9.2 Checking the reducing capacity of the column	6
9.3 Regeneration of the column.....	7
9.4 Preparation of test portion	7
9.5 Extraction and deproteination	8
9.6 Reduction of nitrate to nitrite.....	8
9.7 Blank test	9
9.8 Determination	9
9.9 Preparation of calibration graph	9
10 Calculation and expression of results	9
10.1 Nitrite content	9
10.2 Nitrate content.....	10
11 Precision	10
11.1 General	10
11.2 Repeatability.....	10
12 Test report.....	11
Bibliography	13

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 14673-1|IDF 189-1 was prepared by Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 5, *Milk and milk products*, and the International Dairy Federation (IDF), in collaboration with AOAC International. It is being published jointly by ISO and IDF and separately by AOAC International.

This second edition cancels and replaces the first edition (ISO 14673-1|IDF 189-1:2001), of which it constitutes a minor revision.

ISO 14673|IDF 189 consists of the following parts, under the general title *Milk and milk products — Determination of nitrate and nitrite contents*:

- *Part 1: Method using cadmium reduction and spectrometry*
- *Part 2: Method using segmented flow analysis (Routine method)*
- *Part 3: Method using cadmium reduction and flow injection analysis with in-line dialysis (Routine method)*

Foreword

IDF (the International Dairy Federation) is a worldwide federation of the dairy sector with a National Committee in every member country. Every National Committee has the right to be represented on the IDF Standing Committees carrying out the technical work. IDF collaborates with ISO and AOAC International in the development of standard methods of analysis and sampling for milk and milk products.

Draft International Standards adopted by the Action Teams and Standing Committees are circulated to the National Committees for voting. Publication as an International Standard requires approval by at least 50 % of the National Committees casting a vote.

ISO 14673-1|IDF 189-1 was prepared by Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 5, *Milk and milk products*, and the International Dairy Federation (IDF), in collaboration with AOAC International. It is being published jointly by ISO and IDF and separately by AOAC International.

All work was carried out by the Joint ISO/IDF/AOAC Action Team *Minerals and minor compounds*, of the Standing Committee on *Minor components characterization of physical properties*, under the aegis of its project leader, Mr G. Bråthen (NO).

This second edition, together with ISO 14673-2|IDF 189-2 and ISO 14673-3|IDF 189-3, cancels and replaces IDF 84A:1984, IDF 95A:1982, IDF 96A:1987, IDF 97A:1985 and IDF 120:1984, which have been technically revised.

Milk and milk products — Determination of nitrate and nitrite contents —

Part 1: Method using cadmium reduction and spectrometry

WARNING — The use of this International Standard may involve hazardous materials, operations and equipment. This standard does not purport to address all the safety problems associated with its use. It is the responsibility of the user of this standard to establish safety and health practices and determine the applicability of regulatory limitations prior to use.

1 Scope

This part of ISO 14673|IDF 189 specifies a method for the determination of the nitrate and nitrite contents of milk and milk products by cadmium reduction and spectrometry. The method is applicable to

- whole and partly skimmed and skimmed dried milk;
- hard, semi-hard and soft cheeses;
- processed cheese;
- whey cheese, caseins and caseinates, and dried whey.

The method may be performed using automatic equipment, in particular by segmented flow analysis (SFA) or flow injection analysis (FIA), thus reducing cadmium contamination in laboratory work places and waste water.

NOTE These methods are described in ISO 14673-2|IDF 189-2 and ISO 14673-3|IDF 189-3, respectively.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 565, *Test sieves — Metal wire cloth, perforated metal plate and electroformed sheet — Nominal sizes of openings*

ISO 648, *Laboratory glassware — One-mark pipettes*

ISO 835-1, *Laboratory glassware — Graduated pipettes — Part 1: General requirements*

ISO 1042, *Laboratory glassware — One-mark volumetric flasks*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

nitrate content

mass fraction of nitrate determined by the procedure specified in this part of ISO 14673|IDF 189

NOTE The nitrate content is expressed as the mass in milligrams of nitrate ions (NO_3^-) per kilogram of product.

3.2

nitrite content

mass fraction of nitrite determined by the procedure specified in this part of ISO 14673|IDF 189

NOTE The nitrite content is expressed as the mass in milligrams of nitrite ions (NO_2^-) per kilogram of product.

4 Principle

A test portion is dispersed in warm water, with precipitation of the fat and proteins, then filtration. The nitrate ions are reduced to nitrite ions in a portion of the filtrate by means of copperized cadmium.

A red colour is developed in portions of both unreduced filtrate and the reduced solution, by addition of sulfanilamide and *N*-1-naphthyl ethylenediamine dihydrochloride. Spectrometric measurements are carried out at a wavelength of 538 nm.

The nitrite content of the sample and the total nitrite content after reduction of nitrate ions are calculated by comparing the measured absorbances with those of a set of sodium nitrite calibration solutions. The nitrate content is calculated from the difference between these two contents.

5 Reagents

Use only reagents of recognized analytical grade unless otherwise specified.

5.1 Water, distilled or deionized, or water of equivalent purity, free from nitrate and nitrite ions.

To avoid the possible inclusion of small gas bubbles in the copperized cadmium column (9.1.6), freshly boil the distilled or deionized water and cool to room temperature. Use the thus-prepared water for the preparation of the column (9.1), to check the reducing capacity of the column (9.2), and to regenerate the column (9.3).

5.2 Cadmium granules, of diameter 0,3 mm to 0,8 mm.

Prepare cadmium granules, if not available commercially, as follows.

Place a suitable number of zinc rods in a beaker. Cover the rods with cadmium sulfate solution (5.3). Scrape the cadmium sponge from the rods from time to time over a period of 24 h. Remove the zinc rods and decant the liquid until only sufficient remains to cover the cadmium sponge. Wash the sponge two or three times with water. Transfer the cadmium sponge to a laboratory blender together with 400 ml of the hydrochloric acid working solution (5.7) and blend for a few seconds to obtain granules of the required size. Return the contents of the blender to the beaker and leave to stand for several hours, while stirring occasionally to remove bubbles. Decant most of the liquid and immediately copperize the granules as described in 9.1.

WARNING — Because of its toxicity, the used cadmium should be delivered as chemical waste to the relevant authorities.

5.3 Cadmium sulfate solution, $c(\text{CdSO}_4 \cdot 8\text{H}_2\text{O}) = 40 \text{ g/l}$.

Dissolve 40 g of cadmium sulfate solution in water in a 1 000 ml volumetric flask (6.4). Dilute to the mark with water and mix.

5.4 Copper(II) sulfate solution, $c(\text{CuSO}_4 \cdot 5\text{H}_2\text{O}) = 20 \text{ g/l}$.

Dissolve 20 g of copper(II) sulfate in water in a 1 000 ml volumetric flask (6.4). Dilute to the mark with water and mix.

5.5 Hydrochloric acid (HCl), ($\rho_{20} = 1,19 \text{ g/ml}$).**5.6 Dilute hydrochloric acid**, $c(\text{HCl}) \approx 2 \text{ mol/l}$.

Carefully add 160 ml of hydrochloric acid (5.5) to about 700 ml of water in a 1 000 ml volumetric flask (6.4) while regularly swirling the contents. Cool the contents to room temperature. Dilute to the mark with water and mix carefully.

5.7 Hydrochloric acid working solution, $c(\text{HCl}) \approx 0,1 \text{ mol/l}$.

Add 50 ml of dilute hydrochloric acid (5.6) to a 1 000 ml volumetric flask (6.4). Dilute to the mark with water and mix.

5.8 Zinc sulfate solution, $c(\text{ZnSO}_4 \cdot 7\text{H}_2\text{O}) = 535 \text{ g/l}$.

Dissolve 53,5 g of zinc sulfate in water in a 100 ml volumetric flask (6.4). Dilute to the mark with water and mix.

5.9 Potassium hexacyanoferrate(II) solution, $c(\text{K}_4[\text{Fe}(\text{CN})_6] \cdot 3\text{H}_2\text{O}) = 172 \text{ g/l}$.

Dissolve 17,2 g of potassium hexacyanoferrate(II) trihydrate in water in a 100 ml volumetric flask (6.4). Dilute to the mark with water and mix.

5.10 Disodium ethylenediaminetetraacetate dihydrate (EDTA) solution ($\text{Na}_2\text{C}_{10}\text{H}_{14}\text{N}_2\text{O}_8 \cdot 2\text{H}_2\text{O}$).

Dissolve 33,5 g of EDTA in about 900 ml water in a 1 000 ml volumetric flask (6.4). Dilute to the mark with water and mix.

5.11 Solution I.

Carefully add 450 ml of hydrochloric acid (5.5) to a 1 000 ml volumetric flask (6.4). Dilute to the mark with water and mix.

5.12 Solution II.

Dissolve by heating on a water bath (6.15) 0,5 g of sulfanilamide ($\text{NH}_2\text{C}_6\text{H}_4\text{SO}_2\text{NH}_2$) in a mixture of 75 ml of water and 5 ml of hydrochloric acid (5.5) in a 100 ml volumetric flask (6.4). Cool to room temperature. Dilute to the mark with water and mix. Filter the obtained solution, if necessary.

5.13 Solution III.

Dissolve 0,1 g of *N*-1-naphthyl ethylenediamine dihydrochloride ($\text{C}_{10}\text{H}_7\text{NHCH}_2\text{CH}_2\text{NH}_2 \cdot 2\text{HCl}$) in water in a 100 ml volumetric flask (6.4). Dilute to the mark with water and mix. Filter the obtained solution, if necessary.

The solution may be stored for up to 1 week in a well-stoppered brown bottle in a refrigerator.

5.14 Sodium nitrite stock solution (NaNO_2).

Dry a few grams of sodium nitrite in an oven (6.16) at 110 °C to 120 °C to constant mass (i.e. until the difference between two successive weighings does not exceed 1 mg). Dissolve 0,150 g of the sodium nitrite in water in a 1 000 ml volumetric flask (6.4). Dilute to the mark with water and mix.

5.15 Sodium nitrite working solution.

Prepare the sodium nitrite working solution on the day of use. Transfer with a pipette (6.5), 10 ml of the stock solution (5.14) and 20 ml of the buffer solution (5.19) to a 1 000 ml volumetric flask (6.4). Dilute to the mark with water and mix. The nitrite content of the sodium nitrite working solution is 1 µg/ml.

5.16 Potassium nitrate stock solution (KNO₃).

Dry a few grams of potassium nitrate in an oven (6.16) at 110 °C to 120 °C to constant mass (i.e. until the difference between two successive weighings does not exceed 1 mg). Dissolve 1,468 g of the potassium nitrate in water in a 1 000 ml volumetric flask (6.4). Dilute to the mark with water and mix.

5.17 Potassium nitrate working solution.

Prepare the potassium nitrate working solution on the day of use. Transfer with a pipette (6.5), 5 ml of the potassium nitrate stock solution (5.16) and 20 ml of the buffer solution (5.19) to a 1 000 ml volumetric flask (6.4). Dilute to the mark with water and mix. The nitrate content of the potassium nitrate working solution is 4,50 µg/ml.

5.18 Ammonia solution (NH₃), ($\rho_{20} = 0,91$ g/ml).

If an ammonia solution of above-mentioned concentration is not available, an equivalent amount of a more concentrated ammonia solution may be used in 5.19 [e.g. 103 ml of a 35 % (mass fraction) ammonia solution ($\rho_{20} = 1,19$ g/ml)].

5.19 Buffer solution, pH 9,6 to 9,7.

Dilute 50 ml of hydrochloric acid (5.5) with 600 ml of water in a conical flask (6.3) and mix. Add 135 ml of the ammonia solution (5.18) and dilute to 1 000 ml with 215 ml of water and mix. Adjust the pH, if necessary, to between 9,6 and 9,7.

6 Apparatus

Clean all glassware thoroughly and rinse with distilled water to ensure that it is free from nitrate and nitrite ions.

Usual laboratory equipment and, in particular, the following.

6.1 Analytical balance, capable of weighing to the nearest 1 mg, with a readability of 0,1 mg.

6.2 Sample container, provided with an airtight lid.

6.3 Conical flasks, of capacity 250 ml, 500 ml and 1 000 ml.

6.4 Volumetric flasks, of nominal capacity 100 ml, 500 ml and 1 000 ml, complying with the requirements of ISO 1042, class B.

6.5 Pipettes, capable of delivering 2 ml, 4 ml, 5 ml, 6 ml, 8 ml, 10 ml, 12 ml, 20 ml and 25 ml, complying with the requirements of ISO 648, class A, or ISO 835-1. Where appropriate, burettes may be used instead of pipettes.

6.6 Measuring cylinders, of capacities 5 ml, 10 ml, 25 ml, 100 ml, 250 ml, 500 ml and 1 000 ml.

6.7 Glass funnels, of diameter 7 cm, with short stem.

6.8 Filter paper, medium grade, of diameter about 15 cm, free from nitrate and nitrite ions.

6.9 Reduction column, made of glass, an example of which is given in Figure 1.

6.10 Spectrometer, suitable for measuring absorbance at a wavelength of 538 nm, with cells of optical path length 1 cm to 2 cm.

6.11 Grinding device, appropriate for grinding the test sample, if necessary. To avoid loss of moisture, the device should not produce undue heat. A hammer shall not be used.

6.12 Laboratory mixer or homogenizer, with glass containers of capacity 250 ml or 400 ml, suitable for suspending test portions of cheese and whey cheese.

6.13 Test sieve, of woven wire cloth, of diameter 200 mm, nominal size of openings 500 μm , and a receiver complying with the requirements of ISO 565.

6.14 Magnetic stirrer.

6.15 Water bath, capable of boiling water.

6.16 Oven, capable of maintaining a temperature of between 110 °C and 120 °C.

7 Sampling

Sampling is not part of the method specified in this part of ISO 14673|IDF 189. A recommended sampling method is given in ISO 707.

It is important that the laboratory receive a sample which is truly representative and has not been damaged or changed during transport or storage.

Store the test sample in such a way that deterioration and change in composition are prevented.

8 Preparation of test sample

8.1 Dried milk and dried whey

Transfer the test sample to a sample container (6.2) of capacity about twice the volume of the test sample. Close the container immediately. Mix the test sample thoroughly by repeatedly shaking and inverting the container until a homogeneous sample is obtained.

8.2 Caseins and caseinates

8.2.1 Thoroughly mix the test sample, if necessary after transferring all of it to a sample container (6.2) of suitable capacity, by repeatedly shaking and inverting the container.

8.2.2 Transfer 50 g of the test sample to the test sieve (6.13). If the 50 g portion passes directly through the sieve, or almost completely, pass the whole mixed test sample (8.2.1) through the sieve.

8.2.3 If the test sample does not pass completely through the sieve, use the grinding device (6.11) to achieve that condition. Immediately transfer all the sieved test sample to the sample container (6.2) and mix thoroughly in the closed container. During these operations, take precautions to avoid any change in the water content of the product.

8.2.4 After the test sample has been prepared, proceed with the preparation of the test portion (9.4) as soon as possible.

8.3 Cheese

8.3.1 Prior to analysis, remove the rind or mouldy surface layer of the test sample so as to provide a test sample representative of the cheese as it is usually consumed.

8.3.2 Grind the test sample by means of an appropriate device (6.11). Mix the ground mass quickly and, if possible, grind a second time and again mix thoroughly. Clean the device after grinding of each sample. If the test sample cannot be ground, mix it thoroughly by intensive stirring and kneading.

8.3.3 As soon as possible after grinding, transfer the test sample to an airtight sample container (6.2) to await the determination which, preferably, should be carried out immediately. If a delay is unavoidable, take all precautions to ensure proper conservation of the test sample and to prevent moisture collecting on the inside surface of the container.

8.3.4 Do not examine ground cheese showing unwanted mould growth or beginning to deteriorate.

8.4 Whey cheese

Prepare the test sample as specified in 8.3.2.

9 Procedure

9.1 Preparation of the copperized cadmium column

9.1.1 Transfer an amount of cadmium granules (5.2) of 40 g to 60 g for each column to a 250 ml conical flask (6.3). Add sufficient hydrochloric acid working solution (5.7) to cover the cadmium. Swirl for a few minutes.

9.1.2 Decant the solution (9.1.1). Wash the cadmium in the conical flask with water until it is free from chloride ions (i.e. until reaction with silver nitrate is negative).

9.1.3 Copperize the cadmium granules by adding the copper(II) sulfate solution (5.4), of which about 2,5 ml of copper solution per gram of cadmium is needed. Swirl for 1 min.

9.1.4 Decant the solution (9.1.3) and wash the copperized cadmium immediately with water, taking care that the cadmium is continuously covered with water. Terminate the washing when the wash water is free from precipitated copper.

9.1.5 Fit a glass wool plug to the bottom of the glass column (6.9) intended to contain the copperized cadmium (see Figure 1). Fill the glass column with water.

9.1.6 Transfer the copperized cadmium to the glass column with minimum exposure to air. The height of the copperized cadmium shall be 15 cm to 20 cm. Avoid trapping air bubbles between the copperized cadmium granules. The level of the liquid shall not fall below the top of the copperized cadmium.

9.1.7 Condition the newly prepared column by running through it a mixture of 750 ml of water, 225 ml of the potassium nitrate working solution (5.17), 20 ml of the buffer solution (5.19) and 20 ml of the EDTA solution (5.10), at a flow rate not exceeding 6 ml/min. Wash the column with 50 ml of water.

9.2 Checking the reducing capacity of the column

9.2.1 Check the reducing capacity of the column at least twice a day, but also at the beginning and at the end of a series of determinations.

9.2.2 Pipette 20 ml of the potassium nitrate working solution (5.17) into the reservoir on top of the column. Immediately add 5 ml of the buffer solution (5.19) to the contents of the reservoir. Run the contents of the reservoir through the column at a flow rate not exceeding 6 ml/min. Collect the eluate in a 100 ml volumetric flask (6.4).

9.2.3 When the reservoir of the reduction column is nearly empty, wash the walls of the reservoir with about 15 ml of water. Repeat the washing with another 15 ml of water after the water has run off. When the second washing has run into the column, completely fill the reservoir with water. Run the complete contents of the reservoir through the column at maximum flow rate. Collect nearly 100 ml of the eluate.

9.2.4 Remove the 100 ml volumetric flask (9.2.3). Dilute its contents to the mark with water and mix well.

9.2.5 Pipette 10 ml of the eluate (9.2.4) into another 100 ml volumetric flask (6.4). Dilute the eluate to about 60 ml with water and mix. Proceed as specified in 9.7 to 9.9.

9.2.6 Calculate the percentage reducing capacity of the column (0,067 μg of NO_2^- per millilitre corresponds to 100 % reducing capacity) from the nitrite content obtained in 10.1 of the diluted eluate (9.2.5) and that determined from the calibration graph (9.9.4). If the reducing capacity is less than 95 %, regenerate the column as specified in 9.3.

9.3 Regeneration of the column

9.3.1 Regenerate the column at the end of each day of use or, if the check (9.2) indicates a loss of efficiency, more frequently.

9.3.2 Add about 5 ml of the EDTA solution (5.10) and 2 ml of hydrochloric acid working solution (5.7) to 100 ml of water and mix. Run the thus-obtained solution through the column at a flow rate of about 10 ml/min.

9.3.3 When the reservoir is empty, wash the column successively with water, with hydrochloric acid working solution (5.7) and again with water.

9.3.4 If the efficiency of the column still is not satisfactory, repeat the procedure specified in 9.1.7.

9.4 Preparation of test portion

9.4.1 Dried milk

Weigh, to the nearest 1 mg, approximately 10 g of the prepared test sample (8.1). Transfer the test portion quantitatively to a 500 ml conical flask (6.3). Add progressively to the test portion, 136 ml of water preheated to between 50 °C and 55 °C. Disperse the test portion by stirring with a glass rod or by shaking the conical flask.

9.4.2 Dried whey

Weigh, to the nearest 0,1 mg, approximately 5 g of the prepared test sample (8.1). Transfer the test portion quantitatively to a 500 ml conical flask (6.3). Add progressively to the test portion, 136 ml of water preheated to between 50 °C and 55 °C. Disperse the test portion by stirring with a glass rod or by shaking the conical flask. Cover the conical flask with aluminium foil or a watch glass and place it in the water bath (6.15) of boiling water for 15 min. Remove the flask from the water bath and wait until the temperature has dropped to between 50 °C and 60 °C.

9.4.3 Caseins

Weigh, to the nearest 1 mg, approximately 10 g of the prepared test sample (8.2). Transfer the test portion quantitatively to a 500 ml conical flask (6.3). Add progressively to the test portion, 136 ml of water preheated to between 50 °C and 55 °C and 10 ml of buffer solution (5.19). Disperse the test portion by stirring, using the magnetic stirrer (6.14).

9.4.4 Caseinates

Weigh, to the nearest 0,1 mg, approximately 2 g of the prepared test sample (8.2). Transfer the test portion quantitatively to a 500 ml conical flask (6.3). Add progressively to the test portion, 136 ml of water preheated

to between 50 °C and 55 °C and 10 ml of buffer solution (5.19). Disperse the test portion by stirring, using the magnetic stirrer (6.14).

9.4.5 Cheese

Weigh, to the nearest 1 mg, approximately 10 g of the prepared test sample (8.3). Transfer the test portion quantitatively to the glass container of the laboratory mixer or homogenizer (6.12). Add progressively to the test portion, 144 ml of water preheated to between 50 °C and 55 °C. Mix in the mixer or homogenizer (6.12) until the test portion is well suspended.

9.4.6 Whey cheese

Weigh, to the nearest 1 mg, approximately 5 g of the prepared test sample (8.4). Transfer the test portion quantitatively to the glass container of the laboratory mixer or homogenizer (6.12). Add progressively to the test portion, 134 ml of water preheated to between 50 °C and 55 °C. Mix in the mixer or homogenizer (6.12) until the test portion is well suspended.

9.5 Extraction and deproteination

9.5.1 Dried milk, dried whey, caseins and caseinates, and whey cheese

9.5.1.1 Add to the test portion (9.4.1, 9.4.2, 9.4.3, 9.4.4 or 9.4.6 respectively), in the following order, 12 ml of zinc sulfate solution (5.8), 12 ml of potassium hexacyanoferrate(II) solution (5.9) and 40 ml of buffer solution (5.19), swirling thoroughly after each addition, and mix. In order to obtain a clear filtrate, leave the mixture in the conical flask for at least 15 min, but not longer than 1 h. Then pass through a filter paper (6.8), collecting the filtrate in a 250 ml conical flask (6.3).

9.5.1.2 It is essential to obtain a clear filtrate within the time specified. For this purpose, it may be necessary to use a larger volume of each precipitation reagent (5.8 and 5.9) (for example, if well-matured cheeses are analysed). Reduce the volume of the preheated water accordingly to maintain the volume of filtrate at about 200 ml.

NOTE The total volume of filtrate will be approximately 200 ml. This volume is assumed in the calculation (10.1 and 10.2).

9.5.2 Cheese

Add to the test portion (9.4.5), in the following order, 6 ml of zinc sulfate solution (5.8), 6 ml of potassium hexacyanoferrate(II) solution (5.9) and 40 ml of buffer solution (5.19), swirling thoroughly after each addition, and mix. In order to obtain a clear filtrate, leave the mixture in the glass container for at least 15 min, but not longer than 1 h. Then pass through a filter paper (6.8), collecting the filtrate in a 250 ml conical flask (6.3) (see 9.5.1.2 and note).

9.6 Reduction of nitrate to nitrite

9.6.1 Pipette 20 ml of the filtrate (9.5.1 or 9.5.2) into the reservoir on top of the prepared reduction column (9.1). Add 5 ml of buffer solution (5.19) to the contents of the reservoir. Mix by stirring with a small glass rod. Pass the contents of the reservoir through the column at a flow rate not exceeding 6 ml/min. Collect the eluate in a 100 ml volumetric flask (6.4).

9.6.2 When the reservoir of the reduction column is nearly empty, wash the walls of the reservoir with about 15 ml of water. After the water has run off, repeat the same washing with another 15 ml of water. After the second washing has run into the column, completely fill the reservoir with water. Pass the complete content of the reservoir through the column at maximum flow rate. Collect nearly 100 ml of the eluate in the 100 ml volumetric flask (6.4).

9.6.3 Remove the 100 ml volumetric flask. Dilute its contents to the mark with water and mix well.

9.7 Blank test

Carry out a blank test in parallel with the determination, but replacing the test portion in 9.8.1 by an equal volume of water.

9.8 Determination

9.8.1 Pipette equal volumes (for example 25 ml) of the filtrate obtained in 9.5.1 or 9.5.2 and of the eluate (9.6.3) into separate 100 ml volumetric flasks (6.4). Add water to each of the flasks to obtain a volume of about 60 ml and mix.

9.8.2 Add to the solution in the flask (9.8.1) 6 ml of solution I (5.11) and then 5 ml of solution II (5.12). Mix the solutions carefully and leave the flask protected from direct sunlight at room temperature for 5 min.

9.8.3 Add to the solution in the flask (9.8.2) 2 ml of solution III (5.13). Again mix these solutions carefully and leave the flask protected from direct sunlight at room temperature for 5 min. Dilute the contents of the flask to the 100 ml mark with water and mix.

9.8.4 Measure the absorbance of the solution obtained in 9.8.3 against that of the blank test (9.5) using the spectrometer (6.10) at a wavelength of 538 nm within 15 min.

9.9 Preparation of calibration graph

9.9.1 Pipette 0 ml (blank), 2 ml, 4 ml, 6 ml, 8 ml, 12 ml and 20 ml of the sodium nitrite working solution (5.15) into separate 100 ml volumetric flasks (6.4). Add water to each of the flasks to obtain volumes of about 60 ml.

9.9.2 Proceed as specified in 9.8.2 and 9.8.3.

9.9.3 Using the spectrometer (6.10), measure the absorbances of the sodium nitrite working solutions against that of the blank at a wavelength of 538 nm within 15 min.

9.9.4 Plot the absorbances obtained in 9.9.3 against the nitrite concentrations, in micrograms per millilitre, calculated from the amounts of sodium nitrite working solution added (9.9.1).

10 Calculation and expression of results

10.1 Nitrite content

10.1.1 Calculation of nitrite content

Calculate the nitrite content of the sample, ω_{N1} , using the following equation:

$$\omega_{N1} = \frac{20\,000\ c_1}{mV}$$

where

ω_{N1} is the nitrite content of the sample, in milligrams of nitrite ions per kilogram;

c_1 is the numerical value of the concentration read from the calibration graph, corresponding to the measured absorbance of the test solution (9.8.4), in micrograms of nitrite ions per millilitre;

m is the mass of the test portion (9.4), in grams;

V is the volume of the aliquot portion taken from the filtrate (9.8.1), in millilitres.

10.1.2 Expression of results

Express the results to 1 decimal place.

10.2 Nitrate content**10.2.1 Calculation of nitrate content**

Calculate the nitrate content of the sample, ω_{N2} , using the following equation:

$$\omega_{N2} = 1,35 \left[\left(\frac{100\,000\,c_2}{mV} \right) - \omega_{N1} \right]$$

where

ω_{N2} is the nitrate content of the sample, in milligrams of nitrate ions per kilogram;

c_2 is the numerical value of the concentration read from the calibration graph, corresponding to the measured absorbance of the test solution (9.9.4), in micrograms of nitrite ions per millilitre;

m is the mass of the test portion (9.4), in grams;

V is the volume of the aliquot portion taken from the eluate (9.8.1), in millilitres.

10.2.2 Calculation of nitrate content, considering the reducing capacity of the column

If the reducing capacity of the column is taken into account, calculate the nitrate content of the sample, ω_{N2} , using the following equation:

$$\omega_{N2} = 1,35 \left[\left(\frac{100\,000\,c_2}{mV} \times \frac{100}{r} \right) - \omega_{N1} \right]$$

where r is the numerical value of the reducing capacity of the column at the end of a series of determinations.

10.2.3 Expression of results

Express the results to whole numbers.

11 Precision**11.1 General**

The values for repeatability and reproducibility limits are expressed for the 95 % probability level and may not be applicable to concentration ranges and matrices other than those given.

NOTE The values for repeatability and reproducibility have been adopted from the former International Standards for the determination of nitrite and nitrate content in milk products, ISO 4099, ISO 6736, ISO 6739, ISO 6740 and ISO 8195. These International Standards were cancelled and replaced by ISO 14673-1:2001.

11.2 Repeatability**11.2.1 Nitrites**

The absolute difference between two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, will in not more than 5 % of cases be greater than 1 mg/kg of product.

11.2.2 Nitrates

The absolute difference between two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, will in not more than 5 % of cases be greater than:

- for dried milk, dried whey, caseins, caseinates and cheese with a nitrate content < 30 mg/kg: 3 mg/kg;
- for dried milk, dried whey, caseins, caseinates and cheese with a nitrate content \geq 30 mg/kg: 10 % of the arithmetic mean of the results;
- for whey cheese with a nitrate content < 30 mg/kg: 5 mg/kg;
- for whey cheese with a nitrate content \geq 30 mg/kg: 15 % of the arithmetic mean of the results.

11.2.3 Reproducibility


The absolute difference between two single test results, obtained using the same method on identical test material in different laboratories with different operators using different equipment, will in not more than 5 % of cases be greater than:

- for dried milk with a nitrate content < 30 mg/kg: 8 mg/kg;
- for dried milk with a nitrate content \geq 30 mg/kg: 25 % of the arithmetic mean of the results;
- for dried whey with a nitrate content < 30 mg/kg: 5 mg/kg;
- for dried whey with a nitrate content \geq 30 mg/kg: 15 % of the arithmetic mean of the results;
- for caseins and caseinates: 25 % of the arithmetic mean of the results;
- for cheese with a nitrate content < 30 mg/kg: 6 mg/kg;
- for cheese with a nitrate content \geq 30 mg/kg: 25 % of the arithmetic mean of the results;
- for whey cheese with a nitrate content < 30 mg/kg: 10 mg/kg;
- for whey cheese with a nitrate content \geq 30 mg/kg: 15 % of the arithmetic mean of the results.

12 Test report

The test report shall specify:

- all information necessary for the complete identification of the sample;
- the sampling method used, if known;
- the test method used, with reference to this part of ISO 14673|IDF 189;
- all operating details not specified in this part of ISO 14673|IDF 189, or regarded as optional, together with details of any incidents which may have influenced the result(s);
- the test result(s) obtained or, if the repeatability has been checked, the final quoted results obtained.

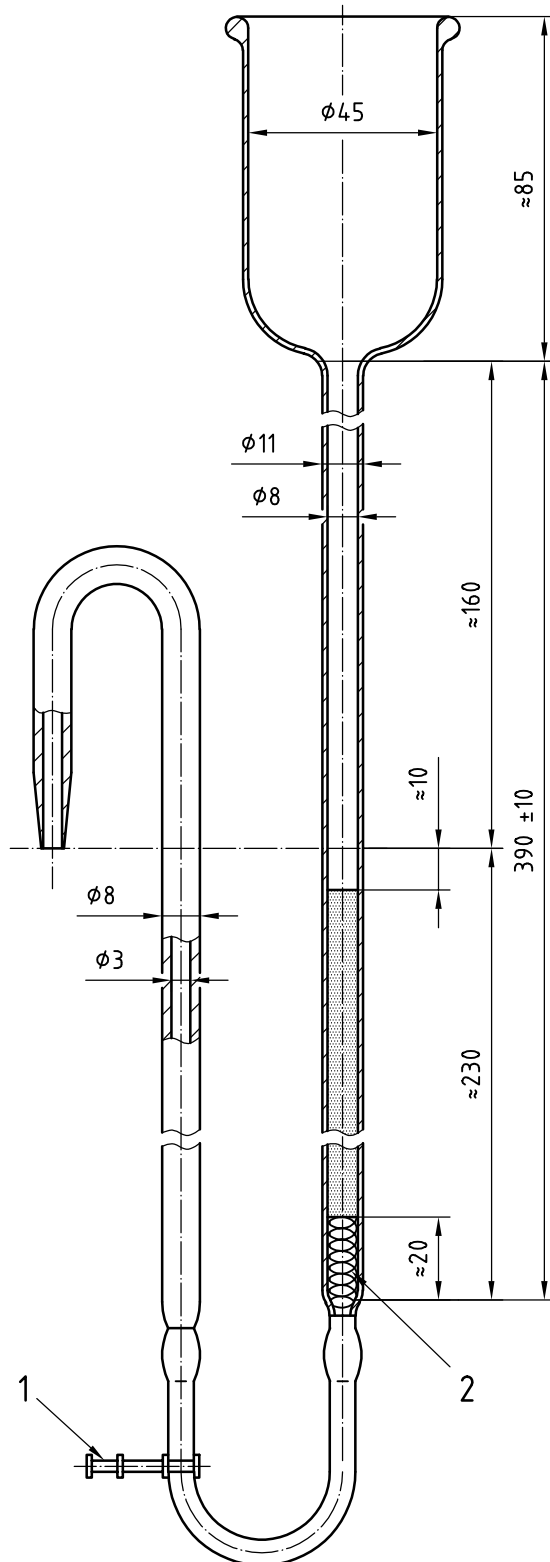

Key

- 1 screw clamp
- 2 glass wool plug

Figure 1 — Apparatus for nitrate reduction

Bibliography

- [1] ISO 707:1997, *Milk and milk products — Guidance on sampling*

Annex ZA
(normative)

**Normative references to international publications
with their relevant European publications**

This European Standard incorporates by dated or undated reference, provisions from other publications. These normative references are cited at the appropriate places in the text and the publications are listed hereafter. For dated references, subsequent amendments to or revisions of any of these publications apply to this European Standard only when incorporated in it by amendment or revision. For undated references the latest edition of the publication referred to applies (including amendments).

NOTE Where an International Publication has been modified by common modifications, indicated by (mod.), the relevant EN/HD applies.

<u>Publication</u>	<u>Year</u>	<u>Title</u>	<u>EN</u>	<u>Year</u>
ISO 1042	1998	Laboratory glassware - One-mark volumetric flasks	EN ISO 1042	1999

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001. Email: orders@bsi-global.com. Standards are also available from the BSI website at <http://www.bsi-global.com>.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre. Tel: +44 (0)20 8996 7111. Fax: +44 (0)20 8996 7048. Email: info@bsi-global.com.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002. Fax: +44 (0)20 8996 7001. Email: membership@bsi-global.com.

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsi-global.com/bsonline>.

Further information about BSI is available on the BSI website at <http://www.bsi-global.com>.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright & Licensing Manager. Tel: +44 (0)20 8996 7070. Fax: +44 (0)20 8996 7553. Email: copyright@bsi-global.com.