

# Milk and milk products — Determination of nitrate and nitrite contents —

## Part 3: Method using cadmium reduction and flow injection analysis with in-line dialysis (Routine method)

The European Standard EN ISO 14673-3:2004 has the status of a  
British Standard

ICS 67.100.10

## National foreword

This British Standard is the official English language version of EN ISO 14673-3:2004. It is identical with ISO 14673-3:2004. It supersedes BS EN ISO 14673-3:2001 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee AW/5, Milk and milk products, which has the responsibility to:

- aid enquirers to understand the text;
- present to the responsible international/European committee any enquiries on the interpretation, or proposals for change, and keep the UK interests informed;
- monitor related international and European developments and promulgate them in the UK.

A list of organizations represented on this committee can be obtained on request to its secretary.

### Cross-references

The British Standards which implement international or European publications referred to in this document may be found in the *BSI Catalogue* under the section entitled “International Standards Correspondence Index”, or by using the “Search” facility of the *BSI Electronic Catalogue* or of British Standards Online.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

**Compliance with a British Standard does not of itself confer immunity from legal obligations.**

### Summary of pages

This document comprises a front cover, an inside front cover, the EN ISO title page, the EN ISO foreword page, the ISO title page, pages ii to v, a blank page, pages 1 to 10, an inside back cover and a back cover.

The BSI copyright notice displayed in this document indicates when the document was last issued.

### Amendments issued since publication

Amd. No.	Date	Comments
15081 Corrigendum No. 1	19 March 2004	Corrected EN ISO foreword page

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 25 February 2004

© BSI 19 March 2004

ISBN 0 580 43491 5

English version

Milk and milk products - Determination of nitrate and nitrite contents - Part 3: Method using cadmium reduction and flow injection analysis with in-line dialysis (Routine method) (ISO 14673-3:2004)

Lait et produits laitiers - Détermination des teneurs en nitrates et en nitrites - Partie 3: Méthode par réduction au cadmium et d'analyse par injection de flux avec dialyse en ligne (Méthode de routine) (ISO 14673-3:2004)

Milch und Milchprodukte - Bestimmung des Nitrat- und Nitritgehaltes - Teil 3: Verfahren mit Cadmiumreduktion und Fließinjektionsanalyse mit In-line-Dialyse (Routineverfahren) (ISO14673-3:2004)

This European Standard was approved by CEN on 2 February 2004.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION  
COMITÉ EUROPÉEN DE NORMALISATION  
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

CORRECTED 2004-03-03

## Foreword

This document (EN ISO 14673-3:2004) has been prepared by Technical Committee ISO/TC 34 "Agricultural food products" in collaboration with Technical Committee CEN/TC 302 "Milk and milk products - Methods of sampling and analysis", the secretariat of which is held by NEN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by August 2004, and conflicting national standards shall be withdrawn at the latest by August 2004.

This document supersedes EN ISO 14673-3:2001.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.

## Endorsement notice

The text of ISO 14673-3:2004 has been approved by CEN as EN ISO 14673-3:2004 without any modifications.

INTERNATIONAL  
STANDARD

ISO  
14673-3

IDF  
189-3

Second edition  
2004-02-01

---

---

**Milk and milk products — Determination  
of nitrate and nitrite contents —**

Part 3:

**Method using cadmium reduction and  
flow injection analysis with in-line  
dialysis (Routine method)**

*Lait et produits laitiers — Détermination des teneurs en nitrates et en  
nitrites —*

*Partie 3: Méthode par réduction au cadmium et d'analyse par injection  
de flux avec dialyse en ligne (Méthode de routine)*



Reference numbers  
ISO 14673-3:2004(E)  
IDF 189-3:2004(E)



## Contents

Page

Foreword .....	iv
1 Scope .....	1
2 Normative references .....	1
3 Terms and definitions .....	1
4 Principle .....	2
5 Reagents .....	2
6 Apparatus .....	3
7 Sampling .....	5
8 Preparation of test sample .....	5
8.1 Cheese .....	5
9 Procedure .....	6
9.1 Checking the reducing capacity of the cadmium column .....	6
9.2 Regeneration of the cadmium column .....	6
9.3 Test portion .....	6
9.4 Extraction .....	6
9.5 Determination of nitrite content .....	7
9.6 Determination of nitrate content .....	7
10 Calculation and expression of results .....	7
10.1 Nitrite content .....	7
10.2 Nitrate content .....	8
11 Precision .....	8
11.1 General .....	8
11.2 Nitrite content .....	8
11.3 Nitrate content .....	9
12 Test report .....	9
Bibliography .....	10

## Foreword

**ISO (the International Organization for Standardization)** is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 14673-3|IDF 189-3 was prepared by Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 5, *Milk and milk products*, and the International Dairy Federation (IDF), in collaboration with AOAC International. It is being published jointly by ISO and IDF and separately by AOAC International.

This second edition cancels and replaces the first edition (ISO 14673-3|IDF 189-3:2001), of which it constitutes a minor revision.

ISO 14673|IDF 189 consists of the following parts, under the general title *Milk and milk products — Determination of nitrate and nitrite contents*:

- *Part 1: Method using cadmium reduction and spectrometry*
- *Part 2: Method using segmented flow analysis (Routine method)*
- *Part 3: Method using cadmium reduction and flow injection analysis with in-line dialysis (Routine method)*



## Foreword

**IDF (the International Dairy Federation)** is a worldwide federation of the dairy sector with a National Committee in every member country. Every National Committee has the right to be represented on the IDF Standing Committees carrying out the technical work. IDF collaborates with ISO and AOAC International in the development of standard methods of analysis and sampling for milk and milk products.

Draft International Standards adopted by the Action Teams and Standing Committees are circulated to the National Committees for voting. Publication as an International Standard requires approval by at least 50 % of the National Committees casting a vote.

ISO 14673-3|IDF 189-3 was prepared by Technical Committee ISO/TC 34, *Food products*, Subcommittee SC 5, *Milk and milk products*, and the International Dairy Federation (IDF), in collaboration with AOAC International. It is being published jointly by ISO and IDF and separately by AOAC International.

All work was carried out by the Joint ISO/IDF/AOAC Action Team, *Minerals and minor compounds*, of the Standing Committee on *Minor components characterization of physical properties*, under the aegis of its project leader, Mr G. Bråthen (NO).

This second edition, together with ISO 14673-1|IDF 189-1 and ISO 14673-2|IDF 189-2, cancels and replaces IDF 84A:1984, IDF 95A:1982, IDF 96A:1987, IDF 97A:1985 and IDF 120:1984, which have been technically revised.



# Milk and milk products — Determination of nitrate and nitrite contents —

## Part 3:

### Method using cadmium reduction and flow injection analysis with in-line dialysis (Routine method)

**WARNING —** The use of this International Standard may involve hazardous materials, operations and equipment. This standard does not purport to address all the safety problems associated with its use. It is the responsibility of the user of this standard to establish safety and health practices and determine the applicability of regulatory limitations prior to use.

## 1 Scope

This part of ISO 14673|IDF 189 specifies a routine method for the determination of the nitrate and nitrite contents of milk and milk products by cadmium reduction and flow injection analysis (FIA). The method is applicable to hard, semi-hard and soft cheeses of various ages, and processed cheese. The detection limits of the method are 0,5 mg of nitrate ions per kilogram and 1,0 mg of nitrite ions per kilogram.

The method is also applicable to whey powder, milk powder and milk-based infant food.

NOTE 1 The method closely resembles the FIA method described in reference [2] for the determination of nitrate and nitrite in milk and fluid dairy products. Adaptations were made to allow for the analysis of cheese and to obtain sufficient sensitivity for the determination of low levels of nitrite in cheese and milk-based infant foods.

NOTE 2 For determination of nitrite and nitrate following cadmium reduction, use is made of the same colour reaction as described in ISO 14673-1|IDF 189-1.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1042, *Laboratory glassware — One-mark volumetric flasks*

ISO 14673-1|IDF 189-1, *Milk and milk products — Determination of nitrate and nitrite contents — Part 1: Method using cadmium reduction and spectrometry*

## 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 3.1

#### nitrate content

mass fraction of nitrate determined by the procedure specified in this part of ISO 14673|IDF 189

NOTE The nitrate content is expressed as the mass in milligrams of nitrate ions ( $\text{NO}_3^-$ ) per kilogram of product.

**3.2****nitrite content**

mass fraction of nitrite determined by the procedure specified in this part of ISO 14673|IDF 189

NOTE The nitrite content is expressed as the mass in milligrams of nitrite ions ( $\text{NO}_2^-$ ) per kilogram of product.

**4 Principle**

**4.1** A test portion is suspended in a warm extraction buffer solution. Fat is separated by centrifuging and rapid cooling. Analyses are made of small portions of the de-fatted solution by flow injection analysis (FIA). In-line dialysis is used to remove protein and remaining fat. The nitrate ions are reduced to nitrite ions by cadmium. The nitrite ions are reacted with sulfanilamide and *N*-1-naphthyl ethylenediamine dihydrochloride to give a red-coloured azo dye. The colour is measured in a flow cell at maximum absorption of the dye at 540 nm with reference to the absorption measured at 620 nm.

**4.2** The nitrite and nitrate contents of the test sample are calculated with reference to the measured absorbances for a series of standard solutions of nitrite and nitrate, respectively. If the nitrite content exceeds 0,5 mg/kg, or exceeds 10 % of the nitrate content, correction of the nitrate content is made by subtracting the nitrite content from the obtained nitrate results.

**5 Reagents**

Use only reagents of recognized analytical grade unless otherwise specified.

**5.1 Water**, distilled or deionized, or water of equivalent purity, free from nitrate and nitrite ions.

**5.2 Cadmium reduction column**, for example Aquatec-Tecator<sup>1)</sup>.

**5.3 Extraction buffer solution or carrier solution (C2).**

Dissolve 26,6 g of ammonium chloride ( $\text{NH}_4\text{Cl}$ ) in 800 ml water in a 1 000 ml conical flask. By adding concentrated ammonia, adjust the pH to 8,5. Dilute to 1 000 ml with water and mix.

**5.4 Hydrochloric acid (HCl)**, ( $\rho_{20} = 1,19$  g/ml).

**5.5 Reagent solution (R1).**

Dissolve 5,0 g sulfanilamide ( $\text{NH}_2\text{C}_6\text{H}_4\text{SO}_2\text{NH}_2$ ) in a mixture of 300 ml water and 26 ml of hydrochloric acid (5.4) in a 500 ml volumetric flask (6.3). Dilute to the mark with water and mix.

**5.6 Reagent solution (R2).**

Dissolve 0,5 g of *N*-1-naphthyl ethylenediamine dihydrochloride ( $\text{C}_{10}\text{H}_7\text{NHCH}_2\text{CH}_2\text{NH}_2 \cdot 2\text{HCl}$ ) in water in a 500 ml volumetric flask (6.3). Dilute to the mark with water and mix.

The solution may be stored for up to 1 week in a well-stoppered brown bottle in a refrigerator.

**5.7 Regeneration solution**,  $c(\text{HCl}) = 0,1$  mol/l.

Dilute 80 ml of hydrochloric acid (5.4) with water to 1 litre and mix.

---

1) Aquatec-Tecator is an example of a suitable product available commercially. This information is given for the convenience of users of this part of ISO 14673|IDF 189 and does not constitute an endorsement by ISO or IDF of this product.

**5.8 Sodium nitrate stock solution**,  $c(\text{NO}_3^-) = 1\,000\text{ mg/l}$ .

Before use, dry sodium nitrate ( $\text{NaNO}_3$ ) to constant mass at 110 °C to 120 °C. Dissolve 137,1 mg of the dry  $\text{NaNO}_3$  in water in a 100 ml volumetric flask (6.3). Dilute to the mark with water and mix.

**5.9 Sodium nitrate calibration solutions.**

Prepare the sodium nitrate calibration solutions on the day of use. Pipette amounts of 25 µg, 50 µg, 100 µg, 150 µg and 250 µg of sodium nitrate stock solution (5.8) into separate 50 ml volumetric flasks (6.3). Dilute to the mark with extraction buffer solution (5.3) to obtain sodium nitrate calibration solutions corresponding to 0,50 mg/l, 1,00 mg/l, 2,00 mg/l, 3,00 mg/l and 5,00 mg/l nitrate ions respectively.

**5.10 Sodium nitrite stock solution**,  $c(\text{NO}_2^-) = 1\,000\text{ mg/l}$ .

Before use, dry the sodium nitrite ( $\text{NaNO}_2$ ) to constant mass at 110 °C to 120 °C. Prepare the sodium nitrite stock solution on the day of use. Dissolve 150,0 mg of the dry  $\text{NaNO}_2$  in water in a 100 ml volumetric flask (6.3). Dilute to the mark with water and mix.

**5.11 Sodium nitrite working solution**,  $c(\text{NO}_2^-) = 50,0\text{ mg/l}$ .

Pipette 5,00 ml of the sodium nitrite stock solution (5.10) into a 100 ml volumetric flask. Dilute to the mark with water and mix.

**5.12 Sodium nitrite calibration solutions.**

Shortly before use, pipette amounts of 25 µl, 50 µl, 100 µl, 200 µl and 400 µl of the sodium nitrite working solution (5.11) into separate 50 ml volumetric flasks (6.3). Dilute to the mark with extraction buffer solution (5.3) to obtain sodium nitrite calibration solutions corresponding to 0,025 mg/l, 0,050 mg/l, 0,100 mg/l, 0,200 mg/l and 0,400 mg/l nitrite ions respectively. Mix well.

**5.13 Sodium nitrite reference solution**,  $c(\text{NO}_2^-) = 1,48\text{ mg/l}$ .

Pipette 1 480 µl of the sodium nitrite working solution (5.11) into a 50 ml volumetric flask (6.3). Dilute to the mark with extraction buffer solution (5.3) and mix. Prepare the sodium nitrite reference solution shortly before use.

## 6 Apparatus

Clean all glassware thoroughly and rinse with distilled water to ensure that it is free from nitrate and nitrite ions.

Usual laboratory equipment and, in particular, the following.

**6.1 Analytical balance**, capable of weighing to the nearest 1 mg, with a readability of 0,1 mg.

**6.2 Sample container**, provided with an airtight lid.

**6.3 Volumetric flasks**, of nominal capacity 50 ml, 100 ml and 500 ml, complying with the requirements of ISO 1042, class B.

**6.4 Pipettes**, capable of delivering 25 µl, 50 µl, 100 µl, 150 µl, 200 µl, 250 µl, 400 µl and 1 480 µl (semi-automatic pipettes).

**6.5 Grinding device**, appropriate for grinding the test sample, if necessary. To avoid loss of moisture, the device should not produce undue heat. A hammer mill shall not be used.

**6.6 Laboratory mixer or homogenizer** (e.g. an Ultra-turrax<sup>2)</sup>), with glass containers of capacity 250 ml or 400 ml, suitable for suspending test portions of cheese.

**6.7 Table centrifuge**, with centrifuge tubes of capacity 50 ml, capable of centrifuging at 1 500 g.

**6.8 Flow injection analyser (FIA)** (e.g. a Tecator<sup>2)</sup>), with a Fiastar analyser, controller, dialysis module, sampler, provided with sample cups of 4 ml, with specific instrument control and evaluation software, nitrite/nitrate manifold (see Figure 1), a sample loop volume of 200 µl, two mixing coils of length 60 cm and of diameter 0,7 mm, connecting tubings and pump tubings providing the flow rates given in Table 1.

Other flow injection analysers may use other procedures. The instructions of the manufacturer, therefore, should be strictly followed.

**Table 1 — Flow rates**

Values in millilitres per minute

Solution	Flow rate for nitrate	Flow rate for nitrite
Sample/wash	2	2
Carrier C1 (water) (5.1)	2	1,2
Carrier C2 (5.3)	2	1,2
Reagent R1 (5.5)	0,6	0,4
Reagent R2 (5.6)	0,6	0,4

**6.9 Matrix spectrophotometer** (e.g. SKALAR<sup>2)</sup>), equipped with interference filter 540 nm and interference filter 620 nm, a flow cell of path length 5 cm and of volume 40 µl.

**6.10 FIA program parameters for nitrite.**

**6.10.1 Program parameters**

Evaluation	peak height
Calibration equation	linear
Number of standards	5
FIA-pattern collection time/cycle time	120 s

**6.10.2 Timing parameters**

Window for peak maximum	30 s to 50 s
Signal filtering maximum	2 s
Window for baseline detection	0 to 10 s
Injection period	0 to 60 s
Sample loop wash	60 s to 80 s
Sample loop filling	80 s to 120 s

2) These products are examples of a suitable products available commercially. This information is given for the convenience of users of this part of ISO 14673|IDF 189 and does not constitute an endorsement by ISO or IDF of these products.

**6.10.3 Calibration check**

Tolerance	± 5 %
Repeat after (samples)	10 samples
Standard used	0,100 mg/l NO <sub>2</sub> <sup>-</sup>

**6.11 FIA program parameters for nitrate.****6.11.1 Program parameters**

Evaluation	peak height
Calibration equation	linear
Number of standards	5
FIA-pattern collection time/cycle time	60 s

**6.11.2 Timing parameters**

Window for peak maximum	25 s to 40 s
Signal filtering time	1 s
Window for baseline detection	0 to 15 s
Injection period	0 to 20 s
Sample loop wash	20 s to 35 s
Sample loop filling	35 s to 60 s

**6.11.3 Calibration check**

Tolerance	± 5 %
Repeat after (samples)	10 samples
Standard used	2,00 mg/l NO <sub>3</sub> <sup>-</sup>

**7 Sampling**

Sampling is not part of the method specified in this part of ISO 14673|IDF 189. A recommended sampling method is given in ISO 707.

It is important that the laboratory receive a sample which is truly representative and has not been damaged or changed during transport or storage.

Store the test sample in such a way that deterioration and change in composition are prevented.

**8 Preparation of test sample****8.1 Cheese**

**8.1.1** Prior to analysis, remove the rind or mouldy surface layer of the test sample in such a way as to obtain a sample representative of the cheese as it is usually consumed.

**8.1.2** Grind the test sample by means of an appropriate grinding device (6.5). Mix the ground mass quickly and, if possible, grind a second time and again mix thoroughly. Clean the device after grinding of each sample. If the test sample cannot be ground, mix it thoroughly by intensive stirring and kneading.

**8.1.3** As soon as possible after grinding, transfer the test sample to a sample container (6.2) to await the determination which, preferably, should be carried out immediately. If a delay is unavoidable, take all precautions to ensure proper conservation of the test sample and to prevent moisture collecting on the inside surface of the container.

**8.1.4** Do not examine ground cheese showing unwanted mould growth or beginning to deteriorate.

## **9 Procedure**

### **9.1 Checking the reducing capacity of the cadmium column**

**9.1.1** Check the reducing capacity of the cadmium column at the beginning and at the end of a series of determinations and at least twice a day.

**9.1.2** Prepare the FIA system for operation according to 9.6.1.

**9.1.3** Fill a cup with sodium nitrite reference solution (5.13).

**9.1.4** Fill another cup with the sodium nitrate calibration solution (5.9).

**9.1.5** Analyse the sodium nitrate calibration solution (9.1.4) and the sodium nitrite reference solution (9.1.3). Divide the peak height found for nitrate by the peak height for nitrite and multiply by 100 to obtain the percentage reducing capacity of the cadmium column. If the reducing capacity is less than 95 %, regenerate the column (see 9.2).

### **9.2 Regeneration of the cadmium column**

Regenerate the cadmium column at the end of each day after use, or more frequently if the check of its reducing capacity (9.1.5) indicates a loss of efficiency.

Disable pump flows for carrier solution C2 (5.3) and reagents R1 (5.5) and R2 (5.6). Unscrew the tubing at the inlet of the dialysis module connecting the injector to the dialysis module. Run water (5.1) used as carrier solution C1 through the injector until the system is filled. Connect the cadmium column to the outlet of the injector. Start the pump again and make three to five injections of reagent solution R2 (5.6) followed by the sodium nitrate standard solution (5.8). Wash the column by passage of carrier solution C2 (5.3).

### **9.3 Test portion**

#### **9.3.1 Cheese and dried milk products**

Weigh, to the nearest 1 mg, 2,5 g of the test sample (8.1.2) into a 50 ml centrifuge tube (6.7).

#### **9.3.2 Liquid milk products**

Weigh, to the nearest 1 mg, 10 g of the test sample (8.1.2) into a 50 ml centrifuge tube (6.7).

### **9.4 Extraction**

**9.4.1** Add 24 ml of extraction buffer solution (5.3), preheated to a temperature of 50 °C to 55 °C, to the test portion (9.3) in the 50 ml centrifuge tube. Mix with the homogenizer for about 3 min until the test portion is well suspended.

**9.4.2** Centrifuge the test solution in the tube (9.4.1) at about 1 500 g for 5 min.

**9.4.3** Place the centrifuge tube in a mixture of water and ice for 15 min to cool the test solution.



**9.4.4** Withdraw with a pipette (6.4) the de-fatted test solution from underneath the fat layer in the centrifuge tube. Fill the cups of the FIA, for both the nitrite and nitrate determinations, with the obtained de-fatted test solution.

## 9.5 Determination of nitrite content

**9.5.1** Install the manifold of the flow injection analyser (FIA) according to the scheme in Figure 1. Use the pump tubings of the FIA (6.8) for the determination of nitrite while leaving out the cadmium reduction column (5.2). Connect the bottles with both reagent solutions R1 (5.5) and R2 (5.6) and carrier solution C2 (5.3). Start the pumps of the FIA to flush the system for 5 min to 10 min.

**9.5.2** Load the analyser with the FIA program for nitrite (6.10). Run the sodium nitrite calibration solutions (5.12) to calibrate the system, followed by the de-fatted test solution (9.4.4).

**9.5.3** Check the calibration, both at the end of a series and after each group of 10 test solutions, by analysing the sodium nitrite calibration solution of 0,100 mg/l nitrite ions (5.12).

## 9.6 Determination of nitrate content

**9.6.1** Install the manifold of the flow injection analyser (FIA) according to the scheme in Figure 1. Use the pump tubings of the FIA (6.8) for the determination of nitrate while using the cadmium reduction column (5.2). Connect the bottles with both reagent solutions R1 (5.5) and R2 (5.6) and carrier solution C2 (5.3). Start the pumps of the FIA to fill the system with the liquids. Stop the pumps and install the cadmium reduction column (5.2). Start the pumps again to flush the system for 5 min to 10 min. Check the reducing capacity of the cadmium column (9.1).

**9.6.2** Load the analyser with the FIA program for nitrate (6.11). Run the sodium nitrate calibration solutions (5.9), to calibrate the system, followed by the de-fatted test solution (9.4.4).

**9.6.3** Check the calibration, both at the end of a series and after each group of 10 test solutions, by analysing the sodium nitrate calibration solution of 2,00 mg/l nitrate ions (5.9).

## 10 Calculation and expression of results

### 10.1 Nitrite content

#### 10.1.1 Calculation of nitrite content

Calculate the nitrite content of the test sample,  $\omega_{N1}$ , using the following equation:

$$\omega_{N1} = \frac{25}{m} \times c_{N1}$$

where

$\omega_{N1}$  is the nitrite content of the sample, in milligrams of nitrite ions per kilogram;

$c_{N1}$  is the numerical value of the concentration, read from the calibration graph, corresponding to the measured absorbance of the test solution (9.5.2), in micrograms of nitrite ions per litre;

$m$  is the mass of the test portion (9.3), in grams.

#### 10.1.2 Expression of results

Express the results to one decimal place.

## 10.2 Nitrate content

### 10.2.1 Calculation of nitrate content

Calculate the nitrate content of the sample,  $\omega_{N2}$ , using the following equation:

$$\omega_{N2} = \frac{25}{m} \times c_{N2}$$

where

$\omega_{N2}$  is the nitrate content of the sample, in milligrams of nitrate ions per kilogram;

$c_{N2}$  is the numerical value of the concentration, read from the calibration graph, corresponding to the measured absorbance of the test solution (9.6.2), in micrograms of nitrate ions per litre;

$m$  is the mass of the test portion (9.3), in grams.

### 10.2.2 Calculation of the corrected nitrate content

Calculate the corrected nitrate content of the sample,  $\omega_{NC}$ , using the following equation:

$$\omega_{NC} = \omega_{N2} - 1,35 \omega_{N1}$$

where  $\omega_{NC}$  is the nitrate content of the test sample corrected for its nitrite content, in milligrams of nitrate ions per kilogram.

### 10.2.3 Expression of results

Express the results to whole numbers.

## 11 Precision

### 11.1 General

The values for repeatability and reproducibility limits are expressed for the 95 % probability level and may not be applicable to concentration ranges and matrices other than those given.

### 11.2 Nitrite content

#### 11.2.1 Repeatability

The absolute difference between two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, will in not more than 5 % of cases be greater than 0,5 mg/kg of product.

#### 11.2.2 Reproducibility

The absolute difference between two single test results, obtained using the same method on identical test material in different laboratories with different operators using different equipment, will in not more than 5 % of cases be greater than 1,0 mg/kg of product.

## 11.3 Nitrate content

### 11.3.1 Repeatability

The absolute difference between two independent single test results, obtained using the same method on identical test material in the same laboratory by the same operator using the same equipment within a short interval of time, will in not more than 5 % of cases be greater than:

- for samples with a nitrate content < 100 mg/kg: 10 mg/kg;
- for samples with a nitrate content  $\geq$  100 mg/kg: 15 % of the arithmetic mean of the results.

### 11.3.2 Reproducibility


The absolute difference between two single test results, obtained using the same method on identical test material in different laboratories with different operators using different equipment, will in not more than 5 % of cases be greater than:

- for samples with a nitrate content < 100 mg/kg: 15 mg/kg;
- for samples with a nitrate content  $\geq$  100 mg/kg: 20 % of the arithmetic mean of the results.

## 12 Test report

The test report shall specify:

- all information required for the complete identification of the sample;
- the sampling method used, if known;
- the test method used, with reference to this part of ISO 14673|IDF 189;
- all operating details not specified in this part of ISO 14673|IDF 189, or regarded as optional, together with details of any incident which may have influenced the result(s);
- the test result(s) obtained or, if the repeatability has been checked, the final quoted results obtained.

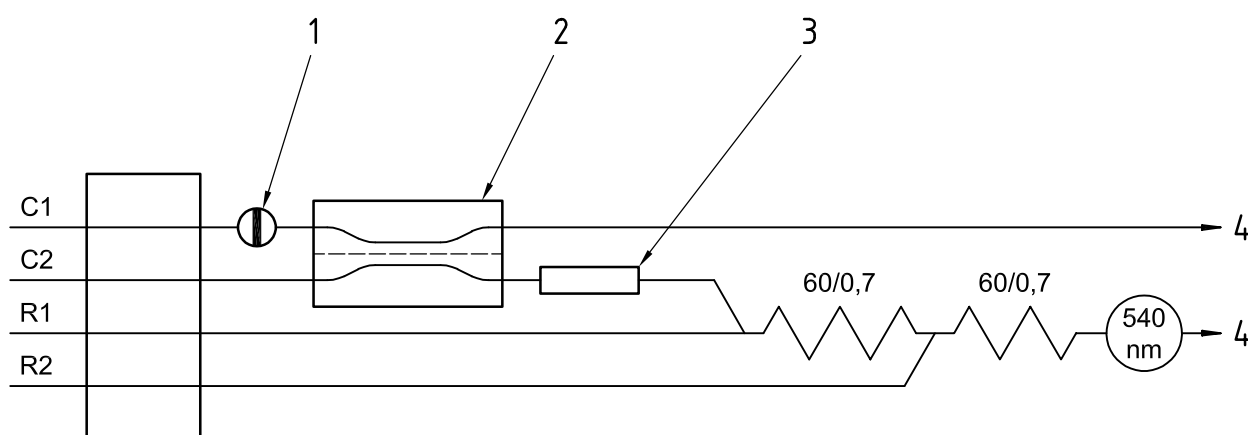

### Key

- |                          |            |
|--------------------------|------------|
| 1 injector (200 $\mu$ l) | 3 reductor |
| 2 dialysis cell          | 4 waste    |

Figure 1 — Schematic view of the nitrite/nitrate manifold

## Bibliography

- [1] ISO 707:1997, *Milk and milk products — Guidance on sampling*
- [2] MUNKSGAARD L. and THYMARK L. Determination of nitrate and nitrite in milk and milk products by Flow Injection Analysis. *Tecator in Focus*, Supplement No. 6, 1987
- [3] DE JONG E.A.M., KLOMP H. and ELLEN G. Geautomatiseerde bepaling nitraat en nitriet met Flow-Injectie-Analyse. *Voedingsmiddelentechnologie*, **28** (4), 1995, pp. 11-14



---

---

## BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

### Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

### Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001. Email: [orders@bsi-global.com](mailto:orders@bsi-global.com). Standards are also available from the BSI website at <http://www.bsi-global.com>.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

### Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre. Tel: +44 (0)20 8996 7111. Fax: +44 (0)20 8996 7048. Email: [info@bsi-global.com](mailto:info@bsi-global.com).

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002. Fax: +44 (0)20 8996 7001. Email: [membership@bsi-global.com](mailto:membership@bsi-global.com).

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsi-global.com/bsonline>.

Further information about BSI is available on the BSI website at <http://www.bsi-global.com>.

### Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright & Licensing Manager. Tel: +44 (0)20 8996 7070. Fax: +44 (0)20 8996 7553. Email: [copyright@bsi-global.com](mailto:copyright@bsi-global.com).