

BS EN ISO 18082:2014



BSI Standards Publication

Anaesthetic and respiratory equipment — Dimensions of non-interchangeable screw-threaded (NIST) low-pressure connectors for medical gases

bsi.

...making excellence a habit.™

National foreword

This British Standard is the UK implementation of EN ISO 18082:2014. It supersedes BS EN 15908:2010 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee CH/121/1, Breathing attachments and anaesthetic machines.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2014. Published by BSI Standards Limited 2014

ISBN 978 0 580 78342 5

ICS 11.040.10

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 30 June 2014.

Amendments issued since publication

Date	Text affected
------	---------------

English Version

Anaesthetic and respiratory equipment - Dimensions of non-interchangeable screw-threaded (NIST) low-pressure connectors for medical gases (ISO 18082:2014)

Matériel respiratoire et anesthésique - Raccords basse pression à tête fileté non interchangeables (NIST) pour gaz médicaux (ISO 18082:2014)

Anästhesie- und Beatmungsgeräte - Maße von nichtverwechselbaren Verbindungsstücken mit Schraubgewinde (NIST) für niedrigen Druck zur Verwendung mit medizinischen Gasen (ISO 18082:2014)

This European Standard was approved by CEN on 22 May 2014.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN-CENELEC Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN-CENELEC Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

CEN-CENELEC Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

This document (EN ISO 18082:2014) has been prepared by Technical Committee ISO/TC 121 “Anaesthetic and respiratory equipment” in collaboration with Technical Committee CEN/TC 215 “Respiratory and anaesthetic equipment” the secretariat of which is held by BSI.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by December 2014, and conflicting national standards shall be withdrawn at the latest by December 2014.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

This document supersedes EN 15908:2010.

According to the CEN-CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Croatia, Cyprus, Czech Republic, Denmark, Estonia, Finland, Former Yugoslav Republic of Macedonia, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland, Turkey and the United Kingdom.

Endorsement notice

The text of ISO 18082:2014 has been approved by CEN as EN ISO 18082:2014 without any modification.

Contents

Page

Foreword	iv
Introduction	v
1 Scope	1
2 Terms and definitions	1
3 Dimensions and allocation of NIST connectors	2
4 Marking	11
5 Test for durability of markings	11
Bibliography	12

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2. www.iso.org/directives

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received. www.iso.org/patents

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT), see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 121, *Anaesthetic and respiratory equipment*, Subcommittee SC 1, *Breathing attachments and anaesthetic machines*.

This is the first edition of this International Standard that contains the requirements for non-interchangeable screw threaded (NIST) connectors for use with medical gases previously included in ISO 5359:2008 and ISO 5359:2008/Amd.1:2011.

Introduction

This International Standard has been prepared in response to the need for a safe method of connecting medical equipment intended to administer medical gases to patients or power medical devices. Medical gases are stored in cylinders or cryogenic vessels, or can be produced on site; several medical devices (e.g. pressure regulators, hose assemblies, flow-metering devices, lung ventilators, anaesthetic workstations) can be fitted between the source of supply and the medical device. At each interface gas-specific connectors are needed to ensure that the intended medical gas is administered to the patient.

While the desirability of achieving agreement on a single International Standard for screw-threaded connectors has never been in doubt, the present pattern of usage has made such agreement impossible.

Nevertheless, fears that proliferation of individual national standards or practices will eventually result in potentially dangerous cross-connection between components for different gases have led to the choice of several different connector systems, all of which are intended to be incompatible with each other.

This International Standard specifies the dimensions and the allocation of non-interchangeable screw threaded (NIST) connectors for use with medical gases.

This International Standard does not specify the dimensions and the allocation of

- diameter index safety system (DISS) connectors specified in CGA V-5^[9],
- sleeve indexed system (SIS) connectors specified in AS 2896^[7], and
- quick connectors designed for terminal units specified in ISO 9170-1^[5].

Anaesthetic and respiratory equipment — Dimensions of non-interchangeable screw-threaded (NIST) low-pressure connectors for medical gases

1 Scope

1.1 This International Standard specifies the dimensions, the allocation and marking of non-interchangeable screw-threaded (NIST) connectors intended to be used at operating pressures up to 1 400 kPa, and for vacuum systems at pressures not greater than 60 kPa absolute.

1.2 This International Standard specifies NIST connectors intended for use with the following medical gases:

- oxygen;
- nitrous oxide;
- medical air;
- helium;
- carbon dioxide;
- xenon;
- specified mixtures of the gases listed above;
- oxygen-enriched air;
- air for driving surgical tools;
- nitrogen for driving surgical tools;

and for use with vacuum.

NOTE Low-pressure hose assemblies for medical gases and vacuum are specified in ISO 5359[3].

1.3 The information to be supplied by the manufacturer is excluded from the scope of this International Standard because information about the use of NIST connectors is supplied by the manufacturer of each medical device to which the connectors are permanently fitted.

NOTE Environmental aspects are dealt with in each International Standard concerning medical devices fitted with NIST connectors.

2 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

2.1

gas-specific

having characteristics which prevent connections between different gas services

[SOURCE: ISO 7396-1:2007, 3.14]

2.2

medical gas

any gas or mixture of gases intended for administration to patients for anaesthetic, therapeutic, diagnostic or prophylactic purposes, or for surgical tool applications

[SOURCE: ISO 4135:2001, 1.1.1]

2.3

non-interchangeable screw-threaded connector

NIST connector

range of male and female components intended to maintain gas specificity by the allocation of a set of different diameters and a left- or right-hand screw thread to the mating components for each particular gas

[SOURCE: ISO 9170-1:2008, 3.10]

3 Dimensions and allocation of NIST connectors

The dimensions of the NIST body, nipple and nut shall comply with [Figures 1, 2, 3 and 4](#) and [Tables 2, 3 and 4](#).

Allocation of NIST connectors shall comply with [Table 1](#).

Compliance shall be verified by measurement and visual inspection.

Table 1 — NIST connector allocation — Right-hand thread

Connector reference	Gas
A1	Medical air/oxygen mixture
A2	Oxygen/nitrous oxide mixture [O ₂ = 50 % (volume fraction)]
A3	Medical air
A4	Nitrous oxide
A5	Nitrous oxide/oxygen mixtures [N ₂ O < 80 % (volume fraction)]
A6	Air for driving surgical tools
A7	Not allocated
A8	Oxygen
A9	Not allocated
A10	Vacuum
B11	Carbon dioxide
B12	Oxygen-enriched air
B13	Oxygen/carbon dioxide mixture [CO ₂ ≤ 7 % (volume fraction)]
B14	Helium/oxygen mixture [He ≤ 80 % (volume fraction)]
B15	Helium/oxygen mixture [O ₂ < 20 % (volume fraction)]
B16	Xenon
B17	Special gas mixture
B18	Nitrogen for driving surgical tools
C19	Carbon dioxide/oxygen mixture [CO ₂ > 7 % (volume fraction)]
C20	Helium
C21	Medical air/helium/carbon monoxide [CO < 1 % (volume fraction)]
C22	Not allocated
C23	Not allocated
C24	Not allocated
NOTE Left-hand threads have not been allocated.	

Table 2 — Indexing diameters including tolerances for NIST body (see [Figure 1](#))

Dimensions in millimetres

Connector reference	Dimension B	Dimension C	Dimension D
A1	8	12,5 $\begin{matrix} +0,043 \\ 0 \end{matrix}$	17
A2	8,5		16,5
A3	9 $\begin{matrix} +0,09 \\ 0 \end{matrix}$		16
A4	9,5		15,5
A5	10		15 $\begin{matrix} +0,11 \\ 0 \end{matrix}$
A6	10,5		14,5
A7	11 $\begin{matrix} +0,11 \\ 0 \end{matrix}$		1
A8	11,5		13,5
A9	12		13
A10	12,5 $\begin{matrix} +0,043 \\ 0 \end{matrix}$		12,5 $\begin{matrix} +0,043 \\ 0 \end{matrix}$
B11	7,5	11 $\begin{matrix} +0,043 \\ 0 \end{matrix}$	14,5
B12	8		14
B13	8,5 $\begin{matrix} +0,09 \\ 0 \end{matrix}$		13,5 $\begin{matrix} +0,11 \\ 0 \end{matrix}$
B14	9		13
B15	9,5		12,5
B16	10		12
B17	10,5 $\begin{matrix} +0,11 \\ 0 \end{matrix}$		11,5
B18	11 $\begin{matrix} +0,043 \\ 0 \end{matrix}$		11 $\begin{matrix} +0,043 \\ 0 \end{matrix}$
C19	7,5	10 $\begin{matrix} +0,043 \\ 0 \end{matrix}$	12,5
C20	8 $\begin{matrix} +0,09 \\ 0 \end{matrix}$		12 $\begin{matrix} +0,11 \\ 0 \end{matrix}$
C21	8,5		11,5
C22	9		11
C23	9,5		10,5
C24	10 $\begin{matrix} +0,043 \\ 0 \end{matrix}$		10 $\begin{matrix} +0,043 \\ 0 \end{matrix}$

Table 3 — Indexing diameters including tolerances for NIST nipple (see [Figure 2](#))

Dimensions in millimetres

Connector reference	Dimension <i>E</i>	Dimension <i>F</i>	Dimension <i>G</i>	Dimension <i>H</i>	Dimension <i>I</i>
A1	17		8		
A2	16,5		8,5 $\begin{matrix} -0,04 \\ -0,13 \end{matrix}$		
A3	16		9		
A4	15,5		9,5		
A5	15		10		
A6	14,5	12,5 $\begin{matrix} -0,05 \\ -0,16 \end{matrix}$	10,5	8,5 $\begin{matrix} 0 \\ -0,10 \end{matrix}$	3,3 $\begin{matrix} 0 \\ -0,20 \end{matrix}$
A7	14		11		
A8	13,5		11,5 $\begin{matrix} -0,05 \\ -0,16 \end{matrix}$		
A9	13		12		
A10	12,5		12,5		
B11	14,5 $\begin{matrix} -0,05 \\ -0,16 \end{matrix}$		7,5		
B12	14		8		
B13	13,5		8,5		
B14	13	11 $\begin{matrix} -0,05 \\ -0,16 \end{matrix}$	9	8,3 $\begin{matrix} 0 \\ -0,10 \end{matrix}$	
B15	12,5		9,5 $\begin{matrix} -0,04 \\ -0,13 \end{matrix}$		
B16	12		10		
B17	11,5		10,5		
B18	11		11 $\begin{matrix} -0,05 \\ -0,16 \end{matrix}$		2,5 $\begin{matrix} 0 \\ -0,20 \end{matrix}$
C19	12,5		7,5		
C20	12		8		
C21	11,5	10 $\begin{matrix} -0,04 \\ -0,13 \end{matrix}$	8,5 $\begin{matrix} -0,04 \\ -0,13 \end{matrix}$	7,3 $\begin{matrix} 0 \\ -0,10 \end{matrix}$	
C22	11		9		
C23	10,5		9,5		
C24	10		10		

Table 4 — Dimensions of “O” rings


Dimensions in millimetres

Connector reference range	Internal diameter	Internal diameter tolerance	Section diameter	Section diameter tolerance
A	7,6	±0,15	2,4	±0,08
B	8,1	±0,15	1,6	±0,08
C	7,1	±0,15	1,6	±0,08

NOTE 1 Recommended hardness 75° IRHD (International Rubber Hardness Degrees, see ISO 48).

NOTE 2 These dimensions are based upon BS 4518[8]. For A, B and C ranges the “O” rings are identified in BS 4518 with the reference numbers 0076-24, 0081-16 and 0071-16 respectively.

Dimensions in millimetres

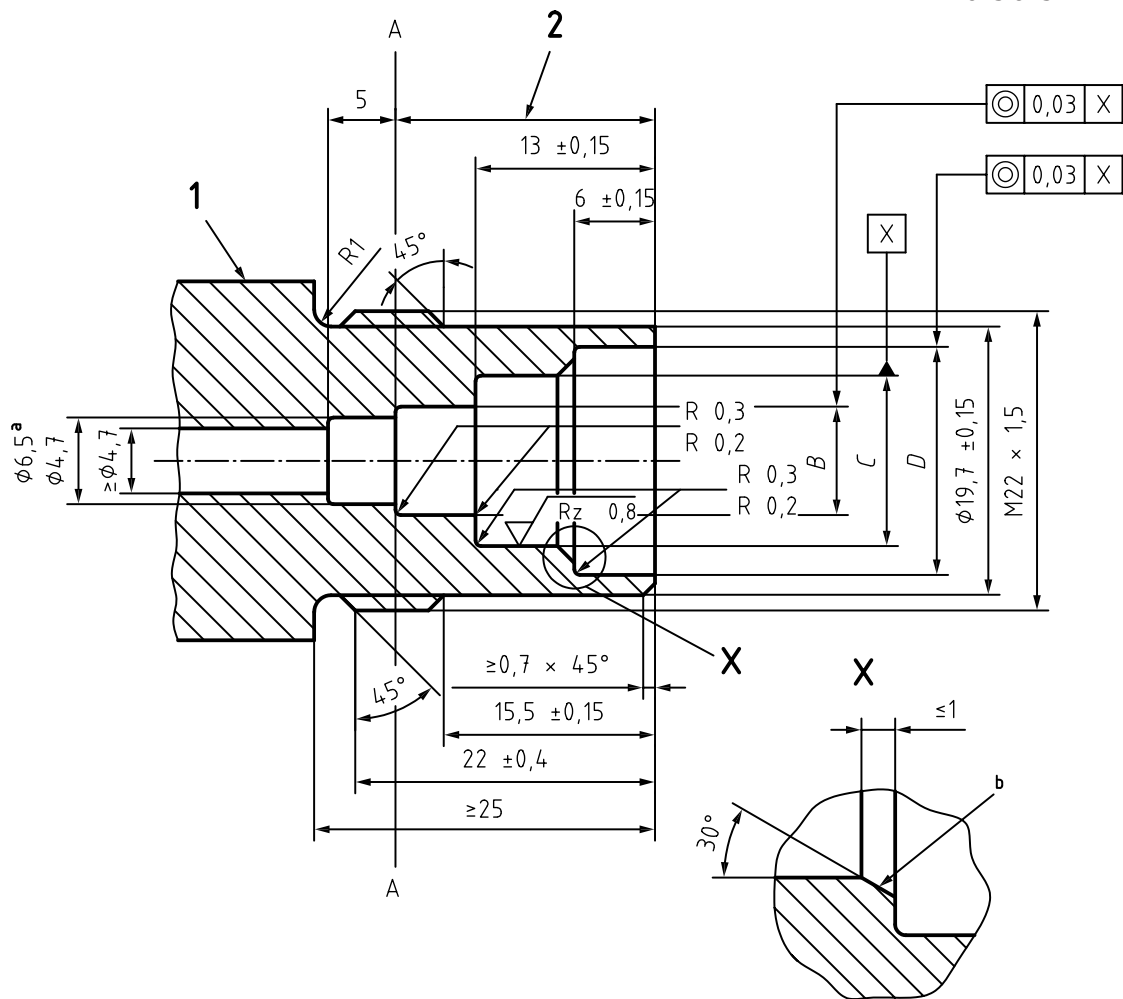


Surface finish shall be $\sqrt{Rz \ 1,6}$ unless otherwise stated.

Key

- 1 position for marking gas identification symbol
- 2 A range = $19 \pm 0,15$; B range = $25 \pm 0,15$; C range = $31 \pm 0,15$
- a Diameters 6,5 and 4,7 and the location of face AA are critical. If this face is movable, for example when it forms part of a check valve, it is essential that means are provided to prevent its movement to a depth greater than 19 mm/25 mm/31 mm. See Table 2 for dimensions B, C and D.
- b For connectors number A10, B18 and C24, the 12,5 mm/11 mm/10 mm diameters extend over the full depths of 19 mm/25 mm/31 mm respectively and this chamfer will appear at the nose of the fitting.

Figure 1 — NIST body

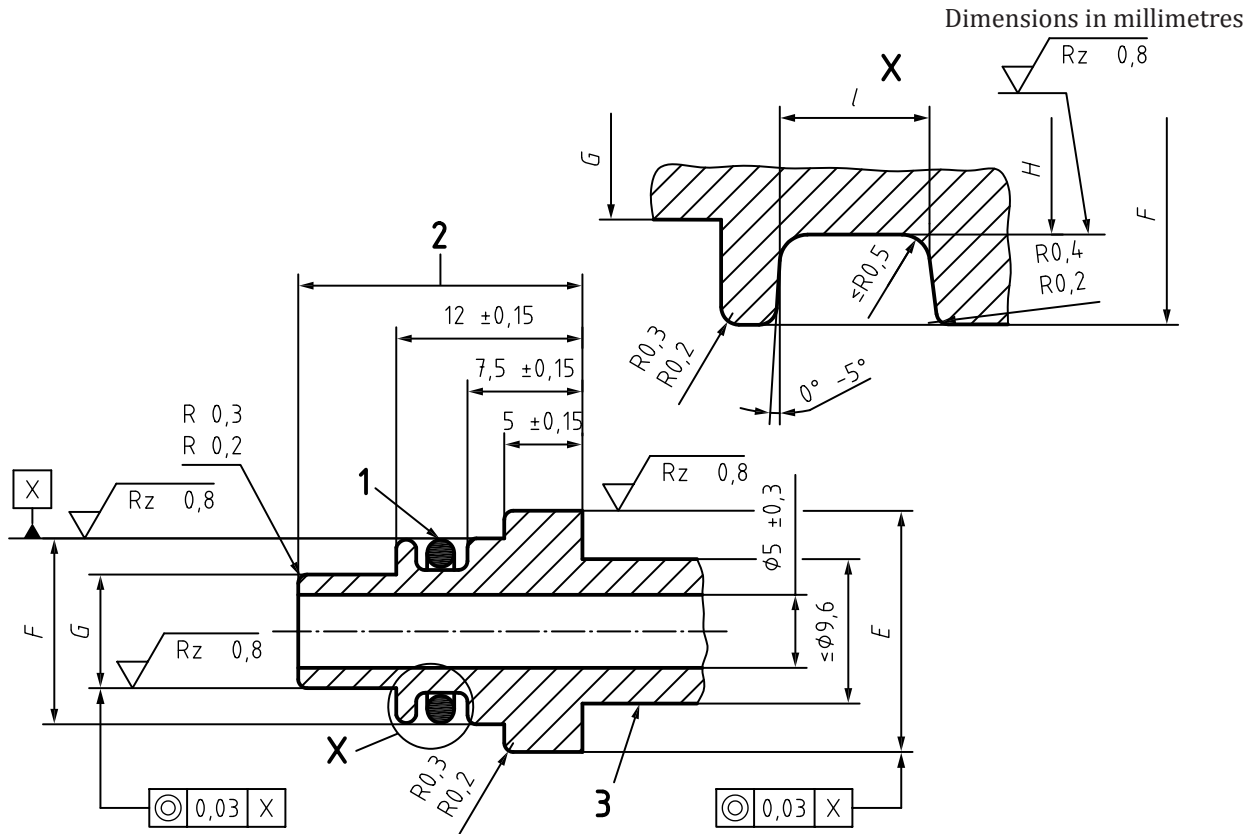


Surface finish shall be $\sqrt{\text{Rz } 1,6}$ unless otherwise stated.

Key

- 1 “O” ring (dimensions given in [Table 4](#))
- 2 A range: $18,5 \pm 0,15$, use “O” ring No 0076-24
 B range: $24,5 \pm 0,15$, use “O” ring No 0081-16
 C range: $30,5 \pm 0,15$, use “O” ring No 0071-16
- 3 position for marking gas identification symbol

NOTE Gas tightness and smooth operation are best achieved when the “O” ring is compressed between 0,66 mm and 0,19 mm in diameter under maximum and minimum tolerancing conditions. See [Table 3](#) for dimensions E, F, G, H and I.

Figure 2 — NIST nipple

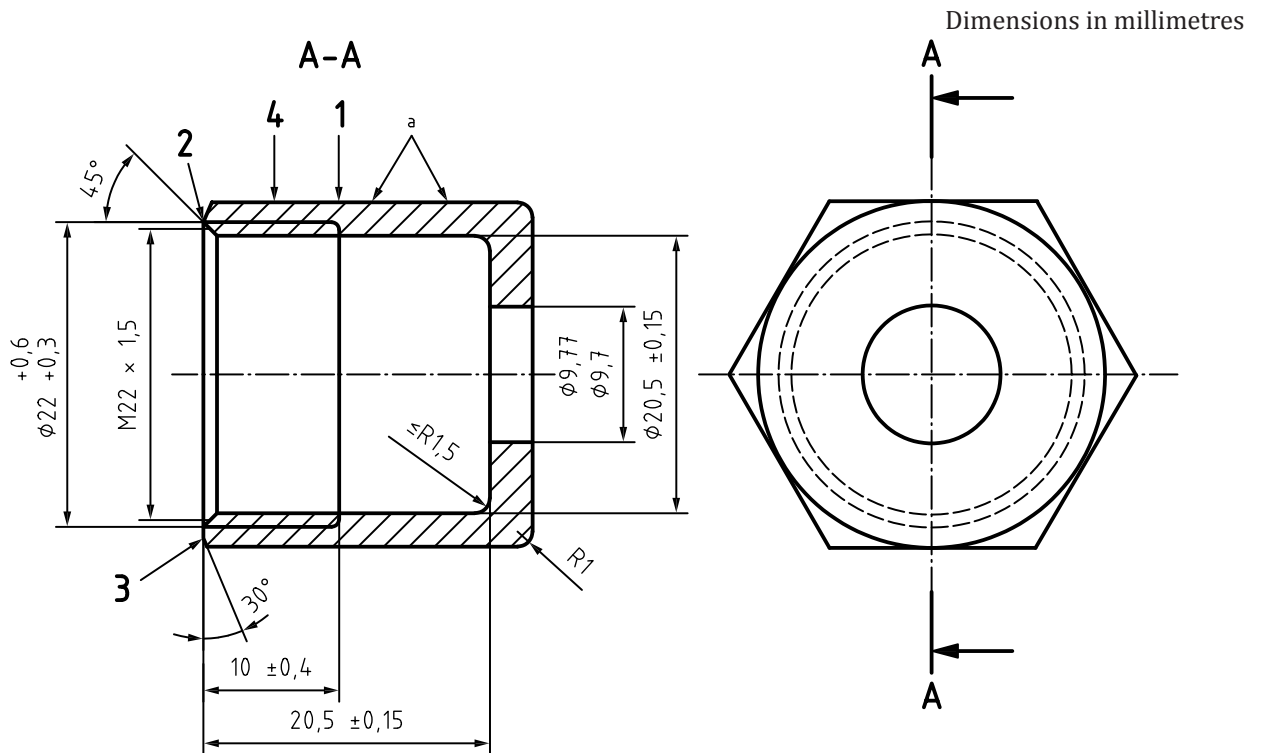

Surface finish shall be $\sqrt{Rz \ 1,6}$ unless otherwise stated.


Key

- 1 notch with Vee across corners of hexagon to depth of flat for identification of left hand nuts only
- 2 chamfer to root of the thread
- 3 external chamfer
- 4 position for marking gas identification symbol
- a This area should preferably be knurled.

NOTE External shape and dimensions can be varied to suit the materials used

Figure 3 — NIST nut

Dimensions in millimetres

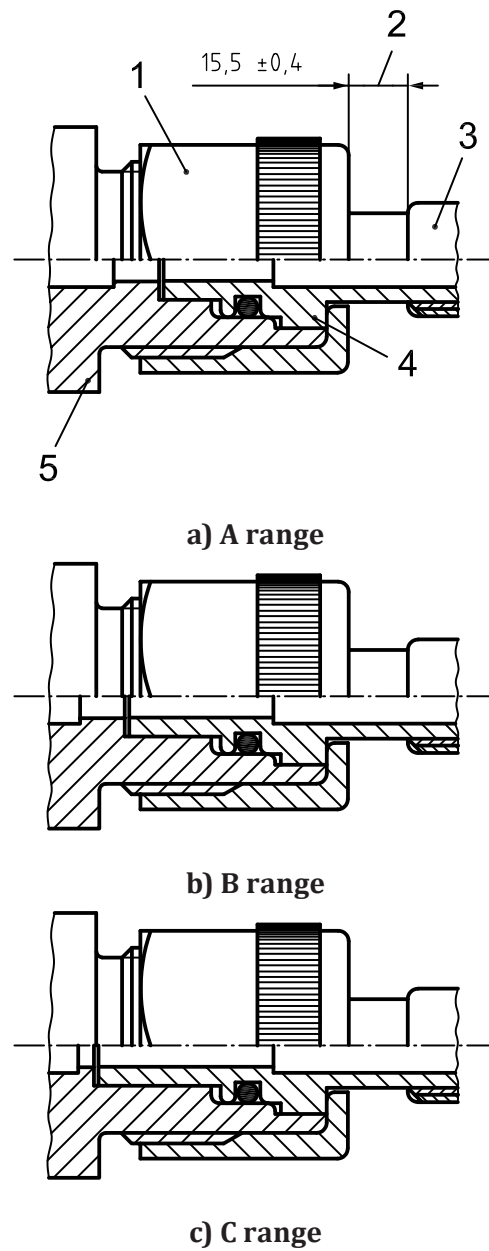

Key

- 1 NIST nut (see [Figure 3](#))
- 2 free motion area
- 3 ferrule or hose fixing device
- 4 NIST nipple (see [Figure 2](#))
- 5 NIST body (see [Figure 1](#))

Figure 4 — NIST assembly

NOTE Dimension 15,5 mm to allow access to “O”-ring on nipple.

4 Marking

The connectors shall be durably and legibly marked with the symbol of the relevant gas in accordance with [Table 5](#).

NOTE In addition to the symbol, the name of the gas may be used.

Check compliance for durability of markings by the test given in [Clause 5](#).

The marking shall be legible to a person having visual acuity (corrected if necessary) of 1 standing 0,5 m from the connector at an illuminance of 215 lx.

5 Test for durability of markings

Rub the markings by hand, without undue pressure, first for 15 s with a cloth rag soaked with distilled water, then for 15 s with a cloth rag soaked with methylated spirit and then for 15 s with a cloth rag soaked with isopropyl alcohol. Carry out these tests at ambient temperature. Verify that the markings are still legible.

Table 5 — Marking

Medical gas or mixture	Symbol
Oxygen	O ₂
Oxygen-enriched air	a
Nitrous oxide	N ₂ O
Oxygen/nitrous oxide mixture [O ₂ = 50 % (volume fraction)]	O ₂ /N ₂ O
Nitrous oxide/oxygen mixtures [N ₂ O < 80 % (volume fraction)]	N ₂ O/O ₂ ^b
Medical air	Air ^c
Air for driving surgical tools	Air - 800 ^c
Vacuum	Vac ^c
Air/oxygen mixture	Air/O ₂ ^c
Nitrogen for driving surgical tools	N ₂ - 800
Helium	He
Helium/oxygen mixture [O ₂ < 20 % (volume fraction)]	He/O ₂
Helium/oxygen mixture [He ≤ 80 % (volume fraction)]	O ₂ /He
Oxygen/carbon dioxide mixture [CO ₂ ≤ 7 % (volume fraction)]	O ₂ /CO ₂
Carbon dioxide	CO ₂
Carbon dioxide/oxygen mixture [CO ₂ > 7 % (volume fraction)]	CO ₂ /O ₂
Xenon	Xe
Medical air/helium/carbon monoxide [CO < 1 % (volume fraction)]	LFT ^d
Special gas mixture	e
<p>a To be defined by national authorities.</p> <p>b Except for oxygen/nitrous oxide mixtures [O₂ = 50 % (volume fraction)].</p> <p>c National languages may be used for air and vacuum.</p> <p>d Lung function test.</p> <p>e For limited experimental applications. Symbols for special gas mixtures should conform to the chemical symbols of the components.</p>	

Bibliography

- [1] ISO 48, *Rubber, vulcanized or thermoplastic — Determination of hardness (hardness between 10 IRHD and 100 IRHD)*
- [2] ISO 4135:2001, *Anaesthetic and respiratory equipment — Vocabulary*
- [3] ISO 5359, *Anaesthetic and respiratory equipment - Low-pressure hose assemblies for use with medical gases*¹⁾
- [4] ISO 7396-1:2007, *Medical gas pipeline systems — Part 1: Pipeline systems for compressed medical gases and vacuum*
- [5] ISO 9170-1:2008, *Terminal units for medical gas pipeline systems — Part 1: Terminal units for use with compressed medical gases and vacuum*
- [6] ISO 15001, *Anaesthetic and respiratory equipment — Compatibility with oxygen*
- [7] AS 2896:1998, *Medical gas systems - Installations and testing of non flammable medical gas pipeline systems*
- [8] BS 4518, *Specification for metric dimensions of toroidal sealing rings (“O” rings) and their housings*
- [9] CGA V-5, *Diameter Index Safety System (Non-Interchangeable Low Pressure Connections for Medical Gas Applications)*²⁾

1) To be published. Revision of ISO 5359:2008 and ISO 5359:2008/Amd.1:2011.

2) Compressed Gas Association Inc. (CGA), 1725 Jefferson Davis Highway, Arlington, VA 22202, USA.

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com



...making excellence a habit.™