

Dentistry — Reusable cartridge syringes intended for intraaligamentary injections

ICS 11.060.20

National foreword

This British Standard is the UK implementation of EN ISO 21533:2003. It is identical to ISO 21533:2003, incorporating corrigendum December 2009.

The UK participation in its preparation was entrusted by Technical Committee CH/106, Dentistry, to Subcommittee CH/106/4, Dental instruments.

A list of organizations represented on this subcommittee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard cannot confer immunity from legal obligations.

Amendments/corrigenda issued since publication

Amd. No.	Date	Comments
14762 Corrig. No. 1	20 October 2003	Incorporating corrected EN ISO foreword page and adding Annex ZA page
	31 March 2010	Implementation of ISO corrigendum December 2009, French title on EN ISO title page amended

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 27 June 2003

© BSI 2010

ICS 11.060.20

English version

Dentistry - Reusable cartridge syringes intended for
intragamutary injections (ISO 21533:2003)

Art dentaire - Seringues à cartouche réutilisables pour
injections intraligamentaires (ISO 21533:2003)

Zahnheilkunde - Wiederverwendbare Ampullenspritzen für
intragamentale Injektionen (ISO 21533:2003)

This European Standard was approved by CEN on 20 May 2003.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Luxembourg, Malta, Netherlands, Norway, Portugal, Slovakia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: rue de Stassart, 36 B-1050 Brussels

CORRECTED 2003-09-24

Foreword

This document (EN ISO 21533:2003) has been prepared by Technical Committee ISO/TC 106 "Dentistry" in collaboration with Technical Committee CEN/TC 55 "Dentistry", the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by December 2003, and conflicting national standards shall be withdrawn at the latest by December 2003.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Czech Republic, Denmark, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Luxembourg, Malta, Netherlands, Norway, Portugal, Slovakia, Spain, Sweden, Switzerland and the United Kingdom.

Endorsement notice

The text of ISO 21533:2003 has been approved by CEN as EN ISO 21533:2003 without any modifications.

NOTE Normative references to International Standards are listed in Annex ZA (normative).

Contents		Page
1	Scope.....	1
2	Normative references	1
3	Terms and definitions	1
4	Requirements	2
4.1	Design	2
4.2	Barrel	3
4.3	Threaded needle-mounting hub	3
4.4	Plunger rod	3
4.5	Volume of local anaesthetic delivered	3
4.6	Resistance against corrosion, autoclaving and thermal exposure	3
5	Test methods	4
5.1	Visual inspection.....	4
5.2	Measurement of volume delivered	4
5.3	Plunger rod displacement	4
5.4	Protective sleeve dislodgement	4
5.5	Boiling-water test	4
5.6	Autoclave test.....	4
5.7	Dry-heat test	4
6	Manufacturer's information.....	4
7	Marking.....	5
7.1	Marking of unit pack	5
7.2	Marking of syringe	5
Annex A (informative) Imperial thread sizes		6

Dentistry — Reusable cartridge syringes intended for intraligamentary injections

1 Scope

This International Standard specifies requirements and test methods for reusable cartridge syringes intended for intraligamentary injections.

It specifies requirements for dental cartridge syringes with ISO metric thread sizes, and only intended for intraligamentary injections. However, attention is drawn to the existence of a variety of syringes with imperial thread sizes (see Annex A).

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1942-3, *Dental vocabulary — Part 3: Dental instruments*

ISO 7885, *Sterile dental injection needles for single use*

ISO 9997, *Dental cartridge syringes*

ISO 11499, *Dental cartridges for local anaesthetics*

ISO 13402, *Surgical and dental hand instruments — Determination of resistance against autoclaving, corrosion and thermal exposure*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1942-3 and the following apply.

3.1

intraligamentary injection

injection made by the dentist via the periodontal ligament

3.2

reusable cartridge syringe intended for intraligamentary injections

syringe used in dentistry which can be resterilized and is specifically designed by the manufacturer for intraligamentary injections and uses a container for local anaesthetics

3.3

unit pack

pack which contains the syringe


3.4 lever
component which delivers the force to the plunger rod

3.5 protective sleeve
component which prevents pieces of a fractured cartridge leaving the syringe through the viewing port


4 Requirements

4.1 Design

The syringe shall be of either a pistol-grip design or a pen-grip design, as shown in Figure 1.

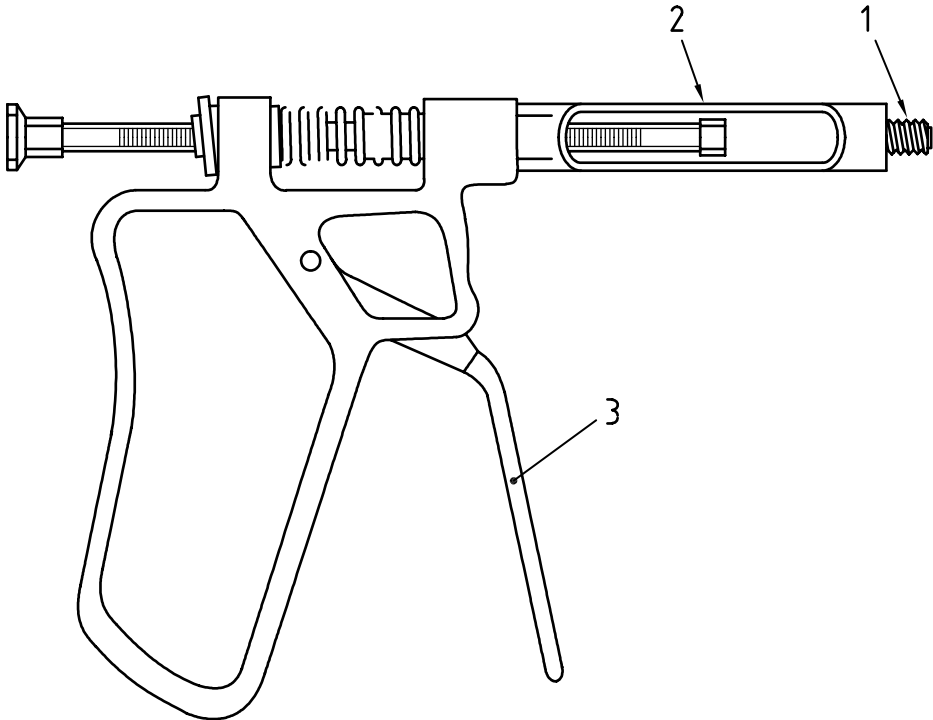

a) Pistol-grip design

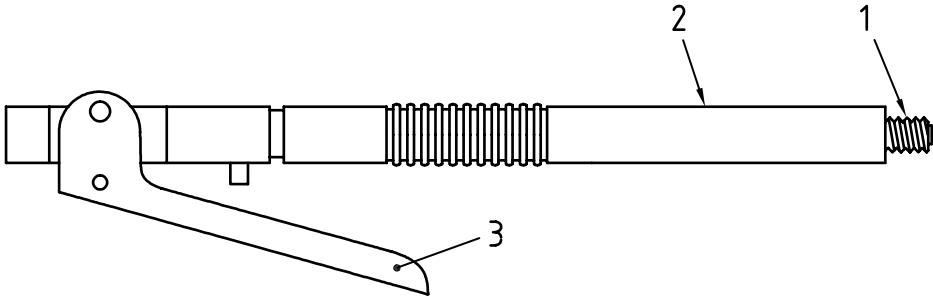

b) Pen-grip design

- Key**
- 1 threaded needle-mounting hub
 - 2 barrel
 - 3 lever

Figure 1 — Pistol-grip and pen-grip syringe designs

4.2 Barrel

4.2.1 General

The dimensions of the barrel shall conform to ISO 9997.

4.2.2 Loading of the cartridge

4.2.2.1 Syringes without viewing ports

Where a viewing port is not present, the dimensions of the barrel shall permit the loading of a cartridge which conforms to ISO 11499.

4.2.2.2 Syringes with viewing ports

Where a viewing port is present, the dimensions of the barrel shall permit the placement of a protective sleeve and shall permit the loading of a cartridge which conforms to ISO 11499.

4.3 Threaded needle-mounting hub

The dimensions of the threaded needle-mounting hub shall conform to ISO 9997.

4.4 Plunger rod

The diameter of the plunger rod tip shall be $6,0_{-1}^0$ mm. The length of the plunger rod shall allow maximum travel of the cartridge plunger.

The maximum sideways displacement of the rod shall not exceed 2 mm in any direction from the long axis of the syringe barrel.

Testing shall be carried out in accordance with 5.1 and 5.3.

4.5 Volume of local anaesthetic delivered

When tested in accordance with 5.2, the volume of local anaesthetic delivered at each depression of the lever shall be within 10 % of the volume claimed by the manufacturer.

4.6 Resistance against corrosion, autoclaving and thermal exposure

4.6.1 Syringe

The syringe shall function normally and show no signs of corrosion after the tests in 5.5, 5.6 and 5.7.

4.6.2 Protective sleeve

The protective sleeve, if supplied, shall be either single-use or capable of resterilization.

Test in accordance with 5.4.

If the sleeve is capable of resterilization, it shall fit after testing to 5.5, 5.6 and 5.7 and shall not become dislodged when tested in accordance with 5.4.

5 Test methods

5.1 Visual inspection

Visual inspection shall be conducted at normal visual acuity without magnification.

5.2 Measurement of volume delivered

Prepare the syringe with a glass dental local anaesthetic cartridge conforming to ISO 11499 and a needle conforming to ISO 7885. Depress the lever completely a sufficient number of times for anaesthetic to be delivered through the needle. Depress the lever three more times and measure the volume of anaesthetic delivered during each of these three depressions. Ensure that the lever returns to its initial position after each depression.

5.3 Plunger rod displacement

Remove the syringe barrel and position the plunger rod fully forward in the syringe. Measure the maximum sideways displacement at the front end of the plunger rod tip.

5.4 Protective sleeve dislodgement

Prepare the syringe for use as described in 5.2. Empty the deliverable contents of the cartridge via the needle. Check for dislodgement of the sleeve during the test.

5.5 Boiling-water test

Test the syringe five times as described in ISO 13402.

Visually inspect for compliance with the requirements of 4.6.

5.6 Autoclave test

Test the syringe five times as described in ISO 13402.

Visually inspect for compliance with the requirements of 4.6.

5.7 Dry-heat test

Test the syringe five times as described in ISO 13402.

Visually inspect for compliance with the requirements of 4.6.

6 Manufacturer's information

Each syringe shall be accompanied by the following information:

- a) indications for use;
- b) instructions for use;
- c) information concerning the mechanical advantage produced by the lever;
- d) the recommended cartridge size and material;
- e) methods of assembly and disassembly;

- f) methods of inserting the cartridge and attaching the needle;
- g) a statement directing the user to check before use that the barrel and handle are securely connected and that the interchangeable barrel end cap with needle hub (if fitted) is securely in position;
- h) the volume of anaesthetic solution delivered per depression of the lever;
- i) recommended methods of reprocessing for re-use.

7 Marking

7.1 Marking of unit pack

Each unit pack shall be marked with the following information:

- a) the contents of the pack;
- b) the name or registered trade mark of the manufacturer;
- c) the words “syringe intended for intraligamentary injections” or equivalent;
- d) the classification as a pistol-grip or pen-grip design;
- e) details of the needle-mounting thread;
- f) the size(s) of dental local anaesthetic cartridge(s) to use;
- g) if a protective sleeve is supplied, an indication of whether the protective sleeve is single-use or can be resterilized;
- h) if a protective sleeve is not supplied, details of the protective sleeve to be used;
- i) the lot number.

7.2 Marking of syringe

Each syringe shall be indelibly marked with the name or registered trade mark of the manufacturer.

Annex A
(informative)

Imperial thread sizes

Clause 1 mentions the existence of imperial thread sizes for the needle-mounting threads.

In the interests of patient safety, the imperial thread size used should be $0,216_{-0,003}^0$ in ($5,486_{-0,08}^0$ mm) in 40 TPI (threads per inch) Whitworth form.

Annex ZA
(normative)

**Normative references to international publications
with their relevant European publications**

This European Standard incorporates by dated or undated reference, provisions from other publications. These normative references are cited at the appropriate places in the text and the publications are listed hereafter. For dated references, subsequent amendments to or revisions of any of these publications apply to this European Standard only when incorporated in it by amendment or revision. For undated references the latest edition of the publication referred to applies (including amendments).

NOTE Where an International Publication has been modified by common modifications, indicated by (mod.), the relevant EN/HD applies.

<u>Publication</u>	<u>Year</u>	<u>Title</u>	<u>EN</u>	<u>Year</u>
ISO 1942-3	1989	Dental vocabulary - Part 3: Dental instruments	EN 21942-3	1993
ISO 7885	2000	Sterile dental injection needles for single use	EN ISO 7885	2000
ISO 9997	1999	Dental cartridge syringes	EN ISO 9997	1999
ISO 11499	1997	Dental cartridges for local anaesthetics	EN ISO 11499	1999
ISO 13402	1995	Surgical and dental hand instruments - Determination of resistance against autoclaving, corrosion and thermal exposure	EN ISO 13402	2000

BSI - British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001 Email: orders@bsigroup.com You may also buy directly using a debit/credit card from the BSI Shop on the Website <http://www.bsigroup.com/shop>

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact Information Centre. Tel: +44 (0)20 8996 7111 Fax: +44 (0)20 8996 7048 Email: info@bsigroup.com

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002 Fax: +44 (0)20 8996 7001 Email: membership@bsigroup.com

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsigroup.com/BSOL>

Further information about BSI is available on the BSI website at <http://www.bsigroup.com>

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright and Licensing Manager. Tel: +44 (0)20 8996 7070 Email: copyright@bsigroup.com