

**Water quality —  
Determination of  
Chromium(VI) —  
Method using flow  
analysis (FIA and CFA)  
and spectrometric  
detection  
(ISO 23913:2006)**

ICS 13.060.50

## National foreword

This British Standard is the UK implementation of EN ISO 23913:2009. It is identical to ISO 23913:2006.

The UK participation in its preparation was entrusted to Technical Committee EH/3/2, Physical chemical and biochemical methods.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

**Compliance with a British Standard cannot confer immunity from legal obligations.**

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 October 2009.  
© BSI 2009

### Amendments/corrigenda issued since publication

Date	Comments

**ISBN 978 0 580 68104 2**

---

EUROPEAN STANDARD  
 NORME EUROPÉENNE  
 EUROPÄISCHE NORM

**EN ISO 23913**

May 2009

ICS 13.060.50

English Version

**Water quality - Determination of chromium(VI) - Method using flow analysis (FIA and CFA) and spectrometric detection (ISO 23913:2006)**

Qualité de l'eau - Dosage du chrome(VI) - Méthode par analyse en flux (FIA et CFA) et détection spectrométrique (ISO 23913:2006)

Wasserbeschaffenheit - Bestimmung von Chrom(VI) - Verfahren mittels Fließanalytik (FIA und CFA) und spektrometrischer Detektion (ISO 23913:2006)

This European Standard was approved by CEN on 14 May 2009.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION  
 COMITÉ EUROPÉEN DE NORMALISATION  
 EUROPÄISCHES KOMITEE FÜR NORMUNG

**Management Centre: Avenue Marnix 17, B-1000 Brussels**

## **Foreword**

The text of ISO 23913:2006 has been prepared by Technical Committee ISO/TC 147 "Water quality" of the International Organization for Standardization (ISO) and has been taken over as EN ISO 23913:2009 by Technical Committee CEN/TC 230 "Water analysis" the secretariat of which is held by DIN.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by November 2009, and conflicting national standards shall be withdrawn at the latest by November 2009.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and the United Kingdom.

### **Endorsement notice**

The text of ISO 23913:2006 has been approved by CEN as a EN ISO 23913:2009 without any modification.

## Contents

Page

Foreword.....	iv
Introduction .....	v
<b>1 Scope .....</b>	<b>1</b>
<b>2 Normative references .....</b>	<b>1</b>
<b>3 Principle.....</b>	<b>1</b>
<b>4 Interferences .....</b>	<b>2</b>
<b>5 Reagents .....</b>	<b>2</b>
<b>6 Apparatus .....</b>	<b>5</b>
<b>7 Sampling and sample preparation .....</b>	<b>6</b>
<b>8 Procedure .....</b>	<b>6</b>
<b>9 Determination .....</b>	<b>7</b>
<b>10 Expression of results .....</b>	<b>8</b>
<b>11 Test report .....</b>	<b>8</b>
<b>Annex A (informative) Examples of flow analysis systems for the determination of chromium(VI) .....</b>	<b>9</b>
<b>Annex B (informative) Performance characteristics.....</b>	<b>12</b>
<b>Bibliography .....</b>	<b>14</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 23913 was prepared by Technical Committee ISO/TC 147, *Water quality*, Subcommittee SC 2, *Physical, chemical and biochemical methods*.

## Introduction

Methods using flow analysis automatic wet chemical procedures are particularly suitable for the processing of many analytes in water, in large sample series at a high analysis frequency.

Analysis can be performed by flow injection analysis (FIA) [1], [2] and continuous flow analysis (CFA). Both methods share the feature of an automatic dosage of the sample into a flow system (manifold) where the analyte in the sample reacts with the reagent solutions on its way through the manifold. The sample preparation may be integrated in the manifold. The reaction product is measured in a flow detector (e.g. flow photometer).

It should be investigated whether and to what extent particular problems will require the specification of additional marginal conditions.





# Water quality — Determination of chromium(VI) — Method using flow analysis (FIA and CFA) and spectrometric detection

**WARNING** — Persons using this International Standard should be familiar with normal laboratory practice. This standard does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

**IMPORTANT** — It is absolutely essential that tests conducted according to this International Standard are carried out by suitably qualified staff.

## 1 Scope

This International Standard specifies flow injection analysis (FIA) and continuous flow analysis (CFA) methods for the determination of chromium(VI) in various types of water. The method applies to the following mass concentration ranges.

FIA: 20 µg/l to 200 µg/l and 200 µg/l to 2 000 µg/l for surface water, leachates and waste water.

CFA: 2 µg/l to 20 µg/l and 20 µg/l to 200 µg/l for drinking water, ground water, surface water, leachates and waste water.

The range of application may be changed by varying the operating conditions.

Seawater may be analysed by these methods with changes in sensitivity and after adaptation of the reagent and calibration solutions to the salinity of the samples.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 5667-3, *Water quality — Sampling — Part 3: Guidance on the preservation and handling of water samples*

ISO 8466-1, *Water quality — Calibration and evaluation of analytical methods and estimation of performance characteristics — Part 1: Statistical evaluation of the linear calibration function*

## 3 Principle

Chromium(VI) reacts with 1,5-diphenylcarbazide (DPC) to form a red-violet chromium-1,5-diphenylcarbazone complex. The absorbance of this complex is measured at  $544 \text{ nm} \pm 10 \text{ nm}$  (maximum absorbance at 544 nm).

## 4 Interferences

Reducing agents in the sample may lead to negative bias for the chromium(VI) concentration.

Nitrite does not interfere with the method under the reaction conditions.

Concentrations of sulfide exceeding 0,2 mg/l interfere with the method.

Oxidizing agents for disinfection in drinking water production like chlorine, chlorine dioxide, ozone and hydrogen peroxide do not interfere with the method provided their mass concentration does not exceed the concentrations given in Table 1.

**Table 1 — Mass concentrations of single disinfection agents not producing significant interference under the given measuring conditions**

Disinfectant	Concentration mg/l
Chlorine	0,6
Chlorine dioxide	0,4
Hydrogen peroxide	0,2
Ozone	0,1

Other oxidizing agents like peroxyacetic acid, or permanganate may interfere in the chromium(VI) determination. This shall be considered in the results.

Strongly alkaline or buffered samples may cause negative bias. This effect may be tested by adding 1 part of acid mixture (5.5.1 or 5.5.2) to 3 parts of the sample. This mixture shall have a pH of < 1. Otherwise, pretreat the samples with acids (HCl, H<sub>2</sub>SO<sub>4</sub>) until the above mentioned test leads to sufficient results.

Iron (III) ions exceeding 10 mg/l interfere with the methods. In the range of 10 mg/l to 100 mg/l, iron (III) ions may lead to a negative bias of up to 8 %.

Coloured or turbid samples can cause a bias. To avoid bias, measure the sample again using solution 5.17 instead of solution 5.10 for feeding line "R2" in Figures A.1 to A.3. Subtract the result of this measurement  $y_s$  from the term  $y$  in Equation (2).

## 5 Reagents

Use analytical grade chemicals unless otherwise specified.

**5.1 Water**, complying to grade 1 as defined in ISO 3696. The chromium blank value shall be checked (see 8.3).

**5.2 Sulfuric acid**,  $\rho(\text{H}_2\text{SO}_4) = 1,84$  g/ml.

**5.3 Orthophosphoric acid**,  $\rho(\text{H}_3\text{PO}_4) = 1,71$  g/ml.

**5.4 Surfactant solution**, aqueous polyethylene glycol dodecyl ether,  $[\text{HO}-(\text{CH}_2-\text{CH}_2\text{O})_n\text{C}_{12}\text{H}_{21}]$ , with a mass fraction of 30 %.

## 5.5 Acid mixtures.

### 5.5.1 Acid mixture for FIA, (R1 in Figure A.1).

Add to a 250 ml volumetric flask about 125 ml of water (5.1). Add 29 ml of sulfuric acid (5.2) and 31 ml of orthophosphoric acid (5.3), mix and bring to volume with water (5.1).

This solution acidifies the reaction mixture passing the detector to a necessary pH of  $< 1$ .

The solution is stable for up to 1 year if stored at room temperature.

### 5.5.2 Acid mixture for CFA, (R1 in Figures A.2 and A.3).

Add 1 ml of surfactant solution (5.4) to 200 ml of acid mixture for FIA (5.5.1).

The solution is stable for up to 1 week if stored at room temperature.

## 5.6 1,5-diphenylcarbazide, $C_{13}H_{14}N_4O$ .

## 5.7 Acetone, $C_3H_6O$ .

## 5.8 1-Propanol, $C_3H_8O$ .

## 5.9 Potassium dichromate, $K_2Cr_2O_7$ .

### 5.10 Diphenylcarbazide solution, (R2 in Figures A.1 to A.3).

Dissolve in a 250 ml beaker 0,43 g of 1,5-diphenylcarbazide (5.6) in 9 ml of acetone (5.7) and 9 ml of 1-propanol (5.8). Add 125 ml of 1-propanol (5.8). Transfer the mixture to a 250 ml volumetric flask, and make up to volume with water (5.1).

The solution is stable for up to 1 week if stored in a brown glass bottle at  $2\text{ }^{\circ}\text{C}$  to  $6\text{ }^{\circ}\text{C}$ .

If precipitation occurs, filter the solution.

NOTE The use of a mixture of acetone and 1-propanol permits the redissolving of precipitates of 1,5-diphenylcarbazide occurring on cooling. In the literature, several solvents (acetone, 1-propanol, 2-propanol, ethanol, in combination with water) are proposed for preparing the diphenylcarbazide solution. These alternatives are also applicable, provided the solutions are stable enough and contain the same concentration of 1,5-diphenylcarbazide (5.6) as given in 5.10.

Degas carefully all reagent solutions for the FIA determinations before use, e.g. by vacuum filtration.

### 5.11 Carrier solution for FIA systems, (C in Figure A.1).

Use water (5.1).

Carrier and samples should have identical acidity. For unpreserved samples, this means that water should be used as a carrier. According to References [5] and [6] in the Bibliography, acidic preservation should be avoided in chromium speciation because of low recovery.

### 5.12 Chromium(VI) stock solution, $\rho[\text{Cr(VI)}] = 1\ 000\ \text{mg/l}$ .

#### **WARNING — Potassium dichromate is carcinogenic.**

Dissolve 2,829 g of potassium dichromate,  $K_2Cr_2O_7$  (5.9) in water (5.1) in a 1 000 ml volumetric flask. Dilute to volume with water (5.1).

The solution is stable for up to 1 year if stored at room temperature.

1 ml of this solution contains 1 mg of Cr(VI).

NOTE Chromium(VI) solutions are commercially available and may be used in this International Standard.

**5.13 Chromium(VI) standard solution I,  $\rho[\text{Cr(VI)}] = 10 \text{ mg/l}$ .**

Pipette 1 ml of the chromium(VI) stock solution (5.12), into a 100 ml volumetric flask. Dilute to volume with water (5.1).

Prepare this solution fresh daily. The solution can be stored during the day of use at room temperature.

1 ml of this solution contains 10  $\mu\text{g}$  of Cr.

**5.14 Chromium(VI) standard solution II,  $\rho[\text{Cr(VI)}] = 1 \text{ mg/l}$ .**

Pipette 10 ml of the chromium(VI) standard solution I (5.13), into a 100 ml volumetric flask. Dilute to volume with water (5.1).

Prepare this solution fresh daily. The solution can be stored during the day of use at room temperature.

1 ml of this solution contains 1  $\mu\text{g}$  of Cr.

**5.15 Chromium(VI) standard solution III,  $\rho[\text{Cr(VI)}] = 0,1 \text{ mg/l}$ .**

Pipette 10 ml of the chromium(VI) standard solution II (5.14), into a 100 ml volumetric flask. Dilute to volume with water (5.1).

Prepare this solution fresh daily. The solution can be stored during the day of use at room temperature.

1 ml of this solution contains 0,1  $\mu\text{g}$  of Cr.

**5.16 Calibration solutions.**

Prepare calibration solutions by diluting solutions 5.13 to 5.15 according to the range required. For examples, see Tables 2, 3 and 4. At least five calibration standards per working range are recommended.

**Table 2 — Example for the preparation of 10 calibration solutions for the range 2  $\mu\text{g/l}$  to 20  $\mu\text{g/l}$  Cr**

Millilitres of chromium(VI) standard solution III (5.15) diluted to 100 ml	2	4	6	8	10	12	14	16	18	20
Concentration of chromium in the calibration solutions in micrograms per litre, $\mu\text{g/l}$	2	4	6	8	10	12	14	16	18	20

**Table 3 — Example for the preparation of 10 calibration solutions for the range 20  $\mu\text{g/l}$  to 200  $\mu\text{g/l}$  Cr**

Millilitres of chromium(VI) standard solution II (5.14) diluted to 100 ml	2	4	6	8	10	12	14	16	18	20
Concentration of chromium in the calibration solutions in micrograms per litre, $\mu\text{g/l}$	20	40	60	80	100	120	140	160	180	200

**Table 4 — Example for the preparation of 10 calibration solutions for the range 200  $\mu\text{g/l}$  to 2 000  $\mu\text{g/l}$  Cr**

Millilitres of chromium(VI) standard solution I (5.13) diluted to 100 ml	2	4	6	8	10	12	14	16	18	20
Concentration of chromium in the calibration solutions in micrograms per litre, $\mu\text{g/l}$	200	400	600	800	1000	1200	1400	1600	1800	2000

Prepare the calibration solutions daily. The solutions can be stored during the day of use at room temperature.

#### **5.17 Solution for measuring the self absorbance of samples** (optional for coloured or turbid samples).

Mix in a 250 ml volumetric flask 9 ml of acetone (5.7), 9 ml of 1-propanol (5.8) and 125 ml of 1-propanol (5.8). Make up to volume with water (5.1).

The mixture is stable for up to 1 month if stored at 2 °C to 6 °C.

## **6 Apparatus**

Usual laboratory apparatus, and, in particular the following.

### **6.1 Flow injection analysis (FIA).**

The system generally consists of the following components (see Figure A.1):

#### **6.1.1 Reagent containers.**

#### **6.1.2 Low-pulsation pump** with suitable pump tubes.

#### **6.1.3 Manifold with transmission tubing**, 0,5 mm to 0,8 mm internal diameter, connectors and T-pieces of chemically inert materials.

#### **6.1.4 Photometric flow-through detector**, wavelength (544 ± 10) nm, wavelength maximum 544 nm.

#### **6.1.5 Data display unit**, such as a PC, printer or plotter; in general, peak height signals are evaluated.

#### **6.1.6 Sample changer**, if required.

### **6.2 Continuous-flow analysis (CFA).**

The system generally consists of the following components (see Figures A.2 and A.3):

#### **6.2.1 Sampler or other device**, for reproducible sample introduction.

#### **6.2.2 Reagent containers.**

#### **6.2.3 Peristaltic pump**, with suitable pump tubes inert to the reagents used.

#### **6.2.4 Thermostated reaction coil**, only for the determination of the sum of chromium(VI) and chromium(III).

#### **6.2.5 Manifold**, with reproducible gas bubble introduction, sample and reagent introduction and components of chemically inert materials.

#### **6.2.6 Photometric flow-through detector**, wavelength (544 ± 10) nm.

#### **6.2.7 Data display unit**, such as a PC, printer or plotter; in general peak height signals are evaluated.

NOTE Figures A.2 and A.3 show CFA systems with 2 mm internal diameter tubing (so-called "macroflow"). Other tubing diameters (e.g. 1 mm; so-called "microflow") may be used as long as the flow rates are in the same proportion and the recovery rates in 8.2 are achieved.

### **6.3 Additional apparatus.**

#### **6.3.1 Graduated flasks**, nominal capacity 100 ml, 200 ml and 1 000 ml.

#### **6.3.2 Pipettes**, nominal capacity 1 ml, 2 ml, 5 ml and 10 ml.

**6.3.3 Membrane filter assembly**, with membrane filters, pore size 0,45 µm.

**6.3.4 Analytical balance**.

## 7 Sampling and sample preparation

Preserve samples as specified in ISO 5667-3. Samples for the determination of Cr(VI) may be stored for a maximum of 24 h at 2 °C to 5 °C. Directly prior to the analysis acidify the samples by adding 10 ml of 0,5 mol/l sulfuric acid to 1 l of sample. The pH should be approximately 3. If necessary, filter the acidified sample (folded filter).

Do not treat the samples for the determination of chromium(VI) by the addition of reagents (e.g. formaldehyde) in order to prevent the change of chromium species by reduction.

## 8 Procedure

### 8.1 General

Use the procedure specified by the analyser manufacturer as long as it is not in contradiction with this International Standard.

### 8.2 Preparing for the analysis

Set up the flow analyser for the desired procedure (FIA or CFA: see Figures A.1 to A.3).

Pump water as sample (line "S" in Figures A.1 to A.3) and the reagents for up to 10 min.

The pH of the reaction mixture (see line "W" in Figure A.1, and line "A" in Figures A.2 and A.3) shall be < 1.

The analyser is ready when there is no baseline drift. Proceed then with steps 8.3 to 8.5.

### 8.3 Quality requirements for the measuring system, instrument performance checks

#### 8.3.1 Checking the reagent blank

Wait for a stable baseline.

Replace the reagent solutions R1 and R2 with water (5.1).

If the absorbance per centimetre is reduced by more than  $0,01 \text{ cm}^{-1}$  the reagents or the water may be contaminated, and suitable measures to eliminate the interference shall be undertaken before starting the analysis.

Pump reagents solutions again.

If the photometric detector (6.1 or 6.2) does not allow any absorbance readings, the absorbance may be determined by comparing with an external absorbance measuring photometer.

#### 8.3.2 Daily sensitivity test and noise test

Calibration solutions (5.16) with the smallest chromium concentration of each working range shall exhibit an absorbance per centimetre of at least  $0,005 \text{ cm}^{-1}$  for FIA and  $0,003 \text{ cm}^{-1}$  for CFA and shall exhibit a signal to noise relation of at least 3:1.

## 8.4 Calibration

Select the desired working range and the appropriate calibration solutions (5.16).

Use a separate calibration with at least 5 calibration solutions for each working range.

Before starting the analysis, set the output signal to zero.

Calibrate by sequentially applying the calibration solutions and reagent blanks.

Obtain the measured values corresponding to the calibration solutions applied. The output signal is proportional to the chromium(VI) concentration.

Make sure that the analytical conditions for the calibration solutions and the analytical samples are identical (see 8.5).

The following general Equation (1) for the linear calibration [ISO 8466-1] applies.

$$y = a + b \cdot \rho \quad (1)$$

where

$y$  is the measured value, in system related units;

$b$  is the slope of the calibration curve, in system related units litres per micrograms, l/ $\mu$ g or in system related units · litres per milligram, l/mg;

$\rho$  is the mass concentration of chromium(VI), in micrograms per litre,  $\mu$ g/l or in milligrams per litre, mg/l;

$a$  is the calibration curve intercept, in system related units.

## 8.5 Measurement

Analyse samples, prepared according to Clause 7, in the same way as the calibration solutions (5.16).

If the sample concentration is higher than the selected working range, analyse the sample in a different range or dilute.

After each group of sample measurements, at least after every 20 measurements, check the system calibration, using one calibration solution (5.16) each for lower and upper part of the respective working range. If the results of these two solutions are placed outside the confidence range of the calibration curve re-calibrate the system.

## 9 Determination

Calculate the mass concentration of chromium(VI) in the samples using Equation (2):

$$\rho = (y - a) / b \quad (2)$$

In the case of coloured or turbid samples, use Equation (3):

$$\rho = (y - y_s - a) / b \quad (3)$$

where

$y_s$  is the measurement value using solution 5.17 instead of solution 5.10 (see Clause 4), in system related unit.

For the explanation of the other symbols, see Equation (1).

Calculate samples according to the calibration range they fall into. Do not extrapolate a calibration curve beyond the working range selected.

## 10 Expression of results

Report the results as  $\mu\text{g/l}$  or  $\text{mg/l}$  to no more than 2 significant figures.

### EXAMPLES

Cr(VI): 8,9  $\mu\text{g/l}$

Cr(VI): 1,5  $\text{mg/l}$

## 11 Test report


The test report shall specify the following:

- a) reference to this International Standard (ISO 23913:2006);
- b) identity of the sample;
- c) outline of the procedure used;
- d) analysis procedure used (CFA or FIA);
- e) sample preparation, if any;
- f) description of the equipment used (6.1 or 6.2);
- g) results, according to Clause 10;
- h) any deviation from this International Standard or any circumstances which might affected the result.



## Annex A (informative)


### Examples of flow analysis systems for the determination of chromium(VI)

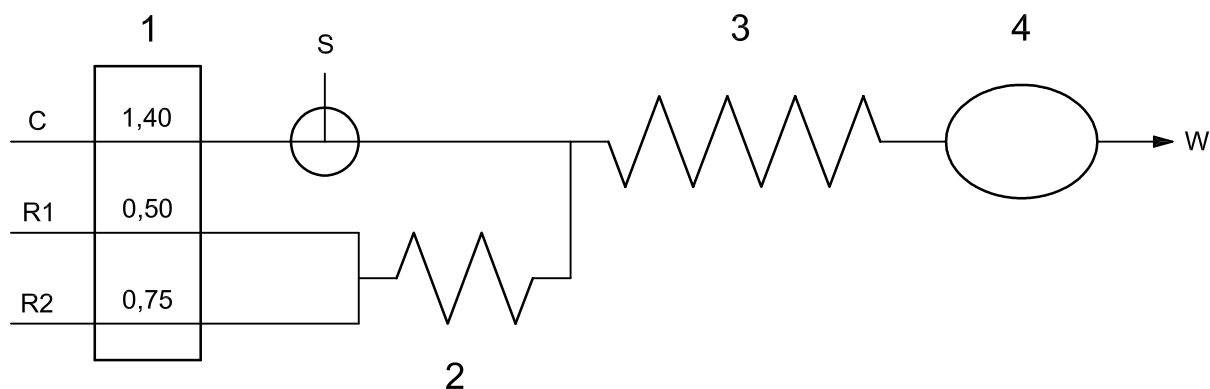

#### Key

- 1 pump; flow rates in millilitres per minute, ml/min
- S sample injector; injected volumes:  
200  $\mu\text{l}$  for the working range 20  $\mu\text{g/l}$  to 200  $\mu\text{g/l}$  Cr;  
30  $\mu\text{l}$  for the working range 0,2 mg/l to 2 mg/l Cr
- 2 reaction coil, length: 100 cm, internal diameter: 0,5 mm
- 3 reaction coil, length: 150 cm, internal diameter: 0,5 mm
- 4 detector, wavelength: 544 nm  $\pm$  10 nm; optical path length: 10 mm
- C carrier (5.11); flow rate 1,4 ml/min
- R1 acid mixture for FIA (5.5.1); flow rate 0,5 ml/min
- R2 diphenylcarbazide solution (5.10), or if the self absorbance of the sample  $y_s$  should be measured, solution 5.17 (see Clauses 4 and 9); flow rate 0,75 ml/min
- W reaction mixture after measurement; pH < 1


**Figure A.1 — Example of a FIA system for the determination of chromium(VI) in the concentration ranges 0,02 mg/l to 0,2 mg/l and 0,2 mg/l to 2 mg/l**

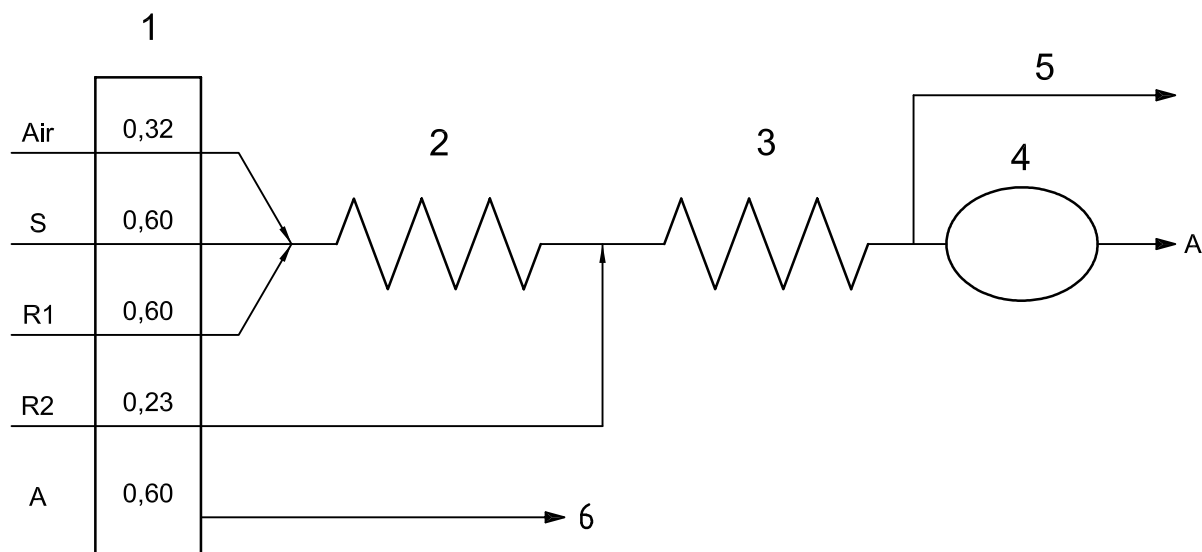

**Key**

- 1 pump; flow rates in millilitres per minute, ml/min
- 2 reaction coil, length: 200 cm, internal diameter: 2 mm
- 3 reaction coil, length: 150 cm, internal diameter: 2 mm
- 4 detector wavelength: 544 nm ± 10 nm, recommended optical path length: 50 mm
- S sample; flow rate 0,60 ml/min
- Air segmentation gas (e.g. air); flow rate 0,32 ml/min
- R1 acid mixture for CFA (5.5.2); flow rate 0,60 ml/min
- R2 diphenylcarbazide solution (5.10), or if the self absorbance of the sample  $y_s$  should be measured, solution 5.17 (see Clauses 4 and 9); flow rate 0,23 ml/min
- A desegmented reaction mixture; flow rate 0,60 ml/min; pH < 1
- 5 waste 1: Reaction mixture containing air bubbles
- 6 waste 2: Reaction mixture without air bubbles; pH < 1

**Figure A.2 — Example of a CFA system for the determination of chromium(VI) in the concentration range 20 µg/l to 200 µg/l Cr(VI)**

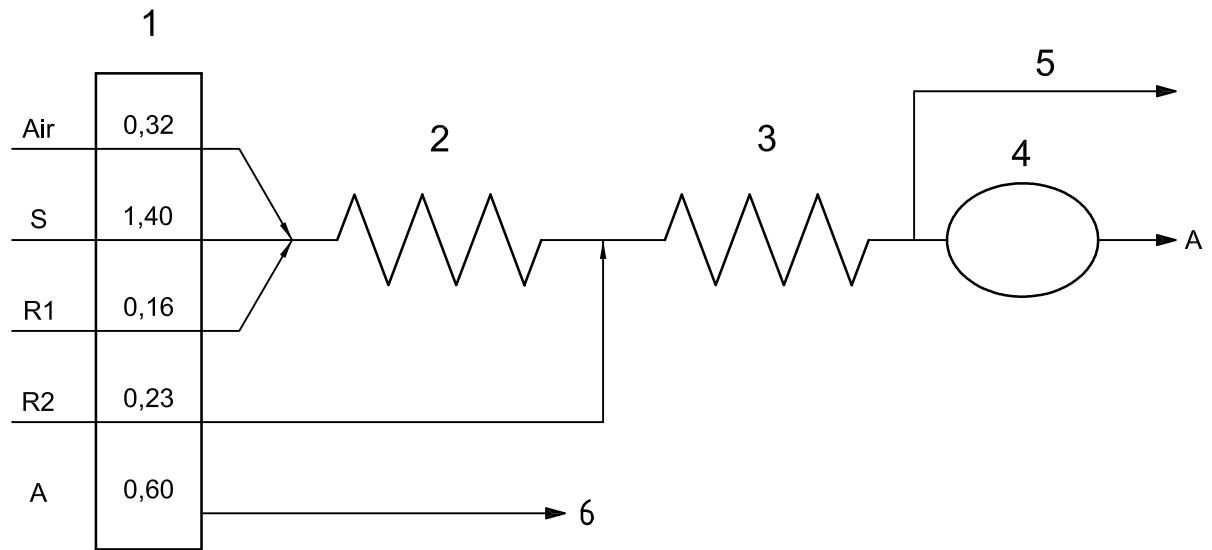

**Key**

- 1 pump; flow rates in millilitres per minute, ml/min
- 2 reaction coil, length: 50 cm, internal diameter: 2 mm
- 3 reaction coil, length: 150 cm, internal diameter: 2 mm
- 4 detector wavelength: 544 nm ± 10 nm; optical path length: 50 mm
- Air segmentation gas (e.g. air); flow rate 0,32 ml/min
- S sample; flow rate 1,4 ml/min
- R1 acid mixture for CFA (5.5.2); flow rate 0,16 ml/min
- R2 diphenylcarbazide solution (5.10) or if the self absorbance of the sample  $y_s$  should be measured solution 5.17 (see Clauses 4 and 9); flow rate 0,23 ml/min
- A desegmented reaction mixture; flow rate 0,60 ml/min, pH < 1
- 5 waste 1: Reaction mixture containing air bubbles
- 6 waste 2: Reaction mixture without air bubbles; pH < 1

**Figure A.3 — Example of a CFA system for the determination of chromium(VI) in the concentration range 2 µg/l to 20 µg/l Cr(VI)**

## Annex B (informative)

### Performance characteristics

The performance characteristics in Tables B.1 and B.2 have been established in an interlaboratory trial carried out in February 2005.

**Table B.1 — Performance data for the determination of chromium(VI) by FIA, according to ISO 5725-2**

Sample	Matrix	<i>l</i>	<i>n</i>	<i>o</i> %	$x_{\text{exp}}$ µg/l	$\bar{x}$ µg/l	$\eta$ %	$s_R$ µg/l	$CV_R$ %	$s_r$ µg/l	$CV_r$ %
7	Drinking water	8	32	11	130	128,7	99	6,057	4,706	3,047	2,368
8	Surface water	8	32	11	70	67,33	96	4,489	6,667	2,891	4,294
9	Waste water	8	32	11	54	50,34	93	3,867	7,681	2,477	4,921
10	Drinking water	8	32	11	500	504,8	101	14,95	2,961	4,899	0,970
11	Surface water	8	32	11	1 600	1 548	97	48,13	3,109	6,618	0,428
12	Waste water	8	32	11	360	349,0	97	17,82	5,106	7,402	2,121

**Symbols:**

- l* is the number of laboratories (outlier-free) (target value:  $\geq 8$ )
- n* is the number of outlier-free individual analytical values
- o* is the relative portion of outliers
- $x_{\text{exp}}$  is the accepted true value
- $\bar{x}$  is the total mean, depending on outlier-free values
- $\eta$  is the recovery rate
- $s_R$  is the reproducibility standard deviation
- $CV_R$  is the reproducibility coefficient of variation
- $s_r$  is the repeatability standard deviation
- $CV_r$  is the repeatability coefficient of variation

**Applied samples:**

- 7 and 10 Drinking water, original content of Cr(VI) < working range; spiked with  $K_2Cr_2O_7$
- 8 and 11 Surface water (Landwehrkanal, Berlin), original content of Cr(VI) < working range; spiked with  $K_2Cr_2O_7$
- 9 and 12 Domestic waste water (city of Berlin), original content of Cr(VI) < working range; spiked with  $K_2Cr_2O_7$

**Working ranges:**

- 20 µg/l to 200 µg/l samples 7, 8 and 9
- 200 µg/l to 2 000 µg/l samples 10, 11 and 12

Table B.2 — Performance data for the determination of chromium(VI) by CFA, according to ISO 5725-2

Sample	Matrix	<i>l</i>	<i>n</i>	<i>o</i> %	$x_{\text{exp}}$ µg/l	$\bar{x}$ µg/l	$\eta$ %	$s_R$ µg/l	$CV_R$ %	$s_r$ µg/l	$CV_r$ %
1	Drinking water	9	36	0	17,8	16,44	92	0,884	5,377	0,302	1,837
2	Surface water	8	32	11	7	6,59	94	1,027	15,581	0,216	3,278
3	Waste water	9	36	0	16	15,57	97	1,394	8,953	0,262	1,683
4	Drinking water	9	36	0	130	127,8	98	2,073	1,622	0,976	0,764
5	Surface water	9	36	0	70	70,04	100	0,870	1,242	0,798	1,139
6	Waste water	9	36	0	54	52,33	97	1,200	2,293	0,912	1,743

Symbols:

*l* is the number of laboratories (outlier-free)  
*n* is the number of outlier-free individual analytical values  
*o* is the relative portion of outliers  
 $x_{\text{exp}}$  is the accepted true value  
 $\bar{x}$  is the total mean, depending on outlier-free values  
 $\eta$  is the recovery rate  
 $s_R$  is the reproducibility standard deviation  
 $CV_R$  is the reproducibility coefficient of variation  
 $s_r$  is the repeatability standard deviation  
 $CV_r$  is the repeatability coefficient of variation

Applied samples:

1 and 4 Drinking water, original content of Cr(VI)<sup>a</sup>: 3,8 ± 1,3 µg/l; spiked with K<sub>2</sub>Cr<sub>2</sub>O<sub>7</sub>  
8 and 11 Surface water (Landwehrkanal, Berlin), original content of Cr(VI): 1,1 ± 1,2<sup>a</sup> < working range; spiked with K<sub>2</sub>Cr<sub>2</sub>O<sub>7</sub>  
9 and 12 Domestic waste water (city of Berlin), original content of Cr(VI): 0,7 ± 0,8<sup>a</sup> < working range; spiked with K<sub>2</sub>Cr<sub>2</sub>O<sub>7</sub>

Working ranges:

2 µg/l to 20 µg/l samples 1, 2 and 3  
20 µg/l to 200 µg/l samples 4, 5 and 6

<sup>a</sup> Measured by 7 CFA participants.

## Bibliography

- [1] RUZICKA, J. and HANSEN, E.H. *Flow Injection Analysis*, Wiley & Sons, 2nd edition, 1988
- [2] MÖLLER, J. *Flow Injection Analysis*, Analytiker Taschenbuch, Bd.7, Springer Verlag, 1988, pp. 199-275
- [3] DE ANDRADE, J.C., ROCHA, J.C. and BACCAN, N. On-line oxidation of Cr(III) to Cr(VI) for use with the flow injection analysis technique. *Analyst*, **109**, 1984, pp. 645-647
- [4] DE ANDRADE, J.C., ROCHA, J.C. and BACCAN, N. Sequential spectrophotometric determination of chromium(III) and chromium(VI) using flow injection analysis. *Analyst*, **110**, 1985, pp. 197-199
- [5] SPERLING, M., YIN, X. and WELZ, B. Differential determination of chromium(VI) and total chromium in natural waters using flow injection on-line separation and preconcentration electrothermal atomic absorption spectrometry. *Analyst*, **117**, 1992, pp. 629-635
- [6] PAVEL, J, KLIMENT, J., STOERK, S. and SUTER, O. Preservation of traces of chromium(VI) in water and waste water samples. *Fresenius Z. Anal. Chem.*, **321**, 1985, pp. 587-591



---

## BSI - British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

### Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

### Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001 Email: [orders@bsigroup.com](mailto:orders@bsigroup.com) You may also buy directly using a debit/credit card from the BSI Shop on the Website <http://www.bsigroup.com/shop>

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

### Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact Information Centre. Tel: +44 (0)20 8996 7111 Fax: +44 (0)20 8996 7048 Email: [info@bsigroup.com](mailto:info@bsigroup.com)

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002 Fax: +44 (0)20 8996 7001 Email: [membership@bsigroup.com](mailto:membership@bsigroup.com)

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsigroup.com/BSOL>

Further information about BSI is available on the BSI website at <http://www.bsigroup.com>

### Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright and Licensing Manager. Tel: +44 (0)20 8996 7070 Email: [copyright@bsigroup.com](mailto:copyright@bsigroup.com)