

Leather — Chemical tests — Determination of the free formaldehyde in process auxiliaries (ISO 27587:2009)

ICS 59.140.30

National foreword

This British Standard is the UK implementation of EN ISO 27587:2009.

The UK participation in its preparation was entrusted to Technical Committee TCI/69, Footwear, leather and coated fabrics.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 January 2010
 © BSI 2010

Amendments/corrigenda issued since publication

Date	Comments

ISBN 978 0 580 62288 5

EUROPEAN STANDARD

EN ISO 27587

NORME EUROPÉENNE

EUROPÄISCHE NORM

October 2009

ICS 59.140.30

English Version

Leather - Chemical tests - Determination of the free formaldehyde in process auxiliaries (ISO 27587:2009)

Cuir - Essais chimiques - Dosage du formaldéhyde libre dans les auxiliaires de traitement (ISO 27587:2009)

Leder - Chemische Prüfverfahren - Bestimmung des Gehalts an freiem Formaldehyd in Hilfsmitteln für die Lederherstellung (ISO 27587:2009)

This European Standard was approved by CEN on 26 September 2009.

CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration. Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the CEN Management Centre or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the CEN Management Centre has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Bulgaria, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and United Kingdom.



EUROPEAN COMMITTEE FOR STANDARDIZATION
COMITÉ EUROPÉEN DE NORMALISATION
EUROPÄISCHES KOMITEE FÜR NORMUNG

Management Centre: Avenue Marnix 17, B-1000 Brussels

Foreword

This document (EN ISO 27587:2009) has been prepared by Technical Committee CEN/TC 289 "Leather", the secretariat of which is held by UNI, in collaboration with the International Union of Leather Technologists and Chemists Societies (IULTCS).

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by April 2010, and conflicting national standards shall be withdrawn at the latest by April 2010.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. CEN [and/or CENELEC] shall not be held responsible for identifying any or all such patent rights.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Bulgaria, Cyprus, Czech Republic, Denmark, Estonia, Finland, France, Germany, Greece, Hungary, Iceland, Ireland, Italy, Latvia, Lithuania, Luxembourg, Malta, Netherlands, Norway, Poland, Portugal, Romania, Slovakia, Slovenia, Spain, Sweden, Switzerland and the United Kingdom.

Contents

Page

Foreword.....	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions.....	1
4 Principle.....	1
5 Reagents	1
6 Apparatus and materials.....	2
7 Methods	3
7.1 Outline of sample preparation system	3
7.2 Sample preparation	3
8 HPLC conditions (recommendations)	4
9 Calibration	4
10 Calculation.....	4
11 Checking reagents for absence of formaldehyde	5
12 Control of the procedure.....	5
13 Determination of formaldehyde in stock solutions.....	5
14 Test report	5
Annex A (informative) Reliability of the method	6

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 27587/IUC 26 was prepared by the European Committee for Standardization (CEN) Technical Committee CEN/TC 289, *Leather*, in collaboration with the Chemical Tests Commission of the International Union of Leather Technologists and Chemists Societies (IUC Commission, IULTCS), in accordance with the Agreement on technical cooperation between ISO and CEN (Vienna Agreement).

IULTCS, originally formed in 1897, is a world-wide organization of professional leather societies to further the advancement of leather science and technology. IULTCS has three Commissions, which are responsible for establishing international methods for the sampling and testing of leather. ISO recognizes IULTCS as an international standardizing body for the preparation of test methods for leather.

Leather — Chemical tests — Determination of the free formaldehyde in process auxiliaries

1 Scope

This International Standard specifies a method for the determination of free formaldehyde in process auxiliaries for leather. The analytical result obtained according to this procedure is expressed in milligrams per kilogram (mg/kg) sample. The upper limit of quantification of the method is given by the capacity of the cartridge (total carbonyls 6 400 µg/cartridge).

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1

free formaldehyde

formaldehyde that is released under dynamic conditions when the sample is heated in an inert dry atmosphere

4 Principle

The sample is heated in an inert atmosphere for a defined period of time. The released formaldehyde is captured and derivatized using a dinitrophenylhydrazine (DNPH) cartridge. The analyte is eluted with acetonitrile and analysed by high-performance liquid chromatography (HPLC) using a UV detector.

5 Reagents

Use only reagents of recognized analytical grade, unless otherwise stated.

5.1 Sulfuric acid, 3 mol/l.

5.2 Sodium hydroxide, 2 mol/l.

5.3 Sodium thiosulfate, 0,1 mol/l.

5.4 Iodine solution, 0,05 mol/l, i.e. 12,68 g iodine per litre of water.

5.5 Starch solution, 1 g/100 ml water.

5.6 Formaldehyde hydrazone solution.

5.7 Calibration standards. Prepare solutions by adequate dilution of the formaldehyde hydrazone solution (5.6).

5.8 Formaldehyde solution, approximately 37 % mass fraction.

5.9 Formaldehyde stock solution S1, prepare by pipetting 5 ml of formaldehyde solution (5.8) in a 1 000 ml volumetric flask and fill to the mark with distilled water.

5.10 Formaldehyde solution S2 in an adequate dilution for procedure control [e.g. 2,5 ml of the formaldehyde stock solution S1 (5.9) in a 100 ml volumetric flask, fill up with distilled water. The concentration of this solution should be adapted to ensure that the formaldehyde content is in the middle of the calibrated range.]

5.11 Distilled water, quality 2 according to ISO 3696.

5.12 2,4-Dinitrophenylhydrazine cartridges (DNPH cartridges), suitable for fixing a total of 6 400 µg of carbonyls per cartridge.

For lower quantities of free formaldehyde, a smaller capacity cartridge can be used. It is recommended that the cartridge have an excess capacity of at least 20 % more than the predicted formaldehyde amount.

5.13 Acetonitrile, HPLC grade.

5.14 Water, HPLC grade.

6 Apparatus and materials

Usual laboratory apparatus is required and, in particular, the following.

6.1 Thermostatic oil bath with stirring facilities, capable of maintaining a constant temperature of (90 ± 3) °C. The oil bath shall be deep enough to allow the U-tube to be dipped in up to the side tubing.

6.2 Silicone oil, suitable for oil bath (6.1).

6.3 Nitrogen, purity 4,6.

6.4 U-tube, calcium chloride tube, U-shaped, with two stopcocks, leg length 150 mm.

6.5 Flow meter.

6.6 Silicone tubing.

6.7 Syringe filters, 0,45 µm, regenerated cellulose.

6.8 Sea sand, purified by acid and calcined; quality grade GR for analysis.

6.9 Polytetrafluoroethylene (PTFE) stopcock grease, free of formaldehyde.

6.10 HPLC equipped with a UV detector.


6.11 HPLC column, of the RP-C18 type.

6.12 Hair dryer.

7 Methods

7.1 Outline of sample preparation system

See Figure 1.

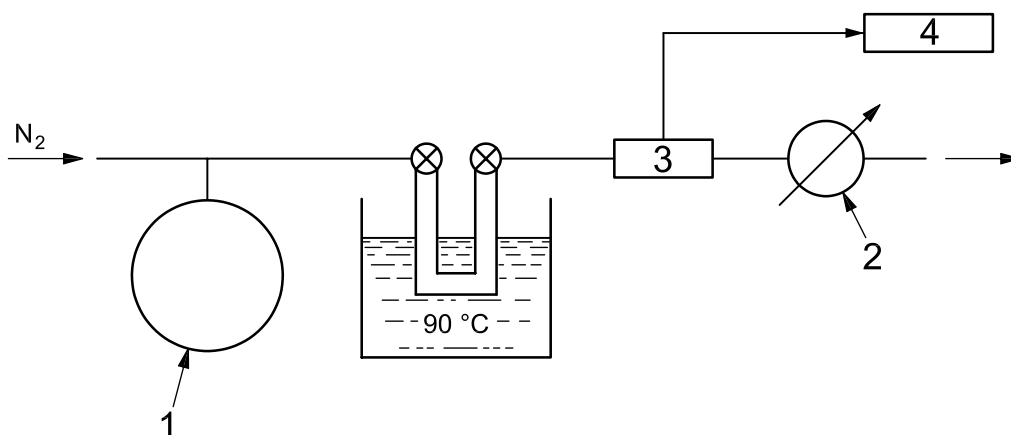

Key

- 1 gas tank
- 2 flow meter
- 3 DNPH cartridge
- 4 HPLC

Figure 1 — Schematic outline of sample preparation system

7.2 Sample preparation

Prepare a sample preparation system as described in 7.1. Initially, the U-tube (6.4) and the DNPH cartridge (5.12) are disconnected from the sampling system. All the parts of the sample preparation system shall be dry prior to use.

Purge the system for 15 min with nitrogen (6.3) at a flow rate of 500 ml/min. It is important that the analysis be carried out under an inert atmosphere. The purging step may be omitted before further analyses if work is done without interruption. The sampling system is slightly pressurized; therefore, all stopcocks should be secured with joint clamps.

Add 3 g to 4 g of sea sand (6.8) to the U-tube (6.4), ensuring that it is not blocked and that the nitrogen flow can be maintained. If this is not possible, use a larger diameter U-tube. Accurately weigh 0,5 g to 2 g of sample to the nearest 0,001 g into the U-tube. It may be necessary to reduce the amount of sample if it is in a liquid phase in order to diminish the likelihood of condensed water giving erroneous results.

Apply a thin layer of stopcock grease (6.9) to the joints of the U-tube. Introduce the U-tube into the system and purge for 5 min with nitrogen (6.3) at a flow rate of 500 ml/min. Reduce the flow rate to between 150 ml/min to 350 ml/min. Introduce the DNPH cartridge (5.12) into the system and place the U-tube into the oil bath (6.1) preheated to 90 °C. Cover the cartridge and U-tube carefully with aluminum foil. During sampling, it may be necessary to readjust the flow rate.

After 30 min, remove the U-tube containing the sample from the oil bath. Remove any condensate from the cartridge side of the tubing and stopcock using a hair dryer (6.12). This step shall be carried out irrespective of whether condensate can be observed visually.

Remove the DNPH cartridge from the system and elute with small portions of acetonitrile (5.13) in a 10 ml volumetric flask. Make up to volume with acetonitrile. Carefully mix the solution by shaking and filter an aliquot for analysis using a syringe filter (6.7). Analyse the resulting filtrate by HPLC (6.10).

It is recommended that the cartridges be removed from the refrigerator immediately prior to use. Experiments have shown that cartridges should be eluted within 3 days.

8 HPLC conditions (recommendations)

Separation column: CC 250/4 Nucleosil® 100-5 C18 HD¹⁾ with pre-column

Flow rate: 0,8 ml/min

Mobile phase: Solvent A, water

Solvent B, acetonitrile

Gradient: 55 % B linear to 95 % B in 20 min

Column oven: 30 °C

UV detection: 360 nm

Injection volume: 20 µl

9 Calibration

Calibration is carried out by means of an external standard in the range of 0,5 µg/10 ml to 50 µg/10 ml. The working range is limited by the capacity of the cartridge.

Prepare adequate dilutions (in acetonitrile) of the formaldehyde hydrazone solution (5.6). Calibration shall be done using at least six concentration levels. The calibration is effected through plotting a graph of the formaldehyde derivative peak area versus the concentration (µg/10 ml).

10 Calculation

Calculate the formaldehyde content (w) expressed in milligrams per kilogram (mg/kg) of sample being tested.

$$w = \frac{\rho \cdot F}{m}$$

where

ρ is the concentration of formaldehyde obtained from the calibration graph, expressed in µg/10 ml;

F is the dilution factor;

m is the mass of the sample, expressed in grams (g).

1) Nucleosil® 100-5 C18 HD is the trade name of a product supplied by Sorbent Technologies. This information is given for the convenience of users of this document and does not constitute an endorsement by ISO of the product named. Equivalent products may be used if they can be shown to lead to the same results.

11 Checking reagents for absence of formaldehyde

Blank analyses should be carried out on a regular basis and at least for each lot of reagents, mobile phase and cartridges or any other change in the system.

The formaldehyde content detected in the blank solution should be below 75 % of the lowest calibration level (0,5 µg/10 ml).

12 Control of the procedure

Spike the sea sand within the U-tube with 250 µl of formaldehyde solution S2 (5.10). Proceed as described in 7.2. Calculations are carried out as described in Clause 10. A minimum recovery rate of 90 % shall be calculated. In the event of lower levels being detected, possible sources of error shall be detected and eliminated prior to routine analysis of samples.

13 Determination of formaldehyde in stock solutions

Pipette 10 ml of formaldehyde stock solution S1 (5.9) into a 250 ml Erlenmeyer flask and mix with 50 ml of iodine solution (5.4) as well as with sodium hydroxide (5.2) until it turns to yellow. Allow it to settle for 15 min at 18 °C to 30 °C and then add 15 ml sulfuric acid (5.1) while swirling.

After adding 2 ml of starch solution (5.5), titrate the excess iodine with sodium thiosulfate (5.3) until the colour changes. Make three individual determinations. Titrate a blank solution in the same manner.

$$\rho_S = \frac{(V_0 - V_1) \cdot c_{Th} \cdot M_{FA}}{2}$$

where

ρ_S is the concentration of the formaldehyde stock solution S1, in mg/10 ml;

V_0 is the titre volume of the thiosulfate solution for the blank solution, in ml;

V_1 is the titre volume of the thiosulfate solution for the sample solution, in ml;

c_{Th} is the concentration of the thiosulfate solution, in mol/l;

M_{FA} is the relative molecular mass of formaldehyde, 30,02 g/mol.

14 Test report

The test report shall include the following:

- a reference to this International Standard (ISO 27587);
- the type, origin and designation of the analysed product and the sampling method used;
- the analytical result for free formaldehyde content in milligrams per kilogram (mg/kg), rounded to one decimal place;
- any deviation from the analytical procedure;
- the date of the test.

Annex A (informative)

Reliability of the method

The method was tested in an interlaboratory trial in 2007 with two different auxiliaries (A and B).

Table A.1 — Interlaboratory trial

Values in milligrams per kilogram (mg/km)

Auxiliary	Free formaldehyde				
	Mean value	s_r	s_R	r	R
A	3,13	0,31	0,87	0,87	2,43
B	8,58	0,62	1,68	1,74	4,69

Symbols:

s_r is the standard deviation of repeatability

s_R is the standard deviation of reproducibility

r is the repeatability

R is the reproducibility

r, R (probability 95 %; confidence factor 2,8)

BSI - British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001 Email: orders@bsigroup.com You may also buy directly using a debit/credit card from the BSI Shop on the Website <http://www.bsigroup.com/shop>

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact Information Centre. Tel: +44 (0)20 8996 7111 Fax: +44 (0)20 8996 7048 Email: info@bsigroup.com

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002 Fax: +44 (0)20 8996 7001 Email: membership@bsigroup.com

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsigroup.com/BSOL>

Further information about BSI is available on the BSI website at <http://www.bsigroup.com>.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright and Licensing Manager. Tel: +44 (0)20 8996 7070 Email: copyright@bsigroup.com