

**Plastics piping systems —
Glass reinforced thermosetting
plastics (GRP) components —
Test methods to prove the
design of cemented
socket-and-spigot joints**

The European Standard EN 1449 : 1996 has the status of a
British Standard

ICS 23.040.60

Committees responsible for this British Standard

The preparation of this British Standard was entrusted to Technical Committee PRI/61, Plastics piping systems and components, upon which the following bodies were represented:

British Gas plc
 British Plastics Federation
 British Plumbing Fittings Manufacturers' Association
 British Valve and Actuator Manufacturers' Association
 Chartered Institution of Water and Environmental Management
 Department of the Environment (British Board of Agrément)
 Department of the Environment (Building Research Establishment)
 Department of the Environment (Property and Buildings Directorate)
 Department of Transport
 Electricity Association
 Federation of Civil Engineering Contractors
 Health and Safety Executive
 Institute of Building Control
 Institute of Materials
 Institution of Civil Engineers
 Institution of Gas Engineers
 National Association of Plumbing, Heating and Mechanical Services Contractors
 Pipeline Industries Guild
 Plastics Land Drainage Manufacturers' Association
 Society of British Gas Industries
 Society of British Water Industries
 Water Companies Association
 Water Services Association of England and Wales

The following bodies were also represented in the drafting of the standard, through subcommittees and panels:

Association of Consulting Engineers
 Engineering Equipment and Materials Users' Association
 Institution of Mechanical Engineers
 RAPRA Technology Ltd.

This British Standard, having been prepared under the direction of the Sector Board for Materials and Chemicals, was published under the authority of the Standards Board and comes into effect on 15 May 1997

© BSI 1997

Amendments issued since publication

Amd. No.	Date	Text affected

The following BSI references relate to the work on this standard:
 Committee reference PRI/61
 Draft for comment 94/341024 DC

ISBN 0 580 27367 9

Contents

	Page
Committees responsible	Inside front cover
National foreword	ii
<hr/>	
Method	
Foreword	2
Introduction	2
1 Scope	3
2 Principle	3
3 Apparatus	3
4 Test pieces	3
5 Test temperature	3
6 Procedure	3
7 Test report	5
<hr/>	
Table	
1 Summary of test conditions for pressure testing	4
<hr/>	
Figure	
1 Typical test arrangement	4
<hr/>	

National foreword

This British Standard has been prepared by Technical Committee PRI/61 and is the English language version of EN 1449 : 1996 *Plastics piping systems — Glass-reinforced thermosetting plastics (GRP) components — Test methods to prove the design of cemented socket-and-spigot joints*, published by the European Committee for Standardization (CEN).

It is incorporated into BS 2782 *Methods of testing plastics : Part 12 : Reinforced plastics pipes, fittings and valves*, as Method 1224C : 1997, for association with related test methods for plastics materials and plastics piping components.

This standard has been prepared for reference by other standards under preparation by CEN for specification of reinforced plastics piping systems and components. It has been implemented to enable experience of the methods to be gained and for use for other fresh applications.

It is also for use for the revision or amendment of other national standards as practicable, but it should not be presumed to apply to any existing standard or specification which contains or makes reference to a different test method until that standard/specification has been amended or revised to make reference to this method and adjust any requirements as appropriate.

Warning note 1. Attention is drawn to the requirements of **6.3.3**, and table 1, which involve application of a test pressure corresponding to at least four times the nominal pressure of the component under test. It is essential to ensure that any components subjected to such pressures, such as the end caps and any associated securing bolts as indicated in figure 1, are selected and contained accordingly.

Warning note 2. This British Standard, which is identical with EN 1449 : 1996, does not necessarily detail all the precautions necessary to meet the requirements of the Health and Safety at Work etc. Act 1974. Attention should be paid to any appropriate safety precautions and the method should be operated only by trained personnel.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

Summary of pages

This document comprises a front cover, an inside front cover, pages i and ii, the EN title page, pages 2 to 6, an inside back cover, and a back cover.

ICS 23.040.60

Descriptors: Plastic tubes, pipe fittings, reinforced plastics, thermosetting resins, test, joining flexural strength, pressure resistance, hydrostatic pressure

English version

Plastics piping systems — Glass-reinforced thermosetting plastics (GRP) components — Test methods to prove the design of cemented socket-and-spigot joints

Systèmes de canalisations en plastique —
Composants en plastique thermodurcissable
renforcé de verre (PRV) — Méthodes d'essai pour
confirmer la conception d'assemblages mâle-femelle
collés

Kunststoff-Rohrleitungssysteme — Bauteile aus
glasfaserverstärkten duroplastischen Kunststoffen
(GFK) — Prüfverfahren zur Bauartprüfung von
geklebten Muffe- und Spitzende-Verbindungen

This European Standard was approved by CEN on 1996-07-13. CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

CEN

European Committee for Standardization
Comité Européen de Normalisation
Europäisches Komitee für Normung

Central Secretariat: rue de Stassart 36, B-1050 Brussels

Foreword

This European Standard has been prepared by Technical Committee CEN/TC 155, Plastics piping systems and ducting systems, the secretariat of which is held by NNI.

This standard is based on the Draft International Standard ISO/DIS 8533, *Pipes and fittings of glass-fibre reinforced thermosetting plastics (GRP) — Cemented socket and spigot, including double socket, joints — Initial performance requirements and test methods*, prepared by the International Organization for Standardization (ISO). It is a modification of ISO/DIS 8533 for reasons of possible applicability to other test conditions and alignment with texts of other standards on test methods.

The modifications are as follows:

- test parameters (pressure, time, temperature) are not specified;
- performance requirements are not given;
- editorial changes have been introduced.

The material-dependent parameters and/or performance requirements are incorporated in the referring standard.

This standard is one of a series of standards on test methods which support System Standards for plastics piping systems and ducting systems.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by May 1997, and conflicting national standards shall be withdrawn at the latest by May 1997.

According to the CEN/CENELEC Internal Regulations, the national standards organizations of the following countries are bound to implement this European Standard: Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and the United Kingdom.

Introduction

In a pipework system, pipes and fittings of different nominal pressures and stiffnesses may be used.

A joint may be made between pipes and/or fittings and should be designed such that its performance is equal to or better than the requirements of the pipeline, but not necessarily of the components being joined.

The requirements for the assembly of the joint are not included in this standard, but they should be in accordance with the manufacturer's recommendations.

1 Scope

This standard specifies methods of test for cemented socket-and-spigot joints for plastics piping systems of glass-reinforced thermosetting plastics (GRP) for pressure and non-pressure applications. This standard is only applicable to the joint and covers methods of test to prove its design.

The tests detailed in **6.1** to **6.3** inclusive are applicable to cemented socket-and-spigot joints intended to be used in buried or above ground applications.

This test procedure is applicable to joints for pipes and fittings of all nominal sizes.

All tests given in this standard are applicable for evaluating joints intended for applications conveying liquids at temperatures up to and including 50 °C and may be applicable to joints for use at higher temperatures (see clause **2**).

2 Principle

A joint is subjected to specified internal pressures. The procedure includes prolonged static tests at elevated pressures and also cyclic testing.

At the end of each test the joint is inspected for signs of leakage and damage.

NOTE. It is assumed that the following test parameters are set by the standard making reference to this standard:

- the number of test pieces to be used (see **4.1**);
- the length, L , of the assembled test piece (see **4.2**);
- the nominal pressure relevant to the joint under test (see **4.2**, **6.2** and **6.3**);
- if applicable, conditioning other than as given in **4.3**;
- the test temperature and its permissible deviations (see clause **5**);
- if applicable, any criteria indicative of damage to the joint components [see clause **6** and i) of clause **7**].

3 Apparatus

3.1 *End sealing devices*, of size and type appropriate to the joint system under test. The end-sealing devices shall be anchored to the pipes to transmit end thrust loads (see **6.2** and **6.3**).

3.2 *A source of hydrostatic pressure*, to meet the needs of the test (see **6.2** and **6.3**).

3.3 *A means to measure the gauge pressure*, at the top of the pipe and check conformity to the specified pressures (see **6.2** and **6.3**).

4 Test pieces

4.1 Number

The number of test pieces shall be as specified in the referring standard.

4.2 Arrangement

The test piece shall be an assembly of one or two pieces of pipe, as applicable, of the correct size and nominal pressure, as specified in the referring standard, in between which the joint to be tested is located.

The length, L , of the assembly shall be not less than that specified in the referring standard.

The joint shall be assembled in accordance with the manufacturer's recommendations and, if applicable, the requirements of the referring standard.

WARNING. Bolts which are normally supplied for use at a certain PN rating can reasonably be used in tests at $2 \times [\text{PN}]$, but it would be dangerous to use them at $4 \times [\text{PN}]$. Therefore when performing the test described in **6.3** it is recommended that the capacity of the bolts be checked and, if necessary, suitable higher capacity bolts should be used.

4.3 Conditioning

Unless otherwise specified in the referring standard, condition the test pieces at the test temperature (see clause **5**) for at least 24 h prior to testing.

5 Test temperature

Conduct the following procedure at the temperature specified in the referring standard.

6 Procedure

6.1 Sequence for testing

Subject each test piece (see **4.2**) to those of the following tests specified in the referring standard, in the sequence as given in table 1, **6.2** and **6.3**.

NOTE. Each reference to hydrostatic pressure specifies an internal gauge pressure (i.e. relative to atmospheric pressure) and the nominal pressure is that relevant to the joint under test.

If a test is interrupted, record the details in the test report and repeat the particular test before carrying on to the next in the series of tests, if applicable. Failure of the end caps shall not constitute failure of the joint. If the test conditions are invalidated thereby, repeat the particular test after replacing the failed component.

6.2 Resistance to internal pressure including hydrostatic end thrust

6.2.1 Using a conditioned test piece conforming to clause 4, assemble the test arrangement as shown in figure 1.

6.2.2 Connect the end caps to the pipes in such a way that the full loads induced by the internal pressure will be transmitted along the pipes to the joint under test.

6.2.3 Fill the test piece with water, taking care to avoid entrapping air.

6.2.4 Apply an initial hydrostatic pressure of 1,5 times the nominal pressure of the joint, expressed in bars¹⁾, and maintain within $\pm 2\%$ for 15 min.

Inspect the joint for signs of leakage or damage. If either has occurred stop the test, disassemble and continue in accordance with **6.1**, otherwise continue in accordance with **6.2.5**.

¹⁾ 1 bar = $10^5 \text{ N/m}^2 = 0,1 \text{ MPa}$.

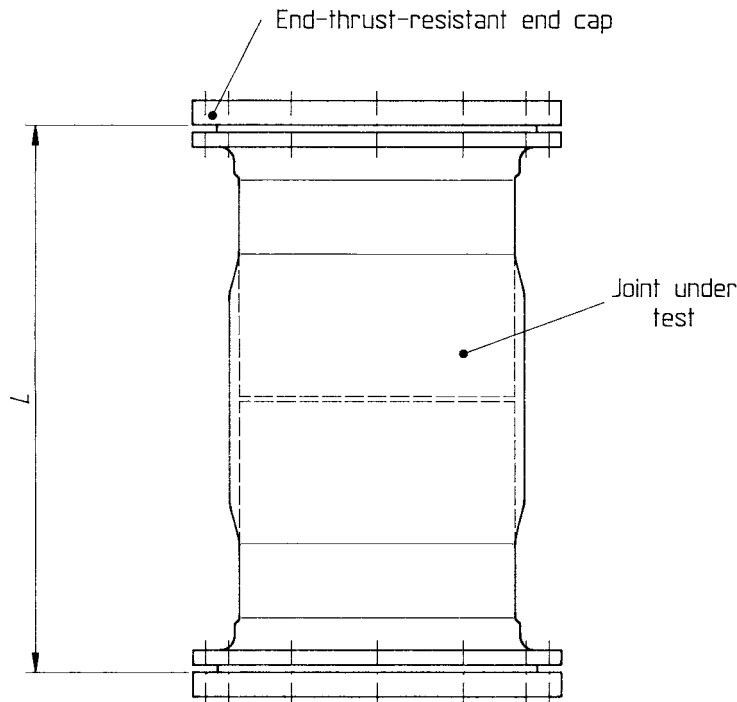


Figure 1. Typical test arrangement

Table 1. Summary of test conditions for pressure testing

Test	Test and sequence	Minimum test pressure	Minimum duration
Initial leakage	Initial pressure	$1,5 \times [\text{PN}]$	15 min
Resistance to internal pressure with hydrostatic end thrust	Preliminary hydrostatic pressure	$1,5 \times [\text{PN}]$	15 min
	Maintained hydrostatic pressure	$2 \times [\text{PN}]$	24 h
	Positive cyclic pressure	Atmospheric to $1,5 \times [\text{PN}]$ to atmospheric	10 cycles of 1,5 min to 3 min each
Short duration pressure resistance with hydrostatic end thrust	Preliminary hydrostatic pressure	$1,5 \times [\text{PN}]$	15 min
	Maintained hydrostatic pressure	$4 \times [\text{PN}]$	6 min

6.2.5 Maintain within $\pm 2\%$ for a further 15 min the hydrostatic pressure of 1,5 times the nominal pressure of the joint, expressed in bars.

6.2.6 Raise the hydrostatic pressure to twice the nominal pressure of the joint, expressed in bars, and maintain within $\pm 2\%$ for not less than 24 h.

6.2.7 Inspect the joint and record any signs of leakage or damage. If either has occurred stop the test, disassemble and continue in accordance with **6.1**, otherwise continue in accordance with **6.2.8**.

6.2.8 Reduce the pressure to atmospheric.

6.2.9 Steadily raise the internal pressure to 1,5 times the nominal pressure of the joint, expressed in bars, and reduce again to atmospheric pressure so as to complete the cycle in between 1,5 min and 3 min inclusive.

6.2.10 Repeat the cycle given in **6.2.9** a further nine times.

6.2.11 Inspect the joint and record any signs of leakage or damage.

6.3 Short duration resistance to internal pressure including end thrust

6.3.1 Fill the test piece with water, taking care to avoid entrapping air.

6.3.2 Apply an initial hydrostatic pressure of 1,5 times the nominal pressure of the joint, expressed in bars, and maintain within $\pm 2\%$ for 15 min.

Inspect the joint for signs of leakage or damage. If either has occurred stop the test, disassemble and continue in accordance with **6.1**, otherwise continue in accordance with **6.3.3**.

6.3.3 Raise the hydrostatic pressure so that a pressure equal to four times the nominal pressure of the joint, expressed in bars, is reached in not less than 1 min and not more than 5 min (see warning note to **4.2**). Maintain this pressure within $\pm 2\%$ for 6 min without causing the joint to rupture (leakage of the joint shall not constitute failure).

6.3.4 Reduce the pressure to atmospheric, empty the test piece and disassemble.

6.3.5 Inspect the joint and record any signs of rupture.

7 Test report

The test report shall include the following information:

- a) a reference to this standard and to the referring standard;
- b) the full identification of the pipes and joint tested;
- c) the nominal pressure, PN, of the pipe(s) and joint;
- d) the description of the adhesive and bonding procedures used;
- e) the temperature range during the tests;
- f) a description of the tests to which the joint was subjected;
- g) the pressures applied, in bars;
- h) any observations on the leaktightness of the joint during each test;
- i) any observations on the condition of the joint components at the end of the testing cycle given in table 1;
- j) the details of interruptions, if any, to the test sequence;
- k) any factors which may have influenced the results, such as incidents or operating details not specified in this standard;
- l) the dates of the period of test.

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre. Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: 020 8996 7002. Fax: 020 8996 7001.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager. Tel: 020 8996 7070.