

Water quality — Determination of total arsenic — Silver diethyldithiocarbamate spectrophotometric method

The European Standard EN 26595:1992 has the status of a
British Standard

UDC 628.1/.3:620.1:543.42:546.19

Confirmed
July 2008

This British Standard, having been prepared under the direction of the Environment and Pollution Standards Committee, was published under the authority of the Board of BSI and comes into effect on 29 April 1983

© BSI 10-1999

The following BSI references relate to the work on this standard:
Committee reference EPC/44
Draft for comment 80/55453 DC

ISBN 0 580 13235 8

Amendments issued since publication

Amd. No.	Date of issue	Comments
7427	May 1993	Indicated by a sideline in the margin

Contents

	Page
National foreword	ii
Foreword	2
Text of EN 26595	3
Publications referred to	Inside back cover

National foreword

This Section of this British Standard, which has been prepared under the direction of the Environment and Pollution Standards Committee, is identical with ISO 6595:1982 “*Water quality — Determination of total arsenic — Silver diethyldithiocarbamate spectrophotometric method*”. The International Standard was prepared by subcommittee 2, Physical, chemical and biochemical methods, of Technical Committee 147, Water quality, of the International Organization for Standardization (ISO) as a result of discussion in which the UK participated.

In 1992 the European Committee for Standardization (CEN) accepted ISO 6595:1982 as European Standard EN 26595:1992. As a consequence of implementing the European Standard this British Standard is renumbered as BS EN 26595 and any reference to BS 6068-2.1 should be read as a reference to BS EN 26595.

This British Standard is being published in a series of Parts subdivided into Sections that will generally correspond to particular International Standards. Sections are being, or will be, published in the following Parts.

- *Part 0: Introduction;*
- *Part 1: Glossary;*
- *Part 2: Physical, chemical and biochemical methods;*
- *Part 3: Radiological methods;*
- *Part 4: Microbiological methods;*
- *Part 5: Biological methods;*
- *Part 6: Sampling.*

Terminology and conventions. The text of the International Standard has been approved as suitable for publication as a British Standard without deviation. Some terminology and certain conventions are not identical with those used in British Standards; attention is drawn especially to the following.

The comma has been used as a decimal marker. It is current practice in British Standards to use a full point on the baseline as the decimal marker.

Wherever the words “International Standard” appear, referring to this standard, they should be read as “British Standard”.

Cross-reference. There is no British Standard identical with ISO 383 to which reference is made in 5.2. A related standard to ISO 383 is BS 572:1960 “*Interchangeable conical ground glass joints*”. Conical ground glass joints complying with the requirements of BS 572 are interchangeable with those complying with the requirements of ISO 383 but different designations are given.

Additional information. The method in this Section is similar technically to the general method for the determination of arsenic given in BS 4404 and in ISO 2590.

A British Standard does not purport to include all the necessary provisions of a contract. Users of British Standards are responsible for their correct application.

Compliance with a British Standard does not of itself confer immunity from legal obligations.

Summary of pages

This document comprises a front cover, an inside front cover, pages i and ii, the EN title page, pages 2 to 8, an inside back cover and a back cover.

This standard has been updated (see copyright date) and may have had amendments incorporated. This will be indicated in the amendment table on the inside front cover.

EUROPEAN STANDARD

EN 26595:1992

NORME EUROPÉENNE

EUROPÄISCHE NORM

October 1992

UDC 628.1/.3:620.1:543.42:546.19

Descriptors: Water, quality, chemical analysis, determination of content, arsenic, spectrophotometric analysis, silver diethyldithiocarbamate

English version

Water quality — Determination of total arsenic — Silver diethyldithiocarbamate spectrophotometric method

(ISO 6595:1982)

Qualité de l'eau — Dosage de l'arsenic total —
Méthode spectrophotométrique au
diéthyldithiocarbamate d'argent
(ISO 6595:1982)

Wasserbeschaffenheit — Bestimmung von
Arsen — Photometrisches Verfahren mit
Silberdiethyldithiocarbamat
(ISO 6595:1982)

This European Standard was approved by CEN on 1992-10-05. CEN members are bound to comply with the CEN/CENELEC Internal Regulations which stipulate the conditions for giving this European Standard the status of a national standard without any alteration.

Up-to-date lists and bibliographical references concerning such national standards may be obtained on application to the Central Secretariat or to any CEN member.

This European Standard exists in three official versions (English, French, German). A version in any other language made by translation under the responsibility of a CEN member into its own language and notified to the Central Secretariat has the same status as the official versions.

CEN members are the national standards bodies of Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland and United Kingdom.

CEN

European Committee for Standardization
Comité Européen de Normalisation
Europäisches Komitee für Normung

Central Secretariat: rue de Stassart 36, B-1050 Brussels

Foreword

This European Standard is the endorsement of ISO 6595. Endorsement of ISO 6595 was recommended by CEN/Technical Committee 230 “*Water analysis*” under whose competence this European Standard will henceforth fall.

This European Standard shall be given the status of a national standard, either by publication of an identical text or by endorsement, at the latest by April 1993, and conflicting national standards shall be withdrawn at the latest by April 1993.

The Standard was approved and in accordance with the CEN/CENELEC Internal Regulations, the following countries are bound to implement this European Standard: Austria, Belgium, Denmark, Finland, France, Germany, Greece, Iceland, Ireland, Italy, Luxembourg, Netherlands, Norway, Portugal, Spain, Sweden, Switzerland, United Kingdom.

Contents

	Page
Foreword	2
1 Scope and field of application	3
2 Definition	3
3 Principle	3
4 Reagents	3
5 Apparatus	4
6 Procedure	4
7 Expression of results	5
8 Test report	5
Annex Special case and interferences	7
Figure — Example of reaction apparatus	6

The procedure specified in this International Standard is intended to be carried out by qualified chemists or by other suitably trained and/or supervised personnel. Attention is especially drawn to the toxic nature of arsenic and its solutions and of other reagents used in this method of analysis and to the need to take particular care in the handling and disposal of solutions. Pyridine and chloroform should be handled in a well-ventilated fume cupboard. Ephedrine is a scheduled drug and should be handled in accordance with appropriate regulations.

1 Scope and field of application

This International Standard specifies a silver diethyldithiocarbamate spectrophotometric method for the determination of arsenic in water and waste water.

It is applicable for the determination of arsenic concentrations in the range from 0,001 to 0,1 mg/l. In the case of arsenic compounds which are difficult to decompose, a method of digestion is described in the annex, clause A.1. By appropriate dilution of the test portion with arsenic-free water, higher concentrations of arsenic may also be determined.

Antimony interferes with the determination (see the annex, clause A.2). Chromium, cobalt, molybdenum, nickel, mercury, silver and platinum, in concentrations up to 5 mg/l, do not interfere with the determination.

2 Definition

For the purpose of this International Standard, the following definition applies.

total arsenic

the total amount of the element arsenic, in elementary form or bound in inorganic or organic compounds

NOTE Depending on the redox potential and the pH of the water, arsenic may be present in the trivalent state [for example as arsenite ions (AsO_3^{3-})], in the pentavalent state [for example as arsenate ions (AsO_4^{3-})], or as organically bound arsenic.

3 Principle

3.1 Oxidation of organic compounds or sulphides by heating with potassium permanganate and potassium peroxodisulphate.

3.2 Reduction of pentavalent arsenic to the trivalent state.

3.3 Reduction of the trivalent arsenic by nascent hydrogen in an acidic medium to arsenic trihydride (arsine).

3.4 Absorption of the arsine in a solution of silver diethyldithiocarbamate in either chloroform or pyridine, and spectrophotometric measurement of the red-violet complex thus formed, at a wavelength of 510 or 525 nm, respectively, according to the solvent.

4 Reagents

Unless otherwise specified, all reagents shall be of recognized analytical grade and the water used should be distilled or deionized water. The arsenic content of the reagents and the water should be negligibly small.

4.1 Sulphuric acid, $\rho = 1,84$ g/ml.

4.2 Sulphuric acid solution, $c(1/2 \text{H}_2\text{SO}_4) = 2$ mol/l.

4.3 Sodium hydroxide solution, $c(\text{NaOH}) = 2$ mol/l.

Store in a polyethylene bottle.

4.4 Potassium permanganate, 50 g/l solution.

Dissolve 50 g of potassium permanganate in water and dilute to 1 000 ml.

Take care to ensure complete dissolution of the reagent.

Store in a dark glass bottle.

4.5 Potassium peroxodisulphate, 40 g/l solution.

Dissolve 40 g of potassium peroxodisulphate in water and dilute to 1 000 ml.

4.6 Hydroxylamine hydrochloride, 100 g/l solution.

Dissolve 10 g of hydroxylamine hydrochloride in water and dilute to 100 ml.

The solution is stable for at least 1 month.

4.7 Potassium iodide, 150 g/l solution.

Dissolve 15 g of potassium iodide in water and dilute to 100 ml.

Store in a dark glass bottle.

The solution is stable for at least 1 month.

4.8 Tin chloride solution

Dissolve 55 g of tin(II) chloride dihydrate in 25 ml of concentrated hydrochloric acid ($\rho = 1,19$ g/ml) and dilute to 100 ml with water.

The solution is stable if stored in a refrigerator.

4.9 Absorption solution A

Dissolve 0,500 g of silver diethyldithiocarbamate and 0,330 g of 1-ephedrine in chloroform and dilute with chloroform to 200 ml.

This solution is stable for at least 1 month if stored in a tightly-stoppered, dark glass bottle.

4.10 Absorption solution B

Dissolve 1,000 g of silver diethyldithiocarbamate in pyridine and dilute with pyridine to 200 ml.

Store in a dark glass bottle.

4.11 Zinc, coarse powder, of particle size 0,5 to 1 mm.

4.12 Copper(II) sulphate solution

Dissolve 15 g of copper(II) sulphate pentahydrate in water and dilute to 100 ml.

4.13 Arsenic, standard solution corresponding to 350 mg of As per litre.

Dissolve exactly 0,462 0 g of arsenic(III) oxide (As_2O_3), previously dried over silica gel to constant mass, in 12 ml of the sodium hydroxide solution (4.3). Neutralize with the sulphuric acid solution (4.2) and dilute to 1 000 ml with water.

1 ml of this standard solution contains 0,35 mg of arsenic.

4.14 Arsenic, standard solution corresponding to 3,5 mg of As per litre.

Dilute 10 ml of the standard arsenic solution (4.13) with water to 1 000 ml.

1 ml of this standard solution contains 3,5 μg of arsenic.

The solution is stable only for a few days.

Prepare the solution just before use.

4.15 Arsenic, standard solution corresponding to 0,35 mg of As per litre.

Dilute 1 ml of the standard arsenic solution (4.13) with water to 1 000 ml.

1 ml of this standard solution contains 0,35 μg of arsenic.

Prepare the solution just before use.

5 Apparatus

Usual laboratory equipment and

5.1 Spectrophotometer, equipped with cells of optical path length 10 to 50 mm [for optical path lengths of more than 10 mm, use micro-cells of small total capacity (maximum 5 ml)].

5.2 Reaction apparatus (as shown in the figure or its equivalent), comprising

- a conical flask, of capacity 500 ml, with a ground glass joint complying with the requirements of ISO 383;

- an absorption tube, with a ground glass joint complying with the requirements of ISO 383.

5.3 Volumetric flask, of capacity 1 000 ml.

5.4 Pipettes, of capacities 1 – 2 – 5 – 10 and 20 ml.

5.5 Measuring cylinders, of capacities 25, 100 and 500 ml.

6 Procedure

6.1 Test portion

Transfer 350 ml of the test sample to a measuring cylinder. If the arsenic content is expected to exceed 0,1 mg/l, take an appropriately smaller test portion and dilute with water to 350 ml.

6.2 Blank test

Carry out a blank test, using the same reagents in the same quantities as used in the determination and following the same procedures, including any pretreatment, but replacing the test portion by 350 ml of arsenic-free water.

6.3 Choice of absorption solution

The choice of absorption solution [A (4.9) or B (4.10)] is left to the discretion of the analyst. Pyridine has an unpleasant odour. It is, however, less volatile than chloroform, and the volume of absorption solution B is less likely to require adjustment during the analysis. The molar absorbance coefficient when using absorption solution B is about 30 % greater than that when using absorption solution A. The same absorption solution shall, therefore, be used in the determination, blank test and for preparation of the calibration graphs.

6.4 Preparation of calibration graphs

6.4.1 Preparation of standard matching solutions

6.4.1.1 Into each of two series of conical flasks (see 5.2), pipette the volumes of the standard arsenic solutions (4.14 and 4.15) shown in the following table, and make up the volume in each flask to 350 ml with water.

Volume of standard arsenic solution (4.14)	Corresponding arsenic content
ml	$\mu\text{g/l}$
0 ^a	0
1,0	10
2,0	20
5,0	50
10,0	100
Volume of standard arsenic solution (4.15)	
ml	
0 ^a	0
1,0	1
2,0	2
5,0	5
10,0	10
20,0	20

^a Blank test of the reagents for calibration.

6.4.1.2 Add to each flask 20 ml of the sulphuric acid (4.1).

6.4.1.3 Add 10 ml of the potassium iodide solution (4.7) and 1 ml of the tin(II) chloride solution (4.8).

6.4.1.4 Transfer 5 ml of absorption solution A (4.9) or of absorption solution B (4.10), as appropriate (see 6.3), to the absorption tube.

Add 1 ml of the copper(II) sulphate solution (4.12) and 15 g of the zinc (4.11) to each flask.

Immediately connect the absorption tube to the flask. To ensure that the reaction apparatus is airtight, a small amount of arsenic-free grease may be applied to the ground glass joint.

Allow to stand for 2 h to complete the evolution of arsine. Make up the volume of absorption solution to 5 ml to replace loss by evaporation by adding chloroform (in the case of absorption solution A) or pyridine (in the case of absorption solution B), as appropriate.

Shake the flasks gently from time to time so as to avoid the formation of precipitates in the entry zone of the absorption solution.

If protected from light, the coloured complex is stable for about 2 h; after complete evolution of arsine, carry out the spectrophotometric measurements within this time.

6.4.2 Spectrophotometric measurements

For each of the standard matching solutions (6.4.1.1) in turn, fill a cell with solution from the absorption tube and fill a reference cell with the appropriate absorption solution solvent (chloroform or pyridine, respectively).

Measure the absorbance of the test solution by means of the spectrophotometer (5.1), set at a wavelength of 510 nm when using absorption solution A (4.9) or set at 540 nm when using absorption solution B (4.10).

6.4.3 Plotting the graphs

Correct the measured absorbances of the solutions from the absorption tubes (see 6.4.2) corresponding to each of the standard matching solutions (6.4.1.1) by deducting the absorbance for the reagent blank.

For each series of standard matching solutions corresponding to the two standard arsenic solutions (4.14 and 4.15), plot a graph of the corrected absorbances as ordinates against the corresponding arsenic contents, in micrograms per litre, as abscissae.

Both plots should be linear.

Prepare new calibration graphs frequently and at least each time new reagent is used.

6.5 Determination

6.5.1 Pretreatment

Transfer the test portion to a conical flask (see 5.2) and add 20 ml of the sulphuric acid (4.1), 5 ml of the potassium permanganate solution (4.4) and 50 ml of the potassium peroxodisulphate solution (4.5). Heat for 2 h at 90 °C (for example on a hot-plate or a water bath). Allow to cool to room temperature and add 20 ml of the hydroxylamine hydrochloride solution (4.6).

NOTE The amount of oxidizing agent is sufficient for chemical oxygen demands up to 100 mg/l.

6.5.2 Development of colour

Proceed as described in 6.4.1.3 and 6.4.1.4.

6.5.3 Spectrophotometric measurement

Proceed as described in 6.4.2.

7 Expression of results

From the calibration graphs, determine the arsenic concentrations corresponding to the absorbances of the test solution and of the blank test solution. Take any dilution of the test portion (see 6.1) into consideration.

The arsenic content, expressed in milligrams per litre, is given by the formula

$$\frac{(A_2 - A_1) \times f}{l}$$

where

- A_1 is the absorbance of the blank test solution;
- A_2 is the absorbance of the test solution;
- f is a calibration factor, in millimetre milligrams per litre;
- l is the optical path length, in millimetres, of the cell.

Report the arsenic content, in milligrams per litre, rounding values below 0,1 mg/l to the nearest 0,001 mg/l and values above 0,1 mg/l to the nearest 0,01 mg/l. (For example, arsenic content 0,42 mg/l.) Alternatively, report the arsenic content in millimoles per litre (for arsenic, 1 mmol = 74,9 mg).

8 Test report

The test report shall include the following information:

- a) a reference to this International Standard;
- b) identification of the sample;
- c) the results and the method of expression used;

- d) any unusual features noted during the determination;
- e) any operating details not specified in this International Standard or regarded as optional.

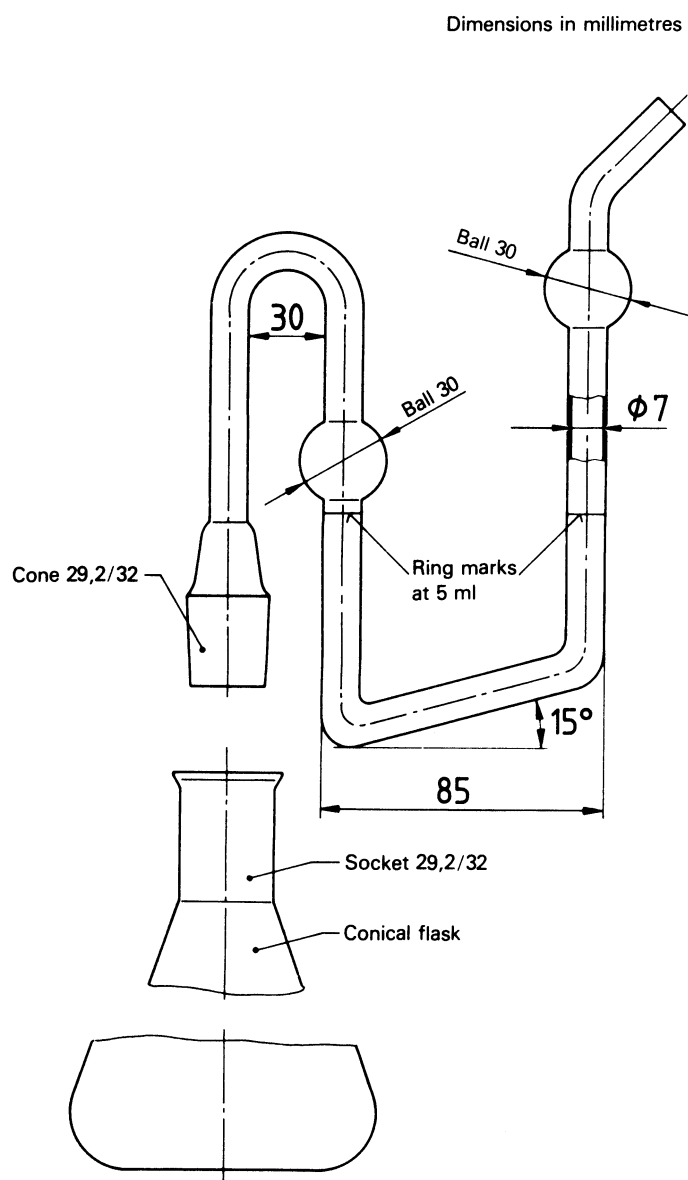


Figure — Example of reaction apparatus

Annex Special case and interferences

A.1 Arsenic compounds which are difficult to decompose

For the determination of total arsenic in water containing silicon fluoride (for example effluents from glass etchings), or in water containing organic arsenic compounds which are difficult to decompose, it is necessary to use a method of digestion by addition of sulphuric acid and hydrogen peroxide. In such cases, heat the sample with sulphuric acid with multiple additions of hydrogen peroxide. Continue the procedure until fumes of sulphur trioxide appear, then dilute the sample with water and continue as specified in **6.4.2**.

A.2 Antimony

Antimony salts are reduced under the test conditions to produce stibine (SbH_3), which reacts with the absorption solution to produce a red complex. If cells of optical path length 10 mm are used, an antimony concentration of 0,5 mg/l would contribute 0,015 % to the absorbance. Interference from antimony is thus only likely to be important when analysing certain waste waters or receiving streams. If it is present in large concentrations, this method should not be used.

Publications referred to

See national foreword.

**BS EN 26595:
1993
BS 6068-2.1:
1993
ISO 6695:1982**

BSI — British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover.
Tel: 020 8996 9000. Fax: 020 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: 020 8996 9001. Fax: 020 8996 7001.

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact the Information Centre.
Tel: 020 8996 7111. Fax: 020 8996 7048.

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration.
Tel: 020 8996 7002. Fax: 020 8996 7001.

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

If permission is granted, the terms may include royalty payments or a licensing agreement. Details and advice can be obtained from the Copyright Manager.
Tel: 020 8996 7070.

BSI
389 Chiswick High Road
London
W4 4AL