

BS ISO 5071-1:2013



BSI Standards Publication

# **Brown coals and lignites — Determination of the volatile matter in the analysis sample**

Part 1: Two-furnace method

**bsi.**

...making excellence a habit.™

**National foreword**

This British Standard is the UK implementation of ISO 5071-1:2013.

The UK participation in its preparation was entrusted to Technical Committee PTI/16, Solid mineral fuels.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2013. Published by BSI Standards Limited 2013

ISBN 978 0 580 81217 0

ICS 73.040

**Compliance with a British Standard cannot confer immunity from legal obligations.**

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 May 2013.

**Amendments issued since publication**

Date	Text affected
------	---------------

---

---

---

**Brown coals and lignites —  
Determination of the volatile matter  
in the analysis sample —**

**Part 1:  
Two-furnace method**

*Charbons bruns et lignites — Détermination des matières volatiles  
dans l'échantillon pour analyse —*

*Partie 1: Méthode avec utilisation de deux fours*





**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2013

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
<b>Foreword</b> .....	<b>iv</b>
<b>Introduction</b> .....	<b>v</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Principle</b> .....	<b>1</b>
<b>5 Reagents</b> .....	<b>1</b>
<b>6 Apparatus</b> .....	<b>2</b>
<b>7 Sample</b> .....	<b>6</b>
<b>8 Procedure</b> .....	<b>6</b>
8.1 Preliminary procedure.....	6
8.2 Predetermination procedure.....	6
8.3 Method using oven-dried coal.....	6
8.4 Method using air-dried coal.....	6
<b>9 Calculation of results</b> .....	<b>6</b>
9.1 For oven-dried coal.....	7
9.2 For air-dried coal.....	7
<b>10 Precision of the method</b> .....	<b>7</b>
10.1 Repeatability limit.....	7
10.2 Reproducibility limit.....	7
<b>11 Test report</b> .....	<b>8</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 5071-1 was prepared by Technical Committee ISO/TC 27, *Solid mineral fuels*, Subcommittee SC 5, *Methods of analysis*.

This second edition cancels and replaces the first edition (ISO 5071-1:1997), of which this constitutes a minor revision.

ISO 5071 consists of the following parts, under the general title *Brown coals and lignites — Determination of volatile matter in the analysis sample*:

*Part 1: Two-furnace method*

## Introduction

The volatile matter is determined as the loss in mass, corrected for moisture, when an analysis sample of brown coal or lignite is heated out of contact with air under specified conditions. The test is empirical and, in order to obtain reproducible results, it is essential that the rate of heating, the final temperature and the overall duration of the test be carefully controlled. Due to the nature of brown coals and lignites, initial heating of the sample at 400 °C is necessary to minimize the possibility of ejection of sample from the test crucible.

Mineral matter associated with the sample may also lose mass under the conditions of the test, the magnitude of the loss being dependent on both the nature and the quantity of the minerals present.





# Brown coals and lignites — Determination of the volatile matter in the analysis sample —

## Part 1: Two-furnace method

### 1 Scope

This part of ISO 5071 specifies a method of determining the volatile matter of brown coals and lignites.

### 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 1170, *Coal and coke — Calculation of analyses to different bases*

ISO 1213-2, *Solid mineral fuels — Vocabulary — Part 2: Terms relating to sampling, testing and analysis*

ISO 5068-2, *Brown coals and lignites — Determination of moisture content — Part 2: Indirect gravimetric method for moisture in the analysis sample*

ISO 5069-2, *Brown coals and lignites — Principles of sampling — Part 2: Sample preparation for determination of moisture content and for general analysis*

### 3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 1213-2 apply.

### 4 Principle

The coal is heated out of contact with air for 7 min at 400 °C, then immediately transferred to another furnace and heated at 900 °C for a further 7 min. The percentage of volatile matter is calculated from the loss in mass of the oven-dried sample or from the loss in mass of the analysis sample corrected for moisture.

### 5 Reagents

**5.1 Desiccants**, fresh or freshly regenerated and preferably self-indicating. Suitable desiccants are magnesium perchlorate, silica gel, activated alumina and anhydrous calcium sulfate.

**WARNING — Magnesium perchlorate is a strong oxidizing agent. Do not attempt to regenerate the absorbent. Do not permit contact with organic materials or reducing agent.**

**5.2 Nitrogen**, dry, with a maximum oxygen content of 30 µl per litre.

## 6 Apparatus

**6.1 Furnace** ([Figure 1](#)), heated by electricity. Two such furnaces are required. One furnace shall have a zone of 160 mm × 100 mm maintained at a uniform temperature of 400 °C ± 10 °C. The second shall have a zone of 160 mm × 100 mm maintained at a uniform temperature of 900 °C ± 5 °C. The furnaces may be the stop-ended type or fitted at the back with a flue approximately 25 mm in diameter by 150 mm long.

The heat capacity of the 900 °C and/or 400 °C furnace shall be such that, with an initial temperature of 900 °C and/or 400 °C, a temperature of 900 °C ± 10 °C and/or 400 °C ± 10 °C is regained within 4 min after insertion of a cold stand and its crucibles. The temperature shall be measured with a thermocouple as described in 6.3. The furnace can be designed specifically either for multiple determinations using a number of crucibles in one stand or for receiving one crucible and its stand. A position for the crucible stand shall be chosen within the zone of uniform temperature and this position used for all determinations.

**6.2 Oven**, capable of being controlled at a temperature within the range 105 °C to 110 °C and with provision for passing a current of dry, oxygen-free nitrogen through it at a rate sufficient to change the atmosphere 15 times per hour. The size of the chamber is suitable for containing the crucible (6.4).

**6.3 Thermocouple**, unsheathed, of wire not thicker than 1 mm, used to check the temperature characteristics of the furnace. The thermo-junction shall be inserted midway between the base of the crucible in its stand and the floor of the furnace. If the stand holds more than one crucible, the temperature under each crucible shall be checked in the same manner. If desired, a sheathed thermocouple may be permanently installed in the furnace with its thermo-junction as close as possible to the centre of the zone of uniform temperature; in this case, its temperature readings shall be correlated at frequent intervals with those of the unsheathed thermocouple, which is then inserted only when necessary.

NOTE The temperature/electromotive force relationship of a thermo-junction maintained at elevated temperatures gradually changes with time.

**6.4 Crucible and lid**, a cylindrical crucible with a well fitting lid, both made of fused silica. The crucible and lid shall weigh between 10 g and 14 g and have dimensions approximating those shown in [Figure 2](#). The fit of the lid on the crucible is critical to the determination and a lid shall be selected to match the crucible so that the horizontal clearance between them is not greater than 0,5 mm. After selection, the crucible and the lid shall be ground together to give smooth surfaces and then be given a common distinguishing mark. Crucibles of other refractory materials, or of platinum, can be used, provided that they give results which agree with the recommended silica crucible, within the stated precision of the method (Clause 10).

**6.5 Stand**, on which the crucible is placed in the muffle furnace, so that the appropriate specified rate of heating can be achieved. For example, it may consist of the following:


a) for a single determination, a ring of heat-resistant steel wire as shown in [Figure 3 a](#)), 27 mm in diameter and 1,5 mm thick, resting on the inner projection of its legs,

or

b) for multiple determinations, a tray of heat-resistant steel wire as shown in [Figure 3 b](#)), of appropriate size, with ceramic plates 2 mm thick supporting the crucibles.

**6.6 Balance**, sensitive to 0,1 mg.

**6.7 Desiccator**.

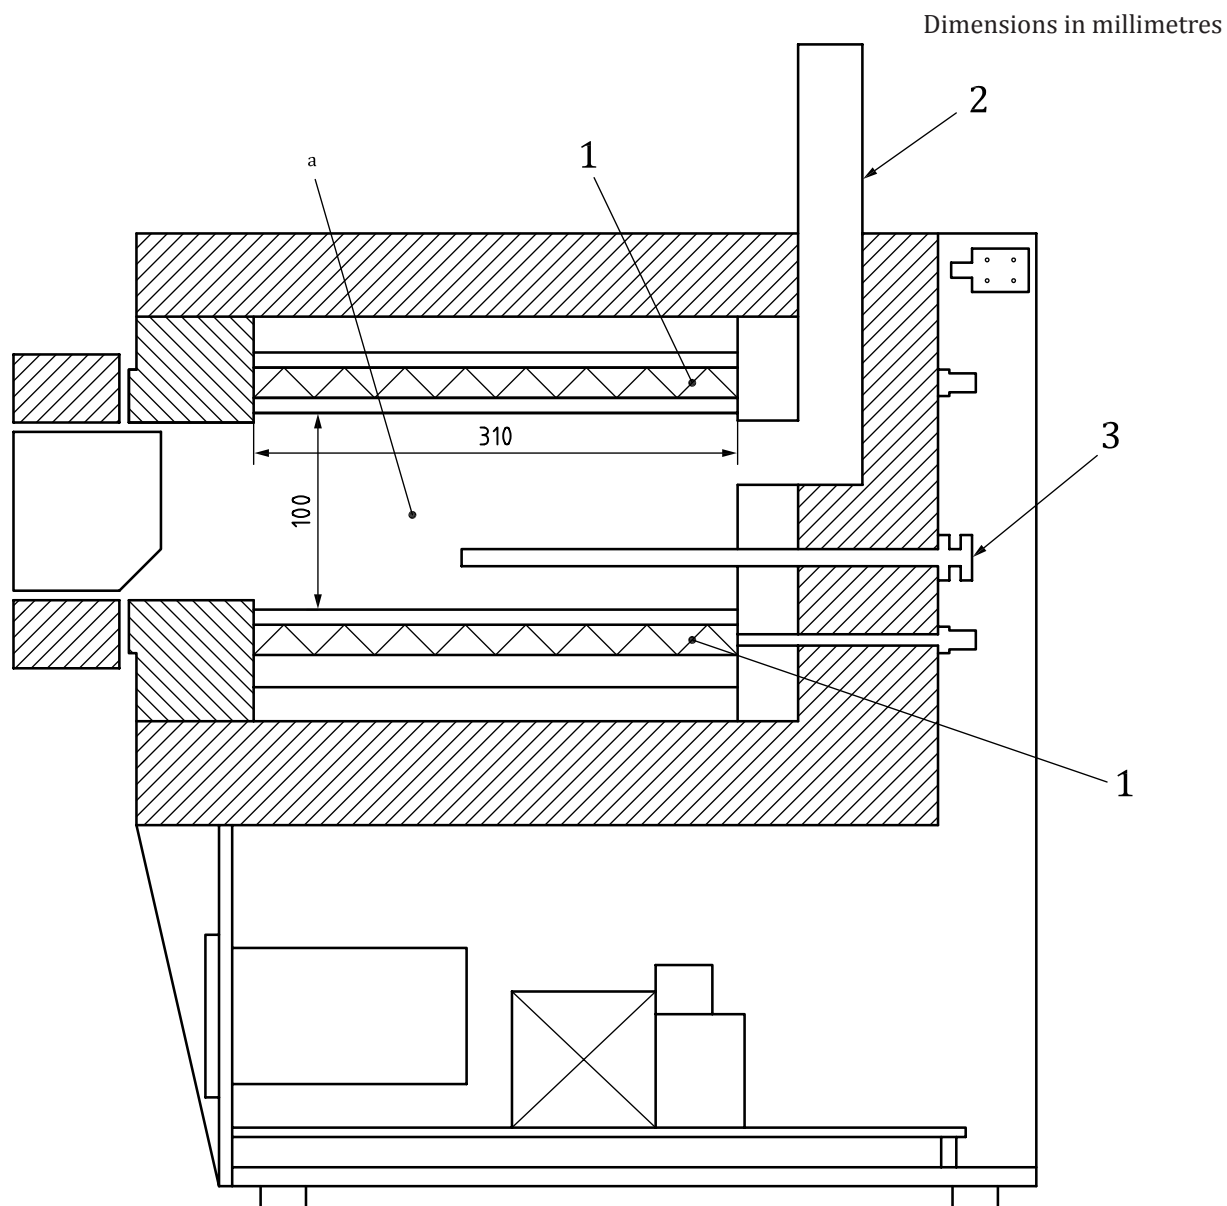

**Key**

- 1 heating system
- 2 flue
- 3 thermocouple
- a Chamber width is 200 mm.

**Figure 1 — Example of a suitable furnace**

Dimensions in millimetres



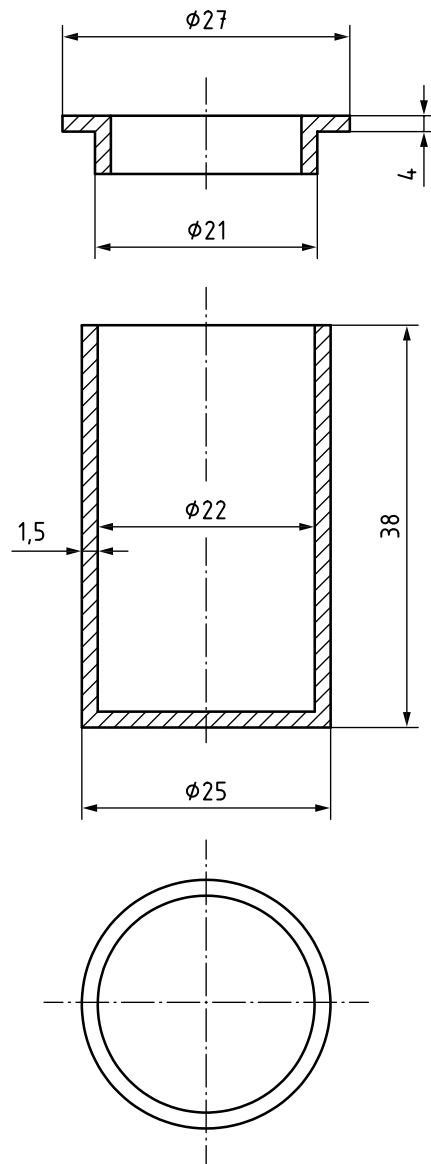


Figure 2 — Silica crucible and lid

Dimensions in millimetres

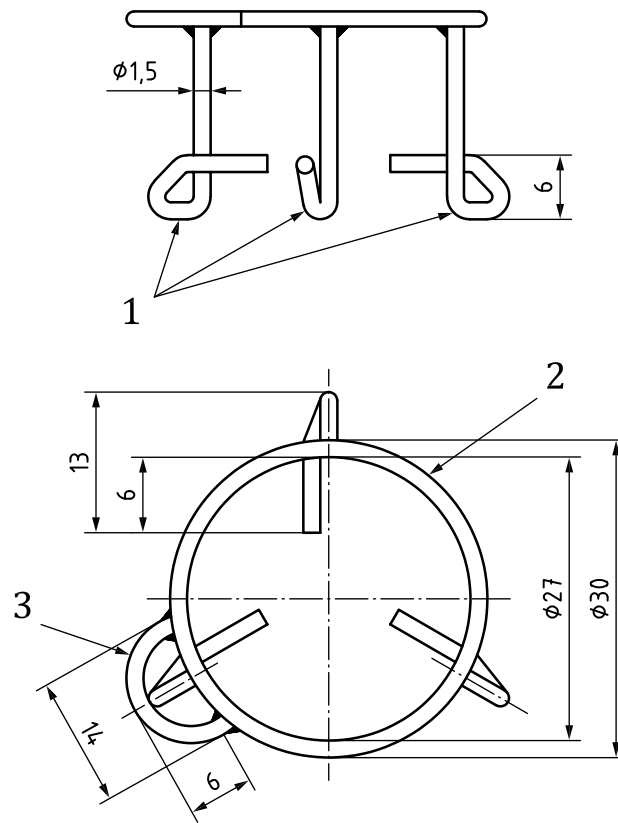

a) Suitable for a single determination

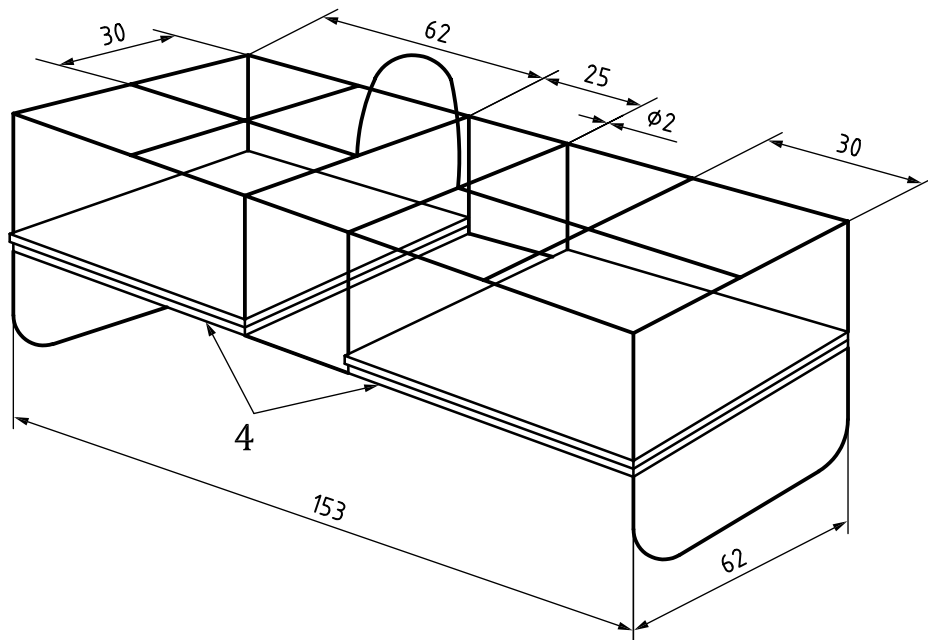

b) Suitable for multiple determinations

**Key**

- 1 three legs spaced 120° apart
- 2 ring

- 3 handle
- 4 ceramic plates

**Figure 3 — Crucible stands**

## 7 Sample

Prepare the sample for the determination of volatile matter in the analysis sample in accordance with ISO 5069-2.

## 8 Procedure

### 8.1 Preliminary procedure

Adjust the temperature of the zone in the furnaces (6.1), loaded with a stand and empty crucibles where appropriate, to  $400\text{ °C} \pm 10\text{ °C}$  and  $900\text{ °C} \pm 5\text{ °C}$  respectively, as indicated by the correctly unsheathed thermocouple (6.3). Remove the stand and crucibles and close the doors of the furnace. Heat, in a furnace (6.1) at  $900\text{ °C}$  for 7 min, either one crucible and lid (6.4) or the requisite number of crucibles and lids to fill the multiple stand. Remove the crucible(s) from the furnace and cool them, first on a metal slab and finally in a desiccator (6.7) located next to the balance. As soon as they are cool, weigh each empty crucible and lid. Record the mass(es) of the preconditioned crucibles and lids to the nearest 0,1 mg (8.4, Note 1).

### 8.2 Predetermination procedure

Before commencing the determination, mix the analysis sample for at least 1 min, preferably by mechanical means. Accurately weigh 1,00 g to 1,01 g of sample (Clause 7) to the nearest 0,1 mg into each preconditioned crucible. Replace the lid and tap the crucible on a clean hard surface until the sample forms a layer of even thickness on the bottom of the crucible. Proceed in accordance with either 8.3 or 8.4 depending on whether or not the coal has been oven-dried or air-dried.

### 8.3 Method using oven-dried coal

Place the charged crucible(s), with lid(s) removed, in the oven (6.2) at  $105\text{ °C}$  to  $110\text{ °C}$ . Dry the sample(s) to constant mass in accordance with the procedure for moisture determination specified in ISO 5068-2. Record the mass(es) of the oven-dried crucible(s), lid(s) and sample(s) to the nearest 0,1 mg.

Place the crucible(s) fitted with lid(s) containing the oven-dried sample(s) in a suitable stand (8.4, Note 2) and transfer to the furnace set at  $400\text{ °C}$  for 7 min. Immediately transfer to the furnace set at  $900\text{ °C}$  for a further 7 min.

Remove the crucible(s) and cool and weigh them in the same manner as for empty crucible(s) (see 8.1). If ash deposits are visible on the stand or crucible(s) then discard the test and repeat (8.4, Note 3).

### 8.4 Method using air-dried coal

Place the charged crucible(s) with the lid(s) in a suitable cool stand (Note 2) and transfer to the muffle furnace set at  $400\text{ °C}$  for 7 min. Immediately transfer to the furnace set at  $900\text{ °C}$  for a further 7 min. Remove the crucible(s) and cool and weigh them in the same manner as for the empty crucible(s) (see 8.1).

NOTE 1 Precisely similar treatment of the crucible(s) and lid(s) before and after the determination minimizes the effect of any film of water absorbed on its surface, while the rapid cooling reduces absorption of moisture by the coal residue.

NOTE 2 If multiple determinations are being made, fill any vacant places in the stand with empty crucibles.

NOTE 3 Certain brown coals and lignites may consistently produce ash deposits either on the crucible lid or the sample tray when tested using the two-furnace procedure. In such a case, it is recommended to press the air-dried sample into small pellets, then determine the volatile matter.

## 9 Calculation of results

Calculate the percentage by mass of volatile matter on a dry basis,  $V_d$ , according to the formulas in 9.1 and 9.2.

## 9.1 For oven-dried coal

$$V_d = 100 \times \frac{(m_2 - m_3)}{m_2 - m_1}$$

where

$m_1$  is the mass, in grams, of the empty crucible and lid (8.1);

$m_2$  is the mass, in grams, of crucible, lid and oven-dried sample (8.3);

$m_3$  is the mass, in grams, of crucible, lid and sample after heating in the furnace (8.3).

## 9.2 For air-dried coal

$$V_{ad} = \frac{100(m_2 - m_3)}{m_2 - m_1} - M_{ad}$$

$$V_d = \frac{100}{100 - M_{ad}} \times V_{ad}$$

where

$m_1$  is the mass, in grams, of the empty crucible and lid (8.1);

$m_2$  is the mass, in grams, of crucible, lid and air-dried sample (8.2);

$m_3$  is the mass, in grams, of crucible, lid and sample after heating (8.4);

$M_{ad}$  is the moisture content, expressed as a percentage by mass, in the air-dried sample, determined according to ISO 5068-2;

$V_{ad}$  is the volatile matter on an air-dried basis, expressed as a percentage by mass.

The results (the mean of duplicate determinations) shall be reported to the nearest 0,1 %.

Calculate the results to other bases in accordance with ISO 1170.

## 10 Precision of the method

### 10.1 Repeatability limit

The results of duplicate determinations, carried out in the same laboratory by the same operator using the same apparatus on the same sample within short intervals of time, shall not differ by more than the value given in [Table 1](#).

### 10.2 Reproducibility limit

The means of the results of duplicate determinations, carried out in each of two laboratories on representative test portions taken from the same sample, shall not differ by more than the value given in [Table 1](#).

**Table 1 — Precision of the method**

Repeatability	Reproducibility
1,0 % absolute	3,0 % absolute

## 11 Test report

The test report shall include the following information:

- a) a reference to this International Standard, including year of publication;
- b) the identification of the sample tested;
- c) the result of the determination, together with the analysis basis;
- d) any unusual features noted during the determination.









# British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

## About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

## Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at [bsigroup.com/standards](http://bsigroup.com/standards) or contacting our Customer Services team or Knowledge Centre.

## Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at [bsigroup.com/shop](http://bsigroup.com/shop), where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

## Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to [bsigroup.com/subscriptions](http://bsigroup.com/subscriptions).

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

**PLUS** is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit [bsigroup.com/shop](http://bsigroup.com/shop).

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email [bsmusales@bsigroup.com](mailto:bsmusales@bsigroup.com).

## BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

## Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

## Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

## Useful Contacts:

### Customer Services

**Tel:** +44 845 086 9001

**Email (orders):** [orders@bsigroup.com](mailto:orders@bsigroup.com)

**Email (enquiries):** [cservices@bsigroup.com](mailto:cservices@bsigroup.com)

### Subscriptions

**Tel:** +44 845 086 9001

**Email:** [subscriptions@bsigroup.com](mailto:subscriptions@bsigroup.com)

### Knowledge Centre

**Tel:** +44 20 8996 7004

**Email:** [knowledgecentre@bsigroup.com](mailto:knowledgecentre@bsigroup.com)

### Copyright & Licensing

**Tel:** +44 20 8996 7070

**Email:** [copyright@bsigroup.com](mailto:copyright@bsigroup.com)



...making excellence a habit.™