



BSI Standards Publication

# Iron ores — Determination of calcium — Flame atomic absorption spectrometric method

**National foreword**

This British Standard is the UK implementation of ISO 10203:2017. It supersedes BS ISO 10203:2015 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee ISE/58, Iron ores.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2017.  
Published by BSI Standards Limited 2017

ISBN 978 0 580 91926 8

ICS 73.060.10

**Compliance with a British Standard cannot confer immunity from legal obligations.**

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 30 April 2017.

**Amendments/corrigenda issued since publication**

Date	Text affected
------	---------------

---

INTERNATIONAL  
STANDARD

BS ISO 10203:2017

**ISO**  
**10203**

Fourth edition  
2017-03

---

---

**Iron ores — Determination of  
calcium — Flame atomic absorption  
spectrometric method**

*Minerais de fer — Dosage du calcium — Méthode par spectrométrie  
d'absorption atomique dans la flamme*



Reference number  
ISO 10203:2017(E)

© ISO 2017



## **COPYRIGHT PROTECTED DOCUMENT**

© ISO 2017, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Ch. de Blandonnet 8 • CP 401  
CH-1214 Vernier, Geneva, Switzerland  
Tel. +41 22 749 01 11  
Fax +41 22 749 09 47  
copyright@iso.org  
www.iso.org

# Contents

Page

<b>Foreword</b> .....	<b>iv</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Principle</b> .....	<b>1</b>
<b>5 Reagents</b> .....	<b>2</b>
<b>6 Apparatus</b> .....	<b>3</b>
<b>7 Sampling and samples</b> .....	<b>3</b>
7.1 Laboratory sample.....	3
7.2 Preparation of predried test samples.....	4
7.2.1 General.....	4
7.2.2 Method specified in ISO 2596.....	4
7.2.3 Method specified in ISO 7764.....	4
<b>8 Procedure</b> .....	<b>4</b>
8.1 Number of determinations.....	4
8.2 Test portion.....	4
8.3 Blank test and check test.....	5
8.3.1 Blank test.....	5
8.3.2 Check test.....	5
8.4 Determination.....	5
8.4.1 Decomposition of the test portion.....	5
8.4.2 Treatment of the residue.....	5
8.4.3 Preparation of the test solution.....	6
8.4.4 Adjustment of the atomic absorption spectrometer.....	6
8.4.5 Atomic absorption measurements.....	7
<b>9 Expression of results</b> .....	<b>7</b>
9.1 Calculation of mass fraction of calcium.....	7
9.2 General treatment of results.....	7
9.2.1 Repeatability and permissible tolerance.....	7
9.2.2 Determination of analytical result.....	8
9.2.3 Between-laboratories precision.....	8
9.2.4 Check for trueness.....	8
9.2.5 Calculation of final result.....	10
9.3 Oxide factor.....	10
<b>10 Test report</b> .....	<b>10</b>
<b>Annex A (normative) Flowsheet of the procedure for the acceptance of analytical values for test samples</b> .....	<b>11</b>
<b>Annex B (informative) Derivation of repeatability and permissible tolerance formulae</b> .....	<b>12</b>
<b>Annex C (informative) Precision data obtained by international analytical trials</b> .....	<b>13</b>
<b>Bibliography</b> .....	<b>14</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: [www.iso.org/iso/foreword.html](http://www.iso.org/iso/foreword.html).

This document was prepared by Technical Committee ISO/TC 102, *Iron ore and direct reduced iron*, Subcommittee SC 2, *Chemical analysis*.

This fourth edition cancels and replaces the third edition (ISO 10203:2015), of which it constitutes a minor revision with the following changes:

- in [5.11](#), minor editorial/grammatical amendments have been incorporated;
- in [6.1](#), “with a lid” has been inserted after “crucible”;
- in [6.3](#) b), “the ratio between” has been inserted before “the slope” and minor editorial/grammatical amendments have been incorporated;
- in [7.2](#), reference to ISO 2596 has been incorporated and [7.2](#) has been rearranged in a more appropriate layout/format;
- in [8.2](#), reference to ISO 2596 has been incorporated;
- “predried” has been deleted where it is inappropriate in [8.1](#), [8.2](#), and [8.3.2](#);
- some references to the reagents in [8.4.2](#), [8.4.3](#), and [Table 2](#) have been corrected;
- in the last line of [9.2.3](#), the formula has been corrected from  $|\mu_1 - A_c| \leq P$  to  $|\mu_1 - \mu_2| \leq P$ ;
- in [9.2.4](#), [Formula \(7\)](#) and the relevant descriptions have been modified to harmonize this subclause across all International Standards for which ISO/TC 102/SC 2 is responsible.

# Iron ores — Determination of calcium — Flame atomic absorption spectrometric method

**WARNING** — This document might involve hazardous materials, operations, and equipment. This document does not purport to address all of the safety problems associated with its use. It is the responsibility of the user of this document to establish appropriate health and safety practices and determine the applicability of regulatory limitations prior to use.

## 1 Scope

This document specifies a flame atomic absorption spectrometric method for the determination of the mass fraction of calcium in iron ores.

This method is applicable to mass fractions of calcium between 0,010 % and 8,00 % in natural iron ores, iron ore concentrates, and agglomerates, including sinter products.

## 2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 648, *Laboratory glassware — Single-volume pipettes*

ISO 1042, *Laboratory glassware — One-mark volumetric flasks*

ISO 2596, *Iron ores — Determination of hygroscopic moisture in analytical samples — Gravimetric, Karl Fischer and mass-loss methods*

ISO 3082, *Iron ores — Sampling and sample preparation procedures*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 7764, *Iron ores — Preparation of predried test samples for chemical analysis*

ISO 80000-1:2009, *Quantities and units — Part 1: General*

## 3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- IEC Electropedia: available at <http://www.electropedia.org/>
- ISO Online browsing platform: available at <http://www.iso.org/obp>

## 4 Principle

The test portion is decomposed by the treatment with hydrochloric acid and a small amount of nitric acid, and then evaporated to dehydrate silica, followed by dilution and filtration.

The residue is ignited and silica is removed by evaporation with hydrofluoric and sulfuric acids. The residue is fused with sodium carbonate and the cooled melt is dissolved in the filtrate.

The solution obtained is aspirated into the flame of an atomic absorption spectrometer using a dinitrogen oxide-acetylene burner.

The absorbance values obtained for calcium are compared with those obtained from calibration solutions.

## 5 Reagents

During the analysis, use only reagents of recognized analytical grade and only water that complies with Grade 2 of ISO 3696.

**5.1 Sodium carbonate**, ( $\text{Na}_2\text{CO}_3$ ), anhydrous.

**5.2 Hydrochloric acid**, ( $\rho$  1,19 g/ml).

**5.3 Hydrochloric acid**,  $\rho$  1,19 g/ml, diluted 1 + 9.

**5.4 Nitric acid**,  $\rho$  1,4 g/ml.

**5.5 Hydrofluoric acid**,  $\rho$  1,13 g/ml, 40 % (mass fraction) or  $\rho$  1,185 g/ml, 48 % (mass fraction).

**5.6 Sulfuric acid**,  $\rho$  1,84 g/ml, diluted 1 + 1.

**5.7 Pure iron**, minimum purity 99,9 % (mass fraction), of mass fraction of calcium less than 0,000 2 %.

### 5.8 Background solution.

Dissolve 5,0 g pure iron (5.7) in 50 ml of hydrochloric acid (5.2) and oxidize by adding nitric acid (5.4) drop by drop. Evaporate until a syrupy consistency is obtained. Add 20 ml of hydrochloric acid (5.2) and dilute to 200 ml with water. Dissolve 17 g of sodium carbonate (5.1) in water, add carefully to the iron solution, and heat to remove carbon dioxide. Transfer the cooled solution to a 1 000 ml one-mark volumetric flask, dilute to volume with water, and mix.

### 5.9 Lanthanum chloride solution.

Dissolve 50 g of lanthanum chloride ( $\text{LaCl}_3 \cdot 7\text{H}_2\text{O}$ ) (of mass fraction of calcium less than 0,002 %) in 50 ml of hydrochloric acid (5.2) and 300 ml of hot water. Cool and dilute to 1 l.

### 5.10 Calcium standard solution, 25 $\mu\text{g}$ Ca/ml.

Dissolve 1,248 7 g of dried calcium carbonate ( $\text{CaCO}_3$ ) [minimum purity 99,9 % (mass fraction), dried at 105 °C for 1 h] in 100 ml of hydrochloric acid (5.2), diluted 1 + 3. When dissolved, cool, transfer to a 1 000 ml one-mark volumetric flask, dilute to volume with water, and mix. Transfer 10 ml of this solution to a 200 ml one-mark volumetric flask, dilute to volume with water, and mix.

### 5.11 Calcium calibration solutions.

Using pipettes, transfer 2,0 ml, 5,0 ml, 10,0 ml, 15,0 ml, and 20,0 ml portions of calcium standard solution (5.10) to 200 ml volumetric flasks (Clause 6). Add 6 ml of hydrochloric acid (5.2), 60 ml of background solution (5.8), and 40 ml of lanthanum chloride solution (5.9) to each flask. Dilute the solution to volume with water and mix. Prepare a zero calcium calibration solution by transferring 60 ml of the background solution to a 200 ml volumetric flask. Then add 6 ml of hydrochloric acid (5.2) and 40 ml of lanthanum chloride solution (5.9). Dilute the solution to volume with water and mix.



## 6 Apparatus

Ordinary laboratory apparatus, including one-mark pipettes and one-mark volumetric flasks complying with the specifications of ISO 648 and ISO 1042, respectively, and the following.

All glassware, volumetric flask lids, and the platinum crucibles shall first be washed in hydrochloric acid (diluted 1 + 1) and then in water.

**6.1 Platinum crucible with a lid**, of minimum capacity 30 ml.

**6.2 Muffle furnace**, capable of maintaining a temperature of approximately 1 100 °C.

**6.3 Atomic absorption spectrometer**, equipped with a dinitrogen oxide/acetylene burner.

**WARNING — Follow the manufacturer's instructions for igniting and extinguishing the dinitrogen oxide-acetylene flame to avoid possible explosion hazards. Wear tinted safety glasses whenever the flame is burning.**

The atomic absorption spectrometer used in this method shall meet the following criteria.

- a) Minimum sensitivity: The absorbance of the most concentrated calcium calibration solution (see [5.11](#)) shall be at least 0,3.
- b) Graph linearity: The ratio between the slope of the calibration graph covering the top 20 % of the concentration range (expressed as a change in absorbance) and the value of the slope for the bottom 20 % of the concentration range determined in the same way shall not be less than 0,7.
- c) Minimum stability: The standard deviation of the absorbance of the most concentrated calibration solution and that of the zero calibration solution, each being calculated from a sufficient number of repetitive measurements, shall be less than 1,5 % and 0,5 %, respectively, of the mean value of the absorbance of the most concentrated calibration solution.

The use of a strip chart recorder and/or digital readout device is recommended to evaluate criteria a), b), and c) and for all subsequent measurements.

**NOTE** Instrument parameters can vary with each instrument. The following parameters were successfully used in several laboratories and they can be used as guidelines. Solutions were aspirated into a dinitrogen oxide-acetylene flame of a premix burner.

In systems where the values shown below for gas flow rates do not apply, the ratio of the gas flow rates may still be a useful guideline.

— Hollow cathode lamp, mA	15
— Wavelength, nm	422,7
— Dinitrogen oxide flow rate, l/min	13,8
— Acetylene flow rate, l/min	6,6

## 7 Sampling and samples

### 7.1 Laboratory sample

For analysis, use a laboratory sample of  $-100 \mu\text{m}$  particle size which has been taken and prepared in accordance with ISO 3082. In the case of ores having significant contents of combined water or oxidizable compounds, use a particle size of  $-160 \mu\text{m}$ .

**NOTE** A guideline on significant contents of combined water and oxidizable compounds is incorporated in ISO 7764.

## 7.2 Preparation of predried test samples

### 7.2.1 General

Depending on the ore type, proceed in accordance with either [7.2.2](#) or [7.2.3](#).

### 7.2.2 Method specified in ISO 2596

This method is applicable to all types of ores.

Thoroughly mix the laboratory sample and, taking multiple increments, extract a test sample in such a way that it is representative of the whole contents of the container. Bring the test sample into equilibrium with the laboratory atmosphere in accordance with ISO 2596.

### 7.2.3 Method specified in ISO 7764

This method is not applicable to the following types of ores:

- a) processed ores containing metallic iron (direct-reduces iron);
- b) natural or processed ores in which the sulfur content is higher than 0,2 %;
- c) natural or processed ores in which the content of combined water is higher than 2,5 % by mass.

Thoroughly mix the laboratory sample and, taking multiple increments, extract a test sample in such a way that it is representative of the whole contents of the container.

## 8 Procedure

### 8.1 Number of determinations

Carry out the analysis at least in duplicate in accordance with [Annex A](#), independently, on one test sample (see [7.2](#)).

NOTE The expression “independently” means that the second and any subsequent result is not affected by the previous result(s). For this particular analytical method, this condition implies that the repetition of the procedure is carried out either by the same operator at a different time or by a different operator including, in either case, appropriate recalibration.

### 8.2 Test portion

Taking several increments, weigh, to the nearest 0,000 2 g, approximately the amount of the air-equilibrated test sample obtained in accordance with [7.2.2](#) specified in [Table 1](#). Concurrently, determine the hygroscopic moisture content in accordance with ISO 2596 and calculate the dried mass of the test portion.

Where the test sample is obtained in accordance with [7.2.3](#), transfer the test portion specified in [Table 1](#) to a weighing bottle, then dry at  $105\text{ °C} \pm 2\text{ °C}$  and determine the dried mass of the test portion to the nearest 0,000 2 g in accordance with ISO 7764.

**Table 1 — Mass of test portion**

Expected mass fraction of calcium in sample, $w_{Ca}$ Mass fraction %	Mass of test portion g
$0,010 \leq w_{Ca} \leq 4,00$	0,5
$4,00 < w_{Ca} \leq 8,00$	0,2

## 8.3 Blank test and check test

### 8.3.1 Blank test

#### 8.3.1.1 Preparation of blank test solution

Using pure iron (5.7) with a 60 % mass of the test portion in place of the test portion, carry out the same procedure described in 8.4.1 to 8.4.3 as the test portion in parallel with it.

#### 8.3.1.2 Measurement of blank value

Carry out in accordance with 8.4.5.

Where the analysis is carried out on several samples at the same time, the blank value may be represented by one test, provided that the procedure is the same and that the reagents used are from the same reagent bottles.

### 8.3.2 Check test

In each run, one analysis of a certified reference material of the same type of ore shall be carried out in parallel with the analysis of the ore sample(s) under the same conditions. A test sample of the certified reference material shall be prepared as specified in 7.2. The certified reference material should be of the same type as the sample to be analysed and the properties of the two materials should be sufficiently similar to ensure that, in either case, no significant changes in the analytical procedure will become necessary.

Where the analysis is carried out on several samples of the same type of ore at the same time, the analytical value of one certified reference material may be used.

## 8.4 Determination

### 8.4.1 Decomposition of the test portion

Transfer the test portion (see 8.2) to a 250 ml beaker. Moisten with a few millilitres of water, add 25 ml of hydrochloric acid (5.2), cover with a watch-glass, and heat gently. Increase the heat and digest just below boiling, until no further attack is apparent. Add 2 ml of nitric acid (5.4) and digest for several minutes. Remove the watch-glass and evaporate the solution until dry. Heat the salts on a hot-plate at 105 °C to 110 °C for 30 min. Add 5 ml of hydrochloric acid (5.2), cover the beaker with a watch-glass, and warm for several minutes. Add 50 ml of water, stirring to avoid the hydrolysis of titanium, and heat to boil. Wash the watch-glass and the walls of the beaker and filter the solution through a medium-texture paper containing some filter pulp into a 250 ml beaker. Carefully remove all adhering particles with a rubber-tipped glass rod or moistened filter paper and transfer to the filter, washing three times with dilute hydrochloric acid (5.3), then with hot water until the filter paper is free of iron. Transfer the paper and residue to a platinum crucible (6.1).

Evaporate the filtrate to about 100 ml and retain it.

The filter paper shall first be washed several times in warm hydrochloric acid (diluted 1 + 2), then in warm water after being attached to the funnel.

### 8.4.2 Treatment of the residue

Ignite the filter paper and residue in a platinum crucible (6.1) at a low temperature (500 °C to 800 °C). Cool, moisten with a few drops of water, and add three or four drops of sulfuric acid (5.6) and 10 ml of hydrofluoric acid (5.5).

Evaporate slowly to expel silica and then fume to remove the excess sulfuric acid. Ignite at about 700 °C. Add 1,0 g of sodium carbonate (5.1) to the residue (see note), cover the crucible, and fuse over a burner or in a muffle furnace (6.2) until a clear melt is obtained (at about 1 100 °C for 15 min).

NOTE If difficulties are experienced with the fusion, 2 g of sodium carbonate (5.1) can be used, in which case, it is advisable to double the amount of sodium carbonate and the volume of hydrochloric acid (5.2) in the background solution (5.8).

### 8.4.3 Preparation of the test solution

Dissolve the cooled melt in the retained filtrate (see 8.4.1), then remove and wash the crucible and cover (see next paragraph).

If the solution is cloudy at this stage, indicating the presence of substantial amounts of hydrolyzed titanium, it should be filtered prior to the transfer to the 200 ml volumetric flask.

Transfer the solution to a 200 ml one-mark volumetric flask.

When the mass fraction of calcium in sample is expected to be  $\leq 0,10$  %, add 40 ml of lanthanum chloride solution (5.9), dilute to volume with water, and mix. This solution is the final test solution for the low Ca sample.

When the mass fraction of calcium in sample is expected to be  $> 0,10$  %, dilute to volume with water and mix.

Transfer an appropriate aliquot of this solution (see Table 2) to a 200 ml one-mark volumetric flask and add 40 ml of lanthanum chloride solution (5.9). Add the amount of background solution (5.8) and hydrochloric acid (5.2) indicated in Table 2, dilute to volume with water, and mix (see last paragraph). This solution is the final test solution for the high Ca sample.

The dilutions shown in Table 2 will provide mass concentrations of calcium falling within the range of the calibration solutions. For instruments having high sensitivity, smaller portions of the test solution may be preferable. Avoid aliquot portions of less than 2 ml by making a preliminary dilution. Treat the blank test solution similarly.

**Table 2 — Dilution guide for test solution**

Expected mass fraction of calcium in sample, $w_{Ca}$ %	Aliquot ml	Equivalent mass of sample g	Background solution (5.8) to be added ml	Hydrochloric acid (5.2) to be added ml
$0,10 < w_{Ca} \leq 1,00$	20	0,05	55	5
$1,00 < w_{Ca} \leq 4,00$	5	0,012 5	60	6
$4,00 < w_{Ca} \leq 8,00$	5	0,005	60	6

### 8.4.4 Adjustment of the atomic absorption spectrometer

Set the wavelength for calcium (422,7 nm) to obtain minimum absorbance. Fit the correct burner and, in accordance with the manufacturer's instructions, light the appropriate flame. After 10 min of preheating the burner, adjust the fuel flow and burner to obtain maximum absorbance while aspirating the calibration solution of highest mass fraction of calcium (see 5.11). Then evaluate the criteria in 6.3.

When the sensitivity of the instrument is too high to meet the criteria, it is permitted to set analytical conditions by which the absorbance is not the maximum. In this case, the criteria in 6.3 shall be met and the conditions shall not be changed during the measurements of all solutions prepared in each independent analysis.

Aspirate water and the calibration solution to establish that the absorbance reading is not drifting and then set the initial reading for water to zero absorbance.

### 8.4.5 Atomic absorption measurements

Aspirate the calibration solutions (5.11), the blank test solution (8.3.1.1), and the final test solution (see 8.4.3) in order of increasing absorption, starting with the blank test solution and the zero calibration solution, with the final test solution being aspirated at the appropriate point in the series. Aspirate water between each solution and record the readings when stable responses are obtained.

Repeat the measurements at least twice.

If necessary, convert the average of the readings for each solution to absorbance. Obtain the net absorbance of each calibration solution by subtracting the absorbance of the zero calibration solution. Prepare a calibration graph by plotting the net absorbance values of the calibration solutions against the concentration of calcium, in micrograms per millilitre.

Convert the net absorbance values of the blank test solution and the final test solution to micrograms of calcium per millilitre by means of the calibration graph.

## 9 Expression of results

### 9.1 Calculation of mass fraction of calcium

The mass fraction of calcium,  $w_{Ca}$ , expressed in percentage, is calculated to four decimal places using [Formula \(1\)](#):

$$w_{Ca} = \frac{(\rho_{Ca} - \rho_{CaB}) \times 200}{m \times 10\,000} \quad (1)$$

$$= \frac{\rho_{Ca} - \rho_{CaB}}{m \times 50}$$

where

$\rho_{Ca}$  is the mass concentration, in micrograms per millilitre, of calcium in the final test solution;

$\rho_{CaB}$  is the mass concentration, in micrograms per millilitre, of calcium in the blank test solution;

$m$  is the mass, in grams, of sample contained in a 200 ml volume of the final test solution, taking into account any preliminary dilution which might have been made.

### 9.2 General treatment of results

#### 9.2.1 Repeatability and permissible tolerance

The precision of this analytical method is expressed by the following regression formulae:

NOTE Additional information is given in [Annex B](#) and [Annex C](#).

$$R_d = 0,027\,22 X^{0,662\,53} \quad (2)$$

$$P = 0,038\,71 X^{0,619\,66} \quad (3)$$

$$\sigma_d = 0,009\,62 X^{0,662\,53} \quad (4)$$

$$\sigma_L = 0,012\ 06\ X^{0,575\ 62} \quad (5)$$

where

$R_d$  is the independent duplicate limit;

$X$  is the mass fraction of calcium, expressed in percentage, of the pre-dried test sample, calculated as follows:

— within-laboratory [Formula \(2\)](#) and [Formula \(4\)](#): the arithmetic mean of the duplicate values;

— between-laboratories [Formula \(3\)](#) and [Formula \(5\)](#): the arithmetic mean of the final results (see [9.2.5](#)) of the two laboratories;

$P$  is the permissible tolerance between laboratories;

$\sigma_d$  is the independent duplicate standard deviation;

$\sigma_L$  is the between-laboratories standard deviation.

### 9.2.2 Determination of analytical result

Having computed the independent duplicate results according to [Formula \(1\)](#), compare them with the independent duplicate limit ( $R_d$ ), using the procedure given in [Figure A.1](#), and obtain the final laboratory result,  $\mu$ , which is calculated to five decimal places for mass fractions of calcium less than 1 % and to four decimal places for mass fractions greater than 1 %.

### 9.2.3 Between-laboratories precision

Between-laboratories precision is used to determine the agreement between the final laboratory results reported by two laboratories.

Compute the following quantity using [Formula \(6\)](#):

$$\mu_{12} = \frac{\mu_1 + \mu_2}{2} \quad (6)$$

where

$\mu_{12}$  is the mean of final results;

$\mu_1$  is the final result reported by laboratory 1;

$\mu_2$  is the final result reported by laboratory 2.

Substitute  $\mu_{12}$  for  $X$  in [Formula \(3\)](#) and calculate  $P$ .

If  $|\mu_1 - \mu_2| \leq P$ , the final results are in agreement.

### 9.2.4 Check for trueness

The trueness of the analytical method shall be checked by applying it to a certified reference material (CRM) or a reference material (RM). The procedure is the same as that described above. After

confirmation of the precision, the final laboratory result is compared with the reference or certified value,  $A_C$ . The following are two possibilities:

- a)  $|\mu_c - A_c| \leq C$ , in which case, the difference between the reported result and the reference/certified value is statistically insignificant;
- b)  $|\mu_c - A_c| > C$ , in which case, the difference between the reported result and the reference/certified value is statistically significant.

where

$\mu_c$  is the final result for the certified reference material;

$A_C$  is the certified/reference value for the CRM/RM;

$C$  is a value dependent on the type of CRM/RM used.

Certified reference materials used for this purpose should be prepared and certified in accordance with ISO Guide 35.

$C$  shall be calculated using [Formula \(7\)](#):

$$C = 2 \sqrt{\frac{s_{Lc}^2 + \frac{s_{Wc}^2}{n_{Wc}}}{N_c} + \sigma_L^2 + \frac{\sigma_d^2}{n}} \quad (7)$$

where

$s_{Lc}$  is the between-laboratories standard deviation of the certifying laboratories;

$s_{Wc}$  is the within-laboratory standard deviation of the certifying laboratories;

$n_{Wc}$  is the average number of replicate determinations in the certifying laboratories;

$N_c$  is the number of certifying laboratories;

$n$  is the number of replicate determinations carried out on the CRM/RM;

$\sigma_L$  and  $\sigma_d$  are as defined in [9.2.1](#).

The following procedure should be used when the information on the reference material certificate is incomplete:

- if there are sufficient data to enable the between-laboratories standard deviation to be estimated, delete the expression  $s_{Wc}^2 / n_{Wc}$  and regard  $s_{Lc}$  as the standard deviation of the laboratory means;
- if the certification has been made by only one laboratory or if the interlaboratory results are missing, use [Formula \(8\)](#):

$$C = 2 \sqrt{2\sigma_L^2 + \frac{\sigma_d^2}{n}} \quad (8)$$

A CRM certified by only one laboratory should be avoided, unless it is known to have an unbiased certified value.

### 9.2.5 Calculation of final result

The final result is rounded off the final laboratory result to the third decimal place for mass fractions of calcium less than 1 % and to the second decimal place for mass fraction greater than or equal to 1 % according to Rule A shown in ISO 80000-1:2009, B.3.

### 9.3 Oxide factor

The oxide factor, expressed as a percentage, is given by [Formula \(9\)](#):

$$w_{\text{CaO}} = 1,399 w_{\text{Ca}} \quad (9)$$

## 10 Test report


The test report shall include the following information:

- a) the name and address of the testing laboratory;
- b) the date of issue of the test report;
- c) a reference to this document, i.e. ISO 10203;
- d) the details necessary for the identification of the sample;
- e) the result of the analysis;
- f) the reference number of the result;
- g) any characteristics noticed during the determination and any operations not specified in this document which might have had an influence on the result, for either the test sample or the certified reference material(s).



## Annex A (normative)

### Flowsheet of the procedure for the acceptance of analytical values for test samples

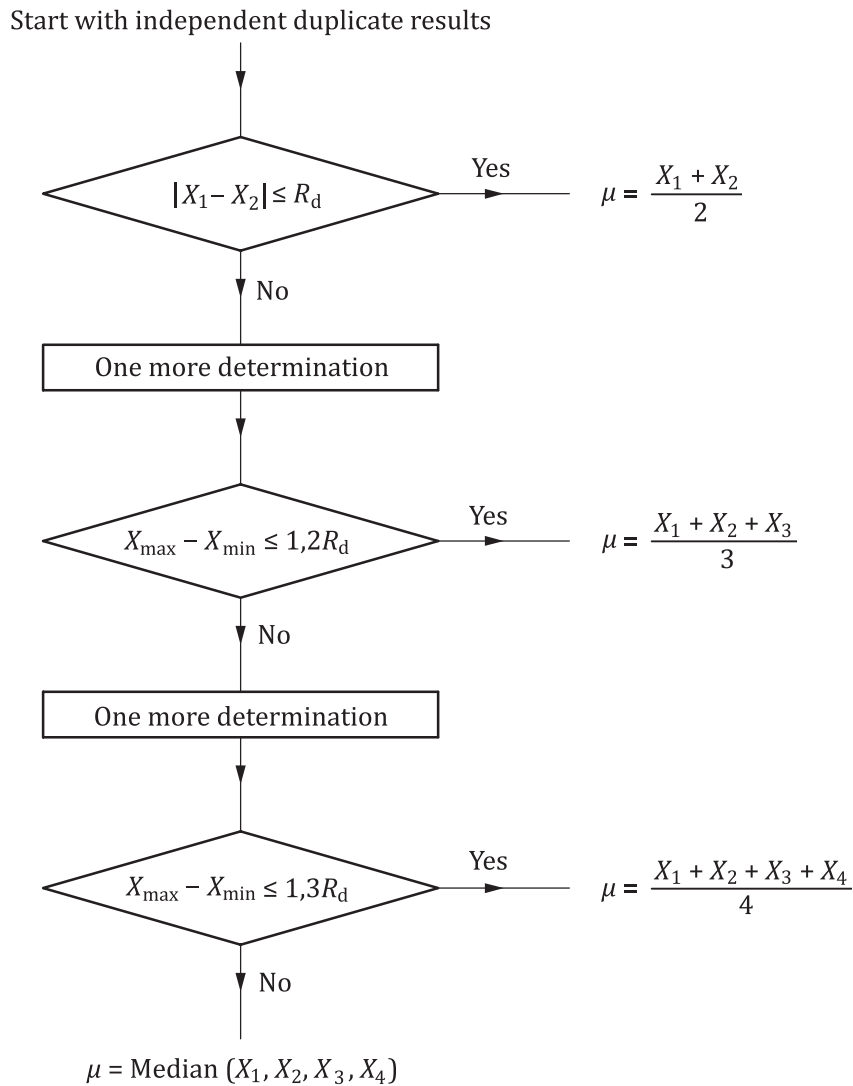

**Key**

$R_d$  permissible tolerance within a laboratory (repeatability)

**Figure A.1 — Flowsheet of the procedure for the acceptance of analytical values for test samples**

## Annex B (informative)

### Derivation of repeatability and permissible tolerance formulae

The formulae in [9.2.1](#) were derived from the results of international analytical trials carried out in 2007 to 2011 on eight iron ore samples, involving eight laboratories in four countries.

Graphical treatment of the precision data is given in [Figure C.1](#).

The test samples used are listed in [Table B.1](#).

NOTE 1 A report of the international trials and a statistical analysis of the results [Documents ISO/TC 102/SC 2 N1969, (March 2012)] is available from the Secretariat of ISO/TC 102/SC 2.


NOTE 2 The statistical analysis was performed in accordance with the ISO/TC 102/TCR 5 (Technical committee report No. 5): Procedures for statistical evaluation of data resulting from international tests, principles embodied in ISO 5725 (all parts).

**Table B.1 — Mass fractions of calcium in test samples**

Sample	Mass fraction of calcium %
JSS 801-6 Indian hematite	0,014 <sup>a</sup>
JSS 803-6 Hamersley hematite	0,013 <sup>a</sup>
JSS 804-2 Iscor hematite	0,049 0
JSS 820-3 Robe river limonite	0,269
JSS 831-1 Taharoa iron sand	0,95
JSS 853-1 Algarrobo pellet	1,78
JSS 851-4 Sintered ore	7,08
JSS 851-5 Sintered ore	7,94
<sup>a</sup> Non-certified value.	

## Annex C (informative)

### Precision data obtained by international analytical trials

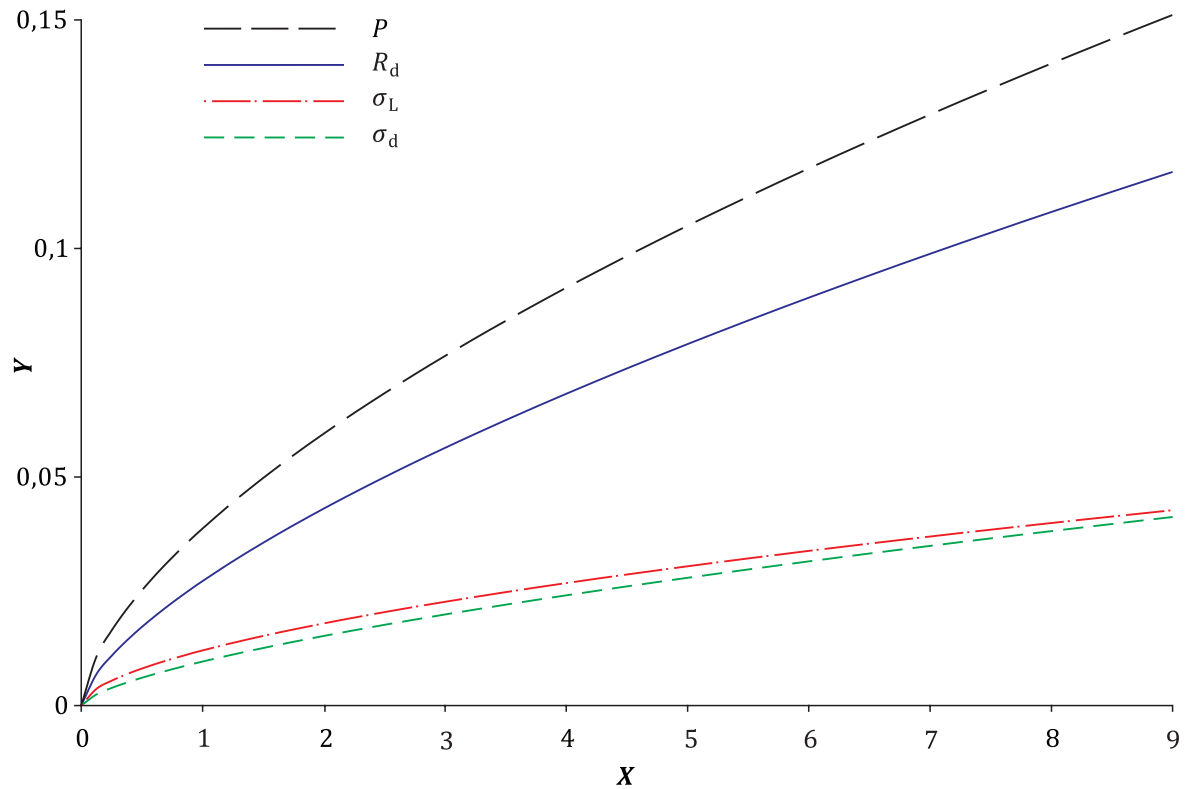

**Key**

$X$  mass fraction of calcium, %

$Y$  precision, %

**Figure C.1 — Precision data obtained by international analytical trials and regression lines**

## Bibliography

- [1] ISO 5725 (all parts), *Accuracy (trueness and precision) of measurement methods and results*
- [2] ISO Guide 35, *Reference materials — General and statistical principles for certification*







# British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

## About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

## Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at [bsigroup.com/standards](http://bsigroup.com/standards) or contacting our Customer Services team or Knowledge Centre.

## Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at [bsigroup.com/shop](http://bsigroup.com/shop), where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

## Copyright in BSI publications

All the content in BSI publications, including British Standards, is the property of and copyrighted by BSI or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use.

Save for the provisions below, you may not transfer, share or disseminate any portion of the standard to any other person. You may not adapt, distribute, commercially exploit, or publicly display the standard or any portion thereof in any manner whatsoever without BSI's prior written consent.

## Storing and using standards

Standards purchased in soft copy format:

- A British Standard purchased in soft copy format is licensed to a sole named user for personal or internal company use only.
- The standard may be stored on more than 1 device provided that it is accessible by the sole named user only and that only 1 copy is accessed at any one time.
- A single paper copy may be printed for personal or internal company use only.

Standards purchased in hard copy format:

- A British Standard purchased in hard copy format is for personal or internal company use only.
- It may not be further reproduced – in any format – to create an additional copy. This includes scanning of the document.

If you need more than 1 copy of the document, or if you wish to share the document on an internal network, you can save money by choosing a subscription product (see 'Subscriptions').

## Reproducing extracts

For permission to reproduce content from BSI publications contact the BSI Copyright & Licensing team.

## Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to [bsigroup.com/subscriptions](http://bsigroup.com/subscriptions).

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

**PLUS** is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit [bsigroup.com/shop](http://bsigroup.com/shop).

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email [subscriptions@bsigroup.com](mailto:subscriptions@bsigroup.com).

## Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

## Useful Contacts

### Customer Services

**Tel:** +44 345 086 9001

**Email (orders):** [orders@bsigroup.com](mailto:orders@bsigroup.com)

**Email (enquiries):** [cservices@bsigroup.com](mailto:cservices@bsigroup.com)

### Subscriptions

**Tel:** +44 345 086 9001

**Email:** [subscriptions@bsigroup.com](mailto:subscriptions@bsigroup.com)

### Knowledge Centre

**Tel:** +44 20 8996 7004

**Email:** [knowledgecentre@bsigroup.com](mailto:knowledgecentre@bsigroup.com)

### Copyright & Licensing

**Tel:** +44 20 8996 7070

**Email:** [copyright@bsigroup.com](mailto:copyright@bsigroup.com)

### BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK