

BS ISO 10677:2011



BSI Standards Publication

# Fine ceramics (advanced ceramics, advanced technical ceramics) — Ultraviolet light source for testing semiconducting photocatalytic materials

**bsi.**

...making excellence a habit.™

**National foreword**

This British Standard is the UK implementation of ISO 10677:2011.

The UK participation in its preparation was entrusted to Technical Committee RPI/13, Advanced technical ceramics.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© BSI 2011

ISBN 978 0 580 63924 1

ICS 81.060.30

**Compliance with a British Standard cannot confer immunity from legal obligations.**

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 July 2011.

**Amendments issued since publication**

Date	Text affected
------	---------------

---

---

---

**Fine ceramics (advanced ceramics,  
advanced technical ceramics) —  
Ultraviolet light source for testing  
semiconducting photocatalytic materials**

*Céramiques techniques — Sources lumineuses UV destinées aux  
essais des matériaux photocatalytiques semi-conducteurs*





**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2011

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 10677 was prepared by Technical Committee ISO/TC 206, *Fine ceramics*.

## Introduction

This International Standard describes the light source which is used for the performance test of photocatalysts excited by ultraviolet (UV) radiation. A photocatalyst displays its performance by light irradiation and the type of light source used depends on its applied product. Its performance includes self-cleaning, air purification, anti-bacteria, anti-mold, water purification, etc.

While it is possible to describe the light source individually depending on each performance test, this International Standard specifies independently a common standard, considering that photocatalytic materials offer complex effects and there are many common items in the light source.

# Fine ceramics (advanced ceramics, advanced technical ceramics) — Ultraviolet light source for testing semiconducting photocatalytic materials

## 1 Scope

This International Standard describes an ultraviolet (UV) light source and specifies a method of measuring the radiation intensity which is used in testing the performance of semiconducting photocatalytic materials in a laboratory.

## 2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 22197-1:2007, *Fine ceramics (advanced ceramics, advanced technical ceramics) — Test method for air-purification performance of semiconducting photocatalytic materials — Part 1: Removal of nitric oxide*

IEC 50 (845):1987/CIE Publication No.17.4:1987, *International lighting vocabulary*

CIE Publication No.85:1989, *Solar spectral irradiance*

## 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 3.1

#### **fluorescent UV lamps**

fluorescent UV lamps in which radiant intensity in the UV region of the spectrum, i.e. below 400 nm, makes up at least 80 % of the total output

### 3.2

#### **xenon arc lamps**

arc discharge lamp radiating by excited xenon gas and of the quartz-sealed type

### 3.3

#### **UV radiometer**

UV irradiance meter

UV radiometer that measures UV irradiance in wavelengths 300 nm to 400 nm

**NOTE** In general, a UV radiometer is an instrument that measures the optical radiation in wavelengths 1 nm to 400 nm.

## 4 Light source

### 4.1 General

Photocatalysts, including TiO<sub>2</sub>, are excited by UV radiation of wavelength less than 400 nm. When irradiated by UV radiation, oxidation and reduction reactions can occur at the surface of the photocatalyst. Therefore, photocatalytic materials are activated by sunlight or UV light sources. The photocatalytic efficiency depends upon the spectral distribution and radiant intensity. Light sources which include radiation of wavelength between 300 nm and 400 nm are therefore suitable for the testing of photocatalytic materials. As the UV irradiance can differ depending upon the location, it is preferable that the irradiance of the UV light source used for the test should be representative of the actual irradiance where the photocatalytic material will be utilized.

UV light sources include a fluorescent UV lamp, xenon arc lamp, germicidal lamp, mercury lamp, metal halide lamp and UV-LED. Considering the wavelength distribution, stability of irradiance and ability to produce a continuous spectrum, a fluorescent UV lamp and xenon arc lamp shall be used for testing of photocatalyst materials.

### 4.2 Fluorescent ultraviolet lamps

Fluorescent lamps use the emission from a low-pressure mercury arc to excite a phosphor that produces a continuous spectrum. In a fluorescent UV lamp, phosphors emitting UV radiation of wavelength 300 nm to 400 nm are used, and a spectral distribution depends on the type of phosphors. Moreover, in fluorescent UV lamps, a blacklight lamp (BL lamp) made of a colourless transparent glass tube, and a blacklight blue lamp (BLB lamp) made of a blue glass which absorbs a visible radiation, exist.

In evaluating a photocatalyst excited by UV radiation, fluorescent UV lamps that have peak irradiance at 351 nm or 368 nm shall be used. Examples of relative spectral irradiances are shown in Table 1.


**Table 1 — Relative spectral irradiance of fluorescent UV lamps**

Wavelength $\lambda$ nm	351 nm peak (351 BLB) %	368 nm peak (368 BLB) %
$270 \leq \lambda < 300$	0	0
$300 \leq \lambda < 320$	2,2	0,4
$320 \leq \lambda < 340$	17,6	0,1
$340 \leq \lambda < 360$	43,3	5,3
$360 \leq \lambda < 380$	29,7	76,9
$380 \leq \lambda < 400$	7,2	17,3
NOTE Irradiance between 270 nm and 400 nm is defined as 100 %.		

Example of spectral irradiance of BLB lamps and sunlight on the earth's surface are shown in Figure 1.

A spectral irradiance of a fluorescent UV lamp with a 351 nm peak is widely distributed in the UV-A region, and its short wavelength is close to sunlight transmitting window glass, thus is suitable in evaluating photocatalytic materials for indoor application.



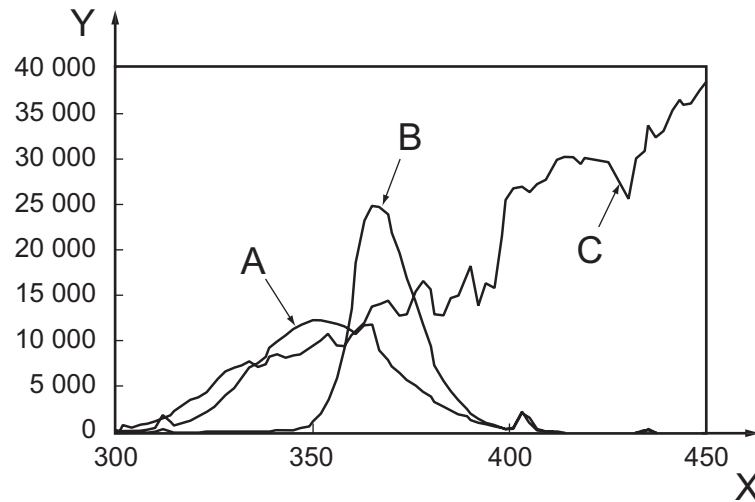

**Key**

- X wavelength, nm
- Y relative irradiance
- A 351 BLB
- B 368 BLB
- C sunlight

**Figure 1 — Spectral distribution of fluorescent UV lamps and sunlight**

**4.3 Xenon arc lamps**

Xenon arc lamps emit radiation in a range that extends from below 200 nm in the UV through the visible and into the infrared (IR) range.

Xenon arc lamps shall be used in evaluating photocatalytic materials utilizing sunlight.

Relative spectral irradiance of xenon arc lamps (Reference [1]) and sunlight on the earth's surface are shown in Table 2.

**Table 2 — Relative spectral irradiance of xenon arc lamps and sunlight on the earth's surface**

Wavelength, $\lambda$ nm	Xenon arc lamp %	Sunlight <sup>a</sup> %
$270 \leq \lambda < 300$	15,6	0,0
$300 \leq \lambda < 320$	12,9	4,5
$320 \leq \lambda < 340$	15,1	16,8
$340 \leq \lambda < 360$	17,0	21,0
$360 \leq \lambda < 380$	18,8	26,5
$380 \leq \lambda < 400$	20,6	31,2
NOTE Irradiance between 270 nm and 400 nm is defined as 100 %.		
<sup>a</sup> Adapted from Table 4 of CIE No.85:1989. (Unit is modified from W/m <sup>2</sup> to %).		

Since radiation from a xenon arc lamp contains predominately UV radiation of short wavelengths which are not present in sunlight on the earth's surface, optical filters shall be used in order to make the spectral distribution closer to that on the earth's surface, when evaluating photocatalytic materials excited by sunlight. Table 4 of CIE Publication No.85:1989 shall be used for spectral distribution of sunlight.

In the case of photocatalytic material utilizing for light transmitted by window glass, a soda-lime glass of thickness 3 mm or more shall be added.

When ozone is generated from a lamp, it is necessary to exhaust this ozone so that it does not come into contact with the test piece.

Unfiltered xenon arc lamps are not suitable for test substances and reaction products that absorb in the visible spectral region, such as methylene blue.

Xenon arc lamps emit much IR radiation. In order to prevent a rise in temperature, either a water filter or an IR absorption filter can be used.

## **5 Test chamber and apparatus**

### **5.1 Test chamber**

The test chamber shall irradiate a test piece uniformly. Moreover, UV irradiance shall be adjusted by the distance between a test piece and lamp.

If installing a reflection plate or a test-piece cover, a material which has small ultraviolet absorption or small deterioration shall be used and the structure shall be able to measure irradiance at the test piece.

### **5.2 Test chamber for testing of low irradiance**


In the case of testing for low irradiance, a metal mesh or a light insulation metal plate shall be inserted between a lamp and a test piece in order to reduce irradiance. The metal mesh or a light insulation plate shall be set near the lamp so that irradiance on the test piece shall be uniform.

### **5.3 UV radiometer**

- a) The UV radiometer shall be used for measurement of UV irradiance at the test piece. In the case of not being able to measure UV irradiance at the test piece, the UV irradiance measured shall be corrected for the irradiance on the surface of test piece.
- b) In the case of a large light source, such as fluorescent UV lamps, or using multi-light sources, a UV radiometer with a good cosine response shall be used.
- c) The UV radiometer shall be calibrated against the light source of testing.

The spectral sensitivity of a UV radiometer generally depends on the wavelength, and is mainly calibrated at the specified wavelength (such as the 365 nm mercury line). If using a light source with a different spectral distribution from the calibrated light source, the UV radiometer shall be recalibrated against the light source for testing, or the measurement values have to be corrected using measured calibration factors.

An example of the spectral sensitivity of a UV radiometer in which the spectral sensitivity is constant in the range between 310 nm and 380 nm is shown in Figure 2.

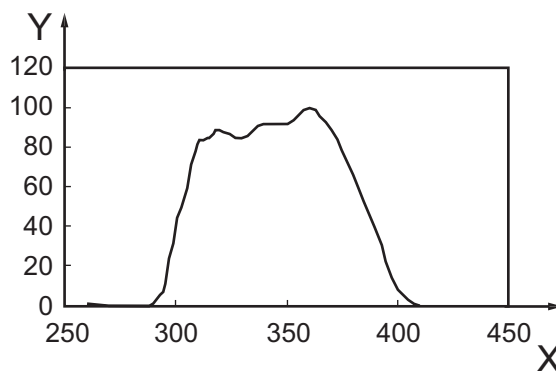

**Key**

- X wavelength, nm
- Y spectral sensitivity, %

**Figure 2 — Spectral sensitivity of a UV radiometer with constant spectral sensitivity**

## 6 Measurement of UV radiation

UV irradiance depends on the material and structure of the test chamber. Especially when a painted plate or plastic is used as a reflection plate or cover, which absorbs UV radiation. In such a case, the measurement of UV irradiance shall be done on a test piece with the same conditions of testing.

The measurement value shall be expressed in watts per square metre ( $W/m^2$ ) or milliwatts per square centimetre ( $mW/cm^2$ ).

Since UV irradiance depends on the lamp's temperature, the measurement of UV irradiance shall be done at least 15 min after switching the lighting on.

The UV radiation of lamps decreases with hours of operation. The UV irradiance shall be measured at both the start and end of the test period.

## 7 Test report

The test report shall include the items described in the test method used.

For irradiation conditions, the following information shall be included.

- a) Type of lamp used (peak wavelength, catalogue number, manufacturers' name).
- b) Type of filter used (catalogue number, manufacturers' name, thickness).
- c) Type of UV radiometer used in the measurement (spectral sensitivity of the UV radiometer and details of the calibration).
- d) UV irradiance (if the operation time of lamp is 100 h or more, UV irradiance at the start and finish of testing).

## Bibliography

- [1] JIS Z8902:1984, *Xenon Standard White Light Source*







# British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

## About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

## Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at [bsigroup.com/standards](http://bsigroup.com/standards) or contacting our Customer Services team or Knowledge Centre.

## Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at [bsigroup.com/shop](http://bsigroup.com/shop), where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

## Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to [bsigroup.com/subscriptions](http://bsigroup.com/subscriptions).

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

**PLUS** is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit [bsigroup.com/shop](http://bsigroup.com/shop).

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email [bsmusales@bsigroup.com](mailto:bsmusales@bsigroup.com).

## BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

## Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

## Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

## Useful Contacts:

### Customer Services

**Tel:** +44 845 086 9001

**Email (orders):** [orders@bsigroup.com](mailto:orders@bsigroup.com)

**Email (enquiries):** [cservices@bsigroup.com](mailto:cservices@bsigroup.com)

### Subscriptions

**Tel:** +44 845 086 9001

**Email:** [subscriptions@bsigroup.com](mailto:subscriptions@bsigroup.com)

### Knowledge Centre

**Tel:** +44 20 8996 7004

**Email:** [knowledgecentre@bsigroup.com](mailto:knowledgecentre@bsigroup.com)

### Copyright & Licensing

**Tel:** +44 20 8996 7070

**Email:** [copyright@bsigroup.com](mailto:copyright@bsigroup.com)



...making excellence a habit.™