

Iron ores — Determination of cobalt — Flame atomic absorption spectrometric method

ICS 73.060.10

National foreword

This British Standard is the UK implementation of ISO 11533:2009. It supersedes BS ISO 11533:1996 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee ISE/58, Iron Ores.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 July 2009

© BSI 2009

ISBN 978 0 580 62729 3

Amendments/corrigenda issued since publication

Date	Comments

INTERNATIONAL STANDARD

ISO
11533

Second edition
2009-06-15

Iron ores — Determination of cobalt — Flame atomic absorption spectrometric method

*Minerais de fer — Dosage du cobalt — Méthode par spectrométrie
d'absorption atomique dans la flamme*



Reference number
ISO 11533:2009(E)

© ISO 2009

PDF disclaimer

This PDF file may contain embedded typefaces. In accordance with Adobe's licensing policy, this file may be printed or viewed but shall not be edited unless the typefaces which are embedded are licensed to and installed on the computer performing the editing. In downloading this file, parties accept therein the responsibility of not infringing Adobe's licensing policy. The ISO Central Secretariat accepts no liability in this area.

Adobe is a trademark of Adobe Systems Incorporated.

Details of the software products used to create this PDF file can be found in the General Info relative to the file; the PDF-creation parameters were optimized for printing. Every care has been taken to ensure that the file is suitable for use by ISO member bodies. In the unlikely event that a problem relating to it is found, please inform the Central Secretariat at the address given below.



COPYRIGHT PROTECTED DOCUMENT

© ISO 2009

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Principle.....	1
4 Reagents.....	2
5 Apparatus	2
6 Sampling and samples.....	3
6.1 Laboratory sample	3
6.2 Preparation of predried test samples	3
7 Procedure	3
7.1 Number of determinations	3
7.2 Test portion	4
7.3 Blank test and check test	4
7.4 Determination	4
7.4.1 Decomposition of the test portion	4
7.4.2 Treatment of residue	4
7.4.3 Treatment of combined filtrate and washings	4
7.4.4 Preparation of the set of calibration solutions	5
7.4.5 Adjustment of atomic absorption spectrometer	5
7.4.6 Atomic absorption measurements	5
8 Expression of results	6
8.1 Calculation of mass fraction of cobalt	6
8.2 General treatment of results.....	6
8.2.1 Repeatability and permissible tolerances.....	6
8.2.2 Determination of analytical result.....	7
8.2.3 Between-laboratories precision	7
8.2.4 Check for trueness	7
8.2.5 Calculation of final result.....	8
8.3 Oxide factor.....	8
9 Test report.....	9
Annex A (normative) Flowsheet of the procedure for the acceptance of analytical values for test samples	10
Annex B (informative) Derivation of repeatability and permissible tolerance equations.....	11
Annex C (informative) Precision data obtained by international analytical trials	12

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 11533 was prepared by Technical Committee ISO/TC 102, *Iron ore and direct reduced iron*, Subcommittee SC 2, *Chemical analysis*.

This second edition cancels and replaces the first edition (ISO 11533:1996), which has been technically revised.

Iron ores — Determination of cobalt — Flame atomic absorption spectrometric method

WARNING — This International Standard may involve hazardous materials, operations and equipment. This International Standard does not purport to address all of the safety problems associated with its use. It is the responsibility of the user of this International Standard to establish appropriate health and safety practices and determine the applicability of regulatory limitations prior to use.

1 Scope

This International Standard specifies a flame atomic absorption spectrometric method for the determination of the mass fraction of cobalt in iron ores.

This method is applicable to a mass-fraction range of 0,000 7 % to 0,06 % of cobalt in natural iron ores, iron ore concentrates and agglomerates, including sinter products.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 648, *Laboratory glassware — Single-volume pipettes*

ISO 1042, *Laboratory glassware — One-mark volumetric flasks*

ISO 3082, *Iron ores — Sampling and sample preparation procedures*

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 7764, *Iron ores — Preparation of predried test samples for chemical analysis*

3 Principle

A test portion is decomposed by treatment with hydrochloric, nitric, sulfuric and hydrofluoric acids. The solution is evaporated to dryness, then dissolved and filtered.

The residue is ignited, then silica is removed by treatment with hydrofluoric acid and evaporation to dryness. The residue is fused with sodium carbonate. The cooled melt is dissolved with hydrochloric acid, and combined with the original filtrate.

Iron is extracted with isobutyl acetate. The aqueous phase is evaporated to reduced volume, acidified with nitric acid and diluted to volume.

The solution is aspirated into the flame of an atomic absorption spectrometer using an air/acetylene burner.

The absorbance values obtained for cobalt are compared with those obtained from the calibration solutions.

4 Reagents

During the analysis, use only reagents of recognized analytical grade and water that complies with grade 2 of ISO 3696.

- 4.1 **Sodium carbonate** (Na_2CO_3), anhydrous.
- 4.2 **Hydrochloric acid**, ρ 1,16 g/ml to 1,19 g/ml.
- 4.3 **Hydrochloric acid**, ρ 1,16 g/ml to 1,19 g/ml, diluted 1 + 1.
- 4.4 **Nitric acid**, ρ 1,4 g/ml.
- 4.5 **Hydrofluoric acid**, ρ 1,13 g/ml, 40 % (by mass), or ρ 1,185 g/ml, 48 % (by mass).
- 4.6 **Sulfuric acid**, ρ 1,84 g/ml, diluted 1 + 1.
- 4.7 **Isobutyl acetate**.
- 4.8 **Sodium background solution**.

Dissolve 15 g of sodium carbonate (4.1) in 50 ml of water. While stirring, slowly add 25 ml of hydrochloric acid (4.2). Warm to eliminate carbon dioxide, then cool. Dilute to 250 ml and mix.

4.9 Cobalt standard solutions.

4.9.1 Stock solution, 1 000 μg Co/ml.

Dissolve 1,000 g of cobalt metal [of purity > 99,5 % (by mass)] by heating in 30 ml of hydrochloric acid (4.2). Add 5 ml of nitric acid (4.4) and heat to expel the oxides of nitrogen. Cool, dilute to 1 000 ml with water in a one-mark volumetric flask and mix.

4.9.2 Standard solution A, 25 μg Co/ml.

Transfer 25 ml of cobalt stock solution (4.9.1) to a 1 000 ml one-mark volumetric flask. Dilute to volume with water and mix.

4.9.3 Standard solution B, 200 μg Co/ml.

Transfer 50 ml of cobalt stock solution (4.9.1) to a 250 ml one-mark volumetric flask. Dilute to volume with water and mix.

5 Apparatus

Ordinary laboratory apparatus, including one-mark pipettes and one-mark volumetric flasks complying with the specifications of ISO 648 and ISO 1042, respectively, and the following.

- 5.1 **Separating funnels**, of capacity 100 ml.
- 5.2 **Platinum crucibles**, of capacity 30 ml.
- 5.3 **Atomic absorption spectrometer**, equipped with an air/acetylene burner.

WARNING — To avoid possible explosion hazards, follow the manufacturer's instructions for igniting and extinguishing the air/acetylene flame. Wear tinted safety glasses whenever the burner is in operation.

The atomic absorption spectrometer used in this method shall meet the following criteria:

- a) **Minimum sensitivity:** the absorbance of the 4 µg/ml cobalt calibration solution, when measured in a flame of 10 cm path length at 240,7 nm, shall be at least 0,20, and the absorbance of the 32 µg/ml cobalt calibration solution, when measured in a flame of 10 cm path length at 252,2 nm, shall be at least 0,60 when scale-expansion facilities are not used.
- b) **Graph linearity:** the slope of the calibration graph covering the top 20 % of the concentration range (expressed as a change in absorbance) shall not be less than 0,7 of the value of the slope for the bottom 20 % of the concentration range determined in the same way.
- c) **Minimum stability:** the standard deviation of the absorbance of the most concentrated calibration solution and that of the zero calibration solution, each being calculated from a minimum number of 10 repetitive measurements, shall be less than 1,5 % and 0,5 %, respectively, of the mean value of the absorbance of the most concentrated calibration solution.

The use of a strip-chart recorder and/or digital read-out device is recommended to evaluate criteria a), b) and c) and for all subsequent measurements.

NOTE Instrument parameters can vary with each instrument. The following parameters have been successfully used in several laboratories and they can be used as guidelines. Solutions were aspirated into an air/acetylene flame.

Hollow cathode lamp, mA	7
Wavelength, nm	240,7 252,2
Air flow rate, l/min	20
Acetylene flow rate, l/min	5

In systems where the values shown for gas flow rates do not apply, the ratio of the gas flow rates can still be a useful guideline.

Criteria b) and c) should be determined separately at wavelengths of 240,7 nm and 252,2 nm.

6 Sampling and samples

6.1 Laboratory sample

For analysis, use a laboratory sample of minus 100 µm particle size which has been taken and prepared in accordance with ISO 3082. In the case of ores having significant contents of combined water or oxidizable compounds, use a particle size of minus 160 µm.

NOTE Guidance on significant contents of combined water and oxidizable compounds is incorporated in ISO 7764.

6.2 Preparation of predried test samples

Thoroughly mix the laboratory sample and, taking multiple increments, extract a test sample in such a way that it is representative of the whole contents of the container. Dry the test sample at 105 °C ± 2 °C as specified in ISO 7764. (This is the predried test sample.)

7 Procedure

7.1 Number of determinations

Carry out the analysis at least in duplicate in accordance with Annex A, independently, on one predried test sample.

NOTE The expression “independently” means that the second and any subsequent result is not affected by the previous result(s). For this particular analytical method, this condition implies that the repetition of the procedure is carried

out either by the same operator at a different time or by a different operator, including appropriate recalibration in both cases.

7.2 Test portion

Taking several increments, weigh, to the nearest 0,000 2 g, approximately 2 g of the predried test sample obtained in accordance with 6.2.

The test portion should be taken and weighed quickly in order to avoid reabsorption of moisture.

7.3 Blank test and check test

In each run, one blank test and one analysis of a certified reference material of the same type of ore shall be carried out in parallel with the analysis of the ore sample(s) under the same conditions. A predried test sample of the certified reference material shall be prepared as specified in 6.2.

The certified reference material should be of the same type as the sample to be analysed and the properties of the two materials should be sufficiently similar to ensure that, in both cases, no significant changes in the analytical procedure will become necessary.

Where the analysis is carried out on several samples at the same time, the blank value may be represented by one test, provided that the procedure is the same and the reagents used are from the same reagent bottles.

Where the analysis is carried out on several samples of the same type of ore at the same time, the analytical value of one certified reference material may be used.

7.4 Determination

7.4.1 Decomposition of the test portion

Transfer the test portion (7.2) to a 250 ml beaker. Moisten with a few millilitres of water, add 50 ml of hydrochloric acid (4.2), cover with a watch-glass, and heat at 95 °C for 1 h.

If after this digestion the amount of insoluble residue is high, raise the hotplate temperature to about 105 °C and continue heating, avoiding boiling.

Add 5 ml of nitric acid (4.4) and 0,5 ml of sulfuric acid (4.6) and heat at 105 °C for 15 min. Displace the watch-glass to provide a gap of approximately 5 mm, and add 1 ml of hydrofluoric acid (4.5). Evaporate to dryness and heat for a further 15 min.

Add 20 ml of hydrochloric acid (4.3) and heat gently to dissolve the soluble salts. Wash the watch-glass and wall of the beaker. Filter through a close-texture filter paper (maximum diameter 11 cm) into a 250 ml beaker. Remove all adhering particles from the beaker with a rubber-tipped rod, and wash the paper and residue with several minimum volumes of warm hydrochloric acid (4.3) until the paper is free from iron stain, then wash thoroughly with warm water. Retain the filtrate.

7.4.2 Treatment of residue

Place the paper and residue in a platinum crucible (5.2). Evaporate most of the water from the filter paper by placing the crucible on a hotplate for approximately 20 min. Char the paper at 600 °C for 30 min, then ignite at 850 °C for 60 min. Cool and add 5 ml of hydrofluoric acid (4.5) and 0,5 ml of sulfuric acid (4.6). Evaporate to dryness on a hotplate at 200 °C. Add 300 mg of sodium carbonate (4.1) and fuse at 900 °C for 30 min. Dissolve the cooled melt by warming with 10 ml of hydrochloric acid (4.3) on a hotplate.

7.4.3 Treatment of combined filtrate and washings

Evaporate the filtrate (7.4.1) and washings to between 5 ml and 10 ml.

Add 20 ml of hydrochloric acid (4.2). Add the processed residue solution (7.4.2), using 2 ml of hydrochloric acid (4.3) from the jet of a wash bottle to rinse out the crucible.

Transfer to a separating funnel (5.1), using 5 ml to 7 ml of hydrochloric acid (4.3) from the jet of a wash bottle. Add 25 ml of isobutyl acetate (4.7) and shake vigorously for 1 min. Allow the layers to separate, then run the lower aqueous layer into a 250 ml beaker until 0,5 ml of the aqueous layer remains. Add 5 ml of hydrochloric acid (4.2) and allow 1 ml to flow through the stopcock. Shake vigorously for 30 s, allow the layers to separate, then run all of the lower aqueous layer into the beaker. Discard the organic layer containing the extracted iron.

Rinse the aqueous solution back into the separating funnel, using 2 ml of hydrochloric acid (4.3) from the jet of a wash bottle, and repeat the isobutyl acetate extraction step described above.

Evaporate the beaker containing the aqueous phase to approximately 5 ml.

Rinse the walls of the beaker with 5 ml of water. Add 5 ml of nitric acid (4.4). Transfer to a 50 ml volumetric flask and dilute to volume with water.

7.4.4 Preparation of the set of calibration solutions

Prepare a range of calibration solutions to suit the expected mass fraction of cobalt in the sample. For the mass-fraction range of 0,000 7 % to 0,010 0 % of cobalt, use standard solution A (4.9.2). For the mass-fraction range of 0,010 0 % to 0,06 % of cobalt, use standard solution B (4.9.3).

Transfer 2 ml; 4 ml; 6 ml and 8 ml portions of the appropriate standard solution to 50 ml one-mark volumetric flasks. Add 5 ml of sodium background solution (4.8), 5 ml of nitric acid (4.4) and 5 ml of hydrochloric acid (4.3). Dilute each solution to volume with water and mix. Prepare a zero calibration solution by transferring 5 ml of sodium background solution (4.8), 5 ml of nitric acid (4.4) and 5 ml of hydrochloric acid (4.3) to a 50 ml one-mark volumetric flask. Dilute to volume with water and mix.

The range of cobalt that can be covered may vary from instrument to instrument. Attention should be paid to the minimum criteria given in 5.3. For instruments having high sensitivity, smaller aliquots of the standard solutions can be used. In this situation, the concentrations in Table 1 will have to be adjusted accordingly.

7.4.5 Adjustment of atomic absorption spectrometer

Set the wavelength for cobalt (240,7 nm for a mass fraction of cobalt less than 0,010 0 %, 252,2 nm for a mass fraction of cobalt range 0,010 0 % to 0,06 %) to obtain minimum absorbance. Fit the correct burner and, in accordance with the manufacturer's instructions, light the air/acetylene flame. After 10 min of preheating the burner, adjust the fuel and burner to obtain maximum absorbance while aspirating the calibration solution with the highest concentration (see 7.4.4), and evaluate the criteria in 5.3.

Aspirate water and the calibration solution to verify that the absorbance reading is not drifting, then set the initial reading for water to zero absorbance.

7.4.6 Atomic absorption measurements

Aspirate the calibration solutions and the final test solution in order of increasing absorption, starting with the diluted blank test solution and the zero calibration solution, with the final test solution being aspirated at the proper point in the series. Aspirate water between each solution and record the absorbance readings when stable responses are obtained.

Repeat the measurements at least twice more, and average the readings. Obtain the net absorbance of each calibration solution by subtracting the absorbance of the zero calibration solution. Similarly, obtain the net absorbance of the final test solution by subtracting the absorbance of the diluted blank test solution.

Prepare a calibration graph by plotting the net absorbance values of the calibration solutions against the concentrations, in micrograms per millilitre, of cobalt (see Table 1).

Convert the net absorbance values of the final test solution to micrograms of cobalt per millilitre by means of the calibration graph.

Table 1 — Calibration solutions

Solution number	Standard solution A (4.9.2) ml	Standard solution B (4.9.3) ml	Concentration of cobalt µg/ml
0	0	0	0
1	2	—	1
2	4	—	2
3	6	—	3
4	8	—	4
5	—	2	8
6	—	4	16
7	—	6	24
8	—	8	32

8 Expression of results

8.1 Calculation of mass fraction of cobalt

The mass fraction of cobalt, w_{Co} , expressed as a percentage to six decimal places, is calculated from Equation (1):

$$w_{\text{Co}} = \frac{\rho_{\text{Co}} \times 50}{1000\,000 \times m} \times 100 = \frac{\rho_{\text{Co}}}{200 \times m} \quad (1)$$

where

ρ_{Co} is the concentration, in micrograms per millilitre, of cobalt in the test solution;

m is the mass, in grams, of the test portion.

8.2 General treatment of results

8.2.1 Repeatability and permissible tolerances

The precision of this analytical method is expressed by the following equations:

$$R_d = 0,053\,2X + 0,000\,3 \quad (2)$$

$$P = 0,101\,8X + 0,000\,4 \quad (3)$$

$$\sigma_d = 0,018\,8X + 0,000\,1 \quad (4)$$

$$\sigma_L = 0,032\,5X + 0,000\,1 \quad (5)$$

where

- X is the mass fraction of cobalt, expressed as a percentage, of the predried test sample, calculated as follows:
- within-laboratory Equations (2) and (4): the arithmetic mean of the duplicate values;
 - between-laboratories Equations (3) and (5): the arithmetic mean of the final results (8.2.5) of the two laboratories.
- σ_d is the independent duplicate standard deviation;
- σ_L is the between-laboratories standard deviation;
- R_d is the independent duplicate limit;
- P is the permissible tolerance between laboratories.

Additional information is given in Annexes B and C.

8.2.2 Determination of analytical result

Having computed the independent duplicate results according to Equation (1), compare them with the independent duplicate limit (R_d), using the procedure given in Annex A.

8.2.3 Between-laboratories precision

Between-laboratories precision is used to determine the agreement between the final results reported by two laboratories. The assumption is that both laboratories followed the procedure described in 8.2.2.

Compute the following quantity:

$$\mu_{1,2} = \frac{\mu_1 + \mu_2}{2} \quad (6)$$

where

- μ_1 is the final result reported by laboratory 1;
- μ_2 is the final result reported by laboratory 2;
- $\mu_{1,2}$ is the mean of the final results.

If $|\mu_1 - \mu_2| \leq P$, the final results are in agreement.

8.2.4 Check for trueness

The trueness of the analytical method shall be checked by applying it to a certified reference material (CRM) or a reference material (RM). The procedure is the same as that described above. After confirmation of the precision, the final laboratory result is compared with the reference or certified value, A_C . There are two possibilities:

- a) $|\mu_C - A_C| \leq C$ in which case the difference between the reported result and the reference/certified value is statistically insignificant;
- b) $|\mu_C - A_C| > C$ in which case the difference between the reported result and the reference/certified value is statistically significant;

where

- μ_C is the final result for the certified reference material;

A_c is the reference/certified value for the CRM/RM;

C is a value dependent on the type of CRM/RM used.

Certified reference materials used for this purpose should be prepared and certified in accordance with ISO Guide 35:2006, *Reference materials — General and statistical principles for certification*.

C shall be calculated as follows:

$$C = 2 \sqrt{\frac{s_c^2}{N_c} + \sigma_L^2 + \frac{\sigma_d^2}{n}} \quad (7)$$

where

s_c is the standard deviation of laboratory means (each value for calculating the standard deviation is the average value in each certifying laboratory) of the CRM/RM;

N_c is the number of certifying laboratories;

n is the number of replicate determinations carried out on the CRM/RM.

For CRMs certified by only one laboratory, C shall be calculated as follows:

$$C = \sqrt{2\sigma_L^2 + \frac{\sigma_d^2}{n}} \quad (8)$$

A CRM certified by only one laboratory should be avoided, unless it is known to have an unbiased certified value.

8.2.5 Calculation of final result

The final result is the arithmetic mean of the acceptable analytical values for the test sample, or as otherwise determined by the operations specified in Annex A, calculated to six decimal places and rounded off to the fourth decimal place as follows:

- when the figure in the fifth decimal place is less than 5, it is discarded and the figure in the fourth decimal place is kept unchanged;
- when the figure in the fifth decimal place is 5 and there is a figure other than 0 in the sixth decimal place, or when the figure in the fifth decimal place is greater than 5, the figure in the fourth decimal place is increased by one;
- when the figure in the fifth decimal place is 5 and the figure 0 is in the sixth decimal place, the 5 is discarded and the figure in the fourth decimal place is kept unchanged if it is 0, 2, 4, 6 or 8 and is increased by one if it is 1, 3, 5, 7 or 9.

8.3 Oxide factor

The oxide factor, expressed as a percent, is given by the following equation:

$$w_{\text{CoO}} = 1,271 w_{\text{Co}} \quad (9)$$

9 Test report


The test report shall include the following information:

- a) name and address of the testing laboratory;
- b) date of issue of the test report;
- c) a reference to this International Standard;
- d) details necessary for the identification of the sample;
- e) result of the analysis;
- f) reference number of the result;
- g) any characteristics noticed during the determination, and any operations not specified in this International Standard which may have had an influence on the result, for either the test sample or the certified reference material(s).

Annex A (normative)

Flowsheet of the procedure for the acceptance of analytical values for test samples

Start with independent duplicate results

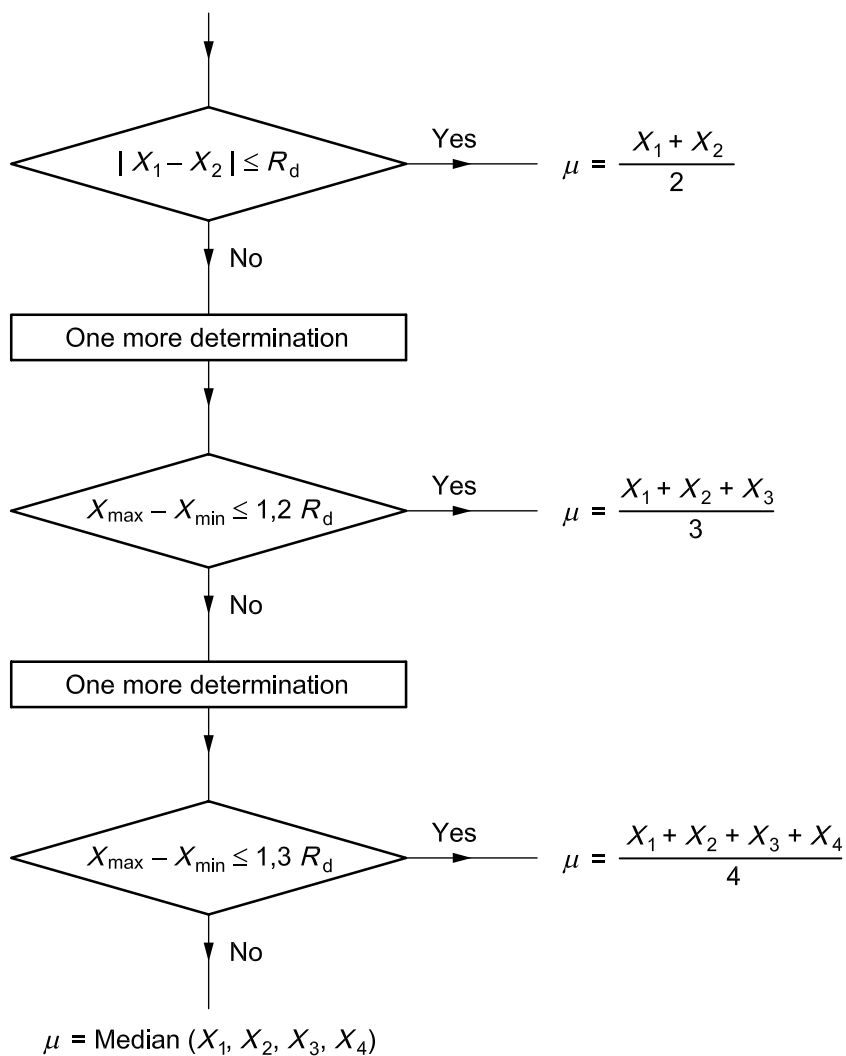

R_d : as defined in 8.2.1

Annex B (informative)

Derivation of repeatability and permissible tolerance equations

The equations in 8.2.1 were derived from the results of international analytical trials carried out in 1990 to 1992 on seven iron ore samples, involving 14 laboratories in six countries.

The graphical treatment of the precision data is given in Annex C.

The test samples used are listed in Table B.1.

Table B.1 — Mass fractions of cobalt in test samples

Sample	Mass fraction of cobalt %
NBS Sibley 27 f	0,000 7
Whyalla pellets	0,002 6
Algarrobo	0,006 2
Peru magnetite	0,008 2
Philippine iron sand	0,014 4
Palabora magnetite	0,021 2
USSR ore	0,059 0

NOTE 1 A report of the international trials (Document ISO/TC 102/SC 2 N1094, September 1992) and a statistical analysis of the results (Document ISO/TC 102 TRC 13, March 2008) are available from the Secretariat of ISO/TC 102/SC 2.

NOTE 2 The statistical analysis was performed in accordance with the principles embodied in ISO 5725 (all parts), *Accuracy (trueness and precision) of measurement methods and results*.

Annex C (informative)

Precision data obtained by international analytical trials

Figure C.1 is a graphical representation of the equations in 8.2.1.

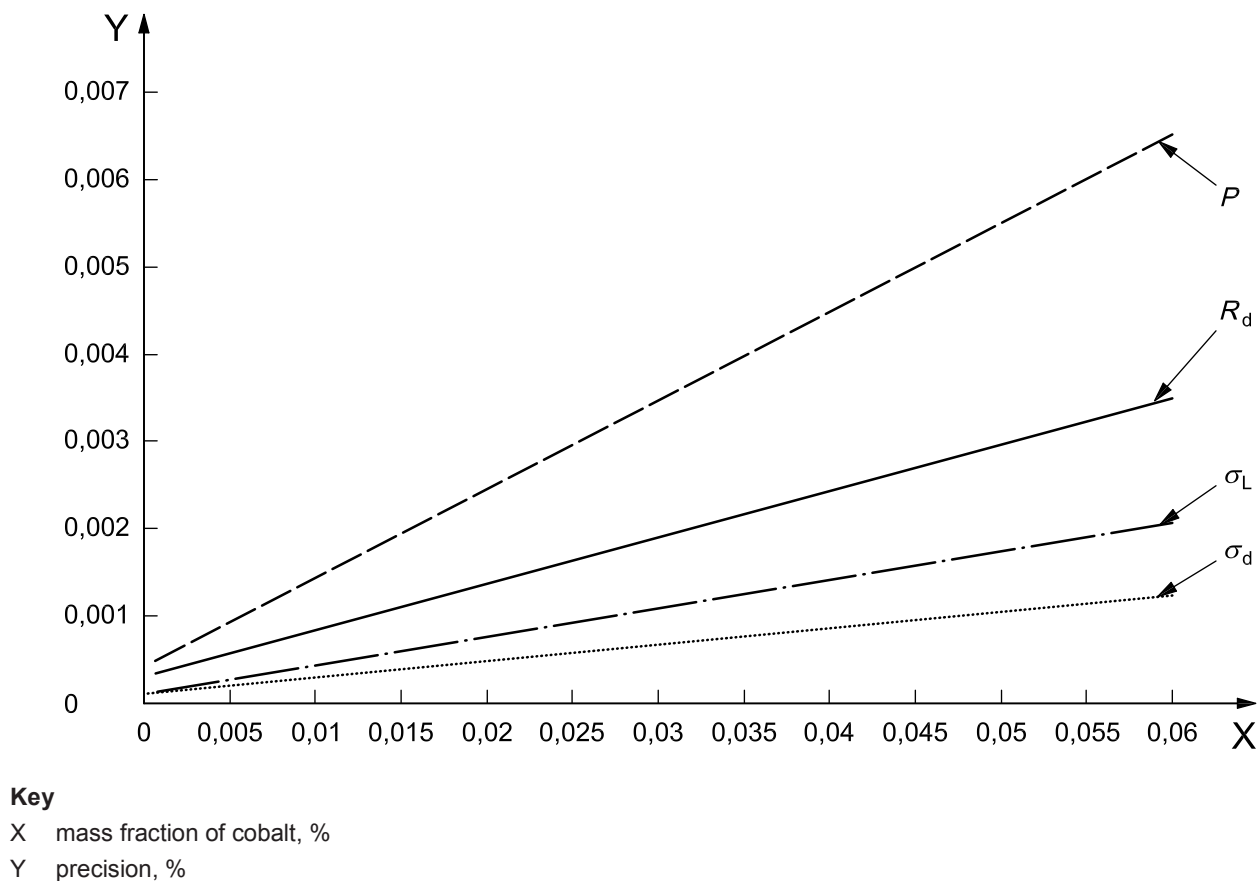


Figure C.1 — Least-squares fit of precision against X for cobalt

ICS 73.060.10

Price based on 12 pages

BSI - British Standards Institution

BSI is the independent national body responsible for preparing British Standards. It presents the UK view on standards in Europe and at the international level. It is incorporated by Royal Charter.

Revisions

British Standards are updated by amendment or revision. Users of British Standards should make sure that they possess the latest amendments or editions.

It is the constant aim of BSI to improve the quality of our products and services. We would be grateful if anyone finding an inaccuracy or ambiguity while using this British Standard would inform the Secretary of the technical committee responsible, the identity of which can be found on the inside front cover. Tel: +44 (0)20 8996 9000. Fax: +44 (0)20 8996 7400.

BSI offers members an individual updating service called PLUS which ensures that subscribers automatically receive the latest editions of standards.

Buying standards

Orders for all BSI, international and foreign standards publications should be addressed to Customer Services. Tel: +44 (0)20 8996 9001. Fax: +44 (0)20 8996 7001 Email: orders@bsigroup.com You may also buy directly using a debit/credit card from the BSI Shop on the Website <http://www.bsigroup.com/shop>

In response to orders for international standards, it is BSI policy to supply the BSI implementation of those that have been published as British Standards, unless otherwise requested.

Information on standards

BSI provides a wide range of information on national, European and international standards through its Library and its Technical Help to Exporters Service. Various BSI electronic information services are also available which give details on all its products and services. Contact Information Centre. Tel: +44 (0)20 8996 7111 Fax: +44 (0)20 8996 7048 Email: info@bsigroup.com

Subscribing members of BSI are kept up to date with standards developments and receive substantial discounts on the purchase price of standards. For details of these and other benefits contact Membership Administration. Tel: +44 (0)20 8996 7002 Fax: +44 (0)20 8996 7001 Email: membership@bsigroup.com

Information regarding online access to British Standards via British Standards Online can be found at <http://www.bsigroup.com/BSOL>

Further information about BSI is available on the BSI website at <http://www.bsigroup.com>

Copyright

Copyright subsists in all BSI publications. BSI also holds the copyright, in the UK, of the publications of the international standardization bodies. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI.

This does not preclude the free use, in the course of implementing the standard, of necessary details such as symbols, and size, type or grade designations. If these details are to be used for any other purpose than implementation then the prior written permission of BSI must be obtained.

Details and advice can be obtained from the Copyright and Licensing Manager. Tel: +44 (0)20 8996 7070 Email: copyright@bsigroup.com