

BS ISO 12154:2014



BSI Standards Publication

# Determination of density by volumetric displacement — Skeleton density by gas pycnometry

**bsi.**

...making excellence a habit.™

**National foreword**

This British Standard is the UK implementation of ISO 12154:2014.

The UK participation in its preparation was entrusted to Technical Committee LBI/37, Particle characterization including sieving.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2014. Published by BSI Standards Limited 2014

ISBN 978 0 580 79043 0

ICS 19.120

**Compliance with a British Standard cannot confer immunity from legal obligations.**

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 30 April 2014.

**Amendments issued since publication**

Date	Text affected
------	---------------

---

INTERNATIONAL  
STANDARD

**ISO**  
**12154**

First edition  
2014-04-01

---

---

**Determination of density by  
volumetric displacement — Skeleton  
density by gas pycnometry**

*Détermination de la masse volumique par déplacement  
volumétrique — Masse volumique du squelette mesurée par  
pycnométrie à gaz*



Reference number  
ISO 12154:2014(E)

© ISO 2014



**COPYRIGHT PROTECTED DOCUMENT**

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office  
Case postale 56 • CH-1211 Geneva 20  
Tel. + 41 22 749 01 11  
Fax + 41 22 749 09 47  
E-mail [copyright@iso.org](mailto:copyright@iso.org)  
Web [www.iso.org](http://www.iso.org)

Published in Switzerland

# Contents

	Page
<b>Foreword</b> .....	<b>iv</b>
<b>Introduction</b> .....	<b>v</b>
<b>1 Scope</b> .....	<b>1</b>
<b>2 Normative references</b> .....	<b>1</b>
<b>3 Terms and definitions</b> .....	<b>1</b>
<b>4 Symbols and abbreviated terms</b> .....	<b>2</b>
<b>5 Principle of the method</b> .....	<b>2</b>
<b>6 Apparatus and procedure</b> .....	<b>3</b>
6.1 Apparatus.....	3
6.2 Sample pre-treatment and determination of sample mass.....	4
6.3 Determination of the solid skeleton volume of the sample.....	5
6.4 Calculation of skeleton density.....	6
6.5 Calibration procedure.....	6
<b>7 Test report</b> .....	<b>8</b>
<b>Annex A (informative) Interferences</b> .....	<b>9</b>
<b>Bibliography</b> .....	<b>11</b>

## Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see [www.iso.org/directives](http://www.iso.org/directives)).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see [www.iso.org/patents](http://www.iso.org/patents)).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: Foreword - Supplementary information

The committee responsible for this document is ISO/TC 24, *Particle characterization including sieving*, Subcommittee SC 4, *Particle characterization*.

## Introduction

The true solid state density of a material is defined as the ratio of the mass to the volume occupied by that mass. Therefore, the contribution to the volume made by pores or internal voids and also interparticle voids (in the case of granulated or highly dispersed samples) shall be subtracted when calculating the true density.

If the material has no porosity, the true density can be measured by displacement of any fluid in which the solid remains inert. The accuracy of the method is limited by the accuracy with which the fluid volume can be determined. Usually, however, the pores, cracks, or crevices of the material will not easily be completely penetrated by a displaced liquid. In these instances, the true density can be measured by using a gas as the displaced fluid if the material does not contain closed pores, which cannot be penetrated by the analysis gas. Therefore, the density experimentally determined by gas pycnometry generally is the so called skeleton density of the material which equals the true solid state density only for samples without closed pores.

Apparatus used to measure solid volumes are often referred to as pyknometers or pycnometers after the Greek “pyknos”, meaning thick or dense. With gas pycnometry, materials of irregular shape can be analysed.

Once the volume of solid skeleton of the sample and the sample mass have been determined, the skeleton density is readily calculated.





# Determination of density by volumetric displacement — Skeleton density by gas pycnometry

## 1 Scope

This International Standard specifies a method for rapid and efficient determination of the skeleton density of solid material samples of regular or irregular shape, whether powdered or in one piece, by means of a gas displacement pycnometer.

## 2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 14488, *Particulate materials — Sampling and sample splitting for the determination of particulate properties*

ISO 9277, *Determination of the specific surface area of solids by gas adsorption — BET method*

ISO 15901-3, *Pore size distribution and porosity of solid materials by mercury porosimetry and gas adsorption — Part 3: Analysis of micropores by gas adsorption*

## 3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

### 3.1

#### **density**

ratio of the mass of a certain amount of a sample to the volume occupied by that mass

### 3.2

#### **true solid state density**

ratio of the sample mass to the volume of the compact solid skeleton of the sample which excludes the volume of open and closed pores or internal voids and also interparticle voids as in the case of granulated or highly dispersed samples

### 3.3

#### **skeleton density**

ratio between sample mass and the volume of the sample including the volume of closed pores (if present) but excluding the volumes of open pores as well as that of void spaces between particles within the bulk sample

### 3.4

#### **closed pore**

pore totally enclosed by its walls and hence not interconnecting with other pores and not accessible to fluids

### 3.5

#### **open pore**

pore not totally enclosed by its walls and open to the surface either directly or by interconnecting with other pores and therefore accessible to fluids

### 3.6

#### gauge pressure sensor

because gauge pressure is defined relative to atmospheric conditions, the signal or reading of a gauge pressure sensor is the total pressure minus atmospheric pressure

### 3.7

#### absolute pressure sensor

absolute pressure sensor measures the pressure relative to an absolute vacuum that means the reference is full vacuum (zero pressure)

## 4 Symbols and abbreviated terms

Table 1 — Symbols

Symbol	Name	Unit
$\rho_s$	skeleton density	$\text{g cm}^{-3}$
$m_s$	sample mass	g
$V_s$	skeleton volume of the sample	$\text{cm}^3$
$V_{\text{cell}}$	sample chamber volume	$\text{cm}^3$
$V_{\text{ref}}$	reference chamber volume	$\text{cm}^3$
$V_{\text{cal}}$	volume of the calibrated reference sample	$\text{cm}^3$
$p_1$	equilibrated gauge pressure prior to expansion <sup>a</sup>	Pa
$p_2$	equilibrated gauge pressure after expansion <sup>a</sup>	Pa
$p_{A1}$	equilibrated gauge pressure before expansion (calibration step A) <sup>a</sup>	Pa
$p_{A2}$	equilibrated gauge pressure after expansion (calibration step A) <sup>a</sup>	Pa
$p_{B1}$	equilibrated gauge pressure before expansion (2nd calibration step) <sup>a</sup>	Pa
$p_{B2}$	equilibrated gauge pressure after expansion (2nd calibration step) <sup>a</sup>	Pa
$p_a$	pycnometer pressure at start of analysis	Pa
$p_i^*$	pycnometer absolute gas pressure $i$ ( $i = 1, 2, A1, A2, B1, \text{ or } B2$ )	Pa
$p_i$	pycnometer excess gas pressure $i$ ( $i = 1, 2, A1, A2, B1, \text{ or } B2$ )	Pa

<sup>a</sup> gauge pressure (excess gas pressure)  $p_i$  is defined as the difference between the absolute pressure  $p_i^*$  and the pycnometer pressure  $p_a$  at start of analysis, i.e.  $p_i = p_i^* - p_a$  (see 3.6, 3.7, and 6.3.2.1)

## 5 Principle of the method

The skeleton density will be determined volumetrically in a gas expansion pycnometer. This technique is based on the displacement of a volume of gas by the solid space. The measurement is performed by expanding gas from one chamber to another (see Figure 1) under isothermal conditions. First, the weight of the dry sample is to be determined and the sample loaded into the sample chamber. The sample chamber then is pressurized to a set value when using the experimental configuration 1 of Figure 1. In a further step, the analysis gas will be expanded into a second chamber, the reference volume. The equilibrated pressures for both steps will be recorded by the instrument. Density is calculated using these values.

For gas pycnometers according to the experimental configuration 2 of Figure 1, the first step consists in pressurizing the reference chamber to a set value followed by the expansion into the sample chamber having a lower initial pressure than the set value. It is important for both experimental pycnometer configurations, that every chamber of the pycnometer is at the same pressure  $p_a$  prior to starting the

analysis steps (see [Clause 6](#)) Furthermore, all parts of the pycnometer shall have the same controlled temperature.

The analysis gas of sufficient purity (see [6.1](#)) shall be nonreactive and also non-adsorbing onto the solid sample. It has to behave as ideally as possible. Therefore, helium is used for most applications. Another reason for the preferred use of helium as the analysis gas for gas pycnometry is that it is able to penetrate even the smallest pores or cracks of a material.

NOTE 1 Because of its pronounced ability to permeate thin inner walls of samples with closed cells, helium can cause difficulties if permeable samples are to be analysed. Therefore, as described in Annex [A.6](#), gas pycnometric measurements using helium can be erroneous in the case of organic samples like cellulose and cellular polymers with low density. For density measurements of those samples, the use of alternative inert gases such as nitrogen, argon, or sulfur hexafluoride as well as dry air is recommended.

NOTE 2 If the sample contains no closed pores, then the volume measured by gas pycnometry is the true volume. To test the presence of closed pores, after a first density determination the sample can be powdered revealing any possible closed pores accessible to the test gas. An increased density value of the ground sample material indicates closed pores in the original sample.

## 6 Apparatus and procedure

### 6.1 Apparatus

**6.1.1 Gas expansion pycnometer**, with fixed-volume sample chamber (see [Figure 1](#)).<sup>[1] [2] [3]</sup>

**6.1.2 Calibrated reference sample**, (in general calibration spheres made of stainless steel with known traceable volume).

**6.1.3 Analysis gas**, in general helium (see [Clause 5](#)) with a minimum purity of 99,996 % (by volume).

**6.1.4 Analytical balance**.


**6.1.5 Drying oven**, for pre-treatment of samples preferably with the option of purging during heating or heating in a vacuum.

[Figure 1](#) is a schematic diagram of the two principal configurations of automatic gas expansion pycnometers having fixed sample chamber size. Main components of such instruments are two chambers connected by tubes (a sample chamber which can be sealed for inserting the sample or the calibration spheres and a reference chamber), a pressure-measuring sensor, and three valves. The difference between the pycnometer configurations is in the sequence of the sample chamber and the reference chamber.


Sample volumes of commercially available gas expansion pycnometers vary from 0,1 cm<sup>3</sup> to about 500 cm<sup>3</sup>. This is accomplished either by having fixed-volume sample chambers of different sizes, or by means of volume-filling inserts placed into a sample chamber. These variations in sample chamber

volume are necessary because the accuracy of the pycnometric measurement is related to the percent of total capacity the sample material occupies in the sample chamber.

Configuration 1

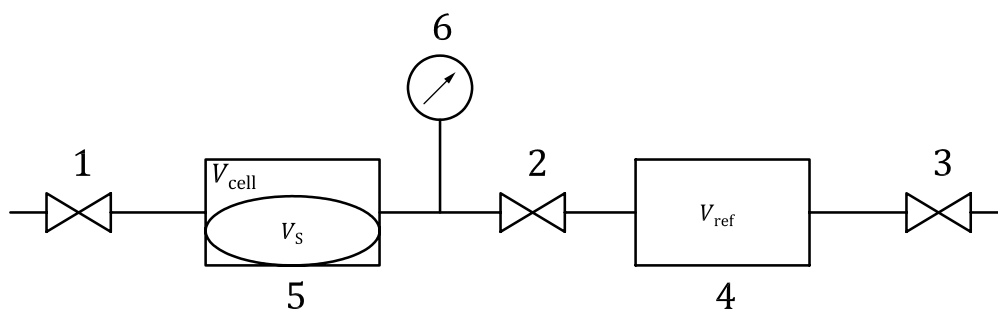

Configuration 2

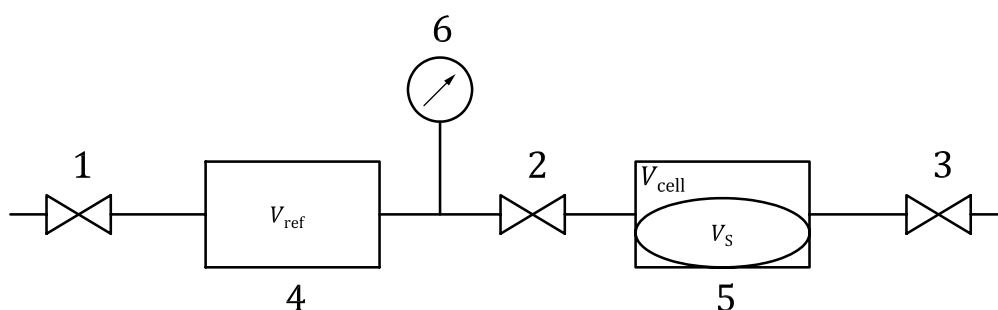

**Key**

- |                       |                     |
|-----------------------|---------------------|
| 1 valve 1, gas inlet  | 4 reference chamber |
| 2 valve 2             | 5 sample chamber    |
| 3 valve 3, gas outlet | 6 pressure sensor   |

NOTE The pressure sensor can be either an absolute pressure sensor or a gauge sensor.

**Figure 1 — Two principal experimental gas pycnometer configurations**

**6.2 Sample pre-treatment and determination of sample mass**

Preparing the sample is the first step in obtaining accurate results from the pycnometer. Samples shall be free of moisture in order to obtain true sample mass and to avoid the distorting effect of water vapour on the volume measurement. The following procedures are recommended, however, modifications may be necessary for some materials.

Sampling shall be carried out in accordance with ISO 14488. Removing the atmospheric gases from the sample can be carried out by timed evacuation, timed flow of purge gas, or repetitive pulsing (think multiple rinses) of purge gas. External oven drying of wet samples is recommended.

Heat sensitive materials can be dried by long-time exposure to silica gel, freeze drying, etc. Materials having a low melting point can be dried using the purge process. In this case, do not weigh the sample and cup until after the purge and analysis have been completed.

NOTE Outgassing can be considered complete when the results of duplicate skeleton density analyses are found within the repeatability limits of the pycnometer used.

It is important to consider that each preparation step should be conducted to avoid exposure of the dried sample to atmospheric moisture. This means weighing (see below) as rapidly as possible and installing the sample in the instrument without unnecessary delay.

The sample chamber should be capped except when inserting or removing a sample. The sample chamber shall be free of particles and as dry as possible for accurate analysis results.

For the determination of sample mass  $m_s$ , use an analytical balance readable, without estimation, to at least 0,1 % of the sample mass.

- Weigh the empty sample cup (sample holder).
- Place a quantity of sample in the sample cup. Use as large a quantity of sample as possible to fill the cup (see Annex A.1). The cup, however, should be at least two-thirds full.
- Place the sample cup with sample in a drying oven. The amount of time the sample shall be heated depends upon the material and the temperature it will tolerate; this can be established by other tests. Remove the sample cup from the oven and transfer it to a desiccator provided with active desiccant. Allow it to cool until near room temperature. In the steps which follow, minimize air exposure of the sample.
- Weigh the cup and sample and record the weight. Subtract the empty sample cup weight from the sample cup and sample weight to determine the sample weight.
- Insert sample cup with sample into the sample chamber and seal it carefully.

Microporous materials should be prepared according to the recommendations given in ISO 15901-3 and ISO 9277.

Microporous materials such as carbons, zeolites, or metal organic frameworks readily adsorb atmospheric impurities and often have a high affinity for atmospheric moisture. Contaminants can contribute to a significant fraction of the sample mass. The undesirable effects can be that the mass of the sample material is difficult to establish with precision, and a long sequence of analyses is required to obtain stable volume measurements as the impurities are being purged.

The recommended procedure for such materials is to transfer the sample in a previously weighed pycnometer sample cup directly from a vacuum oven to the pycnometer and start the analysis even though the sample is still above room temperature. Allow the analysis to proceed long enough for the sample to cool and thermal equilibrium to be established. Weigh the sample immediately after the analysis. If possible perform this weighing with the sample blanketed by nitrogen or dry air. Use this weight to calculate sample density.

## 6.3 Determination of the solid skeleton volume of the sample

### 6.3.1 Pycnometric measurement

Pycnometric analysis should be performed according to the operator's manual. A typical modern automated pycnometer allows performing automated multiple determinations on a single sample. Repeat measurements are usually required to ensure the complete removal of atmospheric gases and the proper thermal equilibration of the sample with analysis gas. Sample skeleton volume should be determined a minimum of five times. The average skeleton volume and the standard deviation are calculated using standard statistical methods.

Initially, all valves are closed with both chambers of the system at the same pressure  $p_a$ . When valve 1 opens, the sample chamber (pycnometer configuration 1) or the reference chamber (pycnometer configuration 2) is filled with the analysis gas at an elevated pressure  $p_1 > p_a$ . This valve closes and the pressure  $p_1$  about the sample (pycnometer configuration 1) or in the reference chamber (pycnometer configuration 2) is measured accurately. Valve 2 opens allowing the analysis gas to expand into the second chamber and the new equilibrium pressure  $p_2$  in both chambers again is measured accurately.

Valve 3 now opens, the gas is vented to atmosphere or to a vacuum, and the cycle repeated until consecutive volume determinations are reproduced within user-prescribed limits.

As described in [6.3.2.2](#) and [6.3.2.3](#), the sample skeleton volume will be calculated using the known calibrated volumes  $V_{\text{cell}}$  and  $V_{\text{ref}}$  of the sample chamber and the reference chamber respectively as well as the pressure readings  $p_1$  before and  $p_2$  after the gas expansion step. Finally, the skeleton density is then calculated from the sample mass divided by the solid skeleton volume of the sample (see [6.4](#)).

## 6.3.2 Calculation of the skeleton volume of the sample

### 6.3.2.1 General remarks

The pressure  $p_i$  used in the equations for calculation of the sample volume is excess values above the initial gas pressure  $p_a$  in the pycnometer at the start of the measurement. This means that every pressure value used here represents the difference between the absolute pressure and the initial pressure. This shall be noted for pycnometers without the option of zeroing the pressure sensor at the beginning of each analysis or calibration run. After zeroing, the pressure readings directly represent excess gas pressure values.

### 6.3.2.2 Calculation of $V_s$ from the configuration 1 pycnometer

The volume  $V_s$  of solid skeleton of the sample is calculated by Formula 1 when using a pycnometer according to configuration 1 in [Figure 1](#).

$$V_s = V_{\text{cell}} - \frac{p_2}{p_1 - p_2} \cdot V_{\text{ref}} \quad (1)$$

### 6.3.2.3 Calculation of $V_s$ from the configuration 2 pycnometer

In the case of pycnometer configuration 2, the volume  $V_s$  of solid skeleton is calculated by Formula 2.

$$V_s = V_{\text{cell}} - \frac{p_1 - p_2}{p_2} \cdot V_{\text{ref}} \quad (2)$$

## 6.4 Calculation of skeleton density

Use Formula 3 for the calculation of skeleton density.

$$\rho_s = \frac{m_s}{V_s} \quad (3)$$

## 6.5 Calibration procedure

### 6.5.1 General remarks

Calibration is an operation for determination of the exact values of the internal pycnometer volumes  $V_{\text{cell}}$  of the sample chamber and the volume  $V_{\text{ref}}$  of the reference chamber. Calibrating the pycnometer is necessary after changing the measurement temperature and after any changes to the sample chamber, tubing, fitting, sample cup/vessel, etc. Calibration should be performed according to the operator's manual. The calibration procedure consists of two independent expansion experiments (calibration steps A and B) because two volumes are to be calibrated. Calibration step A is an expansion experiment with an empty sample chamber including measurement of pressure values  $p_{A1}$  and  $p_{A2}$ . This gives a relationship between the sample chamber volume  $V_{\text{cell}}$  and the volume  $V_{\text{ref}}$  of the reference chamber.

Calibration step B is an expansion experiment with a calibrated reference sample of volume  $V_{\text{cal}}$  in the sample chamber including measurement of pressure values  $p_{B1}$  and  $p_{B2}$ .

NOTE The reference sample can be a certified calibration sphere of sufficient size made of high performance material such as stainless steel, titanium, silicon nitride, etc (as obtainable from accredited institutions either as primary or traceable secondary standards). In general, such spheres (or balls) are provided in form of calibration kits as standard equipment for commercial gas pycnometers.

Combining the results of these two calibration steps yields the sample chamber volume and the reference volume. Note that all pressures used are excess values (see 6.3.2.1) above the initial gas pressure  $p_a$  in the pycnometer at the start of the calibration procedure.

### 6.5.2 Calibration of pycnometer configuration 1

Calibration step A (gas expansion experiment with the empty pycnometer, experimental readings are  $p_{A1}$  and  $p_{A2}$ ).

Relationship between sample chamber volume and reference chamber volume:

$$V_{\text{cell}} = \frac{p_{A2}}{p_{A1} - p_{A2}} \cdot V_{\text{ref}} \quad (4)$$

Calibration step B (gas expansion experiment with calibrated reference sample of volume  $V_{\text{cal}}$  in the sample chamber, experimental readings are  $p_{B1}$  and  $p_{B2}$ )

Relationship between sample chamber volume, reference chamber volume, and the volume of the reference sample:

$$V_{\text{cell}} = V_{\text{cal}} + \frac{p_{B2}}{p_{B1} - p_{B2}} \cdot V_{\text{ref}} \quad (5)$$

Combining Formulae (4) and (5) gives the relationships (6) and (7) for the calculation of the sample chamber volume and the reference chamber volume using the volume of the calibrated reference sample and the pressure readings of calibration steps A and B.

Calculation of the sample chamber volume:

$$V_{\text{cell}} = \frac{p_{A2} \cdot (p_{B1} - p_{B2})}{p_{A2} \cdot p_{B1} - p_{A1} \cdot p_{B2}} \cdot V_{\text{cal}} \quad (6)$$

Calculation of the reference chamber volume:

$$V_{\text{ref}} = \frac{(p_{A1} - p_{A2}) \cdot (p_{B1} - p_{B2})}{p_{A2} \cdot p_{B1} - p_{A1} \cdot p_{B2}} \cdot V_{\text{cal}} \quad (7)$$

### 6.5.3 Calibration of pycnometer configuration 2

Calibration step A (gas expansion experiment with the empty pycnometer, experimental readings are  $p_{A1}$  and  $p_{A2}$ ).

Relationship between sample chamber volume and reference chamber volume:

$$V_{\text{cell}} = \frac{p_{A1} - p_{A2}}{p_{A2}} \cdot V_{\text{ref}} \quad (8)$$

Calibration step B (gas expansion experiment with calibrated reference sample of volume  $V_{\text{cal}}$  in the sample chamber, experimental readings are  $p_{B1}$  and  $p_{B2}$ ).

Relationship between sample chamber volume, reference chamber volume, and the volume of the reference sample:

$$V_{\text{cell}} = V_{\text{cal}} + \frac{p_{\text{B1}} - p_{\text{B2}}}{p_{\text{B2}}} \cdot V_{\text{ref}} \quad (9)$$

Combining Formulae (8) and (9) gives the relationships (10) and (11) for the calculation of the sample chamber volume and the reference chamber volume using the volume of the calibrated reference sample and the pressure readings of calibration steps A and B.

Calculation of the sample chamber volume:

$$V_{\text{cell}} = \frac{p_{\text{B2}} \cdot (p_{\text{A1}} - p_{\text{A2}})}{p_{\text{A1}} \cdot p_{\text{B2}} - p_{\text{A2}} \cdot p_{\text{B1}}} \cdot V_{\text{cal}} \quad (10)$$

Calculation of the reference chamber volume:

$$V_{\text{ref}} = \frac{p_{\text{A2}} \cdot p_{\text{B2}}}{p_{\text{A1}} \cdot p_{\text{B2}} - p_{\text{A2}} \cdot p_{\text{B1}}} \cdot V_{\text{cal}} \quad (11)$$

## 7 Test report

The test report shall include the following details:

- the date of the test;
- a reference to this International Standard (ISO 12154:2014) and any agreed deviations from it;
- details of the sample and the sample preparation;
- the type of pycnometer and its manufacturer, chamber volumes, sample mass, sample volume, temperature;
- the skeleton density of the sample including the uncertainty [combined standard deviation of repeat measurements according to the Guide to the Expression of Uncertainty in Measurement (GUM)].<sup>[4]</sup>



## Annex A (informative)

### Interferences

#### A.1 Improper sample quantity

The most common mistake operators make relative to sample quantity is using too little sample. The sample chamber and the expansion chamber volumes are sized in automated pycnometers such that maximum accuracy is achieved when the chamber volume is nearly filled with sample. Simply stated, the greatest quantity of sample the cup will accommodate should always be used. If only a limited quantity of sample is available, it is better to include a steel calibrating sphere with the sample and then manually subtract the sphere volume from the resulting measured volume to get the sample volume.

Most commercial gas pycnometers have several sample holders (sample cups) of different sizes which can be used dependent upon the quantity of sample material available.

#### A.2 Thermal effects and pressure stability

A gas pycnometer shall measure pressures and therefore shall rely on constant and equal temperature. Thermal equality between the sample, analysis gas, and analysis block of the pycnometer is an important feature for stability of the instrument. If the temperature of the sample chamber or reference chamber and the contained gas changes, then a less stable operation can be expected until the instrument again establishes thermal equilibrium. In the case when the sample is not in equilibrium with the sample chamber, the output of the instrument will drift due to the expansion and associated pressure changes of the gas.

If the pycnometer has a gauge instead of an absolute pressure sensor, the atmospheric pressure  $p_0$  shall not vary during a pycnometric test. Therefore, it is important to check that the drift of  $p_0$  during any test is small compared to the accuracy of pressure measurements.<sup>[4]</sup>

#### A.3 Influence of humidity and adsorbed gases

Undisturbed volume measurements are to be expected only for samples exhibiting essentially zero vapour pressure. A sample that contains volatile components outgasses in the sample chamber of a gas pycnometer. The result is a varying pressure measurement reported as a varying volume or density over several sequential analyses. The presence of atmospheric gases within the pores of the sample material will also affect the volume determination. Any volume contributed by the presence of liquid water usually is insignificant compared to the sample volume but the water vapour pressure can be significant. Since it is pressure that the instrument actually measures, any conditions that affect the pressure in the system influence both volume and density determinations. The effect for a less-than-dry or -outgassed sample will be an increase in the indicated sample volume and a decrease in its density, as water or adsorbed gases are driven off. If at the conclusion of an analysis the mass of the sample has decreased then a new dry or outgassed sample mass should be used to calculate density.

In the case when the material to be analysed has swelling or shrinkage effects, which are dependent upon the humidity content, density measurement by gas pycnometry is impossible.

#### A.4 Leaks

If debris is allowed to collect on the sealing surfaces of the sample cap, a leak can ensue. A small leak from this source can go unnoticed when the instrument performs a fixed number of fill-and-expansion

tests. If, however, the unit is set to achieve a required analysis precision and it terminates after a number of trials by displaying an error message, the likely source of error can be an imperfectly sealed sample cap. It is important to examine the cap seal each time it is installed and clean it if needed.

## A.5 Permeable samples

Permeability effects are most commonly encountered with samples containing closed cells. Similar effects also can be observed when using helium to analyse organic samples or some microporous carbons. Helium can permeate thin walls and even enter into the structure of some materials. This results in an incorrect density measurement. The recourse can be to use another gas, such as nitrogen or dry air, as these gases usually show a lower ability to permeate.

## A.6 Compressible samples

Some samples, such as nonrigid, closed cell foams, can collapse under normally applied experimental pressures. The result is an observed decrease in volume (and increase in density). Lowering the pressure of the displacement gas usually allows these materials to be satisfactorily analysed.

## A.7 Thermally sensitive samples

A few materials, most notably some explosives and pharmaceuticals, cannot be heated significantly above room temperature to free them of contaminants gained from atmospheric exposure. The only recourse can be to have repetitive helium purges to achieve sample cleaning together with repetitious analysis to establish how many purge cycles are required. Constancy of results should be attained once sufficient purges are achieved.

## A.8 High surface area samples

For large surface area samples, such as nanopowders, the annulus volume between the powder surface and the centre of mass of the gas molecules at the solid-adsorbate interface can be significant. This criterium could lead to a measured solid skeleton volume larger and a calculated skeleton density smaller than actual. Corrections for the contribution of the annulus volume can be made with knowledge of the effective diameter (i.e. Van der Waals diameter) of the gas molecules and the specific surface area of the powder under investigation.<sup>[5]</sup>

## A.9 Finely ground samples

It is necessary to acknowledge that when comparing the results of gas pycnometric measurements of very fine powders, the calculated skeleton density can not be the same as that of larger pieces of the same material. The reason being is that in the process of preparing many finely powdered materials, atoms or molecules located near the surface are often forced out of their positional equilibrium within the solid structure. With large pieces of material, the percentage of atoms near the surface is negligibly small. As the particle size decreases, however, this percentage increases with a resultant effect upon the density.

## Bibliography

- [1] TAMARI S. Optimum design of the constant-volume gas pycnometer for determining the volume of solid particles. *Meas. Sci. Technol.* 2004, **15** pp. 549–558
- [2] WEBB P.A., & ORR C. *Analytical Methods in Fine Particle Technology*. Micromeritics Instrument Corp, Norcross, GA, 1997
- [3] LOWELL S., SHIELDS J.E., THOMAS M.A., THOMMES M. *Characterization of Porous Solids and Powders: Surface Area, Pore Size and Density*. Kluwer Academic Publishers, Dordrecht 2004
- [4] ISO/IEC Guide 98-3:2008, *Uncertainty of measurement — Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)*
- [5] AYRAL A., PHALIPPOU J., WOIGNIER T. Skeletal density of silica aerogels determined by helium pycnometry. *J. Mater. Sci.* 1992, **27** pp. 1166–1170





# British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

## About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

## Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at [bsigroup.com/standards](http://bsigroup.com/standards) or contacting our Customer Services team or Knowledge Centre.

## Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at [bsigroup.com/shop](http://bsigroup.com/shop), where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

## Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to [bsigroup.com/subscriptions](http://bsigroup.com/subscriptions).

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

**PLUS** is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit [bsigroup.com/shop](http://bsigroup.com/shop).

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email [bsmusales@bsigroup.com](mailto:bsmusales@bsigroup.com).

## BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

## Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

## Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

## Useful Contacts:

### Customer Services

**Tel:** +44 845 086 9001

**Email (orders):** [orders@bsigroup.com](mailto:orders@bsigroup.com)

**Email (enquiries):** [cservices@bsigroup.com](mailto:cservices@bsigroup.com)

### Subscriptions

**Tel:** +44 845 086 9001

**Email:** [subscriptions@bsigroup.com](mailto:subscriptions@bsigroup.com)

### Knowledge Centre

**Tel:** +44 20 8996 7004

**Email:** [knowledgecentre@bsigroup.com](mailto:knowledgecentre@bsigroup.com)

### Copyright & Licensing

**Tel:** +44 20 8996 7070

**Email:** [copyright@bsigroup.com](mailto:copyright@bsigroup.com)



...making excellence a habit.™