



BSI Standards Publication

Nuclear fuel technology — Guidelines on the measurement of the specific surface area of uranium oxide powders by the BET method

National foreword

This British Standard is the UK implementation of ISO 12800:2017.

The UK participation in its preparation was entrusted to Technical Committee NCE/9, Nuclear fuel cycle technology.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2017
Published by BSI Standards Limited 2017

ISBN 978 0 580 87784 1

ICS 27.120.30

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 July 2017.

Amendments/corrigenda issued since publication

Date	Text affected
------	---------------

**Nuclear fuel technology — Guidelines
on the measurement of the specific
surface area of uranium oxide
powders by the BET method**

*Technologie du combustible nucléaire — Lignes directrices pour le
mesurage de l'aire massique (surface spécifique) des poudres d'oxyde
d'uranium par la méthode BET*





COPYRIGHT PROTECTED DOCUMENT

© ISO 2017, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Ch. de Blandonnet 8 • CP 401
CH-1214 Vernier, Geneva, Switzerland
Tel. +41 22 749 01 11
Fax +41 22 749 09 47
copyright@iso.org
www.iso.org

Contents

Page

Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	1
4.1 Summary of the BET method	1
4.2 Isothermal adsorption curves.....	1
4.3 Conditions and assumptions.....	2
5 Procedure	3
5.1 Sample preparation	3
5.2 Volumetric measurement	3
5.3 Gravimetric measurement.....	3
5.4 Original and single-point methods.....	3
5.5 Dynamic method (carrier gas method).....	4
5.6 Alternative methods.....	4
6 Expression of results	4
6.1 Methods of calculation	4
6.1.1 Multipoint determination	4
6.1.2 Single-point determination	7
6.2 Precision and accuracy.....	7
7 Test report	7
Bibliography	8

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT) see the following URL: www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 85, *Nuclear energy, nuclear technologies, and radiological protection*, Subcommittee SC 5, *Nuclear installations, processes and technologies*.

This second edition cancels and replaces the first edition (ISO 12800:2003), which has been technically revised.

Nuclear fuel technology — Guidelines on the measurement of the specific surface area of uranium oxide powders by the BET method

1 Scope

This document gives guidelines on the determination of the specific surface area of as-fabricated uranium dioxide powder by volumetric or gravimetric determination of the amount of nitrogen adsorbed on the powder, and can be applied to other similar materials, e.g. U_3O_8 , UO_2 - PuO_2 powders, and other bodies with similar surface areas, e.g. powder granules or green pellets, provided that the conditions described are fulfilled. Modifications using other adsorbing gases are included.

The method is relevant as long as the expected value is in the range between $1 \text{ m}^2/\text{g}$ and $10 \text{ m}^2/\text{g}$.

2 Normative references

There are no normative references in this document.

3 Terms and definitions

No terms and definitions are listed in this document.

ISO and IEC maintain terminological databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <http://www.iso.org/obp>
- IEC Electropedia: available at <http://www.electropedia.org/>

4 Principle

4.1 Summary of the BET method

The BET method is based on the determination of the amount of gas necessary to cover the surface by a monomolecular layer. This amount is determined from the isothermal adsorption curve of nitrogen (N_2) at the temperature of liquid nitrogen (77,4 K) according to Reference [2]. The amount of N_2 adsorbed at a given pressure is determined by volumetric or gravimetric measurement[6]. In order to remove surface contamination of the adsorbent, the sample has to be evacuated and heated under appropriate conditions before the measurement is performed.

4.2 Isothermal adsorption curves


The isothermal adsorption curve describes the relationship between the mass of the adsorbate, m_A (N_2), adsorbed per gram of adsorbent (e.g. UO_2 powder) at an equilibrium pressure of p at constant temperature T , as shown in [Formula \(1\)](#):

$$m_A = f(p, T) \quad (1)$$

Generally, the relative pressure p/p_0 is introduced instead of the absolute pressure p , where p_0 is the saturation vapour pressure which is $1,013 \times 10^5 \text{ Pa}$ for nitrogen at 77,4 K.

Most isothermal adsorption curves can be classified according to Reference [3] to be one of the five common types (see [Figure 1](#)).

Materials with pure micropores (<2 nm diameter) result in a type 1 adsorption curve. Most frequently, types 2 and 4 adsorption curves are observed where the adsorption energy of the first layer, E_1 , is much higher than that of subsequent layers, E_n . When $E_1 \approx E_n$, type 3 or type 5 adsorption curves result. The BET method can be applied to type 2 and type 4 curves only. The practice shows that the UO_2 , U_3O_8 and PuO_2 powders meet this condition.

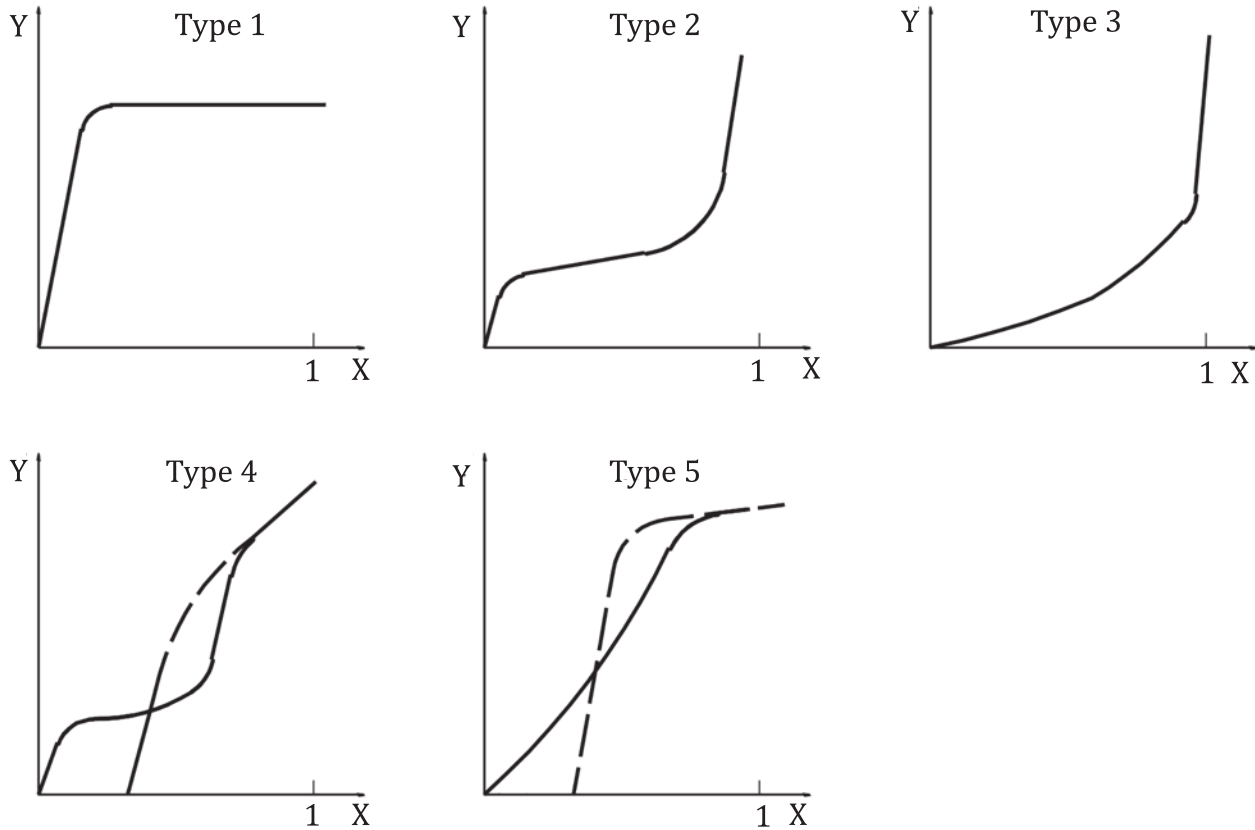

Key

X	relative pressure
Y	specific amount adsorbed
Type 1	Langmuir type
Type 2	adsorption followed by condensation
Type 3	condensation type
Type 4	two-fold adsorption
Type 5	condensation followed by adsorption

Figure 1 — Classification of adsorption isotherms

4.3 Conditions and assumptions

The method can only be applied to materials where

- a) nitrogen is not absorbed by the material,
- b) nitrogen does not react chemically with the adsorbent,
- c) all pores can be reached by the nitrogen molecule, and

d) a type 2 or type 4 adsorption curve is observed.

The BET theory includes the following assumptions.

- The adsorption energy of the first layer is independent of the degree of occupation. The adsorption energy as well as the kinetic parameters and condensation/evaporation equilibrium conditions for the second and higher layers are equal.
- The probability of adsorption at a vacant site is independent of the occupation of the neighbouring sites.
- Horizontal interactions between the adsorbed N₂ molecules can be neglected.
- The heterogeneity of the adsorbent surface can be neglected.

5 Procedure

5.1 Sample preparation

Impurities on the sample surface, especially water vapour, shall be removed before the adsorption measurement. Conditions for removing impurities (vacuum, temperature, time) have to be found which are compatible with the powder type. Chemical reactions (decomposition), sintering, change of crystal structure and other processes on the surface shall be avoided. Long evacuation periods are needed for highly porous powders. In order to shorten the heating time, the optimum temperature should be determined. In most cases, the measured specific surface area first increases with an increase in the heating temperature and then decreases, e.g. by sintering of the powder.

The optimum pre-treatment of hyperstoichiometric UO₂ powder depends on its specific surface area, intra-particle open pore size, and stoichiometry. For powders with a specific surface area between 2 m²/g and 8 m²/g, evacuation down to 2 mPa to 10 mPa (10⁻⁵ Torr to 10⁻⁴ Torr) followed by heating for 2,5 h at (150 °C ± 10 °C) is sufficient. Equivalent conditions, like 1,5 h at (180 °C ± 10 °C) or others, can be utilized as well. To prevent sintering, heating temperatures higher than 350 °C should be avoided if the O to U ratio exceeds 2,10. Shorter heating times to 20 min are possible. Instead of evacuation, the powder can be purged with purified inert gas at the temperatures and for the times mentioned above after having verified that there is no deleterious effect on characteristics of powders.

Mass of sample required depends upon material density and expected specific surface area.

5.2 Volumetric measurement

The pre-treated sample of known mass is placed in a bulb of calibrated volume, which is filled with nitrogen at a defined temperature and pressure. At ambient temperature and pressure, measurable adsorption does not occur. The closed bulb is cooled to the temperature of liquid nitrogen. The adsorbed amount of nitrogen can be calculated from the amount of nitrogen enclosed in the bulb, the volume, the temperature, and the pressure drop. Accurate volumetric measurements^{[4][5]} can be obtained by measuring the difference in pressure between the sample-containing bulb and an empty reference bulb.

5.3 Gravimetric measurement

In this case, the nitrogen is adsorbed at constant temperature and pressure. The amount of nitrogen adsorbed is directly measured by means of a microbalance.

5.4 Original and single-point methods

The determination of the specific surface area requires the static volumetric or gravimetric measurement of at least three data points of the adsorption curve in the relative pressure region $0,05 < p/p_0 < 0,35$. The measurements shall be made under equilibrium conditions.

If less accuracy is acceptable, the determination can be made easier by application of the single-point method, taking only one point of the adsorption curve in the relative pressure range $0,05 < p/p_0 < 0,35$ ("single-point method").

5.5 Dynamic method (carrier gas method)

The BET method may also be applied in a dynamic, flowing gas system. The relative pressure of the adsorbing gas (p/p_0) is obtained by mixing with an inert gas, usually helium. A stream of this gas mixture is passed over the sample which is cooled to 77,4 K in liquid nitrogen. Nitrogen from the gas stream is adsorbed on the sample.

On warming the sample to ambient temperature, the adsorbed nitrogen is desorbed into the gas stream. The amount of nitrogen desorbed is detected using a katharometer coupled to an integrator. The katharometer is calibrated by an injection of pure nitrogen.

5.6 Alternative methods

Modified methods use other adsorptives and other temperatures (see [Table 1](#)). The occupied areas per adsorbed molecule (or atom in the case of argon, krypton, and xenon) are also reported in [Table 1](#).

Another indirect method is the tracer method^{[8][9]}, where the amount of a radioactive adsorbed gas is determined by activity measurements.

Table 1 — Occupied areas per adsorbed molecule

Gas	Temperature K	Saturation pressure, p_0 Pa	Occupied area ^a per molecule nm ²
Nitrogen	77,4	$1,01 \times 10^5$	0,162
Argon	77,4	$2,58 \times 10^4$	0,138
Argon	87,3	$1,33 \times 10^5$	0,142
Krypton	77,4	$2,66 \times 10^2$	0,202
Krypton	90,2	$2,27 \times 10^2$	0,214
Xenon	90,2	8,00	0,232

^a Standard values.

6 Expression of results

6.1 Methods of calculation

6.1.1 Multipoint determination

The so-called BET equation is given by [Formula \(2\)](#):

$$V_A = \frac{V_m \cdot C \cdot p_r}{(1 - p_r)(1 - p_r + C \cdot p_r)} \quad (2)$$

where

- V_A is the adsorbed gas volume [standard temperature and pressure (S.T.P.)] at the relative pressure on unit mass of sample, in $\text{cm}^3 \text{g}^{-1}$;
- $p_r = p/p_0$ p_r is the relative pressure, p_0 is the saturation vapour pressure at the temperature of measurement;
- V_m is the gas volume (S.T.P.) needed for a complete monolayer on unit mass of sample, in $\text{cm}^3 \text{g}^{-1}$;
- C is a parameter of kinetics. $\left[C = \exp\left(\frac{E_1 - E_l}{RT}\right) \right]$
where
 E_1 is the adsorption energy;
 E_l is the liquefaction energy.

Rearrangement of [Formula \(2\)](#) yields [Formula \(3\)](#):


$$\frac{p_r}{V_A(1-p_r)} = \frac{1}{V_m C} + \frac{C-1}{V_m C} p_r \quad (3)$$

[Formula \(3\)](#) is the formula of a straight line $y = a + bx$ obtained by linear regression with [Formula \(4\)](#):

$$a = \frac{1}{V_m C} \text{ and } b = \frac{C-1}{V_m C} \quad (4)$$

If $p_r/V_A(1-p_r)$ is plotted as a function of p_r , one obtains the so-called BET line (see [Figure 2](#)). From [Formula \(4\)](#) follows [Formula \(5\)](#):

$$V_m = \frac{1}{a+b} \text{ and } C = \frac{b}{a} + 1 \quad (5)$$

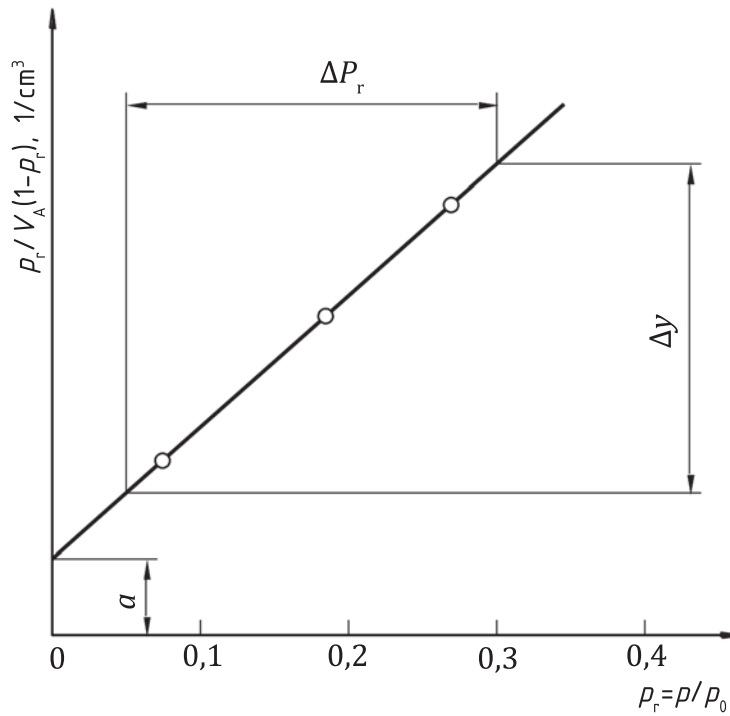

$$y = a + b \cdot p_r$$

$$a = 1 / (V_m C)$$

$$b = \Delta y / \Delta P_r = (C - 1) / (V_m C)$$

NOTE The symbols are defined in 6.1.1.

Figure 2 — The BET line

The parameters *a* and *b* can be obtained by calculation, as well as by graphical determination. The specific surface area, *S_m* (volumetric method), is determined by Formula (6):

$$S_m = \frac{v_m \cdot N_A}{m \cdot v_A} \cdot f \tag{6}$$

where

- m* is the mass of the adsorbent in g (e.g. UO₂ powder);
- N_A* is the Avogadro number (6,023 × 10²³·mol⁻¹);
- v_m* is the volume (S.T.P) of the adsorbate required for making a monolayer on the powder surface, in cm³;
- v_A* is the molar volume of adsorbate gas (S.T.P) in cm³ mol⁻¹;
- f* is the occupied area per adsorbed molecule in m² (see Table 1).

When the capacity of the monolayer is determined as the mass of adsorbate (gravimetric method), the specific surface area yields [Formula \(7\)](#):

$$S_m = \frac{m_m \cdot N_A}{m \cdot M} f \quad (7)$$

where

m_m is the mass of the adsorbate,

M is the molar mass of the adsorbate.

6.1.2 Single-point determination

The specific surface area can be determined by a single point measurement if $C \gg 1$ (preferably $C \geq 100$) and $1/C < p/p_0$. [Formula \(2\)](#) is simplified to [Formula \(8\)](#):

$$V_m = V_A(1 - p_r) \quad (8)$$

6.2 Precision and accuracy

The precision of this method depends on the particular equipment used for the measurement.

As mass of sample needed depends upon material density and expected specific surface area, the user is responsible for determining accuracy and precision as part of their method qualification process.

The apparatus should be periodically calibrated using a certified reference material such as those proposed in ISO 9277.

7 Test report

The test report shall include the following information:

- a) a reference to this document, i.e. ISO 12800:2017;
- b) all data necessary for identification of the sample;
- c) results of the test, expressed as the measure with units of measure and the expanded uncertainty with the appropriate coverage factor, calculated in accordance with JCGM 100 (ISO/GUM);
- d) location and date of the test;
- e) certified or working reference material(s) used for performance testing of the instrument and validation of results;
- f) the following procedural measurement details have to be reported:
 - method of degassing; heating conditions;
 - test method; apparatus and calculation method used;
 - adsorbate (including purity);
 - measurement temperature.

Bibliography

- [1] ISO 9277, *Determination of the specific surface area of solids by gas adsorption — BET method*
- [2] BRUNAUER S., EMMETT P.H., TELLER E., *J. Am. Chem. Soc.* **60** (1938), p. 309
- [3] BRUNAUER S., DEMING L.S., DEMING W.S., TELLER E., *J. Am. Chem. Soc.* **62** (1940), p. 1723
- [4] JOY A.S., *Vacuum* **3** (1953), p. 254
- [5] British Standard BS ISO 9277:2010, 2nd Edition, British Standard Institution, London, (2010)
- [6] ROBENS E., SANDSTEDT G., *Chemi-Ing. Techn.* **40** (1968), p. 957
- [7] NELSEN F.M., EGGERSTEN F.T., *Anal. Chem.* **30** (1958), p. 1387
- [8] HOUTMANN J.P.W., MEDEMA J., *Ber. Bunsengesellsch. für physik. Chem.* **70** (1966), p. 489
- [9] GLAWITSCH G., *Atompraxis* **2** (1956), p. 395

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Copyright in BSI publications

All the content in BSI publications, including British Standards, is the property of and copyrighted by BSI or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use.

Save for the provisions below, you may not transfer, share or disseminate any portion of the standard to any other person. You may not adapt, distribute, commercially exploit, or publicly display the standard or any portion thereof in any manner whatsoever without BSI's prior written consent.

Storing and using standards

Standards purchased in soft copy format:

- A British Standard purchased in soft copy format is licensed to a sole named user for personal or internal company use only.
- The standard may be stored on more than 1 device provided that it is accessible by the sole named user only and that only 1 copy is accessed at any one time.
- A single paper copy may be printed for personal or internal company use only.

Standards purchased in hard copy format:

- A British Standard purchased in hard copy format is for personal or internal company use only.
- It may not be further reproduced – in any format – to create an additional copy. This includes scanning of the document.

If you need more than 1 copy of the document, or if you wish to share the document on an internal network, you can save money by choosing a subscription product (see 'Subscriptions').

Reproducing extracts

For permission to reproduce content from BSI publications contact the BSI Copyright & Licensing team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email subscriptions@bsigroup.com.

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Useful Contacts

Customer Services

Tel: +44 345 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 345 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK