BS ISO 13165-3:2016



BSI Standards Publication

Water quality — Radium-226

Part 3: Test method using coprecipitation and gamma-spectrometry



BS ISO 13165-3:2016

National foreword

This British Standard is the UK implementation of ISO 13165-3:2016.

The UK participation in its preparation was entrusted to Technical Committee EH/3/8, Radioactivity measurements methods.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2016. Published by BSI Standards Limited 2016

ISBN 978 0 580 77411 9

ICS 13.060.60; 17.240

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 March 2016.

Amendments issued since publication

Date Text affected

BS ISO 13165-3:2016

INTERNATIONAL STANDARD

ISO 13165-3

First edition 2016-03-01

Water quality — Radium-226 —

Part 3:

Test method using coprecipitation and gamma-spectrometry

Qualité de l'eau — Radium 226 —

Partie 3: Méthode d'essai par coprécipitation et spectrométrie gamma



BS ISO 13165-3:2016 **ISO 13165-3:2016(E)**



COPYRIGHT PROTECTED DOCUMENT

$\, @ \,$ ISO 2016, Published in Switzerland

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office Ch. de Blandonnet 8 • CP 401 CH-1214 Vernier, Geneva, Switzerland Tel. +41 22 749 01 11 Fax +41 22 749 09 47 copyright@iso.org www.iso.org

Foreword Introduction 1 Scope 2 Normative references 3 Terms and definitions	v 111
1 Scope Normative references	11233
2 Normative references	1233
2 Normative references	1233
	1 233
	3 3
4 Symbols	33
5 Principle of the measurement	3
6 Reagents and equipment	3
6.1 Reagents	
6.2 Equipment	
7 Sampling	4
7.1 Sample collection	4
7.2 Sample transport and storage	4
8 Procedures	
8.1 Blank sample preparation	
8.2 Sample preparation 8.3 Counting procedure	
9 Quality assurance and quality control programme 9.1 General	
9.1 General 9.2 Influence quantities	
9.3 Instrument verification	
9.4 Method verification	
9.5 Demonstration of analyst capability	6
10 Expression of results	
10.1 General	
10.2 Water-soluble ²²⁶ Ra activity concentration	
10.4 Decision threshold	
10.5 Detection limit	7
10.6 Limits of the confidence interval	
10.7 Corrections for contributions from other radionuclides and background	
10.7.1 General 10.7.2 Contribution from other radionuclides	
10.7.2 Contribution from background	
11 Expression of results	
Annex A (informative) Uranium and its decay chain	
Bibliography	

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: Foreword - Supplementary information

The committee responsible for this document is ISO/TC 147, *Water quality*, Subcommittee SC 3, *Radioactivity measurements*.

ISO 13165 consists of the following parts, under the general title *Water quality — Radium-226*:

- Part 1: Test method using liquid scintillation counting
- Part 2: Test method using emanometry
- Part 3: Test method using coprecipitation and gamma-spectrometry

Introduction

Radioactivity from several naturally occurring and human-made sources is present throughout the environment. Thus, water bodies (surface waters, ground waters, sea waters) can contain radionuclides of natural and human-made origins:

Natural radionuclides, including potassium-40, and those of the thorium and uranium decay series, in particular radium-226, radium-228, uranium-234, uranium-238, and lead-210, can be found in water for natural reasons (e.g. desorption from the soil and wash-off by rain water) or releases from technological processes involving naturally occurring radioactive materials (e.g. the mining and processing of mineral sands or phosphate fertilizer production and use).

Human-made radionuclides such as transuranium elements (americium, plutonium, neptunium, curium), tritium, carbon-14, strontium-90, and gamma emitters radionuclides can also be found in natural waters as they can be authorized to be routinely released into the environment in small quantities in the effluent discharge from nuclear fuel cycle facilities and following their use in unsealed form in medicine or industry. They are also found in the water due to the past fallout of the explosion in the atmosphere of nuclear devices and those following the Chernobyl and Fukushima accident.

Human-made radionuclides, such as transuranium elements (americium, plutonium, neptunium, curium), tritium, carbon-14, strontium-90, and some gamma emitting radionuclides, can also be found in natural waters as a result of authorized routine releases into the environment in small quantities in the effluent discharged from nuclear fuel cycle facilities. They are also released into the environment following their use in unsealed form for medical and industrial applications. They are also found in the water as a result of past fallout contamination resulting from the explosion in the atmosphere of nuclear devices and accidents such as those that occurred in Chernobyl and Fukushima.

Drinking water can thus contain radionuclides at activity concentration which could present a risk to human health. In order to assess the quality of drinking water (including mineral waters and spring waters) with respect to its radionuclide content and to provide guidance on reducing health risks by taking measures to decrease radionuclide activity concentrations, water resources (groundwater, river, lake, sea, etc.) and drinking water are monitored for their radioactivity content as recommended by the World Health Organization (WHO) and can be required by some national authorities.

The need of a standard on a test method of radium-226 activity concentrations in water samples is justified for test laboratories carrying out these measurements, required sometimes by national authorities, as they may have to obtain a specific accreditation for radionuclide measurement in drinking water samples.

Radium-226 activity concentration can vary widely according to local geological and climatic characteristics and ranges from $0.001~Bq\cdot l^{-1}$ in surface waters up to $50~Bq\cdot l^{-1}$ in natural groundwaters; the guidance level for radium 226 in drinking water as recommended by WHO is $1~Bq\cdot l^{-1}$ (see Reference [13]).

NOTE The guidance level is the activity concentration (rounded to the nearest order of magnitude) with an intake of $2 \cdot 1 \cdot d^{-1}$ of drinking water for 1 year that results in an effective dose of 0,1 mSv·y⁻¹ for members of the public, an effective dose that represents a very low level of risk that is not expected to give rise to any detectable adverse health effect.

This International Standard is one of a series on determination of the activity concentration of radionuclides in water samples.

Water quality — Radium-226 —

Part 3:

Test method using coprecipitation and gammaspectrometry

WARNING — Persons using this part of ISO 13165 should be familiar with normal laboratory practice. This part of ISO 13165 does not purport to address all of the safety problems, if any, associated with its use. It is the responsibility of the user to establish appropriate safety and health practices and to ensure compliance with any national regulatory conditions.

IMPORTANT — It is absolutely essential that tests conducted in accordance with this part of ISO 13165 be carried out by suitably qualified staff.

1 Scope

This part of ISO 13165 specifies the determination of radium-226 (²²⁶Ra) activity concentration in all types of water by coprecipitation followed by gamma-spectrometry (see ISO 18589-3).

The method described is suitable for determination of soluble 226 Ra activity concentrations greater than 0,02 Bq l⁻¹ using a sample volume of 1 l to 100 l of any water type.

For water samples smaller than a volume of 1 l, direct gamma-spectrometry can be performed following ISO 10703 with a higher detection limit.

NOTE This test method also allows other isotopes of radium, ²²³Ra, ²²⁴Ra, and ²²⁸Ra, to be determined.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 5667-3, Water quality — Sampling — Part 3: Preservation and handling of water samples

ISO 10703, Water quality — Determination of the activity concentration of radionuclides — Method by high resolution gamma-ray spectrometry

ISO 11929, Determination of the characteristic limits (decision threshold, detection limit and limits of the confidence interval) for measurements of ionizing radiation — Fundamentals and application

ISO/IEC 17025, General requirements for the competence of testing and calibration laboratories

ISO 80000-10, Quantities and units — Part 10: Atomic and nuclear physics

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 80000-10 and the following apply.

BS ISO 13165-3:2016 **ISO 13165-3:2016(E)**

3.1

activity

number of spontaneous nuclear disintegrations occurring in a given quantity of material during a suitably small interval of time divided by that interval of time

[SOURCE: ISO 921:1997, 23]

3.2

reference standard

standard, generally having the highest metrological quality available at a given location or in a given organisation, from which measurements made there are derived

3.3

working standard

standard which, usually calibrated against a *reference standard* (3.2), is used routinely to calibrate or check material measures, measuring instruments or reference materials. It can be used as a solution of known *activity* (3.1) concentration obtained by precise dilution or dissolution of a reference standard

4 Symbols

For the purposes of this part of ISO 13165, the symbols defined in ISO 11929 and ISO 80000-10, and the following apply.

Table 1 — List of symbols

V	Volume of the test sample in litres
A	Activity of each radionuclide in calibration source, at the calibration time, in becquerels
c_A, c_{Ac}	Activity concentration of ²²⁶ Ra, without and with corrections, expressed in becquerels per litre
$M_{sulfate}$	Mass of barium sulfate, in grams
$M_{ m nitrate}$	Mass of barium nitrate, in grams
M _{carbonate}	Mass of barium carbonate, in grams
t_g	Sample spectrum counting time, in seconds
t_0	Background spectrum counting time, in seconds
t_{s}	Calibration spectrum counting time, in seconds
n_N, n_{N0}, n_{Ns}	Number of counts in the net area of the peak considered, at energy $\it E$, in the sample, background and calibration spectra, respectively
n_g , n_{g0} , n_{gs}	Number of counts in the gross area of the peak considered, at energy E , in the sample, background and calibration spectra, respectively
n_b, n_{b0}, n_{bs}	Number of counts in the background of the peak considered, at energy $\it E$, in the sample, background and calibration spectra, respectively
ε	Efficiency of the detector at energy <i>E</i> , at actual measurement geometry
$R_{\mathcal{C}}$	Chemical yield
P	Probability of the emission of a gamma ray with energy, E , of each radionuclide, per decay, i.e. the branching ratio or the number of γ -quanta per decay
$u(c_A)$	Standard uncertainty of activity concentration, in becquerels per litre
u(x)	Standard uncertainty of measurand x
$u_{\rm rel}(x)$	Relative uncertainty: $u(x)/x$
U	Expanded uncertainty calculated by $U = k u(c_A)$ with k usually equals 2, in becquerels per litre
c_A^*	Decision threshold, in becquerels per litre

Table 1 (continued)

$c_A^{\#}$	Detection limit, in becquerels per litre
$C_A^{\triangleleft}, C_A^{\triangleright}$	Lower and upper confidence limits, of each radionuclide, in becquerels per litre

5 Principle of the measurement

Measurement of ²²⁶Ra activity concentration in water is carried out in two separate steps: a sample preparation step, followed by a measurement by gamma-spectrometry.[13][14][15]

The sample preparation consists of a filtration of the water sample (see ISO 5667-3) to ensure the measurement of the activity concentration of the ²²⁶Ra soluble fraction. The filtration is followed by a pre-concentration, coprecipitation, and accumulation of decay products of ²²⁶Ra.

After filtration and acidification of the water sample, the ²²⁶Ra is coprecipitated into sulfate using a carrier such as barium nitrate or carbonate. The radium and barium sulfates are then washed, dried, and weighed. The chemical yield is obtained gravimetrically.

For water samples that may have an existing concentration of soluble barium, another tracer should be used to avoid a chemical yield above $100\,\%$.

When a radiometric tracer, such as 133 Ba is used as an internal standard to assess the recovery yield, then this recovery yield is used instead of R_c in the Formulae (2) and (4).

The ²²⁶Ra activity concentration of the precipitate is measured by gamma-spectrometry using a high purity germanium detector with low system background.

The presence of other gamma emitters, such as 235 U, in the precipitate can interfere with the quantification of 226 Ra activity.

The assessment of the soluble 226 Ra activity concentration is carried out by the measurement of its decay products, 214 Pb and 214 Bi, at equilibrium reached four weeks after the last coprecipitation step.

6 Reagents and equipment

6.1 Reagents

Unless otherwise stated, use only reagents of recognized analytical grade and distilled or demineralized water or water of equivalent purity and no undesirable radioactivity.

- **6.1.1** Concentrated nitric acid solution (HNO₃), 65 % or 69 %.
- **6.1.2** Nitric acid solution (HNO₃), diluted to 2,28 %.
- **6.1.3** Nitric acid solution (HNO₃), diluted to 18 %.
- **6.1.4** Carrier solution, $10.0 \text{ g} \cdot l^{-1} \cdot Ba^{2+}$.

Slowly dissolve barium nitrate $Ba(NO_3)_2$ (19,0 g) or barium carbonate $BaCO_3$ (14,3 g) in one litre of nitric acid solution (6.1.2). The salt mass shall be weighed accurately (better than 1 %) and recorded.

It is recommended to use a $Ba(NO_3)_2$ or $BaCO_3$ reagent with a low ^{226}Ra activity concentration. The presence of ^{226}Ra in the reagent shall be controlled using a blank sample prepared with distilled or demineralized water.

- 6.1.5 Concentrated sulfuric acid solution (H₂SO₄), 98 %.
- **6.1.6** Cellulose ester filter of porosity, 0,45 μm.

6.2 Equipment

Usual laboratory equipment and, in particular, the following:

- 6.2.1 Peristaltic or membrane pump.
- 6.2.2 Magnetic bar stirrer.
- 6.2.3 Centrifuge and tubes.
- 6.2.4 Precision balance.
- 6.2.5 Drying oven.
- 6.2.6 Gas-tight container.
- **6.2.7 Gamma-spectrometry system**, with low background capability.

7 Sampling

The method can be used on water samples up to 100 l.

7.1 Sample collection

The sampling conditions shall comply with ISO 5667-3.

If required, the filtration is carried out during or immediately after collection and before acidification, otherwise, radioactive material already adsorbed onto the suspended particulate material can be desorbed.

It is recommended that plastic single-use type containers are used for sample collection.

The volume of the water sample to collect for measurement depends on the detection limits required by the customer.

7.2 Sample transport and storage

The water sample shall be transported and stored according to ISO 5667-3.

When pre-concentration is desired, acidify the sample to between pH 1 and pH 3 with HNO₃. Acidification of the water sample minimizes the loss of radioactive material from solution by adsorption.

The test shall be performed as soon as possible.

8 Procedures

8.1 Blank sample preparation

Prepare a blank with distilled or demineralized water by performing the operations described in step a) to i) in 8.2.

8.2 Sample preparation

- a) To prevent adsorption effects and proliferation of algae, the water sample is acidified to pH 1 with nitric acid (see <u>6.1.1</u>). The water sample volume can be 1 l to 100 l. Acidification of the sample shall not be performed with hydrochloric acid as barium sulfate is partially soluble in it.
- b) Pour dropwise, precisely, 50 ml of carrier solution (see <u>6.1.4</u>) into the solution to be analysed, with vigorous stirring. In the case of natural water rich in sulfate ions, such as seawater, the barium and radium have to be mixed before the sulfate is precipitated.
- c) Add 20 ml of concentrated H_2SO_4 (see <u>6.1.5</u>) to precipitate the sulfate.
- d) Stop mixing.
- e) Leave the barium radium sulfate precipitate Ba(Ra)SO₄ to settle for about 24 h.
- f) Separate most of the supernatant, e.g. using the pump, and centrifuge the remainder at about 2 000 rpm for about 5 min or filter to recover the precipitate.
- g) Wash the precipitate with nitric acid (see <u>6.1.3</u>) in the centrifuge tube, shake, and centrifuge again. Repeat steps f) and g) two times.
- h) Eliminate the supernatant.
- i) Rinse the precipitate with water (e.g. shaking and centrifuging each time).
- j) Dry the precipitate in an oven at 105 °C for at least 24 h.
- k) Weigh a gas-tight container.
- l) Place the precipitate in the weighed gas-tight container and tightly seal to prevent any loss of radon (see ISO 18589-3).
- m) Weigh the container.

8.3 Counting procedure

 226 Ra activity is assessed by gamma-spectrometry using the detection of emissions of 214 Pb and/or 214 Bi following an ingrowth period of approximately 4 weeks, during which, 222 Rn reaches secular equilibrium with 226 Ra (see ISO 18589-3).

Calibration shall be performed using the same geometry as the one used to count the sample precipitate.

In the case of counting before the equilibrium is reached, a correction for the subsequent accumulation of the decay products has to be applied.

The 226 Ra activity concentration can be determined directly from its own energy emission at 186 keV, without the need for decay products ingrowth. The disadvantages of this technique relate primarily in that the emission probability of this gamma photopeak is weak (3,28 %), and furthermore by the presence of the interfering primary gamma emission of 235 U at 185,7 eV that has a higher emission probability of 57,24 %. Assuming the equilibrium between 226 Ra and 214 Bi, the theoretical detection limit of 226 Ra can be improved using the energy line of 214 Bi at 609 keV to measure the 226 Ra activity.

9 Quality assurance and quality control programme

9.1 General

Quality control operations shall meet the requirements of ISO/IEC 17025 and ISO 10703.

9.2 Influence quantities

Special precautions shall be taken to minimize the influence of quantities that can affect the measurement results:

- loss of ²²²Rn from the container to be measured:
- 226Ra present in a Ba(NO₃)₂ or BaCO₃ reagent. The presence of ²²⁶Ra in reagent shall be assessed by measuring a blank sample;
- wide temporal variations of the radon activity concentration can be observed in the atmosphere of the laboratory. The continuous monitoring of the ²²²Rn activity concentration in the laboratory using a radon measuring device is recommended, since even in well-ventilated rooms, considerable variations are possible in special weather conditions (see ISO 11665-1 and ISO 11665-5);
- to maintain a constant temperature and relative humidity, the air should be continuously renewed through an air-conditioning system. In order to limit the release of radon from material within the walls, the walls of the laboratory should be painted with a suitable material such as epoxy paint.

A case may be added around the detector and filled with a radon-free gas (e.g. N_2 , air passed through a granulated activated charcoal filter) in order to prevent any accumulation of radon in the vicinity of the detector.

9.3 Instrument verification

Major instrument parameters (energy calibration, efficiency calibration as a function of energy, and background spectrum) shall be periodically checked within a quality assurance programme established by the laboratory and following the manufacturer's instructions (see ISO 10703).

9.4 Method verification

Periodical verifications of the accuracy of the method shall be run. These may be accomplished by the following:

- participating in intercomparison exercises;
- analysing reference materials.

Method repeatability shall also be checked, e.g. by replicate measurements.

The acceptance limits of the tests mentioned in the preceding shall be defined.

9.5 Demonstration of analyst capability

If an analyst has not used this procedure before, a precision and bias test shall be performed by running a duplicate measurement of a reference or spiked material. Acceptance limits shall be defined by the laboratory.

A similar test shall be performed by analysts routinely using this procedure with a periodicity defined by the laboratory. Acceptance limits shall be defined.

10 Expression of results

10.1 General

Except for the chemical yield, R_C , computation for the activity concentration is developed in ISO 10703, and in this clause, only final formulae are presented.

10.2 Water-soluble ²²⁶Ra activity concentration

The activity concentration measured by gamma-spectrometry, expressed in Bq·l⁻¹, has to be corrected for the barium sulfate or other precipitation yield (R_C) determination.

This yield is the ratio of the mass of separated barium sulfate to the mass of barium nitrate or barium carbonate introduced:

$$R_C = \frac{M_{\text{sulfate}}}{M_{\text{nitrate}}} \times 0,893 \text{ or } R_C = \frac{M_{\text{sulfate}}}{M_{\text{carbonate}}} \times 1,18$$
 (1)

where 0,893 and 1,18 are the molar mass ratios.

Thus, for an undisturbed peak at an energy, E, the activity concentration measured by gamma-spectroscopy is expressed in Bq·l⁻¹ as shown in Formula (2):

$$c_A = \frac{n_g - n_b}{P \cdot \varepsilon \cdot V \cdot R_C \cdot t_g} = (n_g - n_b) \cdot w / t_g \text{ with } w = \frac{1}{P \cdot \varepsilon \cdot V \cdot R_C}$$
 (2)

where ε is given by the calibration curve in the measurement set-up (see ISO 10703).

It should be considered that for the purpose of this part of ISO 13165, the correction factor, f_E , that appears in ISO 10703, is taken equal to 1 and the radiochemical yield, R_C , is taken into account.

10.3 Standard uncertainty of activity concentration

According to the *Guide to the Expression of Uncertainty in Measurement* [9], the combined uncertainty of c_A is calculated by Formula (3):

$$u(c_A) = \sqrt{(w/t_g)^2 \cdot (u^2(n_g) + u^2(n_b)) + c_A^2 \cdot u_{\text{rel}}^2(w)}$$
(3)

where the standard uncertainty of the counting time is neglected, and the relative standard uncertainty of *w* is calculated by Formula (4):

$$u_{\rm rel}^{2}(w) = u_{\rm rel}^{2}(P) + u_{\rm rel}^{2}(V) + u_{\rm rel}^{2}(\varepsilon) + u_{\rm rel}^{2}(R_{C})$$
(4)

Details about the calculation of $u_{\rm rel}^2(\varepsilon)$ can be found in ISO 10703.

10.4 Decision threshold

In accordance with ISO 11929, the decision threshold, c_A^* , is obtained from the Formula (3) for $c_A = 0$. This yields the following:

$$c_A^* = k_{1-\alpha} \cdot w \cdot \sqrt{2} \cdot u(n_b) / t_a \tag{5}$$

where $\alpha = 0.05$ and then, $k_{1-\alpha} = 1.65$ is often chosen by default.

10.5 Detection limit

The detection limit, $c_A^\#$, is calculated according to ISO 11929 using the implicit Formula (6):

$$c_{A}^{\#} = c_{A}^{*} + k_{1-\beta} \cdot \sqrt{w^{2} \left[\left(c_{A}^{\#} / w + n_{b} / t_{g} \right) / t_{g} + u^{2}(n_{b}) / t_{g}^{2} \right) + c_{A}^{\#2} \cdot u_{\text{rel}}^{2}(w) }$$
 (6)

where $\beta = 0.05$ and then, $k_{1-\beta} = 1.65$ is often chosen by default.

The detection limit can be calculated by solving Formula (6) for $c_A^\#$ or, more simply, by iteration with a starting approximation, $c_A^\# = 2 \cdot c_A^*$.

When taking $k_{1-\alpha}=k_{1-\beta}=k$, the solution of Formula (6) is given by Formula (7):

$$c_A^{\#} = \frac{2c_A^{*} + (k^2 \cdot w) / t_g}{1 - k^2 u_{\text{rel}}^2(w)}$$
(7)

10.6 Limits of the confidence interval

The lower, $C_A^{\ }$, and upper, $C_A^{\ }$, limits of the confidence interval are calculated using the following formulae (see ISO 11929):

$$C_A^{\ \ } = C_A - k_p \cdot u(C_A)$$
, $p = \omega \cdot (1 - \gamma/2)$ (8)

$$C_A^{\ \ } = C_A + k_a \cdot u(C_A)$$
, $q = 1 - \omega \cdot \gamma/2$ (9)

where

 $\omega=\Phi\left[y\Big/u\Big(y\Big)\right]$, Φ being the distribution function of the standardized normal distribution;

 $\omega=1$ may be set if $C_A\geq 4\times u\left(C_A\right)$. In this case,

$$C_A^{\triangleleft \triangleright} = C_A \pm k_{1-\gamma/2} \cdot u(C_A)$$

where $\gamma = 0.05$ with $k_{1-\gamma/2} = 1.96$ are often chosen by default.

10.7 Corrections for contributions from other radionuclides and background

10.7.1 General

If the determination of soluble 226 Ra activity concentration is determined directly from the gamma ray emissions of the 226 Ra, other gamma emitters such as 235 U can interfere. In this case, the contributing radionuclide has another gamma line from which the contribution to the line in question can be estimated, taking into account the branching ratios of the gamma lines.

If the determination of soluble 226 Ra activity concentration is estimated by the measurement of its decay products 214 Pb and 214 Bi at equilibrium, reached four weeks after the coprecipitation step, it should be taken into account that the gamma line of the radionuclide to be determined occurs also in the background of the spectrometer. By measuring a background spectrum without a sample for a counting time, t_0 , this contribution can be corrected for, taking into account the different counting times of the two spectra.

For both cases, the activity concentration can be calculated using a model according to Formula (10):

$$c_{Ac} = (n_N / t_q - x \cdot n_{N0} / t_0) \cdot w \tag{10}$$

For the both cases of contribution, this model gives the necessary corrections, which are developed in ISO 10703.

10.7.2 Contribution from other radionuclides

The gamma line to be corrected at the energy, E_1 , has the net peak area n_{N,E_1} . The contribution of another radionuclide having more than one gamma line at gamma energy, E_1 , is calculated through the ratio of the respective emission probability, deducted from the gamma line, E_2 . Using Formula (10) with $x=P_{E_1}/P_{E_2}$ and $t_0=t_g$, this yields to:

$$c_{Ac} = (n_{N,E_1} - x \cdot n_{N,E_2}) \cdot w / t_g$$
 (11)

Neglecting the standard uncertainty of x, the standard uncertainty of c_{Ac} is calculated by Formula (12):

$$u^{2}(c_{Ac}) = (w / t_{g})^{2} \left\{ n_{g,E_{1}} + u^{2}(n_{b,E_{1}}) + x^{2} \left[n_{g,E_{2}} + u^{2}(n_{b,E_{2}}) \right] \right\} + c_{Ac}^{2} \cdot u_{\text{rel}}^{2}(w)$$
(12)

The decision threshold, c_{Ac}^* , is given by Formula (13):

$$c_{Ac}^{*} = k_{1-\alpha} \cdot (w / t_g) \cdot \sqrt{n_{b,E_1} + u^2(n_{b,E_1}) + x(n_{g,E_2} - n_{b,E_2}) + x^2[n_{g,E_2} + u^2(n_{b,E_2})]}$$
 (13)

and the detection limit, $c_{Ac}^{\#}$, by Formula (14):

$$c_{Ac}^{\#} = c_{Ac}^{*} + k_{1-\beta} \sqrt{(w/t_{g})^{2} (c_{Ac}^{\#}t_{g}/w + n_{b,E_{1}} + u^{2}(n_{b,E_{1}}) + x(n_{g,E_{2}} - n_{b,E_{2}}) + x^{2} [n_{g,E_{2}} + u^{2}(n_{b,E_{2}})]) + c_{Ac}^{\#2} u_{\mathrm{rel}}^{2}(w)}$$
(14)

The detection limit can be calculated by solving Formula (14) for $c_{Ac}^{\#}$ or, more simply, by iteration with a starting approximation: $c_{Ac}^{\#}=2\cdot c_{Ac}^{*}$.

When taking $k_{1-\alpha} = k_{1-\beta} = k$, the solution of Formula (14) is given by Formula (15):

$$c_{Ac}^{\#} = \frac{2 \cdot c_{Ac}^{*} + \left(k^{2} \cdot w\right) / t_{g}}{1 - k^{2} \cdot u_{rel}(w)}$$
(15)

10.7.3 Contribution from background

In this case, Formula (10) is used for the correction with x = 1 and u(x) = 0. n_{N0} is the net peak area of the gamma line in the background spectrum and t_0 the counting time of the background spectrum. This yields:

$$c_{AC} = (n_N / t_a - n_{N0} / t_0) \cdot w \tag{16}$$

The standard uncertainty of c_{AC} is calculated by Formula (17):

$$u^{2}(c_{Ac}) = w^{2}(n_{g}/t_{g}^{2} + n_{g0}/t_{0}^{2} + u^{2}(n_{b})/t_{g}^{2} + u^{2}(n_{b0})/t_{0}^{2}) + c_{Ac}^{2} \cdot u_{rel}^{2}(w)$$
(17)

The decision threshold, c_{Ac}^{*} , is given by Formula (18):

$$c_{Ac}^{*} = k_{1-\alpha} \cdot w \cdot \sqrt{\left[n_b + u^2(n_b)\right] / t_g^2 + \left[n_{g0} + u^2(n_{b0})\right] / t_0^2 + \left(n_{g0} - n_{b0}\right) / t_0 t_g}$$
 (18)

and the detection limit, $c_{Ac}^{\#}$, by Formula (19):

$$c_{Ac}^{\#} = c_{Ac}^{*} + k_{1-\beta} \sqrt{w^{2} \left[\frac{c_{Ac}^{\#}}{t_{g}w} + (n_{b} + u^{2}(n_{b}))\right]/t_{g}^{2} + \left[n_{g0} + u^{2}(n_{b0})\right]/t_{0}^{2} + (n_{g0} - n_{b0})/t_{0}t_{g}) + c_{Ac}^{\#2}u_{rel}^{2}(w)}}$$
(19)

The detection limit can be calculated by solving Formula (19) for $c_{Ac}^{\#}$ or, more simply, by iteration with a starting approximation: $c_{Ac}^{\#} = 2 \cdot c_{Ac}^{*}$.

When taking $k_{1-\alpha} = k_{1-\beta} = k$, the solution of Formula (19) is given by Formula (20):

$$c_{Ac}^{\#} = \frac{2 \cdot c_{Ac}^{*} + \left(k^{2} \cdot w\right) / t_{g}}{1 - k^{2} \cdot u_{\text{rel}}^{2}\left(w\right)}$$
(20)

The limits of the confidence interval are calculated according to Formulae (8) and (9).

11 Expression of results

This test report shall meet the requirements of ISO/IEC 17025 and shall contain at least the following information:

- a) the test method used, together with a reference to this part of ISO 13165, i.e. ISO 13165-3:2016;
- b) a reference to the measuring and evaluation procedure implemented;
- c) the identification of the sample;
- d) the measurement date;
- e) the units in which the results are expressed;
- f) the test result, ${\it C}_A \pm u \left({\it C}_A\right)$ or ${\it C}_A \pm U$, with the associated k value and reference date.

Complementary information can be provided, such as the following:

— probabilities: α , β , and $(1 - \gamma)$;

- the decision threshold and the detection limit; depending on the customer request, the following are the different ways to present the result:
 - when the 226 Ra activity concentration is compared with the decision threshold (see ISO 11929), the result of the measurement shall be expressed as $\leq c_A^*$ when the result is below the decision threshold;
 - when the ²²⁶Ra activity concentration is compared with the detection limit, the result of the measurement can be expressed as when the result is below the detection limit. If the detection limit exceeds the guideline value, it shall be documented that the method is not suitable for the measurement purpose;
- mention of any relevant information likely to affect the results.

The test report can be completed by any useful information according to ISO/IEC 17025.

Annex A (informative)

Uranium and its decay chain

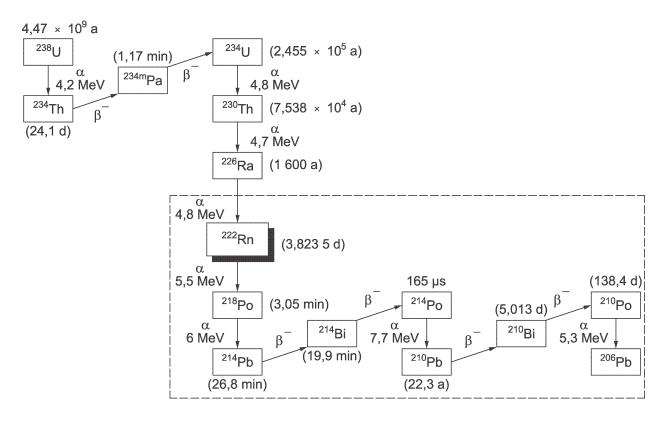


Figure A.1 — Uranium and its decay chain [16]

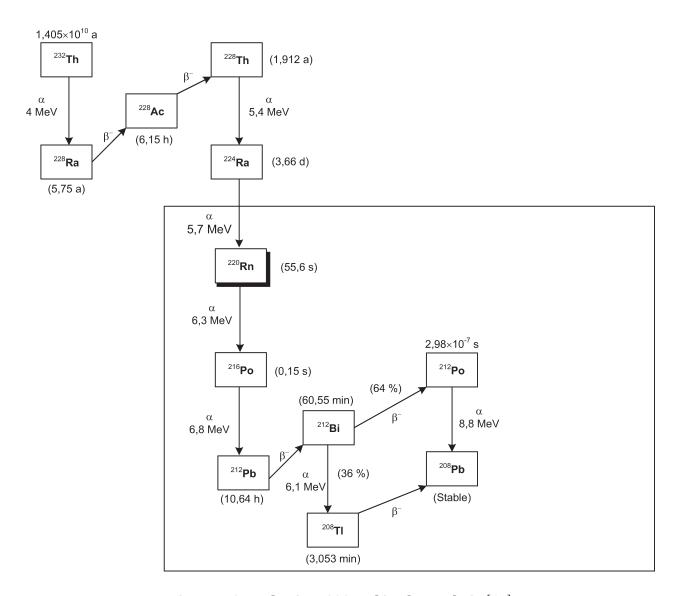



Figure A.2 — Thorium 232 and its decay chain $[\underline{16}]$

Bibliography

- [1] ISO 31-91), Quantities and units Part 9: Atomic and nuclear physics
- [2] ISO 921:1997²), Nuclear energy Vocabulary
- [3] ISO 3696, Water for analytical laboratory use Specification and test methods
- [4] ISO 5667-1, Water quality Sampling Part 1: Guidance on the design of sampling programmes and sampling techniques
- [5] ISO 6107-2, Water quality Vocabulary Part 2
- [6] ISO 11665-1, Measurement of radioactivity in the environment Air: radon-222 Part 1: Origins of radon and its short-lived decay products and associated measurement methods
- [7] ISO 11665-5, Measurement of radioactivity in the environment Air: radon-222 Part 5: Continuous measurement method of the activity concentration
- [8] ISO 18589-3, Measurement of radioactivity in the environment Soil Part 3: Test method of gamma-emitting radionuclides using gamma-ray spectrometry
- [9] ISO/IEC Guide 98-3, Uncertainty of measurement Part 3: Guide to the expression of uncertainty in measurement (GUM:1995)
- [10] European cooperation for accreditation of laboratories. *Traceability of Measuring and Test Equipment to National Standards.* EAL-G12, 1995
- [11] QUANLU G., & HENGDE W. Sources and protection measures for indoor radon. *Radiat. Prot. Dosimetry.* 1998, **76** pp. 261–266
- [12] WHO. *Guidelines for drinking-water quality,* 4th edition. Geneva: World Health Organization. 2011. 541 p. Available (viewed 2012-12-10) at: http://www/who.int/water_sanitation_health/publications/2011/dwg_chapters/en/index.html
- [13] IAEA. Analytical Methodology for the Determination of Radium Isotopes in Environmental Samples. No. IAEA/AQ/19, Vienna, 2010
- [14] SCHMIDT S., & REYSS J-L. Radium as internal tracer of Mediterranean Outflow Water. *J. Geophys. Res.* 1996 February 15, **101** (C2) pp. 3589–3596
- [15] REYSS J-L., SCHMIDT S., LEGELEUX F., BONTE P. Large, low background welltype detectors for measurements of environmental radioactivity. *Nucl. Inst. Meth.* A. 1995, **357** pp. 391–397
- [16] Nuclear Data Base issued from the Decay Data Evaluation Project. http://www.nucleide.org/DDEP_WG/DDEPdata.htm

¹⁾ Withdrawn. Replaced by ISO 80000-10.

²⁾ Withdrawn standard.





British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards -based solutions

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com
Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070 Email: copyright@bsigroup.com

