

BS ISO 13314:2011



BSI Standards Publication

Mechanical testing of metals — Ductility testing — Compression test for porous and cellular metals

bsi.

...making excellence a habit.™

National foreword

This British Standard is the UK implementation of ISO 13314:2011.

The UK participation in its preparation was entrusted to Technical Committee ISE/101/2, Ductility testing.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2012

ISBN 978 0 580 67814 1

ICS 77.040.10

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 January 2012.

Amendments issued since publication

Date	Text affected
------	---------------

**Mechanical testing of metals — Ductility
testing — Compression test for porous
and cellular metals**

*Essais mécaniques des métaux — Essais de ductilité — Essai de
compression des métaux poreux et cellulaires*





COPYRIGHT PROTECTED DOCUMENT

© ISO 2011

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized in any form or by any means, electronic or mechanical, including photocopying and microfilm, without permission in writing from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

Page

Foreword	iv
Introduction.....	v
1 Scope.....	1
2 Normative references.....	1
3 Terms and definitions	1
4 Principle	4
5 Apparatus.....	4
6 Test specimen.....	4
6.1 Geometry.....	4
6.2 Number of test specimens	4
6.3 Sampling of test specimen.....	4
7 Test procedure.....	5
7.1 Test temperature.....	5
7.2 Measurement of initial dimensions of test specimen.....	5
7.3 Test speed.....	5
7.4 General conduct of test	6
7.5 Preliminary test and unloading test	6
7.6 Zero point for the compressive strain.....	6
7.7 Energy absorption and energy absorption efficiency	6
8 Test report.....	7
8.1 General information	7
8.2 Optional information	7

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

International Standards are drafted in accordance with the rules given in the ISO/IEC Directives, Part 2.

The main task of technical committees is to prepare International Standards. Draft International Standards adopted by the technical committees are circulated to the member bodies for voting. Publication as an International Standard requires approval by at least 75 % of the member bodies casting a vote.

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights.

ISO 13314 was prepared by Technical Committee ISO/TC 164, *Mechanical testing of metals*, Subcommittee SC 2, *Ductility testing*.

Introduction

Porous and cellular metals have attractive properties due to their unique cell morphology. When they are used as a crush energy absorbing component of automotive machines, compressive properties are necessary for industrial design. However, the deformation behaviour of porous metals and metallic foams is quite different from conventional dense metals. Test methods for conventional metallic materials are not suitable for porous metals and metallic foams. Standardization of a test method for porous metals and metallic foams is required.

Mechanical testing of metals — Ductility testing — Compression test for porous and cellular metals

1 Scope

This International Standard specifies a test method for compressive properties of porous and cellular metals with a porosity of 50 % or more. Compressive tests can be carried out at ambient temperature under quasi-static strain rate conditions.

2 Normative references

The following referenced documents are indispensable for the application of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 7500-1, *Metallic materials — Verification of static uniaxial testing machines — Part 1: Tension/compression testing machines — Verification and calibration of the force-measuring system*

ISO 9513, *Metallic materials — Calibration of extensometers used in uniaxial testing*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

3.1 compressive stress

σ

compressive force divided by the initial cross-sectional area perpendicular to the loading direction

NOTE Compressive stress is expressed in newtons per square millimetre.

3.2 compressive strain

e

overall compressive displacement divided by the initial height (gauge length) of the test specimen

NOTE Compressive strain is expressed as a percentage.

3.3 first maximum compressive strength

compressive stress corresponding to the first local maximum in the stress-strain curve

See Figure 1.

NOTE It cannot be determined if no local maximum occurs.

3.4 plateau stress

σ_{pl}
arithmetical mean of the stresses at 0,1 % or smaller strain intervals between 20 % and 30 % or 20 % and 40 % compressive strain

See Figure 1.

NOTE The strain range/interval, 20 % and 30 % or 20 % and 40 %, for arithmetical mean varies depending on the plateau end strain.

3.5 plateau end point in the stress-strain curve at which the stress is 1,3 times the plateau stress

See Figure 1.

NOTE If this point does not adequately represent the end of the plateau range, another stress can be selected which corresponds to the curve trace (see 7.4).

3.6 energy absorption

W
area under the stress-strain curve up to 50 % strain or up to the plateau end strain, e_{ple}

NOTE The energy absorption up to other strain values can also be determined (see 7.7).

3.7 energy absorption efficiency

W_e
energy absorption divided by the product of the maximum compressive stress within the strain range and the magnitude of the strain range

3.8 quasi-elastic gradient

gradient of the straight line determined within the linear deformation region at the beginning of the compressive stress-strain curve

NOTE This gradient is not a modulus for the material (see Figure 1). The quasi-elastic gradient is optionally measured and it is used to determine the zero point for the compressive strain [see Figure 2 a)].

3.9 compressive offset stress

compressive stress at the plastic compressive strain of 0,2 %, unless otherwise specified or recorded

NOTE The plastic strain is determined using of the quasi-elastic gradient [see Figure 2 a)]. The compressive 0,2 % offset stress is optionally measured and it can be used as an alternative to the compressive yield strength.

3.10 elastic gradient

gradient of the elastic straight lines determined by elastic loading and unloading between stresses of σ_{70} and σ_{20}

NOTE 1 σ_{70} and σ_{20} correspond to 70 % and 20 %, respectively, of the plateau stress, σ_{pl} .


NOTE 2 The elastic straight line is the secant line obtained from the hysteresis loop which occurs during unloading and subsequent loading (see Figure 1). The elastic gradient represents a porosity-dependent rigidity, not a modulus of the material, and generally changes during the course of compression. The elastic gradient is optionally measured and it is used to determine the zero point for the compressive strain [see Figure 2 b)].

3.11

compressive proof strength

compressive stress at a plastic compressive strain of 1,0 %, unless otherwise specified or recorded


NOTE The plastic strain is determined using of the elastic gradient [see Figure 2 b)]. The compressive proof strength is optionally measured and it can be used as an alternative to the compressive yield strength.

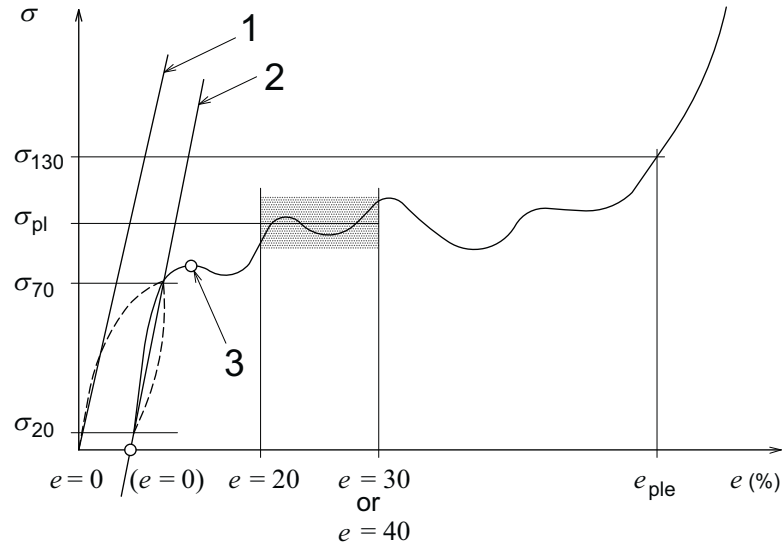

Key

- 1 quasi-elastic gradient
- 2 elastic gradient
- 3 first maximum compressive strength


Figure 1 — Stress-strain curve to determine the characteristic values from compression testing of porous and cellular metals

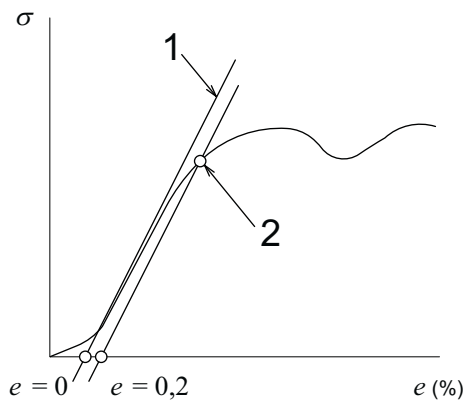

Key

- 1 quasi-elastic gradient
- 2 compressive offset stress

a) Quasi-elastic gradient and compressive offset stress

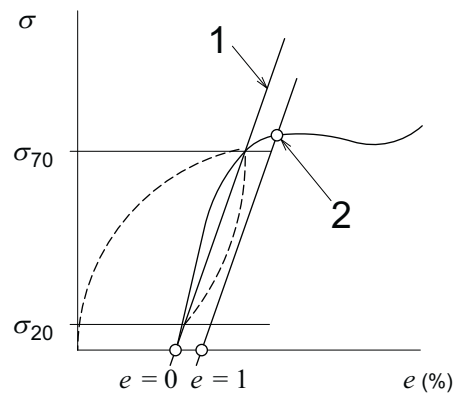

Key

- 1 elastic gradient
- 2 compressive proof strength

b) Elastic gradient and compressive proof strength

Figure 2 — Stress-strain curve to determine the optional characteristic values from compression testing of porous and cellular metals

4 Principle

This test is a method for evaluating compressive properties of porous and cellular metals. The compressive test is carried out using a compression test machine with constant crosshead speed. Compressive stress, σ , and compressive strain, e , are measured from the applied force, F , and displacement of the compressive specimen, respectively.

5 Apparatus

5.1 Test machine, conforming to ISO 7500-1. The machine shall be able to test at constant crosshead speed. Unless otherwise agreed between the parties, a machine of class 1 shall be used for this test.

5.2 Pressing device, consisting of a couple of polished parallel platens, used to apply compressive force to the test specimen. The platens' geometry shall be such that the centres of the upper and lower platens can be aligned to the centre line of the machine casing. Plane-ground, mirror-finished platens with a minimum hardness of at least 60 HRC shall be used. Lubricant may be applied to press surfaces.

5.3 Device for the measurement of compressive strain, consisting of an extensometer or calculated from the measured displacement between two parallel platens.

For the measurement of the elastic gradient and the compressive proof strength, an extensometer mounted on the platens or directly on the respective sample shall be used to measure the compressive strain. Alternatively, the measurement may be carried out using an optical extensometer. In the relevant range, the accuracy of the extensometer shall, as a minimum requirement, correspond to class 1 in accordance with ISO 9513.

6 Test specimen

6.1 Geometry

Test specimens which are cylindrical (recommended) or rectangular in cross-section shall be used in the compressive test (see Figure 3). All spatial dimensions of the specimen (W_0 and D_0 in Figure 3) shall be at least 10 times the average pore size, d_a , and no less than 10 mm, with a sample length to diameter ratio ($H_0:D_0$) or sample length to edge length ratio ($H_0:W_0$) of between 1 and 2. The sample geometry shall be recorded in the test report. The average pore size (i.e. diameter, in the case of spherical porosity, and the axial and transverse dimensions in the case of non-spherical porosity) shall be measured in the cut section and recorded in the test report. The type of porosity (i.e. open or closed) shall also be recorded.

The pore size distribution shall be checked where necessary in the case of closed-pore metal foams by cutting. The average pore size shall be measured in the cut section.

6.2 Number of test specimens

The number of test specimens shall be no less than three and a minimum of five is recommended.


In addition, for the optional measurement of elastic gradient, a specimen for a preliminary test providing an initial estimate of the plateau stress is required.

6.3 Sampling of test specimen

The test specimen shall be sampled from the material structure under test by cutting, milling, turning, electric discharge machining, etc.. Under no circumstances shall the material properties be affected by the cutting procedure.

The areas in contact with the platens during the test shall be parallel. The remaining cut surfaces shall be perpendicular to the contact surfaces. Cut surfaces shall have any burrs removed.

In the case of foamed metals, the skin, in general, is removed. If specimens with skin are used, this fact shall be recorded in the test report.

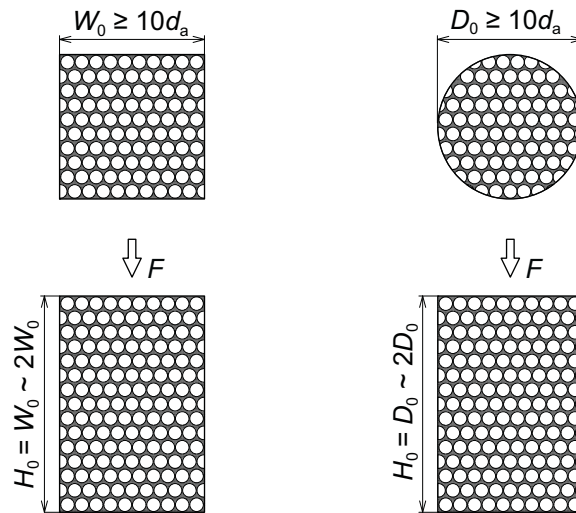

a) Rectangular specimen b) Cylindrical specimen

Key

F force

Figure 3 — Schematic illustration of test specimen

7 Test procedure

7.1 Test temperature

The compressive test shall be carried out at ambient temperature within the range of 10 °C to 35 °C, and temperature shall be recorded, if necessary. When temperature control is especially necessary, it shall be kept in the range of (23 ± 5) °C.

7.2 Measurement of initial dimensions of test specimen

The width, thickness, diameter, etc. of the test specimen shall be measured to the order of 0,1 mm, followed by calculation of the initial cross-sectional area. The height of the test specimen shall be measured to an accuracy of 0,1 mm.

Measurement at a minimum of three measuring points is recommended.

7.3 Test speed

The compression tests are conducted at a constant crosshead speed. The crosshead speed is calculated to obtain an initial compression strain rate of between 10^{-3} s^{-1} and 10^{-2} s^{-1} . The compression speed or the initial strain rate shall be recorded in the test report/record.

7.4 General conduct of test

The test specimen shall be placed between the platens of the test machine while allowing the centre line of the test specimen to coincide with the centre line of the upper and lower platens.

During the compression test, a force/displacement curve shall be recorded for each sample to determine characteristic values according to their definitions in Clause 3.

Data sampling frequency should be at least 30 Hz up to 5 % strain or the strain corresponding to compressive proof strength, whichever is the greater. The data sampling frequency may then be reduced to a minimum of 10 Hz.

If the plateau end does not adequately represent the end of the plateau range, another stress may be selected, which corresponds to the curve trace and it should be recorded in the test report.

7.5 Preliminary test and unloading test

For the optional measurement of elastic gradient, a preliminary test should be carried out to estimate the plateau stress. The plateau stress is used to determine the start and reversal point of hysteresis.

The start of hysteresis is determined at 70 % of the plateau stress; the reversal point is determined at 20 % of the plateau stress from the preliminary test.

7.6 Zero point for the compressive strain

The zero point for the compressive strain is determined as an intersection point of the straight line corresponding to the quasi-elastic gradient or the elastic gradient with the compressive strain axis (see Figure 1).

7.7 Energy absorption and energy absorption efficiency

Energy absorption, W , and energy absorption efficiency, W_e , are calculated using Formulae (1) and (2), respectively.

$$W = \frac{1}{100} \int_0^{e_0} \sigma de \quad (1)$$

$$W_e = \frac{W}{\sigma_0 \times e_0} \times 10^4 \quad (2)$$

where

W is the energy absorption per unit volume (MJ/m³);

W_e is the energy absorption efficiency (%);

σ is the compressive stress (N/mm²);

e_0 is upper limit of the compressive strain (%);

σ_0 is the compressive stress at the upper limit of the compressive strain (N/mm²).

The recommended upper limit of the compressive strain 50 % or the plateau end strain, e_{ple} (see Figure 1). Another upper limit may also be used; in this case, it shall be recorded in the test report.

8 Test report

8.1 General information

The following information shall be included in the test report:

- a) reference to this International Standard, i.e. ISO 13314:2011;
- b) nature and designation of the product being tested;
- c) material, density, porosity, type of porosity (open or closed) and average pore size (diameter, if spherical; axial and transverse dimensions, if nonspherical) of the sample;
- d) dimensions of the test specimens, giving the ratio of length to diameter or length to edge length;
- e) number of test specimens;
- f) test conditions (temperature, lubrication);
- g) compression speed in metres per second [compressive strain rate (s^{-1})];
- h) test results for:
 - 1) plateau stress (indicating the strain range used for determination, e.g. 20 % to 30 %);
 - 2) first maximum compressive strength, if applicable;
 - 3) plateau end strain (indicating the method used for determination);
 - 4) energy absorption (indicating the upper strain for determination, e.g. 50 %);
 - 5) energy absorption efficiency;
 - 6) stress-strain diagrams.

8.2 Optional information

The following optional information may be included in the test report:

- a) type of test machine and measuring range of the measuring equipment;
- b) sample preparation method;
- c) test results for:
 - 1) quasi-elastic gradient;
 - 2) compressive offset stress;
 - 3) elastic gradient;
 - 4) compressive proof strength;
- d) statistics of the quantities measured.

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com



...making excellence a habit.™