



BSI Standards Publication

Implants for surgery — Wear of total hip-joint prostheses

Part 1: Loading and displacement parameters for wear-testing machines and corresponding environmental conditions for test

National foreword

This British Standard is the UK implementation of ISO 14242-1:2014. It supersedes BS ISO 14242-1:2002 which is withdrawn.

The UK participation in its preparation was entrusted to Technical Committee CH/150/4, Surgical Implants - Bone and Joint Replacements.

A list of organizations represented on this committee can be obtained on request to its secretary.

This publication does not purport to include all the necessary provisions of a contract. Users are responsible for its correct application.

© The British Standards Institution 2014. Published by BSI Standards Limited 2014

ISBN 978 0 580 82475 3

ICS 11.040.40

Compliance with a British Standard cannot confer immunity from legal obligations.

This British Standard was published under the authority of the Standards Policy and Strategy Committee on 31 October 2014.

Amendments issued since publication

Date	Text affected
------	---------------

INTERNATIONAL
STANDARD

ISO
14242-1

Third edition
2014-10-15

**Implants for surgery — Wear of total
hip-joint prostheses —**

Part 1:
**Loading and displacement parameters
for wear-testing machines and
corresponding environmental
conditions for test**

*Implants chirurgicaux — Usure des prothèses totales de l'articulation
de la hanche —*

*Partie 1: Paramètres de charge et de déplacement pour machines
d'essai d'usure et conditions environnementales correspondantes d'essai*



Reference number
ISO 14242-1:2014(E)

© ISO 2014



COPYRIGHT PROTECTED DOCUMENT

© ISO 2014

All rights reserved. Unless otherwise specified, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
Case postale 56 • CH-1211 Geneva 20
Tel. + 41 22 749 01 11
Fax + 41 22 749 09 47
E-mail copyright@iso.org
Web www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Principle	2
5 Test and control specimens and test fluid	2
6 Apparatus	2
7 Procedure	6
8 Test report	7
9 Disposal of test specimen	8
Annex A (informative) Generation of rotation and load curves by formulae	9

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation on the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the WTO principles in the Technical Barriers to Trade (TBT) see the following URL: [Foreword - Supplementary information](#)

The committee responsible for this document is ISO/TC 150, *Implants for surgery*, Subcommittee SC 4, *Bone and joint replacements*.

This third edition cancels and replaces the second edition (ISO 14242-1:2012), which has been technically revised.

ISO 14242 consists of the following parts, under the general title *Implants for surgery — Wear of total hip-joint prostheses*:

- *Part 1: Loading and displacement parameters for wear-testing machines and corresponding environmental conditions for test*
- *Part 2: Methods of measurement*
- *Part 3: Loading and displacement parameters for orbital bearing type wear testing machines and corresponding environmental conditions for test*

Implants for surgery — Wear of total hip-joint prostheses —

Part 1:

Loading and displacement parameters for wear-testing machines and corresponding environmental conditions for test

1 Scope

This part of ISO 14242 specifies the relative angular movement between articulating components, the pattern of the applied force, the speed and duration of testing, the sample configuration, and the test environment to be used for the wear testing of total hip-joint prostheses.

2 Normative references

The following documents, in whole or in part, are normatively referenced in this document and are indispensable for its application. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 3696, *Water for analytical laboratory use — Specification and test methods*

ISO 7206-1, *Implants for surgery — Partial and total hip joint prostheses — Part 1: Classification and designation of dimensions*

ISO 14242-2, *Implants for surgery — Wear of total hip-joint prostheses — Part 2: Methods of measurement*

3 Terms and definitions

For the purposes of this document, the terms and definitions given in ISO 7206-1 and the following apply.

3.1

abduction/adduction

angular movement shown in [Figure 1 a\)](#)

3.2

flexion/extension

angular movement shown in [Figure 1 b\)](#)

3.3

inward/outward rotation

angular movement shown in [Figure 1 c\)](#)

3.4

polar axis

axis of the acetabular component which intersects the centre of the spherical articulating surface and is perpendicular to the plane of the flange or, if no flange is present, perpendicular to the plane of the entry diameter

4 Principle

The femoral and acetabular components of a test specimen are placed in position in their normal configuration. The test apparatus transmits a specified time-varying force between the components, together with specified relative angular displacements. A control specimen, if polymers are the object of investigation, is subjected to the same time-varying force to determine the creep of the test specimen and/or the amount of mass change due to fluid transfer. The test takes place in a controlled environment simulating physiological conditions.

5 Test and control specimens and test fluid

5.1 Fluid test medium, calf serum diluted with deionized water in accordance with ISO 3696.

The fluid test medium shall be filtered through a 2 µm filter and have a protein mass concentration of 30 g/l ± 2 g/l. To minimize microbial contamination, the fluid test medium shall be stored frozen until required for testing. An antimicrobial reagent (such as sodium azide) can be added.

WARNING — Antimicrobial reagents can be potentially hazardous.

Routine monitoring of the pH of the fluid test medium can be undertaken. If so, the values and the relevant number of load cycles should be included in the test report [see [Clause 8](#) item f) 6)].

The recommended protein concentration of 30 g/l has been shown to result in reasonably physiological wear mechanisms and wear rates with a variety of materials in a variety of hip simulators, and is stipulated here in the interest of facilitating comparison of results among laboratories implementing this part of ISO 14242. Nevertheless, the user should routinely validate the results obtained in a hip simulator by direct comparison with implants of the same design and bearing materials that have been worn *in vivo*. If substantial differences are noted, the user might wish to use a higher or lower concentration of protein in the test lubricant, if it can be documented that this provides a closer agreement with *in vivo* wear mechanisms and wear rates.

NOTE The use of a fluid test medium of non-biological origin can be considered when performance requirements relating to this test method are being decided.

5.2 Test specimen, femoral head and acetabular components.

The acetabular component shall have the articulating surface attached by its normal immediate backing (for example bone cement or a machined replica of the inner surface of the backing) unless this is impractical due to physical features of the implant system. If the component forming the articulating surface is fixed to the backing by a rim/snap-fit system, the machined replica shall provide the same fixation conditions.

If it is not practical to use the normal backing or cement fixation due to physical features of the implant system, the support system for the acetabular component should reproduce the design features and conditions intended for clinical use but should allow removal of the component for measurement of wear without destruction.

The features connecting the acetabular component to the test rig shall prevent any movement and should not apply forces in restricted regions that might develop localized points of high stress.

5.3 Control specimen, identical to test specimen.

6 Apparatus

6.1 Testing machine, capable of producing the angular displacements specified in [Figures 1](#) and [2](#) in association with the corresponding forces specified in [Figures 1](#) and [3](#), and operating at a frequency of 1 Hz ± 0,1 Hz.

6.2 Means of mounting and enclosing the test specimen, using a corrosion-resistant material, capable of holding femoral and acetabular components using attachment methods comparable to the intended anatomical fixation.

An enclosure shall be provided which is capable of isolating the test specimen to prevent third-body contamination from the test machine and the atmosphere.

6.3 Means of aligning and positioning the femoral component of the test specimen in the inferior position, so that its axis is situated at the centre of the axes of rotation of the test machine and so that the same position and orientation can be reproduced following removal for measurement or cleaning, if required.

6.4 Means of aligning and positioning the acetabular component of the test specimen so that its axis is situated at the centre of the axes of rotation of the test machine and so that the same position and orientation can be reproduced following removal for measurement.

NOTE It is advisable that care be taken during start-up and operation of the test so that air does not accumulate in the acetabular cup and deprive portions of the articulating surfaces of lubricant.

6.5 Motion control system, capable of generating the angular movements of the femoral component given in [Figures 1](#) and [2](#) with an accuracy of $\pm 3^\circ$ at the maxima and minima of the motion and $\pm 1\%$ of the cycle time for phasing.

The angles are specified to produce three-dimensional angular movements. The sequence of the angular transformation is: abduction/adduction, followed by flexion/extension, followed by internal/external rotation. Other sequences should be documented in the test report.

6.6 Force control system, capable of generating a force whose direction is shown in [Figure 1](#) and which varies as shown in [Figure 3](#), and maintaining the magnitude of the maxima and minima of this force cycle to a tolerance of $\pm 3\%$ of the maximum force value for the cycle and $\pm 3\%$ of the cycle time for phasing.


6.7 Lubrication system, capable of maintaining the contact surfaces immersed in the fluid test medium.

NOTE It is advisable to use sealed enclosures in order to prevent evaporation.


6.8 Temperature control system, capable of maintaining the temperature of the fluid test medium at $37\text{ }^\circ\text{C} \pm 2\text{ }^\circ\text{C}$.

The test shall be closely monitored for evidence of excessive temperatures and corrective measures taken if needed. These can include stopping the test periodically to allow the bearing and lubricant to cool, and cooling the lubricant bath by, for example, circulating it through a cooling apparatus.


6.9 Control station(s), capable of applying the loading regime shown in [Figures 1](#) and [3](#) without the angular displacements shown in [Figures 1](#) and [2](#), and incorporating the provisions of [6.2](#), [6.3](#), [6.4](#), [6.6](#), [6.7](#), and [6.8](#).

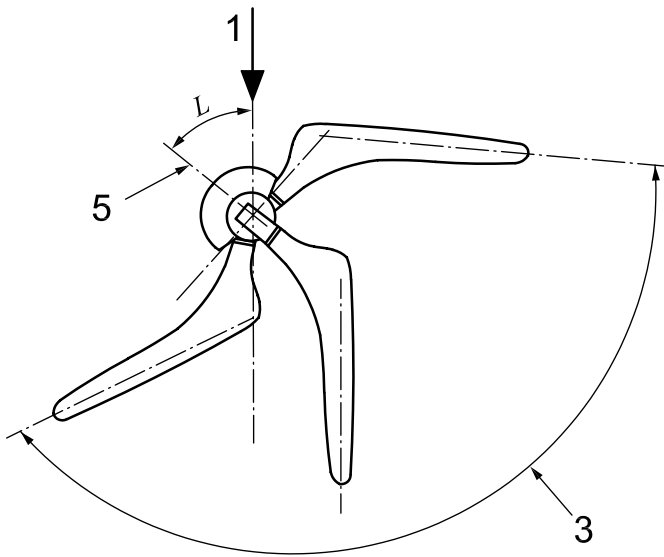


a) Abduction/adduction

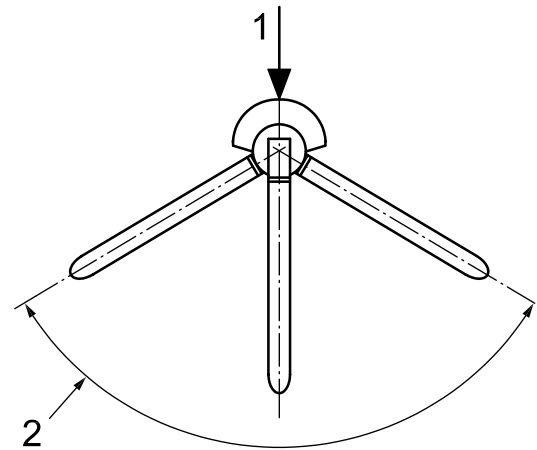

b) Flexion/extension



c) Inward/outward rotation

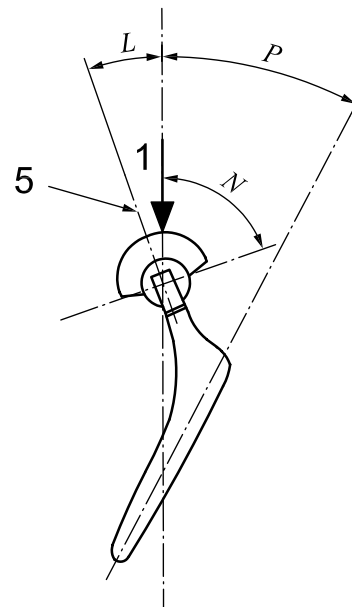

d) Orientation of acetabular component and femoral component in mid-position relative to the load line


Key

- 1 load axis
- 2 flexion/extension angle
- 3 abduction/adduction angle
- 4 inward/outward rotation angle
- 5 polar axis of acetabular component
- L inclination of the polar axis of the acetabular component to the load line

N inclination of the face of the acetabular component equal to $60^\circ \pm 3^\circ$, or as specified by the manufacturer
P inclination of stem axis to load line in mid-position of abduction/adduction range

NOTE Angles *N*, *L*, and *P* are specified in 7.3 and 7.4.

Figure 1 — Angular movement of femoral component and orientation of components relative to the load line

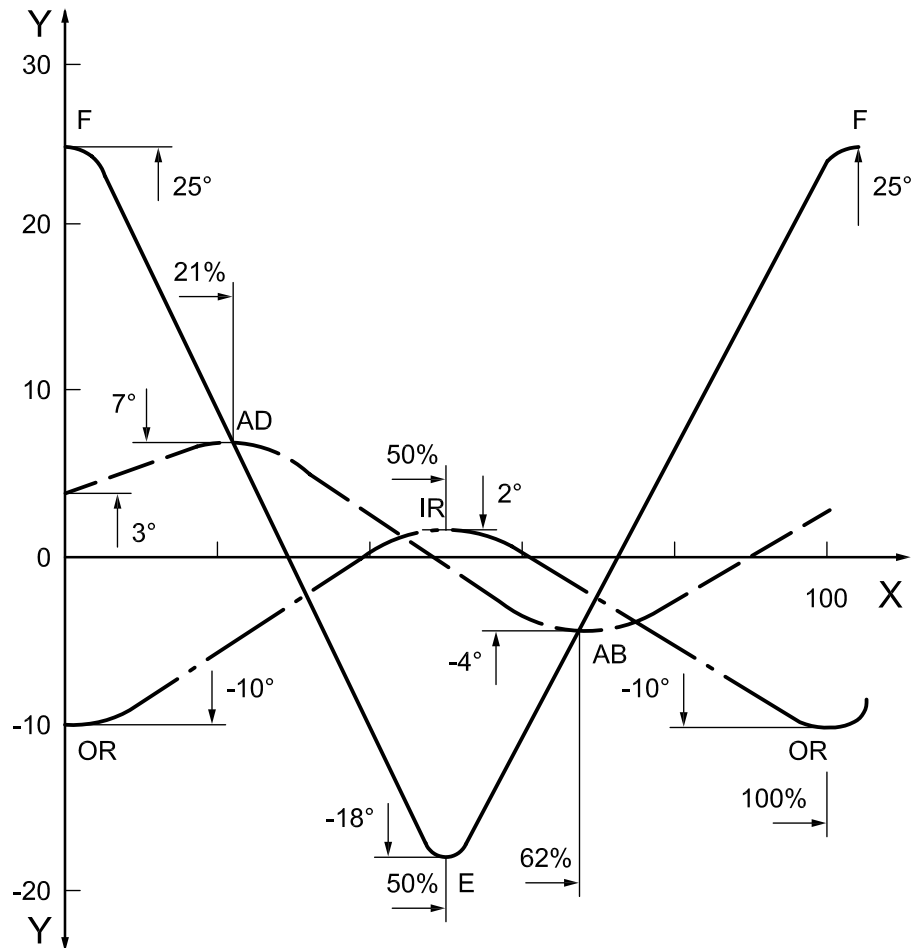


Key

- X time, as a percentage of cycle time
- Y angle of femoral movement, in degrees
- — — — — AB - Abduction
- — — — — AD - Adduction
- — — — — E - Extension
- — — — — F - Flexion
- — — — — IR - Inward rotation
- — — — — OR - Outward rotation

Figure 2 — Variation with time of angular movement to be applied to the femoral test specimen

Time, % of cycle (± 1 %)	0	21	50	62	100
Angle of flexion (+) or extension (-) $\pm 3^\circ$	25		-18		25
Angle of adduction (+) or abduction (-) $\pm 3^\circ$	3	7		-4	3
Angle of inward (+) or outward (-) rotation $\pm 3^\circ$	-10		2		-10

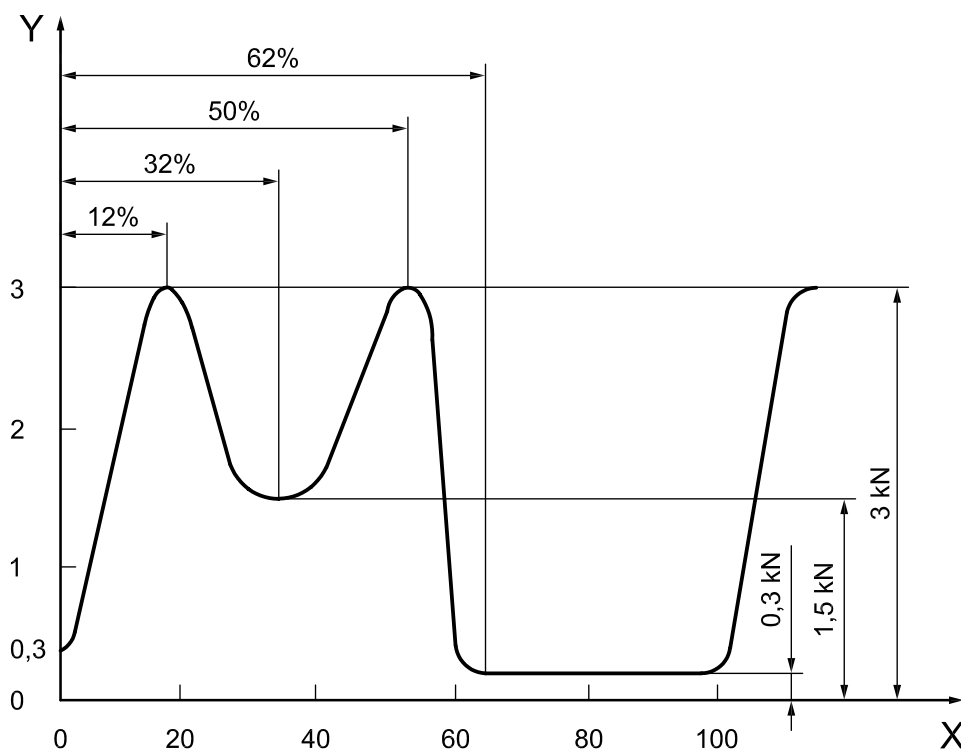

Key

X time, as a percentage of cycle time
 Y load in kN

Figure 3 — Variation with time of the force to be applied along the loading axis

Time, % of cycle (± 3 %)	0	12	32	50	62	100
Applied force, kN (± 90 N)	0,3	3,0	1,5	3,0	0,3	0,3

7 Procedure

7.1 Make any initial measurements required to determine the subsequent amount of wear and/or creep and calibrate each test station using a load cell. Undertake this calibration while the load is being developed at other stations, if any, in the test rig to simulate working conditions of the test frame.

NOTE Methods of measurement of wear are given in ISO 14242-2.

7.2 Following the initial measurements, clean the test specimen as specified in ISO 14242-2.

7.3 Mount the femoral component of the testing specimen in the test machine in the inferior position with its stem in the abduction/adduction position of $P = 10^\circ \pm 3^\circ$, as shown in [Figure 1 a](#)), and in the inward/outward rotation position, $\gamma/2$, as shown in [Figure 1 c](#)).

NOTE For a modular component, the stem of the implant can be replaced by a support which has an identical cone and ensures the same head positioning so that test conditions remain unchanged.

7.4 Mount the acetabular component of the testing specimen in the test machine with the polar axis vertical, as illustrated in [Figure 1 b](#)), and inclined at an angle L , as shown in [Figure 1 a](#)), where L equals $30^\circ \pm 3^\circ$. Alternatively, if the manufacturer specifies an angle of inclination of the component on surgical implantation to be N , as shown in [Figure 1 d](#)), then $L = (75 - N)^\circ \pm 3^\circ$.

7.5 Take the control specimen and repeat the steps described in [7.1](#), [7.2](#), [7.3](#), and [7.4](#). For implants of a specific design with the same material, shape and dimensions, control data from previous tests can be used.

7.6 Introduce the fluid test medium ([5.1](#)) to completely immerse the contact surfaces of the test specimen and the control specimen. Maintain the temperature of the fluid test medium at $37^\circ\text{C} \pm 2^\circ\text{C}$, taking the measurement at a location representative of the bulk temperature of the fluid.

7.7 Start the testing machine and adjust it so that the loads and displacements specified in [Figures 1](#), [2](#), and [3](#) are applied to the test specimen ([6.5](#), [6.6](#)) and the loads specified in [Figures 1](#) and [3](#) are applied to the control specimen. The curves between the defined maxima and minima in [Figures 2](#) and [3](#) shall be smooth with no overshoots. Record the displacement and load waveforms at start-up and after each change of fluid test medium.

7.8 Operate the testing machine at a frequency of $1\text{ Hz} \pm 0,1\text{ Hz}$.

7.9 Replace the fluid lost by evaporation during the test at least daily, by adding deionized water. Replace the fluid test medium completely at least every 5×10^5 cycles.

7.10 Stop the test for measurements at least at 5×10^5 cycles, 1×10^6 cycles, and at least every 1×10^6 cycles thereafter until the test is terminated (see [7.14](#)).

7.11 Remove the test specimen and control specimen from the testing machine and take wear measurements.

7.12 Following wear measurements, clean the test specimen and control specimen as specified in ISO 14242-2 and reinstall in the testing machine (see [7.3](#), [7.4](#), and [7.5](#)).

7.13 Repeat the steps given in [7.6](#) to [7.12](#) until the test is terminated (see [7.14](#)).

7.14 Continue the test until one of the following occurs:

a) completion of 5×10^6 cycles;

NOTE At the request of the party submitting the specimen, the test can be continued beyond this limit. If the test is continued after 5 million cycles, it is advisable that the number of cycles at which the test was stopped be disclosed to the submitter of the implant.

b) break-up or delamination of the articulating surfaces;

c) failure of the testing machine to maintain the force and displacement parameters within the given tolerances (see [6.5](#), [6.6](#)).

8 Test report

The test report shall include the following information:

a) a reference to this part of ISO 14242 (i.e. ISO 14242-1:2014);

- b) the identity of the test specimens, as stated by the party submitting the specimens for test, including size, material, type, and manufacturer;
- c) a description of the testing machine, including number of stations, types of systems used for generating motions and forces, range of motions and forces, sequence of angular transformations, types of systems used for measuring motions and forces, arrangement for mounting of specimen (see 5.2), arrangement for lubrication of articulating surfaces, arrangement for temperature control, and arrangement for the exclusion of contaminant particles;
- d) the type of lubricant and additives used;
- e) whether control specimens were used and, if not, the reference to the tests from which the control data were taken;
- f) a statement of results, including:
 - 1) total number of cycles applied;
 - 2) reason for terminating the test if fewer cycles than the designated cycle limit were applied;
 - 3) justification if a sequence other than abduction/adduction, flexion/extension, internal/external rotation was used;
 - 4) description of all the surfaces of both components at which relative movement has occurred;
 - 5) description of the condition of the interfaces between subcomponents, if the components are of modular construction;
 - 6) pH values and the relevant number of load cycles if routine monitoring was undertaken (see 5.1);
- g) details of the method of measurement of wear and the results obtained (see ISO 14242-2), namely:
 - 1) method of wear measurement (i.e. gravimetric or dimensional);
 - 2) change in mass for each measurement using the gravimetric method, or change in volume for each measurement using the dimensional method;
 - 3) wear rate (gravimetric or dimensional method).

9 Disposal of test specimen

No part of the test specimen or control specimen shall be used for clinical purposes after testing.

Annex A (informative)

Generation of rotation and load curves by formulae

A.1 The displacement curves can be expressed as functions. Using the equations might assist the set-up of computer-controlled test frames.

Table A.1 — Equations to express the generation of displacement curves

X - fraction of cycle %	Abduction/adduction °	Flexion/extension °	Internal/external rotation °
0 to 20	$= [4 \sin(0,074\ 8X) + 3]$	$= [21,5 \cos(0,062\ 8X) + 3,5]$	$= [6 \sin(1,5\pi + 0,062\ 8X) - 4]$
>20 to 61	$= [5,5 \sin(0,074\ 8X) + 1,5]$		
>61 to 100	$= [4 \sin(0,26\pi + 0,062\ 8X)]$		

A.2 The load curve can be expressed as a function. Using the formulae might assist the set-up of computer-controlled test frames.

Table A.2 — Formula to express the generation of load curve

X - fraction of cycle %	Load kN
0 to 61	$= -0,000\ 009\ 304\ 412\ 362\ 497\ 46X^4 + 0,001\ 135\ 691\ 194\ 869\ 52X^3 - 0,044\ 636\ 076\ 549\ 225\ 3X^2 + 0,609\ 263\ 366\ 429\ 307X + 0,3$
>61 to 100	$= 0,3$

British Standards Institution (BSI)

BSI is the national body responsible for preparing British Standards and other standards-related publications, information and services.

BSI is incorporated by Royal Charter. British Standards and other standardization products are published by BSI Standards Limited.

About us

We bring together business, industry, government, consumers, innovators and others to shape their combined experience and expertise into standards-based solutions.

The knowledge embodied in our standards has been carefully assembled in a dependable format and refined through our open consultation process. Organizations of all sizes and across all sectors choose standards to help them achieve their goals.

Information on standards

We can provide you with the knowledge that your organization needs to succeed. Find out more about British Standards by visiting our website at bsigroup.com/standards or contacting our Customer Services team or Knowledge Centre.

Buying standards

You can buy and download PDF versions of BSI publications, including British and adopted European and international standards, through our website at bsigroup.com/shop, where hard copies can also be purchased.

If you need international and foreign standards from other Standards Development Organizations, hard copies can be ordered from our Customer Services team.

Subscriptions

Our range of subscription services are designed to make using standards easier for you. For further information on our subscription products go to bsigroup.com/subscriptions.

With **British Standards Online (BSOL)** you'll have instant access to over 55,000 British and adopted European and international standards from your desktop. It's available 24/7 and is refreshed daily so you'll always be up to date.

You can keep in touch with standards developments and receive substantial discounts on the purchase price of standards, both in single copy and subscription format, by becoming a **BSI Subscribing Member**.

PLUS is an updating service exclusive to BSI Subscribing Members. You will automatically receive the latest hard copy of your standards when they're revised or replaced.

To find out more about becoming a BSI Subscribing Member and the benefits of membership, please visit bsigroup.com/shop.

With a **Multi-User Network Licence (MUNL)** you are able to host standards publications on your intranet. Licences can cover as few or as many users as you wish. With updates supplied as soon as they're available, you can be sure your documentation is current. For further information, email bsmusales@bsigroup.com.

BSI Group Headquarters

389 Chiswick High Road London W4 4AL UK

Revisions

Our British Standards and other publications are updated by amendment or revision.

We continually improve the quality of our products and services to benefit your business. If you find an inaccuracy or ambiguity within a British Standard or other BSI publication please inform the Knowledge Centre.

Copyright

All the data, software and documentation set out in all British Standards and other BSI publications are the property of and copyrighted by BSI, or some person or entity that owns copyright in the information used (such as the international standardization bodies) and has formally licensed such information to BSI for commercial publication and use. Except as permitted under the Copyright, Designs and Patents Act 1988 no extract may be reproduced, stored in a retrieval system or transmitted in any form or by any means – electronic, photocopying, recording or otherwise – without prior written permission from BSI. Details and advice can be obtained from the Copyright & Licensing Department.

Useful Contacts:

Customer Services

Tel: +44 845 086 9001

Email (orders): orders@bsigroup.com

Email (enquiries): cservices@bsigroup.com

Subscriptions

Tel: +44 845 086 9001

Email: subscriptions@bsigroup.com

Knowledge Centre

Tel: +44 20 8996 7004

Email: knowledgecentre@bsigroup.com

Copyright & Licensing

Tel: +44 20 8996 7070

Email: copyright@bsigroup.com



...making excellence a habit.™